


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031621\
Data File : VN066205.D
Acq On : 16 Mar 2021 9:55
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031621W.M
Title : SW846 8260
Last Update : Wed Mar 17 05:05:15 2021

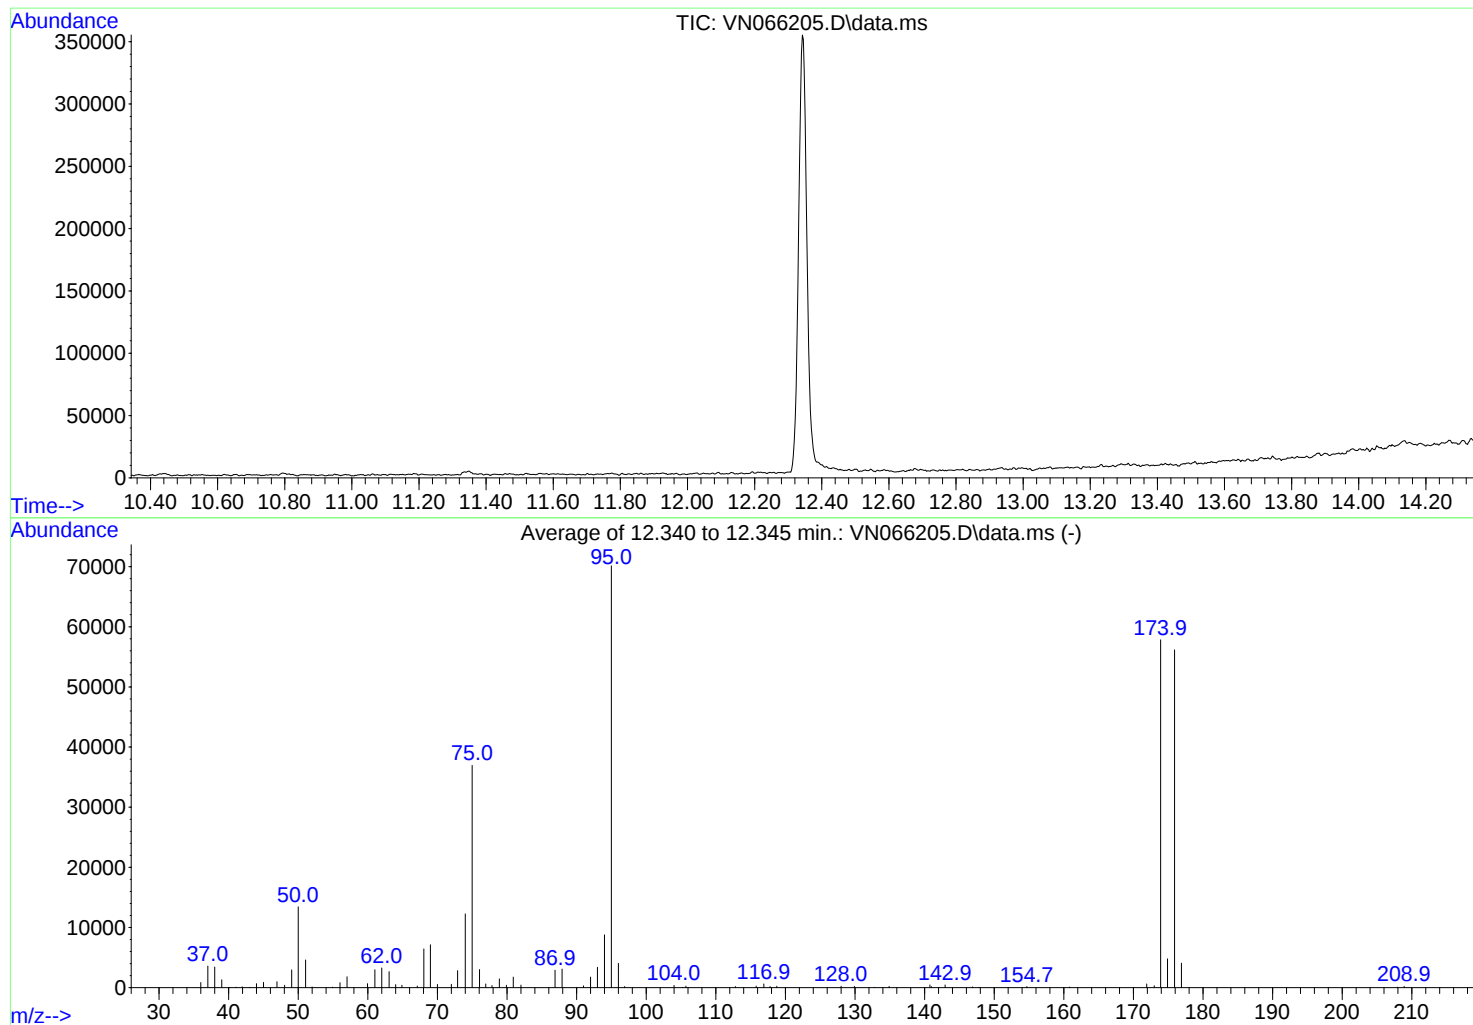

AutoFind: Scans 3971, 3972, 3973; Background Corrected with Scan 3956

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	13430	PASS
75	95	30	60	52.7	36965	PASS
95	95	100	100	100.0	70131	PASS
96	95	5	9	5.8	4046	PASS
173	174	0.00	2	0.6	320	PASS
174	95	50	100	82.5	57848	PASS
175	174	5	9	8.3	4789	PASS
176	174	95	101	97.1	56173	PASS
177	176	5	9	7.3	4084	PASS