

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031622\
 Data File : VN071319.D
 Acq On : 16 Mar 2022 14:28
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Mar 17 05:17:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	907714	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1481349	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1403096	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	771408	50.000	ug/l	# 0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	551514	44.332	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	88.660%
35) Dibromofluoromethane	8.016	113	422497	45.197	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	90.400%
50) Toluene-d8	10.439	98	1831084	48.651	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	97.300%
62) 4-Bromofluorobenzene	12.727	95	648829	50.909	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	101.820%
Target Compounds						
					Qvalue	
3) Chloromethane	2.299	50	3642	0.238	ug/l #	74
5) Bromomethane	2.851	94	1252	Below Cal		99
13) Acrolein	4.051	56	585	0.226	ug/l #	57
16) Acetone	4.298	43	11347	1.875	ug/l #	88
18) Methyl Acetate	4.863	43	18017	1.568	ug/l	94
20) Methylene Chloride	5.104	84	2999	0.651	ug/l #	89
31) Cyclohexane	8.086	56	19722	0.993	ug/l #	17
36) 1,1-Dichloropropene	8.086	75	69601	4.647	ug/l #	51
38) Carbon Tetrachloride	8.086	117	91654	6.327	ug/l #	15
43) Isopropyl Acetate	8.686	43	143201	4.646	ug/l #	56
47) Bromodichloromethane	9.775	83	3199	0.212	ug/l #	38
49) 1,4-Dioxane	9.580	88	69	0.278	ug/l #	1
58) 2-Chloroethyl Vinyl ether	9.786	63	770	28.044	ug/l	97
66) 1,1,1,2-Tetrachloroethane	11.857	131	7098	0.642	ug/l #	8
71) Bromoform	12.392	173	2338	0.279	ug/l #	29
74) N-amyl acetate	12.351	43	306502	10.962	ug/l #	77
75) 1,1,2,2-Tetrachloroethane	12.639	83	154941	4.690	ug/l #	25
76) 1,2,3-Trichloropropane	12.957	75	57916	0.292	ug/l #	16
77) Bromobenzene	12.951	156	741008	42.733	ug/l #	1
78) n-propylbenzene	12.933	91	23459	0.294	ug/l	93
81) trans-1,4-Dichloro-2-b...	12.727	75	327596	45.907	ug/l #	6
82) 4-Chlorotoluene	13.133	91	21708	0.476	ug/l #	38
83) tert-Butylbenzene	13.321	119	44299	0.858	ug/l #	29
84) 1,2,4-Trimethylbenzene	13.245	105	56354	1.017	ug/l #	31
85) sec-Butylbenzene	13.504	105	19594	0.286	ug/l	99
86) p-Isopropyltoluene	13.586	119	36706	0.680	ug/l #	53
92) 1,2-Dibromo-3-Chloropr...	14.598	75	5044	1.166	ug/l #	1
93) 1,2,4-Trichlorobenzene	15.257	180	691	3.041	ug/l #	1
95) Naphthalene	15.498	128	6841	5.241	ug/l #	21
96) 1,2,3-Trichlorobenzene	15.692	180	373	2.761	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031622\
Data File : VN071319.D
Acq On : 16 Mar 2022 14:28
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Mar 17 05:17:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration




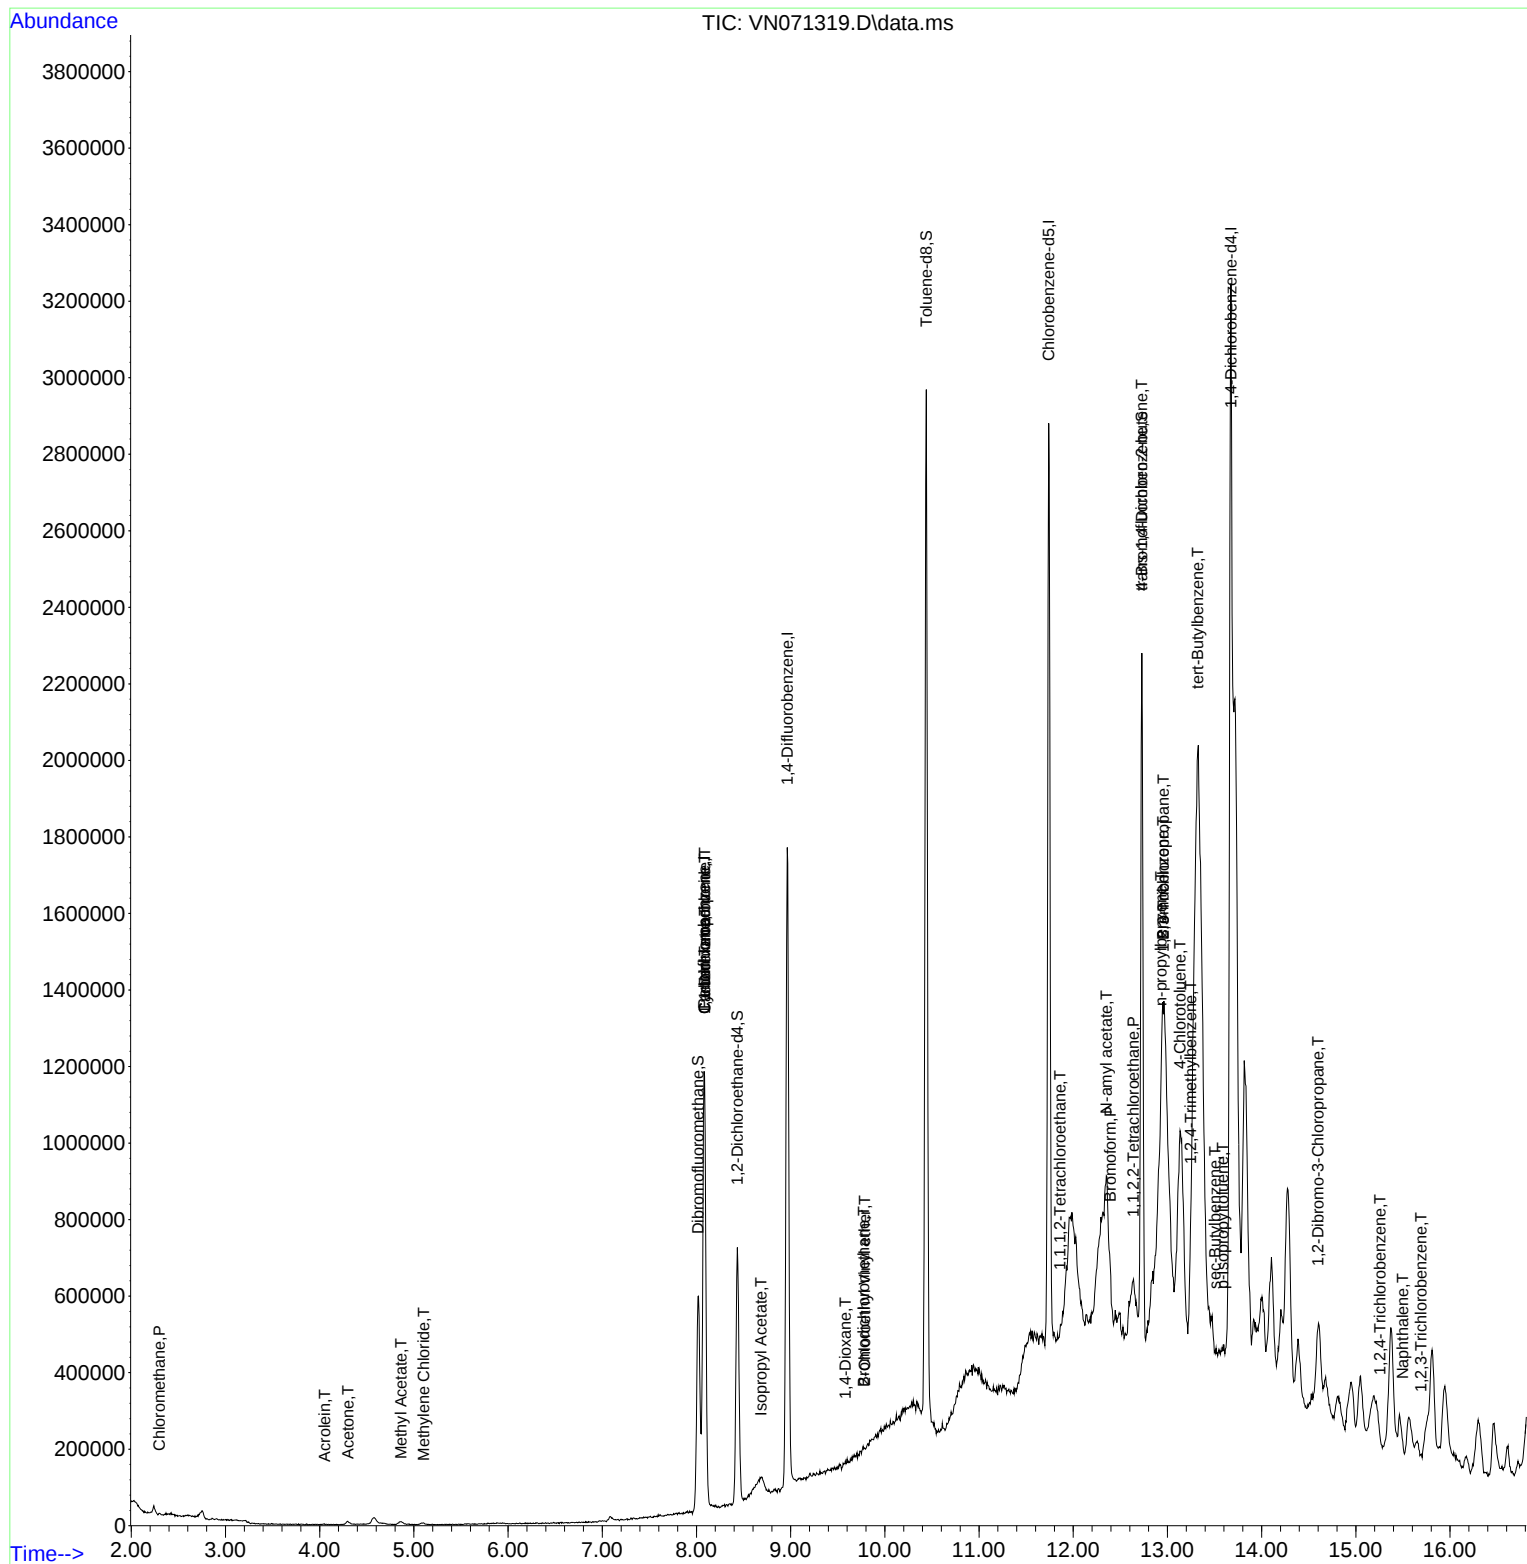




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 10
Delta R.T. -0.005 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 907714
Ion Ratio Lower Upper
168 100
99 58.3 41.3 61.9



#3
Chloromethane
Concen: 0.238 ug/l
RT: 2.299 min Scan# 53
Delta R.T. -0.000 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 50 Resp: 3642
Ion Ratio Lower Upper
50 100
52 17.3 25.4 38.0#


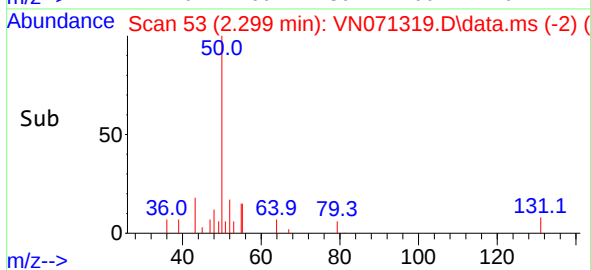






#5
Bromomethane
Concen: Below Cal
RT: 2.851 min Scan# 14
Delta R.T. 0.017 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 94 Resp: 1252
Ion Ratio Lower Upper
94 100
96 92.9 73.8 110.8

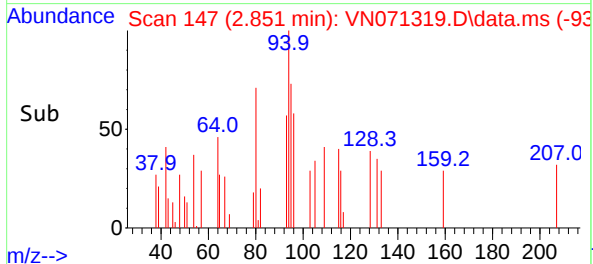

#13
Acrolein
Concen: 0.226 ug/l
RT: 4.051 min Scan# 351
Delta R.T. 0.012 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 56 Resp: 585
Ion Ratio Lower Upper
56 100
55 106.2 56.6 85.0#


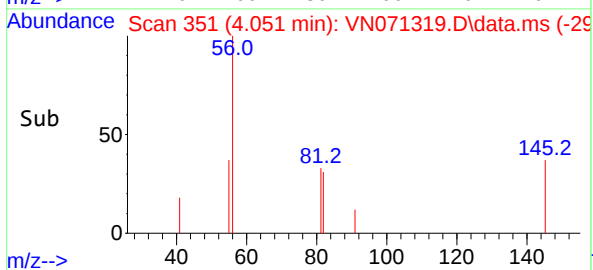

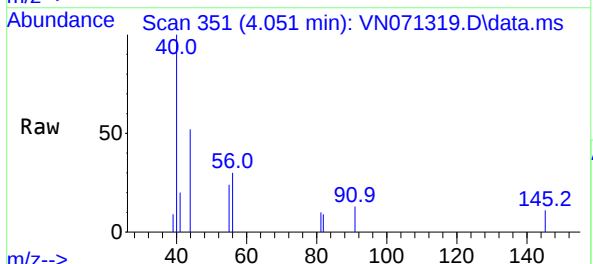




#16
Acetone
Concen: 1.875 ug/l
RT: 4.298 min Scan# 391
Delta R.T. 0.012 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 43 Resp: 11347
Ion Ratio Lower Upper
43 100
58 22.5 23.1 34.7#

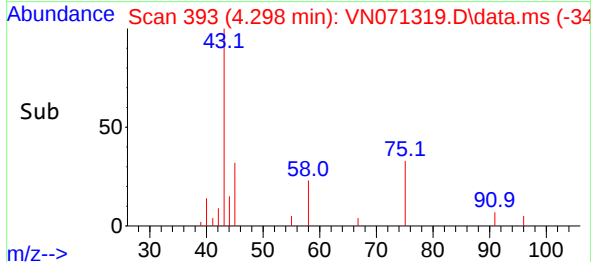

#18
Methyl Acetate
Concen: 1.568 ug/l
RT: 4.863 min Scan# 489
Delta R.T. 0.012 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 43 Resp: 18017
Ion Ratio Lower Upper
43 100
74 21.3 19.4 29.2

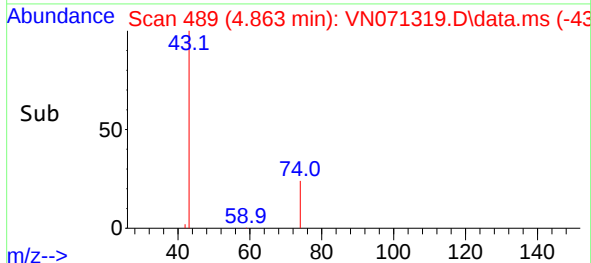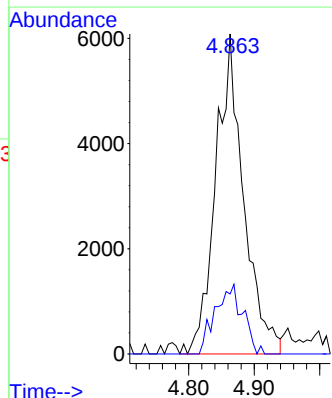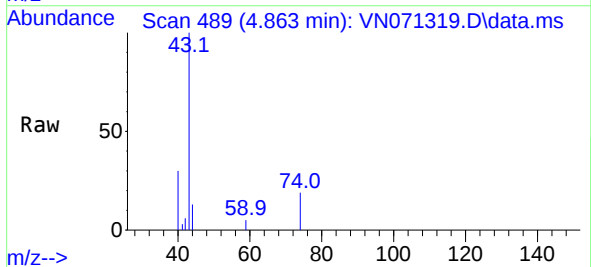







#20
Methylene Chloride
Concen: 0.651 ug/l
RT: 5.104 min Scan# 51
Delta R.T. 0.011 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion: 84 Resp: 2999




Ion	Ratio	Lower	Upper
84	100		
49	112.9	93.5	140.3
51	36.2	29.4	44.2
86	43.4	53.0	79.4

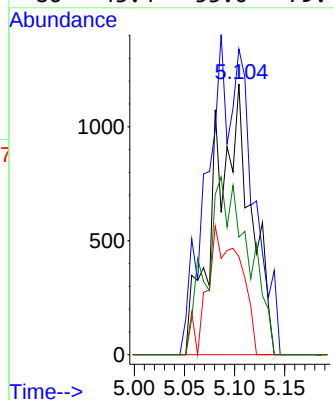


#31
Cyclohexane
Concen: 0.993 ug/l
RT: 8.086 min Scan# 1037
Delta R.T. -0.006 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 56 Resp: 19722

Ion	Ratio	Lower	Upper
56	100		
69	163.8	27.1	40.7
84	119.4	73.4	110.0


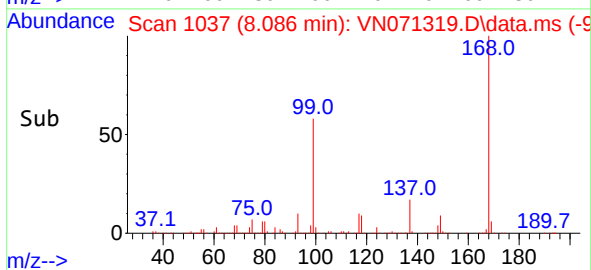
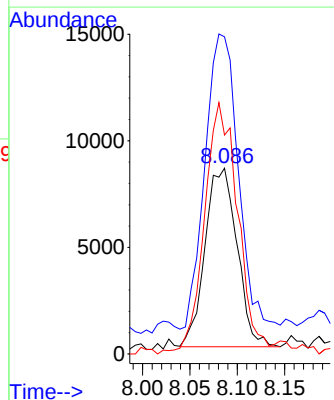
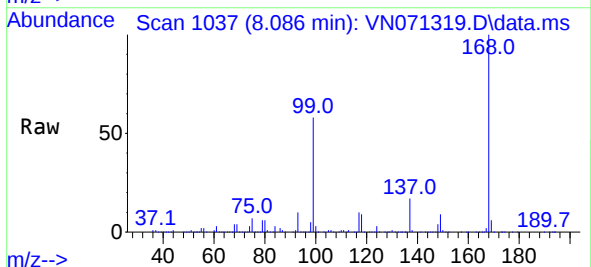


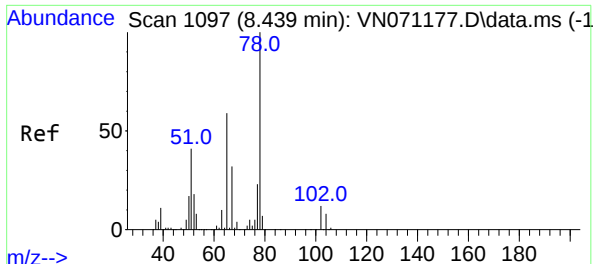

#33
1,2-Dichloroethane-d4
Concen: 44.332 ug/l
RT: 8.433 min Scan# 1097
Delta R.T. -0.006 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 65 Resp: 551514
Ion Ratio Lower Upper
65 100
67 52.6 0.0 103.0

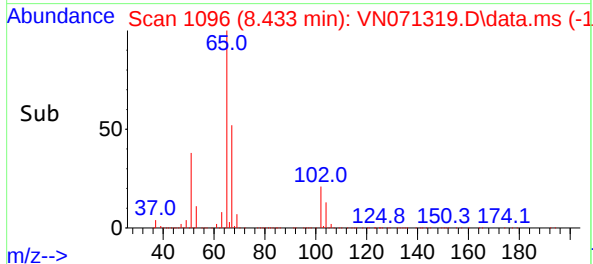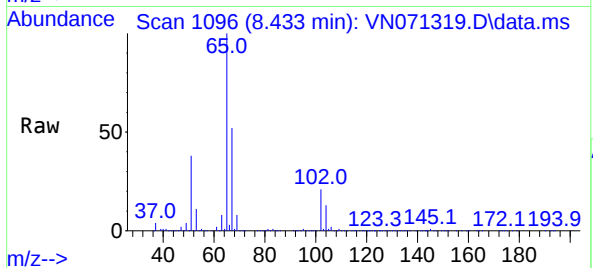

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion:114 Resp: 1481349
Ion Ratio Lower Upper
114 100
63 21.1 0.0 37.8
88 15.8 0.0 27.4


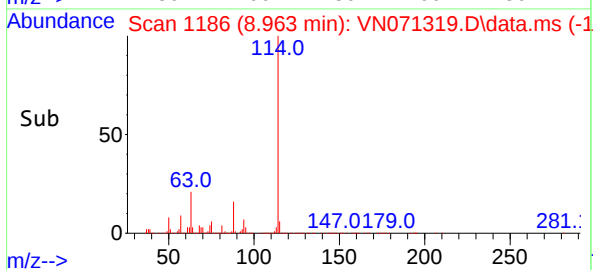

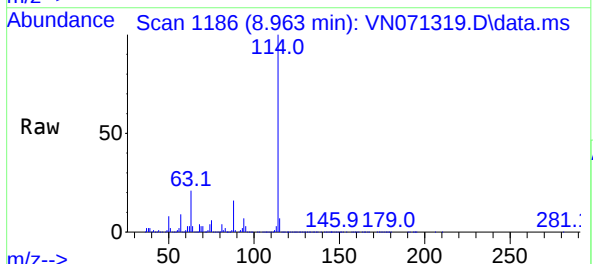


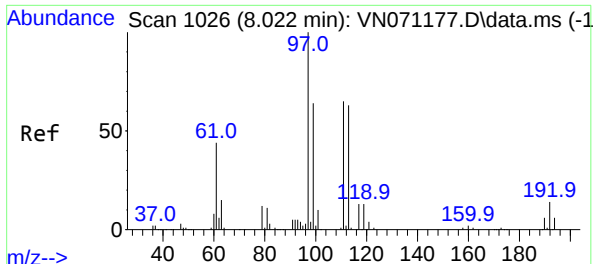

#35
Dibromofluoromethane
Concen: 45.197 ug/l
RT: 8.016 min Scan# 1025
Delta R.T. -0.006 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:113 Resp: 422497
Ion Ratio Lower Upper
113 100
111 103.6 82.2 123.2
192 20.4 16.9 25.3

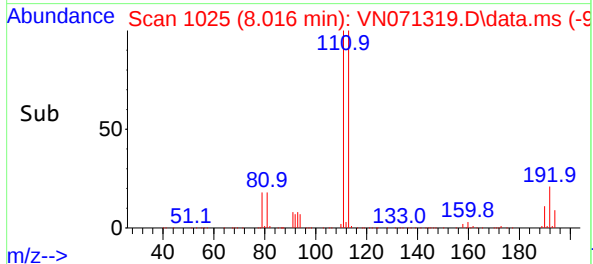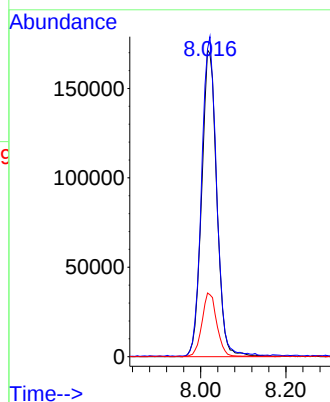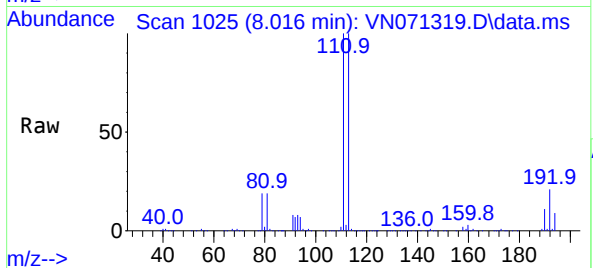

#36
1,1-Dichloropropene
Concen: 4.647 ug/l
RT: 8.086 min Scan# 1037
Delta R.T. -0.129 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 75 Resp: 69601
Ion Ratio Lower Upper
75 100
110 10.2 18.4 55.2#
77 1.2 24.4 36.6#


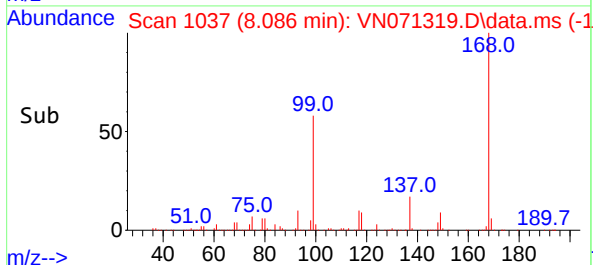

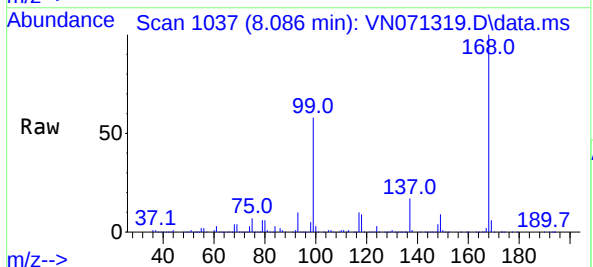




#38
Carbon Tetrachloride
Concen: 6.327 ug/l
RT: 8.086 min Scan# 1139
Delta R.T. -0.118 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:117 Resp: 91654
Ion Ratio Lower Upper
117 100
119 3.6 76.1 114.1#
121 0.1 24.2 36.2#

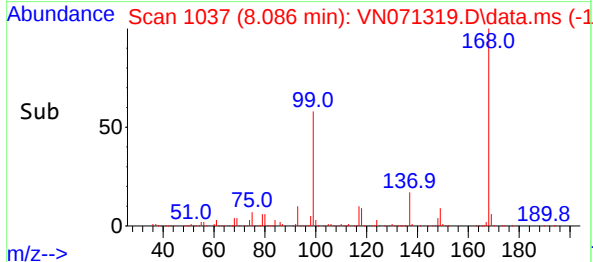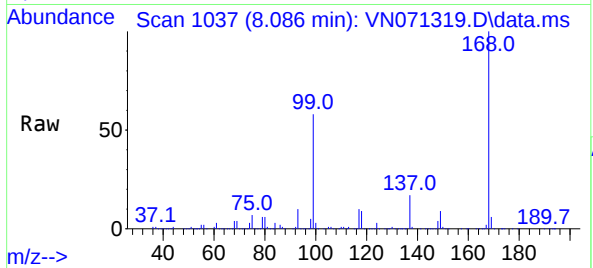

#43
Isopropyl Acetate
Concen: 4.646 ug/l
RT: 8.686 min Scan# 1139
Delta R.T. 0.129 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 43 Resp: 143201
Ion Ratio Lower Upper
43 100
61 0.5 20.4 30.6#
87 0.0 11.2 16.8#


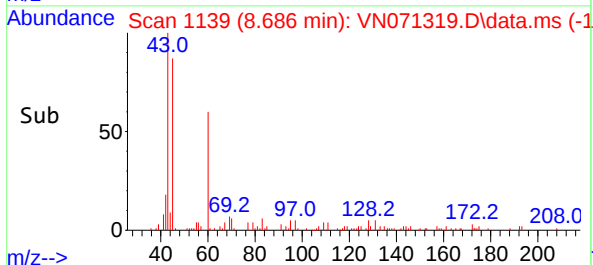
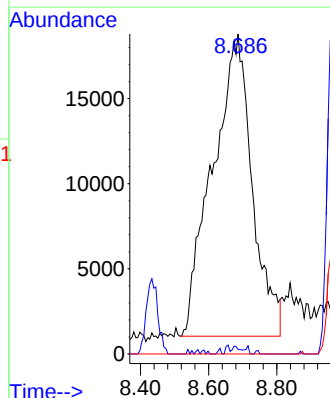
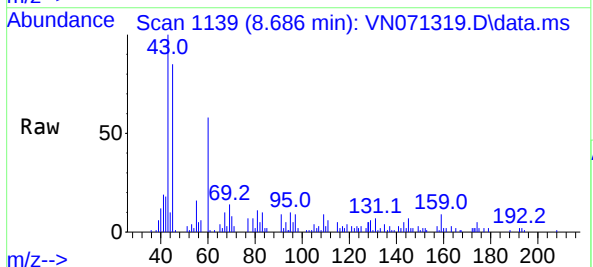




#47
Bromodichloromethane
Concen: 0.212 ug/l
RT: 9.775 min Scan# 11
Delta R.T. 0.018 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 83 Resp: 3199
Ion Ratio Lower Upper
83 100
85 11.2 50.9 76.3#
127 0.0 7.1 10.7#

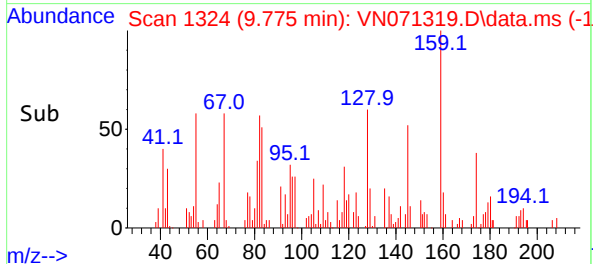

#49
1,4-Dioxane
Concen: 0.278 ug/l
RT: 9.580 min Scan# 1291
Delta R.T. 0.017 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 88 Resp: 69
Ion Ratio Lower Upper
88 100
43 1279.7 23.4 35.2#
58 873.9 50.6 75.8#


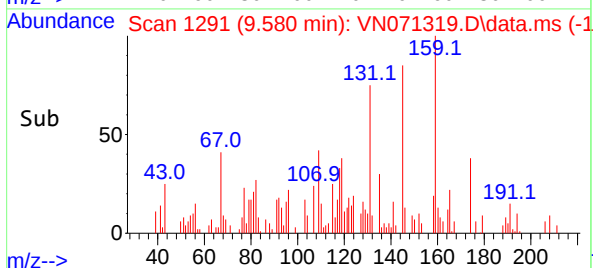
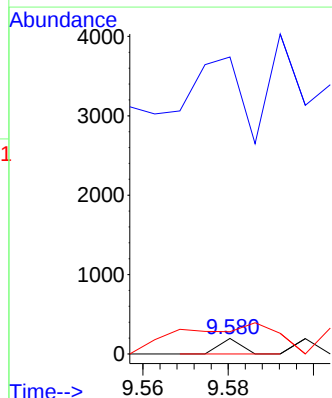
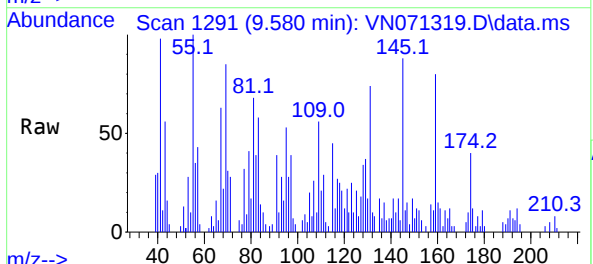




#50
Toluene-d8
Concen: 48.651 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 1831084
Ion Ratio Lower Upper
98 100
100 65.2 50.4 75.6



#58
2-Chloroethyl Vinyl ether
Concen: 28.044 ug/l
RT: 9.786 min Scan# 1326
Delta R.T. -0.253 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 63 Resp: 770
Ion Ratio Lower Upper
63 100
106 31.6 23.9 35.9



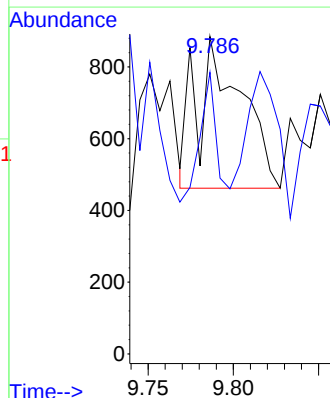





#62
4-Bromofluorobenzene
Concen: 50.909 ug/l
RT: 12.727 min Scan# 1177
Delta R.T. 0.000 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 95 Resp: 648829
Ion Ratio Lower Upper
95 100
174 78.8 0.0 187.2
176 74.3 0.0 181.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. -0.000 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 117 Resp: 1403096
Ion Ratio Lower Upper
117 100
82 57.2 42.4 63.6
119 32.2 25.4 38.2


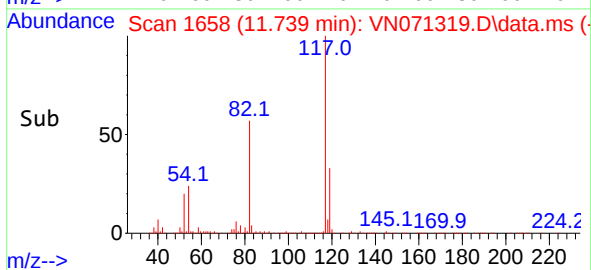






#66
1,1,1,2-Tetrachloroethane
Concen: 0.642 ug/l
RT: 11.857 min Scan# 1769
Delta R.T. 0.018 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:131 Resp: 7098
Ion Ratio Lower Upper
131 100
133 0.0 47.9 143.7#
119 0.0 32.1 96.5#

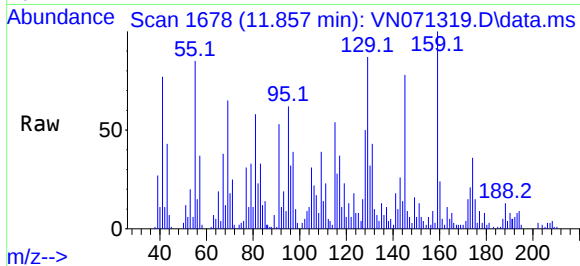

#71
Bromoform
Concen: 0.279 ug/l
RT: 12.392 min Scan# 1769
Delta R.T. -0.065 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion:173 Resp: 2338
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0


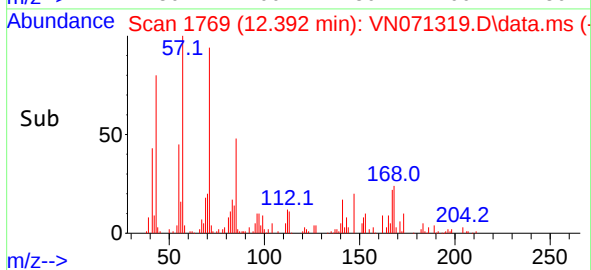

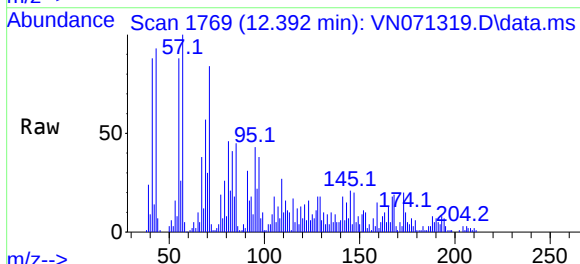




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1986
Delta R.T. 0.006 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:152 Resp: 771408
Ion Ratio Lower Upper
152 100
115 87.6 27.5 82.5#
150 112.1 0.0 344.4

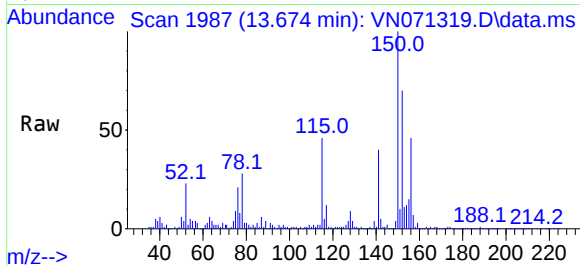

#74
N-ethyl acetate
Concen: 10.962 ug/l
RT: 12.351 min Scan# 1762
Delta R.T. -0.035 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 43 Resp: 306502
Ion Ratio Lower Upper
43 100
70 34.9 33.4 50.0
55 14.2 19.3 28.9#
61 0.2 18.5 27.7#



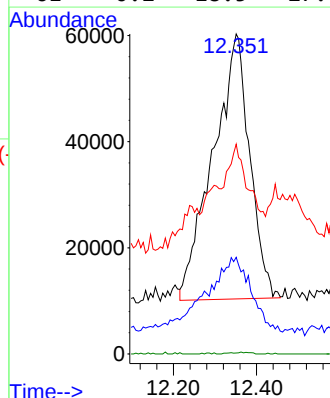





#75
1,1,2,2-Tetrachloroethane
Concen: 4.690 ug/l
RT: 12.639 min Scan# 1811
Delta R.T. -0.182 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 83 Resp: 154941
Ion Ratio Lower Upper
83 100
131 0.0 5.5 16.5#
85 0.0 32.4 97.2#

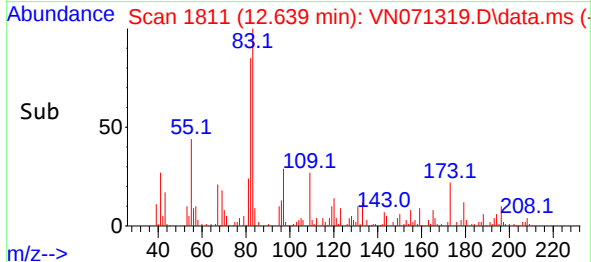

#76
1,2,3-Trichloropropane
Concen: 0.292 ug/l
RT: 12.957 min Scan# 1865
Delta R.T. 0.083 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 75 Resp: 57916
Ion Ratio Lower Upper
75 100
77 52.4 82.6 247.8#


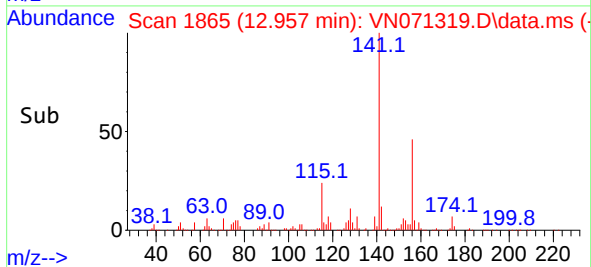

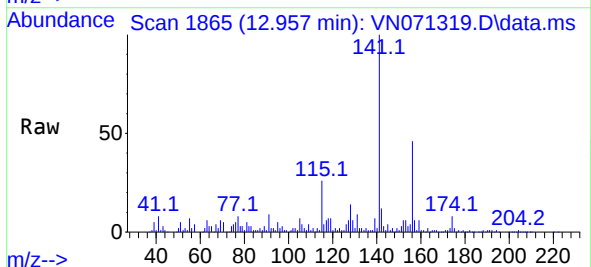




#77
Bromobenzene
Concen: 42.733 ug/l
RT: 12.951 min Scan# 1864
Delta R.T. 0.094 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:156 Resp: 741008
Ion Ratio Lower Upper
156 100
77 4.1 90.6 271.8#
158 0.1 48.9 146.7#

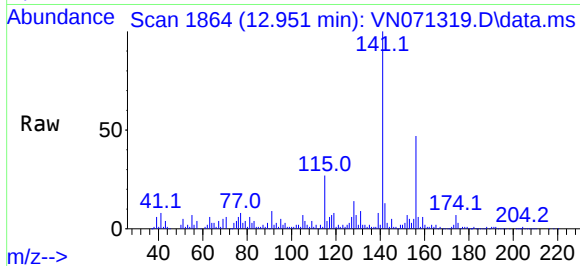

#78
n-propylbenzene
Concen: 0.294 ug/l
RT: 12.933 min Scan# 1861
Delta R.T. 0.018 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 91 Resp: 23459
Ion Ratio Lower Upper
91 100
120 20.7 11.9 35.9


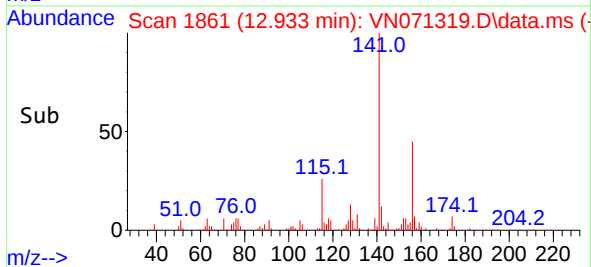

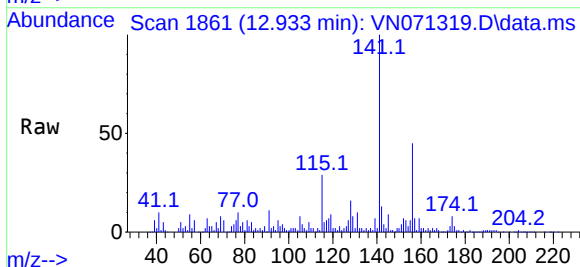


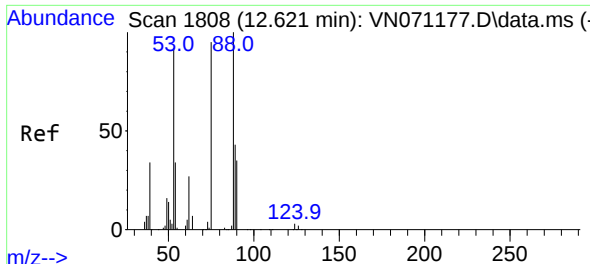

#81
trans-1,4-Dichloro-2-butene
Concen: 45.907 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 75 Resp: 327596
Ion Ratio Lower Upper
75 100
53 0.9 90.5 135.7#
89 0.2 38.2 57.4#

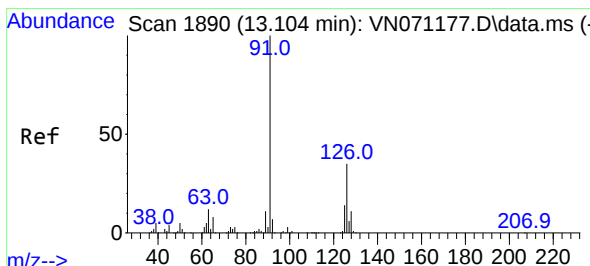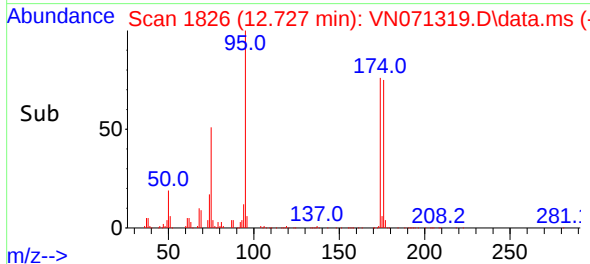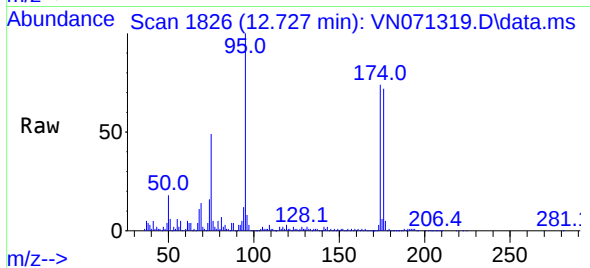

#82
4-Chlorotoluene
Concen: 0.476 ug/l
RT: 13.133 min Scan# 1895
Delta R.T. 0.029 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion: 91 Resp: 21708
Ion Ratio Lower Upper
91 100
126 0.0 18.2 54.6#


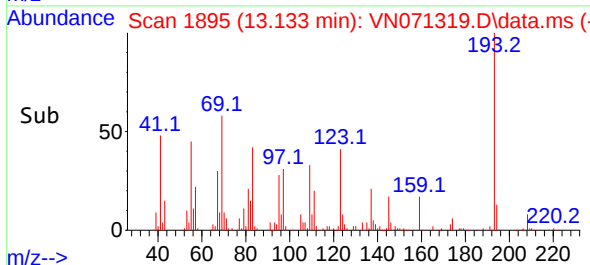
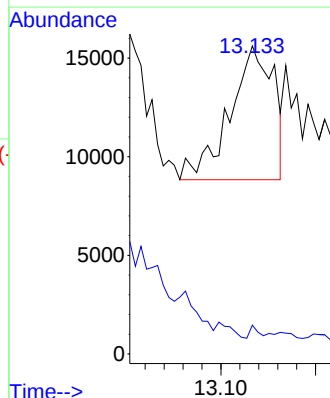
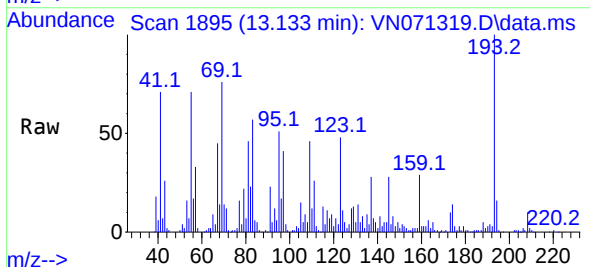




#83
tert-Butylbenzene
Concen: 0.858 ug/l
RT: 13.321 min Scan# 1927
Delta R.T. -0.000 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28



Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:119 Resp: 44299
Ion Ratio Lower Upper
119 100
91 0.0 31.5 94.5#
134 2.1 12.4 37.4#

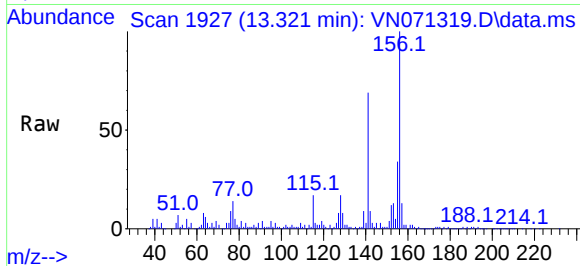

#84
1,2,4-Trimethylbenzene
Concen: 1.017 ug/l
RT: 13.245 min Scan# 1914
Delta R.T. -0.118 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion:105 Resp: 56354
Ion Ratio Lower Upper
105 100
120 0.0 22.8 68.4#



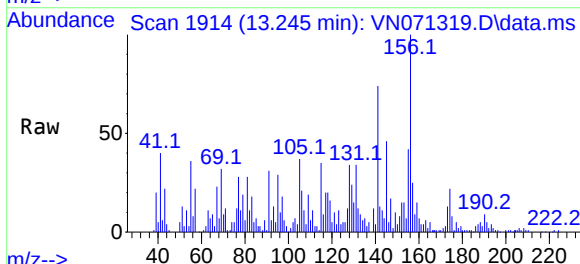




#85
sec-Butylbenzene
Concen: 0.286 ug/l
RT: 13.504 min Scan# 1958
Delta R.T. 0.006 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:105 Resp: 19594
Ion Ratio Lower Upper
105 100
134 21.2 10.4 31.1

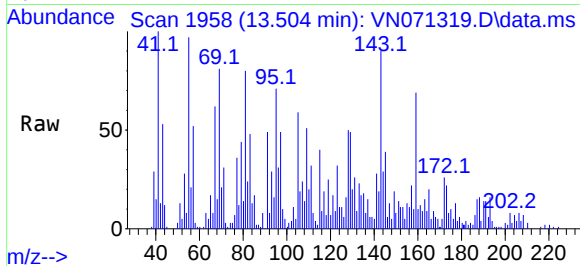

#86
p-Isopropyltoluene
Concen: 0.680 ug/l
RT: 13.586 min Scan# 1972
Delta R.T. -0.024 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion:119 Resp: 36706
Ion Ratio Lower Upper
119 100
134 0.0 13.6 40.7#
91 3.4 11.4 34.1#



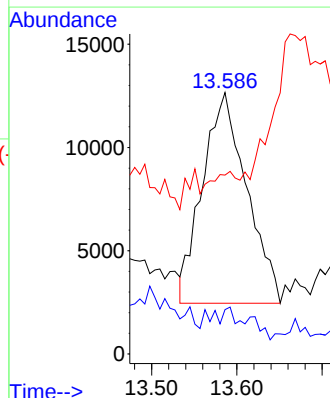
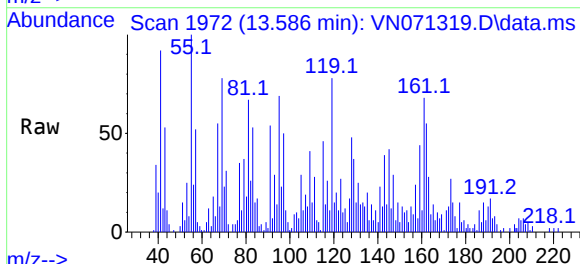


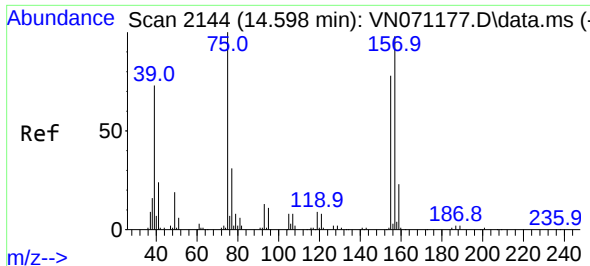

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 1.166 ug/l
 RT: 14.598 min Scan# 2144
 Delta R.T. -0.000 min
 Lab File: VN071319.D
 Acq: 16 Mar 2022 14:28




Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK


Tgt Ion: 75 Resp: 5044
 Ion Ratio Lower Upper
 75 100
 155 606.8 46.9 140.7#
 157 486.2 60.6 181.7#

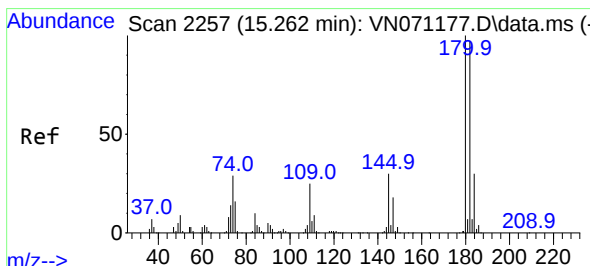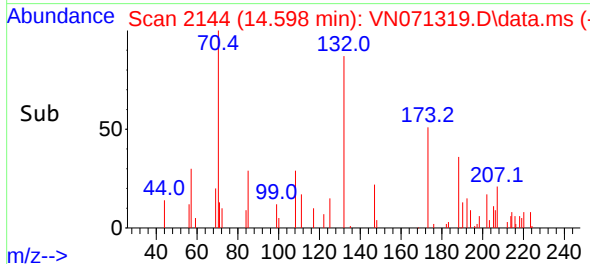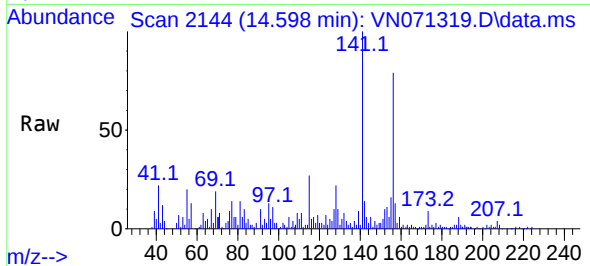

#93
 1,2,4-Trichlorobenzene
 Concen: 3.041 ug/l
 RT: 15.257 min Scan# 2256
 Delta R.T. -0.005 min
 Lab File: VN071319.D
 Acq: 16 Mar 2022 14:28

Tgt Ion: 180 Resp: 691
 Ion Ratio Lower Upper
 180 100
 182 254.3 48.3 144.9#
 145 472.9 14.5 43.5#


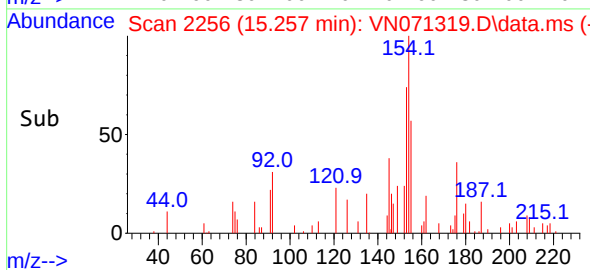

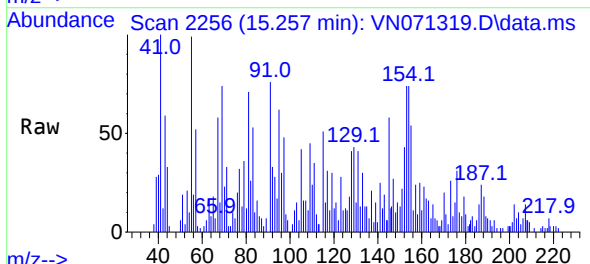


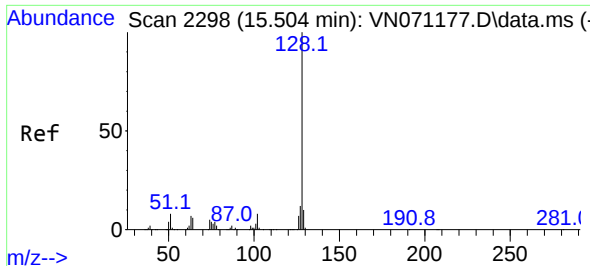

#95
Naphthalene
Concen: 5.241 ug/l
RT: 15.498 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion:128 Resp: 6841
Ion Ratio Lower Upper
128 100
127 34.7 10.5 15.7#
129 52.4 8.7 13.1#

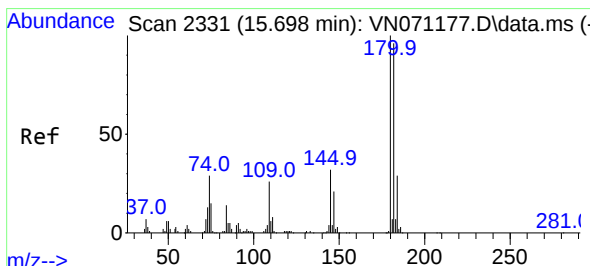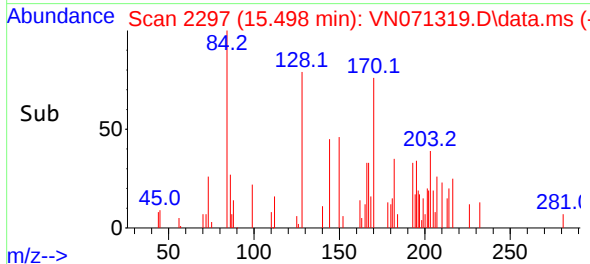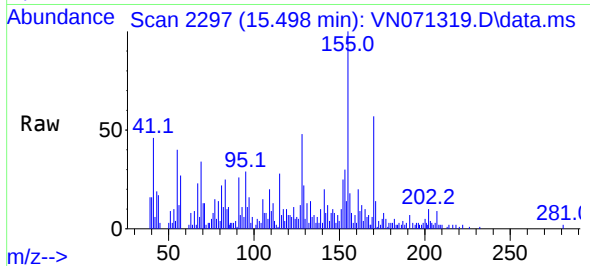

#96
1,2,3-Trichlorobenzene
Concen: 2.761 ug/l
RT: 15.692 min Scan# 2330
Delta R.T. -0.006 min
Lab File: VN071319.D
Acq: 16 Mar 2022 14:28

Tgt Ion:180 Resp: 373
Ion Ratio Lower Upper
180 100
182 100.8 47.4 142.2
145 1003.8 15.0 45.1#

