
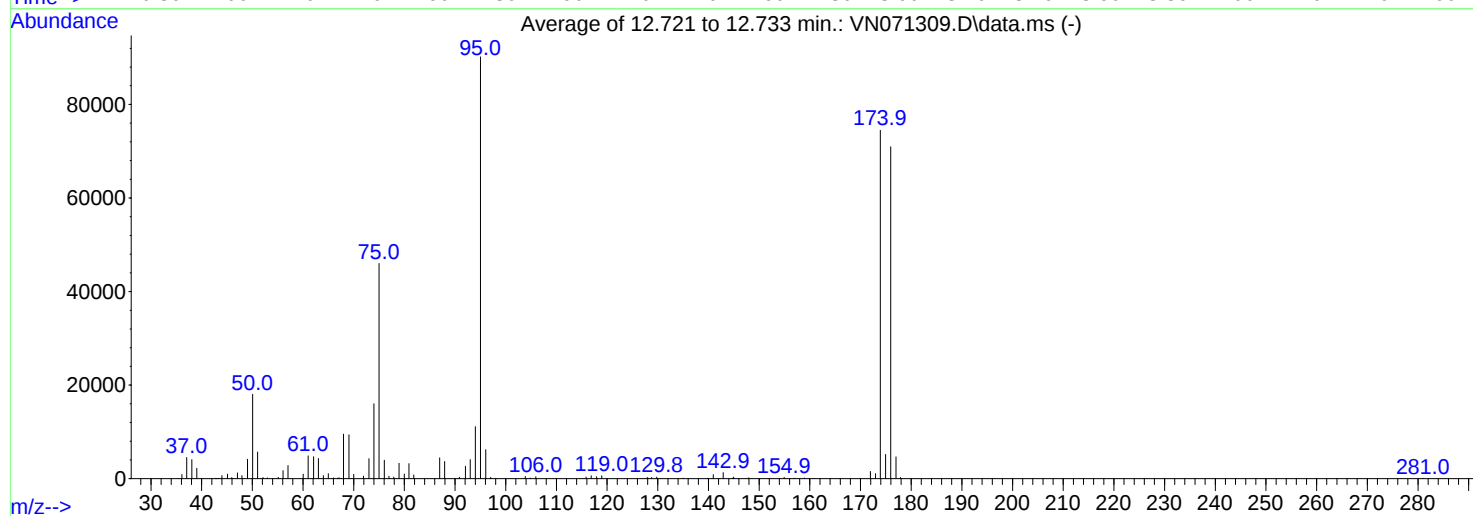


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031622\
 Data File : VN071309.D
 Acq On : 16 Mar 2022 09:47
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Title : SW846 8260
 Last Update : Tue Mar 08 06:52:46 2022

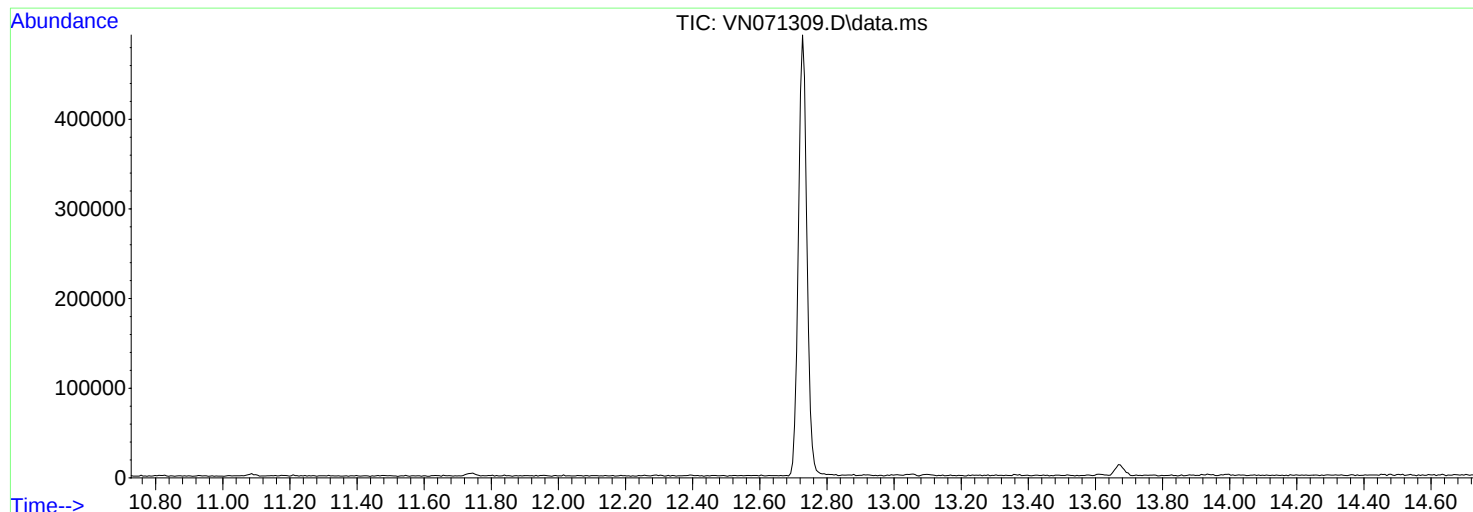

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	18025	PASS
75	95	30	60	51.0	45997	PASS
95	95	100	100	100.0	90179	PASS
96	95	5	9	6.9	6203	PASS
173	174	0.00	2	1.4	1079	PASS
174	95	50	100	82.6	74488	PASS
175	174	5	9	6.9	5161	PASS
176	174	95	101	95.3	70965	PASS
177	176	5	9	6.6	4651	PASS