
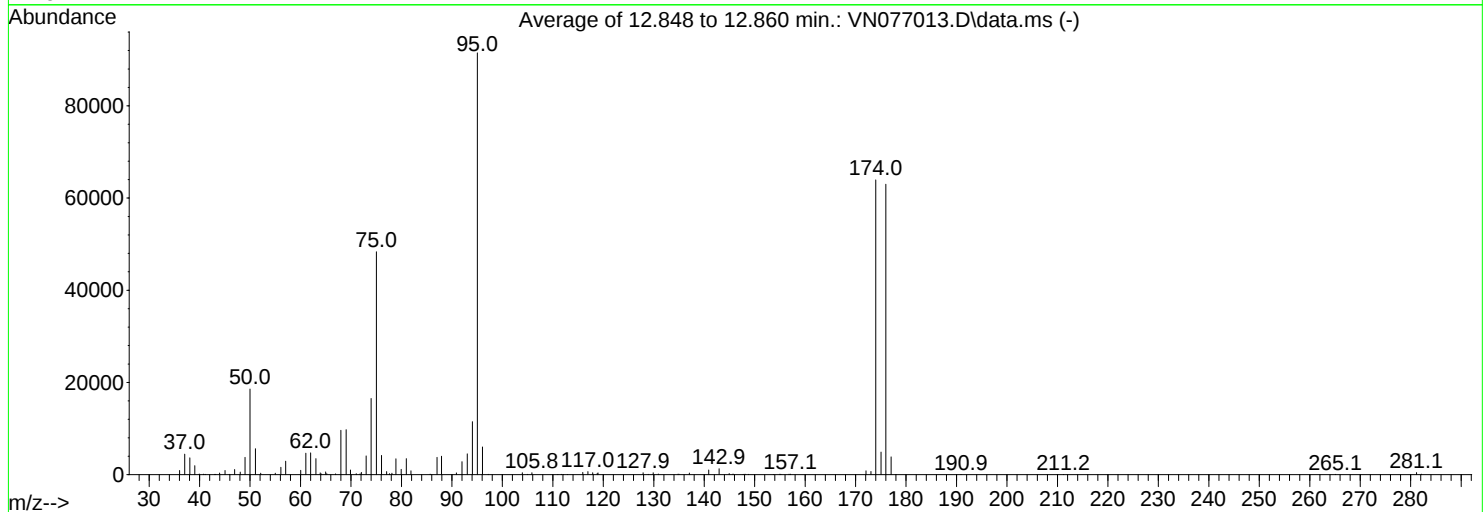


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031623\
Data File : VN077013.D
Acq On : 16 Mar 2023 10:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N030823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Mar 09 04:16:54 2023

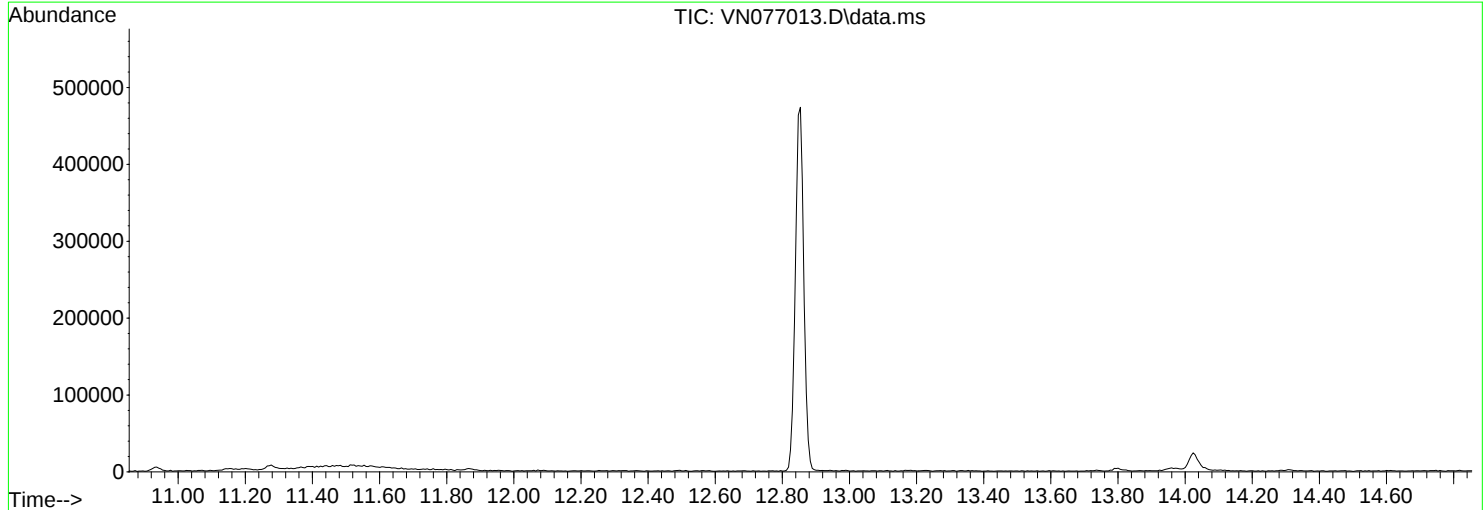

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	18556	PASS
75	95	30	60	52.8	48344	PASS
95	95	100	100	100.0	91504	PASS
96	95	5	9	6.6	5997	PASS
173	174	0.00	2	1.1	681	PASS
174	95	50	100	69.9	63947	PASS
175	174	5	9	7.7	4907	PASS
176	174	95	101	98.5	62997	PASS
177	176	5	9	6.1	3867	PASS