


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN031720\
 Data File : VN060542.D
 Acq On : 17 Mar 2020 8:15
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
 Title : SW846 8260
 Last Update : Thu Feb 27 13:52:50 2020

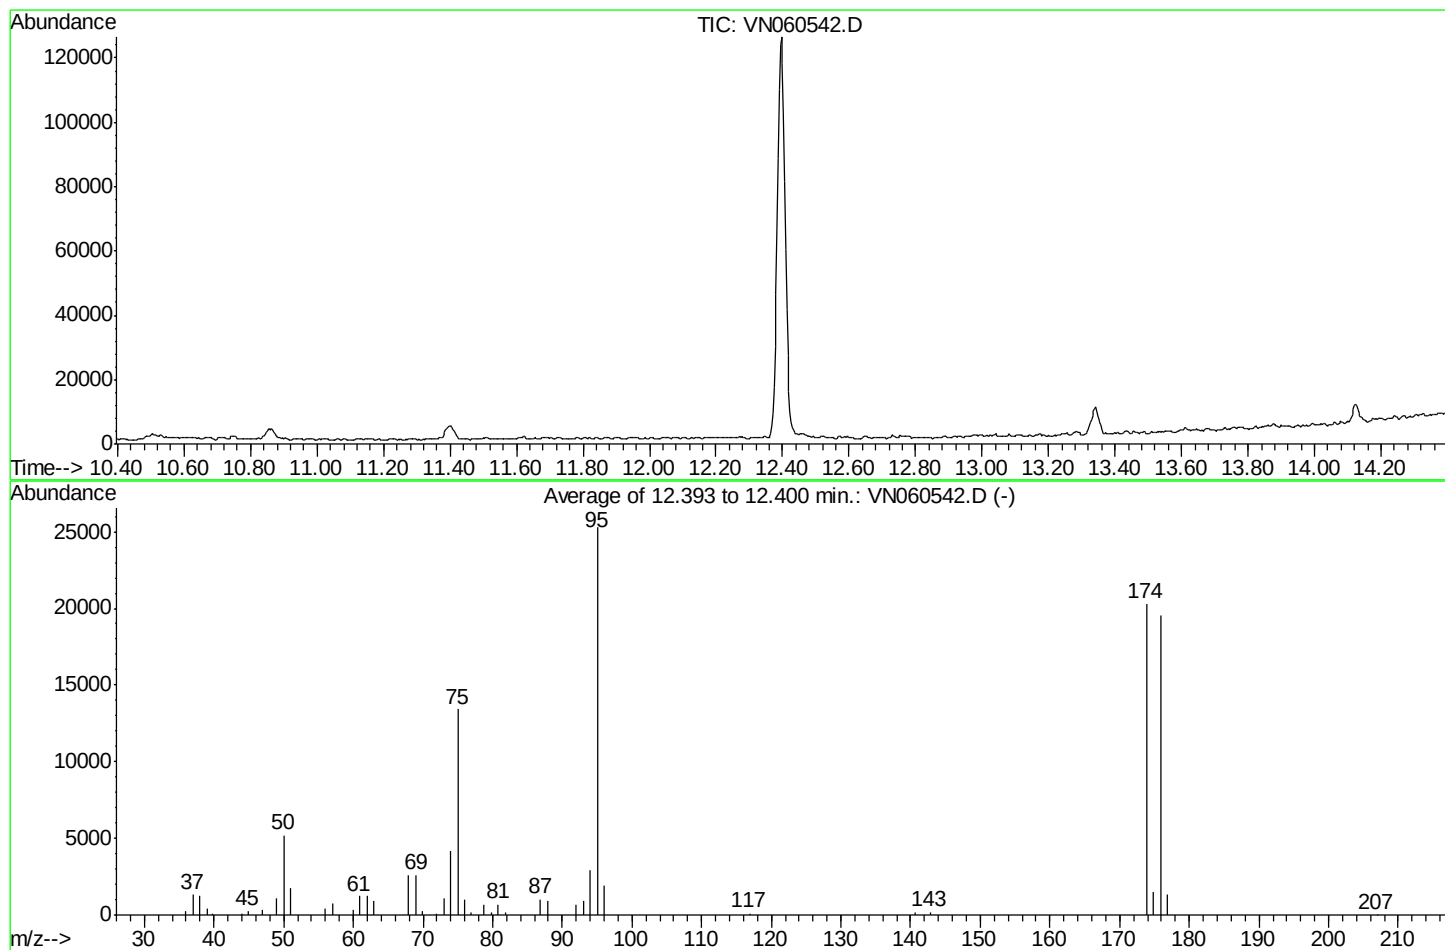

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	5177	PASS
75	95	30	60	53.0	13407	PASS
95	95	100	100	100.0	25288	PASS
96	95	5	9	7.6	1921	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.2	20290	PASS
175	174	5	9	7.2	1469	PASS
176	174	95	101	96.4	19554	PASS
177	176	5	9	7.1	1380	PASS