


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031721\
Data File : VN066226.D
Acq On : 17 Mar 2021 9:59
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031621W.M
Title : SW846 8260
Last Update : Wed Mar 17 05:05:15 2021

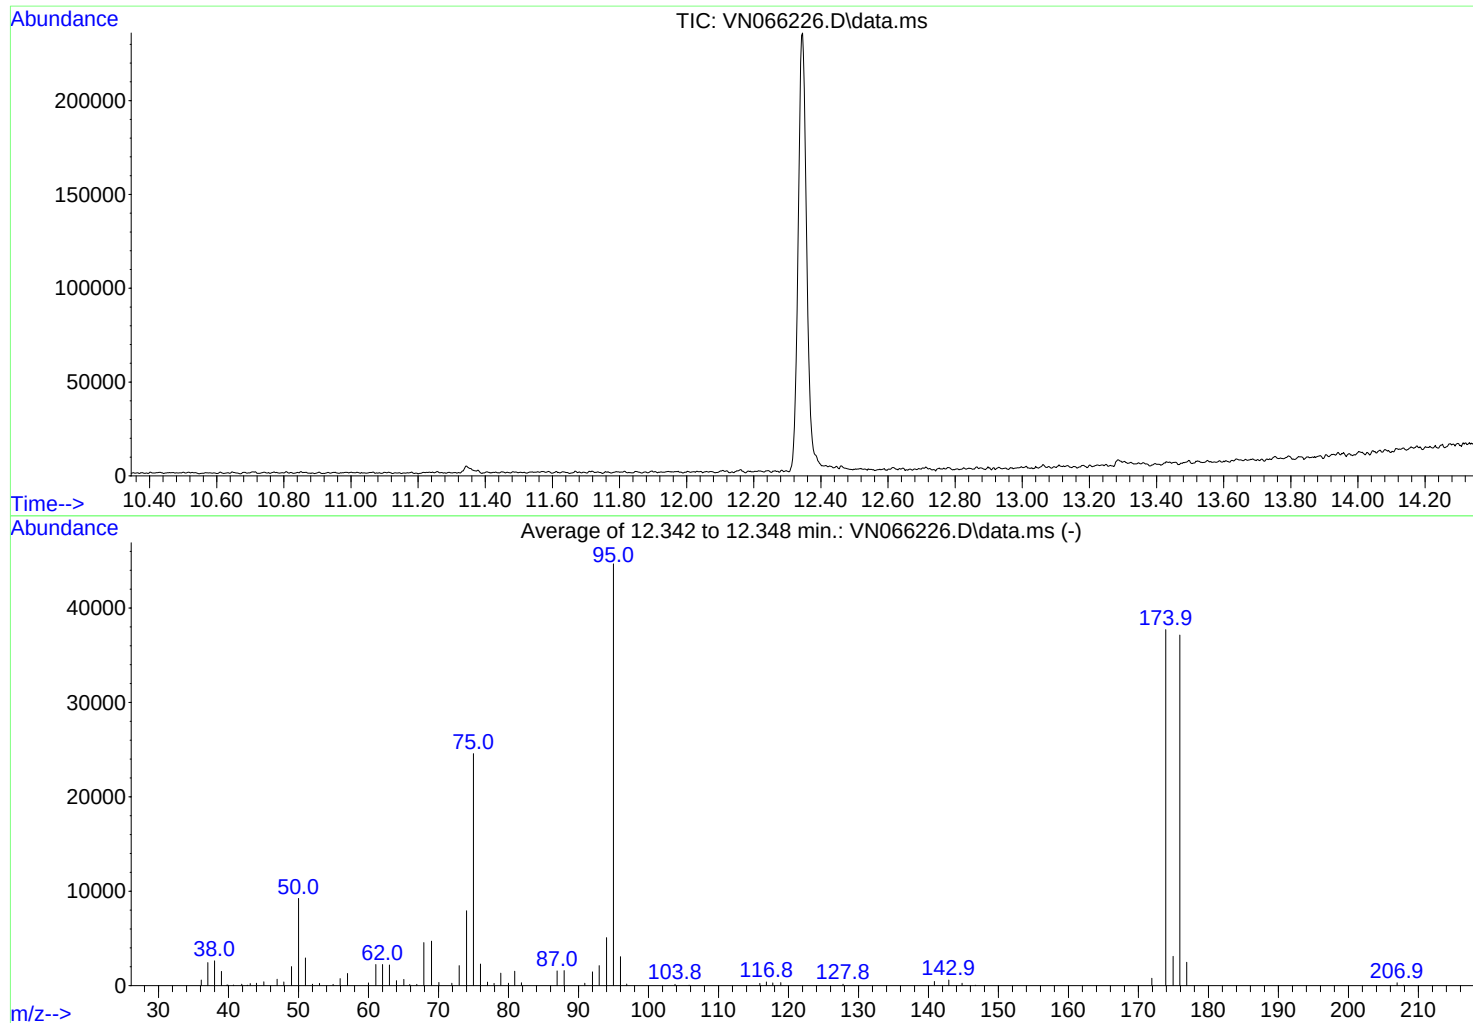

AutoFind: Scans 3972, 3973, 3974; Background Corrected with Scan 3956

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	9234	PASS
75	95	30	60	55.0	24571	PASS
95	95	100	100	100.0	44685	PASS
96	95	5	9	6.9	3064	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.4	37715	PASS
175	174	5	9	8.2	3111	PASS
176	174	95	101	98.5	37147	PASS
177	176	5	9	6.7	2483	PASS