


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031722\
 Data File : VN071336.D
 Acq On : 16 Mar 2022 22:50
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N031722W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Mar 17 06:37:08 2022

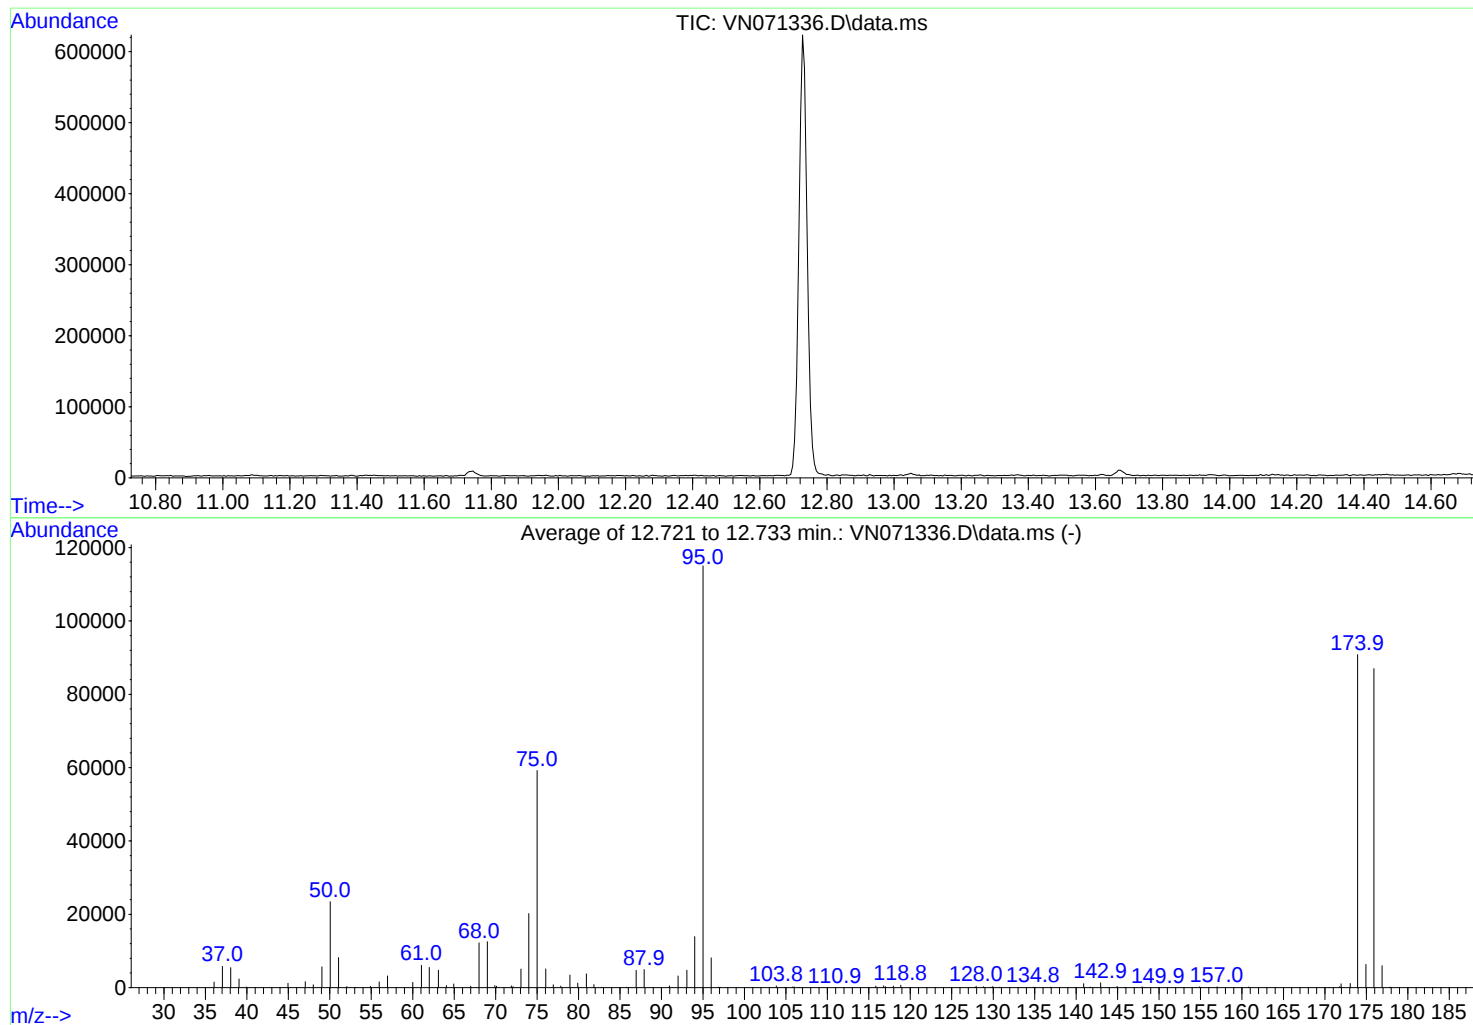

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	23445	PASS
75	95	30	60	51.5	59235	PASS
95	95	100	100	100.0	115027	PASS
96	95	5	9	7.1	8124	PASS
173	174	0.00	2	1.3	1148	PASS
174	95	50	100	78.9	90784	PASS
175	174	5	9	7.0	6348	PASS
176	174	95	101	95.8	86997	PASS
177	176	5	9	6.9	5995	PASS