
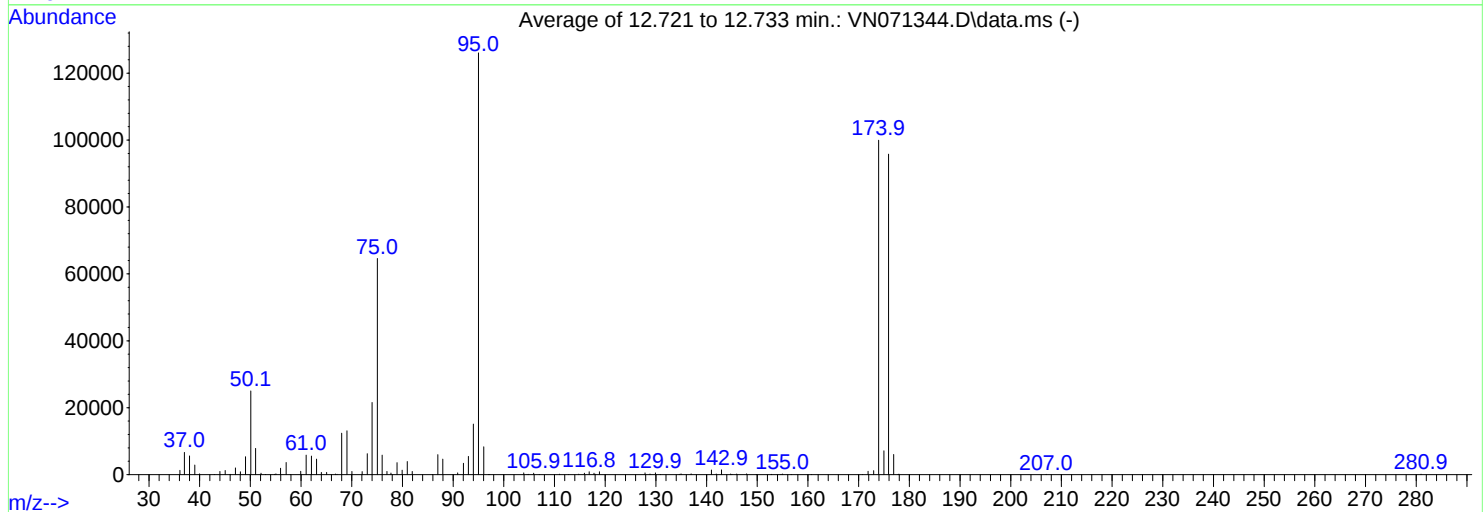


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN031722\  
 Data File : VN071344.D  
 Acq On : 17 Mar 2022 09:50  
 Operator : JC\MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N031722W.M  
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
 Last Update : Thu Mar 17 06:37:08 2022

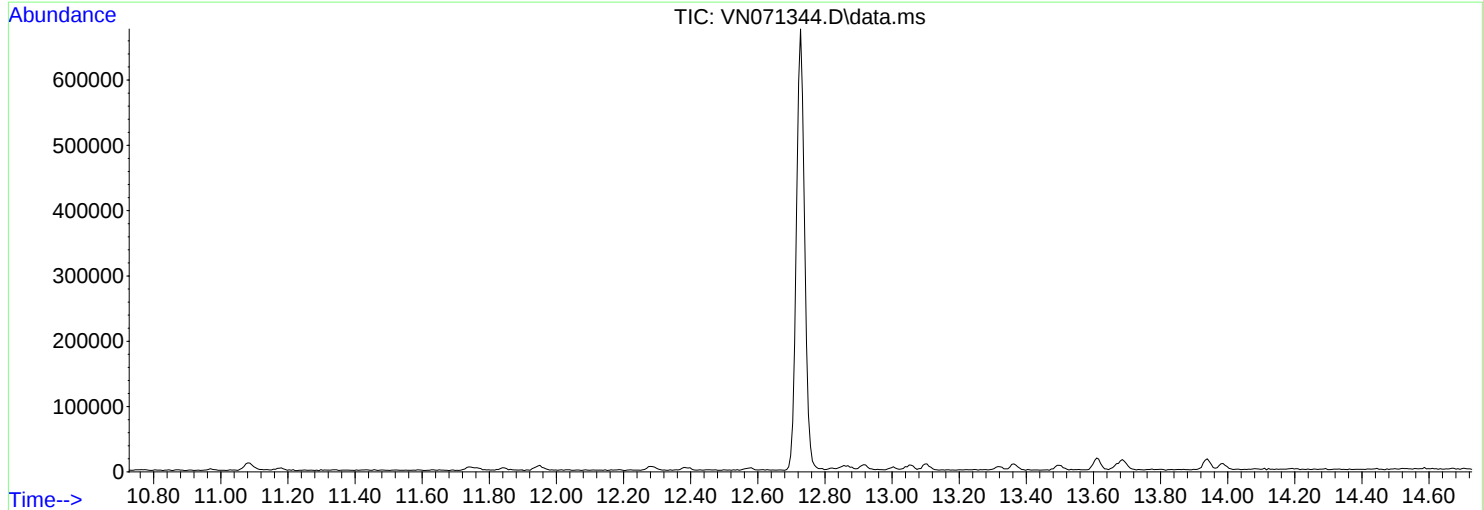

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.8         | 25013      | PASS                |
| 75             | 95              | 30              | 60              | 51.3         | 64627      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 126067     | PASS                |
| 96             | 95              | 5               | 9               | 6.6          | 8319       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 1190       | PASS                |
| 174            | 95              | 50              | 100             | 79.3         | 99968      | PASS                |
| 175            | 174             | 5               | 9               | 7.1          | 7108       | PASS                |
| 176            | 174             | 95              | 101             | 95.8         | 95787      | PASS                |
| 177            | 176             | 5               | 9               | 6.3          | 6008       | PASS                |