
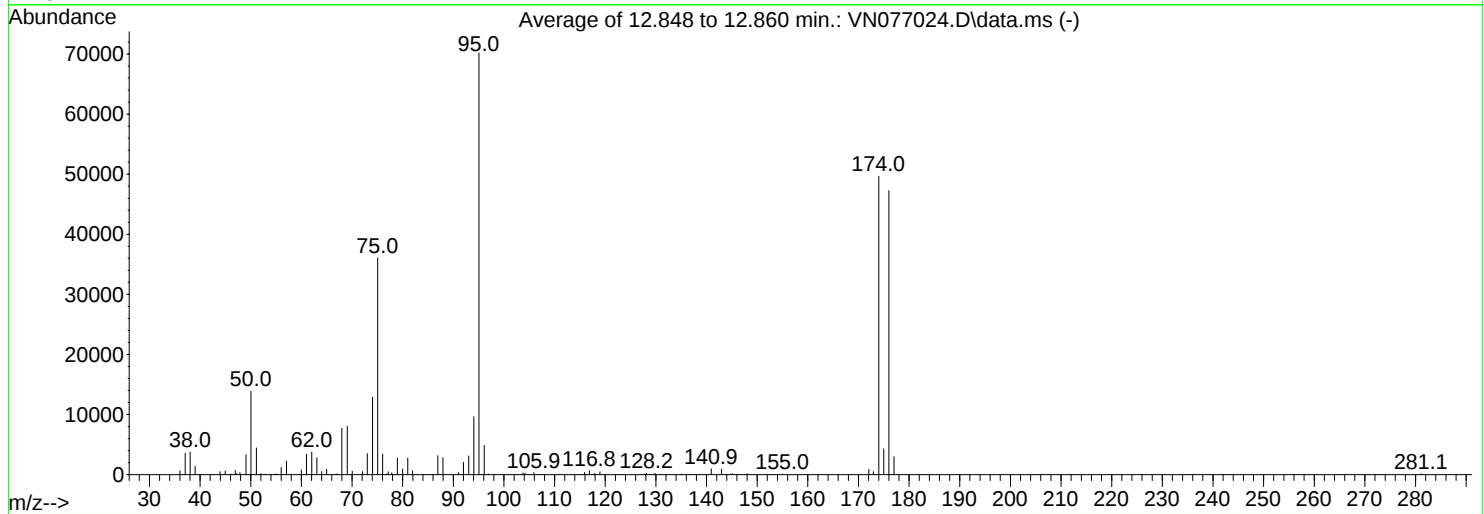


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031723\
Data File : VN077024.D
Acq On : 17 Mar 2023 08:30
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031723W.M
Title : SW846 8260
Last Update : Mon Mar 20 08:50:30 2023

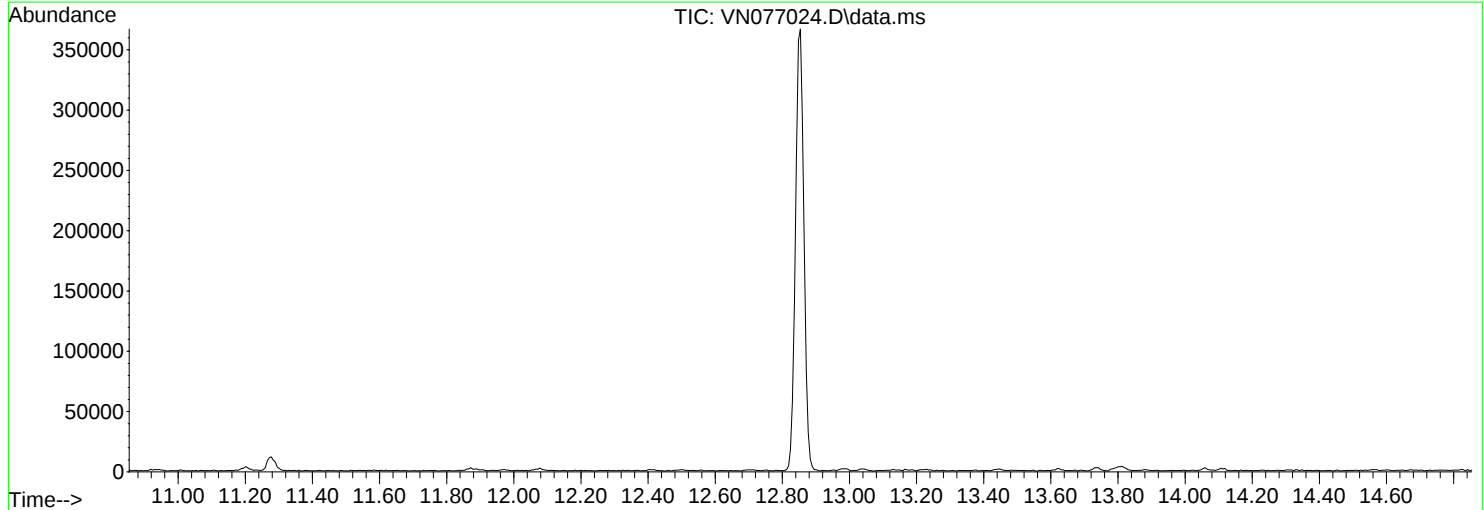

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	13873	PASS
75	95	30	60	51.4	36072	PASS
95	95	100	100	100.0	70200	PASS
96	95	5	9	7.0	4881	PASS
173	174	0.00	2	1.0	513	PASS
174	95	50	100	70.7	49661	PASS
175	174	5	9	8.6	4284	PASS
176	174	95	101	95.2	47277	PASS
177	176	5	9	6.3	2990	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	628	50.05	13873	62.05	3762	73.00	349
37.05	3580	51.10	4455	63.05	2812	74.05	1290
38.05	3721	52.00	150	64.00	517	75.05	3607
39.00	1423	52.90	88	65.00	915	76.05	340
43.95	499	54.90	81	66.70	51	76.90	111
44.95	621	55.15	111	66.90	91	77.15	473
46.10	112	56.00	1212	67.20	78	77.85	301
46.95	695	57.05	2255	68.00	7685	78.95	2760
47.20	190	58.00	116	69.05	8032	80.00	936
47.85	358	60.00	799	70.05	581	81.00	2783
49.05	3305	61.00	3407	72.05	503	81.95	632

Average of 12.848 to 12.860 min.: VN077024.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	3177	105.90	341	129.00	61	146.00	51
87.95	2817	106.80	61	129.70	109	148.00	169
91.05	345	111.00	54	129.85	178	149.60	58
92.00	2067	115.90	340	130.10	61	155.00	124
93.05	3131	116.85	672	135.00	70	172.05	870
94.05	9644	117.70	55	136.80	67	172.95	513
95.05	70200	117.80	87	140.95	949	174.00	49661
96.10	4881	117.95	177	142.95	924	175.00	4284
96.90	119	118.95	468	143.90	51	176.00	47277
103.75	306	127.80	78	144.80	72	177.00	2990
104.15	247	128.15	253	145.10	178	281.10	145

Instrument :

MSVOA_N

ClientSampleId :

BFB