
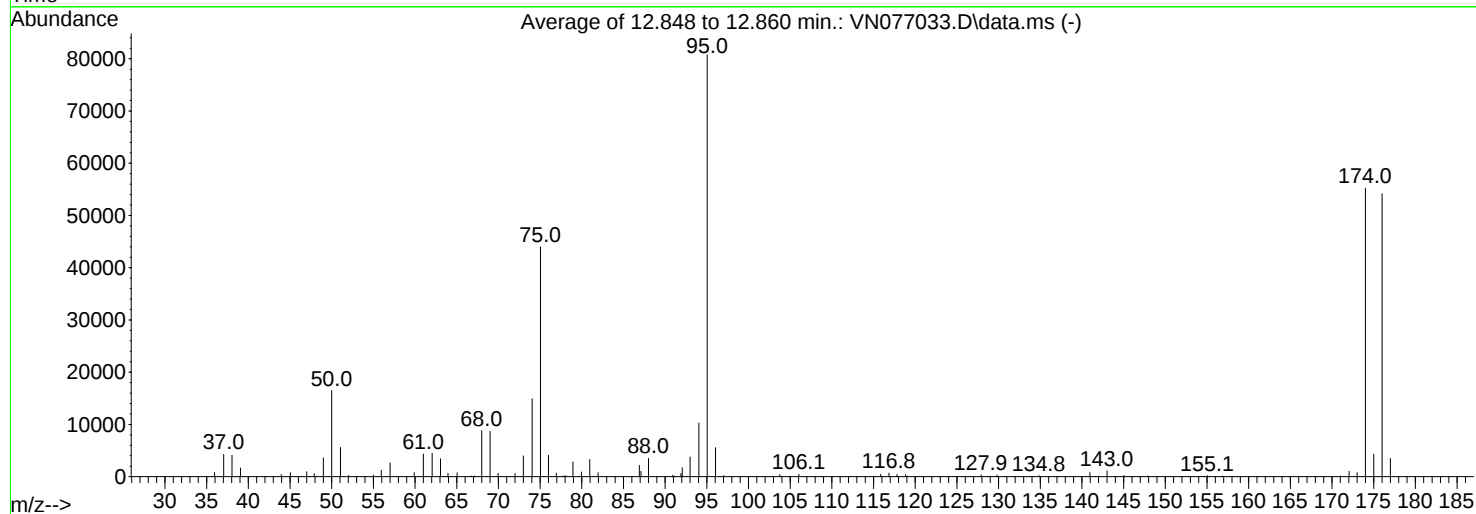


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031723\
Data File : VN077033.D
Acq On : 17 Mar 2023 13:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031723W.M
Title : SW846 8260
Last Update : Mon Mar 20 08:50:30 2023

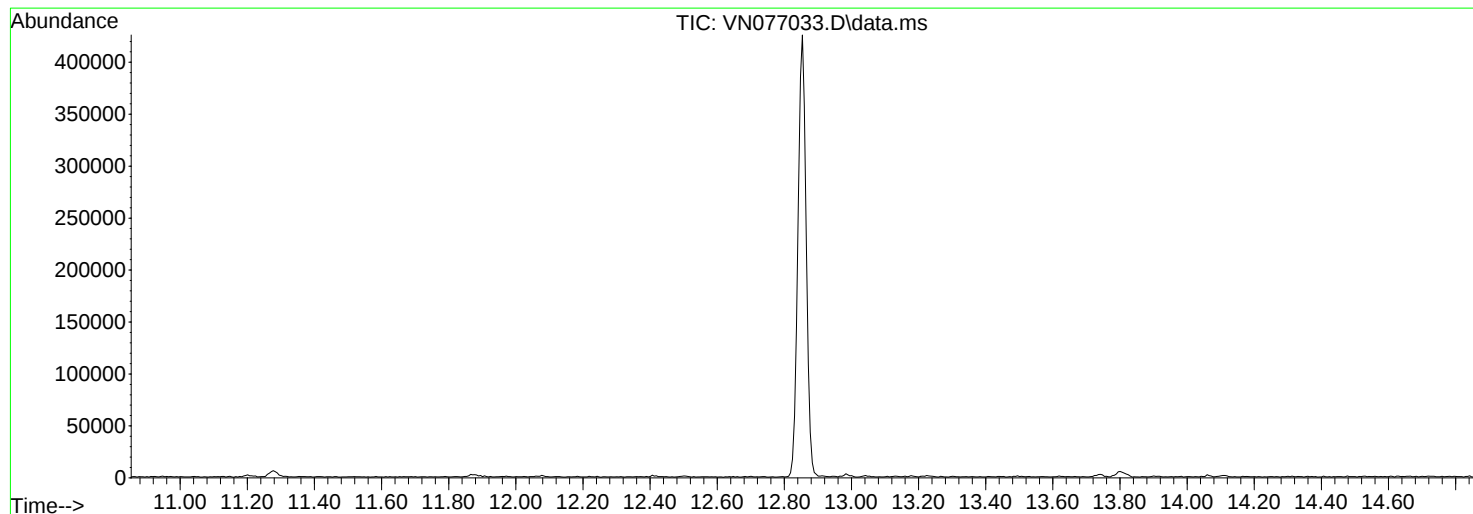

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	16488	PASS
75	95	30	60	54.5	43984	PASS
95	95	100	100	100.0	80749	PASS
96	95	5	9	6.9	5555	PASS
173	174	0.00	2	1.4	770	PASS
174	95	50	100	68.4	55219	PASS
175	174	5	9	7.7	4278	PASS
176	174	95	101	98.1	54144	PASS
177	176	5	9	6.4	3480	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	813	52.05	253	67.10	153	77.90	161
37.05	4271	55.00	292	68.00	8828	78.10	171
38.05	4122	55.95	1235	69.00	8660	78.95	282
39.05	1642	57.00	2639	69.95	633	79.95	89
43.95	398	59.90	778	72.00	587	80.95	3285
45.05	765	61.00	4334	73.00	3970	81.95	781
47.00	938	62.05	4474	74.05	14922	86.00	54
47.90	590	63.05	3447	75.05	43984	86.90	2142
49.00	3596	63.95	605	76.00	4061	87.10	1045
50.00	16488	65.05	726	76.95	675	88.00	3493
51.05	5577	66.75	125	77.70	88	90.90	254

Average of 12.848 to 12.860 min.: VN077033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.10	102	115.85	426	140.95	786	173.00	770
91.90	627	116.85	671	141.60	57	174.00	55219
92.05	1726	117.80	426	142.00	104	175.00	4278
93.00	3765	118.85	371	143.00	1136	176.00	54144
94.05	10274	119.10	139	145.05	214	177.00	3480
95.05	80749	127.90	341	147.95	137		
96.05	5555	128.70	54	154.70	56		
97.05	230	129.00	85	155.05	192		
103.75	407	129.80	307	156.85	118		
104.90	68	130.70	56	171.00	118		
106.05	474	134.85	176	172.05	1023		

Instrument :

MSVOA_N

ClientSampleId :

BFB