

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN031819\
 Data File : VN054394.D
 Acq On : 18 Mar 2019 15:21
 Operator : JC/SP
 Sample : K1970-11
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VOC-TRIP-BLANK

Quant Time: Mar 19 05:12:33 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 13 03:33:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	1874278	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	2664739	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	2228722	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	796216	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	882321	44.33	ug/l	0.00
Spiked Amount			Recovery	=	88.66%	
35) Dibromofluoromethane	7.59	113	798915	46.49	ug/l	0.00
Spiked Amount			Recovery	=	92.98%	
50) Toluene-d8	10.09	98	3075283	48.45	ug/l	0.00
Spiked Amount			Recovery	=	96.90%	
62) 4-Bromofluorobenzene	12.40	95	907548	40.86	ug/l	0.00
Spiked Amount			Recovery	=	81.72%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Methyl Iodide	3.93	142	325	1.508	ug/l #	19
13) Acrolein	3.62	56	578	0.447	ug/l #	31
16) Acetone	3.82	43	2597	0.456	ug/l	91
31) Cyclohexane	7.66	56	26308	Below Cal	#	1
36) 1,1-Dichloropropene	7.67	75	106685	4.347	ug/l #	48
38) Carbon Tetrachloride	7.66	117	154194	5.992	ug/l #	16
43) Isopropyl Acetate	8.28	43	9213	0.372	ug/l #	60
49) 1,4-Dioxane	8.93	88	68	0.383	ug/l #	27
51) 4-Methyl-2-Pentanone	10.09	43	9788	0.747	ug/l #	1
71) Bromoform	12.40	173	6253	2.790	ug/l #	1
76) 1,2,3-Trichloropropane	12.40	75	434105	37.075	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.40	75	434105	126.740	ug/l #	11
93) 1,2,4-Trichlorobenzene	14.91	180	1431	2.598	ug/l	85
95) Naphthalene	15.13	128	7214	3.662	ug/l #	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN031819\
Data File : VN054394.D
Acq On : 18 Mar 2019 15:21
Operator : JC/SP
Sample : K1970-11
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VOC-TRIP-BLANK

Quant Time: Mar 19 05:12:33 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 13 03:33:31 2019
Response via : Initial Calibration

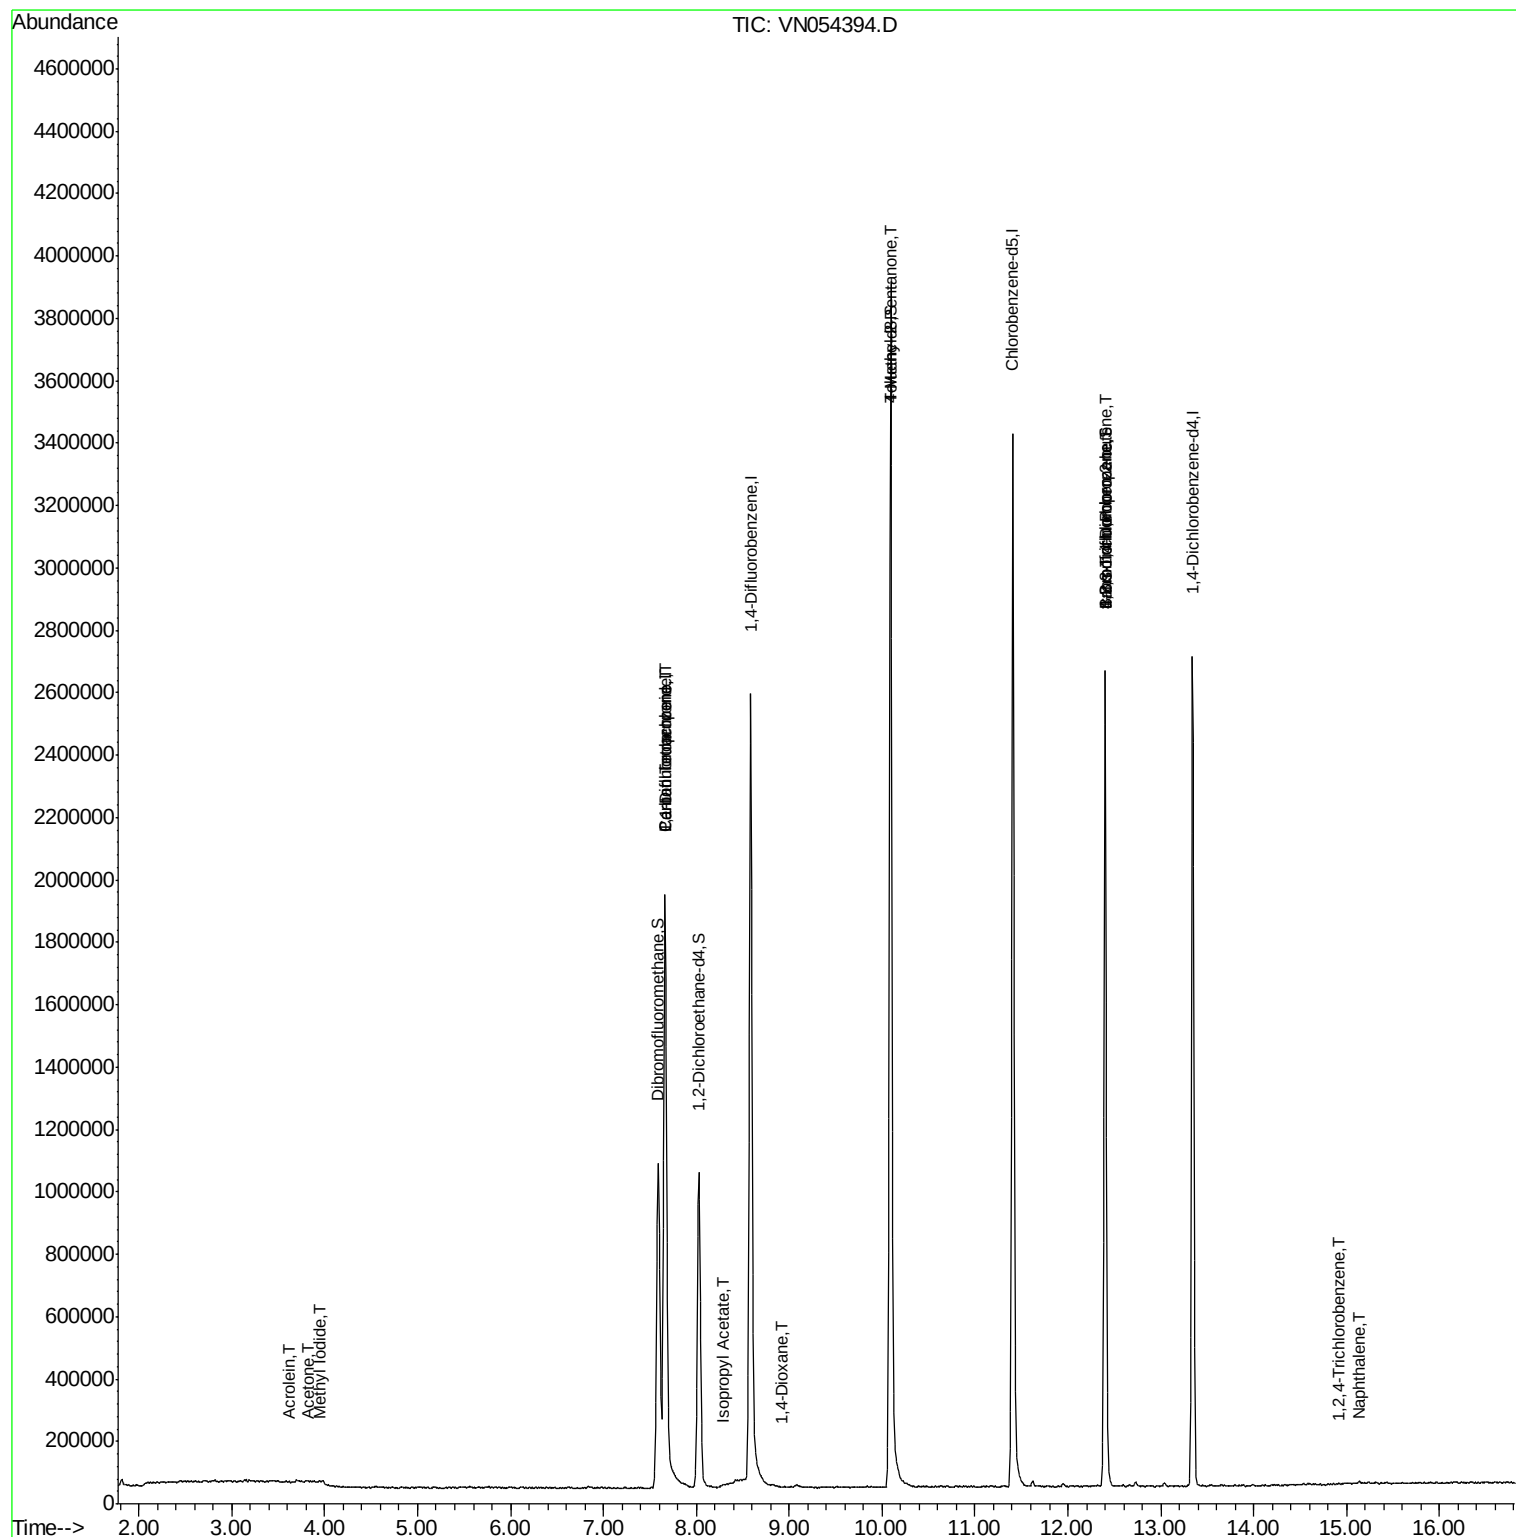

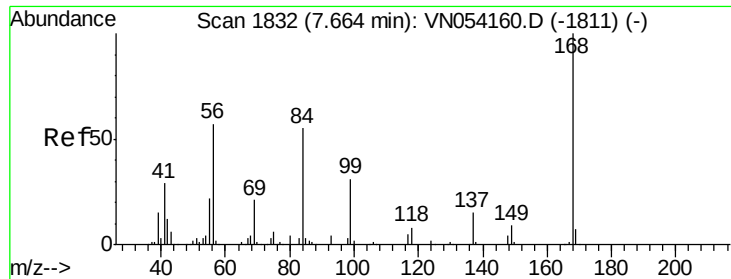

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN054394.D

Acq: 18 Mar 2019 15:21

Instrument :

MSVOA_N

ClientSampleId :


VOC-TRIP-BLANK

Tot Ion:168 Resp: 1874278

Ion Ratio Lower Upper

168 100

99 47.0 37.1 55.7



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.67

800000

600000



400000

200000

0

Time-->

7.50 7.60 7.70 7.80 7.90



#10

Methyl Iodide

Concen: 1.508 ug/l

RT: 3.93 min Scan# 671

Delta R.T. -0.01 min

Lab File: VN054394.D

Acq: 18 Mar 2019 15:21


Tgt Ion:142 Resp: 325

Ion Ratio Lower Upper

142 100

127 96.9 30.3 45.5#

141 0.0 11.2 16.8#



Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

3.93

300


200


100

0

Time-->

3.90 3.91 3.92 3.93 3.94





#13

Acrolein

Concen: 0.447 ug/l

RT: 3.62 min Scan# 573

Delta R.T. 0.01 min

Lab File: VN054394.D

Acq: 18 Mar 2019 15:21

Instrument :

MSVOA_N

ClientSampleId :





VOC-TRIP-BLANK

Tot Ion: 56 Resp: 578

Ion Ratio Lower Upper

56 100

55 13.5 56.7 85.1#

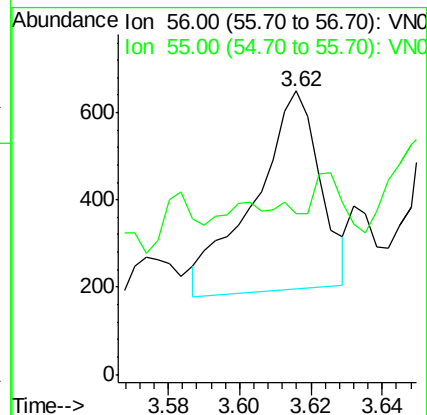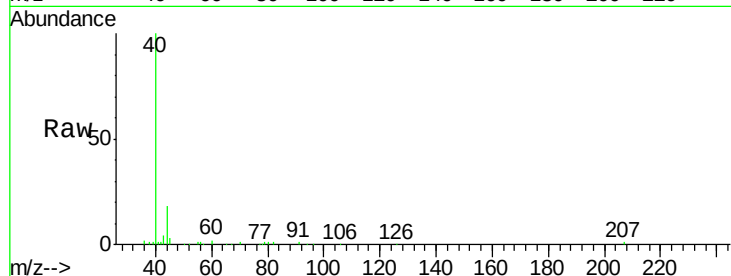

#16

Acetone

Concen: 0.456 ug/l

RT: 3.82 min Scan# 637

Delta R.T. 0.00 min

Lab File: VN054394.D




Acq: 18 Mar 2019 15:21


Tgt Ion: 43 Resp: 2597

Ion Ratio Lower Upper

43 100

58 32.3 29.9 44.9

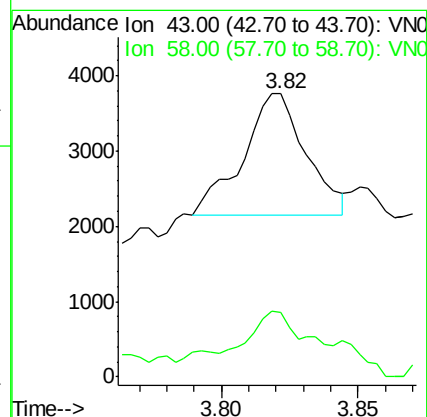

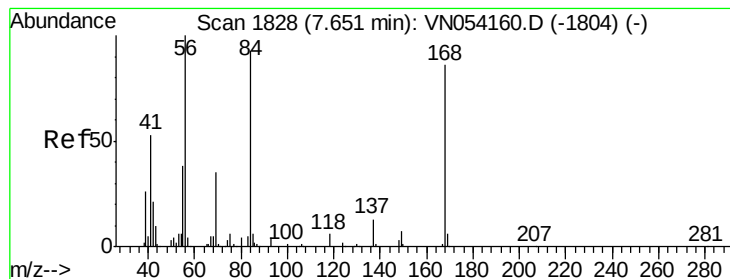

#31

Cyclohexane

Concen: Below Cal

RT: 7.66 min Scan# 1832

Delta R.T. 0.01 min


Lab File: VN054394.D

Acq: 18 Mar 2019 15:21




Instrument :
MSVOA_N
ClientSampleId :
VOC-TRIP-BLANK

Tot Ion: 56 Resp: 26308

Ion	Ratio	Lower	Upper
56	100		
69	182.4	27.8	41.6#
84	145.8	74.6	111.8#

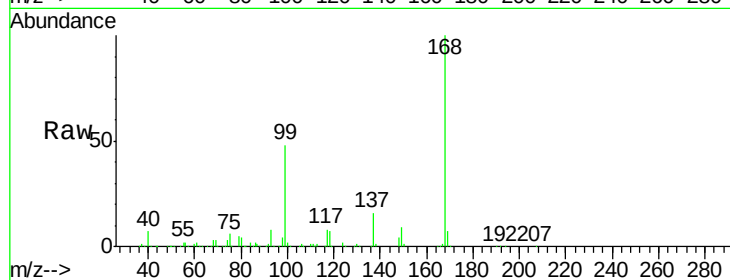

Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0

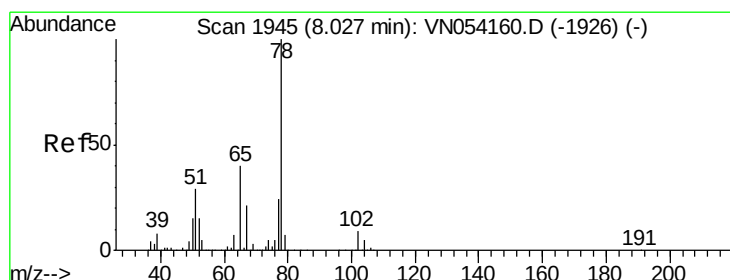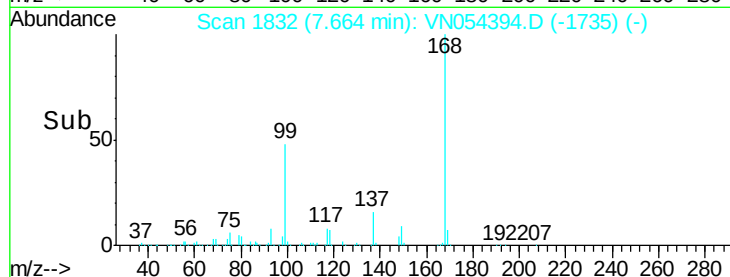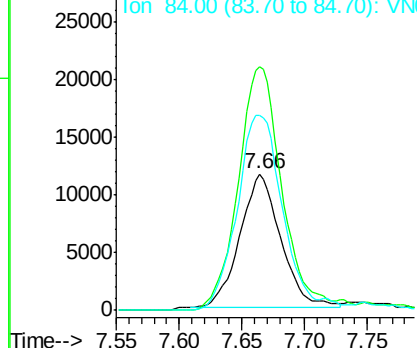

#33

1,2-Dichloroethane-d4

Concen: 44.327 ug/l

RT: 8.03 min Scan# 1945


Delta R.T. 0.00 min

Lab File: VN054394.D



Acq: 18 Mar 2019 15:21


Tgt Ion: 65 Resp: 882321

Ion	Ratio	Lower	Upper
65	100		
67	52.3	0.0	104.6

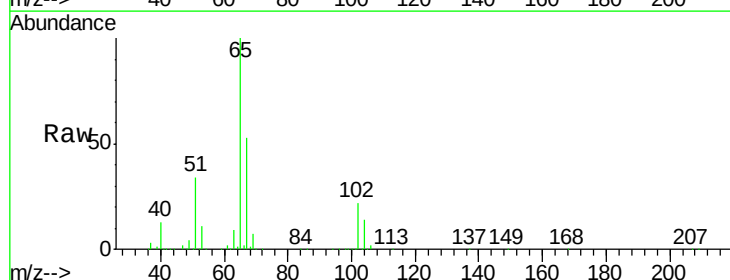

Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

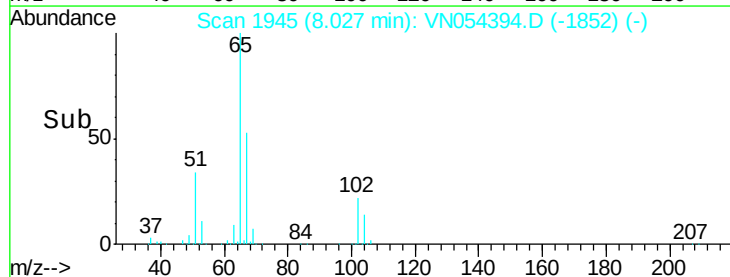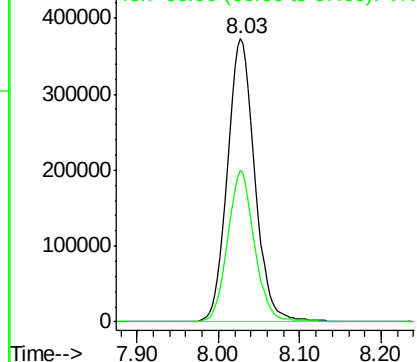







#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN054394.D
 Acq: 18 Mar 2019 15:21

Instrument :
 MSVOA_N
 ClientSampleId :
 VOC-TRIP-BLANK

Tot Ion:114 Resp: 2664739
 Ion Ratio Lower Upper
 114 100
 63 17.9 0.0 35.2
 88 15.0 0.0 30.2

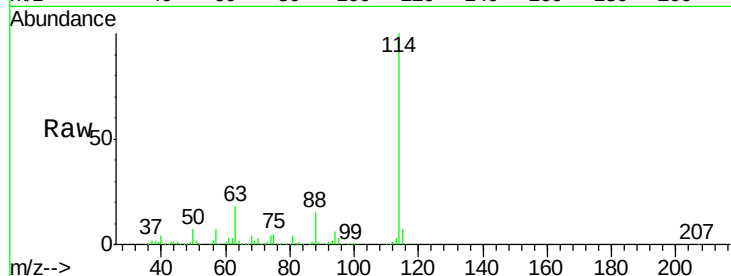


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): V
 Ion 87.90 (87.60 to 88.60): V


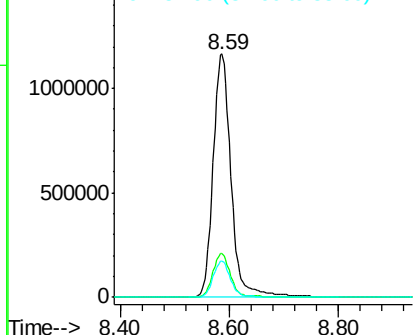



#35
 Dibromofluoromethane
 Concen: 46.485 ug/l
 RT: 7.59 min Scan# 1809
 Delta R.T. 0.00 min
 Lab File: VN054394.D
 Acq: 18 Mar 2019 15:21

Tgt Ion:113 Resp: 798915
 Ion Ratio Lower Upper
 113 100
 111 103.2 82.2 123.4
 192 23.6 19.2 28.8



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V




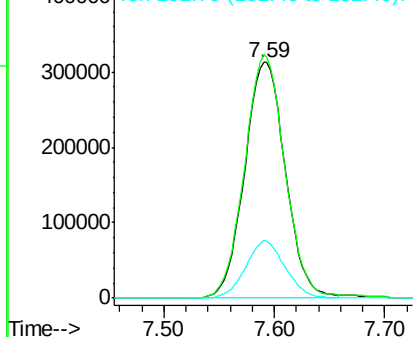


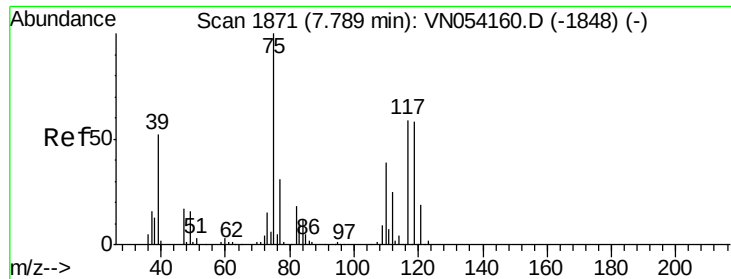

#36
 1,1-Dichloropropene
 Concen: 4.347 ug/l
 RT: 7.67 min Scan# 1833
 Delta R.T. -0.12 min
 Lab File: VN054394.D
 Acq: 18 Mar 2019 15:21




Instrument :
 MSVOA_N
 ClientSampleId :
 VOC-TRIP-BLANK


Tot Ion	Ratio	Lower	Upper
75	100		
110	9.3	19.1	57.5#
77	0.0	25.0	37.4#

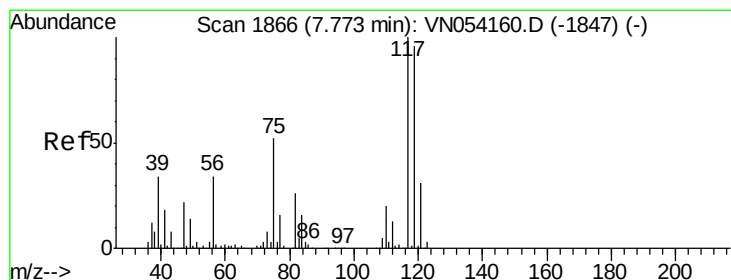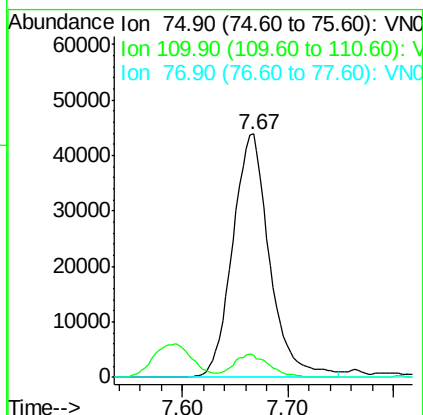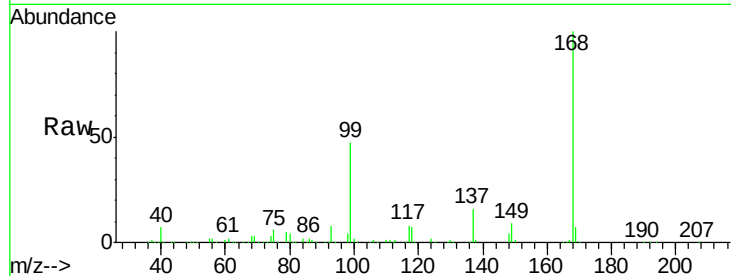

#38
 Carbon Tetrachloride
 Concen: 5.992 ug/l
 RT: 7.66 min Scan# 1832
 Delta R.T. -0.11 min
 Lab File: VN054394.D
 Acq: 18 Mar 2019 15:21

Tgt Ion	Ratio	Lower	Upper
117	100		
119	5.2	76.3	114.5#
121	0.0	24.6	36.8#

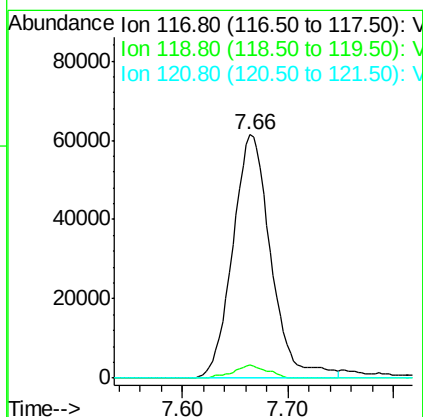

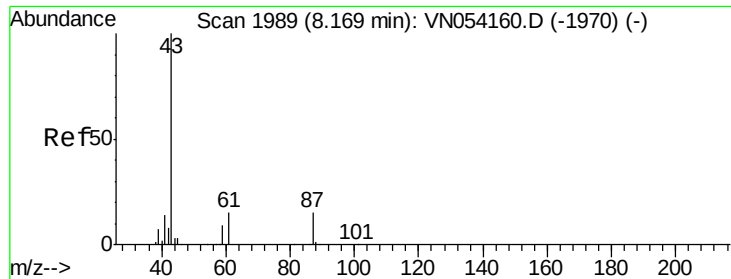

#43

Isopropyl Acetate

Concen: 0.372 ug/l

RT: 8.28 min Scan# 2024

Delta R.T. 0.11 min

Lab File: VN054394.D

Acq: 18 Mar 2019 15:21

Instrument :

MSVOA_N

ClientSampleId :

VOC-TRIP-BLANK





Tot Ion: 43 Resp: 9213

Ion Ratio Lower Upper

43 100

61 0.0 15.8 23.8#

87 0.0 12.0 18.0#

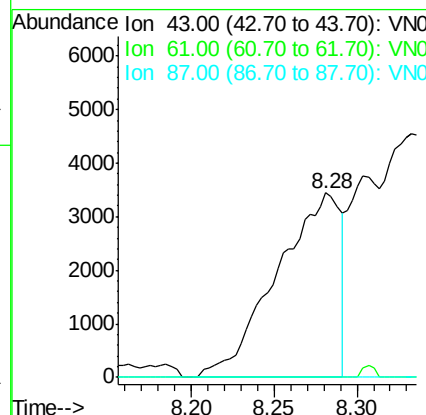

#49

1,4-Dioxane

Concen: 0.383 ug/l

RT: 8.93 min Scan# 2225

Delta R.T. -0.28 min

Lab File: VN054394.D

Acq: 18 Mar 2019 15:21




Tgt Ion: 88 Resp: 68


Ion Ratio Lower Upper

88 100

43 0.0 24.1 36.1#

58 0.0 50.8 76.2#

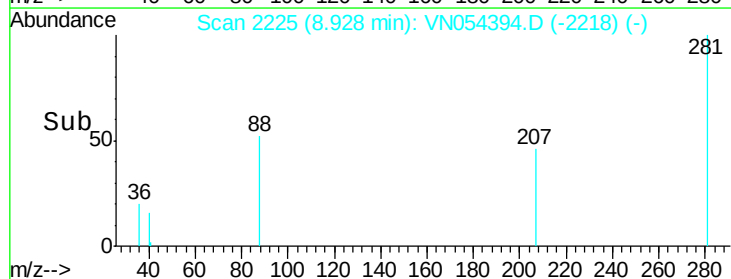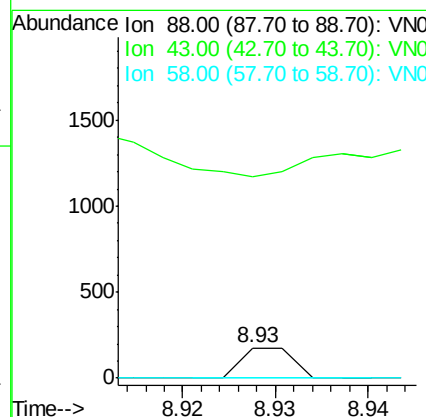



#50

Toluene-d8

Concen: 48.451 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN054394.D

Acq: 18 Mar 2019 15:21

Instrument :

MSVOA_N

ClientSampleId :


VOC-TRIP-BLANK

Tot Ion: 98 Resp: 3075283

Ion Ratio Lower Upper

98 100

100 63.9 51.2 76.8



Abundance Ion 98.00 (97.70 to 98.70): VN054160.D (-2569) (-)

Ion 100.00 (99.70 to 100.70): VN054160.D (-2569) (-)

1500000

1000000



500000

0

10.09

10.00 10.20

Time-->



#51

4-Methyl-2-Pentanone

Concen: 0.747 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.11 min

Lab File: VN054394.D


Acq: 18 Mar 2019 15:21

Tgt Ion: 43 Resp: 9788

Ion Ratio Lower Upper

43 100

58 219.7 31.8 47.6#



Abundance Ion 43.00 (42.70 to 43.70): VN054160.D (-2538) (-)

Ion 58.00 (57.70 to 58.70): VN054160.D (-2538) (-)

10000


5000


0

10.09

10.05 10.10

Time-->



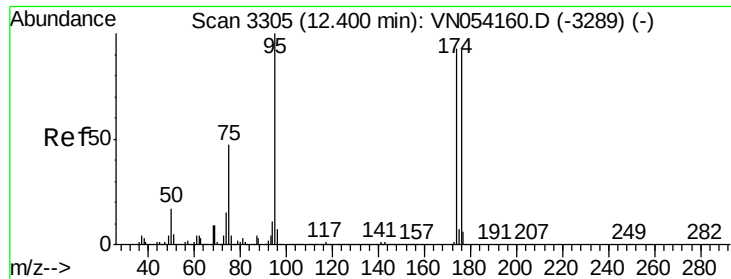

#62

4-Bromofluorobenzene

Concen: 40.864 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.00 min

Lab File: VN054394.D

Acq: 18 Mar 2019 15:21

Instrument :

MSVOA_N

ClientSampleId :

VOC-TRIP-BLANK


Tot Ion: 95 Resp: 907548

Ion Ratio Lower Upper

95 100

174 96.8 0.0 191.0




176 93.7 0.0 187.4

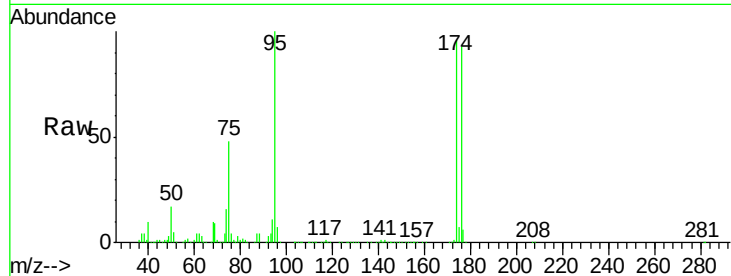

Abundance Ion 94.90 (94.60 to 95.60): VN054160.D (-3289) (-)

Ion 173.80 (173.50 to 174.50): VN054160.D (-3289) (-)

Ion 175.80 (175.50 to 176.50): VN054160.D (-3289) (-)

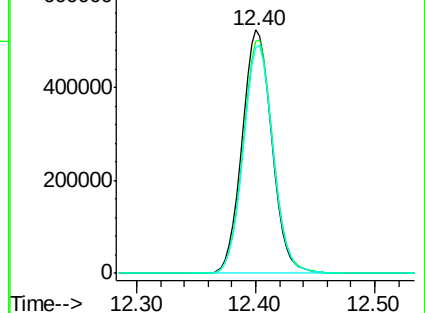

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. 0.00 min

Lab File: VN054394.D

Acq: 18 Mar 2019 15:21


Tgt Ion: 117 Resp: 2228722

Ion Ratio Lower Upper

117 100

82 50.1 40.0 60.0



119 32.3 25.8 38.6




Abundance Ion 116.90 (116.60 to 117.60): VN054160.D (-2980) (-)

Ion 82.00 (81.70 to 82.70): VN054160.D (-2980) (-)

Ion 118.90 (118.60 to 119.60): VN054160.D (-2980) (-)

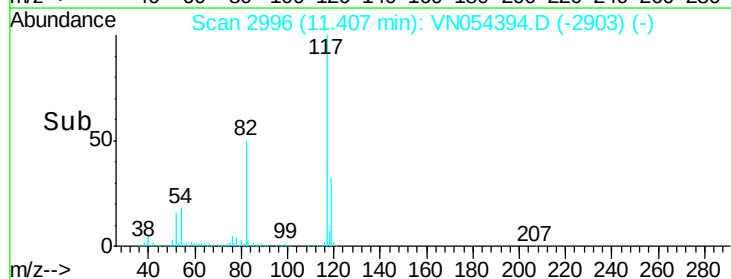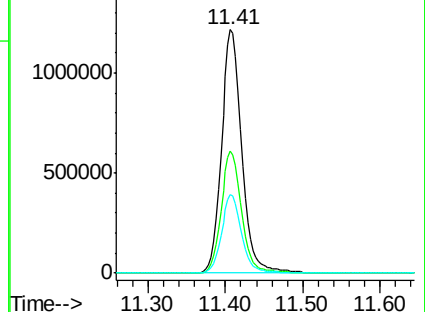

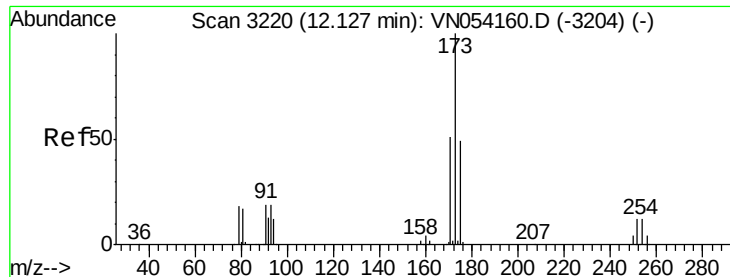

#71

Bromoform

Concen: 2.790 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.28 min

Lab File: VN054394.D

Acq: 18 Mar 2019 15:21

Instrument :

MSVOA_N

ClientSampleId :

VOC-TRIP-BLANK


Tot Ion:173 Resp: 6253

Ion Ratio Lower Upper




173 100

175 862.3 24.4 73.2#

254 0.0 0.1 0.1#

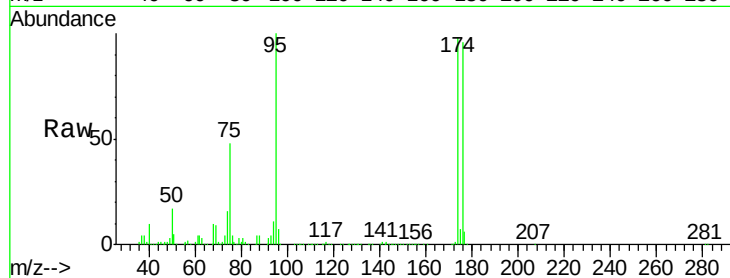

Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

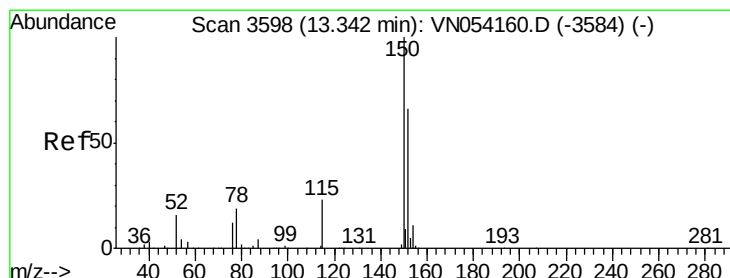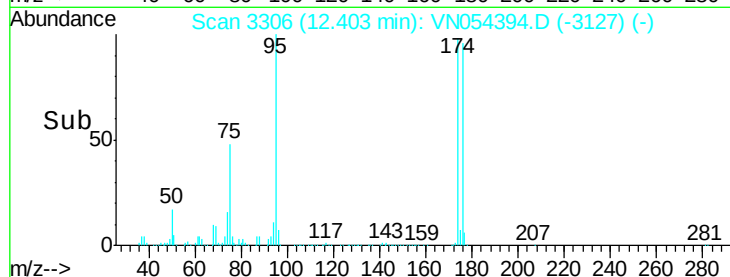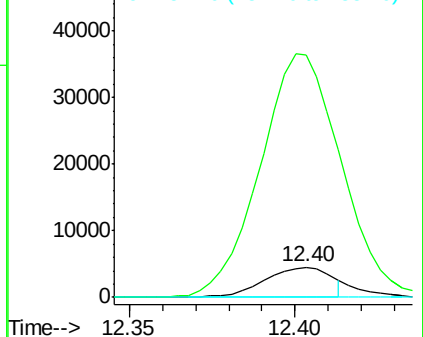

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. 0.00 min

Lab File: VN054394.D

Acq: 18 Mar 2019 15:21


Tgt Ion:152 Resp: 796216

Ion Ratio Lower Upper



152 100


115 54.5 27.2 81.6

150 157.2 0.0 349.2

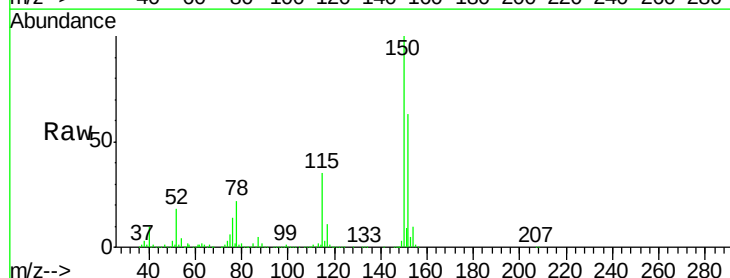

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V



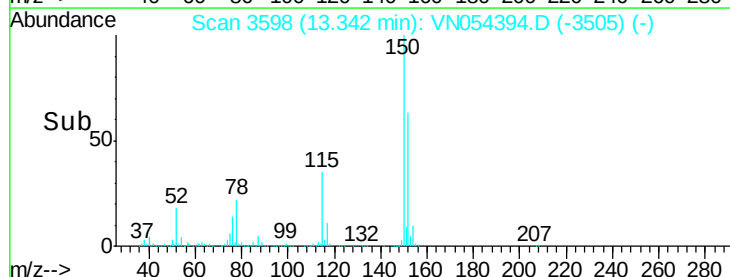
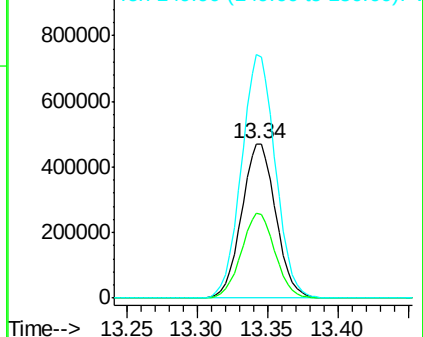


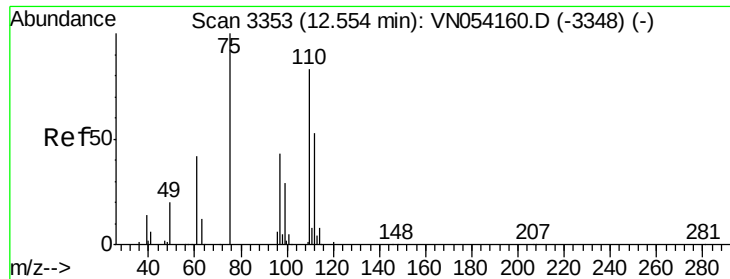

#76
 1,2,3-Trichloropropane
 Concen: 37.075 ug/l
 RT: 12.40 min Scan# 3305
 Delta R.T. -0.15 min
 Lab File: VN054394.D
 Acq: 18 Mar 2019 15:21




Instrument :
 MSVOA_N
 ClientSampleId :
 VOC-TRIP-BLANK


Tot Ion: 75 Resp: 434105
 Ion Ratio Lower Upper
 75 100
 77 1.3 0.0 0.0#

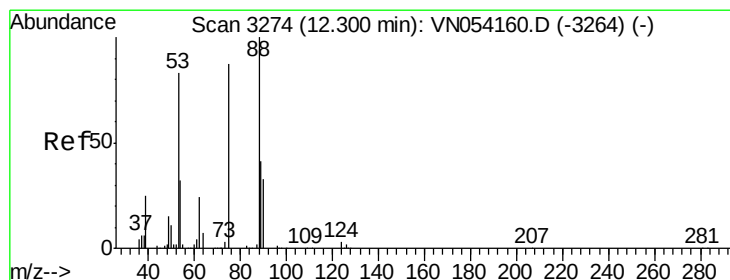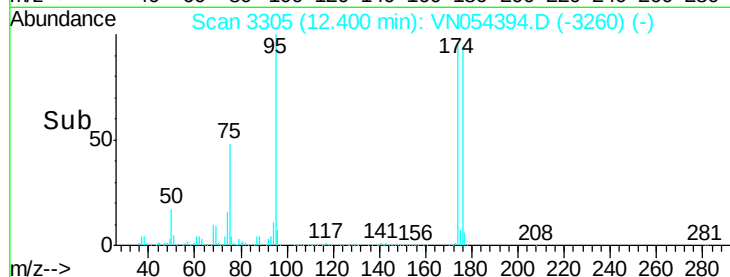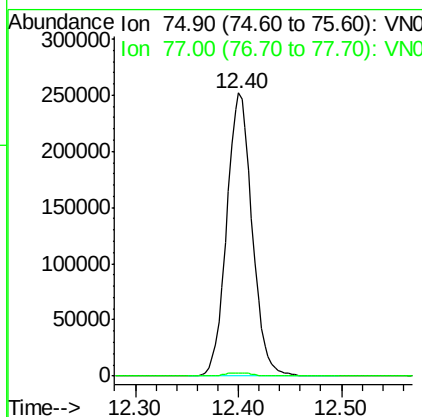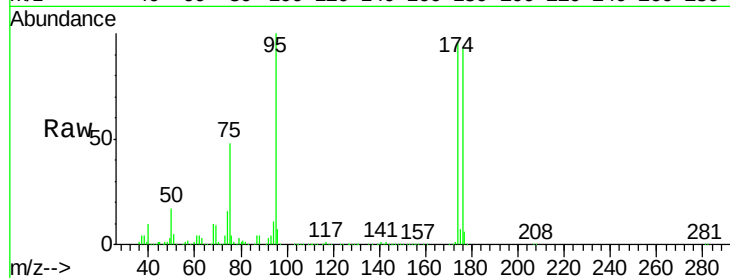

#81
 trans-1,4-Dichloro-2-butene
 Concen: 126.740 ug/l
 RT: 12.40 min Scan# 3305
 Delta R.T. 0.10 min
 Lab File: VN054394.D
 Acq: 18 Mar 2019 15:21

Tgt Ion: 75 Resp: 434105
 Ion Ratio Lower Upper
 75 100
 53 0.0 76.2 114.2#
 89 0.0 39.2 58.8#


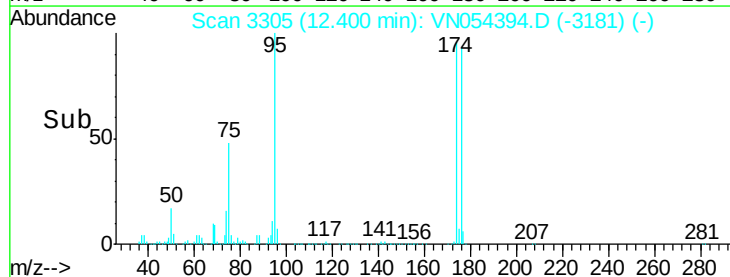
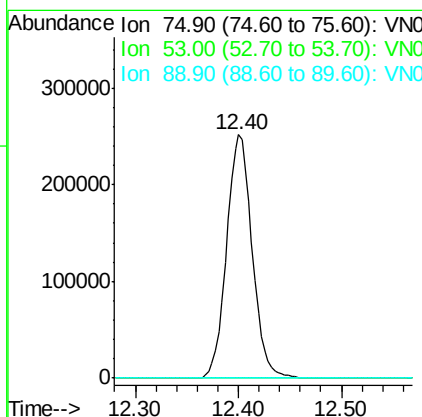
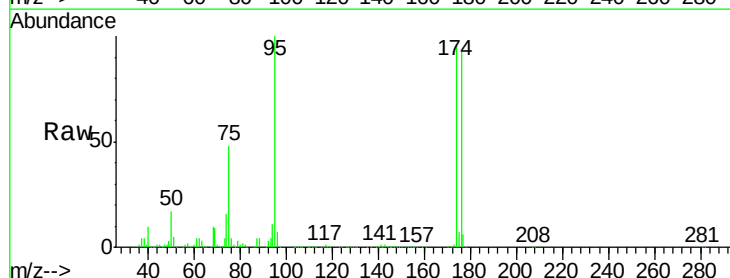




#93
 1,2,4-Trichlorobenzene
 Concen: 2.598 ug/l
 RT: 14.91 min Scan# 4085
 Delta R.T. 0.00 min
 Lab File: VN054394.D
 Acq: 18 Mar 2019 15:21

Instrument :
 MSVOA_N
 ClientSampleId :
 VOC-TRIP-BLANK

Tot Ion:180 Resp: 1431
 Ion Ratio Lower Upper
 180 100
 182 80.6 48.0 144.2
 145 35.6 14.2 42.8

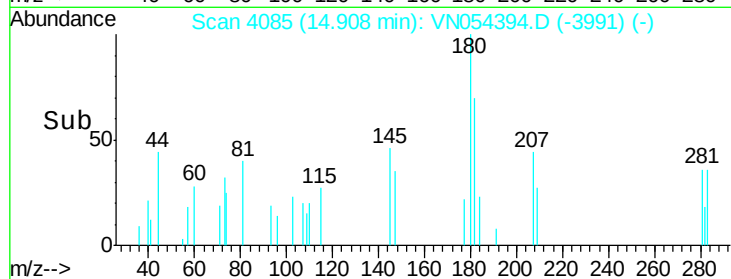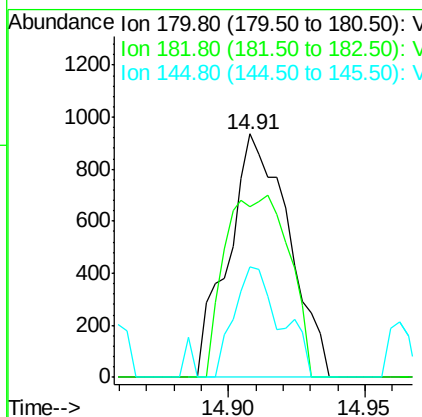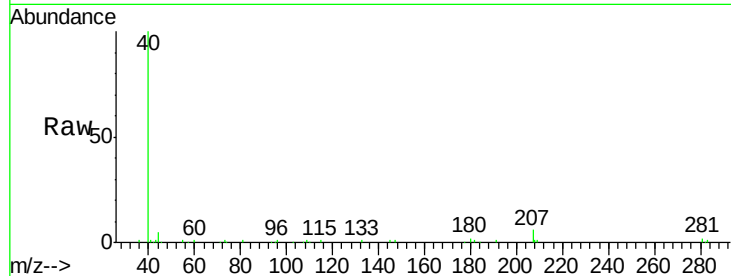

#95
 Naphthalene
 Concen: 3.662 ug/l
 RT: 15.13 min Scan# 4155
 Delta R.T. 0.00 min
 Lab File: VN054394.D
 Acq: 18 Mar 2019 15:21

Tgt Ion:128 Resp: 7214
 Ion Ratio Lower Upper
 128 100
 127 11.0 10.1 15.1
 129 14.4 8.7 13.1#

