


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN031819\
 Data File : VN054379.D
 Acq On : 18 Mar 2019 8:20
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
 Title : SW846 8260
 Last Update : Wed Mar 13 03:33:31 2019

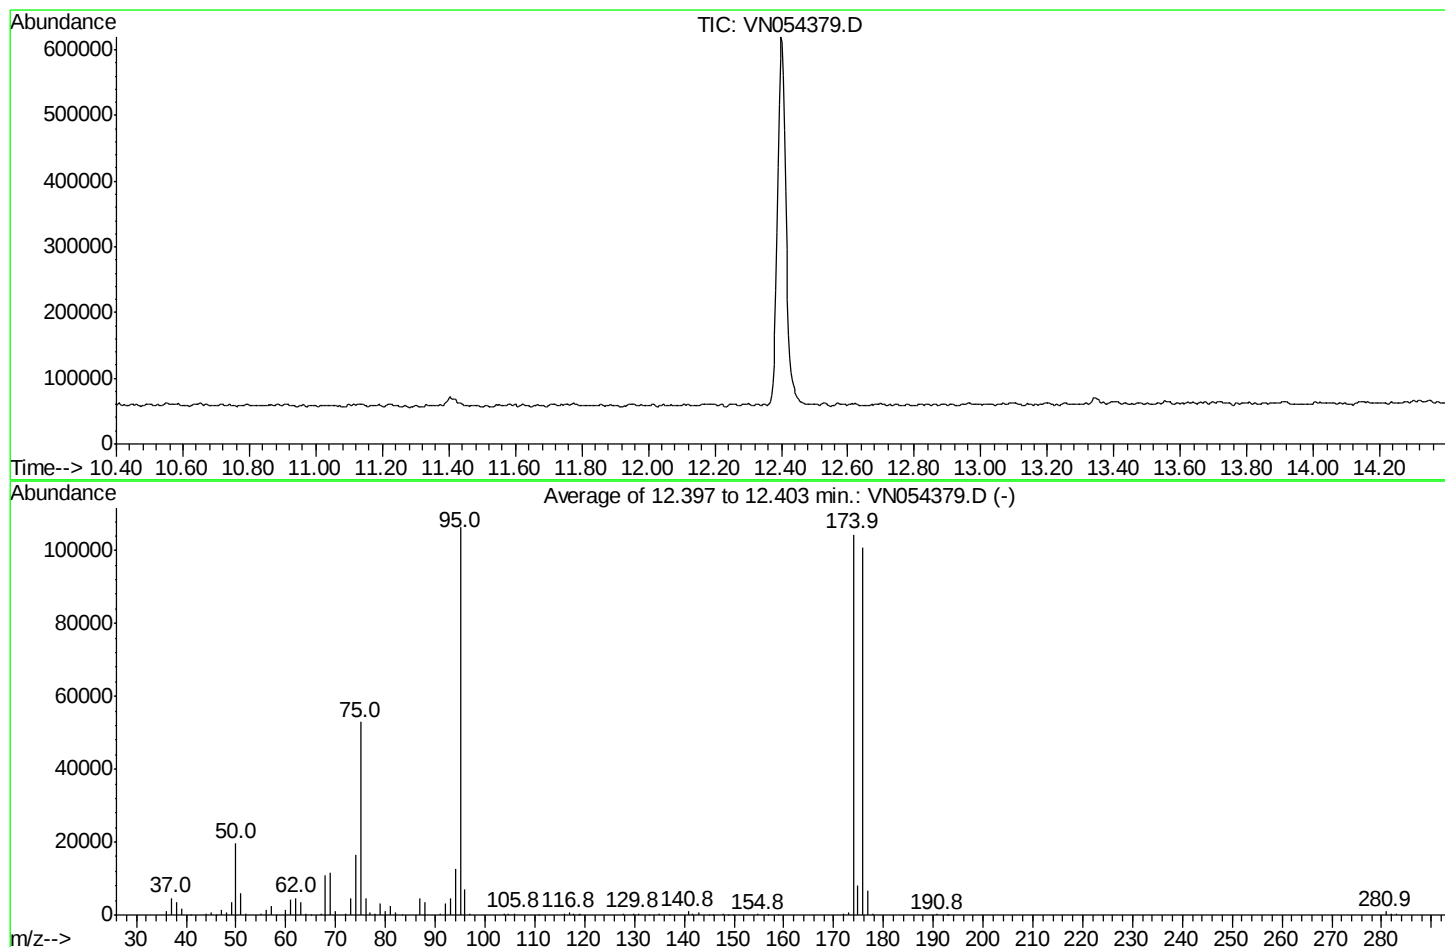

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	19592	PASS
75	95	30	60	49.7	52893	PASS
95	95	100	100	100.0	106370	PASS
96	95	5	9	6.7	7091	PASS
173	174	0.00	2	0.7	680	PASS
174	95	50	100	98.1	104330	PASS
175	174	5	9	7.9	8198	PASS
176	174	95	101	96.6	100765	PASS
177	176	5	9	6.7	6737	PASS