


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031821\
Data File : VN066244.D
Acq On : 18 Mar 2021 9:00
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031621W.M
Title : SW846 8260
Last Update : Wed Mar 17 05:05:15 2021

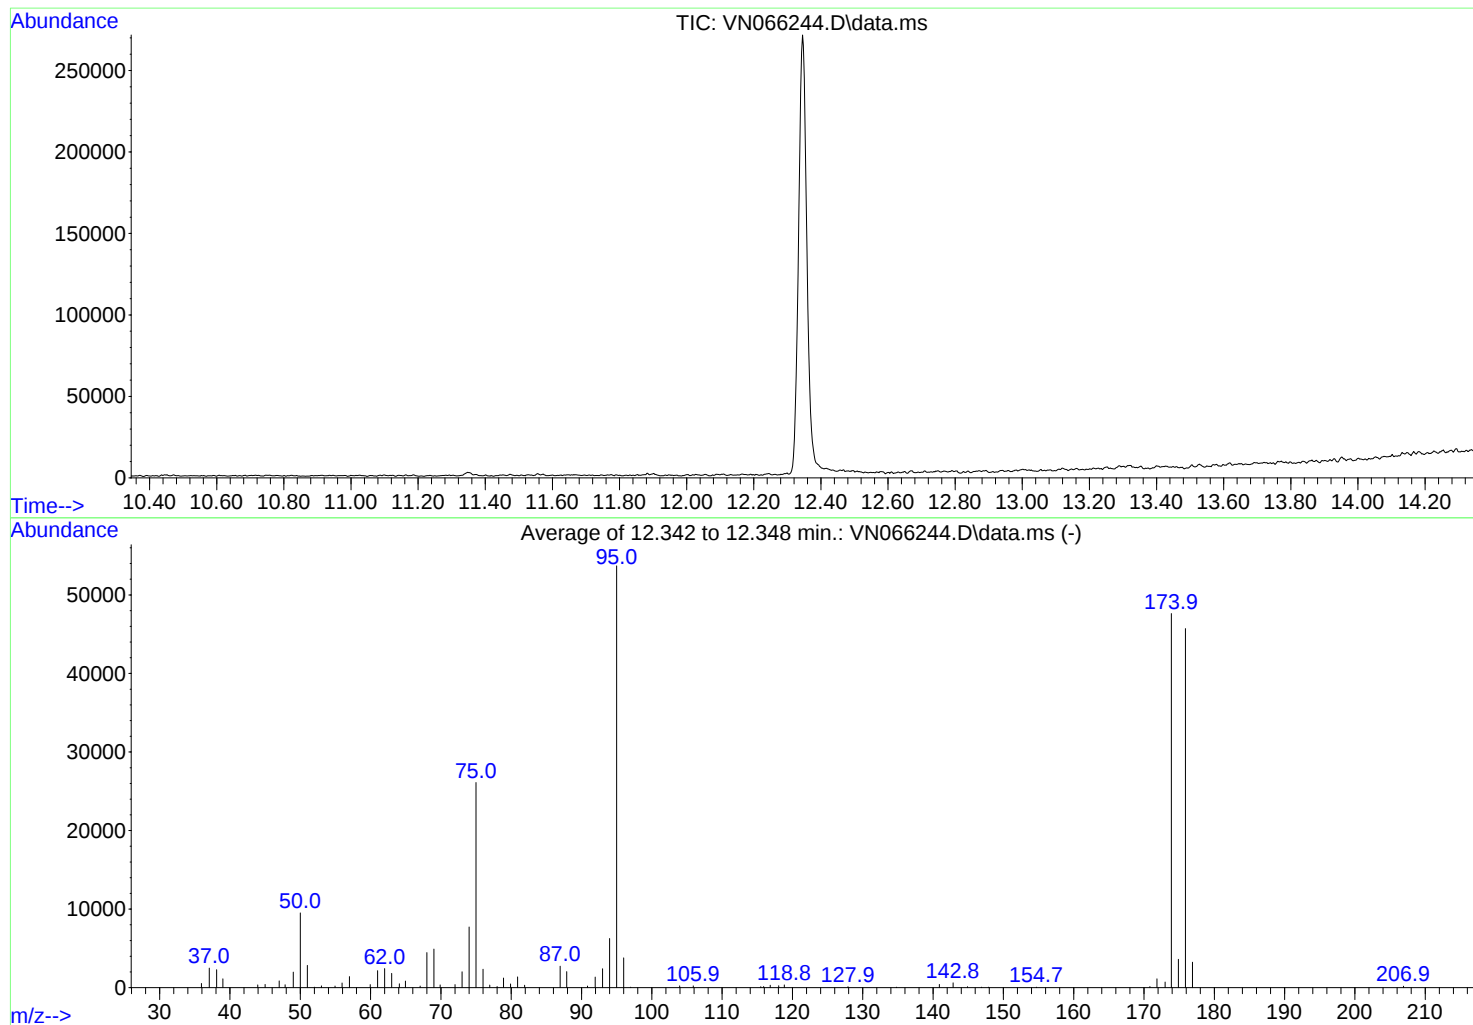

AutoFind: Scans 3972, 3973, 3974; Background Corrected with Scan 3956

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	9525	PASS
75	95	30	60	48.6	26123	PASS
95	95	100	100	100.0	53704	PASS
96	95	5	9	7.0	3781	PASS
173	174	0.00	2	1.5	706	PASS
174	95	50	100	88.7	47637	PASS
175	174	5	9	7.6	3615	PASS
176	174	95	101	96.0	45717	PASS
177	176	5	9	7.1	3231	PASS