

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031822\
 Data File : VN071364.D
 Acq On : 18 Mar 2022 11:40
 Operator : JC\MD
 Sample : VN0318MBL01
 Misc : 5.00g/10.0mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Mar 18 16:56:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	641169	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1076153	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.745	117	976337	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	312528	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	412578	46.951	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	93.900%		
35) Dibromofluoromethane	8.022	113	316259	46.571	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	93.140%		
50) Toluene-d8	10.439	98	1307536	47.821	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	95.640%		
62) 4-Bromofluorobenzene	12.727	95	395702	42.738	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	85.480%		
Target Compounds					Qvalue	
3) Chloromethane	2.299	50	2526	0.233	ug/l #	80
5) Bromomethane	2.834	94	60	Below Cal	#	3
13) Acrolein	4.057	56	1143	0.626	ug/l #	53
15) Acrylonitrile	5.569	53	1510	0.295	ug/l #	76
16) Acetone	4.293	43	11779	2.755	ug/l	95
18) Methyl Acetate	4.863	43	11576	1.469	ug/l #	68
20) Methylene Chloride	5.087	84	1309	0.548	ug/l #	87
25) 2-Butanone	7.351	43	2137	0.310	ug/l #	48
29) Tetrahydrofuran	7.710	42	2037	0.427	ug/l #	61
31) Cyclohexane	8.086	56	12857	0.916	ug/l #	1
36) 1,1-Dichloropropene	8.086	75	50234	4.617	ug/l #	49
38) Carbon Tetrachloride	8.086	117	63993	6.081	ug/l #	15
43) Isopropyl Acetate	8.610	43	16345	0.730	ug/l #	55
49) 1,4-Dioxane	9.592	88	54	0.299	ug/l #	47
51) 4-Methyl-2-Pentanone	10.327	43	4290	0.309	ug/l #	86
59) 2-Hexanone	11.086	43	7951	0.839	ug/l	85
74) N-amyl acetate	12.392	43	3844	0.339	ug/l	98
75) 1,1,2,2-Tetrachloroethane	12.821	83	1208	Below Cal	#	84
76) 1,2,3-Trichloropropane	12.727	75	205992	25.831	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	205992	71.250	ug/l #	5
87) 1,3-Dichlorobenzene	13.615	146	2561	0.224	ug/l	94
88) 1,4-Dichlorobenzene	13.615	146	2561	0.230	ug/l	93
89) n-Butylbenzene	13.945	91	4750	0.278	ug/l	93
91) 1,2-Dichlorobenzene	13.986	146	2506	0.228	ug/l	92
92) 1,2-Dibromo-3-Chloropr...	14.598	75	671	0.383	ug/l #	41
93) 1,2,4-Trichlorobenzene	15.251	180	3726	3.673	ug/l	90
94) Hexachlorobutadiene	15.362	225	767	0.249	ug/l	71
95) Naphthalene	15.504	128	13183	5.894	ug/l	97
96) 1,2,3-Trichlorobenzene	15.698	180	5364	3.765	ug/l	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031822\
Data File : VN071364.D
Acq On : 18 Mar 2022 11:40
Operator : JC\MD
Sample : VN0318MBL01
Misc : 5.00g/10.0mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Mar 18 16:56:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration




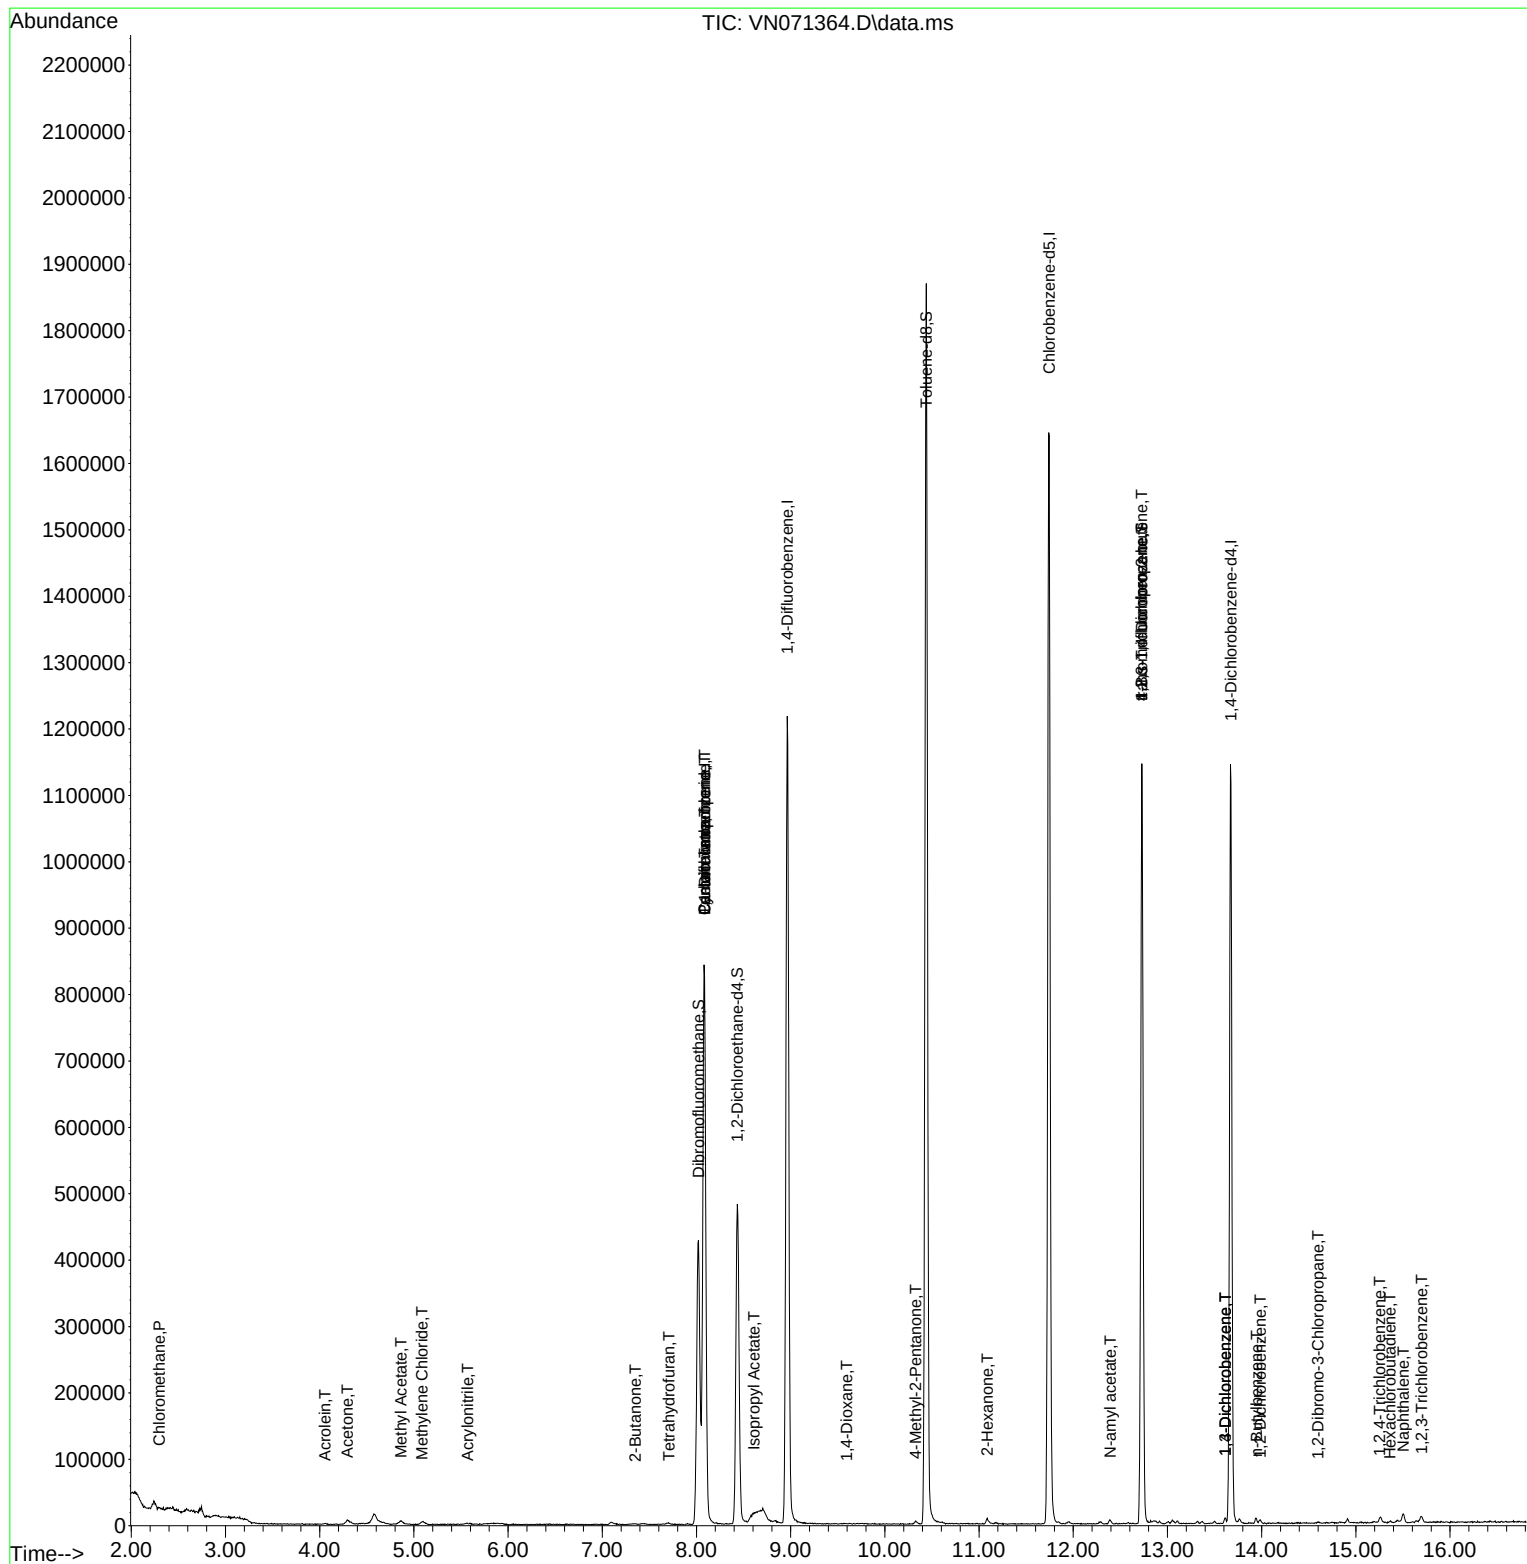




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 1037
Delta R.T. 0.000 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 641169
Ion Ratio Lower Upper
168 100
99 57.0 41.3 61.9

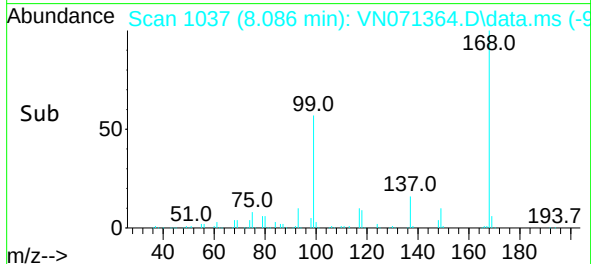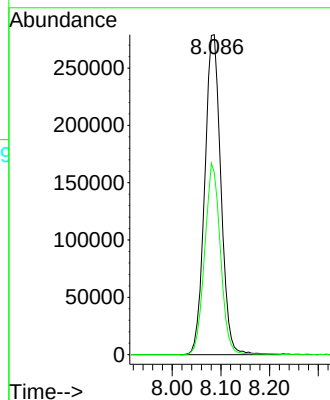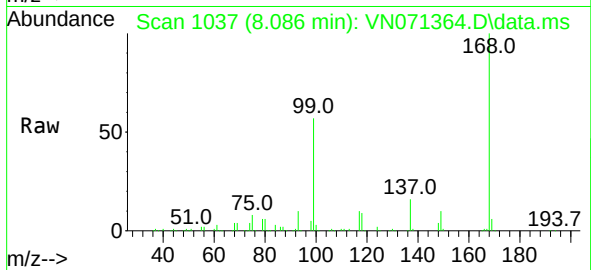

#3
Chloromethane
Concen: 0.233 ug/l
RT: 2.299 min Scan# 53
Delta R.T. -0.000 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40


Tgt Ion: 50 Resp: 2526
Ion Ratio Lower Upper
50 100
52 20.7 25.4 38.0#

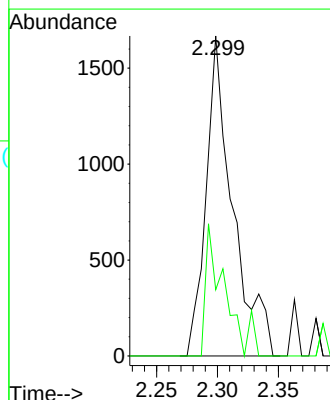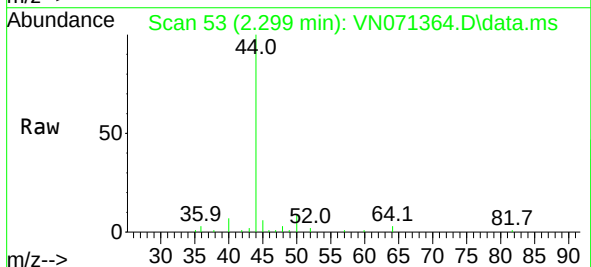



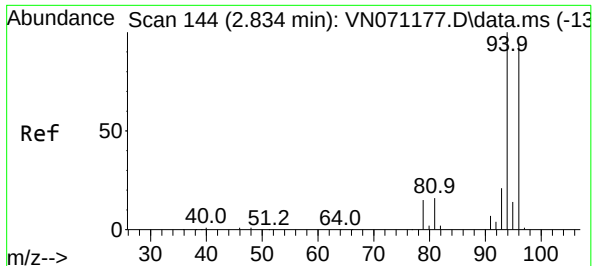


#5
Bromomethane
Concen: Below Cal
RT: 2.834 min Scan# 14
Delta R.T. -0.000 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 94 Resp: 60
Ion Ratio Lower Upper
94 100
96 0.0 73.8 110.8#

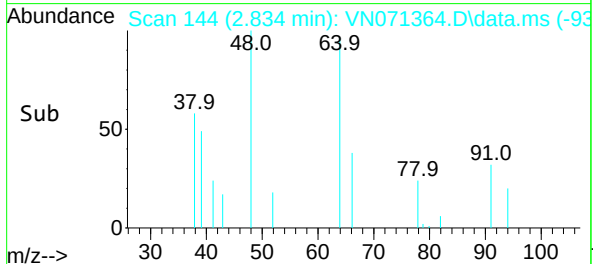

#13
Acrolein
Concen: 0.626 ug/l
RT: 4.057 min Scan# 352
Delta R.T. 0.018 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Tgt Ion: 56 Resp: 1143
Ion Ratio Lower Upper
56 100
55 32.1 56.6 85.0#


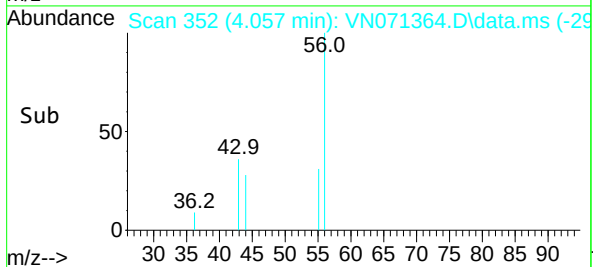

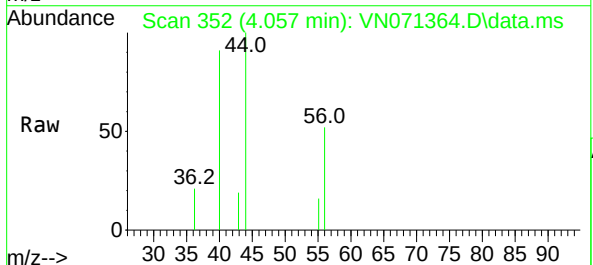




#15
Acrylonitrile
Concen: 0.295 ug/l
RT: 5.569 min Scan# 609
Delta R.T. 0.018 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 53 Resp: 1510
Ion Ratio Lower Upper
53 100
52 67.2 66.2 99.2
51 13.6 29.6 44.4#

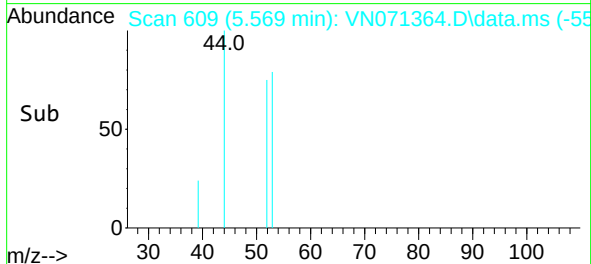

#16
Acetone
Concen: 2.755 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.006 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Tgt Ion: 43 Resp: 11779
Ion Ratio Lower Upper
43 100
58 31.4 23.1 34.7


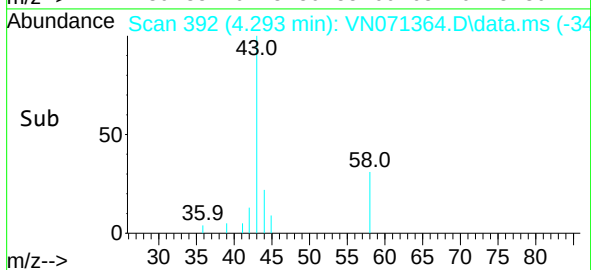

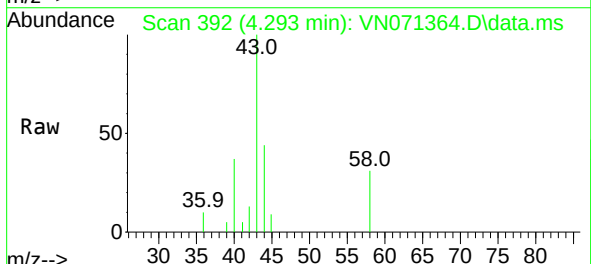


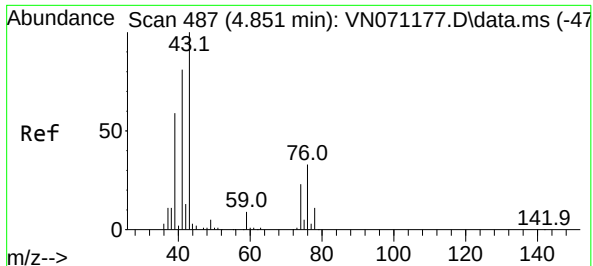

#18
Methyl Acetate
Concen: 1.469 ug/l
RT: 4.863 min Scan# 489
Delta R.T. 0.012 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 11576
Ion Ratio Lower Upper
43 100
74 8.4 19.4 29.2#

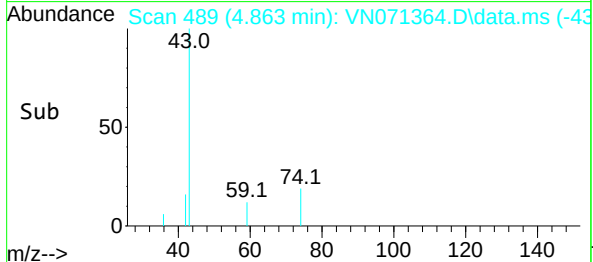

#20
Methylene Chloride
Concen: 0.548 ug/l
RT: 5.087 min Scan# 527
Delta R.T. -0.006 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Tgt Ion: 84 Resp: 1309
Ion Ratio Lower Upper
84 100
49 108.9 93.5 140.3
51 35.2 29.4 44.2
86 44.3 53.0 79.4#


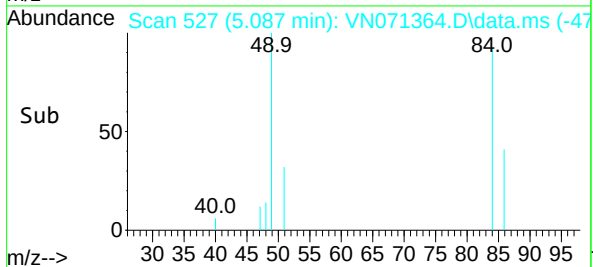

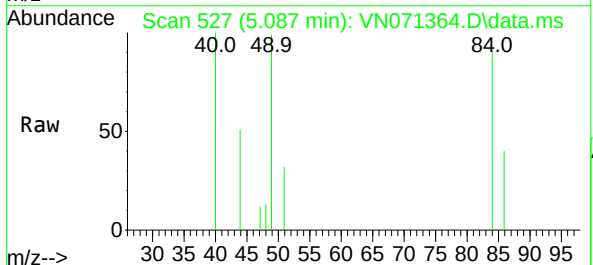


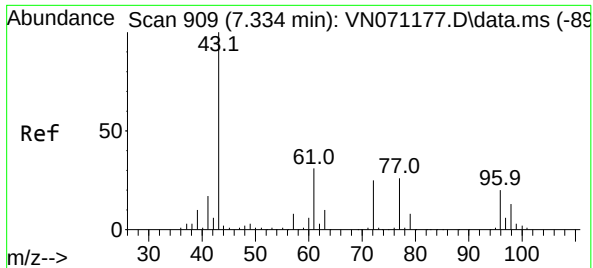

#25
2-Butanone
Concen: 0.310 ug/l
RT: 7.351 min Scan# 912
Delta R.T. 0.018 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 2137
Ion Ratio Lower Upper
43 100
72 0.0 21.7 32.5#

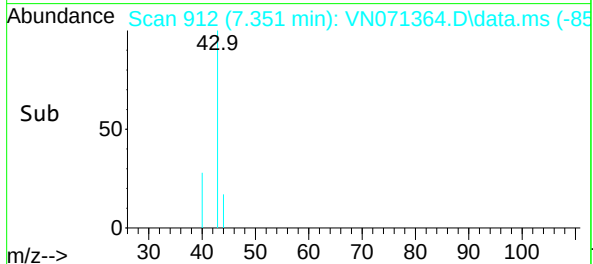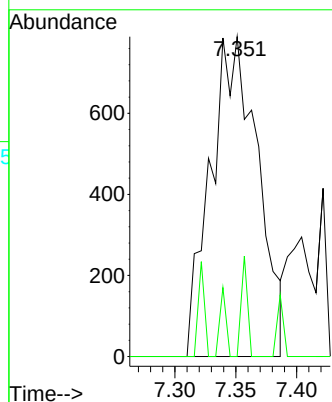

#29
Tetrahydrofuran
Concen: 0.427 ug/l
RT: 7.710 min Scan# 973
Delta R.T. 0.029 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40


Tgt Ion: 42 Resp: 2037
Ion Ratio Lower Upper
42 100
72 28.9 36.3 54.5#
71 9.2 34.7 52.1#

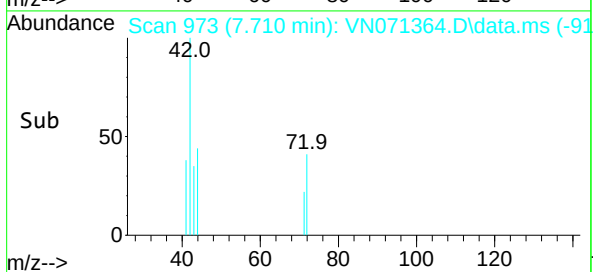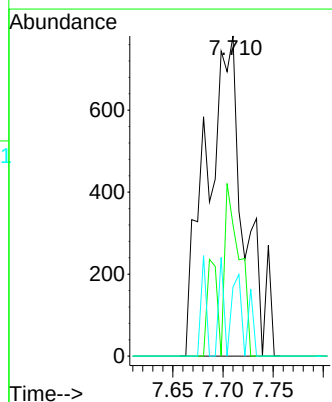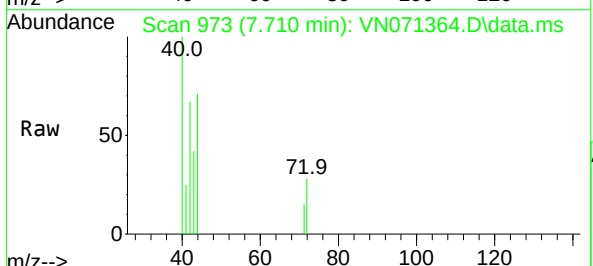






#31
Cyclohexane
Concen: 0.916 ug/l
RT: 8.086 min Scan# 1037
Delta R.T. -0.006 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 12857
Ion Ratio Lower Upper
56 100
69 184.1 27.1 40.7#
84 176.2 73.4 110.0#

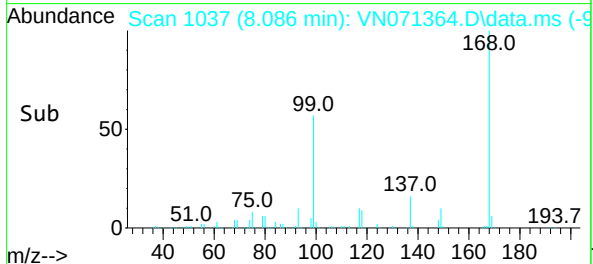

#33
1,2-Dichloroethane-d4
Concen: 46.951 ug/l
RT: 8.433 min Scan# 1096
Delta R.T. -0.006 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Tgt Ion: 65 Resp: 412578
Ion Ratio Lower Upper
65 100
67 52.9 0.0 103.0

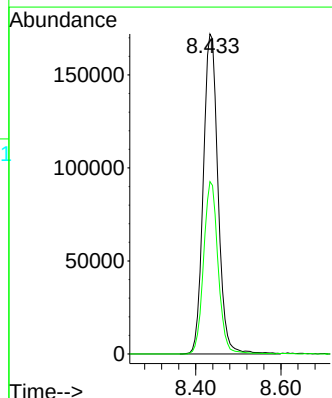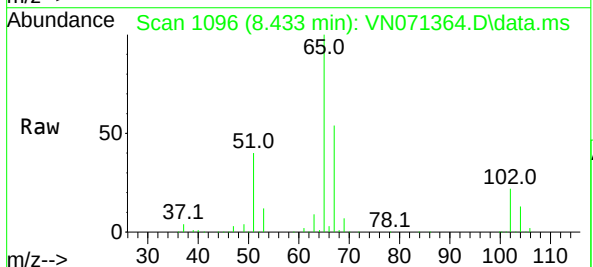

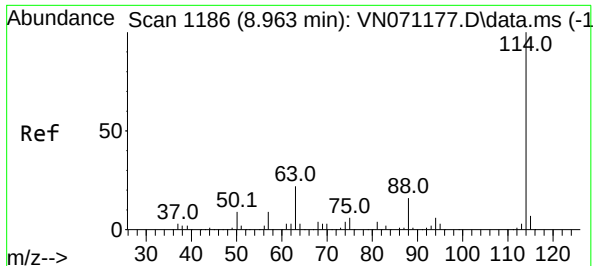

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN071364.D

Acq: 18 Mar 2022 11:40

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 1076153

Ion Ratio Lower Upper

114 100

63 21.9 0.0 37.8

88 16.3 0.0 27.4

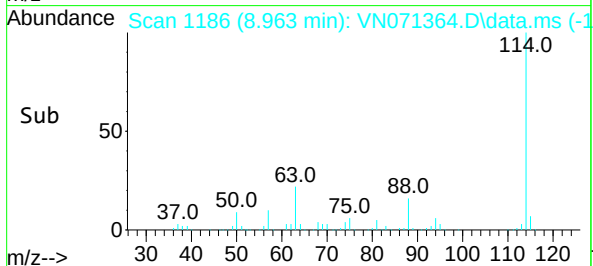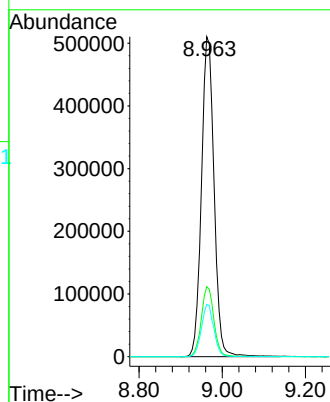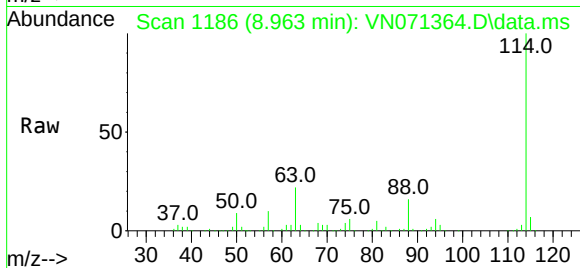

#35

Dibromofluoromethane

Concen: 46.571 ug/l

RT: 8.022 min Scan# 1026

Delta R.T. -0.000 min

Lab File: VN071364.D

Acq: 18 Mar 2022 11:40




Tgt Ion:113 Resp: 316259


Ion Ratio Lower Upper

113 100

111 103.7 82.2 123.2

192 21.0 16.9 25.3


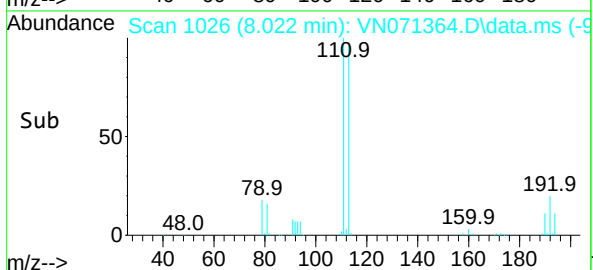
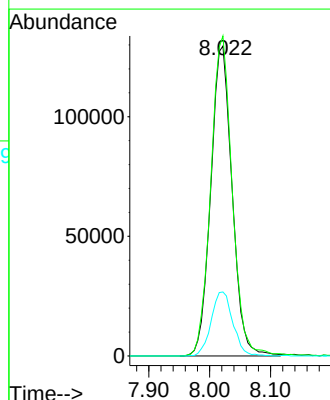
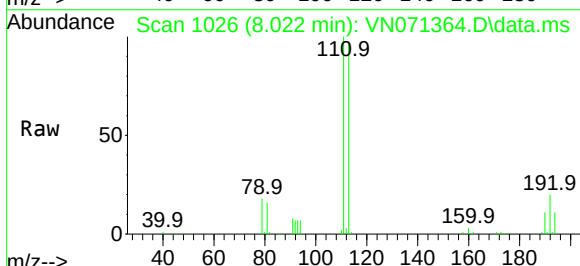


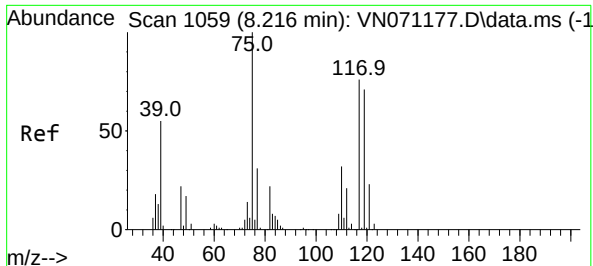

#36
1,1-Dichloropropene
Concen: 4.617 ug/l
RT: 8.086 min Scan# 1037
Delta R.T. -0.129 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 50234
Ion Ratio Lower Upper
75 100
110 9.2 18.4 55.2#
77 0.0 24.4 36.6#

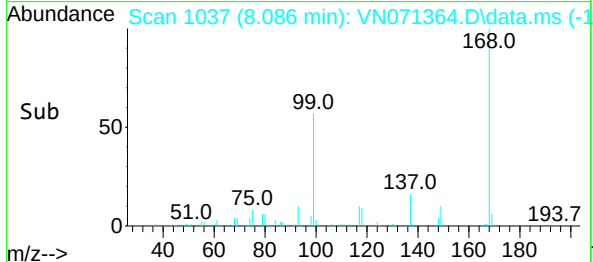

#38
Carbon Tetrachloride
Concen: 6.081 ug/l
RT: 8.086 min Scan# 1037
Delta R.T. -0.118 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Tgt Ion: 117 Resp: 63993
Ion Ratio Lower Upper
117 100
119 4.0 76.1 114.1#
121 0.0 24.2 36.2#

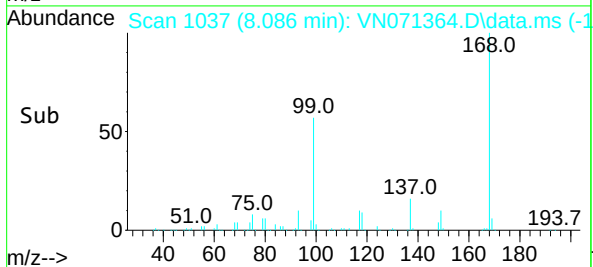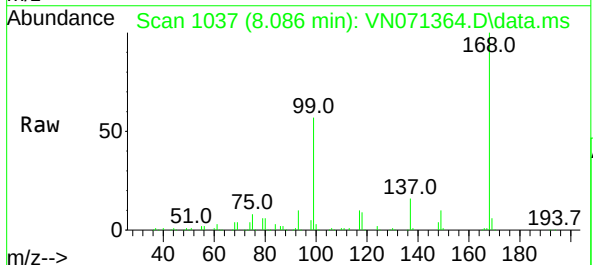

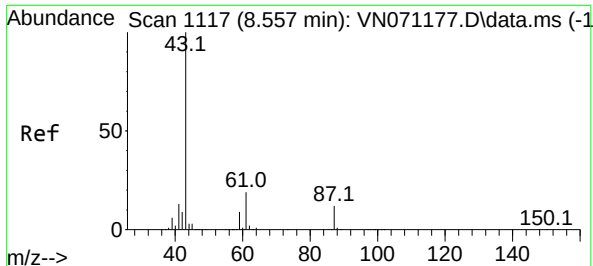

#43

Isopropyl Acetate

Concen: 0.730 ug/l

RT: 8.610 min Scan# 1117

Delta R.T. 0.053 min

Lab File: VN071364.D

Acq: 18 Mar 2022 11:40

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 43 Resp: 16345

Ion Ratio Lower Upper

43 100

61 0.0 20.4 30.6#

87 0.0 11.2 16.8#

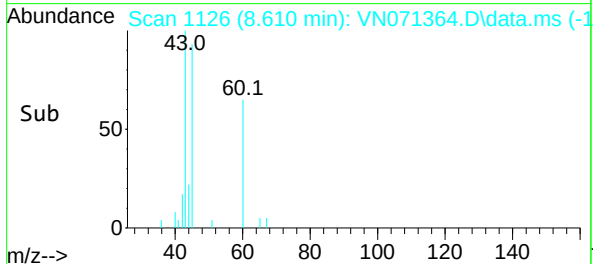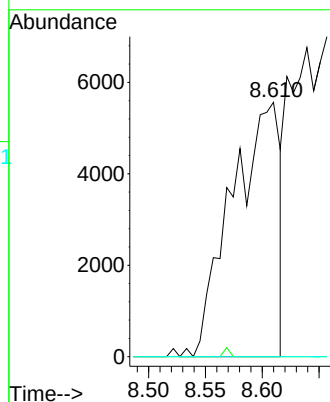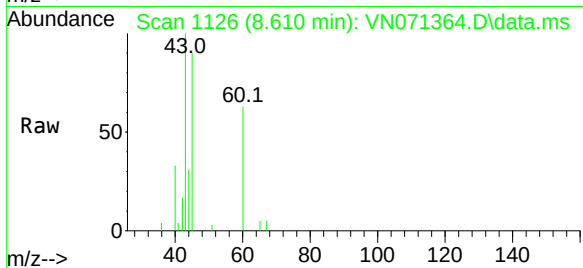

#49

1,4-Dioxane

Concen: 0.299 ug/l

RT: 9.592 min Scan# 1293

Delta R.T. 0.029 min

Lab File: VN071364.D

Acq: 18 Mar 2022 11:40




Tgt Ion: 88 Resp: 54


Ion Ratio Lower Upper

88 100

43 0.0 23.4 35.2#

58 103.7 50.6 75.8#


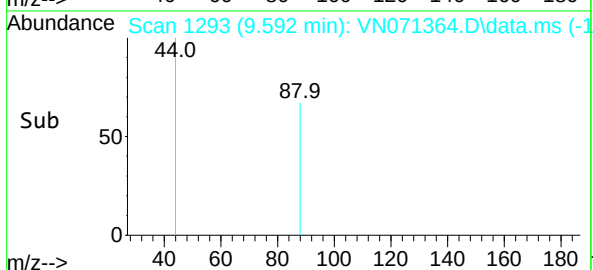
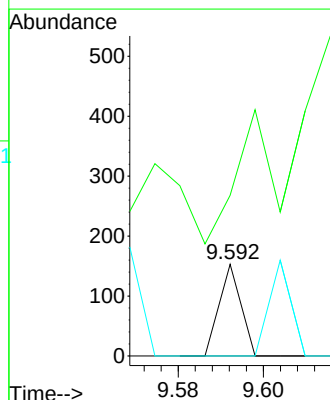
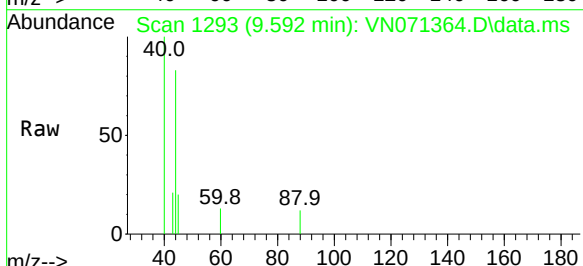




#50
Toluene-d8
Concen: 47.821 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 1307536
Ion Ratio Lower Upper
98 100
100 65.6 50.4 75.6

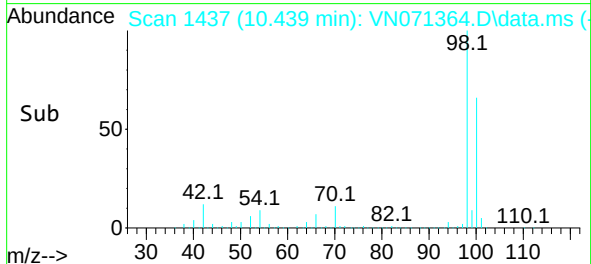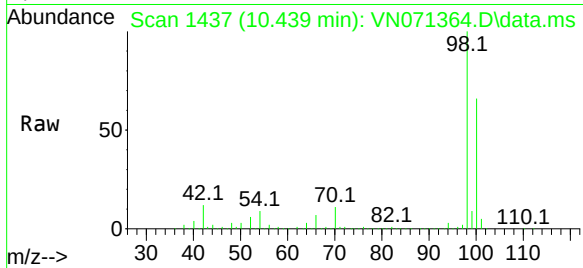

#51
4-Methyl-2-Pentanone
Concen: 0.309 ug/l
RT: 10.327 min Scan# 1418
Delta R.T. 0.000 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Tgt Ion: 43 Resp: 4290
Ion Ratio Lower Upper
43 100
58 29.7 30.4 45.6#


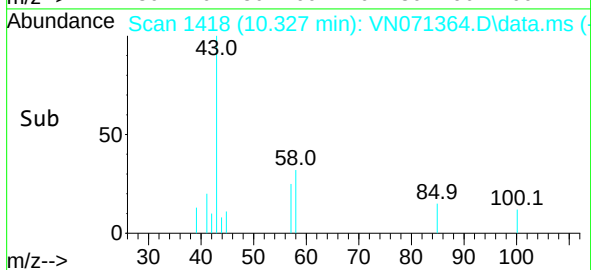

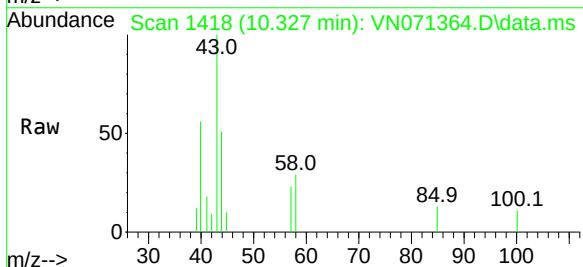




#59
2-Hexanone
Concen: 0.839 ug/l
RT: 11.086 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 7951
Ion Ratio Lower Upper
43 100
58 43.1 26.9 80.7

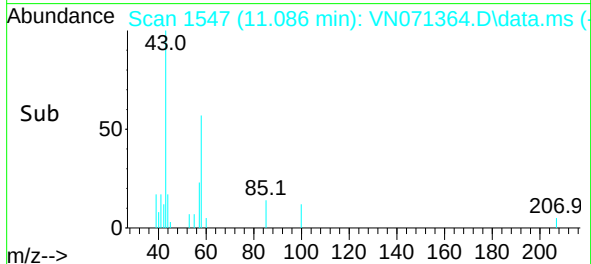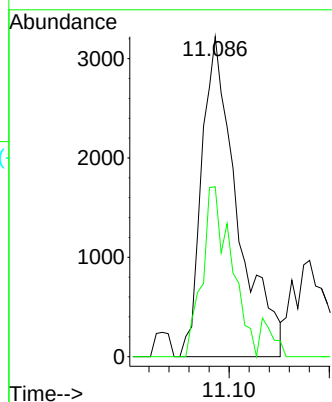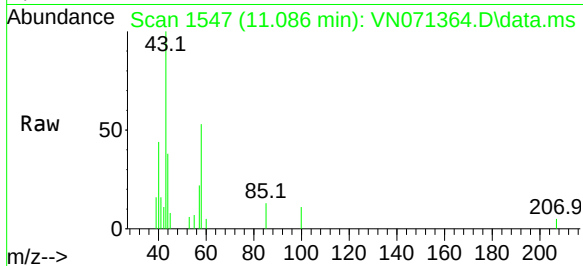

#62
4-Bromofluorobenzene
Concen: 42.738 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Tgt Ion: 95 Resp: 395702
Ion Ratio Lower Upper
95 100
174 79.1 0.0 187.2
176 77.3 0.0 181.4


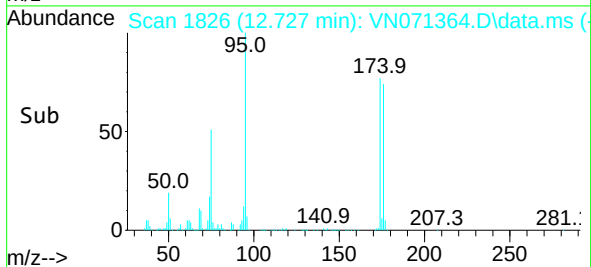
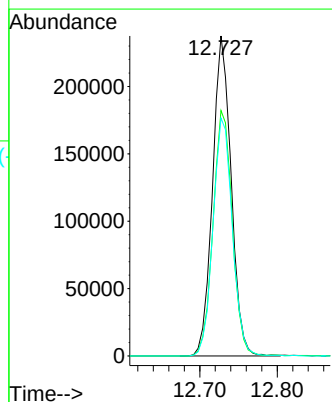
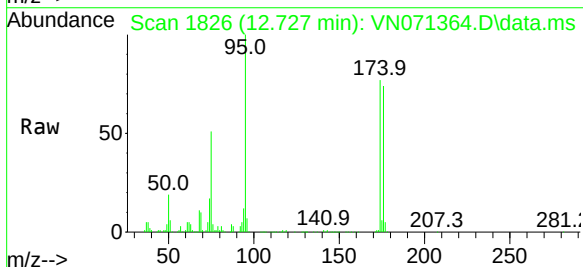




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.745 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 976337
Ion Ratio Lower Upper
117 100
82 57.3 42.4 63.6
119 31.8 25.4 38.2

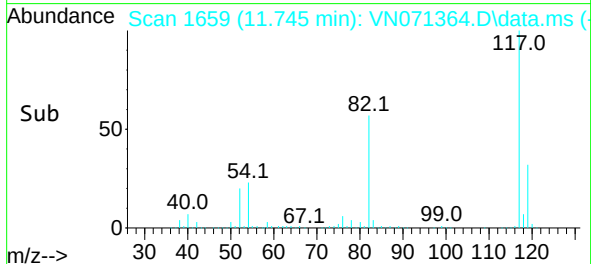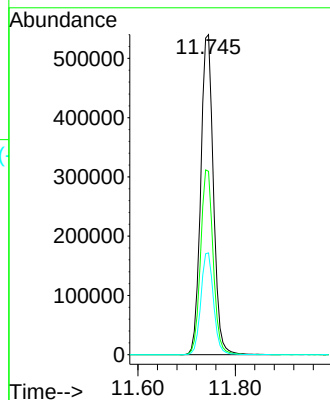

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1987
Delta R.T. 0.006 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Tgt Ion:152 Resp: 312528
Ion Ratio Lower Upper
152 100
115 59.5 27.5 82.5
150 160.4 0.0 344.4

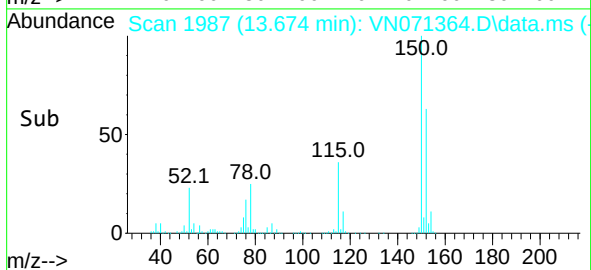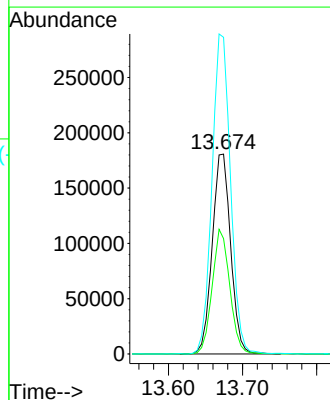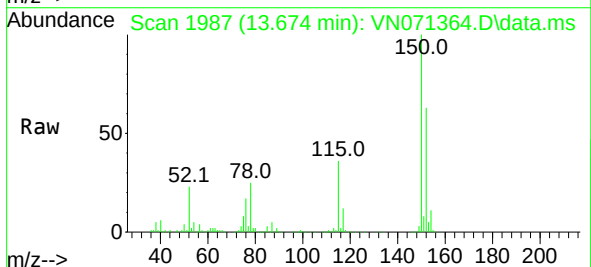



#74

N-amy1 acetate

Concen: 0.339 ug/l

RT: 12.392 min Scan# 1

Delta R.T. 0.006 min


Lab File: VN071364.D

Acq: 18 Mar 2022 11:40

Instrument :

MSVOA_N

ClientSampleId :

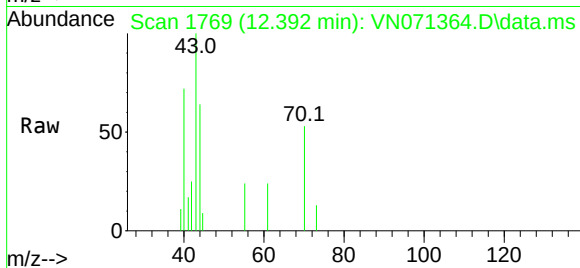

Tgt Ion: 43 Resp: 3844




Ion Ratio Lower Upper

43 100

70 43.2 33.4 50.0

55 23.0 19.3 28.9

61 22.2 18.5 27.7



#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.821 min Scan# 1842

Delta R.T. 0.000 min

Lab File: VN071364.D

Acq: 18 Mar 2022 11:40




Tgt Ion: 83 Resp: 1208


Ion Ratio Lower Upper

83 100

131 0.0 5.5 16.5#

85 53.9 32.4 97.2


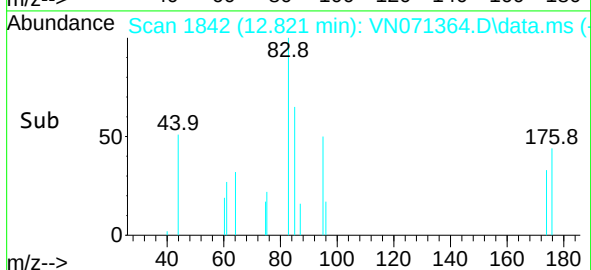

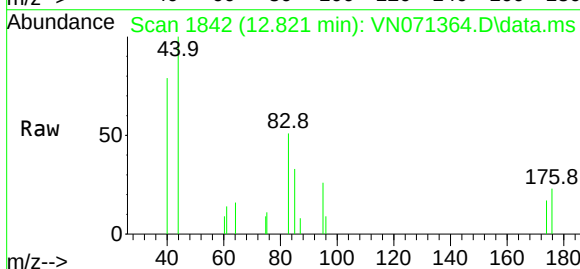




#76
1,2,3-Trichloropropane
Concen: 25.831 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 205992
Ion Ratio Lower Upper
75 100
77 1.2 82.6 247.8#

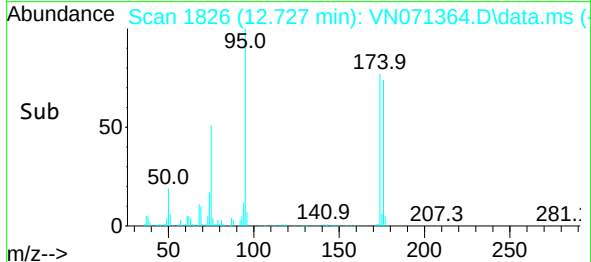

#81
trans-1,4-Dichloro-2-butene
Concen: 71.250 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Tgt Ion: 75 Resp: 205992
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

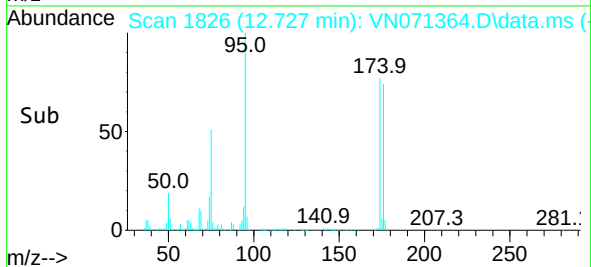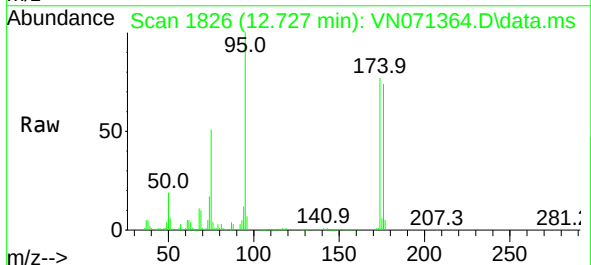



#87

1,3-Dichlorobenzene

Concen: 0.224 ug/l

RT: 13.615 min Scan# 1976

Delta R.T. 0.006 min

Lab File: VN071364.D

Acq: 18 Mar 2022 11:40

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:146 Resp: 2561

Ion Ratio Lower Upper

146 100

111 39.2 18.6 55.6

148 57.2 31.6 95.0

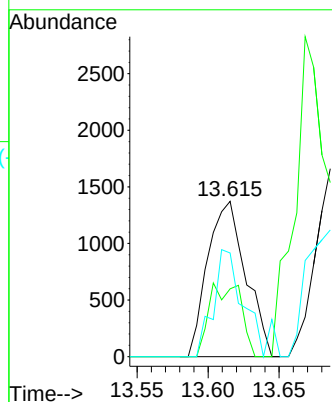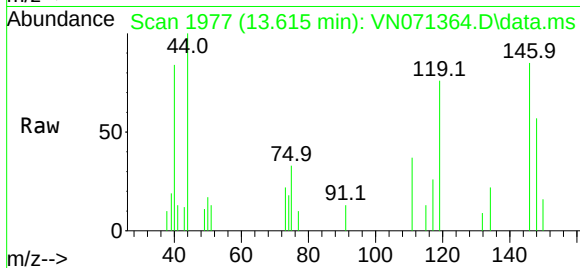

#88

1,4-Dichlorobenzene

Concen: 0.230 ug/l

RT: 13.615 min Scan# 1977

Delta R.T. -0.077 min

Lab File: VN071364.D

Acq: 18 Mar 2022 11:40




Tgt Ion:146 Resp: 2561


Ion Ratio Lower Upper

146 100

111 39.2 18.3 54.8

148 57.2 31.8 95.4

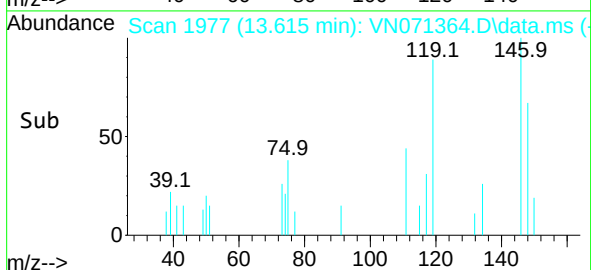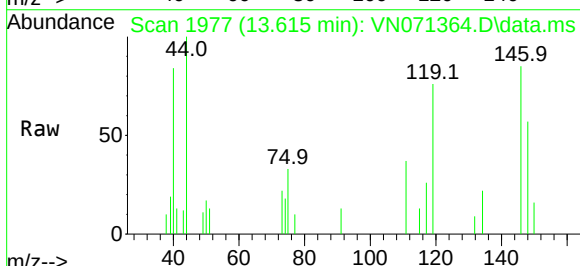

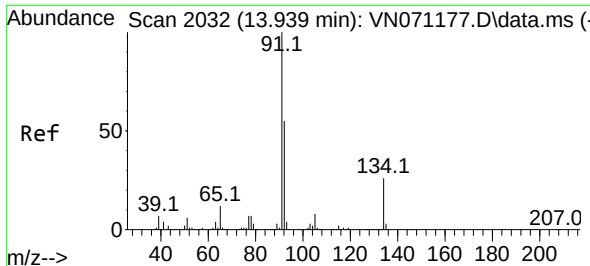

#89

n-Butylbenzene

Concen: 0.278 ug/l

RT: 13.945 min Scan# 2033

Delta R.T. 0.006 min

Lab File: VN071364.D





Acq: 18 Mar 2022 11:40

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion: 91	Resp:	4750
Ion Ratio	Lower	Upper
91	100	
92	55.7	25.4 76.0
134	23.7	13.6 40.8

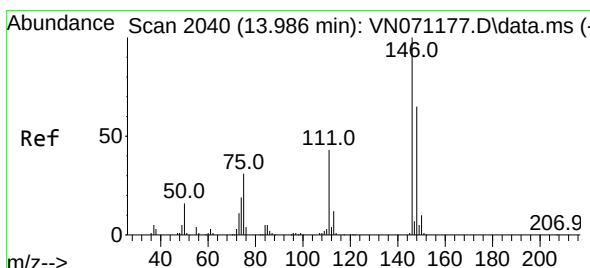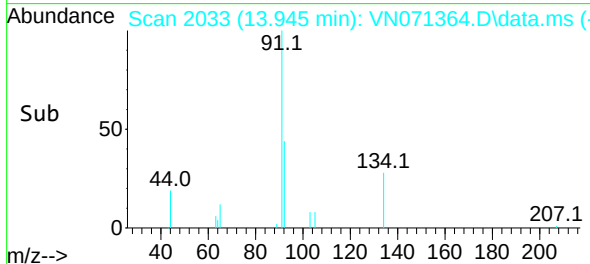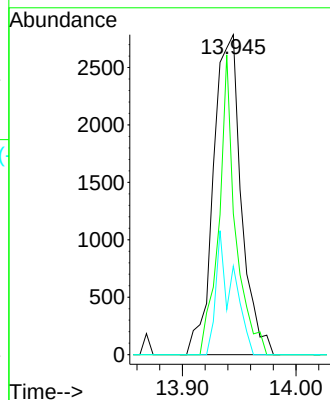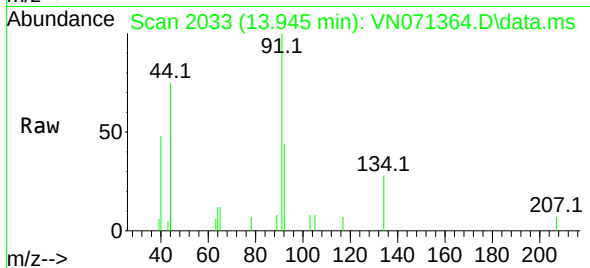

#91

1,2-Dichlorobenzene

Concen: 0.228 ug/l




RT: 13.986 min Scan# 2040


Delta R.T. -0.000 min

Lab File: VN071364.D

Acq: 18 Mar 2022 11:40

Tgt Ion: 146	Resp:	2506
Ion Ratio	Lower	Upper
146	100	
111	43.2	19.1 57.3
148	57.9	32.1 96.3


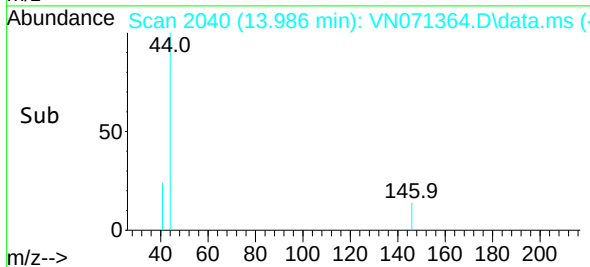
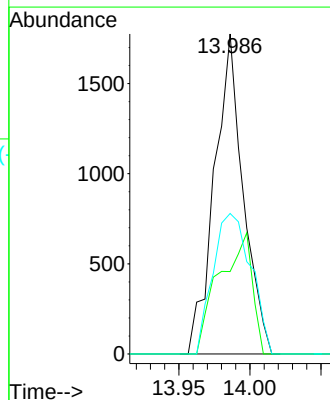
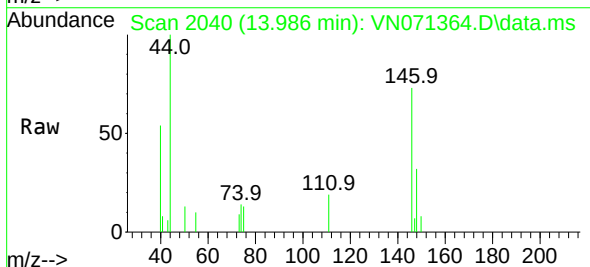


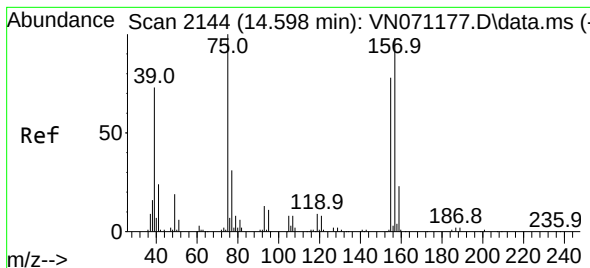

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.383 ug/l
 RT: 14.598 min Scan# 2144
 Delta R.T. -0.000 min
 Lab File: VN071364.D
 Acq: 18 Mar 2022 11:40




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 671
 Ion Ratio Lower Upper
 75 100
 155 28.0 46.9 140.7#
 157 62.4 60.6 181.7

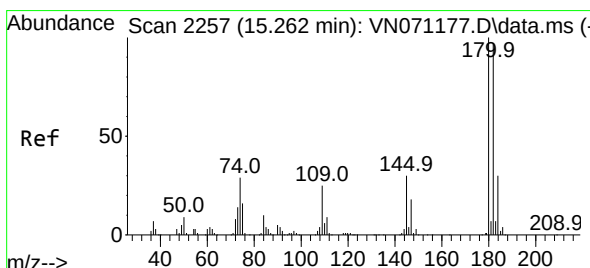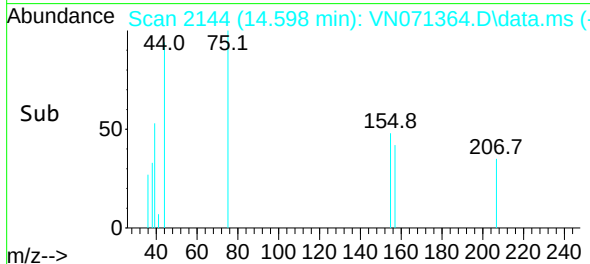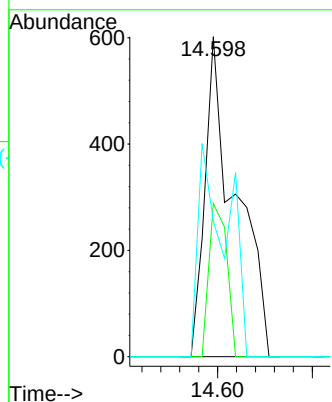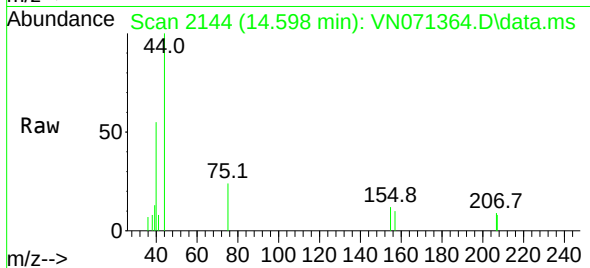

#93
 1,2,4-Trichlorobenzene
 Concen: 3.673 ug/l
 RT: 15.251 min Scan# 2255
 Delta R.T. -0.011 min
 Lab File: VN071364.D
 Acq: 18 Mar 2022 11:40


Tgt Ion: 180 Resp: 3726
 Ion Ratio Lower Upper
 180 100
 182 84.7 48.3 144.9
 145 30.0 14.5 43.5

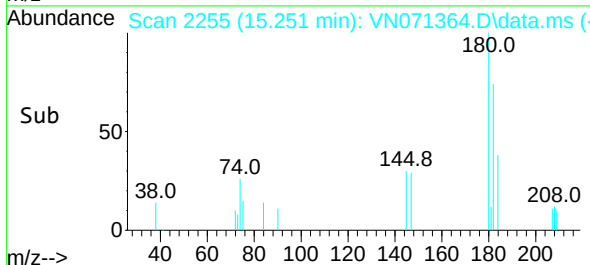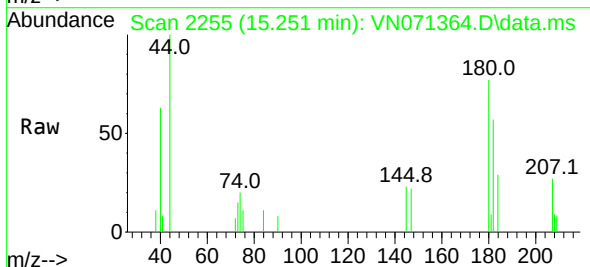






#94
Hexachlorobutadiene
Concen: 0.249 ug/l
RT: 15.362 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40

Instrument :
MSVOA_N
ClientSampleId :



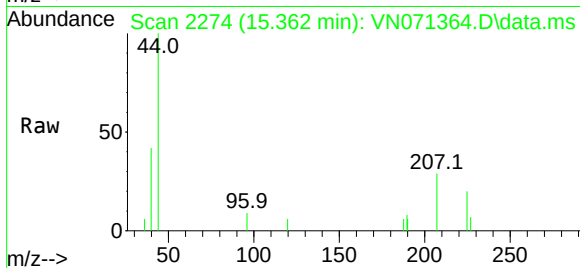



Tgt Ion:	225	Resp:	767
Ion	Ratio	Lower	Upper
225	100		
223	39.8	31.9	95.7
227	42.4	32.1	96.3

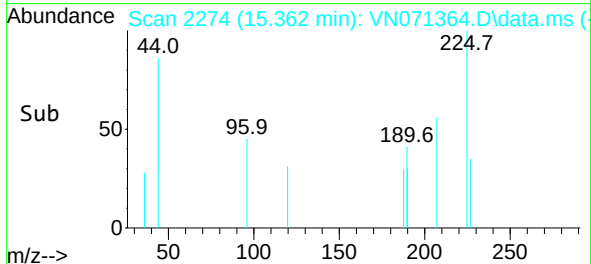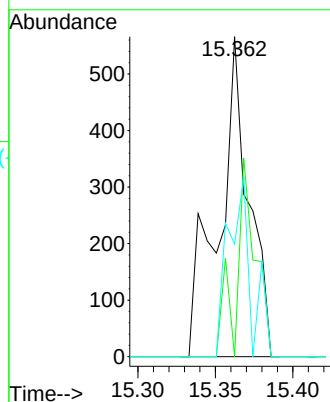

#95
Naphthalene
Concen: 5.894 ug/l
RT: 15.504 min Scan# 2298
Delta R.T. -0.000 min
Lab File: VN071364.D
Acq: 18 Mar 2022 11:40


Tgt Ion:	128	Resp:	13183
Ion	Ratio	Lower	Upper
128	100		
127	14.5	10.5	15.7
129	12.0	8.7	13.1

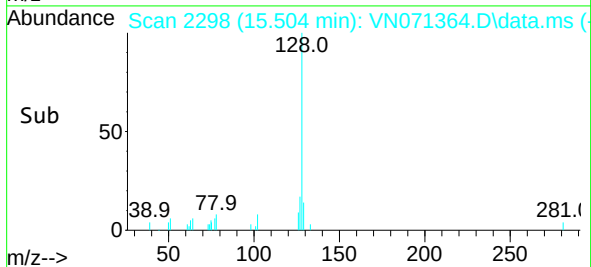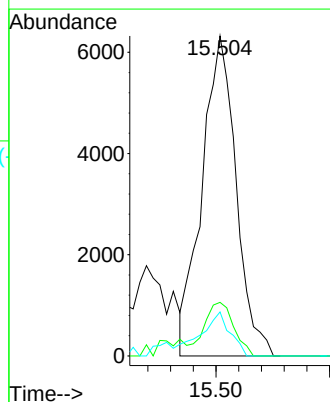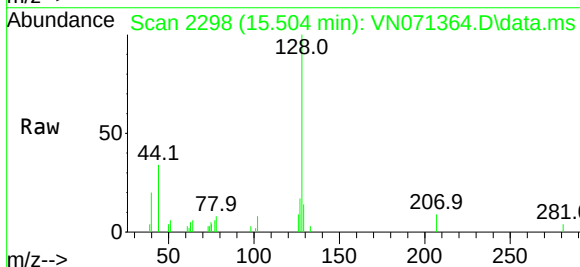



#96
 1,2,3-Trichlorobenzene
 Concen: 3.765 ug/l
 RT: 15.698 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN071364.D
 Acq: 18 Mar 2022 11:40

Instrument :
 MSVOA_N
 ClientSampleId :

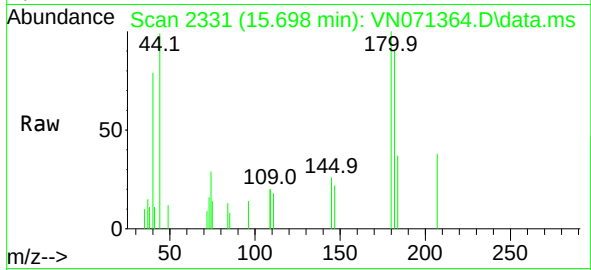

Tgt Ion:180 Resp: 5364
 Ion Ratio Lower Upper
 180 100
 182 75.6 47.4 142.2
 145 23.7 15.0 45.1

