

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031822\
 Data File : VN071368.D
 Acq On : 18 Mar 2022 13:29
 Operator : JC\MD
 Sample : N1875-06
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Mar 19 07:06:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	8.080	168	682091	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1138875	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1045849	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	343202	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	445660	47.673	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	95.340%
35) Dibromofluoromethane	8.016	113	338608	47.116	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	94.240%
50) Toluene-d8	10.439	98	1401983	48.452	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.900%
62) 4-Bromofluorobenzene	12.727	95	497976	50.822	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	101.640%
Target Compounds						
					Qvalue	
3) Chloromethane	2.299	50	3385	0.303	ug/l #	86
5) Bromomethane	2.857	94	1723	Below Cal	#	56
10) Methyl Iodide	4.440	142	2472	0.251	ug/l #	74
11) Tert butyl alcohol	5.322	59	4801	2.614	ug/l #	71
15) Acrylonitrile	5.569	53	1491	0.273	ug/l #	24
16) Acetone	4.292	43	30027	6.601	ug/l	100
17) Carbon Disulfide	4.534	76	5819	0.299	ug/l #	74
18) Methyl Acetate	4.863	43	11862	1.432	ug/l	95
20) Methylene Chloride	5.087	84	2073	0.629	ug/l #	89
25) 2-Butanone	7.333	43	8899	1.215	ug/l #	83
27) cis-1,2-Dichloroethene	7.333	96	3922	0.442	ug/l	89
29) Tetrahydrofuran	7.704	42	2734	0.539	ug/l #	93
31) Cyclohexane	8.080	56	14142	0.947	ug/l #	1
36) 1,1-Dichloropropene	8.080	75	53072	4.609	ug/l #	48
38) Carbon Tetrachloride	8.080	117	67341	6.046	ug/l #	18
43) Isopropyl Acetate	8.622	43	23203	0.979	ug/l #	55
49) 1,4-Dioxane	9.580	88	265	1.388	ug/l #	56
51) 4-Methyl-2-Pentanone	10.327	43	4538	0.309	ug/l	97
59) 2-Hexanone	11.086	43	8570	0.854	ug/l	86
74) N-amyl acetate	12.380	43	4285	0.344	ug/l #	89
75) 1,1,2,2-Tetrachloroethane	12.827	83	1341	Below Cal	#	83
76) 1,2,3-Trichloropropane	12.727	75	256375	29.674	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	256375	80.751	ug/l #	5
87) 1,3-Dichlorobenzene	13.610	146	2656	0.212	ug/l	99
88) 1,4-Dichlorobenzene	13.610	146	2656	0.217	ug/l	98
89) n-Butylbenzene	13.939	91	4882	0.260	ug/l	94
91) 1,2-Dichlorobenzene	13.986	146	2912	0.242	ug/l	86
92) 1,2-Dibromo-3-Chloropr...	14.609	75	576	0.299	ug/l	99
93) 1,2,4-Trichlorobenzene	15.262	180	3477	3.570	ug/l	94
95) Naphthalene	15.504	128	11204	5.708	ug/l	100
96) 1,2,3-Trichlorobenzene	15.698	180	4269	3.481	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031822\
Data File : VN071368.D
Acq On : 18 Mar 2022 13:29
Operator : JC\MD
Sample : N1875-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Mar 19 07:06:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration




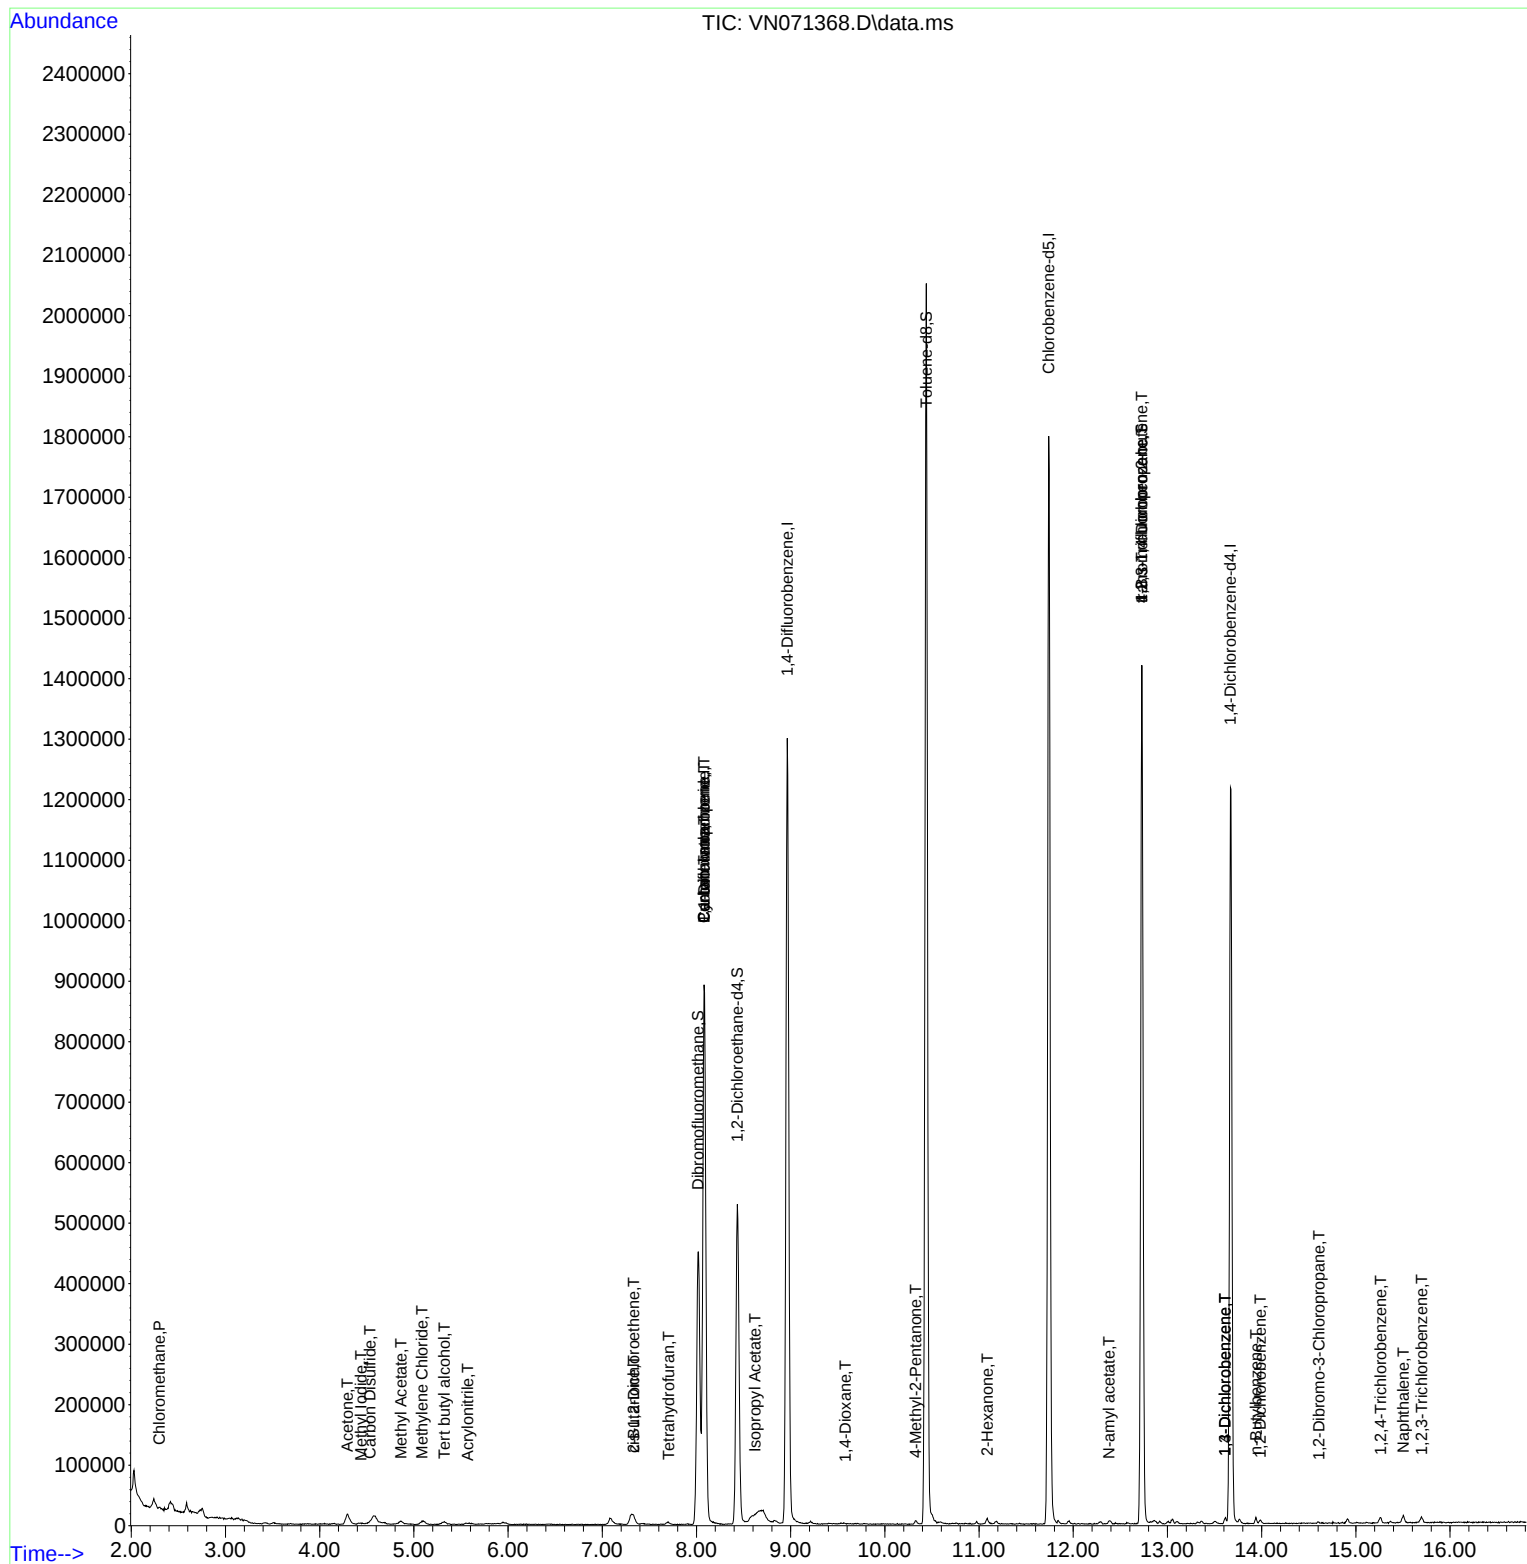




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.080 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 682091
Ion Ratio Lower Upper
168 100
99 57.5 41.3 61.9

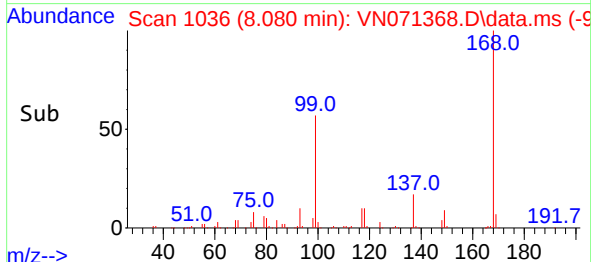

#3
Chloromethane
Concen: 0.303 ug/l
RT: 2.299 min Scan# 53
Delta R.T. -0.000 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29

Tgt Ion: 50 Resp: 3385
Ion Ratio Lower Upper
50 100
52 24.1 25.4 38.0#









#5
Bromomethane
Concen: Below Cal
RT: 2.857 min Scan# 144
Delta R.T. 0.023 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 1723
Ion Ratio Lower Upper
94 100
96 50.6 73.8 110.8#

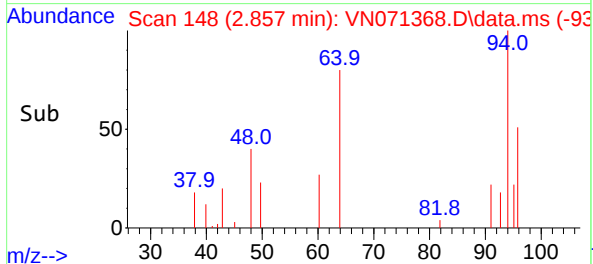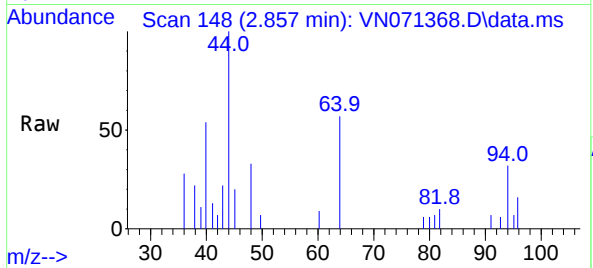

#10
Methyl Iodide
Concen: 0.251 ug/l
RT: 4.440 min Scan# 417
Delta R.T. 0.018 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29

Tgt Ion: 142 Resp: 2472
Ion Ratio Lower Upper
142 100
127 29.5 35.4 53.0#
141 0.0 11.6 17.4#


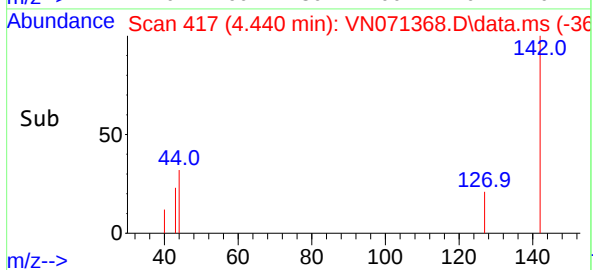

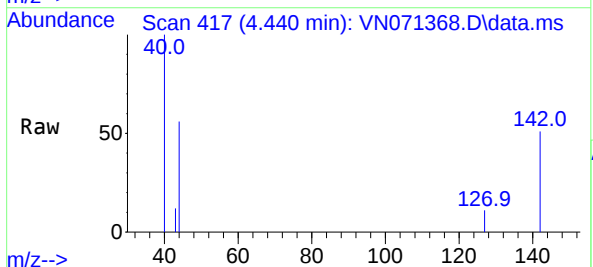




#11
Tert butyl alcohol
Concen: 2.614 ug/l
RT: 5.322 min Scan# 509
Delta R.T. -0.047 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 59 Resp: 4801
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

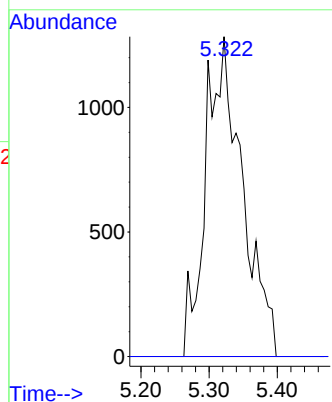

#15
Acrylonitrile
Concen: 0.273 ug/l
RT: 5.569 min Scan# 609
Delta R.T. 0.018 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29

Tgt Ion: 53 Resp: 1491
Ion Ratio Lower Upper
53 100
52 0.0 66.2 99.2#
51 12.9 29.6 44.4#


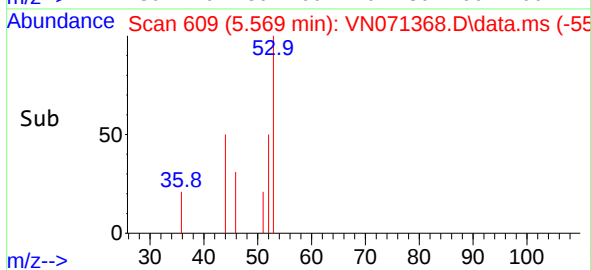
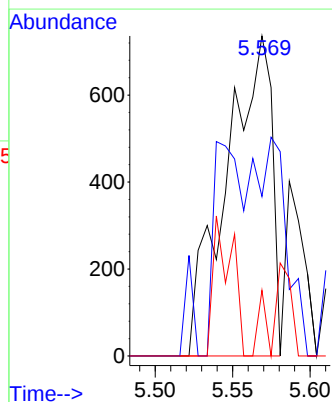





#16
Acetone
Concen: 6.601 ug/l
RT: 4.292 min Scan# 391
Delta R.T. 0.006 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 30027
Ion Ratio Lower Upper
43 100
58 28.9 23.1 34.7



#17
Carbon Disulfide
Concen: 0.299 ug/l
RT: 4.534 min Scan# 433
Delta R.T. 0.006 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29

Tgt Ion: 76 Resp: 5819
Ion Ratio Lower Upper
76 100
78 0.0 7.5 11.3#


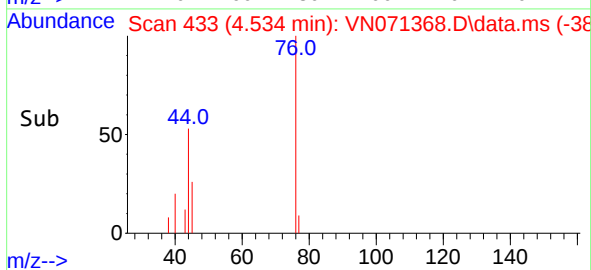






#18
Methyl Acetate
Concen: 1.432 ug/l
RT: 4.863 min Scan# 41
Delta R.T. 0.012 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 11862
Ion Ratio Lower Upper
43 100
74 22.1 19.4 29.2



#20
Methylene Chloride
Concen: 0.629 ug/l
RT: 5.087 min Scan# 527
Delta R.T. -0.006 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29

Tgt Ion: 84 Resp: 2073
Ion Ratio Lower Upper
84 100
49 111.2 93.5 140.3
51 46.2 29.4 44.2#
86 79.7 53.0 79.4#

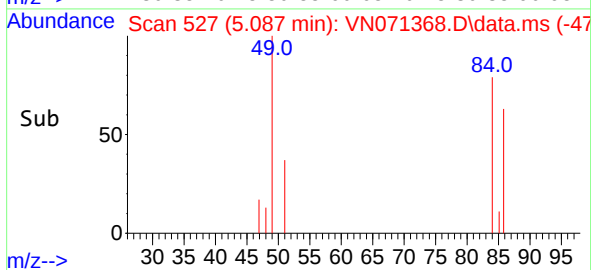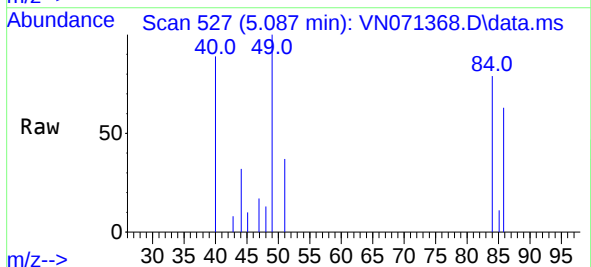



#25

2-Butanone

Concen: 1.215 ug/l

RT: 7.333 min Scan# 909

Delta R.T. -0.000 min

Lab File: VN071368.D

Acq: 18 Mar 2022 13:29

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 8899

Ion Ratio Lower Upper

43 100

72 18.3 21.7 32.5#

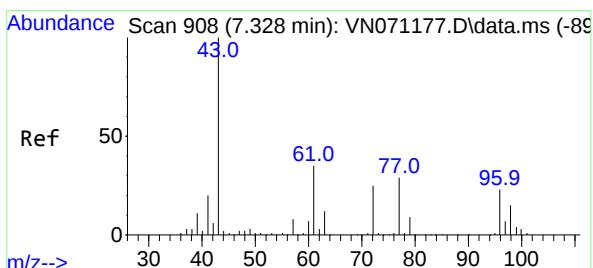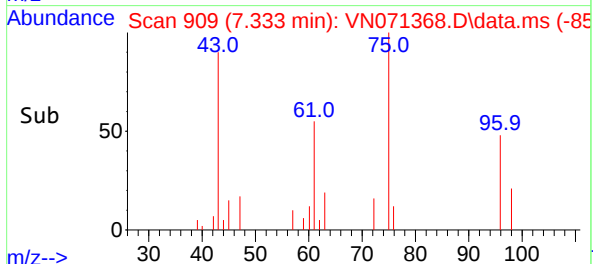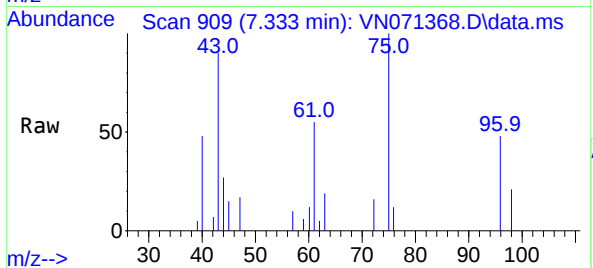

#27

cis-1,2-Dichloroethene

Concen: 0.442 ug/l

RT: 7.333 min Scan# 909

Delta R.T. 0.006 min

Lab File: VN071368.D

Acq: 18 Mar 2022 13:29




Tgt Ion: 96 Resp: 3922


Ion Ratio Lower Upper

96 100

61 155.8 0.0 275.0

98 62.9 0.0 129.6

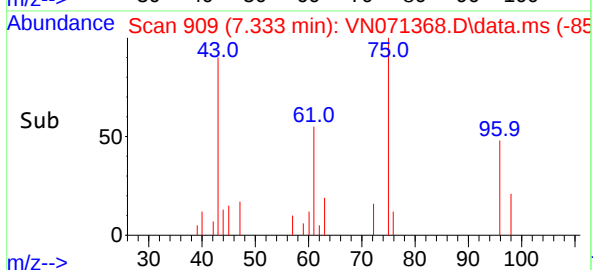



#29

Tetrahydrofuran

Concen: 0.539 ug/l

RT: 7.704 min Scan# 91

Delta R.T. 0.023 min


Lab File: VN071368.D

Acq: 18 Mar 2022 13:29

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 42 Resp: 2734

Ion Ratio Lower Upper

42 100

72 45.6 36.3 54.5

71 52.5 34.7 52.1#

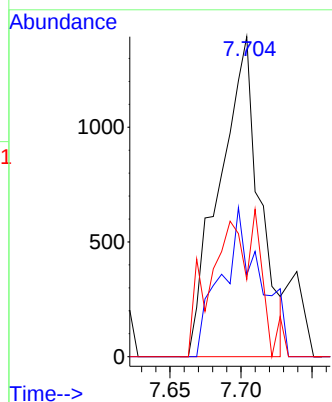

#31

Cyclohexane

Concen: 0.947 ug/l

RT: 8.080 min Scan# 1036

Delta R.T. -0.012 min

Lab File: VN071368.D

Acq: 18 Mar 2022 13:29




Tgt Ion: 56 Resp: 14142


Ion Ratio Lower Upper

56 100

69 172.6 27.1 40.7#

84 169.2 73.4 110.0#

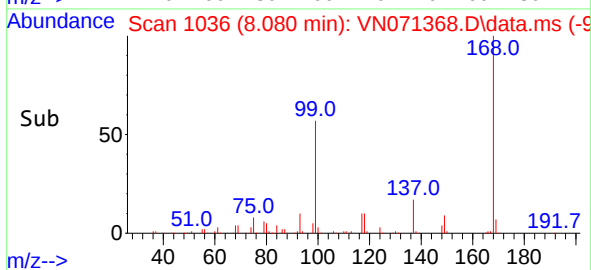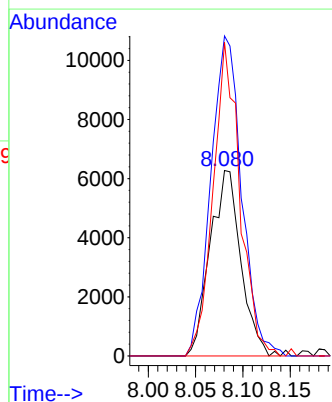



#33

1,2-Dichloroethane-d4

Concen: 47.673 ug/l

RT: 8.433 min Scan# 1097

Delta R.T. -0.006 min

Lab File: VN071368.D

Acq: 18 Mar 2022 13:29

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 445660

Ion Ratio Lower Upper

65 100

67 51.8 0.0 103.0

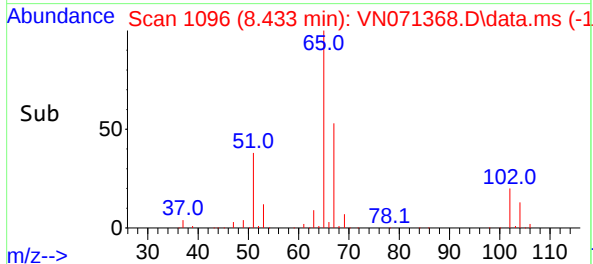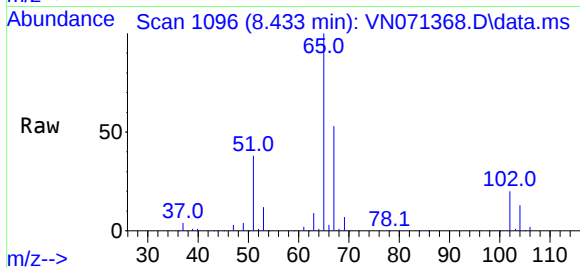

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN071368.D

Acq: 18 Mar 2022 13:29




Tgt Ion:114 Resp: 1138875


Ion Ratio Lower Upper

114 100

63 22.4 0.0 37.8

88 15.9 0.0 27.4


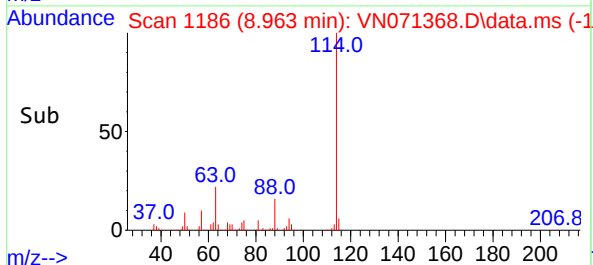

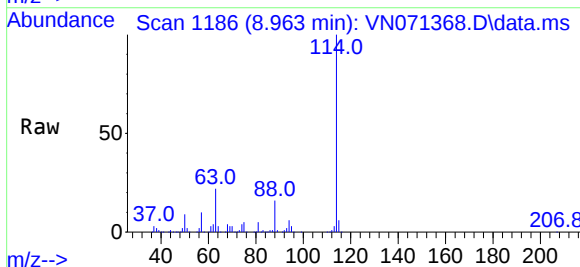


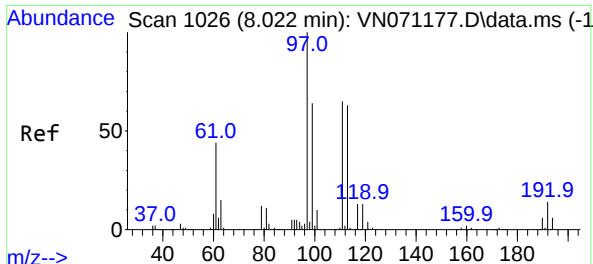

#35
Dibromofluoromethane
Concen: 47.116 ug/l
RT: 8.016 min Scan# 1025
Delta R.T. -0.006 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:113 Resp: 338608
Ion Ratio Lower Upper
113 100
111 102.5 82.2 123.2
192 20.0 16.9 25.3

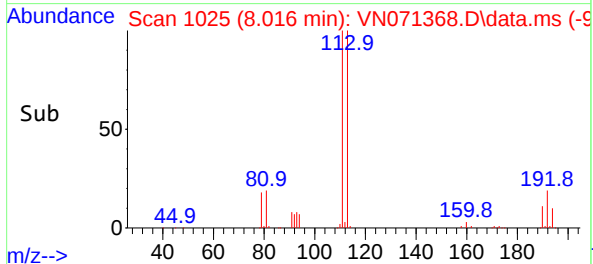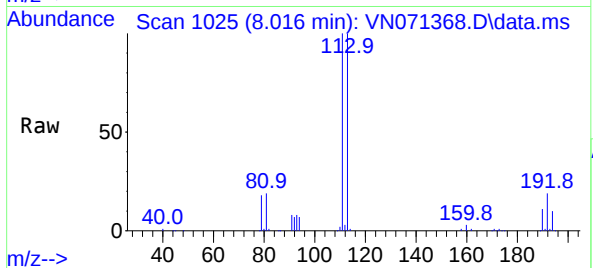

#36
1,1-Dichloropropene
Concen: 4.609 ug/l
RT: 8.080 min Scan# 1036
Delta R.T. -0.135 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29


Tgt Ion: 75 Resp: 53072
Ion Ratio Lower Upper
75 100
110 7.7 18.4 55.2#
77 0.0 24.4 36.6#

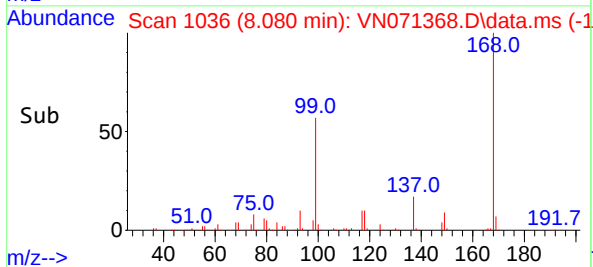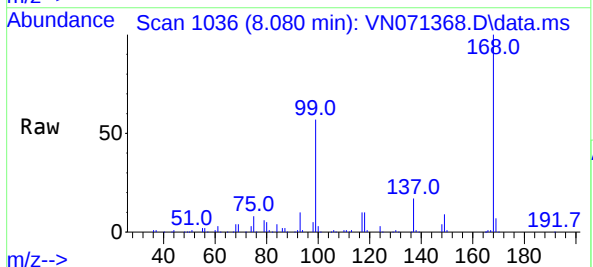






#38
Carbon Tetrachloride
Concen: 6.046 ug/l
RT: 8.080 min Scan# 110
Delta R.T. -0.124 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29


Instrument :
MSVOA_N
ClientSampleId :

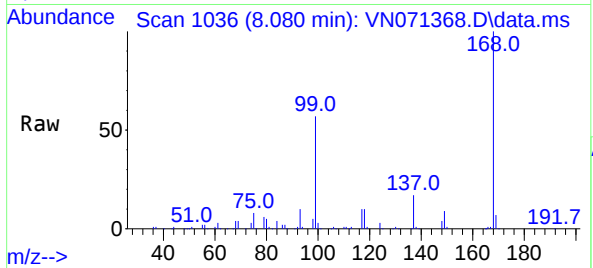



Tgt Ion:117 Resp: 67341
Ion Ratio Lower Upper
117 100
119 6.9 76.1 114.1#
121 0.0 24.2 36.2#

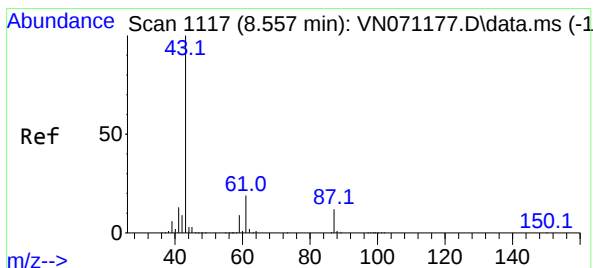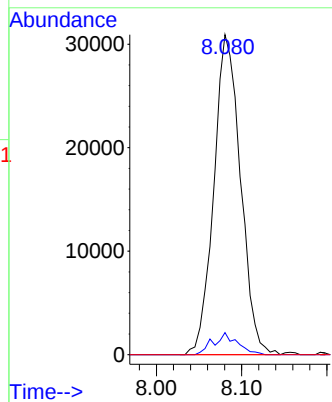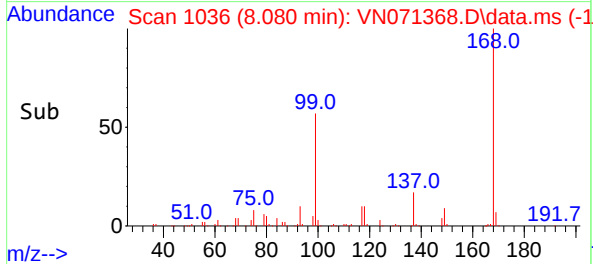


#43
Isopropyl Acetate
Concen: 0.979 ug/l
RT: 8.622 min Scan# 1128
Delta R.T. 0.065 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29

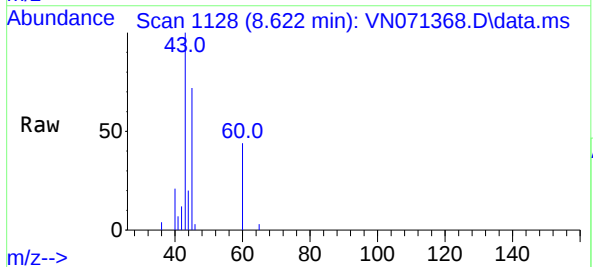

Tgt Ion: 43 Resp: 23203
Ion Ratio Lower Upper
43 100
61 0.0 20.4 30.6#
87 0.0 11.2 16.8#




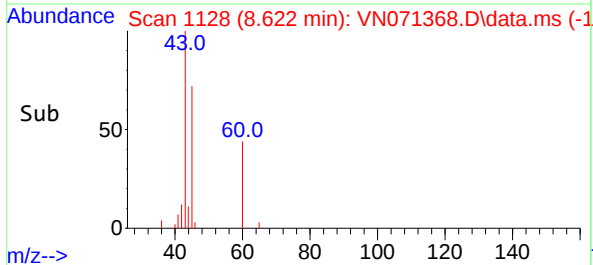




#49
1,4-Dioxane
Concen: 1.388 ug/l
RT: 9.580 min Scan# 11
Delta R.T. 0.017 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 88 Resp: 265
Ion Ratio Lower Upper
88 100
43 0.0 23.4 35.2#
58 94.0 50.6 75.8#

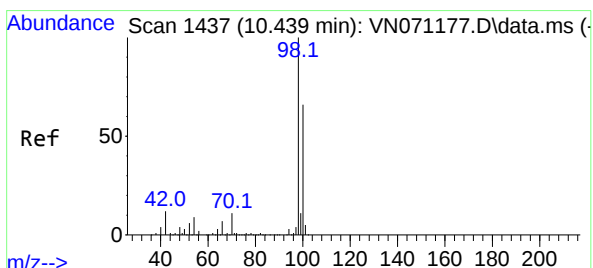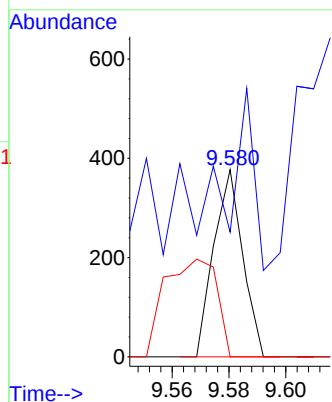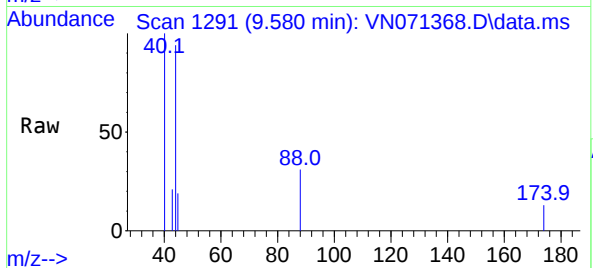

#50
Toluene-d8
Concen: 48.452 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29

Tgt Ion: 98 Resp: 1401983
Ion Ratio Lower Upper
98 100
100 65.3 50.4 75.6


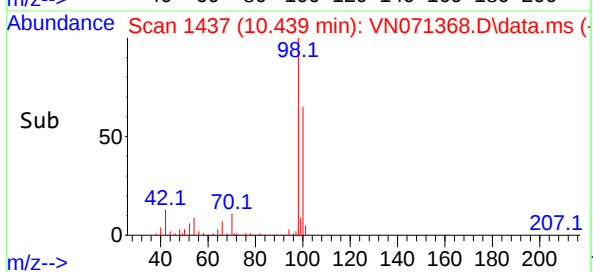
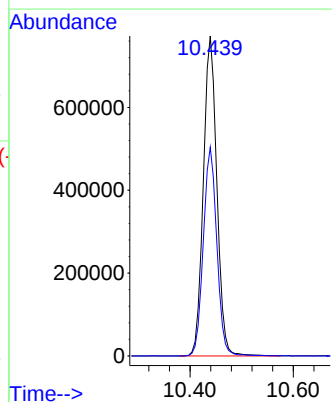





#51
4-Methyl-2-Pentanone
Concen: 0.309 ug/l
RT: 10.327 min Scan# 1418
Delta R.T. 0.000 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 4538
Ion Ratio Lower Upper
43 100
58 39.7 30.4 45.6



#59
2-Hexanone
Concen: 0.854 ug/l
RT: 11.086 min Scan# 1547
Delta R.T. 0.006 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29

Tgt Ion: 43 Resp: 8570
Ion Ratio Lower Upper
43 100
58 43.5 26.9 80.7


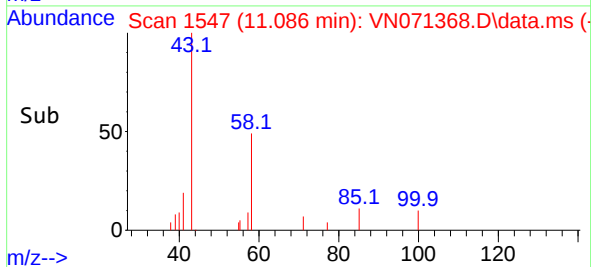

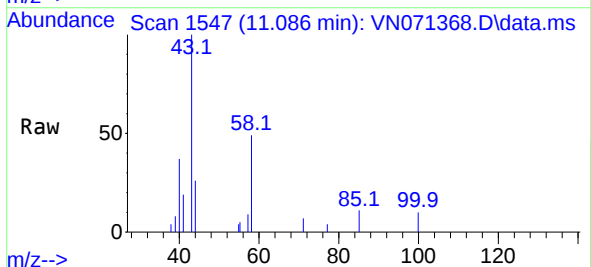


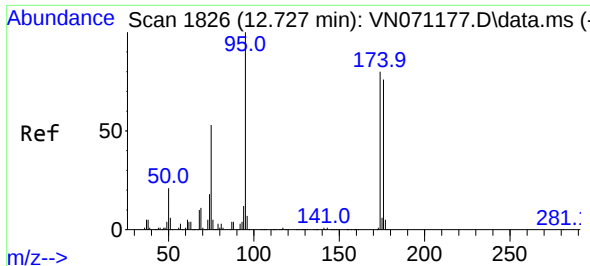

#62
4-Bromofluorobenzene
Concen: 50.822 ug/l
RT: 12.727 min Scan# 1177
Delta R.T. 0.000 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 497976
Ion Ratio Lower Upper
95 100
174 78.2 0.0 187.2
176 75.5 0.0 181.4

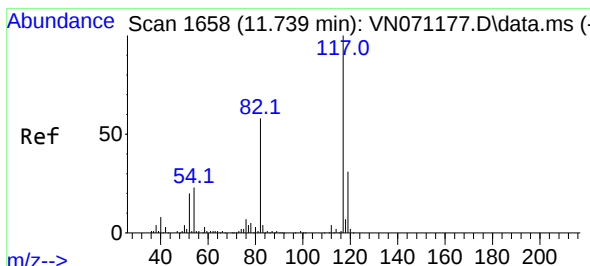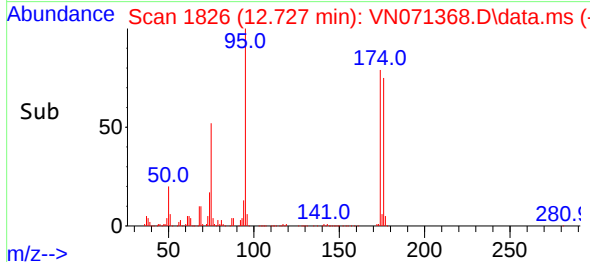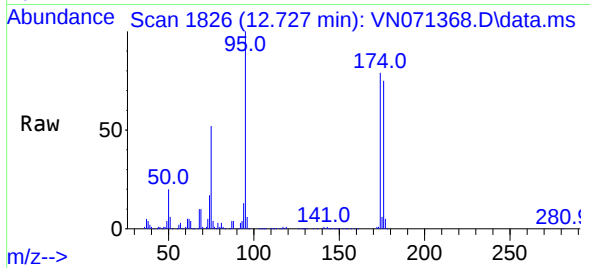

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. -0.000 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29


Tgt Ion: 117 Resp: 1045849
Ion Ratio Lower Upper
117 100
82 58.9 42.4 63.6
119 32.9 25.4 38.2

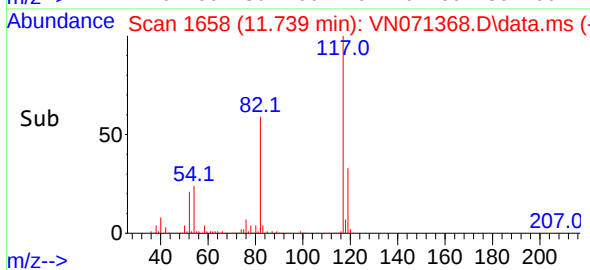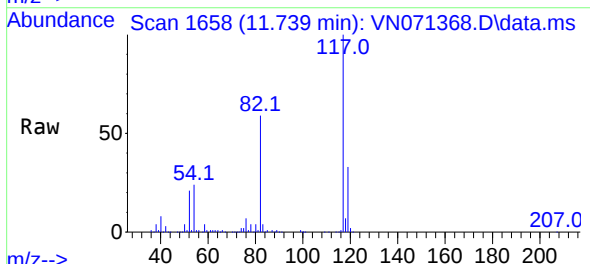






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.668 min Scan# 1986
Delta R.T. 0.000 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:152 Resp: 343202
Ion Ratio Lower Upper
152 100
115 59.4 27.5 82.5
150 158.9 0.0 344.4




#74
N-ethyl acetate
Concen: 0.344 ug/l
RT: 12.380 min Scan# 1767
Delta R.T. -0.006 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29



Tgt Ion: 43 Resp: 4285
Ion Ratio Lower Upper
43 100
70 30.6 33.4 50.0#
55 24.1 19.3 28.9
61 17.1 18.5 27.7#



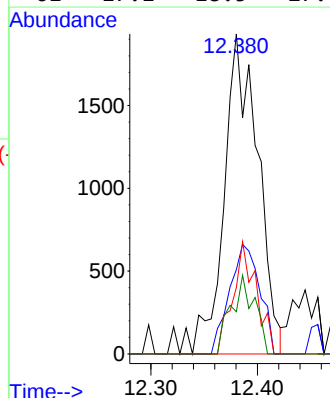





#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.827 min Scan# 1842
Delta R.T. 0.006 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 83 Resp: 1341
Ion Ratio Lower Upper
83 100
131 4.0 5.5 16.5#
85 51.9 32.4 97.2

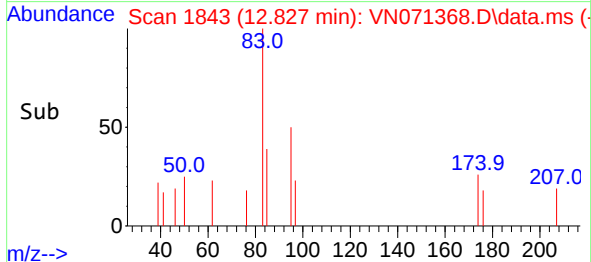

#76
1,2,3-Trichloropropane
Concen: 29.674 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29

Tgt Ion: 75 Resp: 256375
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#


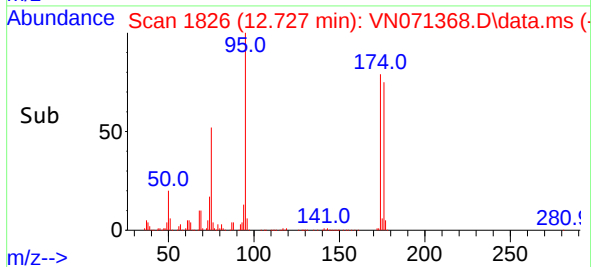

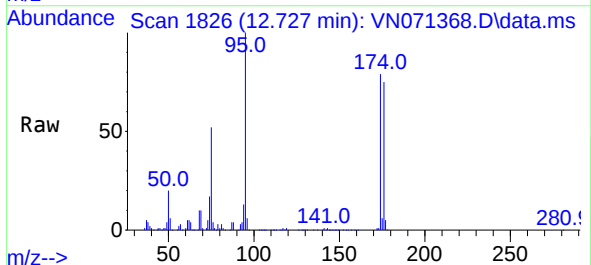




#81
trans-1,4-Dichloro-2-butene
Concen: 80.751 ug/l
RT: 12.727 min Scan# 1808
Delta R.T. 0.106 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 256375
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#



#87
1,3-Dichlorobenzene
Concen: 0.212 ug/l
RT: 13.610 min Scan# 1976
Delta R.T. -0.000 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29


Tgt Ion:146 Resp: 2656
Ion Ratio Lower Upper
146 100
111 39.0 18.6 55.6
148 63.1 31.6 95.0

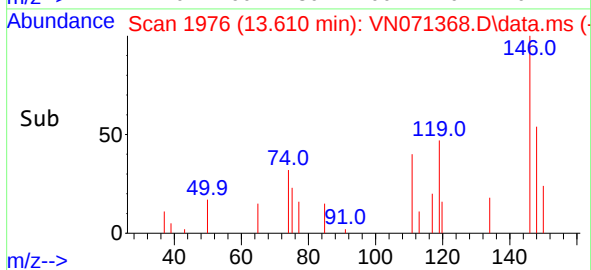






#88
1,4-Dichlorobenzene
Concen: 0.217 ug/l
RT: 13.610 min Scan# 1976
Delta R.T. -0.082 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:146 Resp: 2656
Ion Ratio Lower Upper
146 100
111 39.0 18.3 54.8
148 63.1 31.8 95.4



#89
n-Butylbenzene
Concen: 0.260 ug/l
RT: 13.939 min Scan# 2032
Delta R.T. -0.000 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29

Tgt Ion: 91 Resp: 4882
Ion Ratio Lower Upper
91 100
92 56.8 25.4 76.0
134 27.8 13.6 40.8

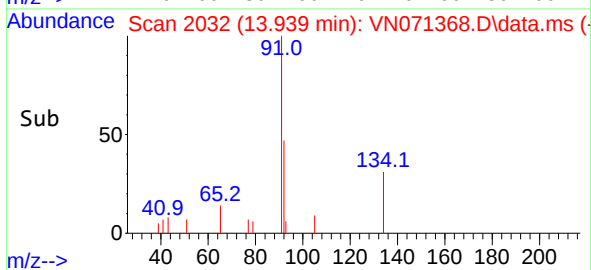



#91

1,2-Dichlorobenzene

Concen: 0.242 ug/l

RT: 13.986 min Scan# 2040

Delta R.T. -0.000 min


Lab File: VN071368.D

Acq: 18 Mar 2022 13:29

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:146 Resp: 2912

Ion Ratio Lower Upper

146 100

111 42.0 19.1 57.3

148 49.4 32.1 96.3

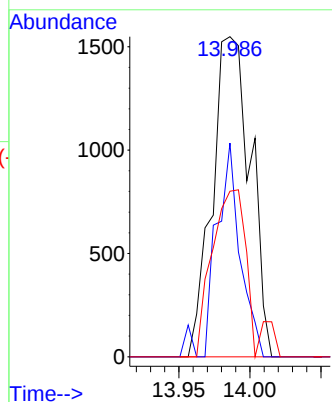

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.299 ug/l

RT: 14.609 min Scan# 2146

Delta R.T. 0.012 min

Lab File: VN071368.D

Acq: 18 Mar 2022 13:29




Tgt Ion: 75 Resp: 576


Ion Ratio Lower Upper

75 100

155 93.9 46.9 140.7


157 124.0 60.6 181.7

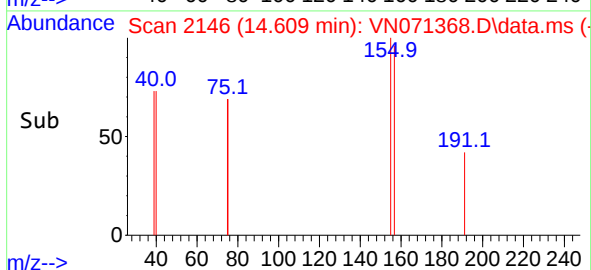






#93
1,2,4-Trichlorobenzene
Concen: 3.570 ug/l
RT: 15.262 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:180 Resp: 3477
Ion Ratio Lower Upper
180 100
182 102.0 48.3 144.9
145 32.6 14.5 43.5




#95
Naphthalene
Concen: 5.708 ug/l
RT: 15.504 min Scan# 2298
Delta R.T. -0.000 min
Lab File: VN071368.D
Acq: 18 Mar 2022 13:29




Tgt Ion:128 Resp: 11204
Ion Ratio Lower Upper
128 100
127 12.9 10.5 15.7
129 11.0 8.7 13.1

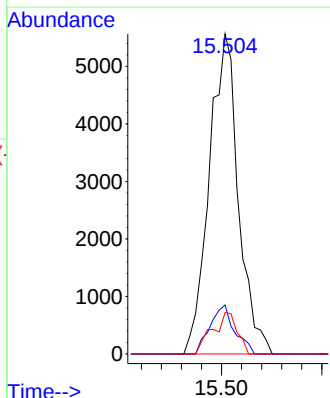



#96
 1,2,3-Trichlorobenzene
 Concen: 3.481 ug/l
 RT: 15.698 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN071368.D
 Acq: 18 Mar 2022 13:29

Instrument :
 MSVOA_N
 ClientSampleId :



Tgt Ion:	180	Resp:	4269
Ion	Ratio	Lower	Upper
180	100		
182	88.9	47.4	142.2
145	17.2	15.0	45.1

