

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031822\
 Data File : VN071376.D
 Acq On : 18 Mar 2022 16:42
 Operator : JC\MD
 Sample : N1974-13
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Mar 19 07:09:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	819708	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.969	114	1376127	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1330497	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	505901	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	531574	47.317	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	94.640%
35) Dibromofluoromethane	8.016	113	405004	46.639	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	93.280%
50) Toluene-d8	10.439	98	1709109	48.882	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	97.760%
62) 4-Bromofluorobenzene	12.727	95	663380	56.031	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	112.060%
Target Compounds						
					Qvalue	
3) Chloromethane	2.287	50	79548	6.566	ug/l #	45
5) Bromomethane	2.845	94	368	Below Cal	#	76
16) Acetone	4.292	43	13092	2.395	ug/l #	85
17) Carbon Disulfide	4.534	76	141450	6.046	ug/l	98
18) Methyl Acetate	4.857	43	9409	1.105	ug/l	94
20) Methylene Chloride	5.098	84	517	0.433	ug/l #	50
25) 2-Butanone	7.345	43	3190	0.362	ug/l	100
31) Cyclohexane	8.080	56	18443	1.028	ug/l #	2
36) 1,1-Dichloropropene	8.080	75	64453	4.632	ug/l #	49
38) Carbon Tetrachloride	8.086	117	80434	5.977	ug/l #	17
39) Methylcyclohexane	9.451	83	3951	0.241	ug/l #	77
40) Benzene	8.457	78	204944	4.889	ug/l	95
43) Isopropyl Acetate	8.610	43	49106	1.715	ug/l #	55
52) Toluene	10.504	92	85867	3.326	ug/l	99
67) Ethyl Benzene	11.845	91	187147	3.704	ug/l	98
68) m/p-Xylenes	11.945	106	119521	6.467	ug/l	99
69) o-Xylene	12.274	106	55968	3.021	ug/l	96
73) Isopropylbenzene	12.574	105	13500	0.277	ug/l	84
75) 1,1,2,2-Tetrachloroethane	12.821	83	385	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.727	75	345245	26.850	ug/l #	1
78) n-propylbenzene	12.915	91	15805	0.302	ug/l	100
79) 2-Chlorotoluene	12.974	91	9849	0.293	ug/l #	41
80) 1,3,5-Trimethylbenzene	13.057	105	26621	0.702	ug/l	91
81) trans-1,4-Dichloro-2-b...	12.727	75	345245	73.771	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.362	105	103747	2.855	ug/l	99
85) sec-Butylbenzene	13.362	105	103747	2.305	ug/l #	56
86) p-Isopropyltoluene	13.609	119	7153	0.202	ug/l	96
90) Hexachloroethane	14.204	117	1731	0.246	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.262	180	454	3.041	ug/l #	1
95) Naphthalene	15.503	128	166384	11.515	ug/l	99
96) 1,2,3-Trichlorobenzene	15.703	180	117	2.746	ug/l #	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Mar 19 07:09:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 10
Delta R.T. 0.000 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 819708
Ion Ratio Lower Upper
168 100
99 57.6 41.3 61.9



#3
Chloromethane
Concen: 6.566 ug/l
RT: 2.287 min Scan# 51
Delta R.T. -0.012 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion: 50 Resp: 79548
Ion Ratio Lower Upper
50 100
52 1.1 25.4 38.0#



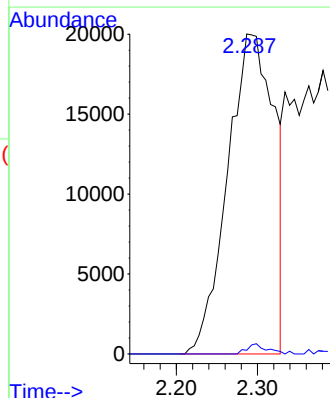





#5
Bromomethane
Concen: Below Cal
RT: 2.845 min Scan# 14
Delta R.T. 0.011 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 368
Ion Ratio Lower Upper
94 100
96 69.8 73.8 110.8#

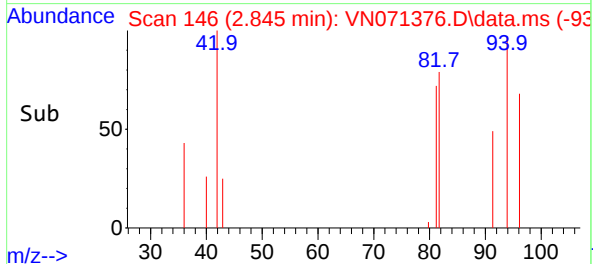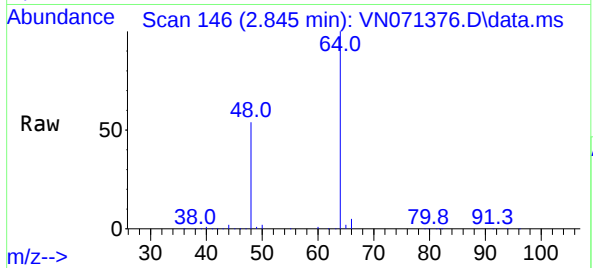

#16
Acetone
Concen: 2.395 ug/l
RT: 4.292 min Scan# 392
Delta R.T. 0.006 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion: 43 Resp: 13092
Ion Ratio Lower Upper
43 100
58 21.0 23.1 34.7#


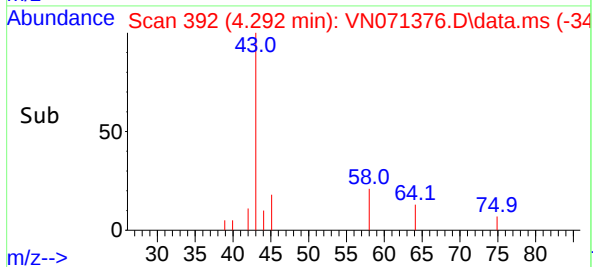

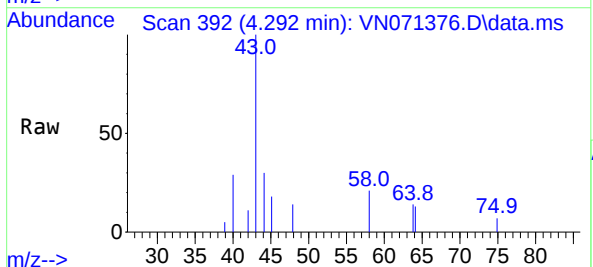




#17
Carbon Disulfide
Concen: 6.046 ug/l
RT: 4.534 min Scan# 411
Delta R.T. 0.006 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 76 Resp: 141450
Ion Ratio Lower Upper
76 100
78 8.6 7.5 11.3

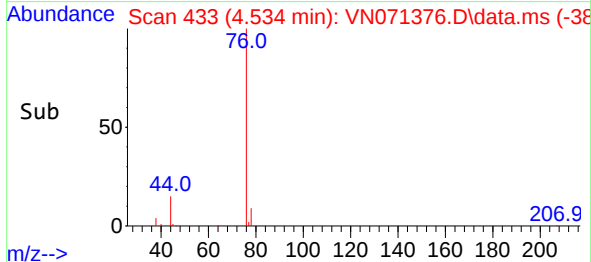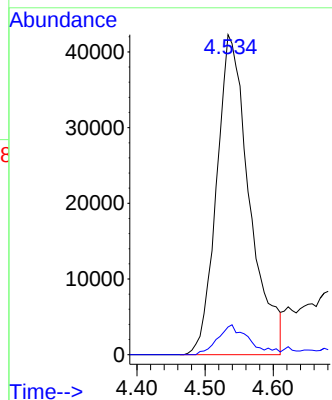

#18
Methyl Acetate
Concen: 1.105 ug/l
RT: 4.857 min Scan# 488
Delta R.T. 0.006 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42


Tgt Ion: 43 Resp: 9409
Ion Ratio Lower Upper
43 100
74 21.2 19.4 29.2

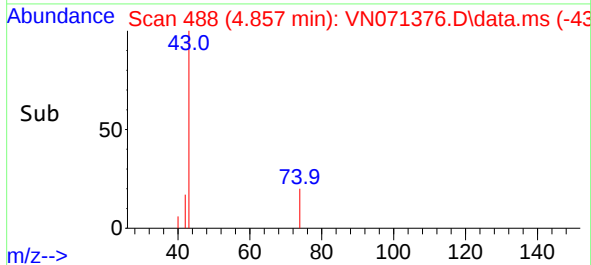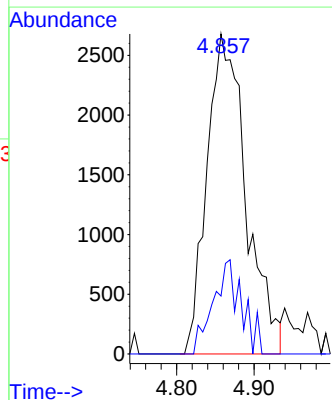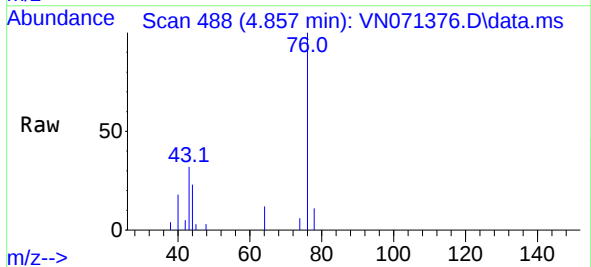






#20
Methylene Chloride
Concen: 0.433 ug/l
RT: 5.098 min Scan# 517
Delta R.T. 0.005 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Instrument :
MSVOA_N
ClientSampleId :



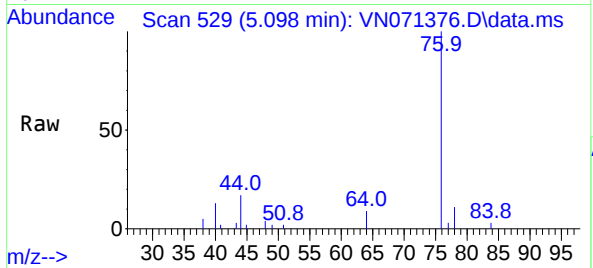



Tgt Ion: 84 Resp: 517
Ion Ratio Lower Upper
84 100
49 75.8 93.5 140.3#
51 54.6 29.4 44.2#
86 0.0 53.0 79.4#

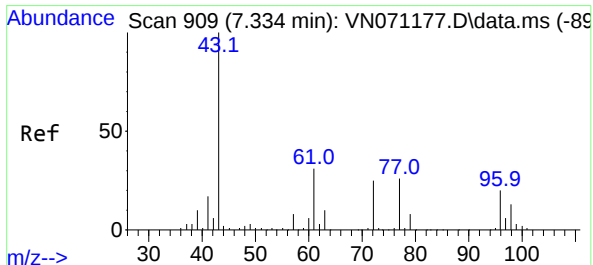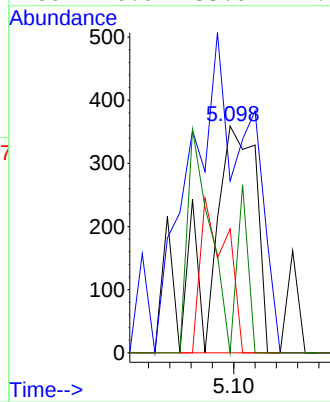

#25
2-Butanone
Concen: 0.362 ug/l
RT: 7.345 min Scan# 911
Delta R.T. 0.012 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion: 43 Resp: 3190
Ion Ratio Lower Upper
43 100
72 27.1 21.7 32.5

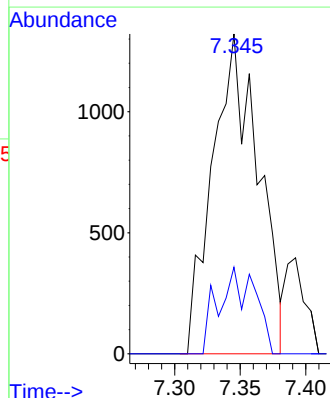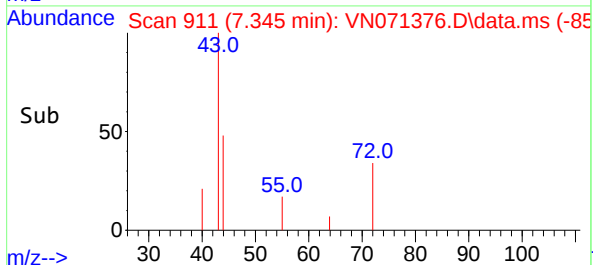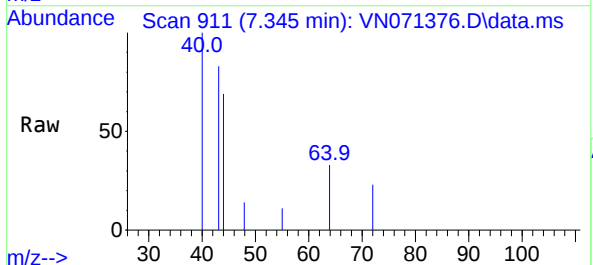



#31

Cyclohexane

Concen: 1.028 ug/l

RT: 8.080 min Scan# 1036

Delta R.T. -0.012 min

Lab File: VN071376.D

Acq: 18 Mar 2022 16:42

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 56 Resp: 18443

Ion Ratio Lower Upper

56 100

69 165.8 27.1 40.7#

84 138.3 73.4 110.0#

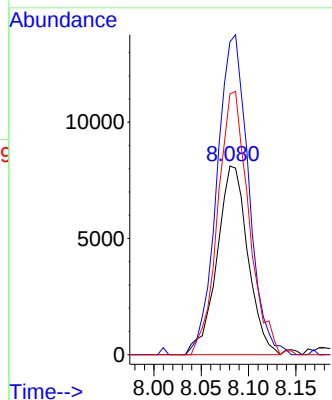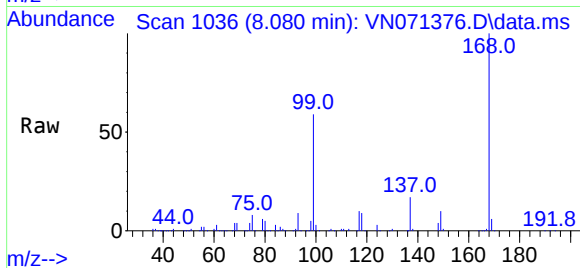

#33

1,2-Dichloroethane-d4

Concen: 47.317 ug/l

RT: 8.433 min Scan# 1096

Delta R.T. -0.006 min

Lab File: VN071376.D




Acq: 18 Mar 2022 16:42


Tgt Ion: 65 Resp: 531574

Ion Ratio Lower Upper

65 100

67 52.2 0.0 103.0

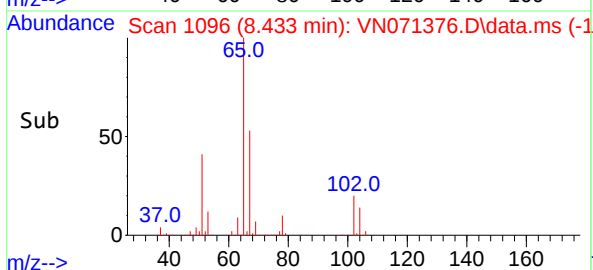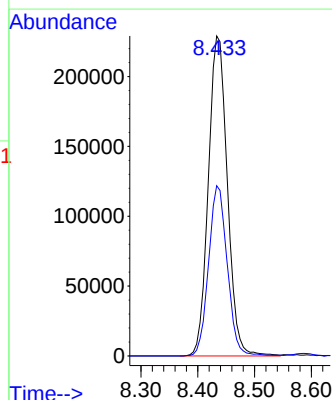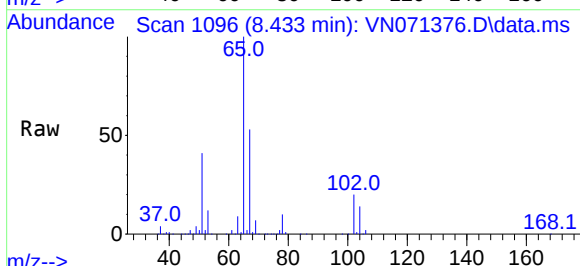

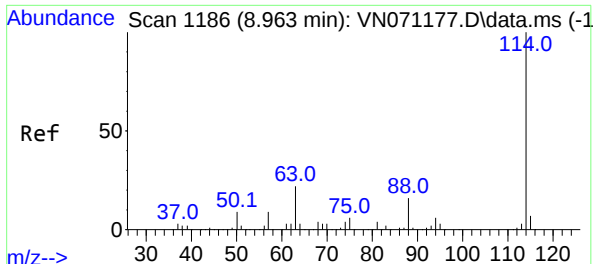

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.969 min Scan# 1186

Delta R.T. 0.006 min

Lab File: VN071376.D

Acq: 18 Mar 2022 16:42

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 1376127

Ion Ratio Lower Upper

114 100

63 21.2 0.0 37.8

88 15.3 0.0 27.4

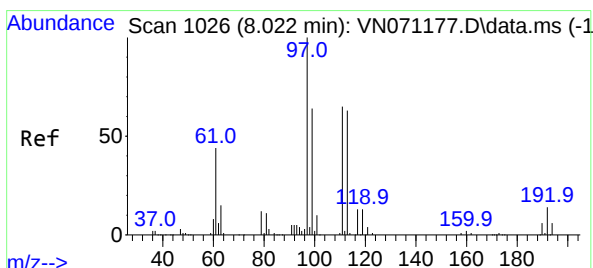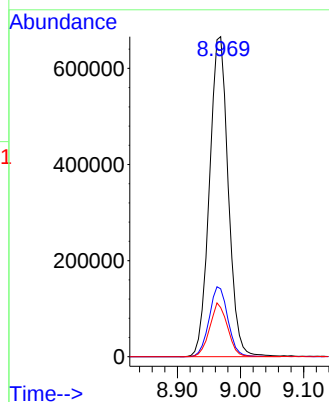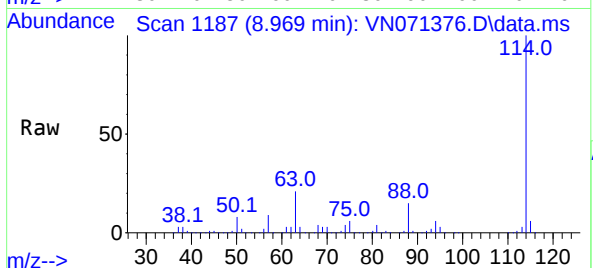

#35

Dibromofluoromethane

Concen: 46.639 ug/l

RT: 8.016 min Scan# 1025

Delta R.T. -0.006 min

Lab File: VN071376.D

Acq: 18 Mar 2022 16:42




Tgt Ion:113 Resp: 405004


Ion Ratio Lower Upper

113 100

111 102.8 82.2 123.2

192 20.2 16.9 25.3

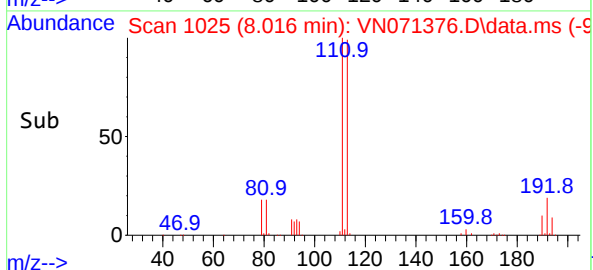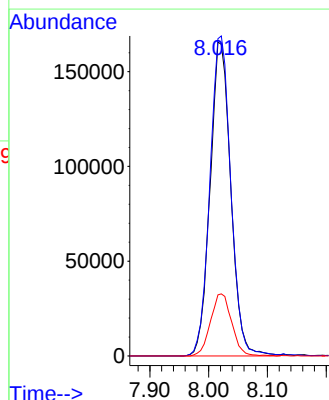



#36

1,1-Dichloropropene

Concen: 4.632 ug/l

RT: 8.080 min Scan# 1036

Delta R.T. -0.135 min

Lab File: VN071376.D

Acq: 18 Mar 2022 16:42

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 75 Resp: 64453

Ion Ratio Lower Upper

75 100

110 9.2 18.4 55.2#

77 0.0 24.4 36.6#

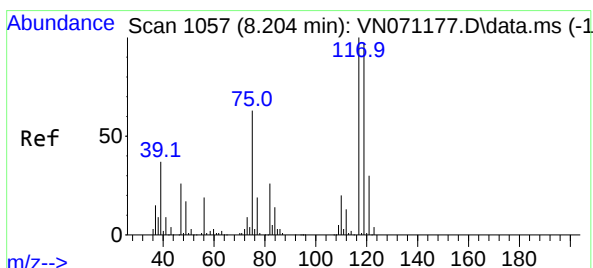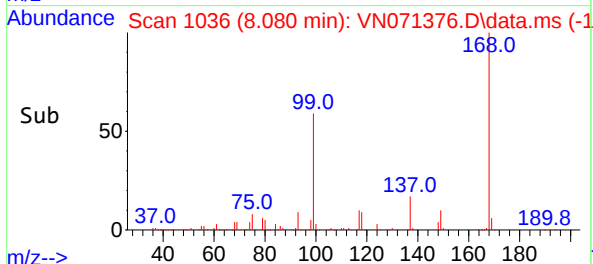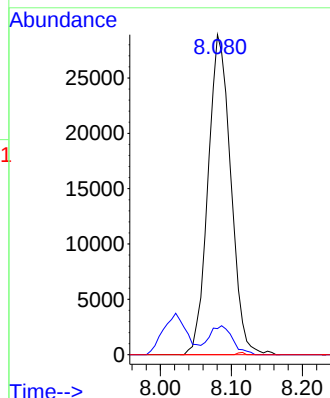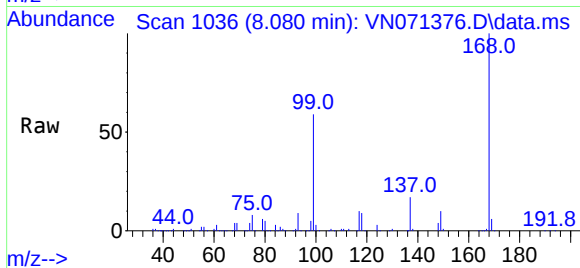

#38

Carbon Tetrachloride

Concen: 5.977 ug/l

RT: 8.086 min Scan# 1037

Delta R.T. -0.118 min

Lab File: VN071376.D

Acq: 18 Mar 2022 16:42




Tgt Ion: 117 Resp: 80434


Ion Ratio Lower Upper

117 100

119 5.8 76.1 114.1#


121 0.0 24.2 36.2#

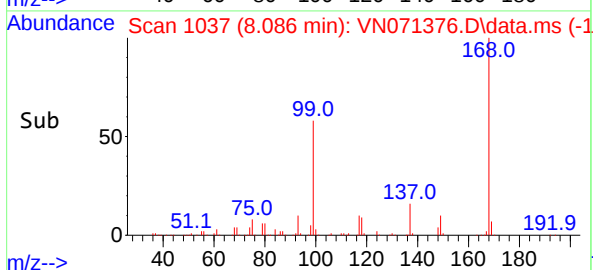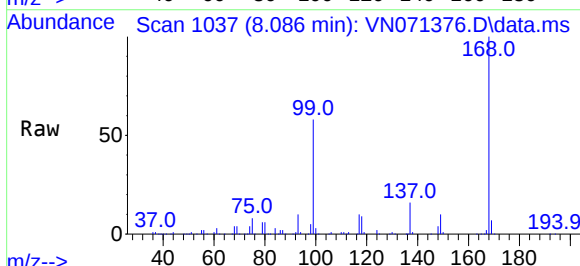






#39
Methylcyclohexane
Concen: 0.241 ug/l
RT: 9.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Instrument :
MSVOA_N
ClientSampleId :



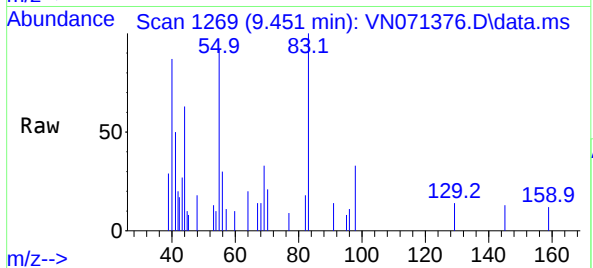



Tgt Ion: 83 Resp: 3951
Ion Ratio Lower Upper
83 100
55 91.8 58.1 87.1#
98 32.6 38.4 57.6#

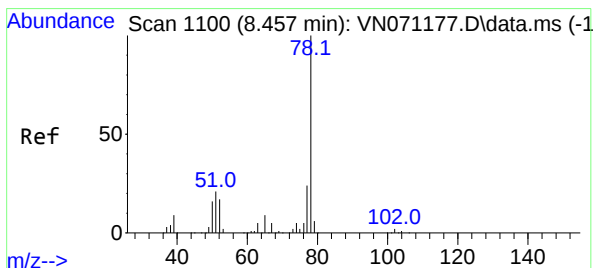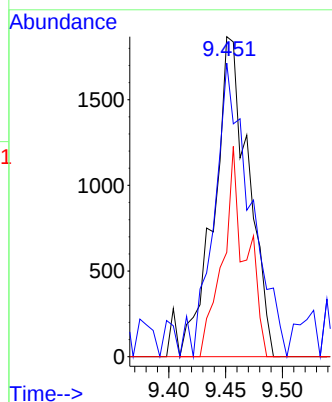

#40
Benzene
Concen: 4.889 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. -0.000 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion: 78 Resp: 204944
Ion Ratio Lower Upper
78 100
77 20.8 18.6 27.8

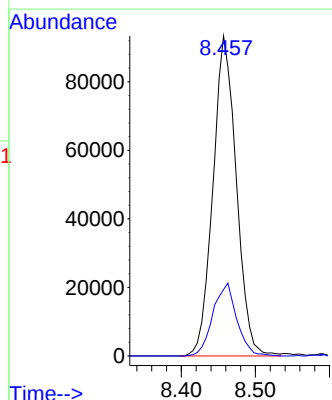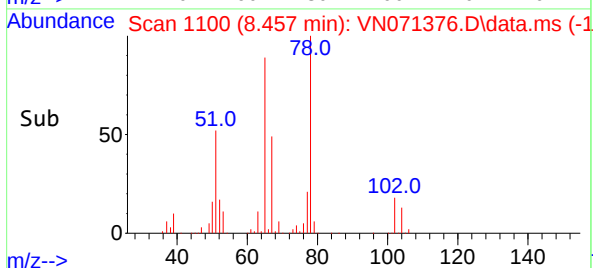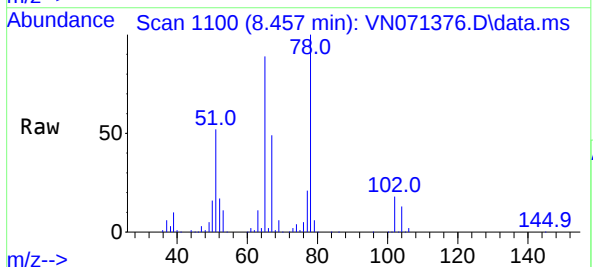

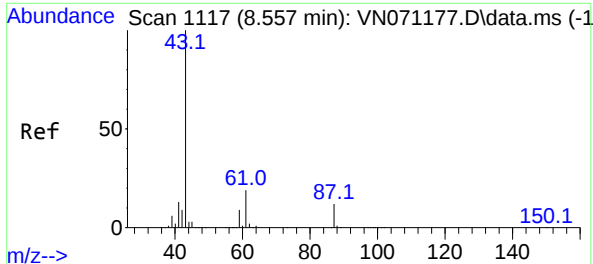

#43

Isopropyl Acetate

Concen: 1.715 ug/l

RT: 8.610 min Scan# 1117

Delta R.T. 0.053 min

Lab File: VN071376.D

Acq: 18 Mar 2022 16:42

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 43 Resp: 49106

Ion Ratio Lower Upper

43 100

61 0.0 20.4 30.6#

87 0.0 11.2 16.8#

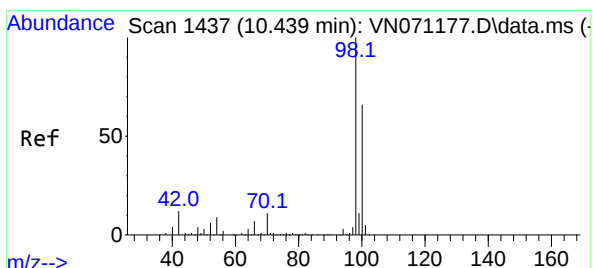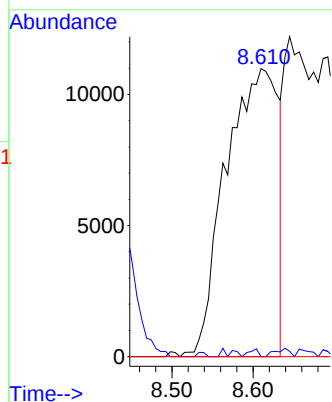

#50

Toluene-d8

Concen: 48.882 ug/l

RT: 10.439 min Scan# 1437

Delta R.T. 0.000 min

Lab File: VN071376.D




Acq: 18 Mar 2022 16:42


Tgt Ion: 98 Resp: 1709109

Ion Ratio Lower Upper

98 100

100 66.0 50.4 75.6


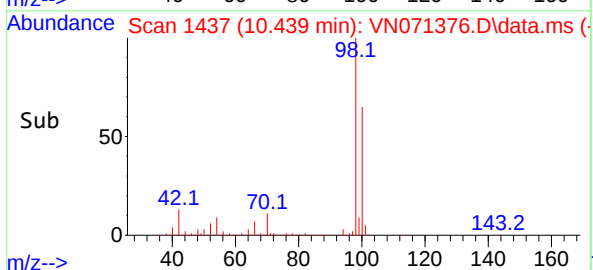
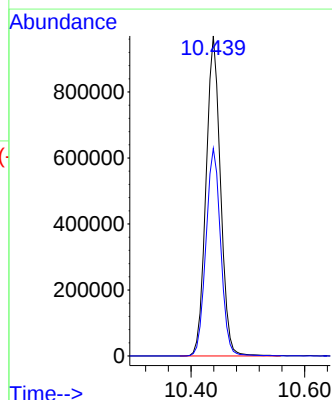
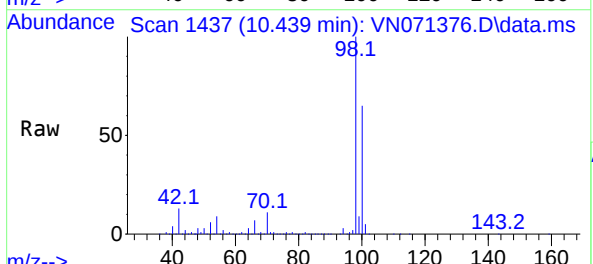




#52
Toluene
Concen: 3.326 ug/l
RT: 10.504 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 92 Resp: 85867
Ion Ratio Lower Upper
92 100
91 175.6 142.0 213.0

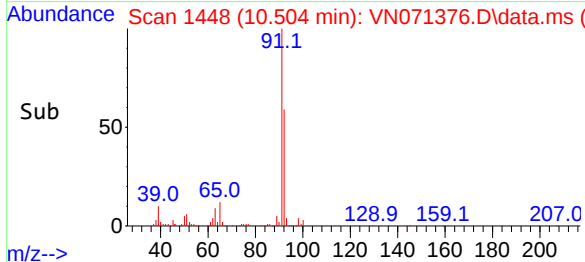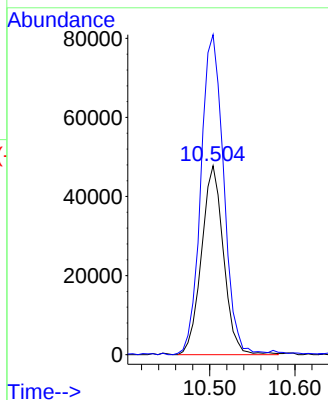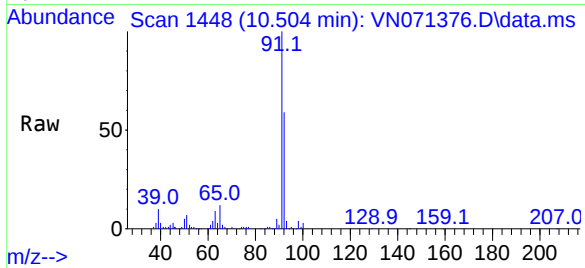

#62
4-Bromofluorobenzene
Concen: 56.031 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion: 95 Resp: 663380
Ion Ratio Lower Upper
95 100
174 77.9 0.0 187.2
176 75.3 0.0 181.4

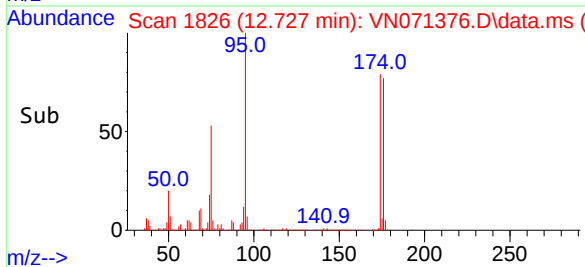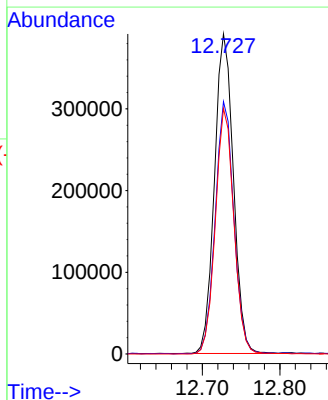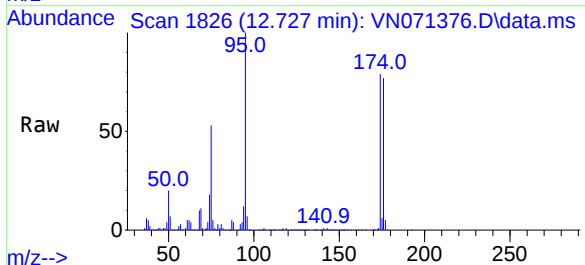



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.739 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN071376.D

Acq: 18 Mar 2022 16:42





Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:117 Resp: 1330497

Ion	Ratio	Lower	Upper
117	100		
82	58.3	42.4	63.6
119	32.0	25.4	38.2

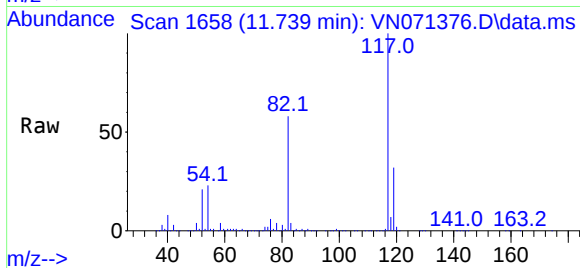

#67

Ethyl Benzene

Concen: 3.704 ug/l

RT: 11.845 min Scan# 1676




Delta R.T. 0.006 min


Lab File: VN071376.D

Acq: 18 Mar 2022 16:42

Tgt Ion: 91 Resp: 187147

Ion	Ratio	Lower	Upper
91	100		
106	31.0	25.7	38.5


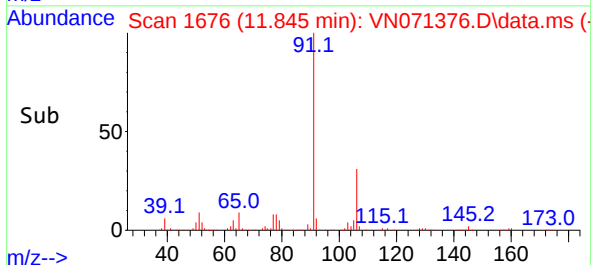
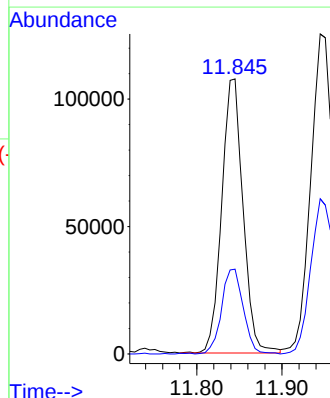
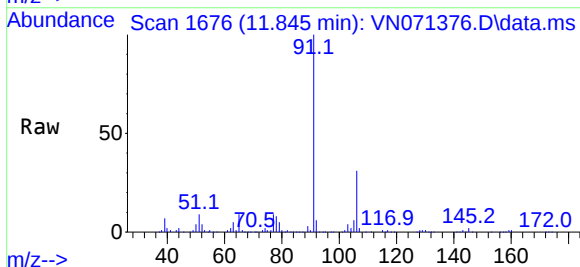




#68
m/p-Xylenes
Concen: 6.467 ug/l
RT: 11.945 min Scan# 119521
Delta R.T. -0.006 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 119521
Ion Ratio Lower Upper
106 100
91 202.8 160.6 240.8



#69
o-Xylene
Concen: 3.021 ug/l
RT: 12.274 min Scan# 1749
Delta R.T. -0.006 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion:106 Resp: 55968
Ion Ratio Lower Upper
106 100
91 218.6 105.8 317.3




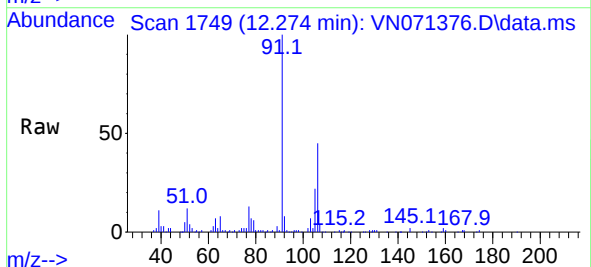




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1986
Delta R.T. 0.006 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:152 Resp: 505901
Ion Ratio Lower Upper
152 100
115 60.4 27.5 82.5
150 155.6 0.0 344.4



#73
Isopropylbenzene
Concen: 0.277 ug/l
RT: 12.574 min Scan# 1800
Delta R.T. 0.000 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion:105 Resp: 13500
Ion Ratio Lower Upper
105 100
120 35.2 13.4 40.1



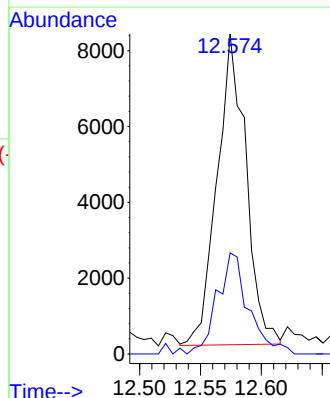





#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.821 min Scan# 1842
Delta R.T. 0.000 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 83 Resp: 385
Ion Ratio Lower Upper
83 100
131 285.5 5.5 16.5#
85 41.8 32.4 97.2

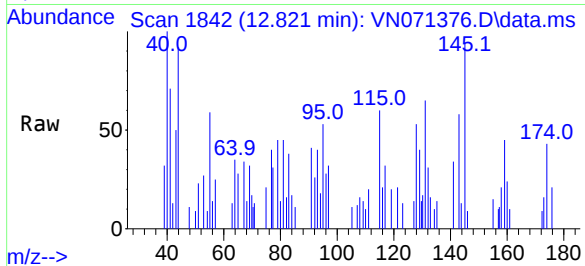

#76
1,2,3-Trichloropropane
Concen: 26.850 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion: 75 Resp: 345245
Ion Ratio Lower Upper
75 100
77 1.4 82.6 247.8#


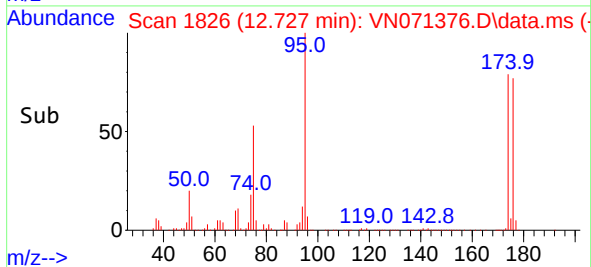

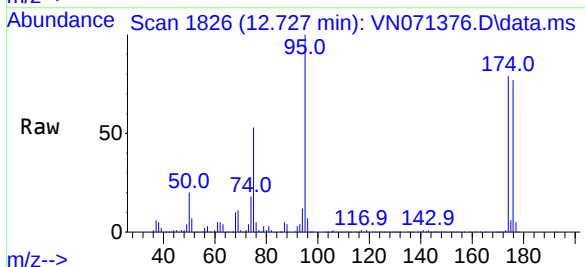


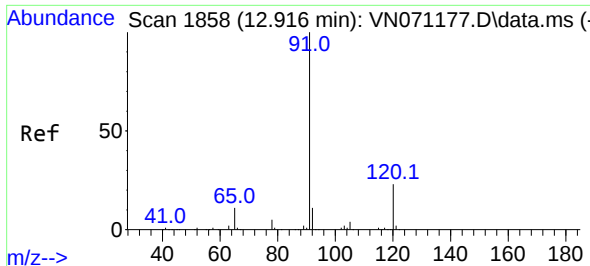

#78
n-propylbenzene
Concen: 0.302 ug/l
RT: 12.915 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 15805
Ion Ratio Lower Upper
91 100
120 24.1 11.9 35.9

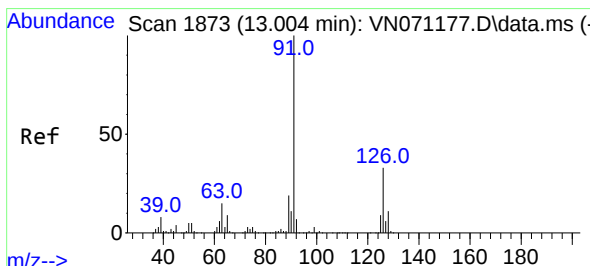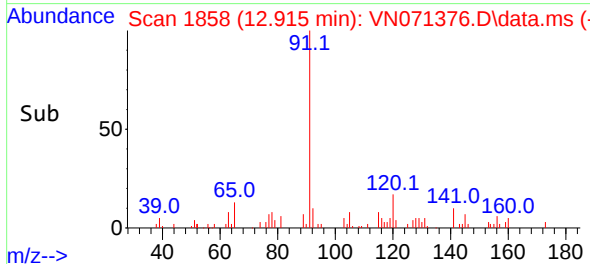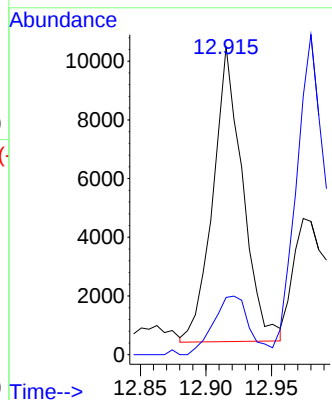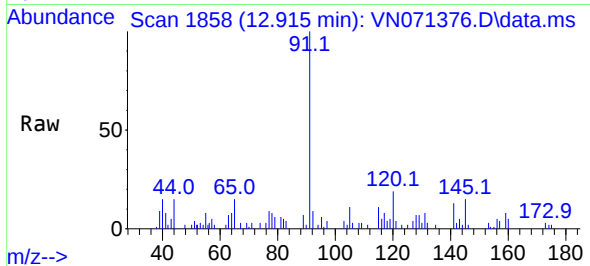

#79
2-Chlorotoluene
Concen: 0.293 ug/l
RT: 12.974 min Scan# 1868
Delta R.T. -0.030 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion: 91 Resp: 9849
Ion Ratio Lower Upper
91 100
126 1.8 18.3 54.8#


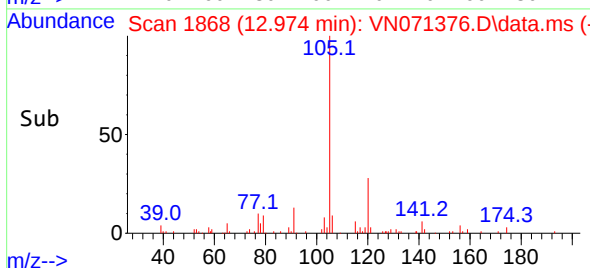
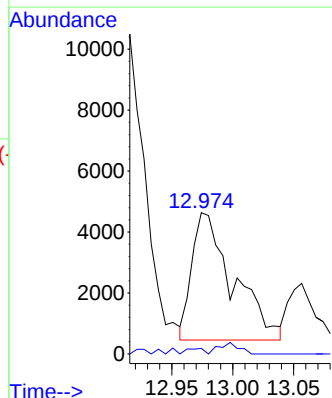
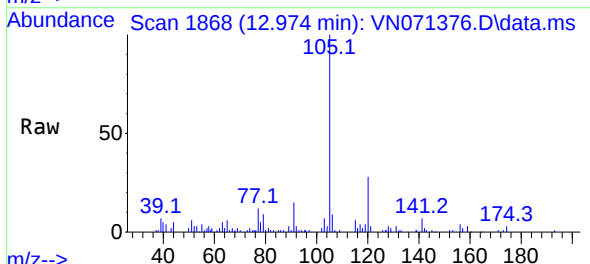




#80
1,3,5-Trimethylbenzene
Concen: 0.702 ug/l
RT: 13.057 min Scan# 1882
Delta R.T. -0.000 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:105 Resp: 26621
Ion Ratio Lower Upper
105 100
120 55.1 24.6 73.6

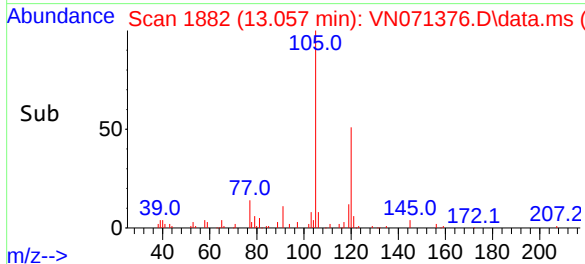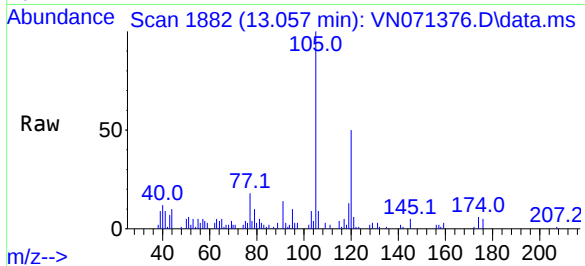

#81
trans-1,4-Dichloro-2-butene
Concen: 73.771 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion: 75 Resp: 345245
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#


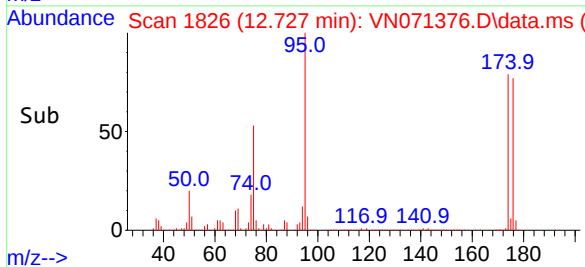

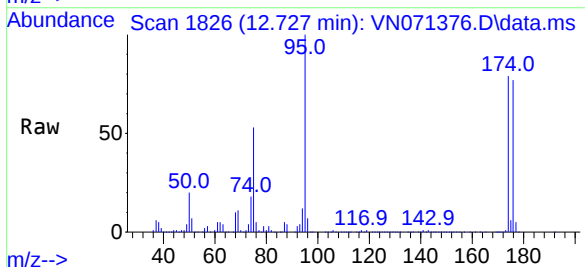




#84
1,2,4-Trimethylbenzene
Concen: 2.855 ug/l
RT: 13.362 min Scan# 1934
Delta R.T. -0.001 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:105 Resp: 103747
Ion Ratio Lower Upper
105 100
120 46.0 22.8 68.4

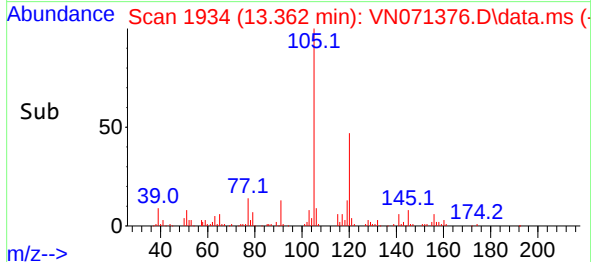

#85
sec-Butylbenzene
Concen: 2.305 ug/l
RT: 13.362 min Scan# 1934
Delta R.T. -0.135 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion:105 Resp: 103747
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#



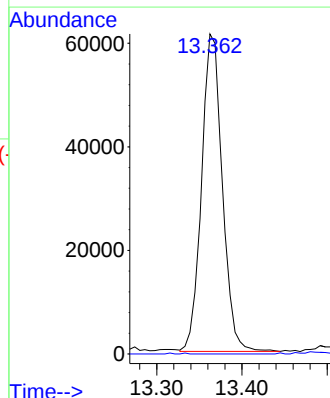





#86
p-Isopropyltoluene
Concen: 0.202 ug/l
RT: 13.609 min Scan# 1976
Delta R.T. -0.000 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42



Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:119 Resp: 7153
Ion Ratio Lower Upper
119 100
134 26.2 13.6 40.7
91 19.7 11.4 34.1



#90
Hexachloroethane
Concen: 0.246 ug/l
RT: 14.204 min Scan# 2077
Delta R.T. -0.006 min
Lab File: VN071376.D
Acq: 18 Mar 2022 16:42

Tgt Ion:117 Resp: 1731
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#





#93

1,2,4-Trichlorobenzene

Concen: 3.041 ug/l

RT: 15.262 min Scan# 21

Delta R.T. 0.000 min

Lab File: VN071376.D





Acq: 18 Mar 2022 16:42

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:180	Resp:	454
Ion Ratio	Lower	Upper
180	100	
182	60.1	48.3 144.9
145	447.6	14.5 43.5#



#95

Naphthalene

Concen: 11.515 ug/l




RT: 15.503 min Scan# 2298


Delta R.T. -0.001 min

Lab File: VN071376.D

Acq: 18 Mar 2022 16:42


Tgt Ion:128	Resp:	166384
Ion Ratio	Lower	Upper
128	100	
127	13.5	10.5 15.7
129	11.3	8.7 13.1

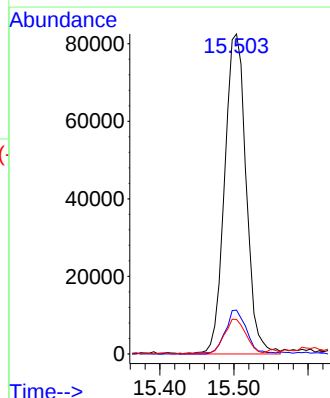



#96
 1,2,3-Trichlorobenzene
 Concen: 2.746 ug/l
 RT: 15.703 min Scan# 21
 Delta R.T. 0.005 min
 Lab File: VN071376.D
 Acq: 18 Mar 2022 16:42

Instrument :
 MSVOA_N
 ClientSampleId :



Tgt Ion:180 Resp: 117
 Ion Ratio Lower Upper
 180 100
 182 120.5 47.4 142.2
 145 0.0 15.0 45.1#

