


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031824\
Data File : VN081450.D
Acq On : 18 Mar 2024 14:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

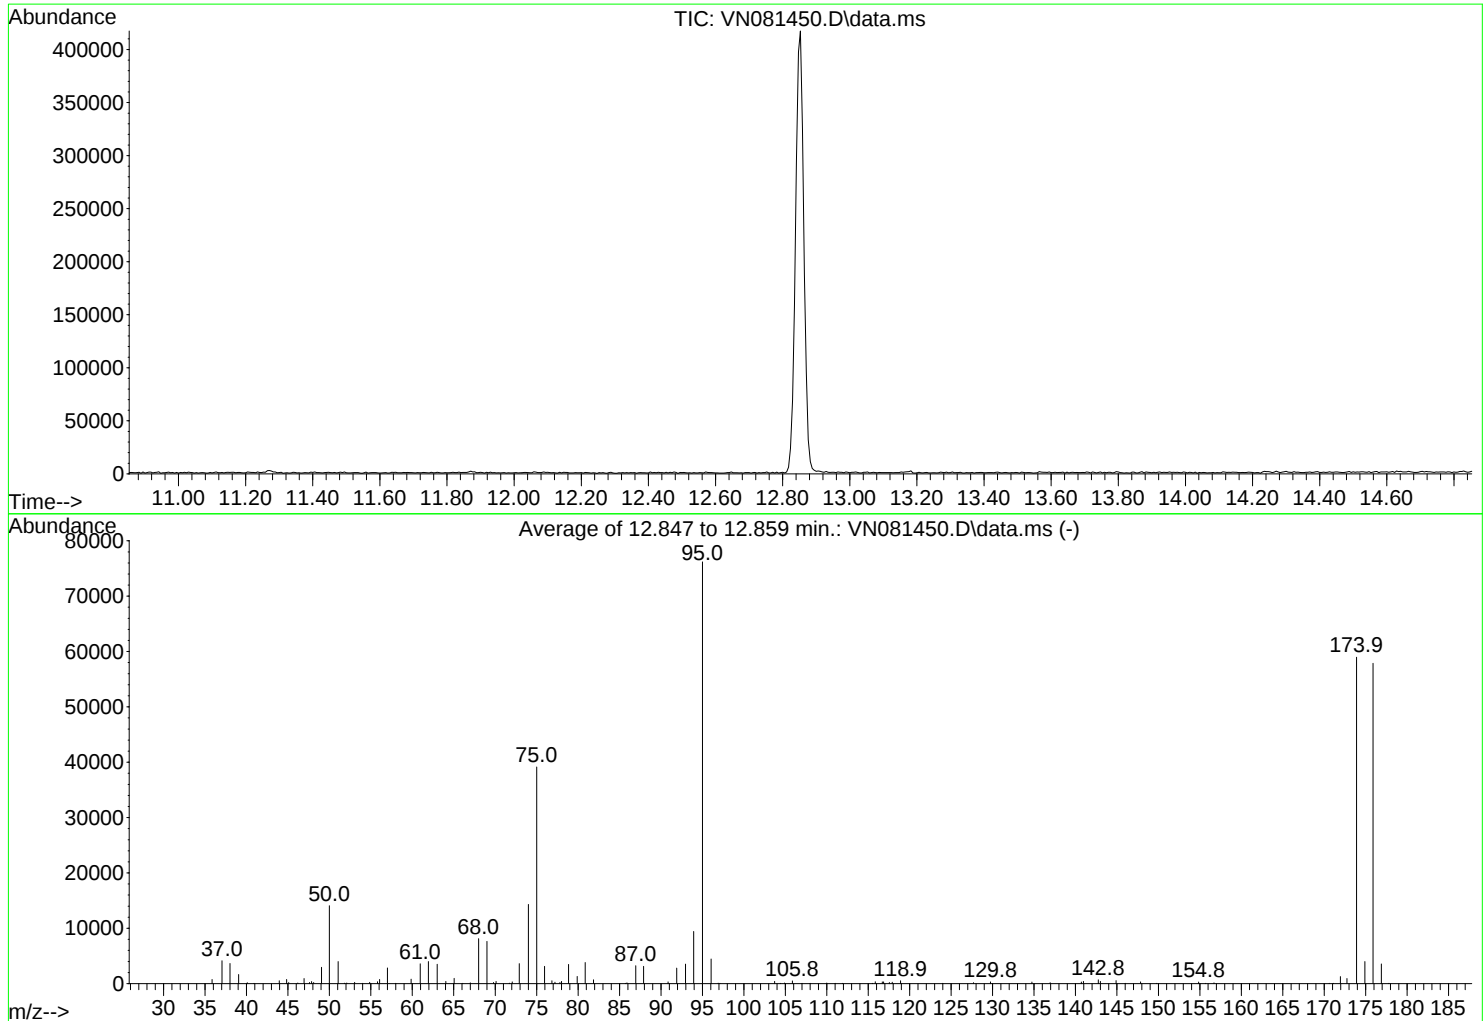

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	14078	PASS
75	95	30	60	51.4	39141	PASS
95	95	100	100	100.0	76200	PASS
96	95	5	9	5.8	4442	PASS
173	174	0.00	2	1.6	922	PASS
174	95	50	100	77.4	58963	PASS
175	174	5	9	6.8	3987	PASS
176	174	95	101	98.1	57867	PASS
177	176	5	9	6.1	3554	PASS

Average of 12.847 to 12.859 min.: VN081450.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	752	47.60	193	55.80	345	67.00	14
37.05	4133	47.85	391	56.05	744	68.00	813
38.00	3638	48.10	201	57.00	2851	69.00	763
39.05	1639	49.05	2938	58.00	59	69.80	20
40.10	175	50.00	14078	59.85	806	70.10	397
40.90	70	51.05	4007	60.95	3574	71.70	83
43.95	525	51.80	96	61.95	3985	72.05	329
44.85	763	52.10	119	63.00	3491	72.90	3606
45.10	206	53.05	243	64.05	393	74.00	14296
46.20	121	54.00	58	65.05	957	75.00	39141
46.95	923	54.85	246	66.10	52	75.95	3139

Average of 12.847 to 12.859 min.: VN081450.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.85	530	87.90	3137	104.90	110	117.55	205
77.20	267	90.85	331	105.85	500	117.90	263
77.80	218	91.90	2795	107.00	74	118.90	532
78.00	405	92.95	3539	108.00	62	124.00	58
78.85	3475	93.95	9413	110.00	123	127.70	161
79.90	1290	95.00	76200	111.00	68	129.75	308
80.85	3825	96.05	4442	111.90	61	134.75	278
81.85	707	96.90	91	115.50	67	136.95	191
85.70	54	97.10	51	115.85	339	140.70	306
85.90	156	103.70	399	116.70	325	140.95	407
86.95	3241	104.40	60	116.85	319	142.75	695

Average of 12.847 to 12.859 min.: VN081450.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
143.00	414	172.75	922				
144.90	557	173.90	58963				
146.00	53	174.90	3987				
147.85	318	175.90	57867				
149.80	53	176.90	3554				
154.85	279	177.80	51				
155.70	56						
156.70	142						
170.60	58						
171.10	69						
171.95	1271						

Instrument :

MSVOA_N

ClientSampleId :

BFB