
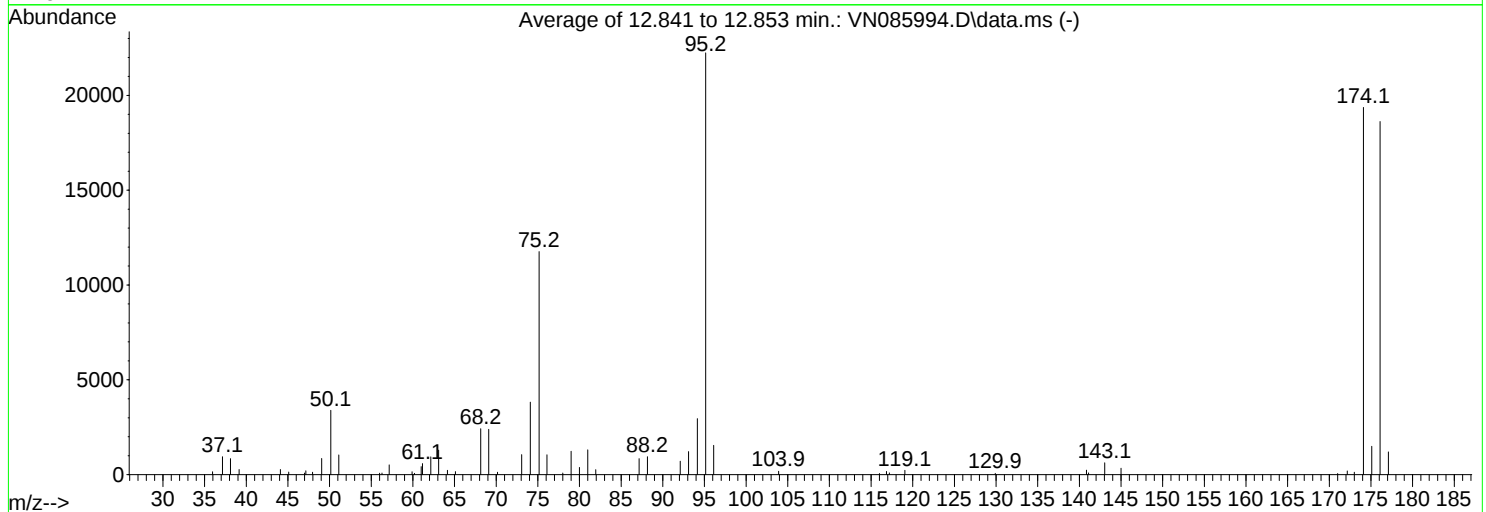


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031825\
Data File : VN085994.D
Acq On : 18 Mar 2025 08:52
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Title : SW846 8260
Last Update : Wed Mar 19 03:20:56 2025

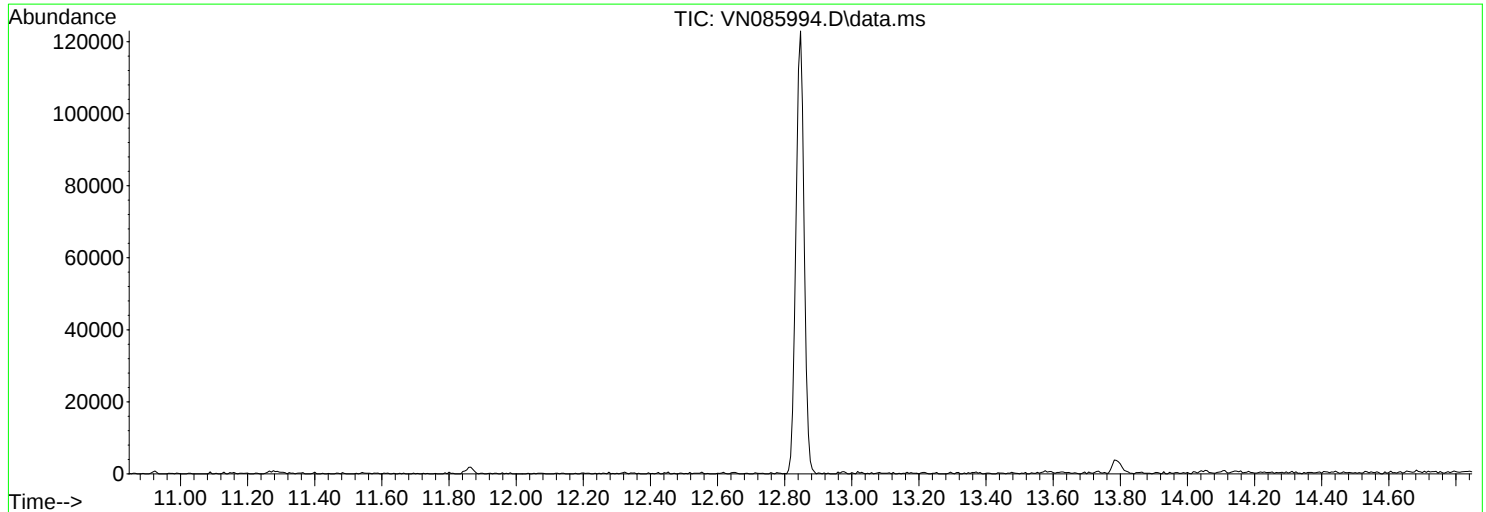

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.2	3392	PASS
75	95	30	60	52.9	11766	PASS
95	95	100	100	100.0	22245	PASS
96	95	5	9	6.9	1542	PASS
173	174	0.00	2	0.7	126	PASS
174	95	50	100	87.1	19365	PASS
175	174	5	9	7.7	1497	PASS
176	174	95	101	96.2	18624	PASS
177	176	5	9	6.4	1198	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	156	51.10	1035	65.10	157	81.00	131
37.15	946	56.00	73	68.15	2419	81.95	26
38.10	841	56.30	84	69.10	2389	87.15	84
39.15	274	57.15	518	70.15	126	88.15	94
44.10	272	59.90	150	73.05	1053	92.10	711
45.10	136	60.20	68	74.10	3825	93.10	1217
47.00	83	61.00	426	75.15	11766	94.15	2957
47.15	204	61.15	582	76.10	1047	95.15	22245
47.95	123	62.15	935	78.00	81	96.10	1542
49.05	855	63.10	1288	79.00	1234	103.90	175
50.15	3392	64.15	232	80.00	379	116.00	62

Average of 12.841 to 12.853 min.: VN085994.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.85	173	174.10	19365				
117.20	93	175.10	1497				
119.05	226	176.10	18624				
129.90	71	177.10	1198				
140.85	239						
141.10	92						
143.05	623						
145.00	335						
171.00	57						
172.15	198						
173.00	126						

Instrument :

MSVOA_N

ClientSampleId :

BFB