


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN031919\
Data File : VN054429.D
Acq On : 19 Mar 2019 9:44
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031219W.M
Title : SW846 8260
Last Update : Wed Mar 13 03:33:31 2019

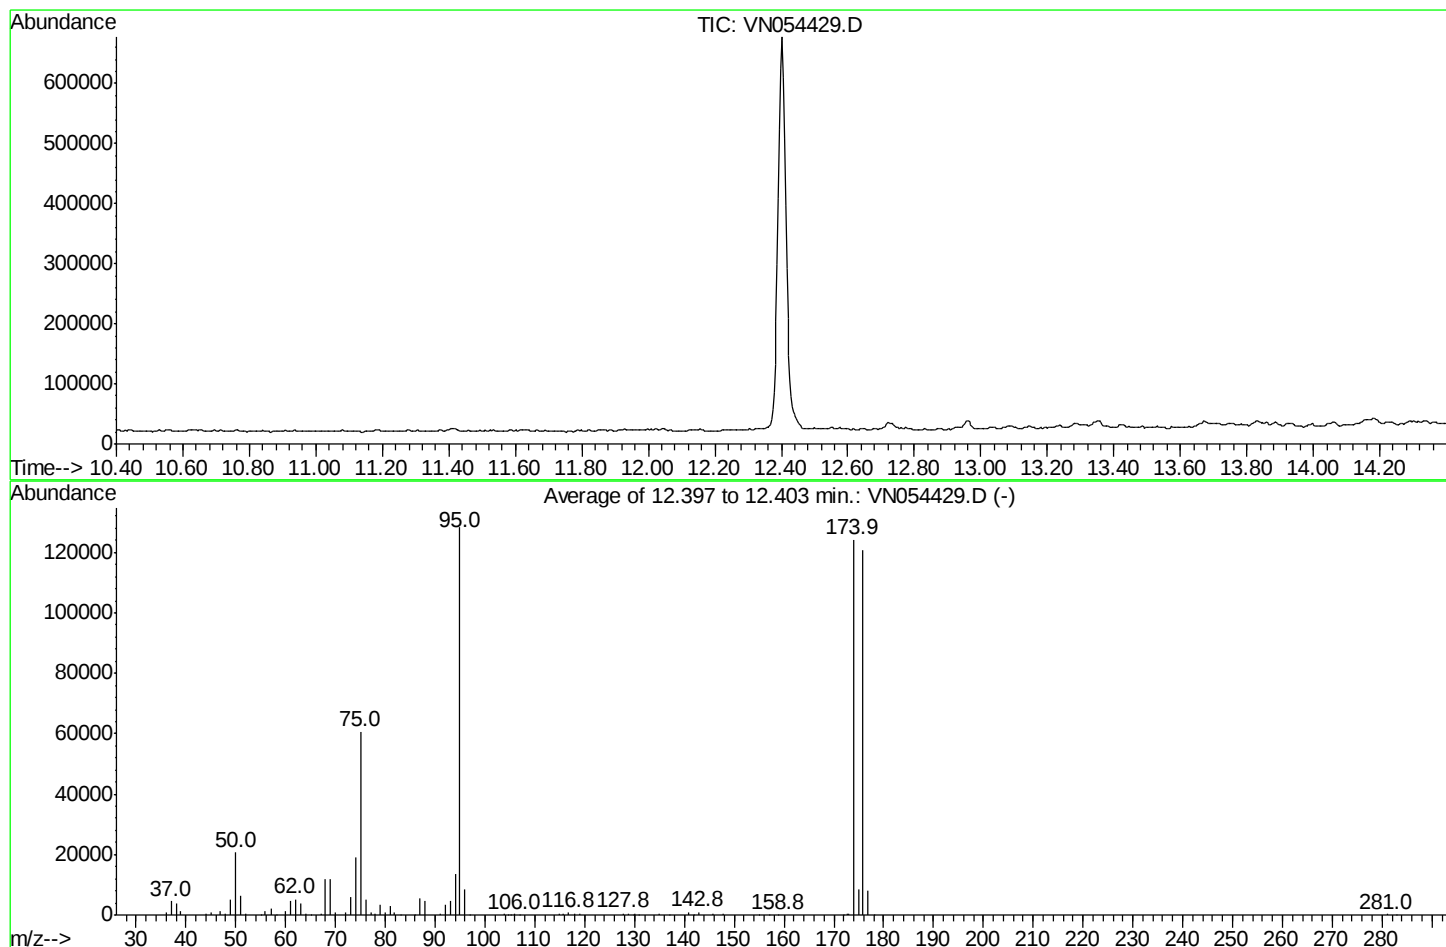

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	20586	PASS
75	95	30	60	47.3	60709	PASS
95	95	100	100	100.0	128306	PASS
96	95	5	9	6.7	8639	PASS
173	174	0.00	2	0.4	545	PASS
174	95	50	100	96.9	124296	PASS
175	174	5	9	7.0	8693	PASS
176	174	95	101	97.2	120797	PASS
177	176	5	9	6.7	8051	PASS