

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031921\
 Data File : VN066283.D
 Acq On : 19 Mar 2021 16:15
 Operator : JC/MD
 Sample : M1707-09
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 ELEVATOR-511-EL-162-157

Quant Time: Mar 20 04:59:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031621W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 17 05:05:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.584	168	287816	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.515	114	430817	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.347	117	397290	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.286	152	132688	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.946	65	200587	48.37	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	96.74%		
35) Dibromofluoromethane	7.507	113	159893	58.18	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	116.36%		
50) Toluene-d8	10.028	98	590173	55.54	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	111.08%		
62) 4-Bromofluorobenzene	12.345	95	164140	42.85	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	85.70%		
Target Compounds						Qvalue
11) Tert butyl alcohol	4.712	59	434	0.61	ug/l #	73
13) Acrolein	3.532	56	3773	Below Cal		84
16) Acetone	3.741	43	89122	44.74	ug/l	100
18) Methyl Acetate	4.237	43	4499	0.81	ug/l	96
20) Methylene Chloride	4.455	84	19988	6.41	ug/l #	82
25) 2-Butanone	6.756	43	11635	3.76	ug/l #	84
29) Tetrahydrofuran	7.128	42	803	0.38	ug/l #	70
31) Cyclohexane	7.590	56	4370	0.70	ug/l #	1
36) 1,1-Dichloropropene	7.584	75	18012	4.13	ug/l #	49
37) Ethyl Acetate	6.756	43	11635	1.87	ug/l #	75
38) Carbon Tetrachloride	7.582	117	24197	6.19	ug/l #	18
43) Isopropyl Acetate	8.094	43	28694	2.98	ug/l	99
45) 1,2-Dichloropropane	9.202	63	2327	0.61	ug/l #	44
48) Methyl methacrylate	9.113	41	7543	1.65	ug/l #	21
49) 1,4-Dioxane	9.207	88	166	3.35	ug/l #	1
51) 4-Methyl-2-Pentanone	9.923	43	10716	1.84	ug/l	99
54) cis-1,3-Dichloropropene	9.845	75	39499	6.98	ug/l #	55
56) Ethyl methacrylate	10.374	69	123	2.18	ug/l #	17
57) 1,3-Dichloropropane	10.706	76	25659	4.57	ug/l #	43
59) 2-Hexanone	10.706	43	378678	84.01	ug/l #	58
65) Chlorobenzene	11.377	112	2516	0.32	ug/l	97
70) Styrene	11.905	104	223	2.17	ug/l #	51
74) N-amyl acetate	12.104	43	376	2.23	ug/l #	49
76) 1,2,3-Trichloropropane	12.345	75	76568	22.35	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.345	75	76568	66.87	ug/l #	11
82) 4-Chlorotoluene	12.726	91	912	0.60	ug/l #	43
88) 1,4-Dichlorobenzene	13.308	146	1113	0.26	ug/l #	1
89) n-Butylbenzene	13.554	91	1219	2.39	ug/l	93
92) 1,2-Dibromo-3-Chloropr...	14.225	75	460	1.46	ug/l #	8
93) 1,2,4-Trichlorobenzene	14.853	180	1693	0.64	ug/l #	77
94) Hexachlorobutadiene	14.949	225	485	0.38	ug/l	83
95) Naphthalene	15.070	128	8973	1.15	ug/l #	93
96) 1,2,3-Trichlorobenzene	15.244	180	1208	0.46	ug/l #	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031921\
Data File : VN066283.D
Acq On : 19 Mar 2021 16:15
Operator : JC/MD
Sample : M1707-09
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157

Quant Time: Mar 20 04:59:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031621W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 17 05:05:15 2021
Response via : Initial Calibration




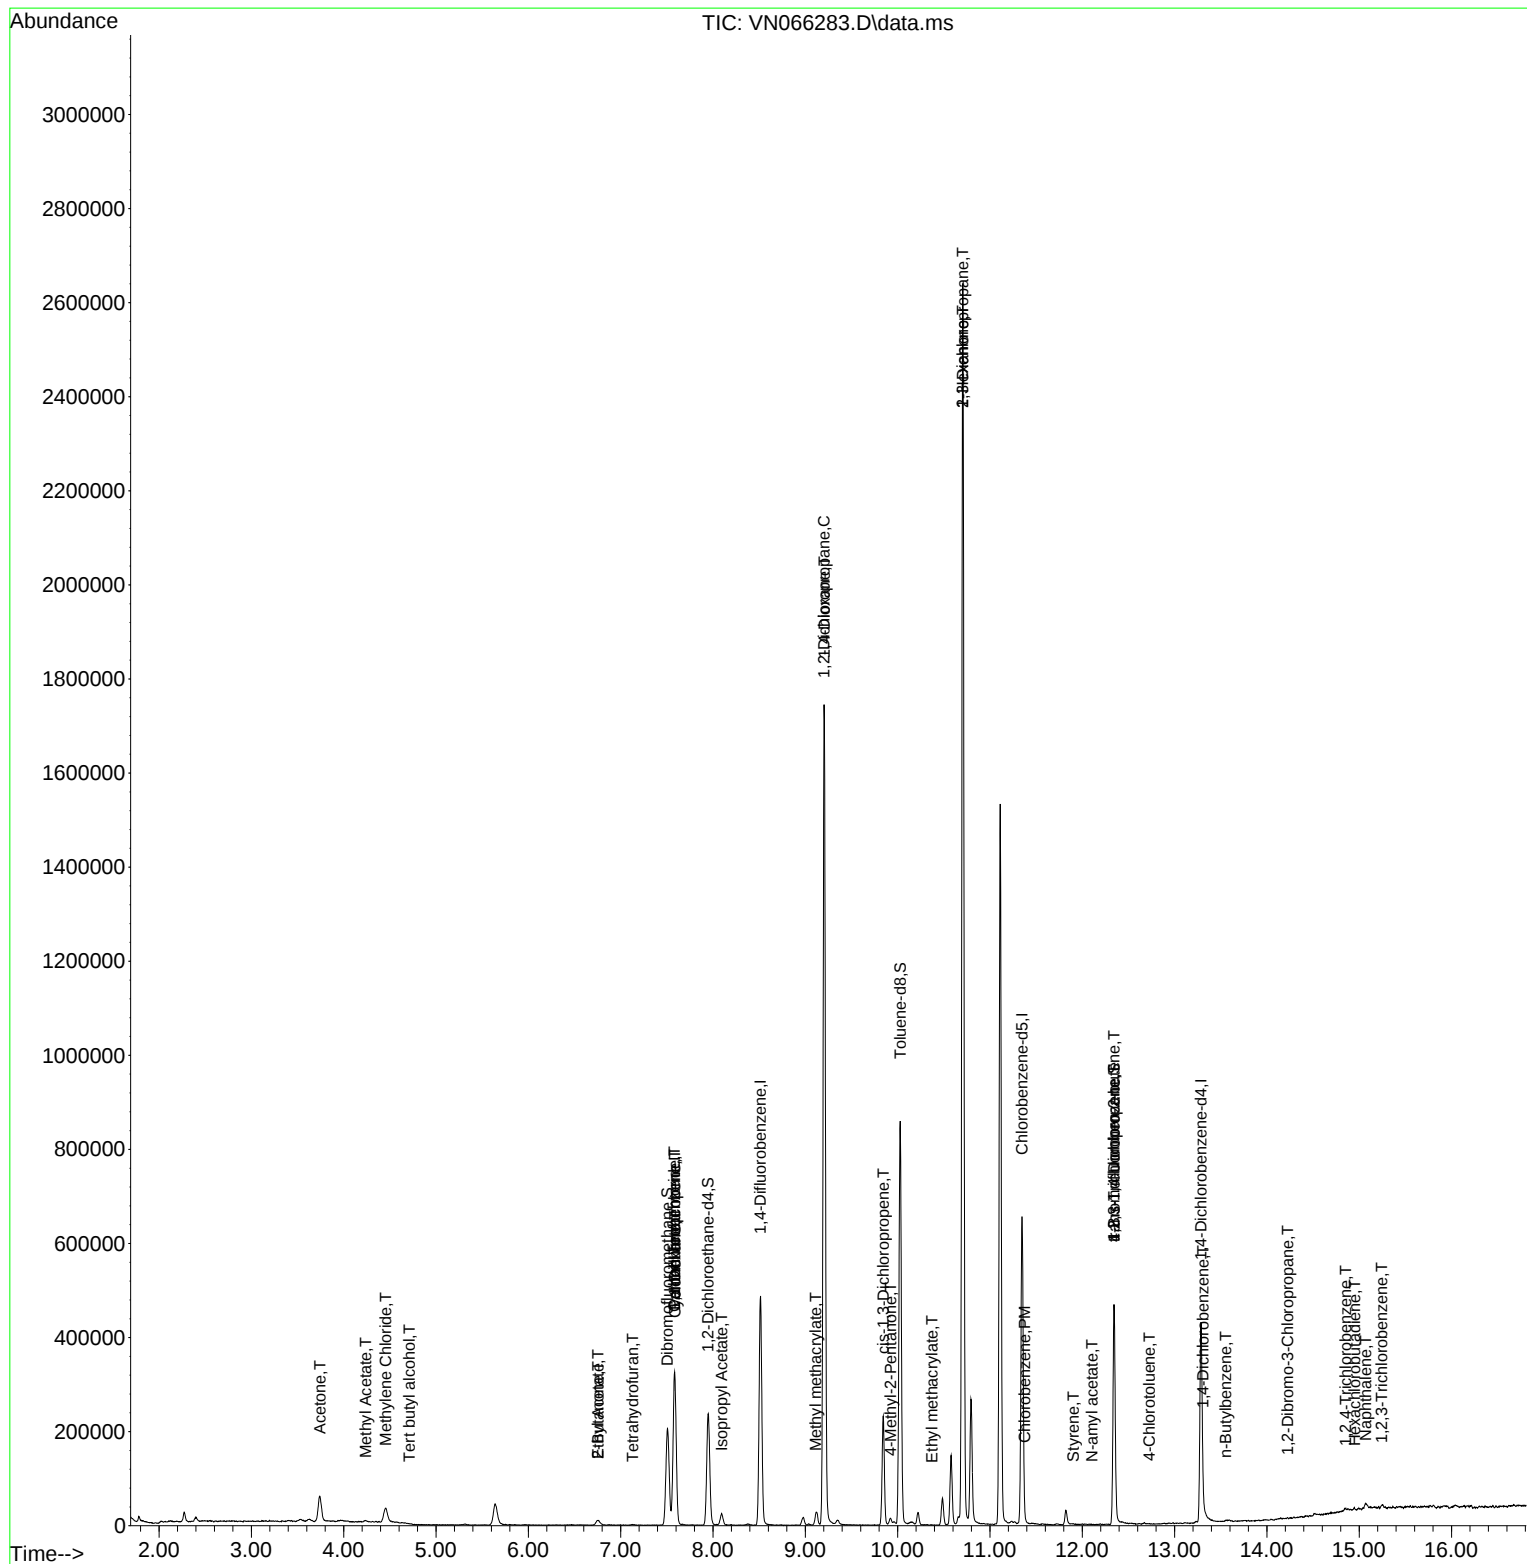




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.584 min Scan# 2198
Delta R.T. -0.001 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15




Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157


Tgt Ion:168 Resp: 287816
Ion Ratio Lower Upper
168 100
99 48.7 45.4 68.0



#11
Tert butyl alcohol
Concen: 0.61 ug/l
RT: 4.712 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Tgt Ion: 59 Resp: 434
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#


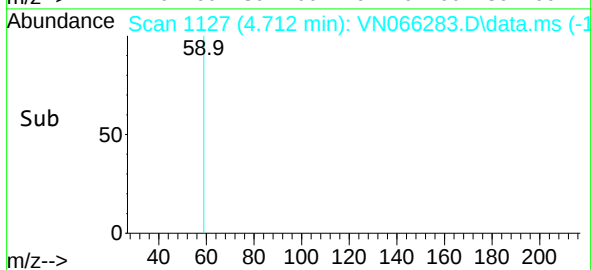






#13
Acrolein
Concen: Below Cal
RT: 3.532 min Scan# 687
Delta R.T. -0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15




Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157


Tgt Ion: 56 Resp: 3773
Ion Ratio Lower Upper
56 100
55 85.6 58.0 87.0

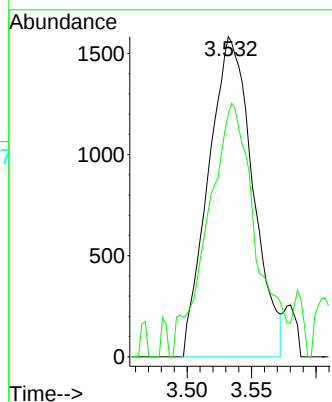

#16
Acetone
Concen: 44.74 ug/l
RT: 3.741 min Scan# 765
Delta R.T. 0.002 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15


Tgt Ion: 43 Resp: 89122
Ion Ratio Lower Upper
43 100
58 27.9 22.3 33.5

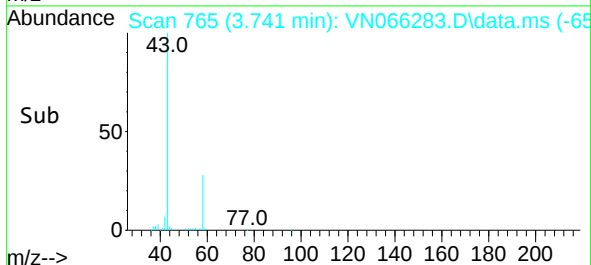






#18
Methyl Acetate
Concen: 0.81 ug/l
RT: 4.237 min Scan# 950
Delta R.T. 0.002 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157







Tgt Ion: 43 Resp: 4499
Ion Ratio Lower Upper
43 100
74 15.8 14.2 21.2

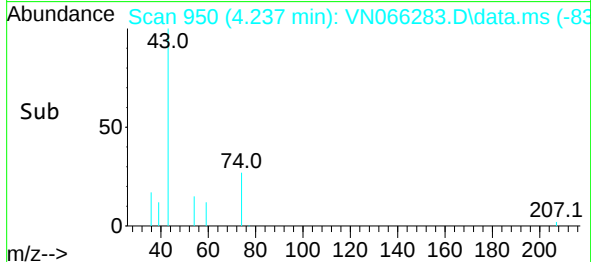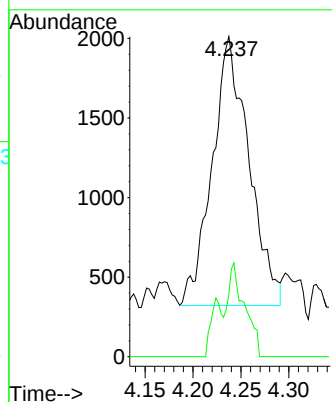

#20
Methylene Chloride
Concen: 6.41 ug/l
RT: 4.455 min Scan# 1031
Delta R.T. -0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15


Tgt Ion: 84 Resp: 19988
Ion Ratio Lower Upper
84 100
49 129.1 130.0 195.0#
51 37.6 39.1 58.7#
86 63.0 50.9 76.3

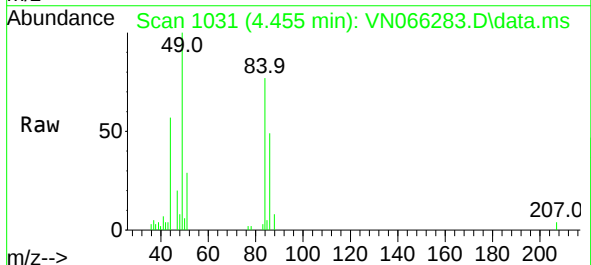



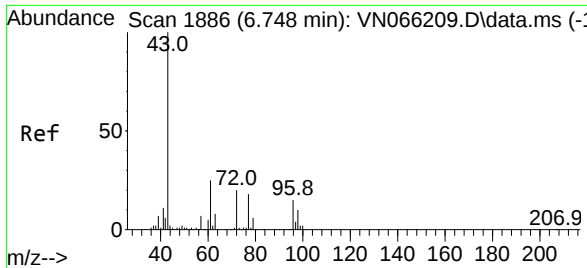


#25
2-Butanone
Concen: 3.76 ug/l
RT: 6.756 min Scan# 1889
Delta R.T. 0.008 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157



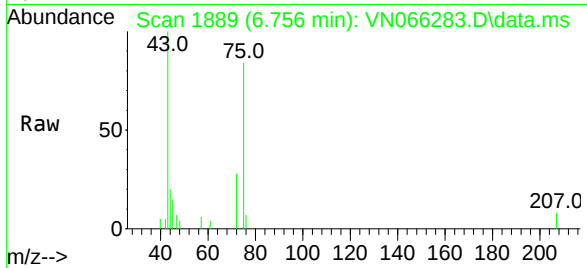



Tgt Ion: 43 Resp: 11635
Ion Ratio Lower Upper
43 100
72 27.7 16.2 24.2#

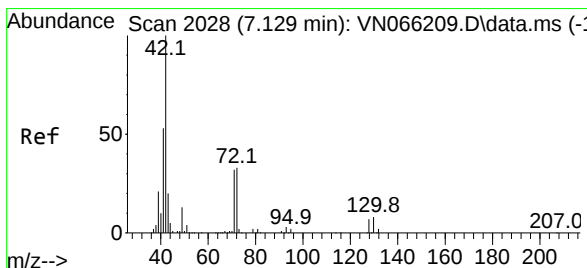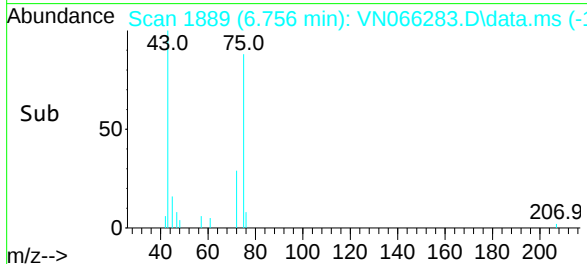

#29
Tetrahydrofuran
Concen: 0.38 ug/l
RT: 7.128 min Scan# 2028
Delta R.T. -0.001 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15


Tgt Ion: 42 Resp: 803
Ion Ratio Lower Upper
42 100
72 15.1 26.2 39.4#
71 16.3 25.4 38.2#

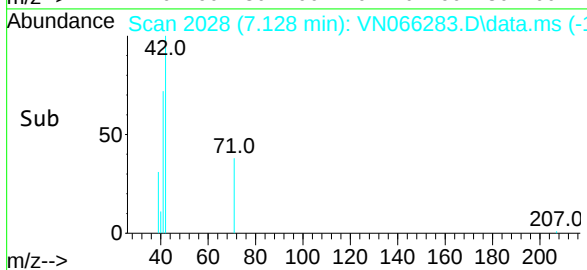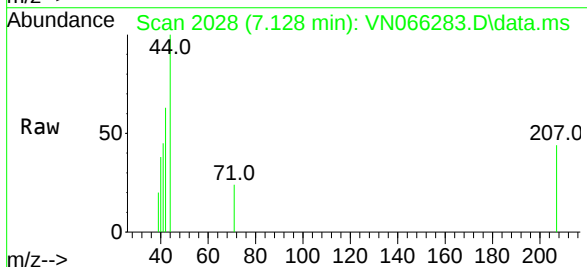






#31
Cyclohexane
Concen: 0.70 ug/l
RT: 7.590 min Scan# 2200
Delta R.T. 0.019 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15


Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157





Tgt Ion: 56 Resp: 4370
Ion Ratio Lower Upper
56 100
69 192.5 23.4 35.0#
84 146.4 57.8 86.6#

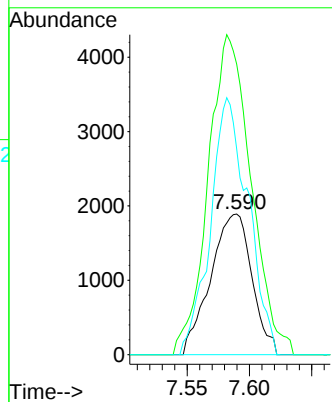


#33
1,2-Dichloroethane-d4
Concen: 48.37 ug/l
RT: 7.946 min Scan# 2333
Delta R.T. -0.003 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

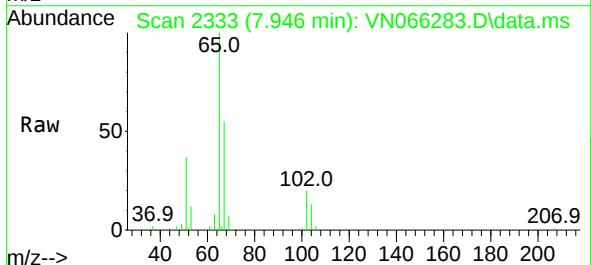


Tgt Ion: 65 Resp: 200587
Ion Ratio Lower Upper
65 100
67 54.0 0.0 107.2








#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.515 min Scan# 2545
Delta R.T. 0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15


Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157





Tgt Ion	Ratio	Lower	Upper
114	100		
63	19.5	0.0	49.2
88	16.1	0.0	33.8

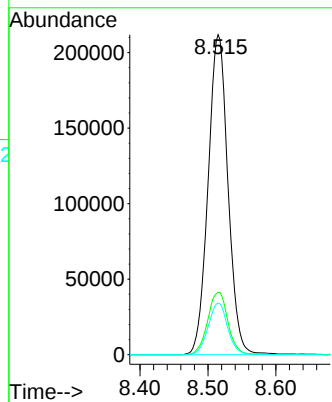


#35
Dibromofluoromethane
Concen: 58.18 ug/l
RT: 7.507 min Scan# 2169
Delta R.T. -0.002 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

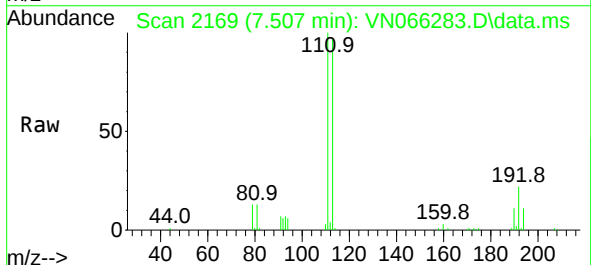


Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.7	84.0	126.0
192	22.8	16.7	25.1








#36
1,1-Dichloropropene
Concen: 4.13 ug/l
RT: 7.584 min Scan# 2198
Delta R.T. -0.127 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157







Tgt Ion: 75 Resp: 18012
Ion Ratio Lower Upper
75 100
110 6.4 16.0 48.0#
77 0.0 24.9 37.3#

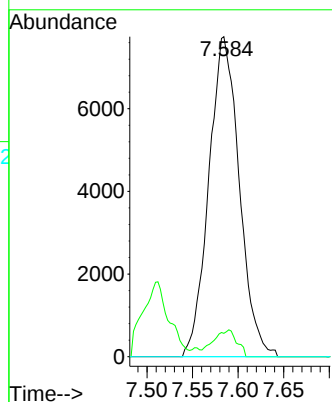

#37
Ethyl Acetate
Concen: 1.87 ug/l
RT: 6.756 min Scan# 1889
Delta R.T. -0.086 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15


Tgt Ion: 43 Resp: 11635
Ion Ratio Lower Upper
43 100
61 1.3 9.2 13.8#
70 0.0 6.1 9.1#

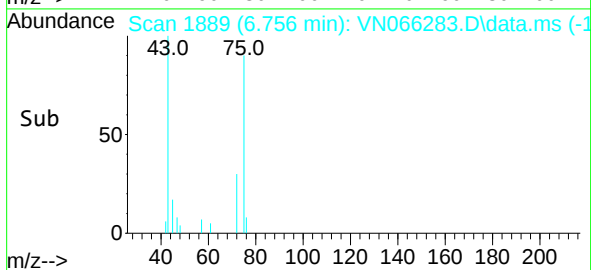






#38
Carbon Tetrachloride
Concen: 6.19 ug/l
RT: 7.582 min Scan# 2197
Delta R.T. -0.110 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15


Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157





Tgt Ion: 117 Resp: 24197
Ion Ratio Lower Upper
117 100
119 5.7 74.6 111.8#
121 0.0 23.9 35.9#

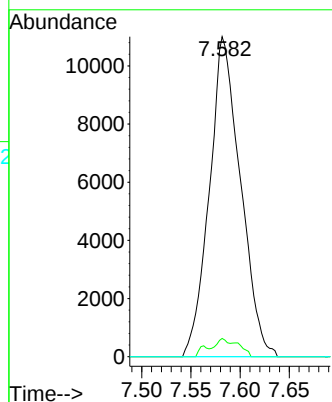


#43
Isopropyl Acetate
Concen: 2.98 ug/l
RT: 8.094 min Scan# 2388
Delta R.T. -0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15



Tgt Ion: 43 Resp: 28694
Ion Ratio Lower Upper
43 100
61 17.5 14.0 21.0
87 11.0 7.9 11.9









#45
1,2-Dichloropropane
Concen: 0.61 ug/l
RT: 9.202 min Scan# 2801
Delta R.T. 0.153 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15




Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157


Tgt Ion: 63 Resp: 2327
Ion Ratio Lower Upper
63 100
65 0.0 24.6 37.0#

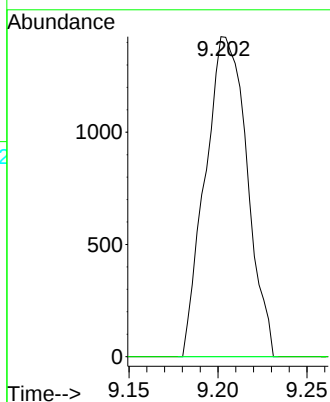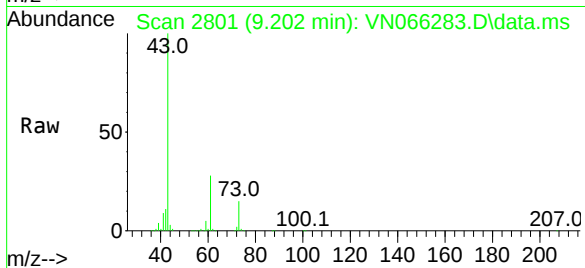

#48
Methyl methacrylate
Concen: 1.65 ug/l
RT: 9.113 min Scan# 2768
Delta R.T. -0.022 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15


Tgt Ion: 41 Resp: 7543
Ion Ratio Lower Upper
41 100
69 0.0 54.7 82.1#
39 0.0 40.2 60.2#

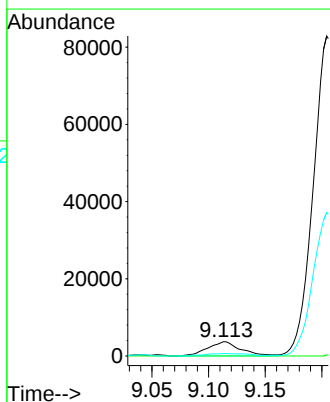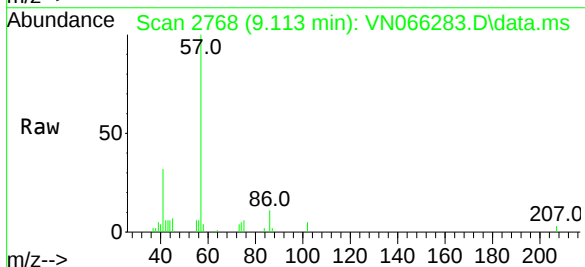






#49
1,4-Dioxane
Concen: 3.35 ug/l
RT: 9.207 min Scan# 2803
Delta R.T. 0.070 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157







Tgt Ion: 88 Resp: 166
Ion Ratio Lower Upper
88 100
43 994907.8 34.4 51.6#
58 5016.3 67.3 100.9#



#50
Toluene-d8
Concen: 55.54 ug/l
RT: 10.028 min Scan# 3109
Delta R.T. -0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Tgt Ion: 98 Resp: 590173
Ion Ratio Lower Upper
98 100
100 65.6 51.0 76.6


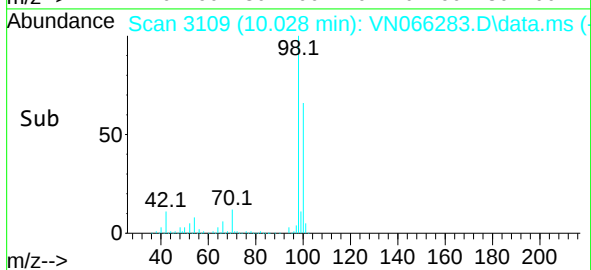






#51
4-Methyl-2-Pentanone
Concen: 1.84 ug/l
RT: 9.923 min Scan# 3070
Delta R.T. 0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15




Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157


Tgt Ion: 43 Resp: 10716
Ion Ratio Lower Upper
43 100
58 34.8 27.5 41.3

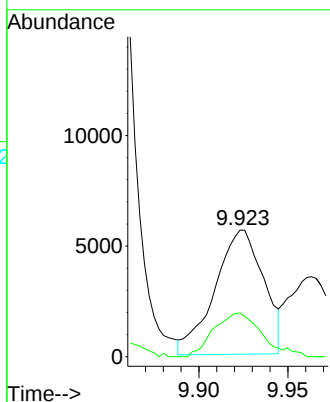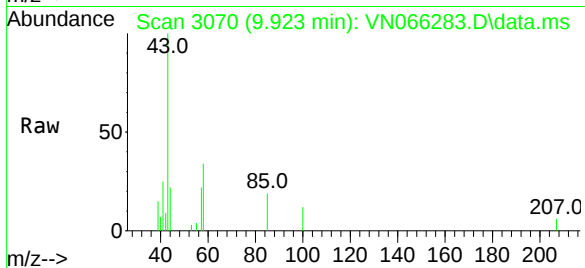

#54
cis-1,3-Dichloropropene
Concen: 6.98 ug/l
RT: 9.845 min Scan# 3041
Delta R.T. 0.069 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Tgt Ion: 75 Resp: 39499
Ion Ratio Lower Upper
75 100
77 1.0 25.0 37.4#
39 28.3 46.2 69.2#



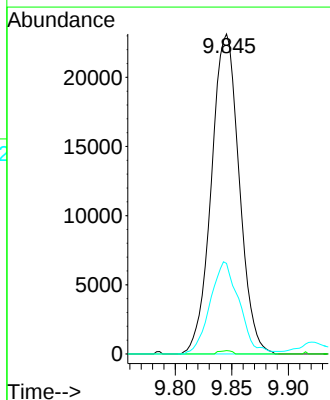
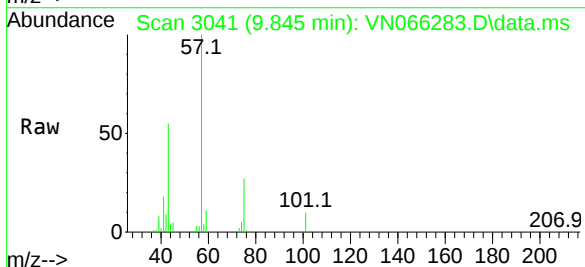




#56
Ethyl methacrylate
Concen: 2.18 ug/l
RT: 10.374 min Scan# 3238
Delta R.T. 0.003 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15




Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157


Tgt Ion: 69 Resp: 123
Ion Ratio Lower Upper
69 100
41 0.0 66.2 99.4#
39 0.0 31.5 47.3#



#57
1,3-Dichloropropane
Concen: 4.57 ug/l
RT: 10.706 min Scan# 3362
Delta R.T. 0.059 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Tgt Ion: 76 Resp: 25659
Ion Ratio Lower Upper
76 100
78 0.0 25.4 38.2#


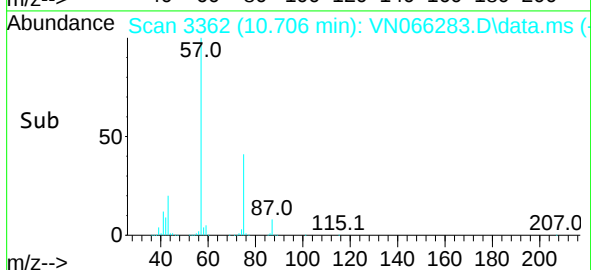

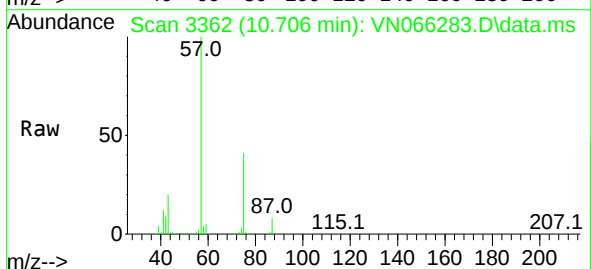


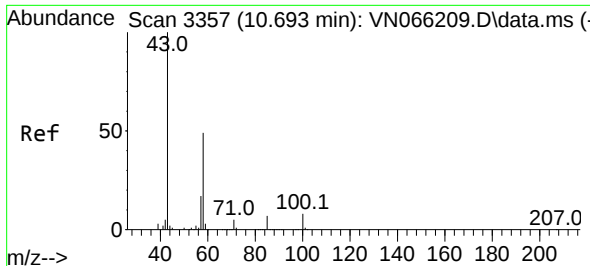

#59
2-Hexanone
Concen: 84.01 ug/l
RT: 10.706 min Scan# 3362
Delta R.T. 0.013 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15




Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157


Tgt Ion: 43 Resp: 378678
Ion Ratio Lower Upper
43 100
58 19.5 23.8 71.5#

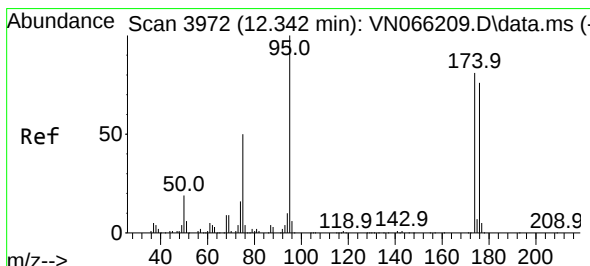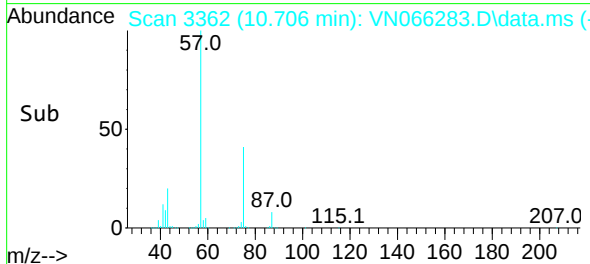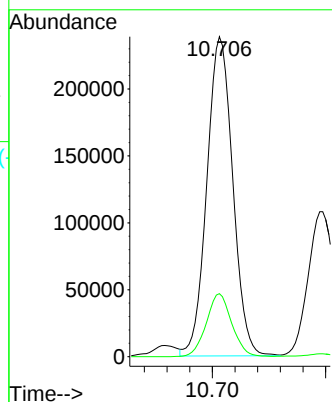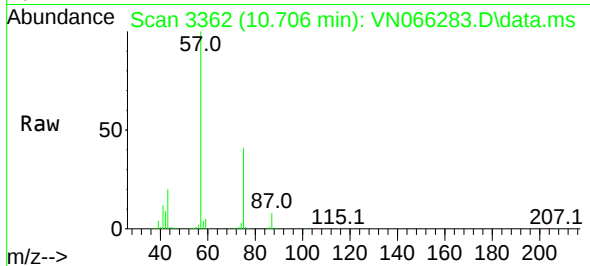

#62
4-Bromofluorobenzene
Concen: 42.85 ug/l
RT: 12.345 min Scan# 3973
Delta R.T. 0.003 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Tgt Ion: 95 Resp: 164140
Ion Ratio Lower Upper
95 100
174 91.6 0.0 162.4
176 86.7 0.0 156.2


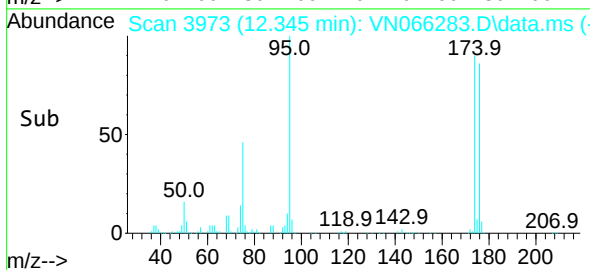

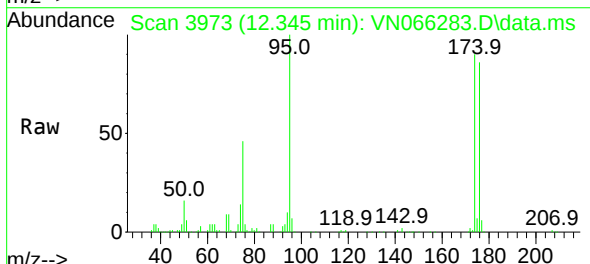


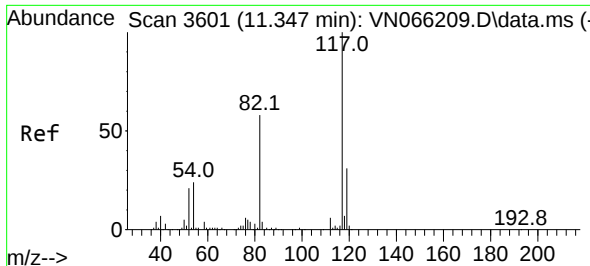

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.347 min Scan# 3601
Delta R.T. 0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15




Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157


Tgt Ion:117 Resp: 397290
Ion Ratio Lower Upper
117 100
82 52.8 49.0 73.6
119 31.7 25.7 38.5

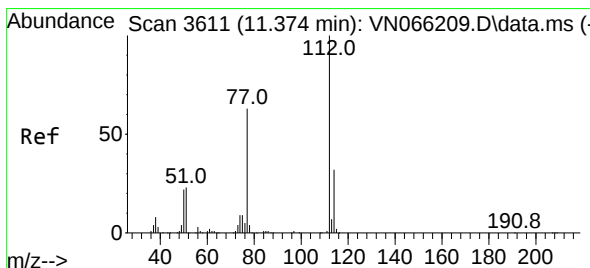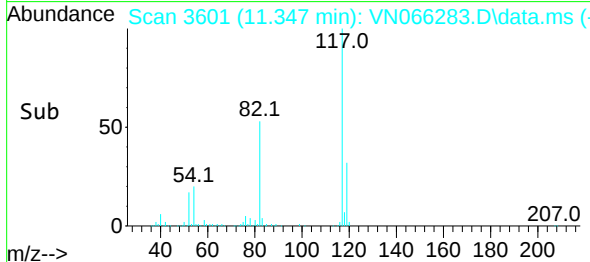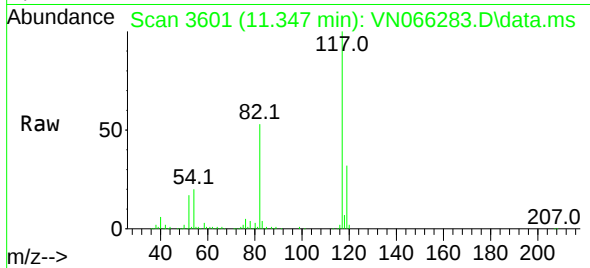

#65
Chlorobenzene
Concen: 0.32 ug/l
RT: 11.377 min Scan# 3612
Delta R.T. 0.003 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Tgt Ion:112 Resp: 2516
Ion Ratio Lower Upper
112 100
114 33.2 25.4 38.0


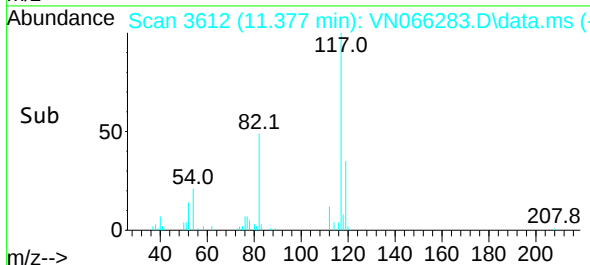

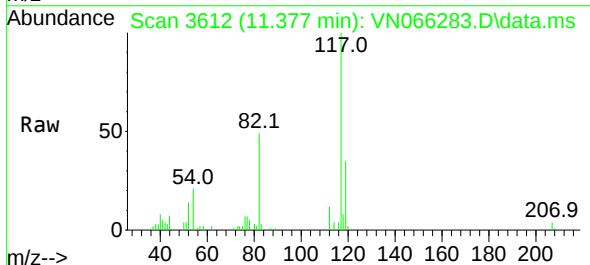


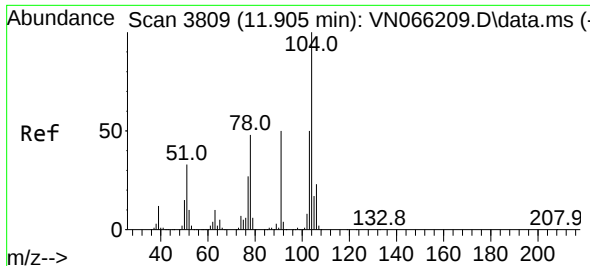

#70
Styrene
Concen: 2.17 ug/l
RT: 11.905 min Scan# 3809
Delta R.T. 0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15




Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157


Tgt Ion:104 Resp: 223
Ion Ratio Lower Upper
104 100
78 0.0 43.8 65.6#
103 38.1 43.7 65.5#

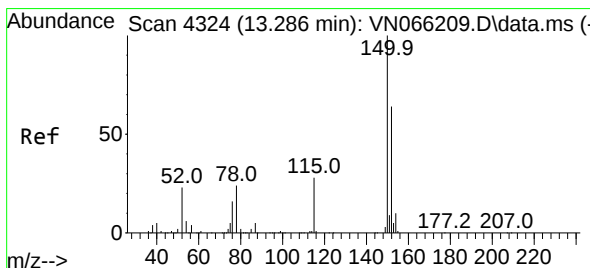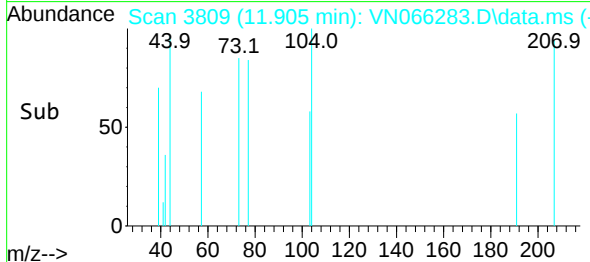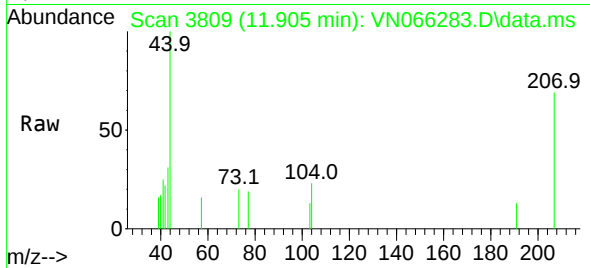

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.286 min Scan# 4324
Delta R.T. 0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15


Tgt Ion:152 Resp: 132688
Ion Ratio Lower Upper
152 100
115 57.3 29.4 88.3
150 156.5 0.0 352.2

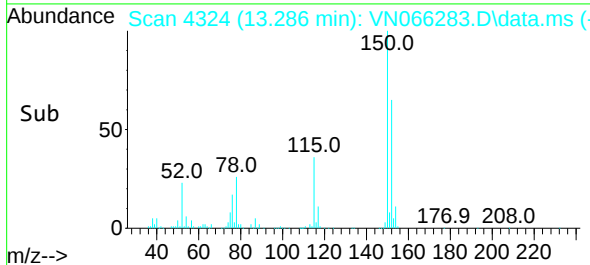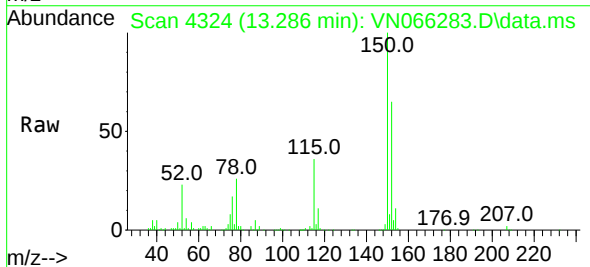






#74
N-amy1 acetate
Concen: 2.23 ug/l
RT: 12.104 min Scan# 3883
Delta R.T. 0.088 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157



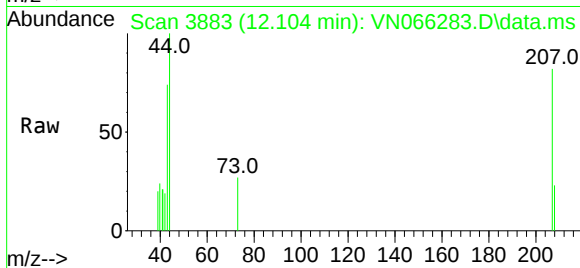



Tgt Ion: 43	Resp: 376
Ion Ratio	Lower Upper
43 100	
70 0.0	26.2 39.4#
55 0.0	17.2 25.8#
61 0.0	17.0 25.4#



#76
1,2,3-Trichloropropane
Concen: 22.35 ug/l
RT: 12.345 min Scan# 3973
Delta R.T. -0.153 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Tgt Ion: 75	Resp: 76568
Ion Ratio	Lower Upper
75 100	
77 1.3	0.0 0.0#


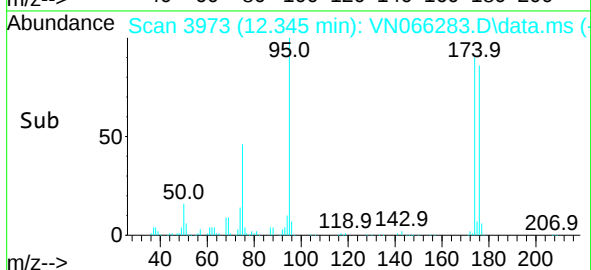

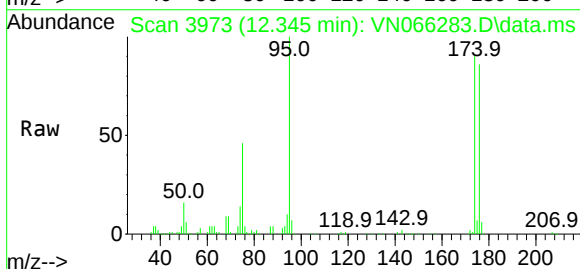




#81
trans-1,4-Dichloro-2-butene
Concen: 66.87 ug/l
RT: 12.345 min Scan# 3973
Delta R.T. 0.102 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15




Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157


Tgt Ion: 75 Resp: 76568
Ion Ratio Lower Upper
75 100
53 0.2 77.8 116.6#
89 0.0 33.7 50.5#

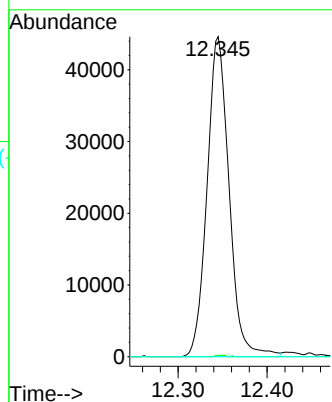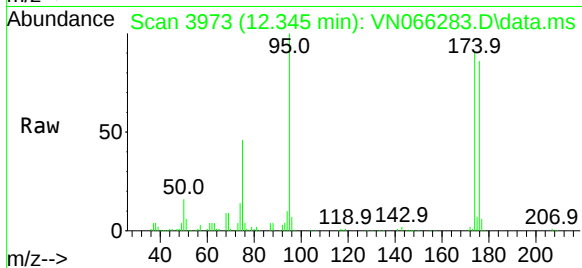

#82
4-Chlorotoluene
Concen: 0.60 ug/l
RT: 12.726 min Scan# 4115
Delta R.T. 0.011 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Tgt Ion: 91 Resp: 912
Ion Ratio Lower Upper
91 100
126 0.0 15.7 47.1#




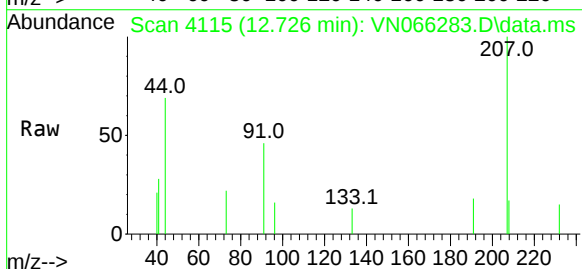




#88
1,4-Dichlorobenzene
Concen: 0.26 ug/l
RT: 13.308 min Scan# 4332
Delta R.T. 0.003 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15




Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157


Tgt Ion:146 Resp: 1113
Ion Ratio Lower Upper
146 100
111 157.6 19.9 59.7#
148 139.7 33.2 99.6#

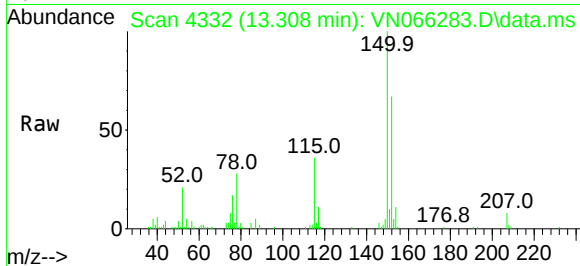

#89
n-Butylbenzene
Concen: 2.39 ug/l
RT: 13.554 min Scan# 4424
Delta R.T. -0.003 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Tgt Ion: 91 Resp: 1219
Ion Ratio Lower Upper
91 100
92 48.0 25.7 77.0
134 29.9 11.8 35.4




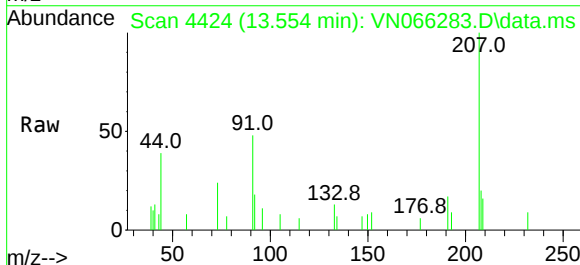




#92
 1,2-Dibromo-3-Chloropropane
 Concen: 1.46 ug/l
 RT: 14.225 min Scan# 4674
 Delta R.T. 0.013 min
 Lab File: VN066283.D
 Acq: 19 Mar 2021 16:15




Instrument :
 MSVOA_N
 ClientSampleId :
 ELEVATOR-511-EL-162-157


Tgt Ion: 75 Resp: 460
 Ion Ratio Lower Upper
 75 100
 155 0.0 36.5 109.7#
 157 0.0 46.3 138.8#

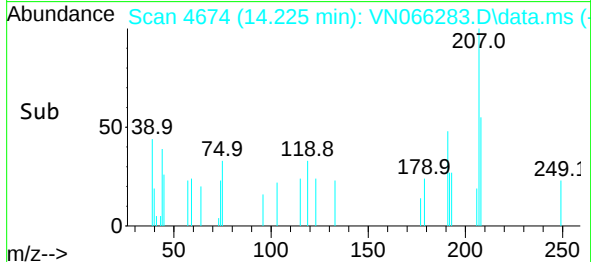

#93
 1,2,4-Trichlorobenzene
 Concen: 0.64 ug/l
 RT: 14.853 min Scan# 4908
 Delta R.T. 0.003 min
 Lab File: VN066283.D
 Acq: 19 Mar 2021 16:15

Tgt Ion:180 Resp: 1693
 Ion Ratio Lower Upper
 180 100
 182 113.9 47.4 142.2
 145 46.7 14.1 42.3#




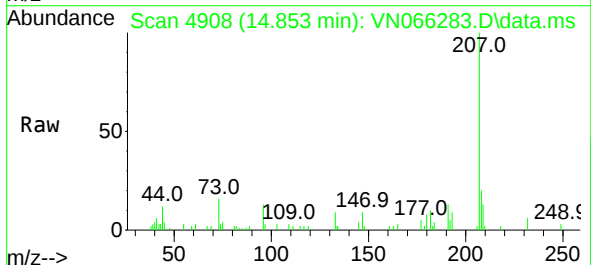


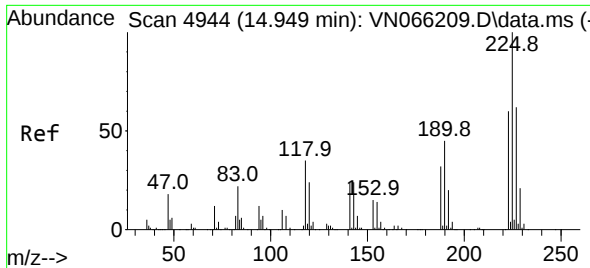

#94
Hexachlorobutadiene
Concen: 0.38 ug/l
RT: 14.949 min Scan# 4944
Delta R.T. 0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15




Instrument :
MSVOA_N
ClientSampleId :
ELEVATOR-511-EL-162-157


Tgt Ion:	225	Resp:	485
Ion	Ratio	Lower	Upper
225	100		
223	45.2	31.3	93.8
227	55.1	31.9	95.7

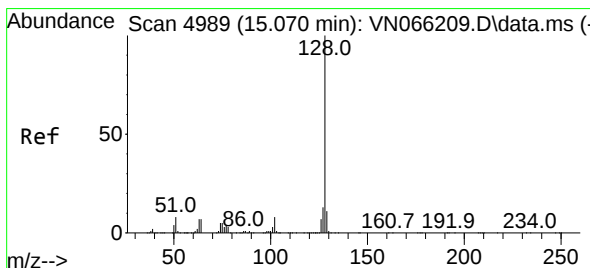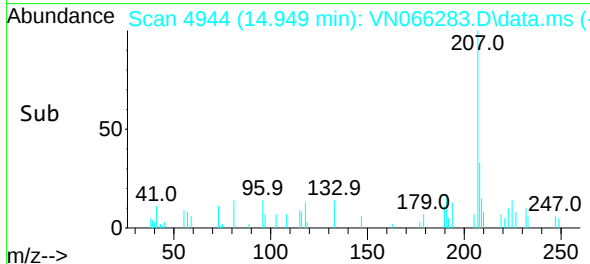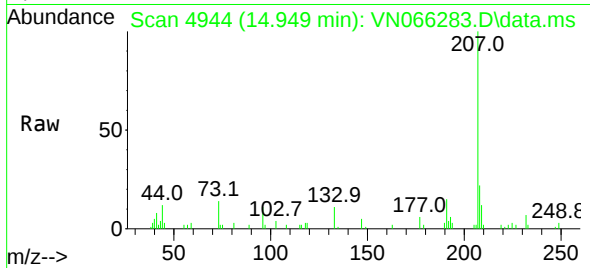

#95
Naphthalene
Concen: 1.15 ug/l
RT: 15.070 min Scan# 4989
Delta R.T. -0.000 min
Lab File: VN066283.D
Acq: 19 Mar 2021 16:15

Tgt Ion:	128	Resp:	8973
Ion	Ratio	Lower	Upper
128	100		
127	8.9	10.3	15.5#
129	9.6	8.4	12.6

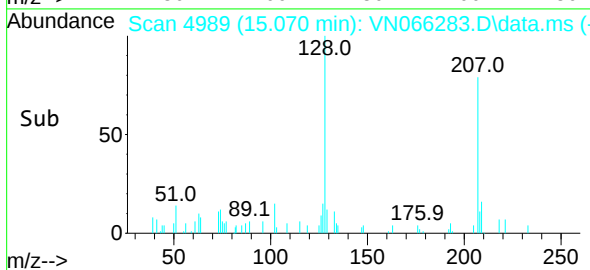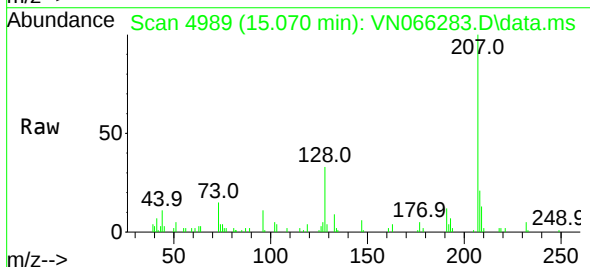



#96
 1,2,3-Trichlorobenzene
 Concen: 0.46 ug/l
 RT: 15.244 min Scan# 5054
 Delta R.T. -0.003 min
 Lab File: VN066283.D
 Acq: 19 Mar 2021 16:15

Instrument :
 MSVOA_N
 ClientSampleId :
 ELEVATOR-511-EL-162-157

Tgt Ion:180 Resp: 1208
 Ion Ratio Lower Upper
 180 100
 182 169.5 47.9 143.8#
 145 57.9 15.6 46.8#

