


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031921\
 Data File : VN066271.D
 Acq On : 19 Mar 2021 10:17
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031621W.M
 Title : SW846 8260
 Last Update : Wed Mar 17 05:05:15 2021

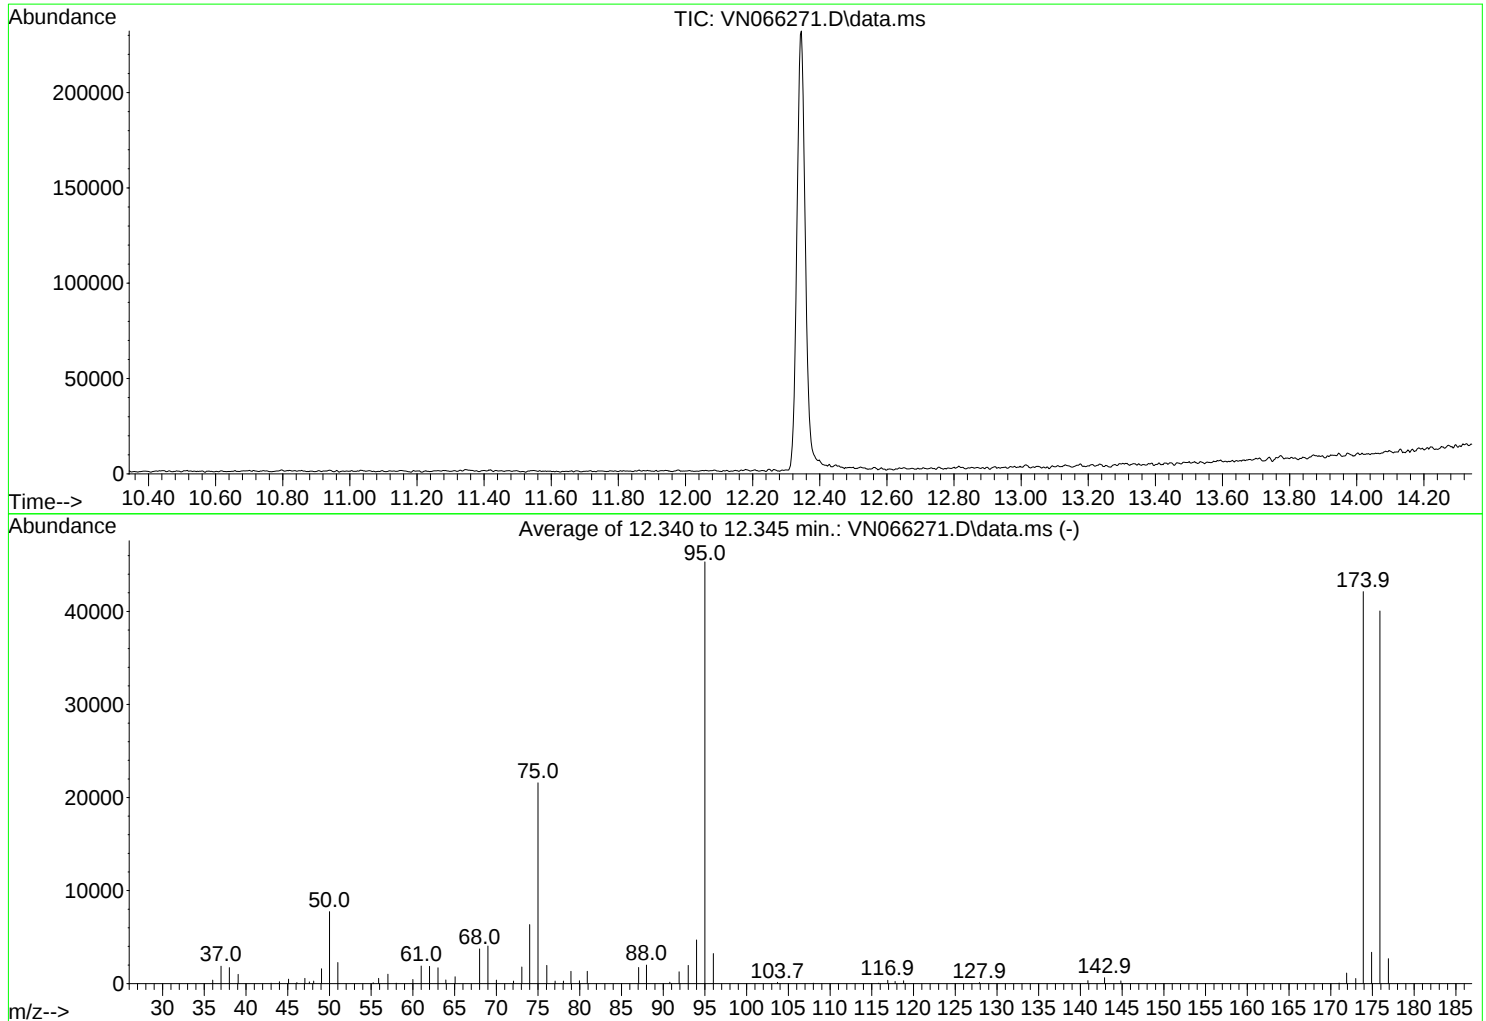

AutoFind: Scans 3971, 3972, 3973; Background Corrected with Scan 3956

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	7743	PASS
75	95	30	60	47.6	21576	PASS
95	95	100	100	100.0	45328	PASS
96	95	5	9	7.1	3228	PASS
173	174	0.00	2	1.3	549	PASS
174	95	50	100	92.9	42125	PASS
175	174	5	9	8.0	3364	PASS
176	174	95	101	95.1	40053	PASS
177	176	5	9	6.7	2688	PASS