

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031922\
 Data File : VN071393.D
 Acq On : 19 Mar 2022 13:18
 Operator : JC\MD
 Sample : N1974-13
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 B-3

Quant Time: Mar 21 05:50:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.087	168	759624	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1261114	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1176127	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	411484	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	486894	46.768	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	93.540%		
35) Dibromofluoromethane	8.022	113	367735	46.209	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	92.420%		
50) Toluene-d8	10.439	98	1572045	49.063	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	98.120%		
62) 4-Bromofluorobenzene	12.727	95	579277	53.389	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	106.780%		
Target Compounds						Qvalue
3) Chloromethane	2.299	50	5133	0.425	ug/l	93
5) Bromomethane	2.834	94	287	Below Cal	#	3
11) Tert butyl alcohol	5.363	59	420	0.205	ug/l #	71
13) Acrolein	4.040	56	648	0.299	ug/l #	14
16) Acetone	4.299	43	7761	1.532	ug/l	98
18) Methyl Acetate	4.863	43	8880	1.117	ug/l #	87
20) Methylene Chloride	5.093	84	340	0.418	ug/l #	8
25) 2-Butanone	7.340	43	2614	0.320	ug/l #	82
31) Cyclohexane	8.087	56	16881	1.015	ug/l #	1
36) 1,1-Dichloropropene	8.087	75	60477	4.743	ug/l #	49
38) Carbon Tetrachloride	8.081	117	74370	6.030	ug/l #	17
39) Methylcyclohexane	9.451	83	3642	0.243	ug/l	92
40) Benzene	8.457	78	180866	4.708	ug/l	96
43) Isopropyl Acetate	8.586	43	10811	0.412	ug/l #	55
49) 1,4-Dioxane	9.575	88	82	0.388	ug/l #	27
52) Toluene	10.504	92	70442	2.978	ug/l	95
59) 2-Hexanone	11.092	43	3771	0.339	ug/l	78
67) Ethyl Benzene	11.839	91	177589	3.977	ug/l	91
68) m/p-Xylenes	11.951	106	75324	4.610	ug/l	94
69) o-Xylene	12.275	106	46891	2.863	ug/l	99
71) Bromoform	12.727	173	3218	0.458	ug/l #	1
73) Isopropylbenzene	12.574	105	12822	0.323	ug/l	95
75) 1,1,2,2-Tetrachloroethane	12.827	83	566	Below Cal	#	40
76) 1,2,3-Trichloropropane	12.727	75	299116	28.796	ug/l #	1
78) n-propylbenzene	12.916	91	11309	0.266	ug/l	98
80) 1,3,5-Trimethylbenzene	13.057	105	23158	0.750	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.727	75	299116	78.580	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.363	105	46123	1.560	ug/l	99
90) Hexachloroethane	14.221	117	1627	0.284	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.263	180	1681	3.224	ug/l #	73
95) Naphthalene	15.504	128	109910	10.304	ug/l	99
96) 1,2,3-Trichlorobenzene	15.692	180	1825	2.999	ug/l #	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031922\
Data File : VN071393.D
Acq On : 19 Mar 2022 13:18
Operator : JC\MD
Sample : N1974-13
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
B-3

Quant Time: Mar 21 05:50:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration




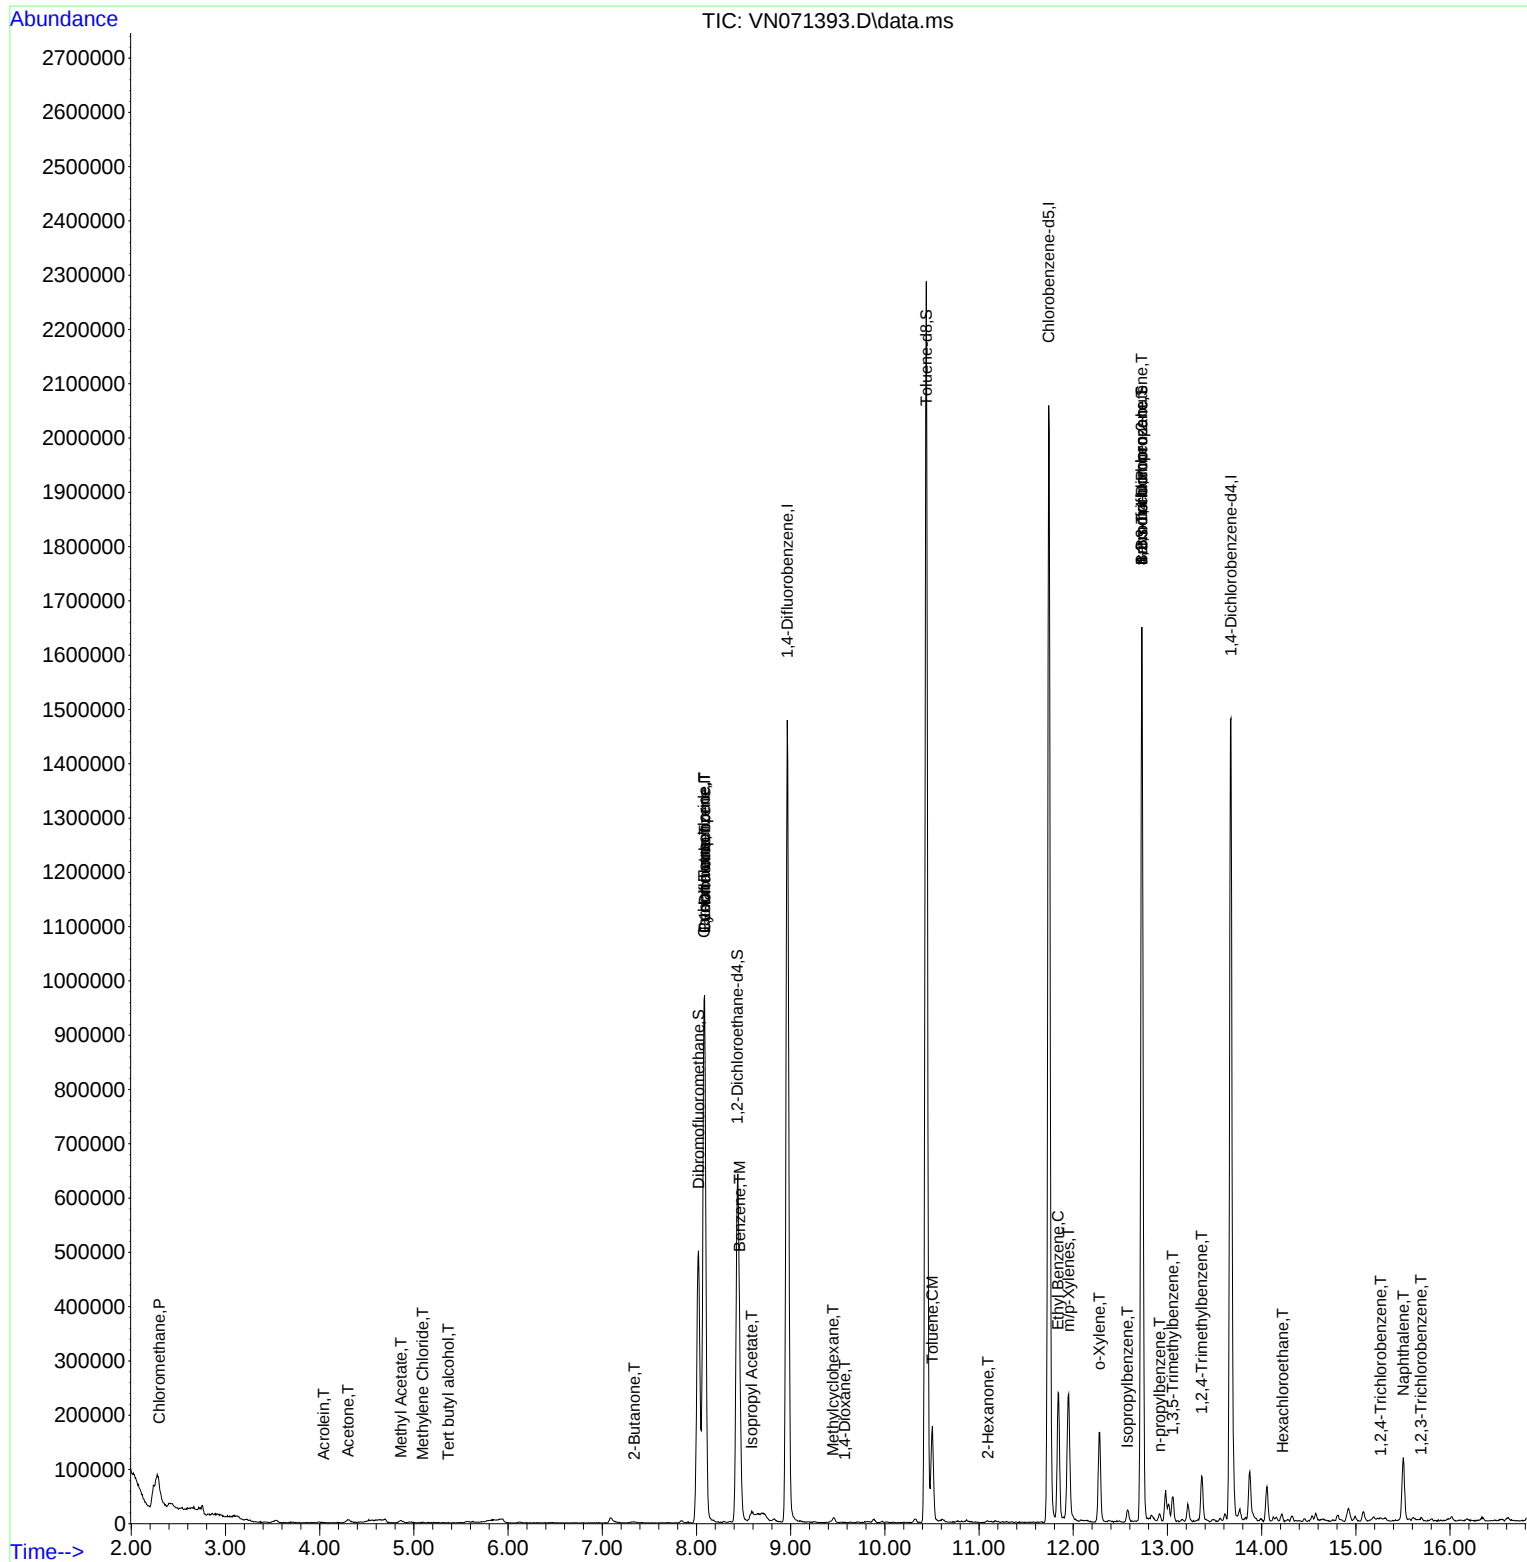




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.087 min Scan# 10
Delta R.T. 0.001 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion:168 Resp: 759624
Ion Ratio Lower Upper
168 100
99 58.5 41.3 61.9



#3
Chloromethane
Concen: 0.425 ug/l
RT: 2.299 min Scan# 53
Delta R.T. -0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 50 Resp: 5133
Ion Ratio Lower Upper
50 100
52 35.6 25.4 38.0









#5
Bromomethane
Concen: Below Cal
RT: 2.834 min Scan# 14
Delta R.T. -0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion: 94 Resp: 287
Ion Ratio Lower Upper
94 100
96 0.0 73.8 110.8#

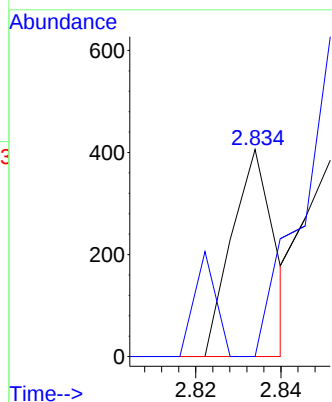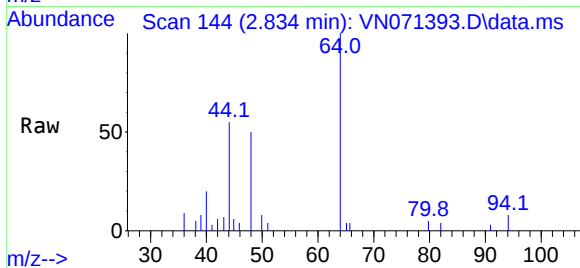

#11
Tert butyl alcohol
Concen: 0.205 ug/l
RT: 5.363 min Scan# 574
Delta R.T. -0.006 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 59 Resp: 420
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


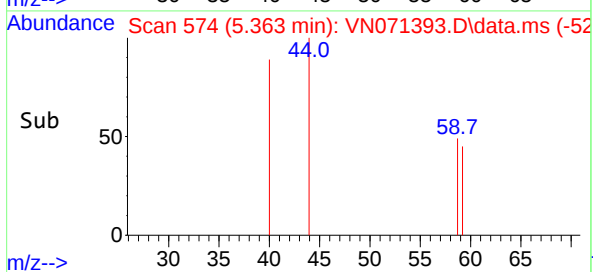
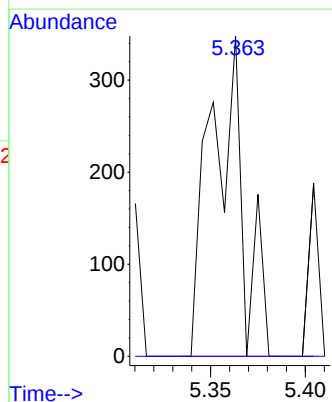
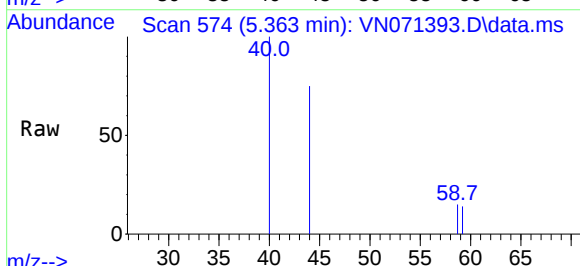




#13
Acrolein
Concen: 0.299 ug/l
RT: 4.040 min Scan# 349
Delta R.T. 0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion: 56 Resp: 648
Ion Ratio Lower Upper
56 100
55 0.0 56.6 85.0#

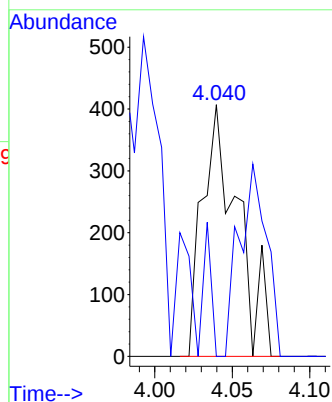

#16
Acetone
Concen: 1.532 ug/l
RT: 4.299 min Scan# 393
Delta R.T. 0.012 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 43 Resp: 7761
Ion Ratio Lower Upper
43 100
58 30.1 23.1 34.7


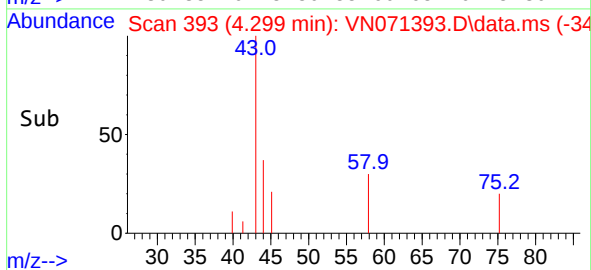






#18
Methyl Acetate
Concen: 1.117 ug/l
RT: 4.863 min Scan# 487
Delta R.T. 0.012 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion: 43 Resp: 8880
Ion Ratio Lower Upper
43 100
74 18.0 19.4 29.2#



#20
Methylene Chloride
Concen: 0.418 ug/l
RT: 5.093 min Scan# 528
Delta R.T. -0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 84 Resp: 340
Ion Ratio Lower Upper
84 100
49 0.0 93.5 140.3#
51 0.0 29.4 44.2#
86 0.0 53.0 79.4#

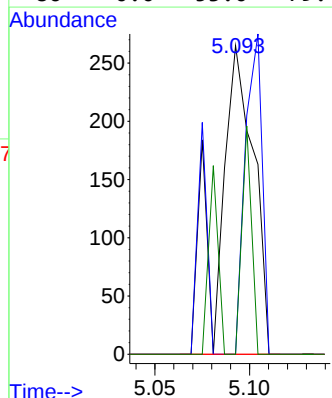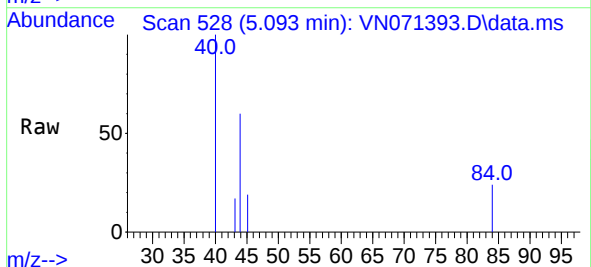



#25

2-Butanone

Concen: 0.320 ug/l

RT: 7.340 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN071393.D

Acq: 19 Mar 2022 13:18

Instrument :

MSVOA_N

ClientSampleId :





B-3

Tgt Ion: 43 Resp: 2614

Ion Ratio Lower Upper

43 100

72 17.7 21.7 32.5#

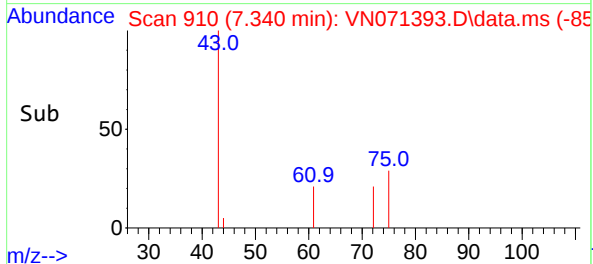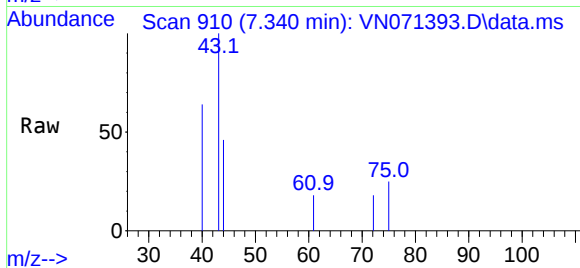

#31

Cyclohexane

Concen: 1.015 ug/l

RT: 8.087 min Scan# 1037

Delta R.T. -0.006 min

Lab File: VN071393.D

Acq: 19 Mar 2022 13:18




Tgt Ion: 56 Resp: 16881


Ion Ratio Lower Upper

56 100

69 182.3 27.1 40.7#

84 144.5 73.4 110.0#

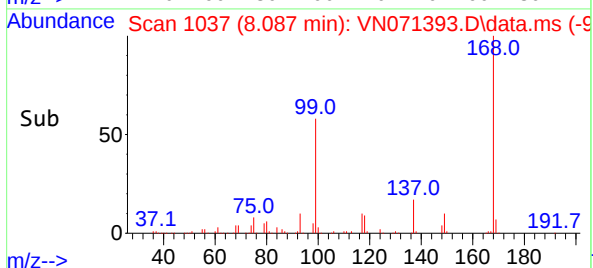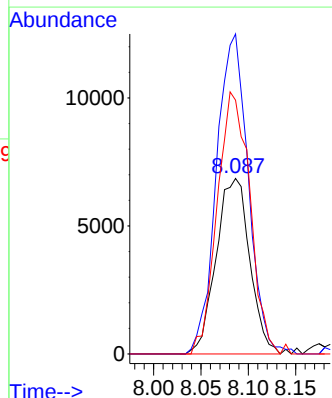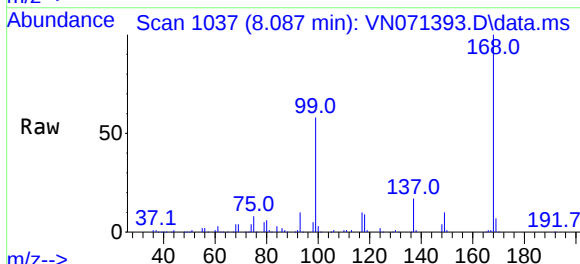



#33

1,2-Dichloroethane-d4

Concen: 46.768 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. -0.006 min

Lab File: VN071393.D

Acq: 19 Mar 2022 13:18

Instrument :

MSVOA_N

ClientSampleId :





B-3

Tgt Ion: 65 Resp: 486894

Ion Ratio Lower Upper

65 100

67 52.3 0.0 103.0

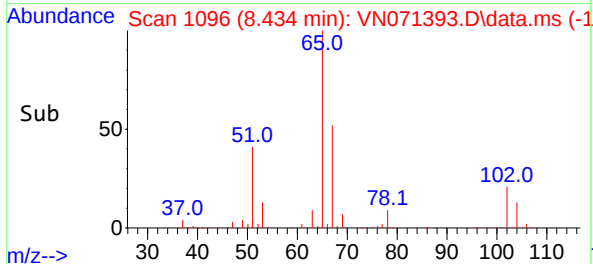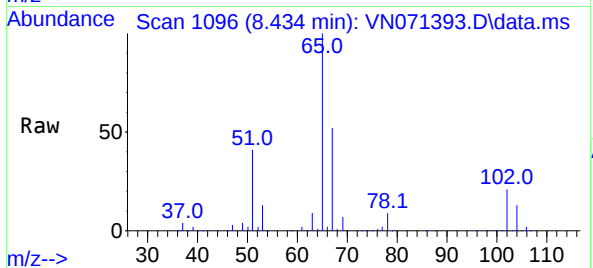

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN071393.D

Acq: 19 Mar 2022 13:18




Tgt Ion: 114 Resp: 1261114


Ion Ratio Lower Upper

114 100

63 21.8 0.0 37.8

88 15.9 0.0 27.4


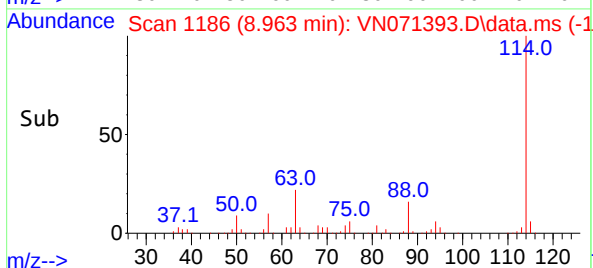
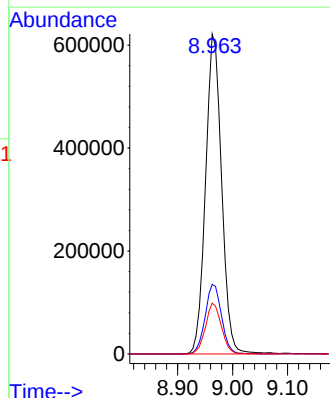
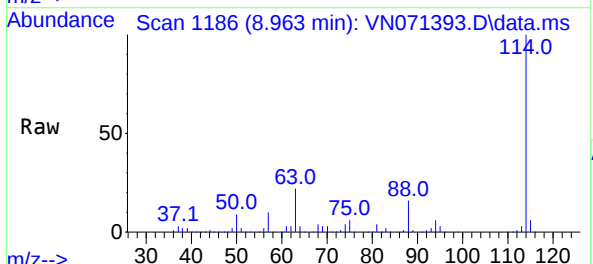




#35
Dibromofluoromethane
Concen: 46.209 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion:113 Resp: 367735
Ion Ratio Lower Upper
113 100
111 102.6 82.2 123.2
192 20.6 16.9 25.3

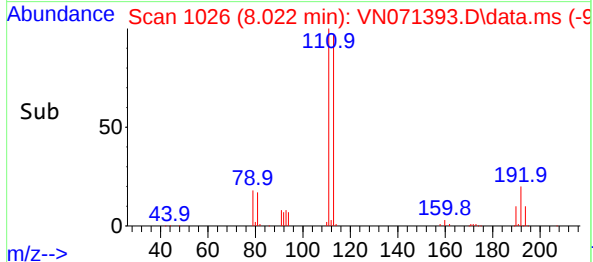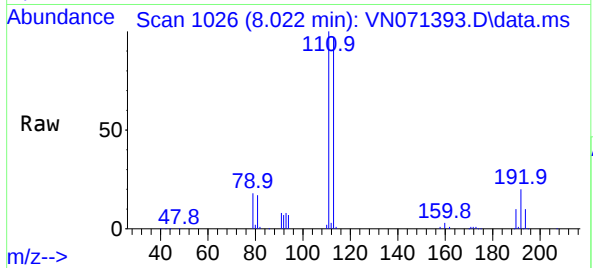

#36
1,1-Dichloropropene
Concen: 4.743 ug/l
RT: 8.087 min Scan# 1037
Delta R.T. -0.129 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 75 Resp: 60477
Ion Ratio Lower Upper
75 100
110 8.6 18.4 55.2#
77 0.0 24.4 36.6#


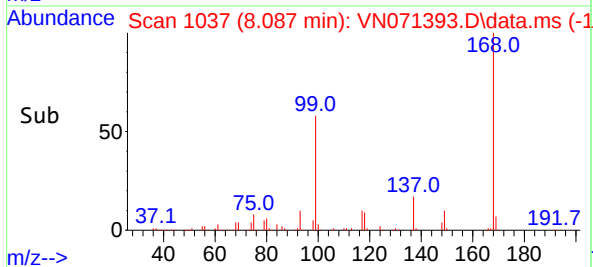

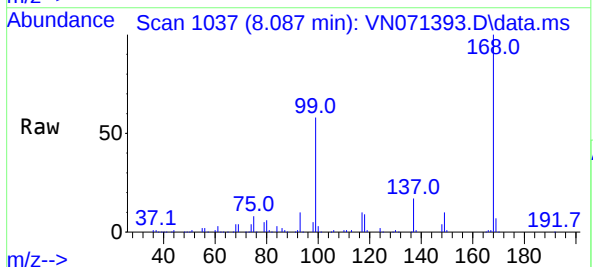




#38
Carbon Tetrachloride
Concen: 6.030 ug/l
RT: 8.081 min Scan# 117
Delta R.T. -0.123 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion:117 Resp: 74370
Ion Ratio Lower Upper
117 100
119 6.1 76.1 114.1#
121 0.0 24.2 36.2#

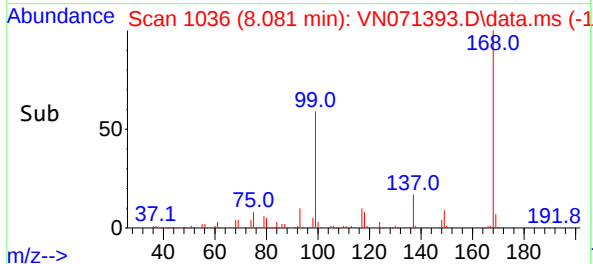

#39
Methylcyclohexane
Concen: 0.243 ug/l
RT: 9.451 min Scan# 1269
Delta R.T. -0.006 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 83 Resp: 3642
Ion Ratio Lower Upper
83 100
55 78.0 58.1 87.1
98 40.5 38.4 57.6


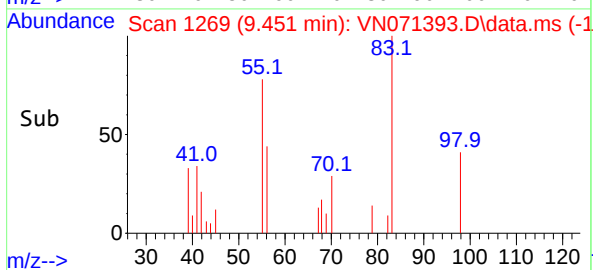

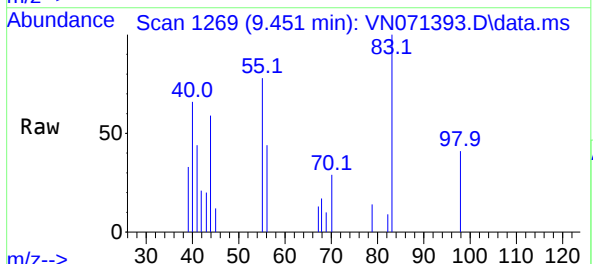




#40
Benzene
Concen: 4.708 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. 0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion: 78 Resp: 180866
Ion Ratio Lower Upper
78 100
77 25.1 18.6 27.8

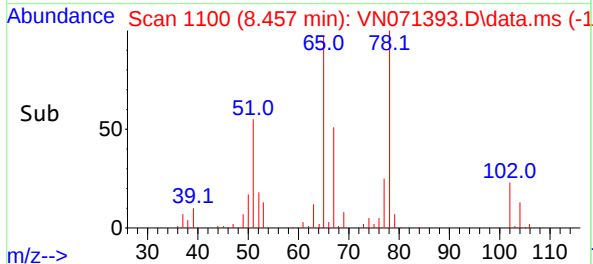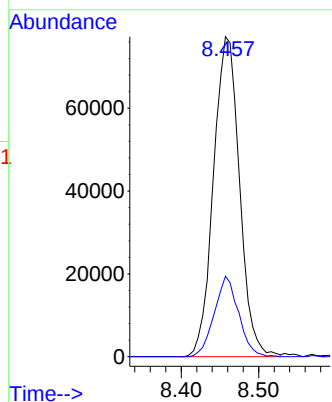

#43
Isopropyl Acetate
Concen: 0.412 ug/l
RT: 8.586 min Scan# 1122
Delta R.T. 0.029 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 43 Resp: 10811
Ion Ratio Lower Upper
43 100
61 0.0 20.4 30.6#
87 0.0 11.2 16.8#


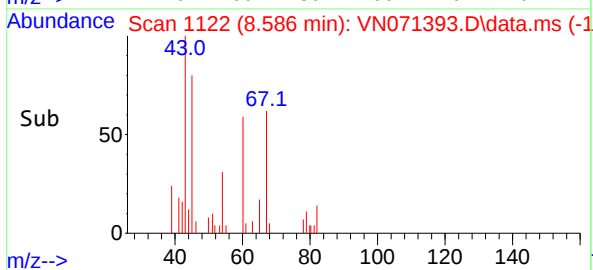
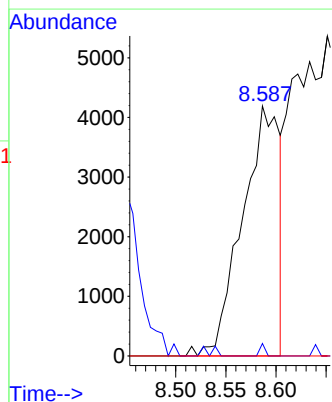
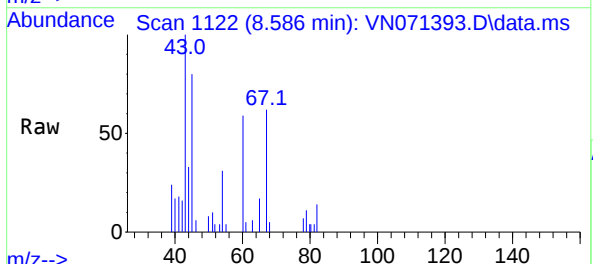




#49
1,4-Dioxane
Concen: 0.388 ug/l
RT: 9.575 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion: 88 Resp: 82
Ion Ratio Lower Upper
88 100
43 0.0 23.4 35.2#
58 0.0 50.6 75.8#

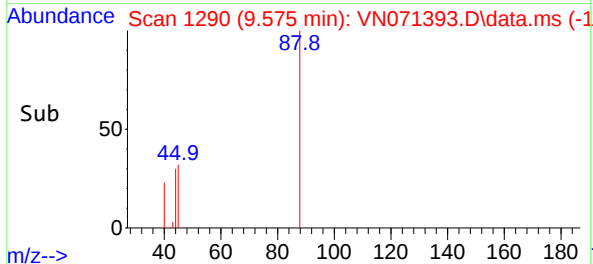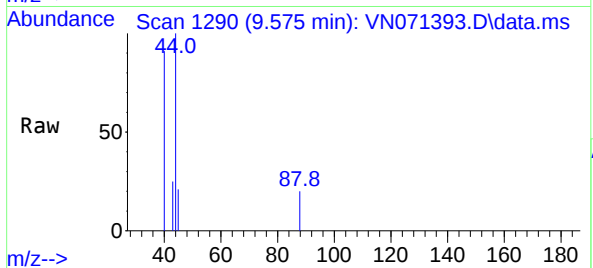

#50
Toluene-d8
Concen: 49.063 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 98 Resp: 1572045
Ion Ratio Lower Upper
98 100
100 64.9 50.4 75.6


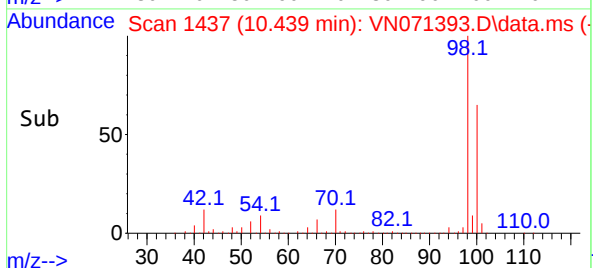

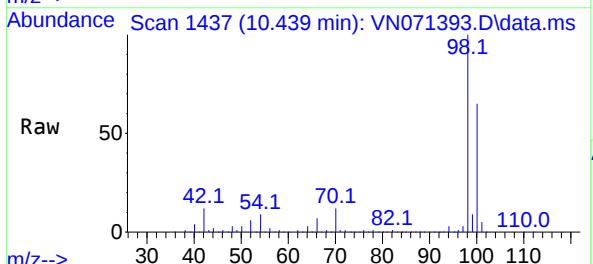




#52
Toluene
Concen: 2.978 ug/l
RT: 10.504 min Scan# 1448
Delta R.T. 0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion: 92 Resp: 70442
Ion Ratio Lower Upper
92 100
91 170.7 142.0 213.0

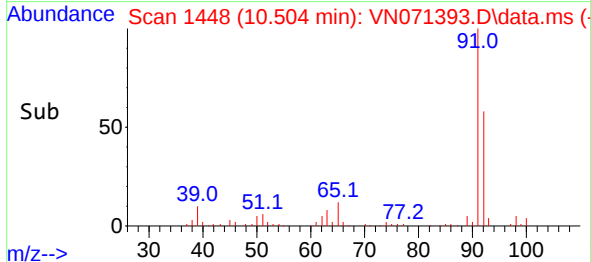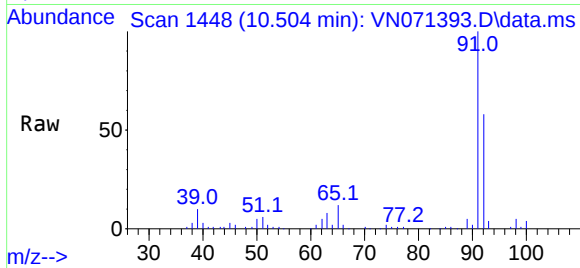

#59
2-Hexanone
Concen: 0.339 ug/l
RT: 11.092 min Scan# 1548
Delta R.T. 0.012 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 43 Resp: 3771
Ion Ratio Lower Upper
43 100
58 38.0 26.9 80.7


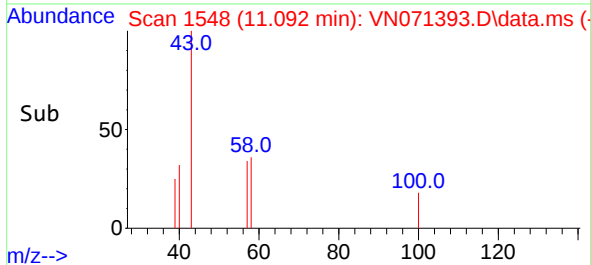

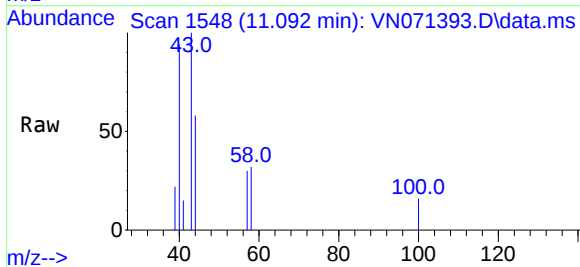




#62
4-Bromofluorobenzene
Concen: 53.389 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion: 95 Resp: 579277
Ion Ratio Lower Upper
95 100
174 78.3 0.0 187.2
176 75.4 0.0 181.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 117 Resp: 1176127
Ion Ratio Lower Upper
117 100
82 57.9 42.4 63.6
119 31.6 25.4 38.2



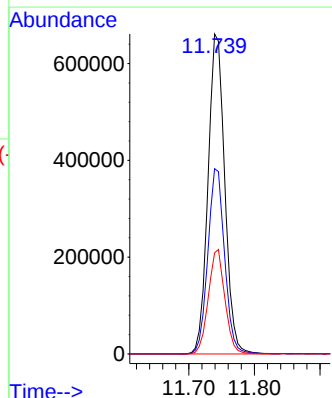





#67
Ethyl Benzene
Concen: 3.977 ug/l
RT: 11.839 min Scan# 1675
Delta R.T. 0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion: 91 Resp: 177589
Ion Ratio Lower Upper
91 100
106 27.0 25.7 38.5

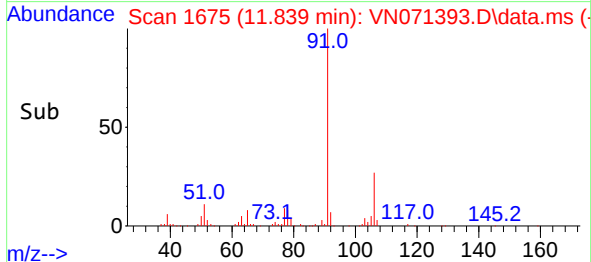

#68
m/p-Xylenes
Concen: 4.610 ug/l
RT: 11.951 min Scan# 1694
Delta R.T. -0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 106 Resp: 75324
Ion Ratio Lower Upper
106 100
91 210.2 160.6 240.8



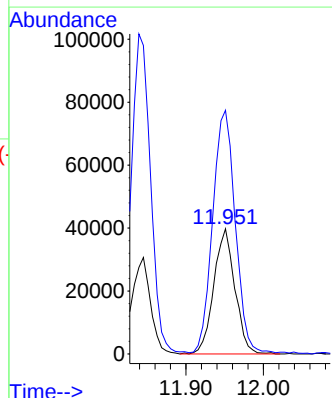





#69
o-Xylene
Concen: 2.863 ug/l
RT: 12.275 min Scan# 11
Delta R.T. -0.005 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion:106 Resp: 46891
Ion Ratio Lower Upper
106 100
91 212.6 105.8 317.3

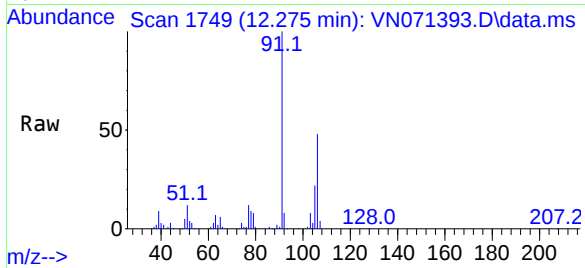

#71
Bromoform
Concen: 0.458 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.270 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion:173 Resp: 3218
Ion Ratio Lower Upper
173 100
175 774.0 24.2 72.6#
254 0.0 0.0 0.0


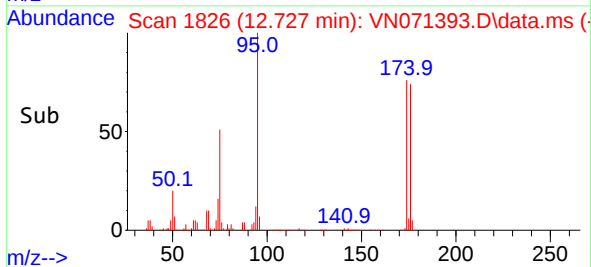

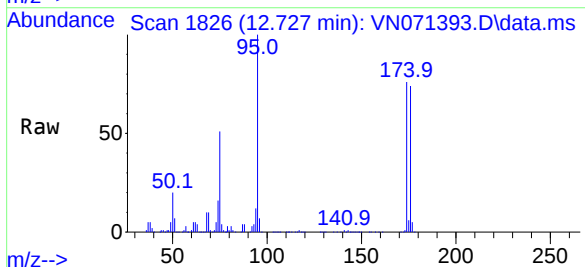




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1986
Delta R.T. 0.006 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion:152 Resp: 411484
Ion Ratio Lower Upper
152 100
115 60.3 27.5 82.5
150 159.0 0.0 344.4

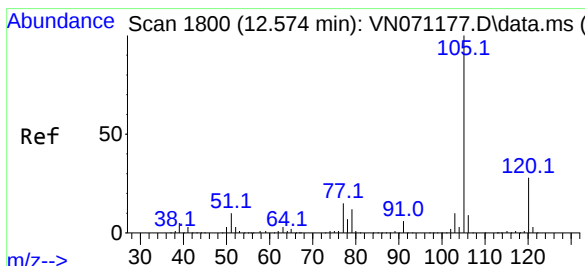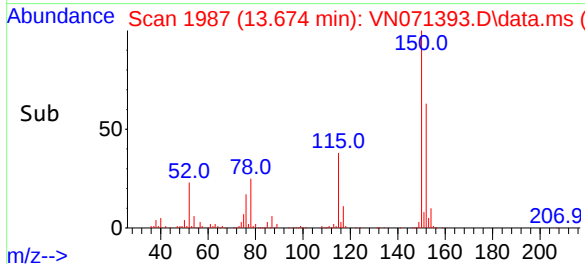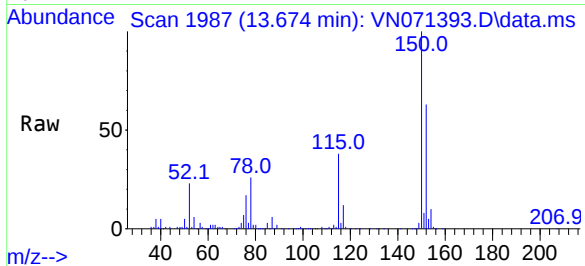

#73
Isopropylbenzene
Concen: 0.323 ug/l
RT: 12.574 min Scan# 1800
Delta R.T. 0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion:105 Resp: 12822
Ion Ratio Lower Upper
105 100
120 24.2 13.4 40.1


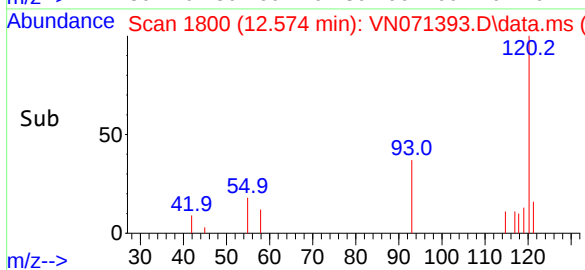

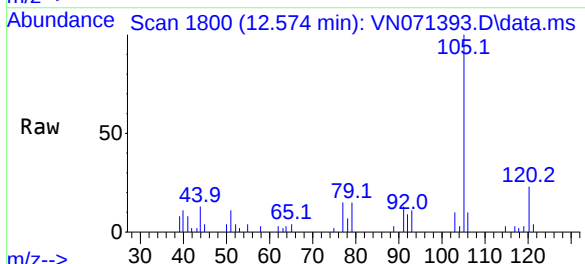




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.827 min Scan# 1842
Delta R.T. 0.006 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion: 83 Resp: 566
Ion Ratio Lower Upper
83 100
131 9.7 5.5 16.5
85 10.2 32.4 97.2#



#76
1,2,3-Trichloropropane
Concen: 28.796 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 75 Resp: 299116
Ion Ratio Lower Upper
75 100
77 1.3 82.6 247.8#









#78
n-propylbenzene
Concen: 0.266 ug/l
RT: 12.916 min Scan# 1858
Delta R.T. 0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion: 91 Resp: 11309
Ion Ratio Lower Upper
91 100
120 22.8 11.9 35.9



#80
1,3,5-Trimethylbenzene
Concen: 0.750 ug/l
RT: 13.057 min Scan# 1882
Delta R.T. 0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 105 Resp: 23158
Ion Ratio Lower Upper
105 100
120 48.2 24.6 73.6



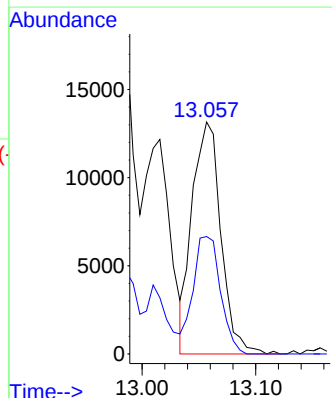





#81
trans-1,4-Dichloro-2-butene
Concen: 78.580 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion: 75 Resp: 299116
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

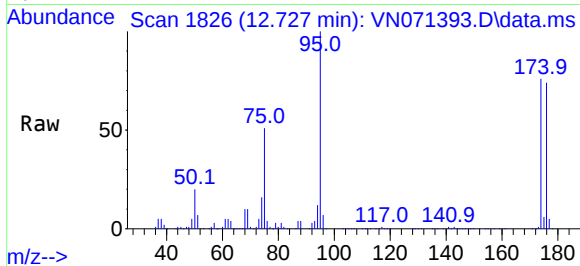

#84
1,2,4-Trimethylbenzene
Concen: 1.560 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion: 105 Resp: 46123
Ion Ratio Lower Upper
105 100
120 46.2 22.8 68.4


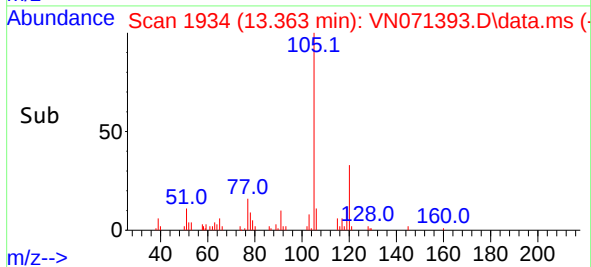

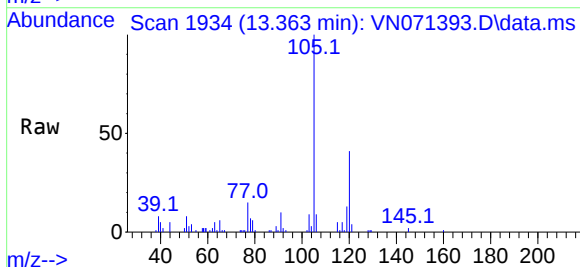




#90
Hexachloroethane
Concen: 0.284 ug/l
RT: 14.221 min Scan# 2078
Delta R.T. 0.012 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18




Instrument :
MSVOA_N
ClientSampleId :
B-3


Tgt Ion:117 Resp: 1627
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

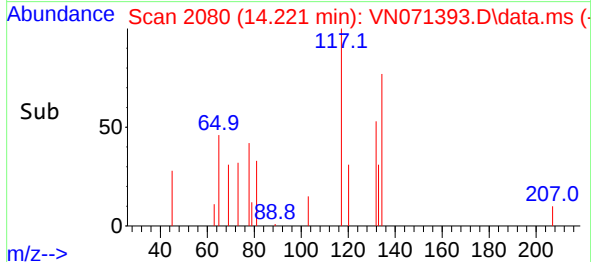

#93
1,2,4-Trichlorobenzene
Concen: 3.224 ug/l
RT: 15.263 min Scan# 2257
Delta R.T. 0.001 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion:180 Resp: 1681
Ion Ratio Lower Upper
180 100
182 88.3 48.3 144.9
145 75.7 14.5 43.5#


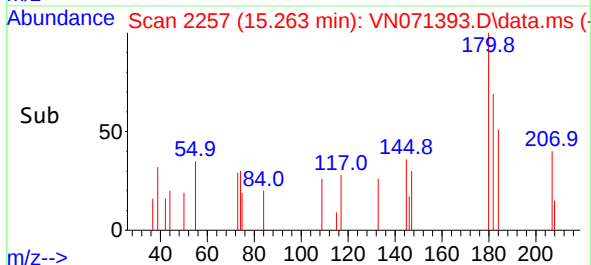
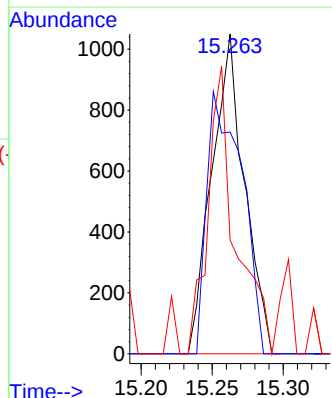
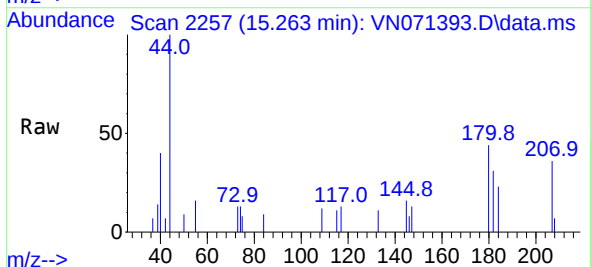




#95
Naphthalene
Concen: 10.304 ug/l
RT: 15.504 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Instrument :
MSVOA_N
ClientSampleId :
B-3

Tgt Ion:128 Resp: 109910
Ion Ratio Lower Upper
128 100
127 13.8 10.5 15.7
129 10.4 8.7 13.1

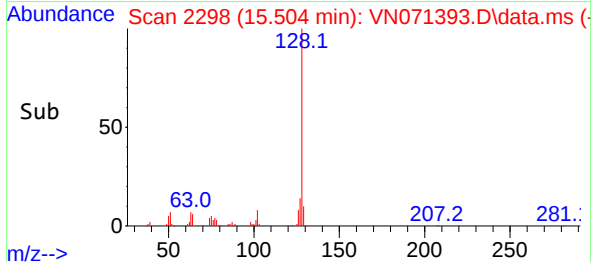

#96
1,2,3-Trichlorobenzene
Concen: 2.999 ug/l
RT: 15.692 min Scan# 2330
Delta R.T. -0.006 min
Lab File: VN071393.D
Acq: 19 Mar 2022 13:18

Tgt Ion:180 Resp: 1825
Ion Ratio Lower Upper
180 100
182 90.7 47.4 142.2
145 0.0 15.0 45.1#

