

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031922\
 Data File : VN071398.D
 Acq On : 19 Mar 2022 15:18
 Operator : JC\MD
 Sample : N1958-19
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 C-4-3-4

Quant Time: Mar 21 05:51:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.087	168	767485	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.969	114	1292143	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1243211	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	428500	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	493673	46.933	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	93.860%		
35) Dibromofluoromethane	8.022	113	375748	46.082	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	92.160%		
50) Toluene-d8	10.439	98	1628439	49.602	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	99.200%		
62) 4-Bromofluorobenzene	12.727	95	593778	53.412	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	106.820%		
Target Compounds						Qvalue
3) Chloromethane	2.299	50	4523	0.366	ug/l	94
5) Bromomethane	2.869	94	842	Below Cal	#	66
13) Acrolein	4.046	56	501	0.229	ug/l #	77
16) Acetone	4.293	43	52131	10.186	ug/l	92
18) Methyl Acetate	4.863	43	21050	1.987	ug/l #	69
20) Methylene Chloride	5.098	84	13078	1.769	ug/l	94
25) 2-Butanone	7.334	43	8550	1.037	ug/l	95
29) Tetrahydrofuran	7.692	42	1724	0.302	ug/l #	84
31) Cyclohexane	8.087	56	16574	0.987	ug/l #	1
36) 1,1-Dichloropropene	8.081	75	61564	4.712	ug/l #	49
38) Carbon Tetrachloride	8.081	117	74357	5.884	ug/l #	15
40) Benzene	8.457	78	15183	0.386	ug/l #	86
43) Isopropyl Acetate	8.557	43	97993	3.645	ug/l #	77
48) Methyl methacrylate	9.539	41	21146	1.697	ug/l #	19
49) 1,4-Dioxane	9.628	88	124	0.573	ug/l #	1
51) 4-Methyl-2-Pentanone	10.328	43	10406	0.624	ug/l #	73
52) Toluene	10.498	92	10593	0.437	ug/l	91
54) cis-1,3-Dichloropropene	10.239	75	95675	6.044	ug/l #	58
57) 1,3-Dichloropropane	11.086	76	35857	2.057	ug/l #	43
59) 2-Hexanone	11.086	43	577138	50.692	ug/l #	49
67) Ethyl Benzene	11.839	91	29762	0.630	ug/l	95
68) m/p-Xylenes	11.945	106	10278	0.595	ug/l	96
69) o-Xylene	12.274	106	7471	0.432	ug/l	94
71) Bromoform	12.727	173	3388	0.456	ug/l #	1
74) N-amyl acetate	12.363	43	3282	0.211	ug/l #	45
75) 1,1,2,2-Tetrachloroethane	12.722	83	168	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.727	75	306502	28.287	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	306502	77.323	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.363	105	6650	0.216	ug/l	98
93) 1,2,4-Trichlorobenzene	15.263	180	60	2.997	ug/l #	12
95) Naphthalene	15.504	128	15787	5.790	ug/l	98
96) 1,2,3-Trichlorobenzene	15.698	180	116	2.748	ug/l #	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031922\
Data File : VN071398.D
Acq On : 19 Mar 2022 15:18
Operator : JC\MD
Sample : N1958-19
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4

Quant Time: Mar 21 05:51:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration




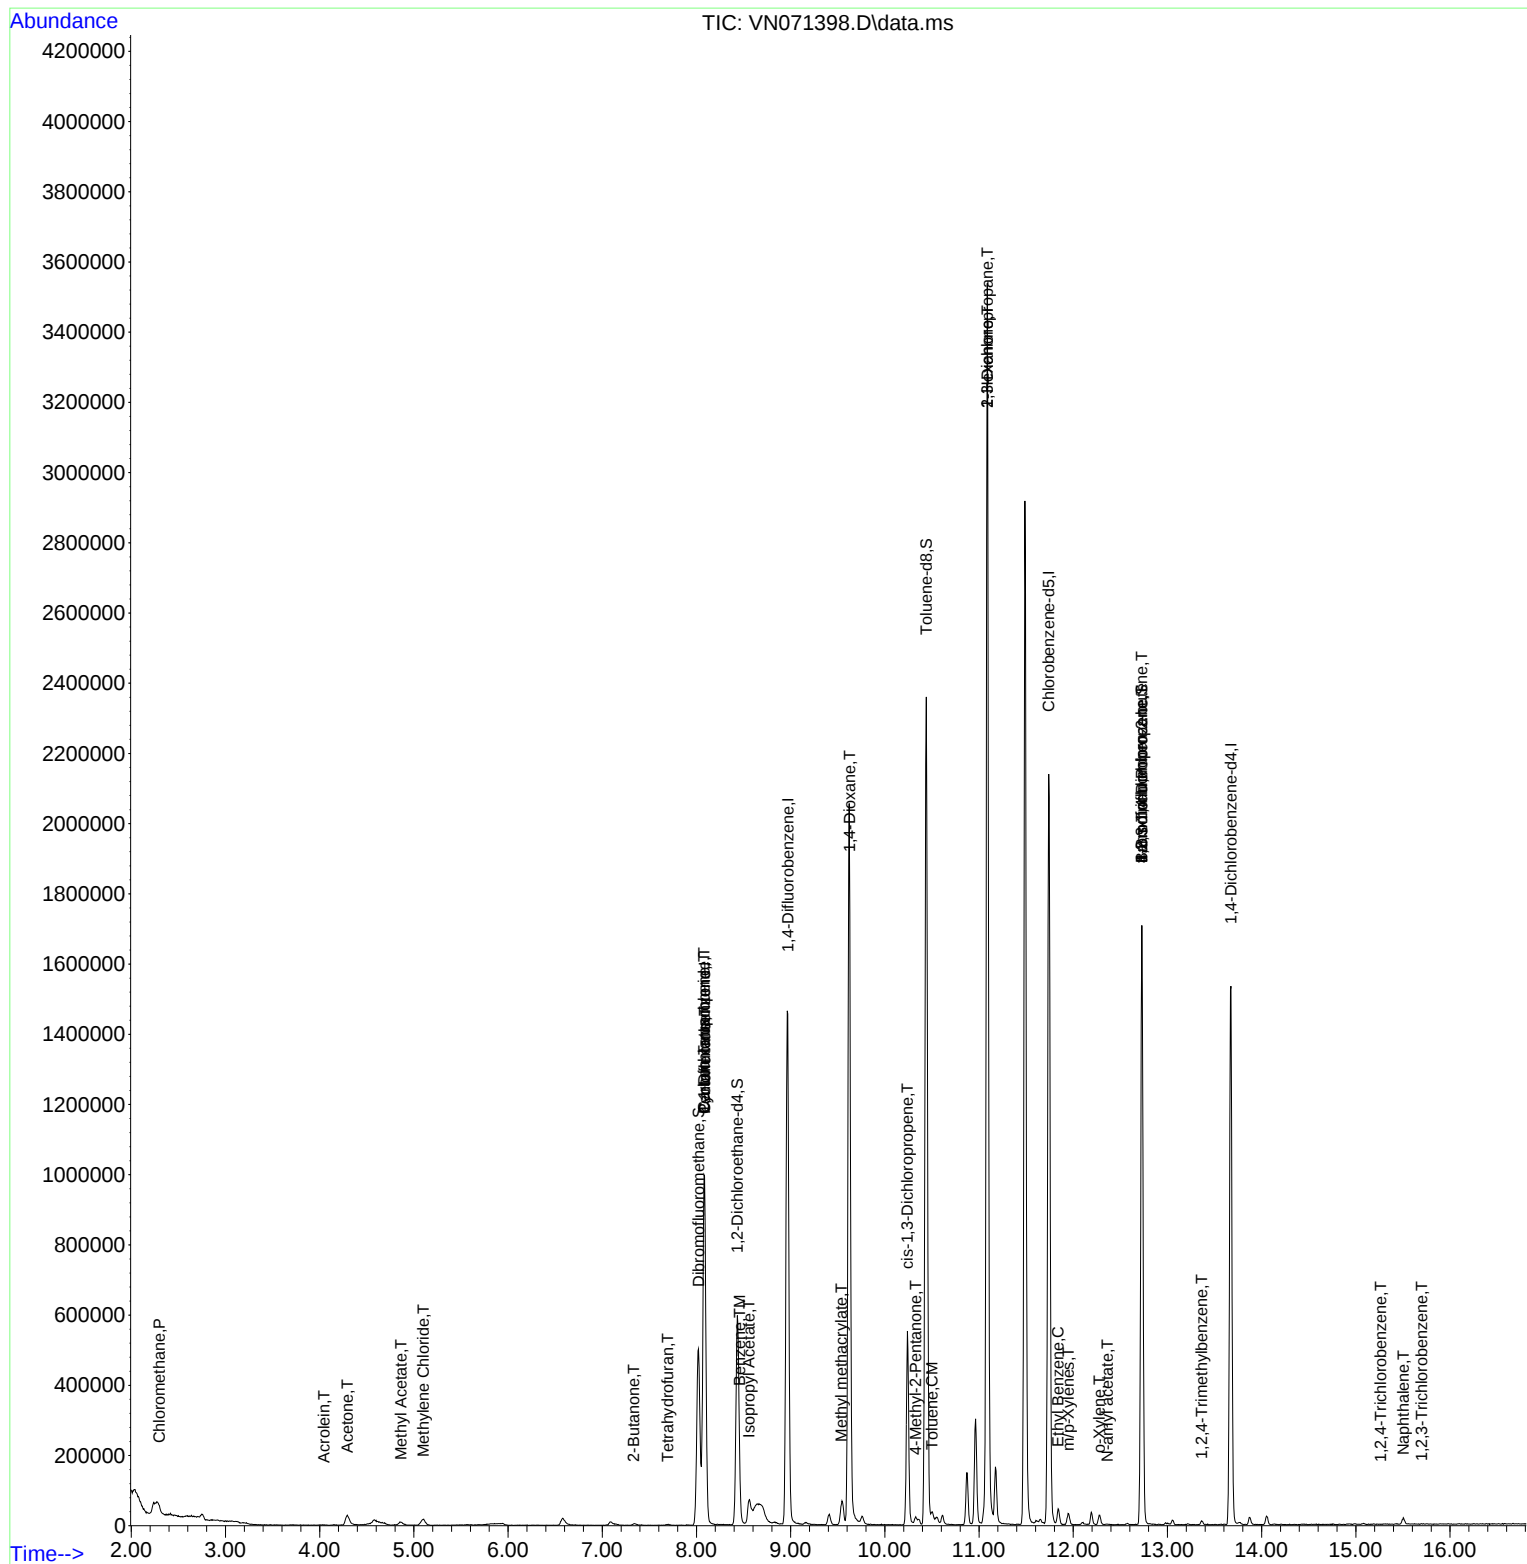




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.087 min Scan# 10
Delta R.T. 0.001 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion:168 Resp: 767485
Ion Ratio Lower Upper
168 100
99 56.3 41.3 61.9

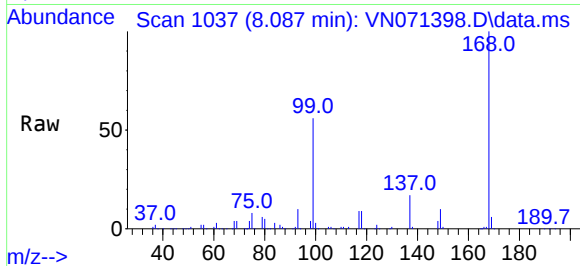

#3
Chloromethane
Concen: 0.366 ug/l
RT: 2.299 min Scan# 53
Delta R.T. -0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 50 Resp: 4523
Ion Ratio Lower Upper
50 100
52 28.4 25.4 38.0


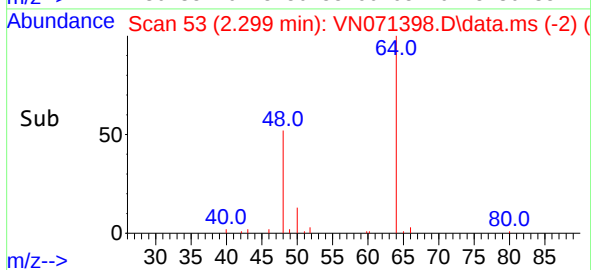

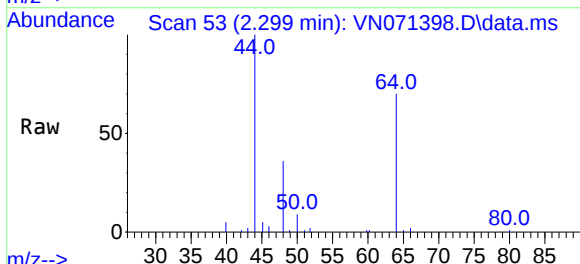




#5
Bromomethane
Concen: Below Cal
RT: 2.869 min Scan# 11
Delta R.T. 0.035 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion: 94 Resp: 842
Ion Ratio Lower Upper
94 100
96 59.7 73.8 110.8#



#13
Acrolein
Concen: 0.229 ug/l
RT: 4.046 min Scan# 350
Delta R.T. 0.006 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 56 Resp: 501
Ion Ratio Lower Upper
56 100
55 51.7 56.6 85.0#


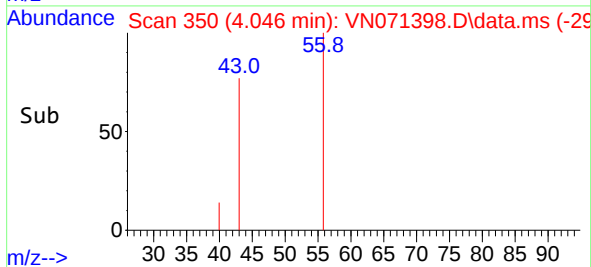

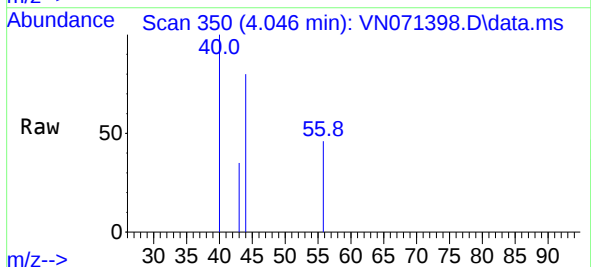




#16
Acetone
Concen: 10.186 ug/l
RT: 4.293 min Scan# 391
Delta R.T. 0.006 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion: 43 Resp: 52131
Ion Ratio Lower Upper
43 100
58 33.3 23.1 34.7

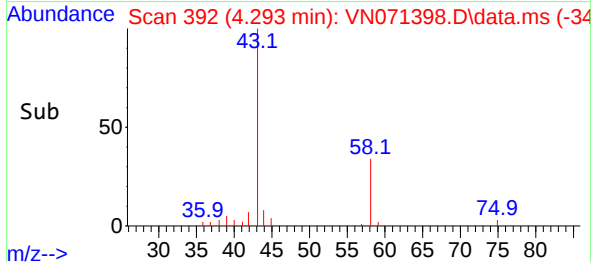

#18
Methyl Acetate
Concen: 1.987 ug/l
RT: 4.863 min Scan# 489
Delta R.T. 0.012 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 43 Resp: 21050
Ion Ratio Lower Upper
43 100
74 8.8 19.4 29.2#

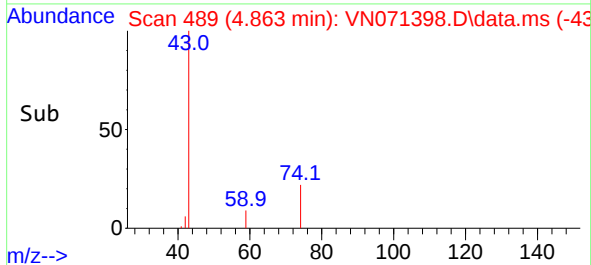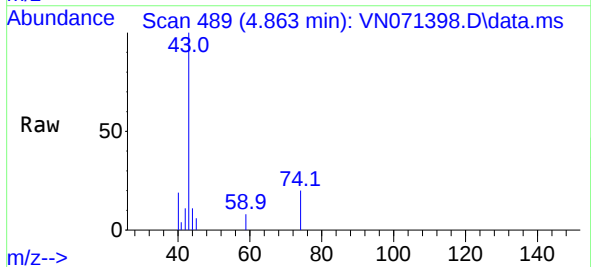







#20
Methylene Chloride
Concen: 1.769 ug/l
RT: 5.098 min Scan# 51
Delta R.T. 0.005 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4

Tgt Ion: 84 Resp: 13078




Ion	Ratio	Lower	Upper
84	100		
49	115.5	93.5	140.3
51	38.5	29.4	44.2
86	54.7	53.0	79.4

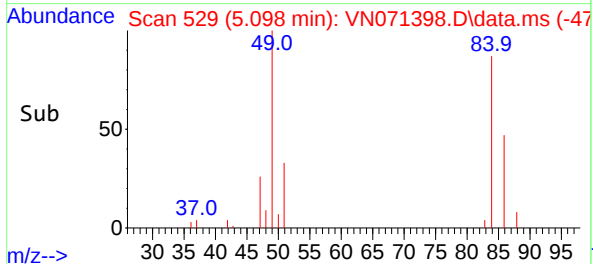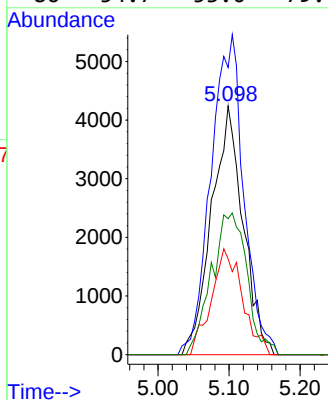


#25
2-Butanone
Concen: 1.037 ug/l
RT: 7.334 min Scan# 909
Delta R.T. 0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 43 Resp: 8550

Ion	Ratio	Lower	Upper
43	100		
72	24.4	21.7	32.5


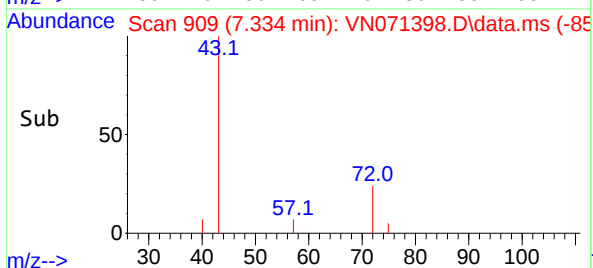
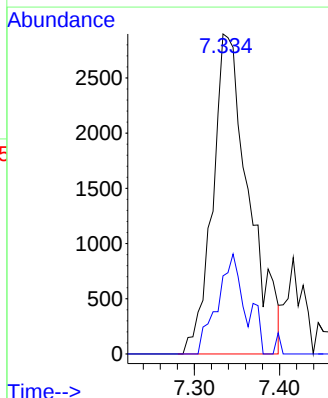
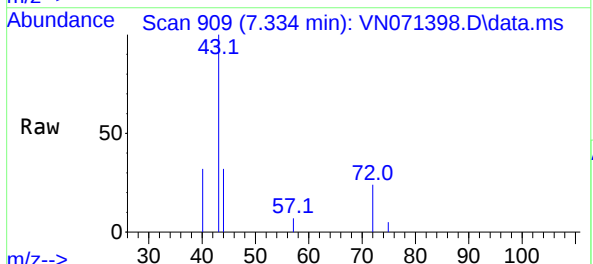


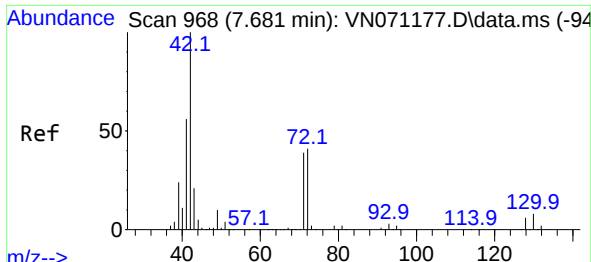

#29
Tetrahydrofuran
Concen: 0.302 ug/l
RT: 7.692 min Scan# 91
Delta R.T. 0.012 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion: 42 Resp: 1724
Ion Ratio Lower Upper
42 100
72 31.1 36.3 54.5#
71 37.4 34.7 52.1

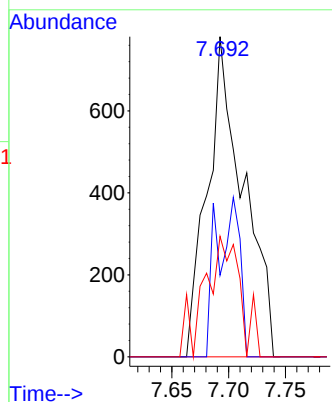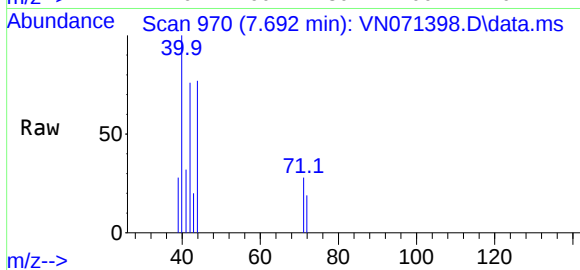

#31
Cyclohexane
Concen: 0.987 ug/l
RT: 8.087 min Scan# 1037
Delta R.T. -0.006 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 56 Resp: 16574
Ion Ratio Lower Upper
56 100
69 167.8 27.1 40.7#
84 140.5 73.4 110.0#


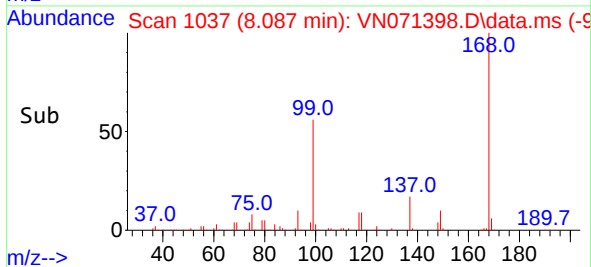
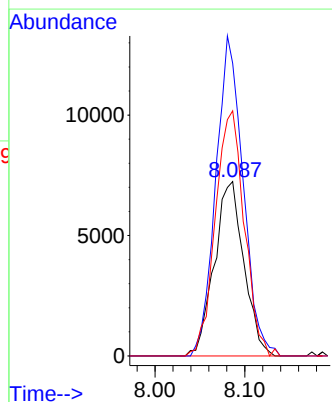
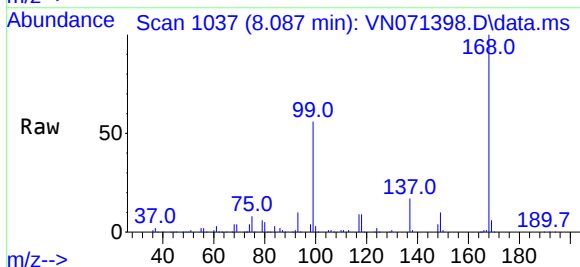


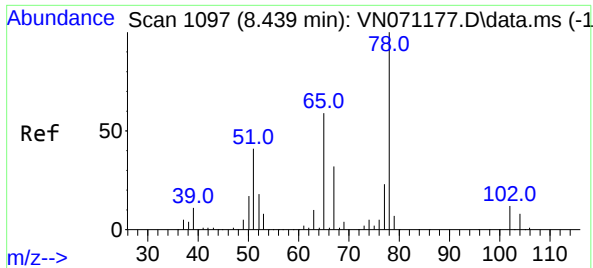

#33
1,2-Dichloroethane-d4
Concen: 46.933 ug/l
RT: 8.434 min Scan# 1096
Delta R.T. -0.006 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion: 65 Resp: 493673
Ion Ratio Lower Upper
65 100
67 52.8 0.0 103.0

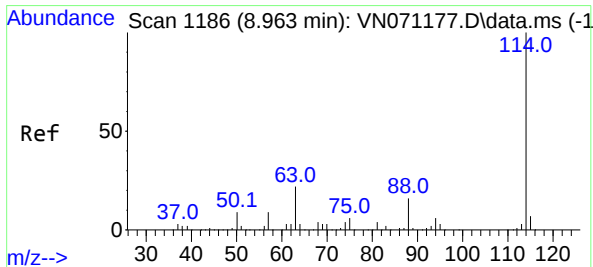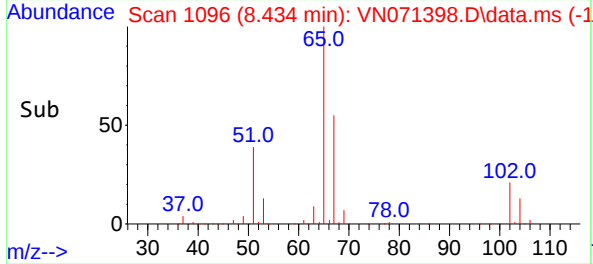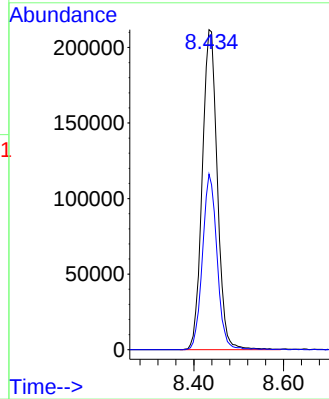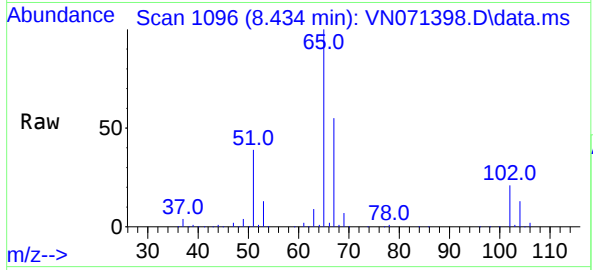

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.969 min Scan# 1187
Delta R.T. 0.006 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 114 Resp: 1292143
Ion Ratio Lower Upper
114 100
63 21.9 0.0 37.8
88 15.8 0.0 27.4


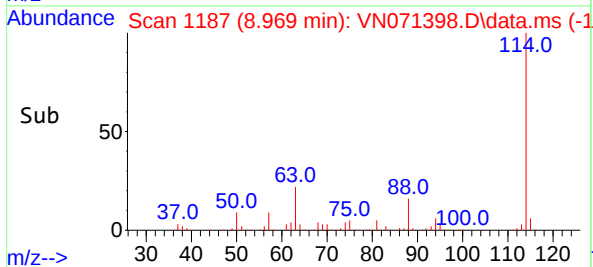
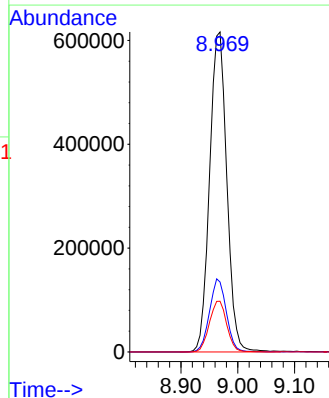
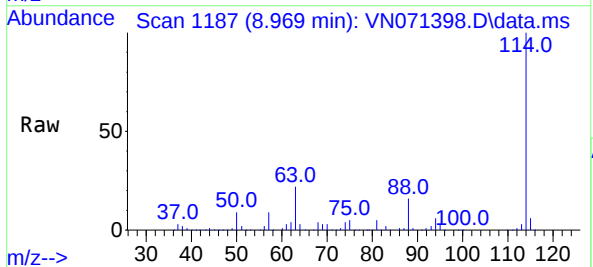


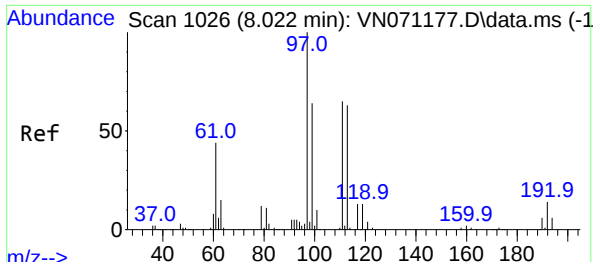

#35
Dibromofluoromethane
Concen: 46.082 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion:113 Resp: 375748
Ion Ratio Lower Upper
113 100
111 102.5 82.2 123.2
192 20.0 16.9 25.3

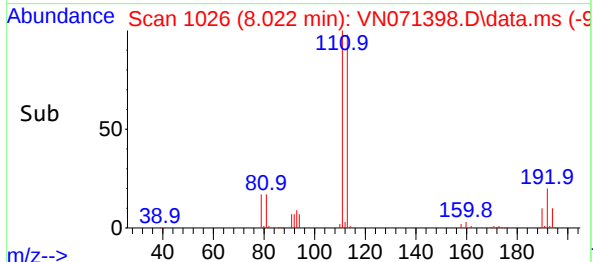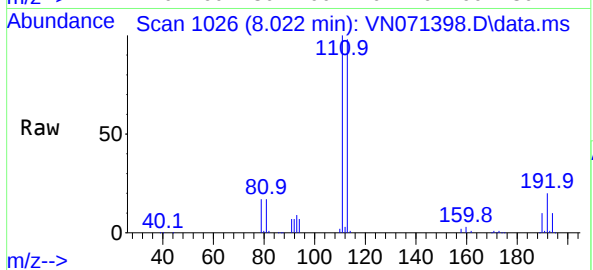

#36
1,1-Dichloropropene
Concen: 4.712 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.135 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 75 Resp: 61564
Ion Ratio Lower Upper
75 100
110 8.9 18.4 55.2#
77 0.0 24.4 36.6#


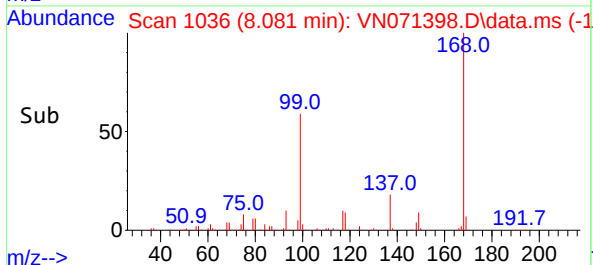

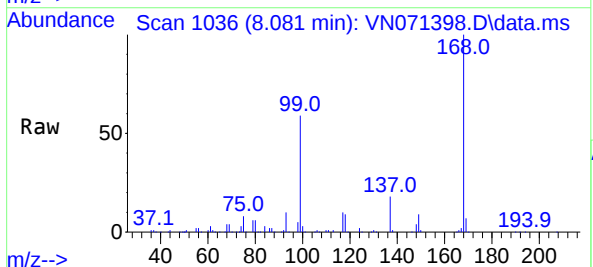




#38
Carbon Tetrachloride
Concen: 5.884 ug/l
RT: 8.081 min Scan# 1100
Delta R.T. -0.123 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion:117 Resp: 74357
Ion Ratio Lower Upper
117 100
119 3.8 76.1 114.1#
121 0.0 24.2 36.2#

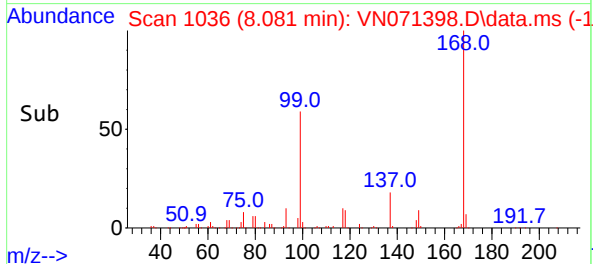

#40
Benzene
Concen: 0.386 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. 0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 78 Resp: 15183
Ion Ratio Lower Upper
78 100
77 16.4 18.6 27.8#


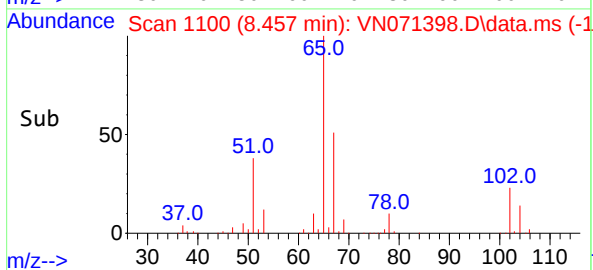

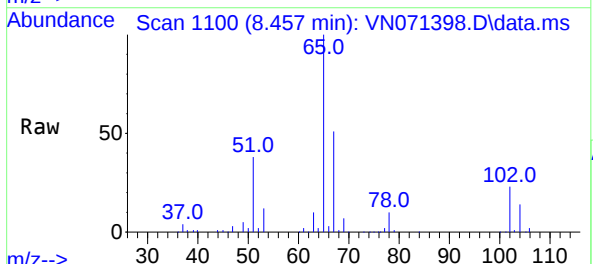




#43
Isopropyl Acetate
Concen: 3.645 ug/l
RT: 8.557 min Scan# 1117
Delta R.T. 0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion: 43 Resp: 97993
Ion Ratio Lower Upper
43 100
61 12.1 20.4 30.6#
87 6.9 11.2 16.8#

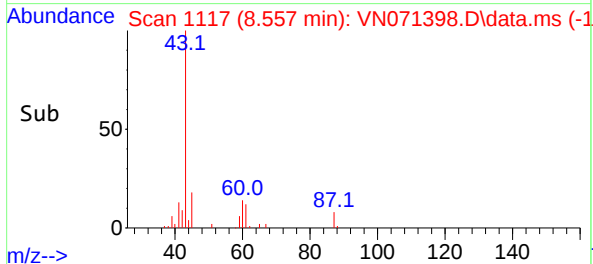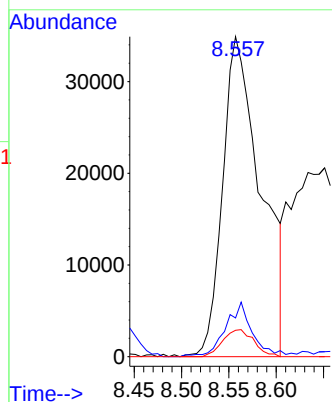

#48
Methyl methacrylate
Concen: 1.697 ug/l
RT: 9.539 min Scan# 1284
Delta R.T. -0.018 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 41 Resp: 21146
Ion Ratio Lower Upper
41 100
69 0.0 72.4 108.6#
39 20.2 58.4 87.6#


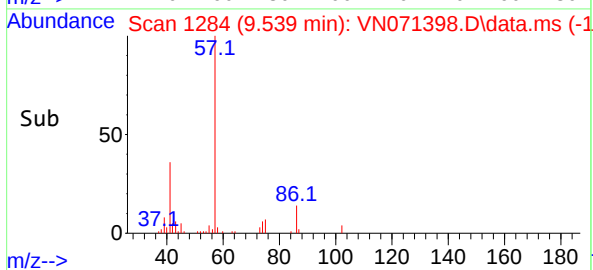

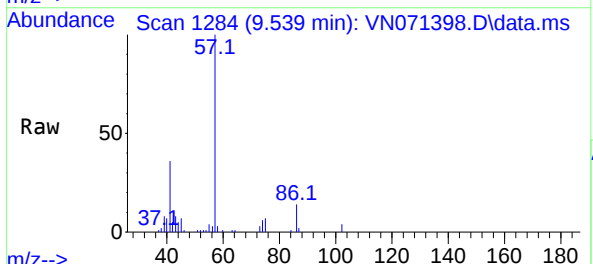


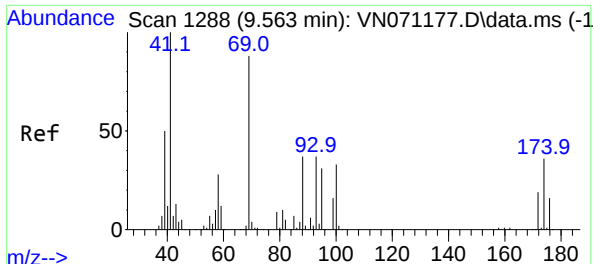

#49
1,4-Dioxane
Concen: 0.573 ug/l
RT: 9.628 min Scan# 11
Delta R.T. 0.065 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion: 88 Resp: 124
Ion Ratio Lower Upper
88 100
43 1650143.5 23.4 35.2#
58 7270.2 50.6 75.8#

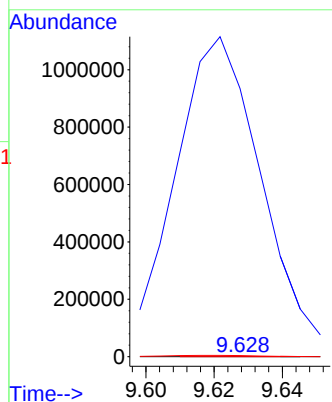

#50
Toluene-d8
Concen: 49.602 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 98 Resp: 1628439
Ion Ratio Lower Upper
98 100
100 65.3 50.4 75.6

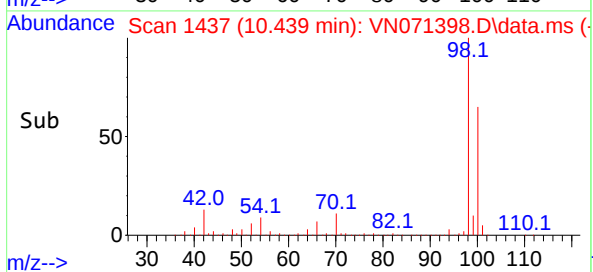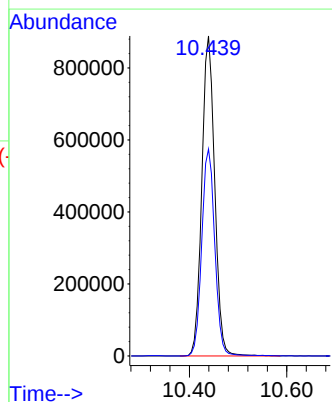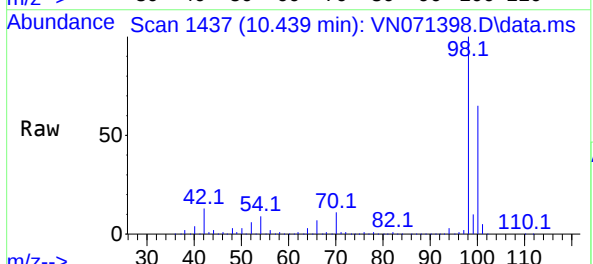



#51

4-Methyl-2-Pentanone

Concen: 0.624 ug/l

RT: 10.328 min Scan# 1418

Delta R.T. 0.001 min

Lab File: VN071398.D

Acq: 19 Mar 2022 15:18

Instrument :

MSVOA_N

ClientSampleId :





C-4-3-4

Tgt Ion: 43 Resp: 10406

Ion Ratio Lower Upper

43 100

58 54.5 30.4 45.6#

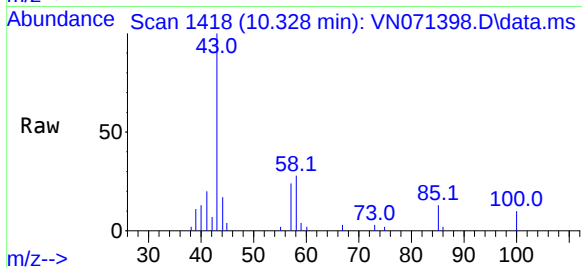

#52

Toluene

Concen: 0.437 ug/l

RT: 10.498 min Scan# 1447

Delta R.T. -0.006 min

Lab File: VN071398.D




Acq: 19 Mar 2022 15:18


Tgt Ion: 92 Resp: 10593

Ion Ratio Lower Upper

92 100

91 190.4 142.0 213.0



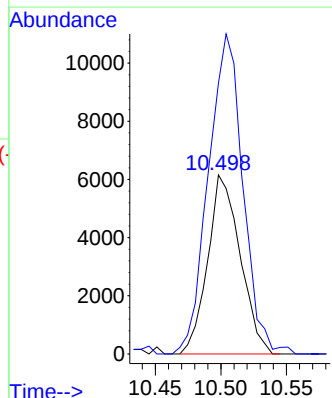
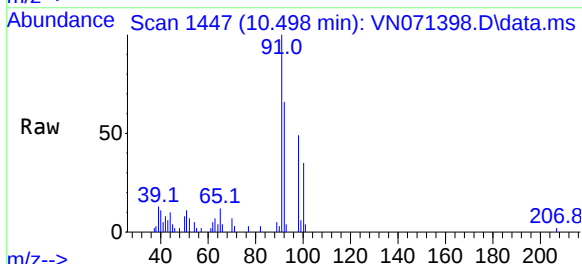




#54
cis-1,3-Dichloropropene
Concen: 6.044 ug/l
RT: 10.239 min Scan# 1403
Delta R.T. 0.053 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion: 75 Resp: 95675
Ion Ratio Lower Upper
75 100
77 0.4 26.4 39.6#
39 29.8 42.5 63.7#

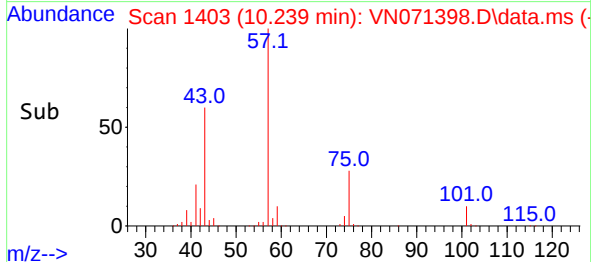

#57
1,3-Dichloropropane
Concen: 2.057 ug/l
RT: 11.086 min Scan# 1547
Delta R.T. 0.047 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 76 Resp: 35857
Ion Ratio Lower Upper
76 100
78 0.2 25.7 38.5#


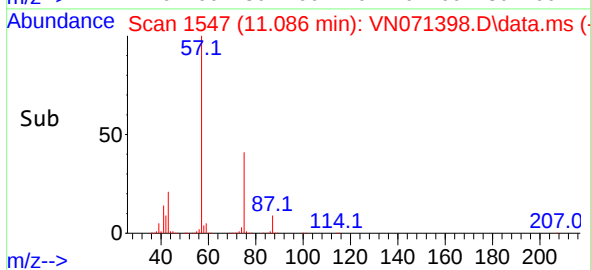






#59
2-Hexanone
Concen: 50.692 ug/l
RT: 11.086 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion: 43 Resp: 577138
Ion Ratio Lower Upper
43 100
58 17.2 26.9 80.7#

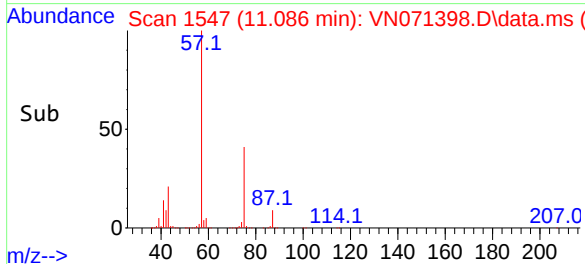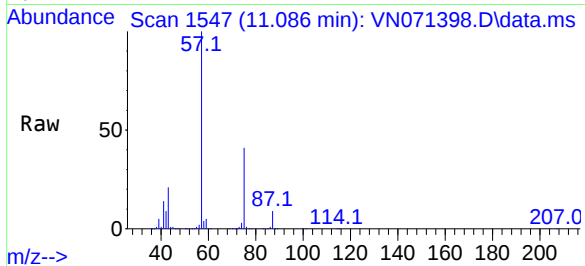

#62
4-Bromofluorobenzene
Concen: 53.412 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 95 Resp: 593778
Ion Ratio Lower Upper
95 100
174 77.5 0.0 187.2
176 75.3 0.0 181.4


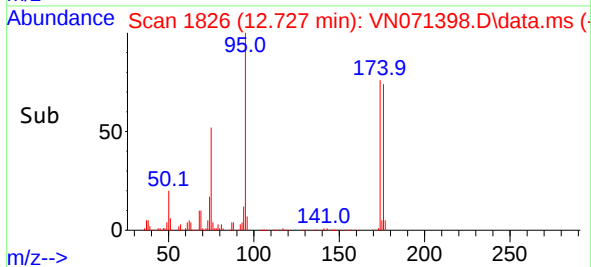

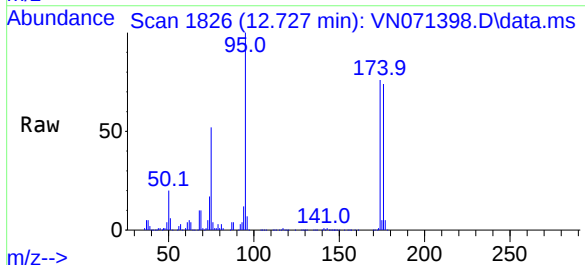




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion:117 Resp: 1243211
Ion Ratio Lower Upper
117 100
82 57.6 42.4 63.6
119 31.6 25.4 38.2

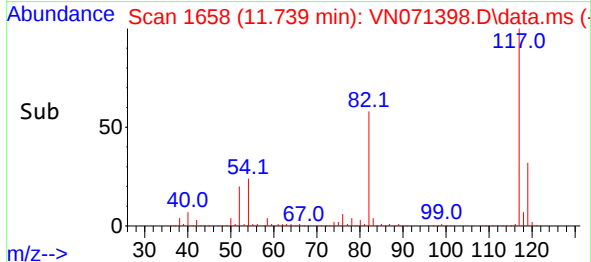

#67
Ethyl Benzene
Concen: 0.630 ug/l
RT: 11.839 min Scan# 1675
Delta R.T. 0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 91 Resp: 29762
Ion Ratio Lower Upper
91 100
106 29.3 25.7 38.5


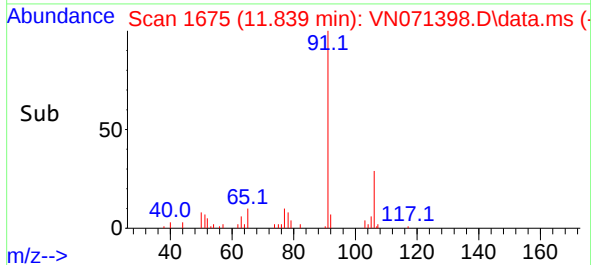

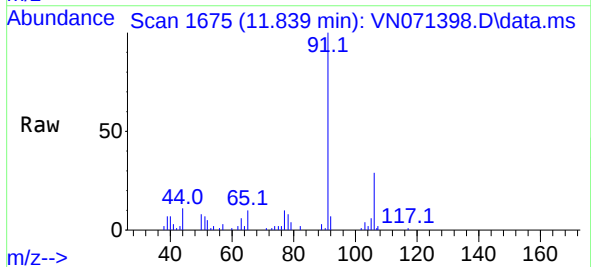




#68
m/p-Xylenes
Concen: 0.595 ug/l
RT: 11.945 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion:106 Resp: 10278
Ion Ratio Lower Upper
106 100
91 207.3 160.6 240.8

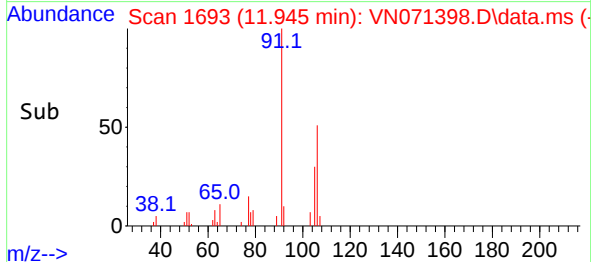

#69
o-Xylene
Concen: 0.432 ug/l
RT: 12.274 min Scan# 1749
Delta R.T. -0.006 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion:106 Resp: 7471
Ion Ratio Lower Upper
106 100
91 221.5 105.8 317.3


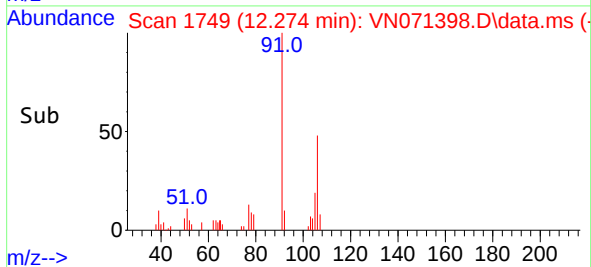

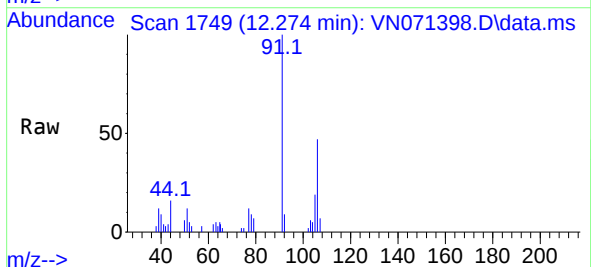




#71
Bromoform
Concen: 0.456 ug/l
RT: 12.727 min Scan# 11
Delta R.T. 0.270 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion:173 Resp: 3388
Ion Ratio Lower Upper
173 100
175 745.0 24.2 72.6#
254 0.0 0.0 0.0

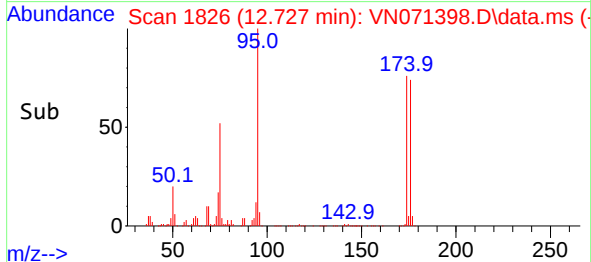

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1987
Delta R.T. 0.006 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion:152 Resp: 428500
Ion Ratio Lower Upper
152 100
115 59.4 27.5 82.5
150 157.4 0.0 344.4



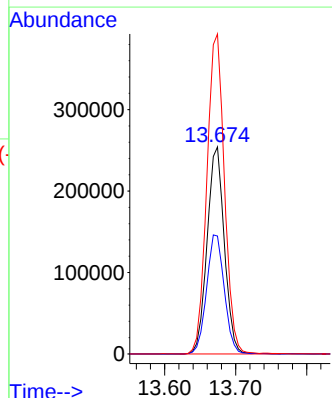





#74
N-amy1 acetate
Concen: 0.211 ug/l
RT: 12.363 min Scan# 11
Delta R.T. -0.023 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18



Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion:	43	Resp:	3282
Ion	Ratio	Lower	Upper
43	100		
70	0.0	33.4	50.0#
55	3.8	19.3	28.9#
61	0.0	18.5	27.7#

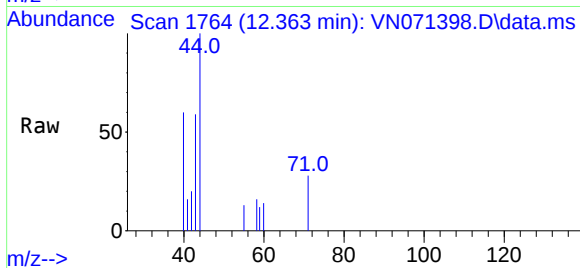

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.722 min Scan# 1825
Delta R.T. -0.099 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion:	83	Resp:	168
Ion	Ratio	Lower	Upper
83	100		
131	432.1	5.5	16.5#
85	0.0	32.4	97.2#



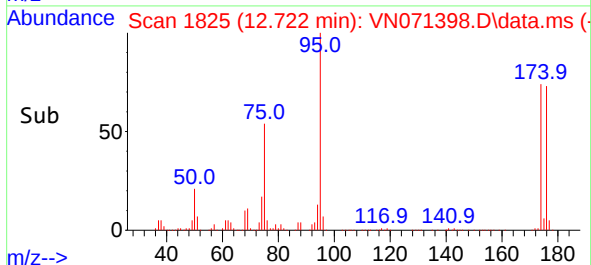
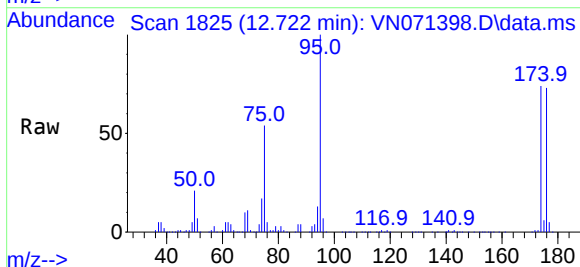




#76
1,2,3-Trichloropropane
Concen: 28.287 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion: 75 Resp: 306502
Ion Ratio Lower Upper
75 100
77 1.2 82.6 247.8#

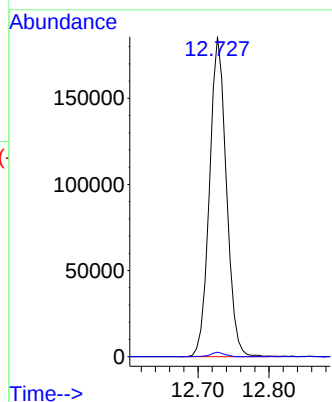

#81
trans-1,4-Dichloro-2-butene
Concen: 77.323 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion: 75 Resp: 306502
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#









#84
1,2,4-Trimethylbenzene
Concen: 0.216 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18




Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4


Tgt Ion:105 Resp: 6650
Ion Ratio Lower Upper
105 100
120 44.6 22.8 68.4

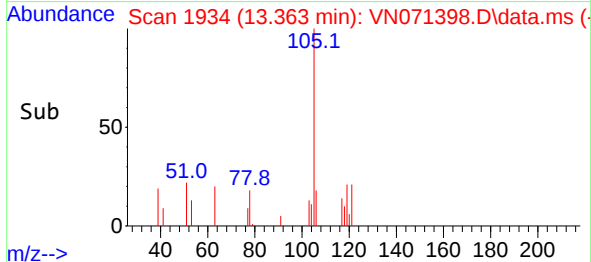

#93
1,2,4-Trichlorobenzene
Concen: 2.997 ug/l
RT: 15.263 min Scan# 2257
Delta R.T. 0.001 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion:180 Resp: 60
Ion Ratio Lower Upper
180 100
182 0.0 48.3 144.9#
145 0.0 14.5 43.5#


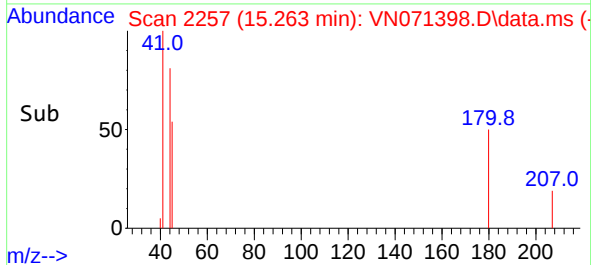

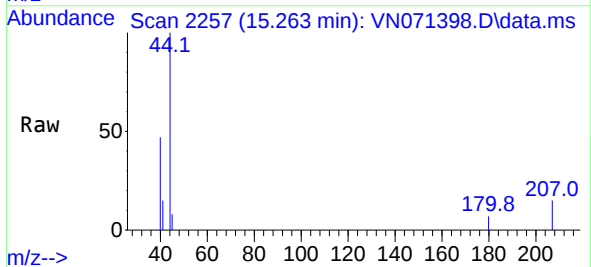


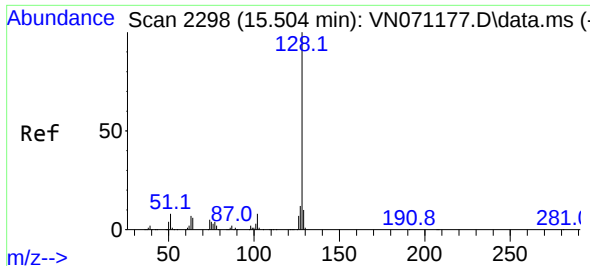

#95
Naphthalene
Concen: 5.790 ug/l
RT: 15.504 min Scan# 2298
Delta R.T. -0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Instrument :
MSVOA_N
ClientSampleId :
C-4-3-4

Tgt Ion:	128	Resp:	15787
Ion	Ratio	Lower	Upper
128	100		
127	14.5	10.5	15.7
129	10.6	8.7	13.1

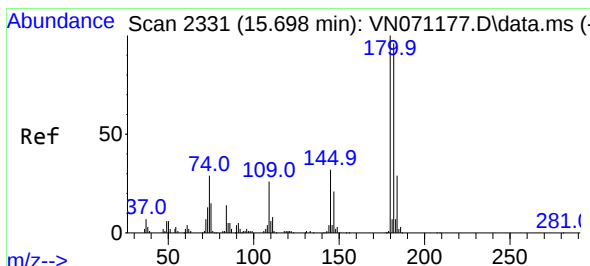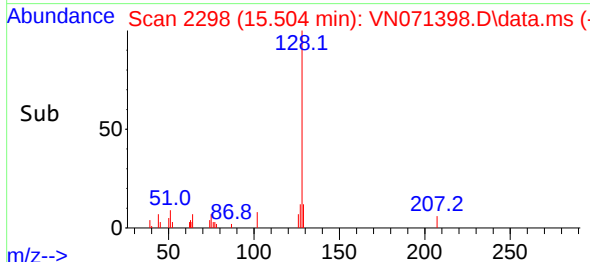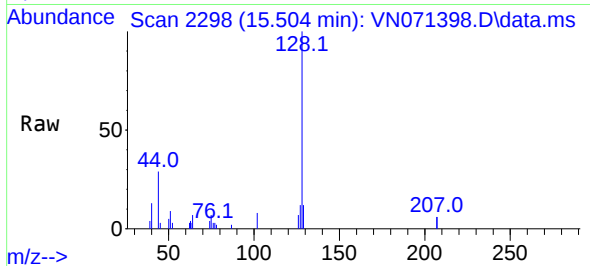

#96
1,2,3-Trichlorobenzene
Concen: 2.748 ug/l
RT: 15.698 min Scan# 2331
Delta R.T. -0.000 min
Lab File: VN071398.D
Acq: 19 Mar 2022 15:18

Tgt Ion:	180	Resp:	116
Ion	Ratio	Lower	Upper
180	100		
182	149.1	47.4	142.2#
145	0.0	15.0	45.1#

