

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031922\
 Data File : VN071400.D
 Acq On : 19 Mar 2022 16:07
 Operator : JC\MD
 Sample : N1958-21
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 C-6-5-6

Quant Time: Mar 21 05:52:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	732299	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1254174	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1210810	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	416082	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	480442	47.870	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	95.740%		
35) Dibromofluoromethane	8.022	113	366654	46.328	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	92.660%		
50) Toluene-d8	10.439	98	1578270	49.530	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	99.060%		
62) 4-Bromofluorobenzene	12.727	95	574679	53.259	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	106.520%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.299	50	3969	0.334	ug/l #	70
5) Bromomethane	2.863	94	644	Below Cal	#	54
16) Acetone	4.293	43	42062	8.613	ug/l	99
18) Methyl Acetate	4.869	43	19566	1.948	ug/l #	90
20) Methylene Chloride	5.093	84	12492	1.771	ug/l #	89
25) 2-Butanone	7.339	43	8419	1.070	ug/l #	77
29) Tetrahydrofuran	7.692	42	1628	0.299	ug/l #	80
31) Cyclohexane	8.086	56	16143	1.007	ug/l #	21
36) 1,1-Dichloropropene	8.081	75	57160	4.508	ug/l #	50
38) Carbon Tetrachloride	8.081	117	73353	5.981	ug/l #	16
40) Benzene	8.457	78	21168	0.554	ug/l	94
43) Isopropyl Acetate	8.563	43	88310	3.384	ug/l #	81
48) Methyl methacrylate	9.539	41	20024	1.656	ug/l #	19
49) 1,4-Dioxane	9.575	88	59	0.281	ug/l #	27
51) 4-Methyl-2-Pentanone	10.333	43	15387	0.950	ug/l	94
52) Toluene	10.498	92	10891	0.463	ug/l	95
54) cis-1,3-Dichloropropene	10.239	75	95253	6.199	ug/l #	60
57) 1,3-Dichloropropane	11.086	76	37700	2.228	ug/l #	43
59) 2-Hexanone	11.086	43	609941	55.195	ug/l #	49
67) Ethyl Benzene	11.845	91	46227	1.005	ug/l	94
68) m/p-Xylenes	11.951	106	16495	0.981	ug/l	98
69) o-Xylene	12.274	106	12459	0.739	ug/l	92
75) 1,1,2,2-Tetrachloroethane	12.739	83	374	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.727	75	295700	28.085	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.057	105	7209	0.231	ug/l	88
81) trans-1,4-Dichloro-2-b...	12.727	75	295700	76.824	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.368	105	10989	0.368	ug/l	94
85) sec-Butylbenzene	13.368	105	10989	0.297	ug/l #	56
93) 1,2,4-Trichlorobenzene	15.257	180	128	3.007	ug/l #	49
95) Naphthalene	15.504	128	35633	6.746	ug/l	98
96) 1,2,3-Trichlorobenzene	15.692	180	73	2.742	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031922\
Data File : VN071400.D
Acq On : 19 Mar 2022 16:07
Operator : JC\MD
Sample : N1958-21
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6

Quant Time: Mar 21 05:52:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration




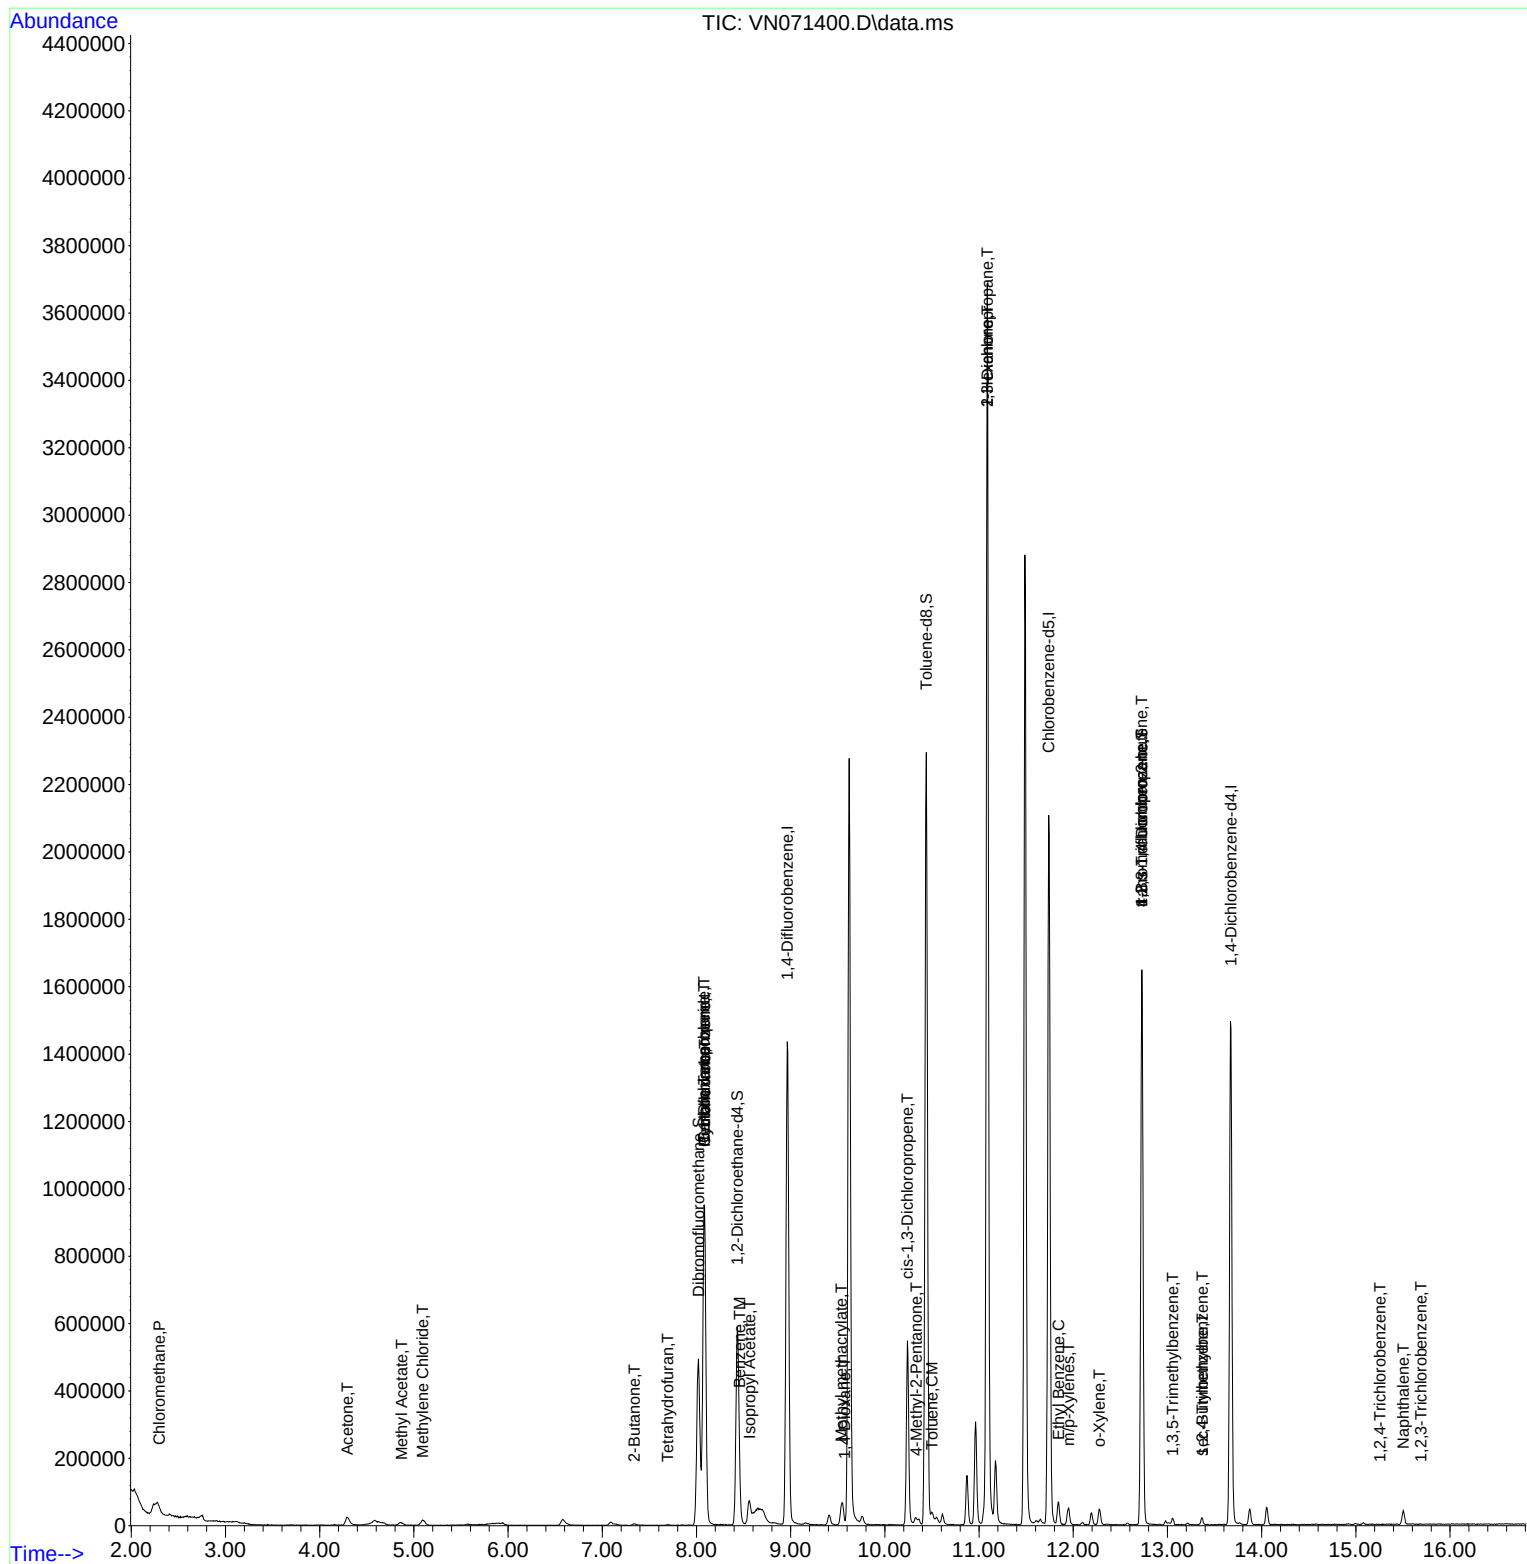




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 10
Delta R.T. 0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion:168 Resp: 732299
Ion Ratio Lower Upper
168 100
99 59.2 41.3 61.9

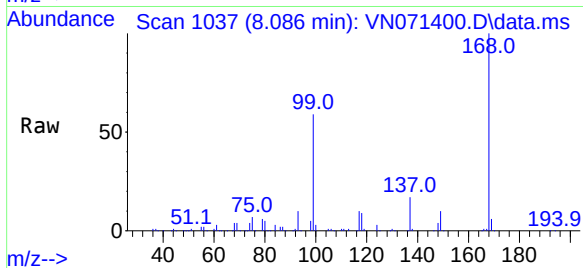

#3
Chloromethane
Concen: 0.334 ug/l
RT: 2.299 min Scan# 53
Delta R.T. -0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 50 Resp: 3969
Ion Ratio Lower Upper
50 100
52 14.9 25.4 38.0#


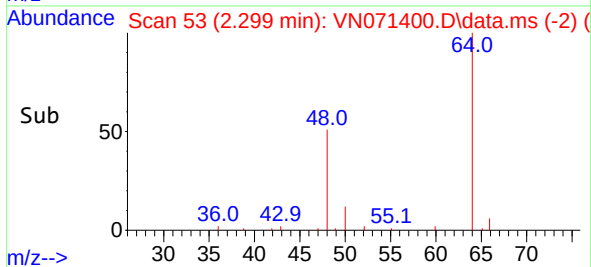

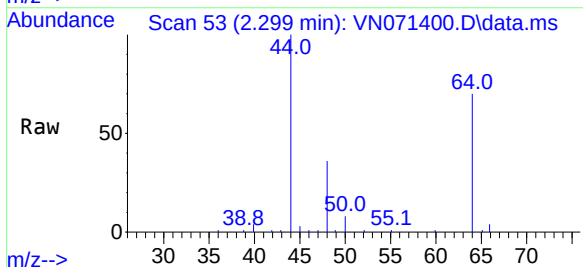




#5
Bromomethane
Concen: Below Cal
RT: 2.863 min Scan# 144
Delta R.T. 0.029 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion: 94 Resp: 644
Ion Ratio Lower Upper
94 100
96 136.2 73.8 110.8#



#16
Acetone
Concen: 8.613 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.006 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 43 Resp: 42062
Ion Ratio Lower Upper
43 100
58 28.5 23.1 34.7


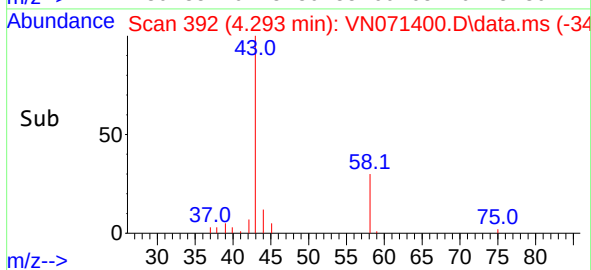






#18
Methyl Acetate
Concen: 1.948 ug/l
RT: 4.869 min Scan# 490
Delta R.T. 0.018 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion: 43 Resp: 19566
Ion Ratio Lower Upper
43 100
74 19.1 19.4 29.2#

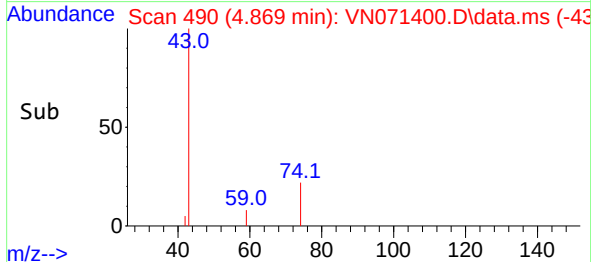

#20
Methylene Chloride
Concen: 1.771 ug/l
RT: 5.093 min Scan# 528
Delta R.T. -0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 84 Resp: 12492
Ion Ratio Lower Upper
84 100
49 125.1 93.5 140.3
51 46.2 29.4 44.2#
86 54.9 53.0 79.4

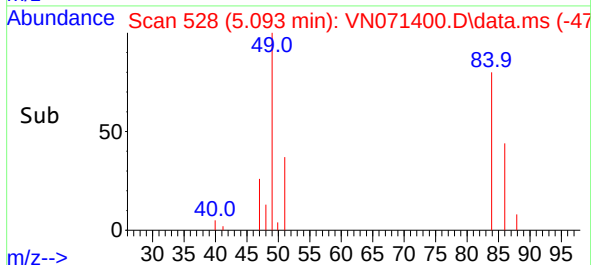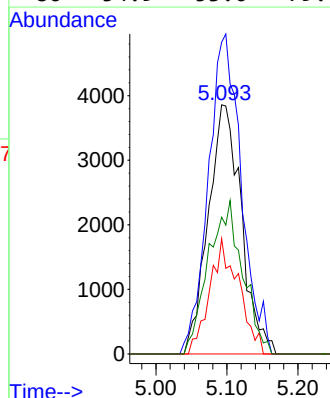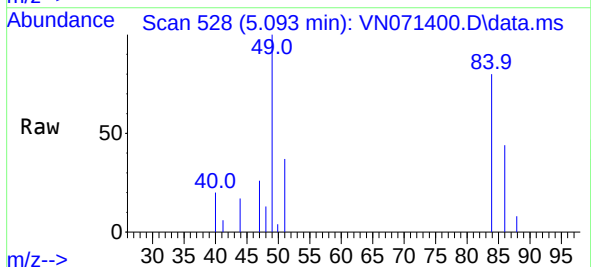



#25

2-Butanone

Concen: 1.070 ug/l

RT: 7.339 min Scan# 910

Delta R.T. 0.006 min

Lab File: VN071400.D

Acq: 19 Mar 2022 16:07

Instrument :

MSVOA_N

ClientSampleId :





C-6-5-6

Tgt Ion: 43 Resp: 8419

Ion Ratio Lower Upper

43 100

72 15.0 21.7 32.5#

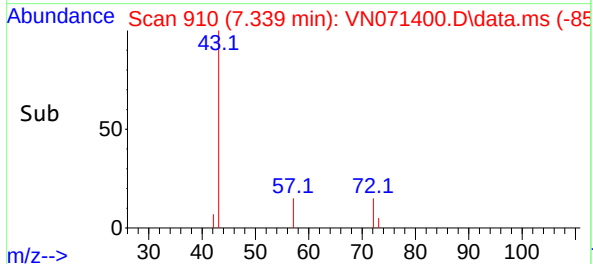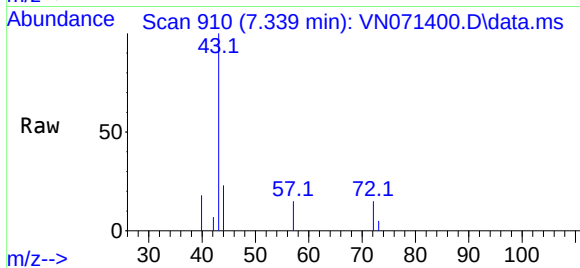

#29

Tetrahydrofuran

Concen: 0.299 ug/l

RT: 7.692 min Scan# 970

Delta R.T. 0.012 min

Lab File: VN071400.D

Acq: 19 Mar 2022 16:07




Tgt Ion: 42 Resp: 1628


Ion Ratio Lower Upper

42 100

72 34.3 36.3 54.5#

71 28.3 34.7 52.1#

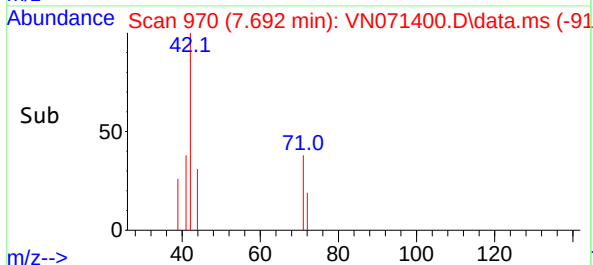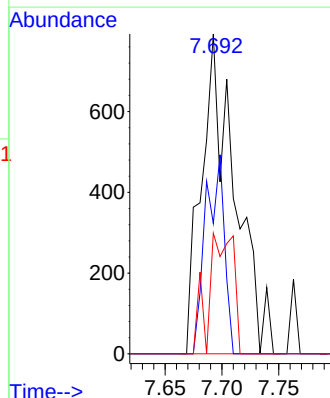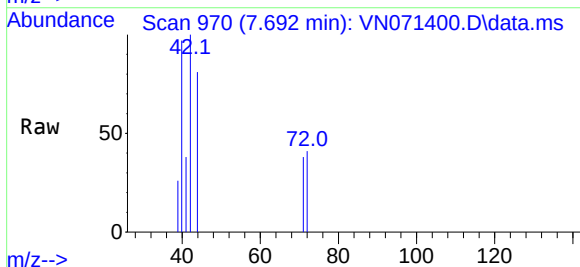



#31

Cyclohexane

Concen: 1.007 ug/l

RT: 8.086 min Scan# 1037

Delta R.T. -0.006 min

Lab File: VN071400.D

Acq: 19 Mar 2022 16:07

Instrument :

MSVOA_N

ClientSampleId :

C-6-5-6





Tgt Ion: 56 Resp: 16143

Ion Ratio Lower Upper

56 100

69 154.3 27.1 40.7#

84 120.0 73.4 110.0#

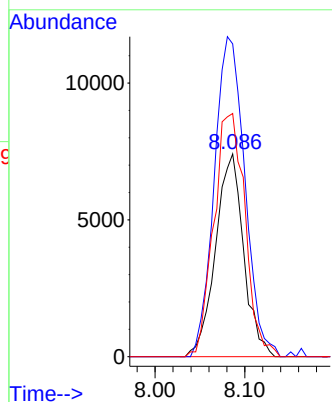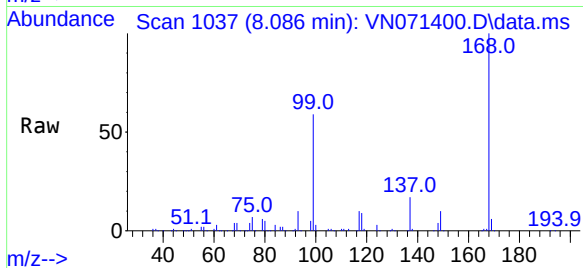

#33

1,2-Dichloroethane-d4

Concen: 47.870 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. -0.006 min

Lab File: VN071400.D




Acq: 19 Mar 2022 16:07


Tgt Ion: 65 Resp: 480442

Ion Ratio Lower Upper

65 100

67 52.4 0.0 103.0


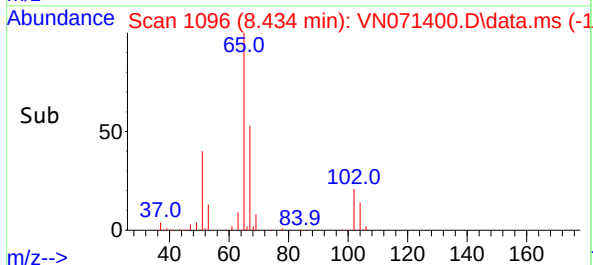

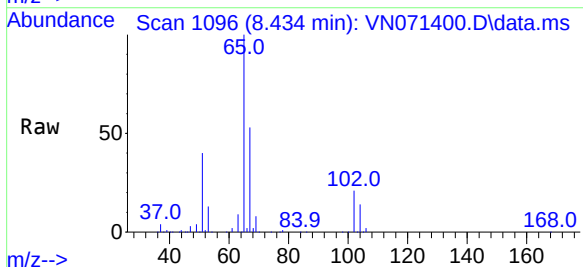


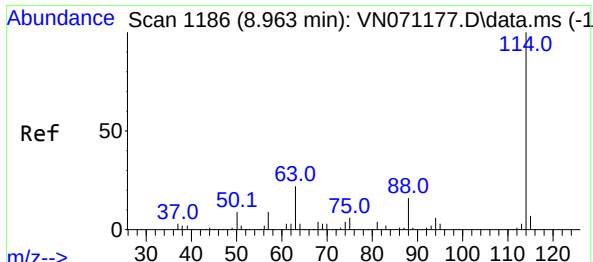

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion:114 Resp: 1254174
Ion Ratio Lower Upper
114 100
63 22.6 0.0 37.8
88 16.0 0.0 27.4

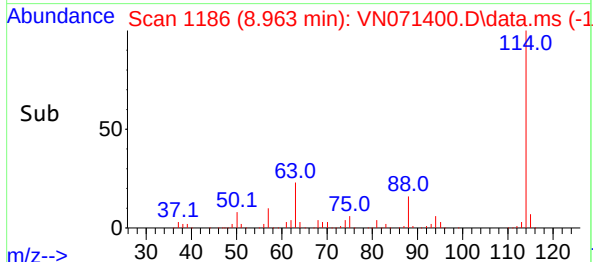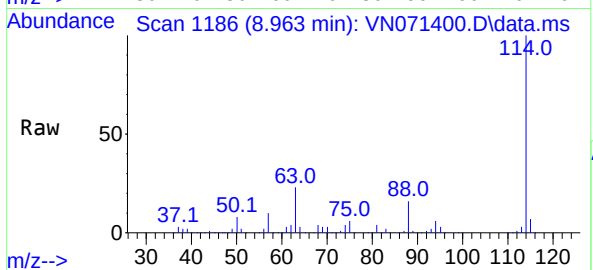

#35
Dibromofluoromethane
Concen: 46.328 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion:113 Resp: 366654
Ion Ratio Lower Upper
113 100
111 102.1 82.2 123.2
192 19.9 16.9 25.3


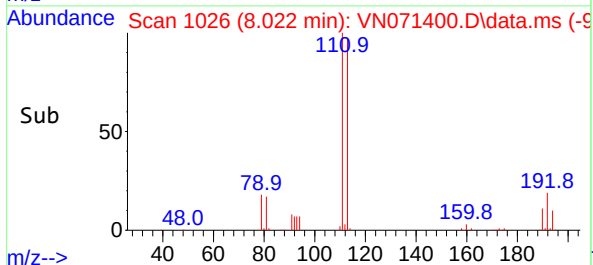

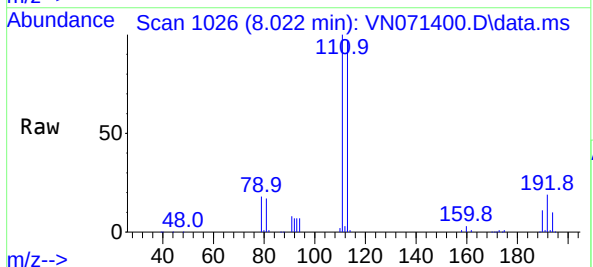




#36
1,1-Dichloropropene
Concen: 4.508 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.135 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion: 75 Resp: 57160
Ion Ratio Lower Upper
75 100
110 9.6 18.4 55.2#
77 0.0 24.4 36.6#

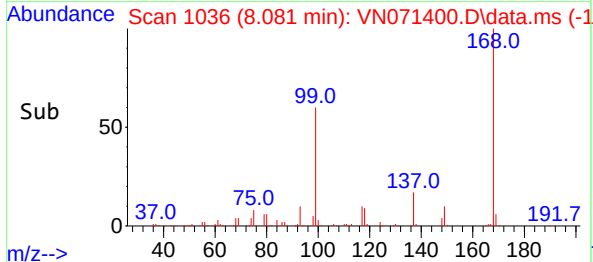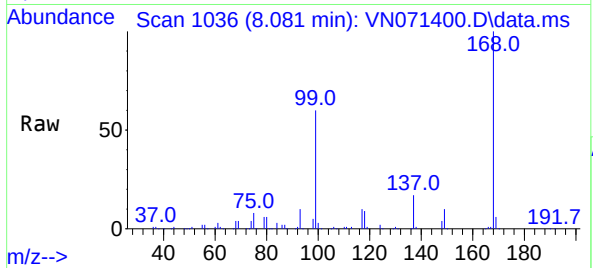

#38
Carbon Tetrachloride
Concen: 5.981 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.123 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 117 Resp: 73353
Ion Ratio Lower Upper
117 100
119 5.3 76.1 114.1#
121 0.0 24.2 36.2#


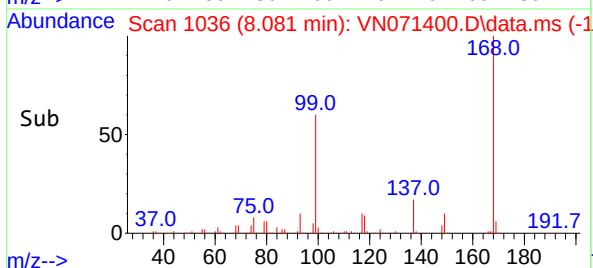
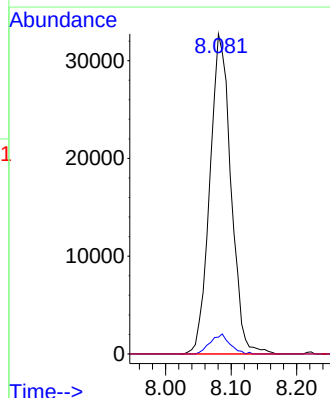
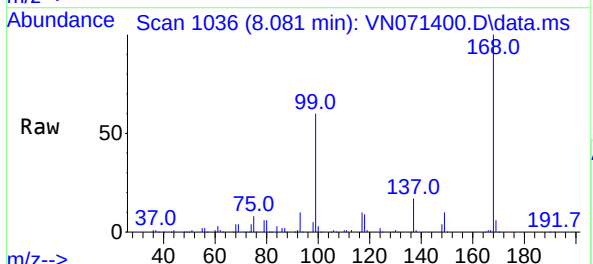




#40
Benzene
Concen: 0.554 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. 0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion: 78 Resp: 21168
Ion Ratio Lower Upper
78 100
77 20.1 18.6 27.8

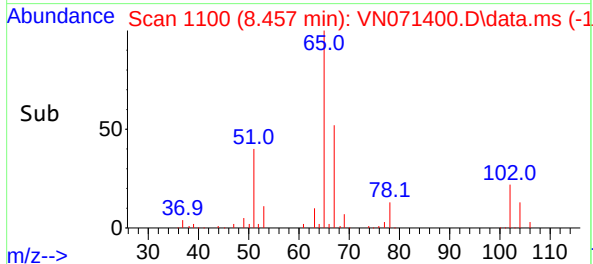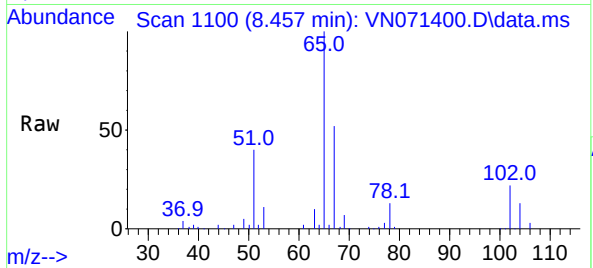

#43
Isopropyl Acetate
Concen: 3.384 ug/l
RT: 8.563 min Scan# 1118
Delta R.T. 0.006 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 43 Resp: 88310
Ion Ratio Lower Upper
43 100
61 14.8 20.4 30.6#
87 7.7 11.2 16.8#

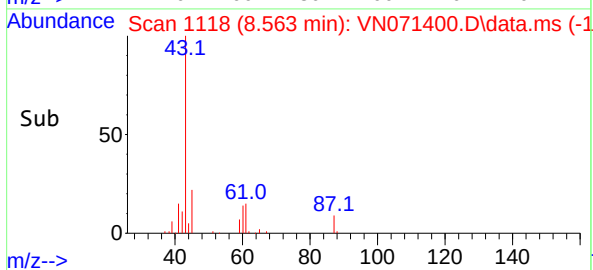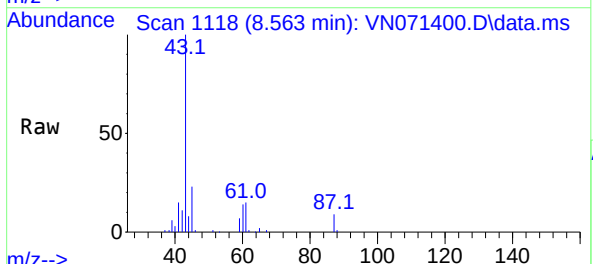

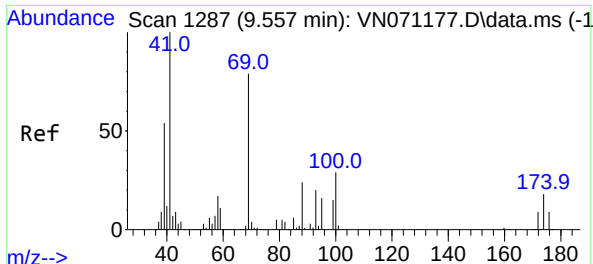

#48

Methyl methacrylate

Concen: 1.656 ug/l

RT: 9.539 min Scan# 11

Delta R.T. -0.018 min

Lab File: VN071400.D

Acq: 19 Mar 2022 16:07

Instrument :

MSVOA_N

ClientSampleId :

C-6-5-6


Tgt Ion: 41 Resp: 20024

Ion Ratio Lower Upper




41 100

69 0.0 72.4 108.6#

39 19.7 58.4 87.6#

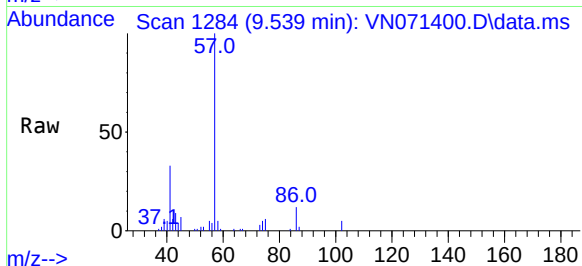

Abundance

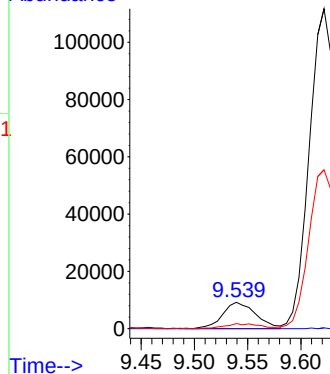

#49

1,4-Dioxane

Concen: 0.281 ug/l

RT: 9.575 min Scan# 1290

Delta R.T. 0.012 min

Lab File: VN071400.D

Acq: 19 Mar 2022 16:07


Tgt Ion: 88 Resp: 59

Ion Ratio Lower Upper



88 100


43 0.0 23.4 35.2#

58 0.0 50.6 75.8#

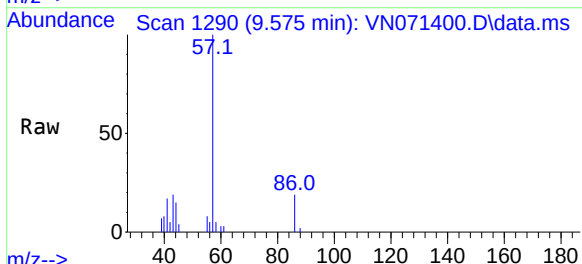

Abundance



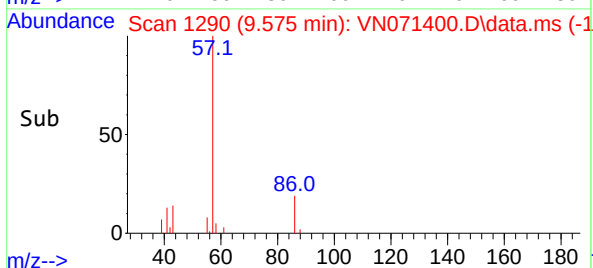
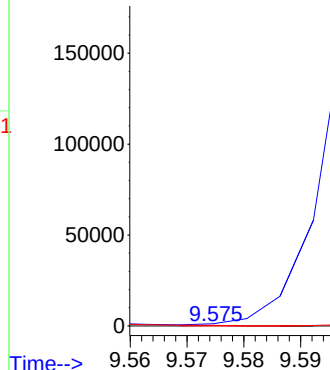




#50
Toluene-d8
Concen: 49.530 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion: 98 Resp: 1578270
Ion Ratio Lower Upper
98 100
100 65.7 50.4 75.6

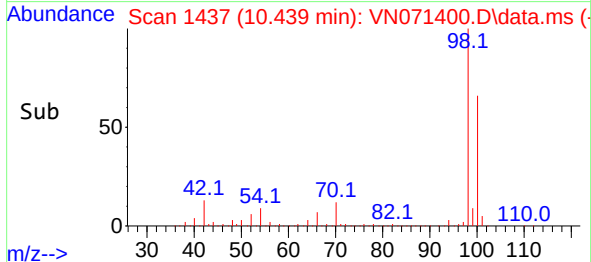

#51
4-Methyl-2-Pentanone
Concen: 0.950 ug/l
RT: 10.333 min Scan# 1419
Delta R.T. 0.006 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 43 Resp: 15387
Ion Ratio Lower Upper
43 100
58 34.2 30.4 45.6


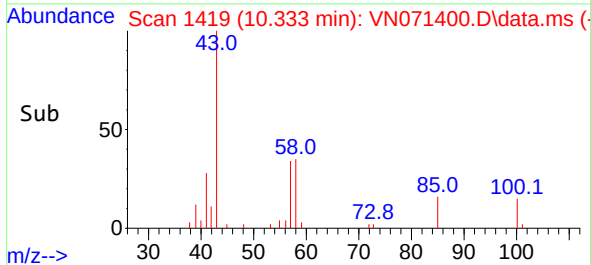

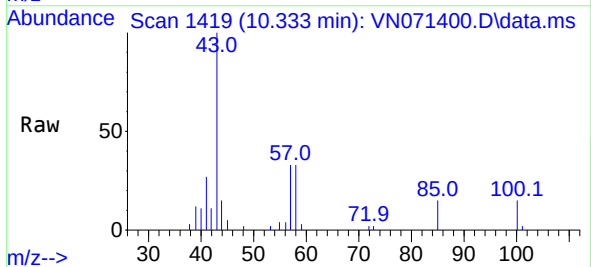




#52
Toluene
Concen: 0.463 ug/l
RT: 10.498 min Scan# 1447
Delta R.T. -0.006 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion: 92 Resp: 10891
Ion Ratio Lower Upper
92 100
91 170.2 142.0 213.0



#54
cis-1,3-Dichloropropene
Concen: 6.199 ug/l
RT: 10.239 min Scan# 1403
Delta R.T. 0.053 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 75 Resp: 95253
Ion Ratio Lower Upper
75 100
77 0.6 26.4 39.6#
39 31.9 42.5 63.7#


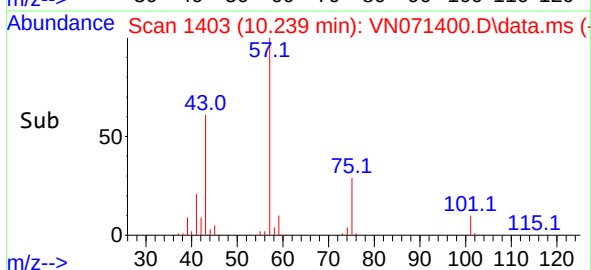






#57
1,3-Dichloropropane
Concen: 2.228 ug/l
RT: 11.086 min Scan# 1547
Delta R.T. 0.047 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion: 76 Resp: 37700
Ion Ratio Lower Upper
76 100
78 0.0 25.7 38.5#



#59
2-Hexanone
Concen: 55.195 ug/l
RT: 11.086 min Scan# 1547
Delta R.T. 0.006 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 43 Resp: 609941
Ion Ratio Lower Upper
43 100
58 17.0 26.9 80.7#


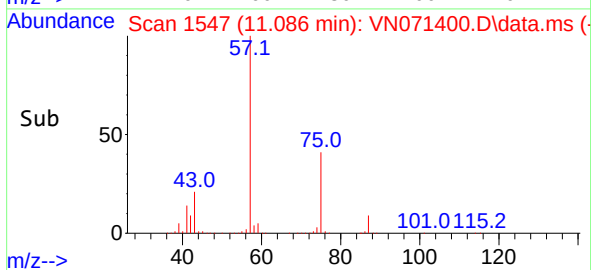






#62
4-Bromofluorobenzene
Concen: 53.259 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion: 95 Resp: 574679
Ion Ratio Lower Upper
95 100
174 77.8 0.0 187.2
176 74.1 0.0 181.4

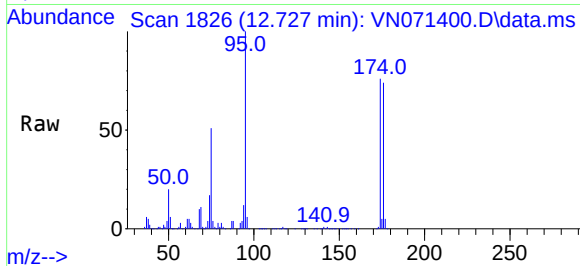

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 117 Resp: 1210810
Ion Ratio Lower Upper
117 100
82 58.2 42.4 63.6
119 31.9 25.4 38.2


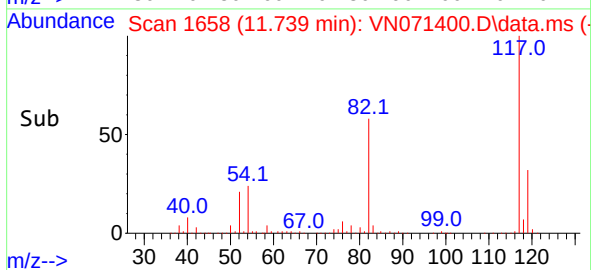

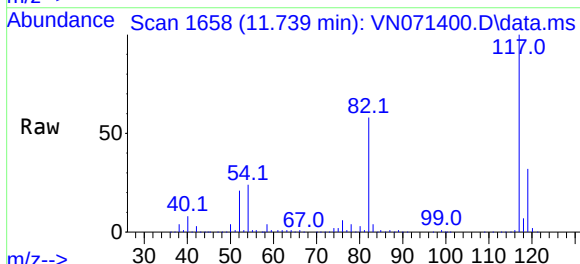




#67
Ethyl Benzene
Concen: 1.005 ug/l
RT: 11.845 min Scan# 1675
Delta R.T. 0.006 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion: 91 Resp: 46227
Ion Ratio Lower Upper
91 100
106 28.7 25.7 38.5

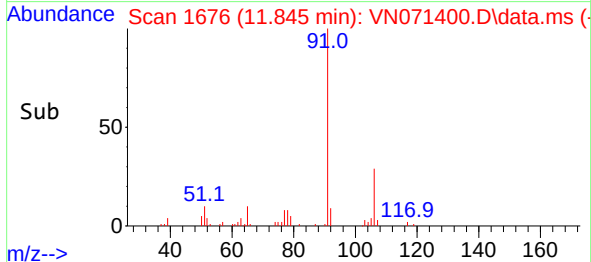

#68
m/p-Xylenes
Concen: 0.981 ug/l
RT: 11.951 min Scan# 1694
Delta R.T. -0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 106 Resp: 16495
Ion Ratio Lower Upper
106 100
91 197.4 160.6 240.8


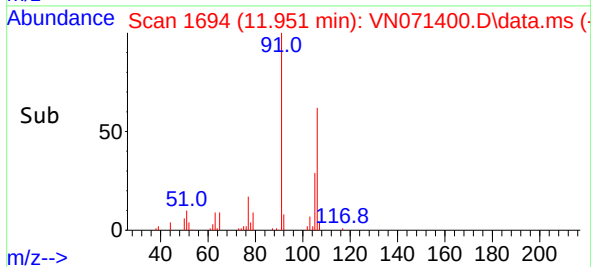

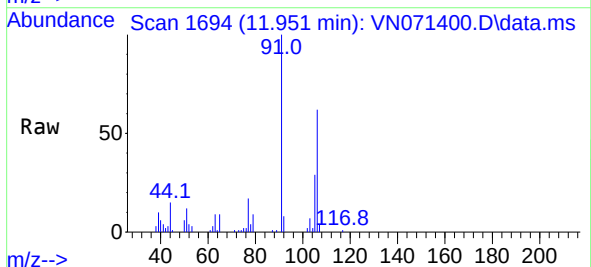




#69
o-Xylene
Concen: 0.739 ug/l
RT: 12.274 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion:106 Resp: 12459
Ion Ratio Lower Upper
106 100
91 223.3 105.8 317.3



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1987
Delta R.T. 0.006 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion:152 Resp: 416082
Ion Ratio Lower Upper
152 100
115 59.6 27.5 82.5
150 157.1 0.0 344.4


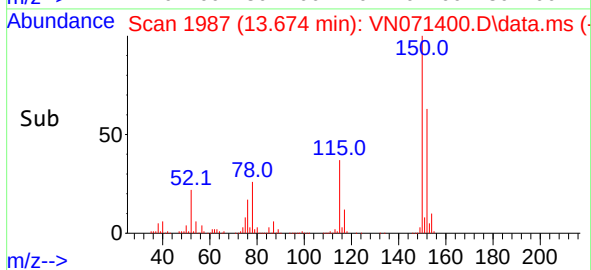

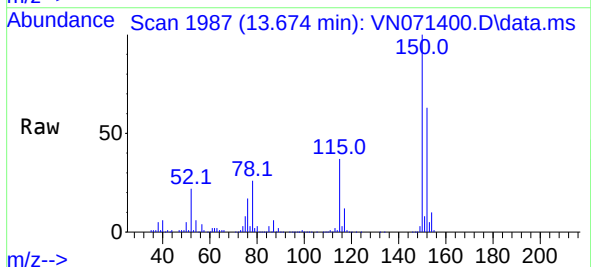




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.739 min Scan# 1828
Delta R.T. -0.082 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion: 83 Resp: 374
Ion Ratio Lower Upper
83 100
131 222.5 5.5 16.5#
85 0.0 32.4 97.2#



#76
1,2,3-Trichloropropane
Concen: 28.085 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 75 Resp: 295700
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#


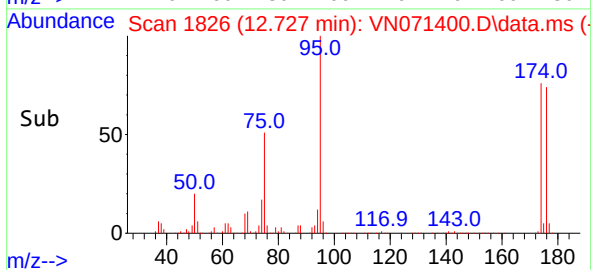






#80
1,3,5-Trimethylbenzene
Concen: 0.231 ug/l
RT: 13.057 min Scan# 1882
Delta R.T. 0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion:105 Resp: 7209
Ion Ratio Lower Upper
105 100
120 41.0 24.6 73.6

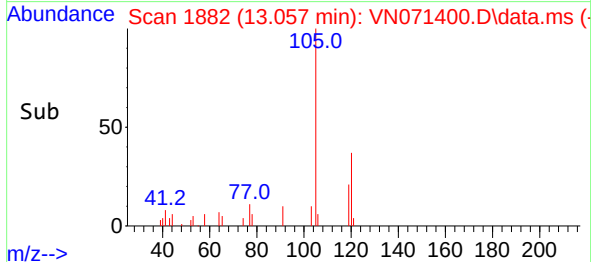

#81
trans-1,4-Dichloro-2-butene
Concen: 76.824 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion: 75 Resp: 295700
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#


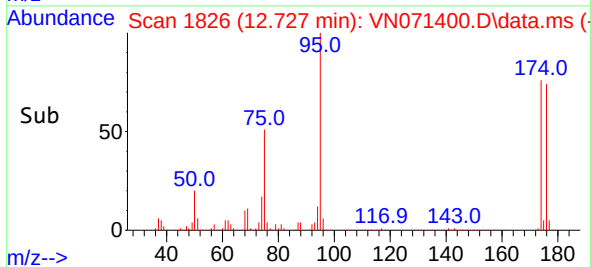

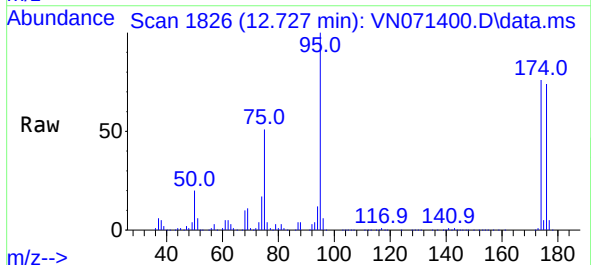




#84
1,2,4-Trimethylbenzene
Concen: 0.368 ug/l
RT: 13.368 min Scan# 1934
Delta R.T. 0.005 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion:105 Resp: 10989
Ion Ratio Lower Upper
105 100
120 49.7 22.8 68.4

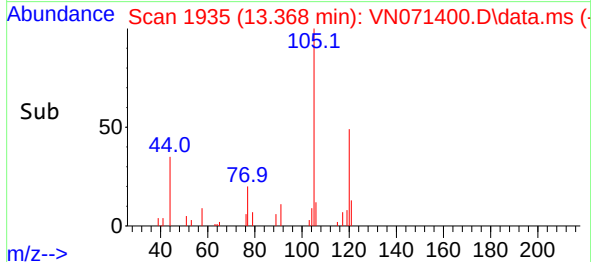

#85
sec-Butylbenzene
Concen: 0.297 ug/l
RT: 13.368 min Scan# 1935
Delta R.T. -0.129 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion:105 Resp: 10989
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#


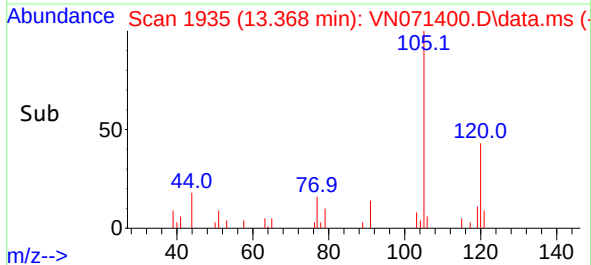

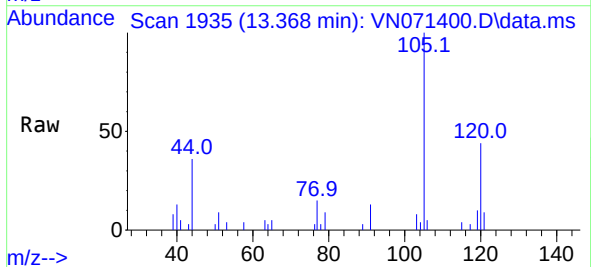




#93
1,2,4-Trichlorobenzene
Concen: 3.007 ug/l
RT: 15.257 min Scan# 21
Delta R.T. -0.005 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07




Instrument :
MSVOA_N
ClientSampleId :
C-6-5-6


Tgt Ion:180 Resp: 128
Ion Ratio Lower Upper
180 100
182 47.7 48.3 144.9#
145 0.0 14.5 43.5#



#95
Naphthalene
Concen: 6.746 ug/l
RT: 15.504 min Scan# 2298
Delta R.T. -0.000 min
Lab File: VN071400.D
Acq: 19 Mar 2022 16:07

Tgt Ion:128 Resp: 35633
Ion Ratio Lower Upper
128 100
127 13.0 10.5 15.7
129 12.1 8.7 13.1

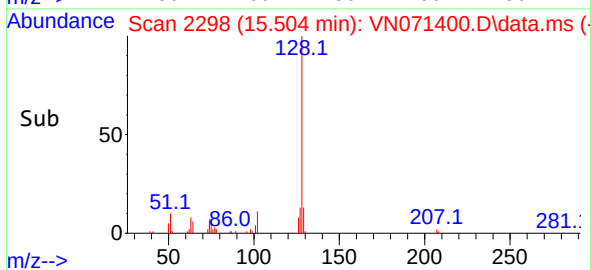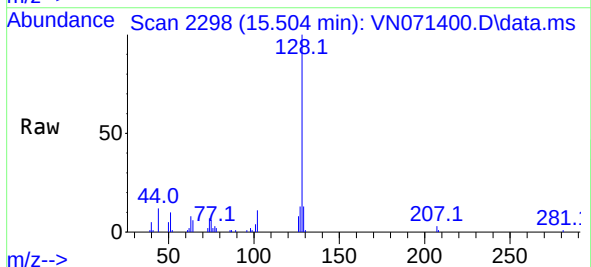



#96

1,2,3-Trichlorobenzene

Concen: 2.742 ug/l

RT: 15.692 min Scan# 21

Delta R.T. -0.006 min

Lab File: VN071400.D


Acq: 19 Mar 2022 16:07

Instrument :

MSVOA_N

ClientSampleId :

C-6-5-6

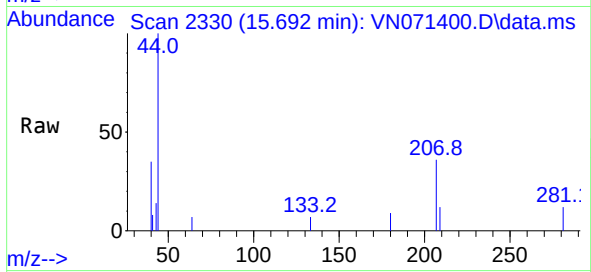

Tgt Ion:180 Resp: 73

Ion Ratio Lower Upper

180 100

182 0.0 47.4 142.2#

145 0.0 15.0 45.1#

