

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031922\
 Data File : VN071403.D
 Acq On : 19 Mar 2022 17:19
 Operator : JC\MD
 Sample : N1958-25
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 C-10-9-10

Quant Time: Mar 21 05:53:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	726945	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1234605	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1188735	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	421932	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	487630	48.944	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	97.880%		
35) Dibromofluoromethane	8.016	113	362386	46.515	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	93.020%		
50) Toluene-d8	10.439	98	1546543	49.303	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	98.600%		
62) 4-Bromofluorobenzene	12.727	95	561549	52.867	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	105.740%		
Target Compounds					Qvalue	
3) Chloromethane	2.293	50	4402	0.377	ug/l	94
5) Bromomethane	2.857	94	515	Below Cal		93
6) Chloroethane	2.999	64	1809	0.306	ug/l #	42
13) Acrolein	4.040	56	463	0.223	ug/l #	32
16) Acetone	4.293	43	58922	12.155	ug/l	95
18) Methyl Acetate	4.851	43	17935	1.835	ug/l	98
20) Methylene Chloride	5.093	84	10156	1.519	ug/l #	84
25) 2-Butanone	7.340	43	9579	1.227	ug/l	95
29) Tetrahydrofuran	7.698	42	1767	0.327	ug/l #	66
31) Cyclohexane	8.081	56	15640	0.983	ug/l #	1
36) 1,1-Dichloropropene	8.087	75	57870	4.636	ug/l #	48
38) Carbon Tetrachloride	8.087	117	72336	5.991	ug/l #	16
40) Benzene	8.457	78	36528	0.971	ug/l	99
43) Isopropyl Acetate	8.557	43	60682	2.362	ug/l #	80
48) Methyl methacrylate	9.551	41	6286	0.528	ug/l #	27
51) 4-Methyl-2-Pentanone	10.328	43	10663	0.669	ug/l #	83
54) cis-1,3-Dichloropropene	10.239	75	70421	4.656	ug/l #	64
57) 1,3-Dichloropropane	11.086	76	14527	0.872	ug/l #	43
59) 2-Hexanone	11.086	43	268182	24.653	ug/l #	47
67) Ethyl Benzene	11.845	91	58073	1.287	ug/l	90
68) m/p-Xylenes	11.951	106	20709	1.254	ug/l	99
69) o-Xylene	12.280	106	6399	0.387	ug/l	99
71) Bromoform	12.722	173	3489	0.491	ug/l #	29
75) 1,1,2,2-Tetrachloroethane	12.733	83	572	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.727	75	291356	27.204	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.051	105	7319	0.231	ug/l	92
81) trans-1,4-Dichloro-2-b...	12.727	75	291356	74.646	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.363	105	14279	0.471	ug/l	97
85) sec-Butylbenzene	13.363	105	14279	0.380	ug/l #	56
95) Naphthalene	15.504	128	28067	6.372	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031922\
Data File : VN071403.D
Acq On : 19 Mar 2022 17:19
Operator : JC\MD
Sample : N1958-25
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10

Quant Time: Mar 21 05:53:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration




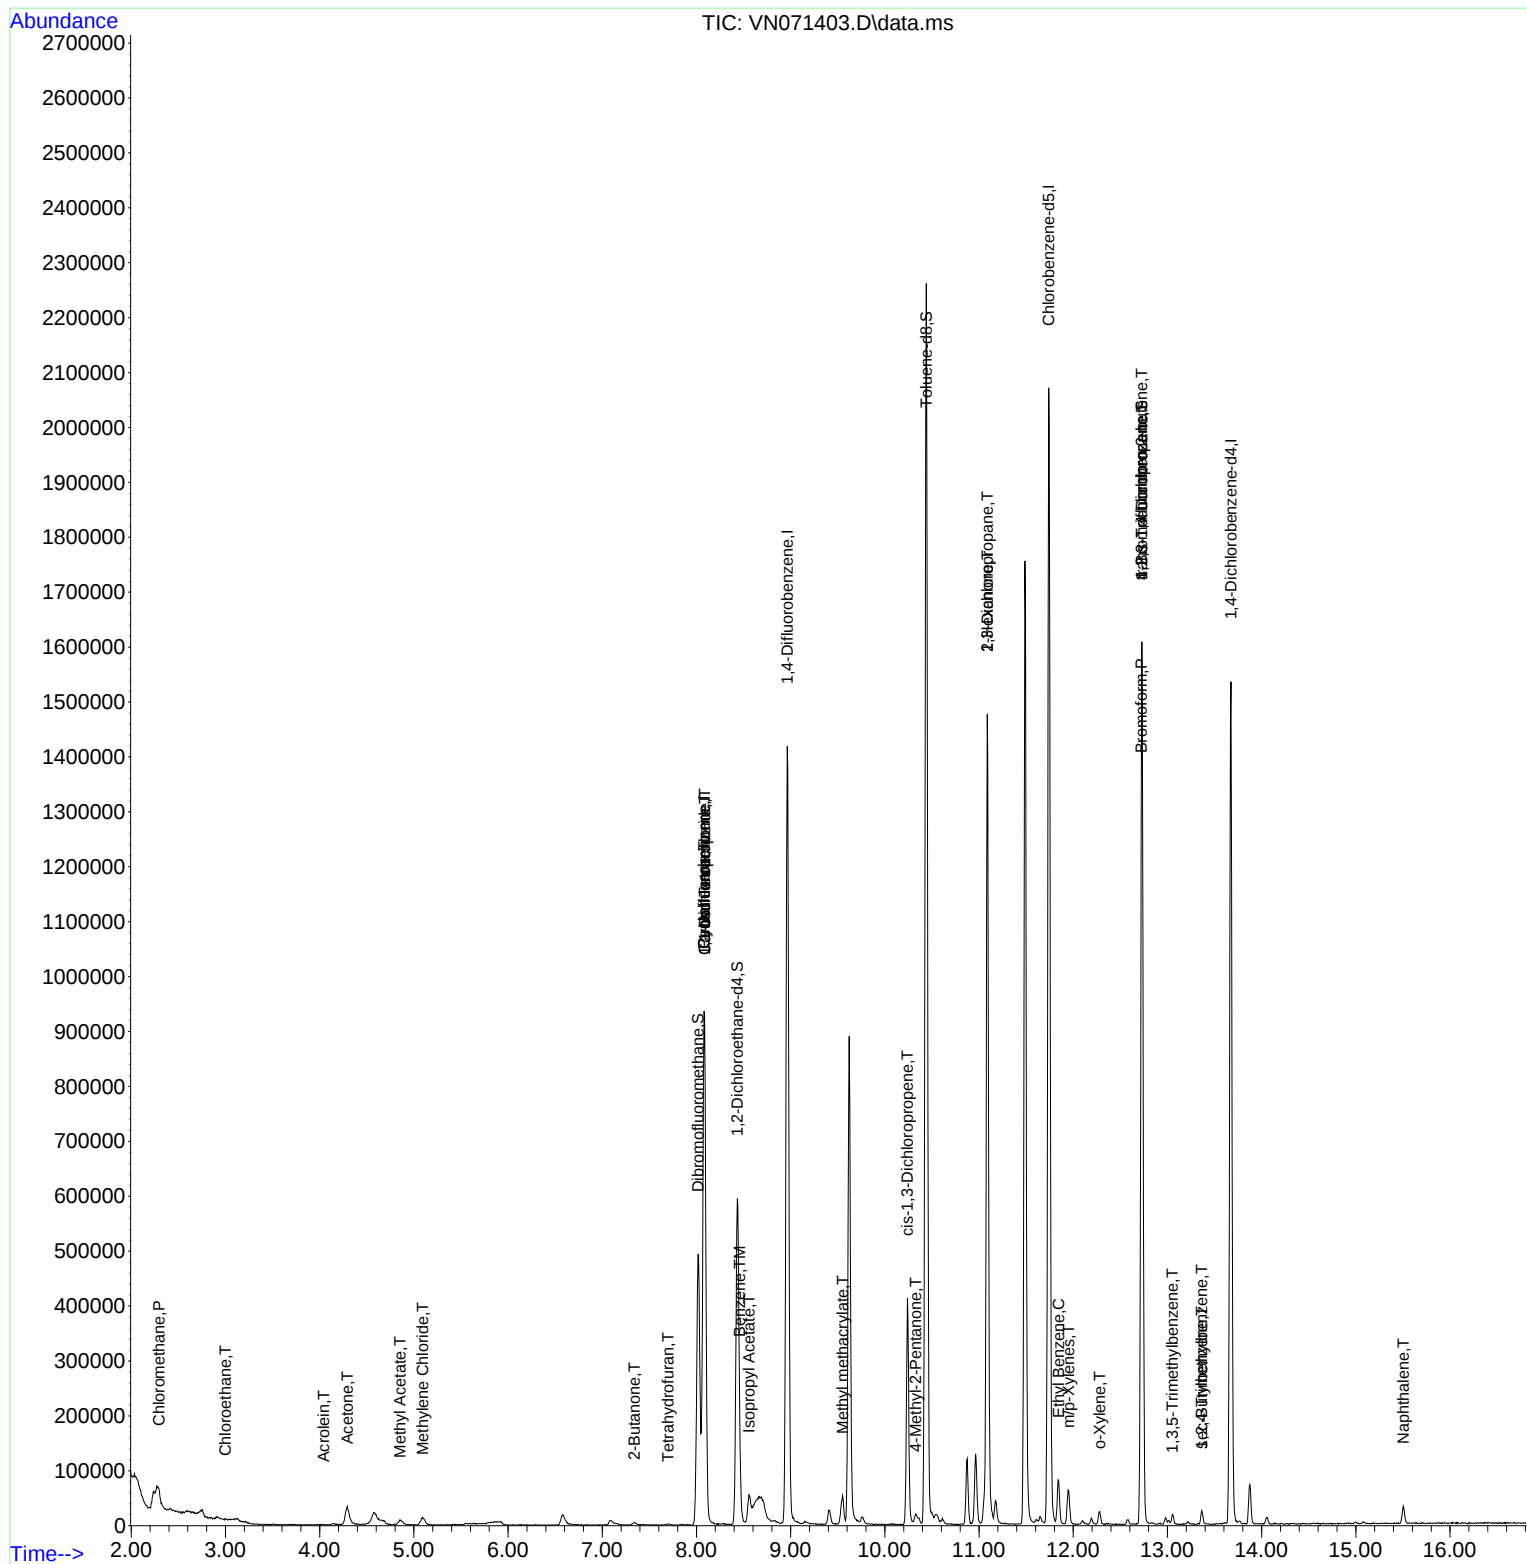




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 10
Delta R.T. -0.005 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion:168 Resp: 726945
Ion Ratio Lower Upper
168 100
99 58.0 41.3 61.9

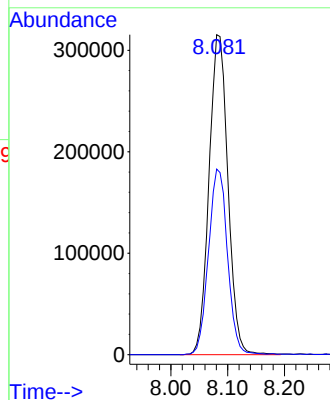

#3
Chloromethane
Concen: 0.377 ug/l
RT: 2.293 min Scan# 52
Delta R.T. -0.006 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 50 Resp: 4402
Ion Ratio Lower Upper
50 100
52 28.3 25.4 38.0



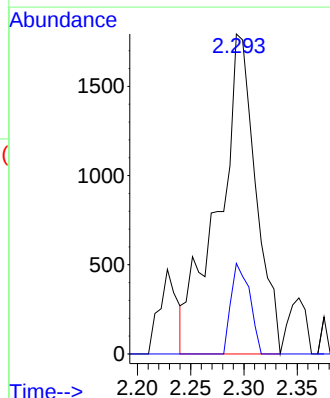





#5
Bromomethane
Concen: Below Cal
RT: 2.857 min Scan# 144
Delta R.T. 0.023 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion: 94 Resp: 515
Ion Ratio Lower Upper
94 100
96 99.1 73.8 110.8

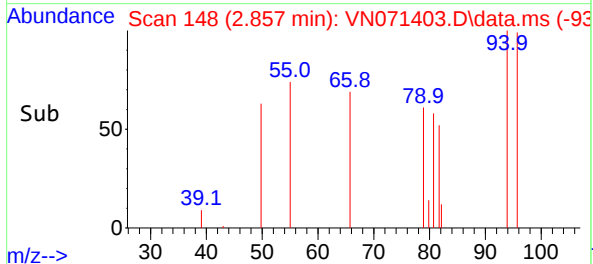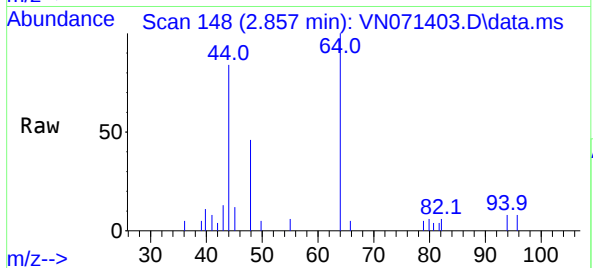

#6
Chloroethane
Concen: 0.306 ug/l
RT: 2.999 min Scan# 172
Delta R.T. -0.005 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 64 Resp: 1809
Ion Ratio Lower Upper
64 100
66 0.0 26.3 39.5#


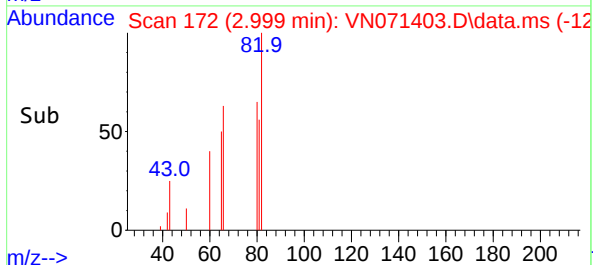

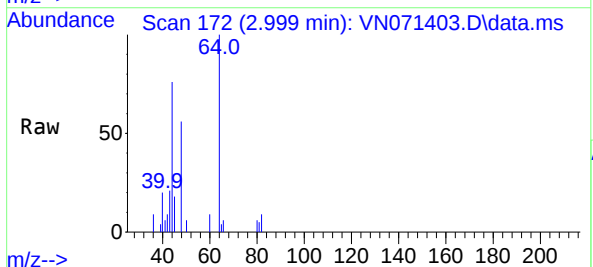




#13
Acrolein
Concen: 0.223 ug/l
RT: 4.040 min Scan# 349
Delta R.T. 0.000 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion: 56 Resp: 463
Ion Ratio Lower Upper
56 100
55 14.3 56.6 85.0#

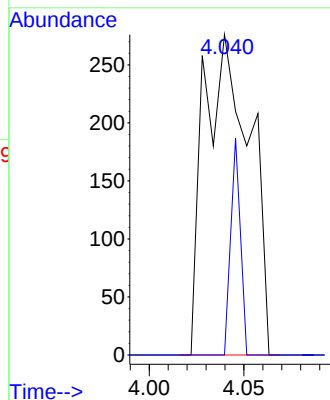

#16
Acetone
Concen: 12.155 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.006 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 43 Resp: 58922
Ion Ratio Lower Upper
43 100
58 31.5 23.1 34.7


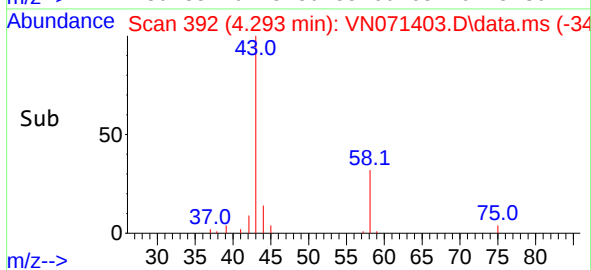
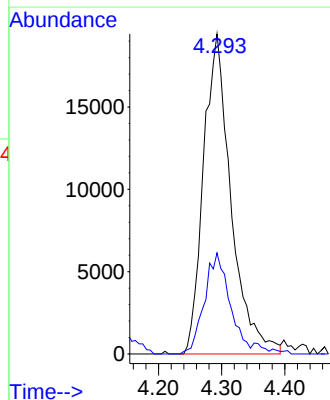





#18
Methyl Acetate
Concen: 1.835 ug/l
RT: 4.851 min Scan# 487
Delta R.T. 0.000 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion: 43 Resp: 17935
Ion Ratio Lower Upper
43 100
74 23.2 19.4 29.2

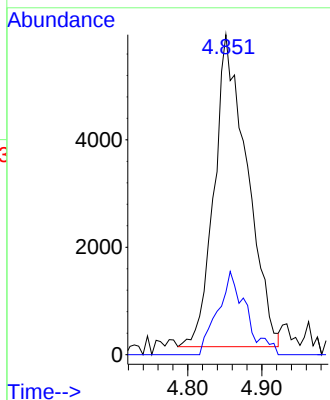

#20
Methylene Chloride
Concen: 1.519 ug/l
RT: 5.093 min Scan# 528
Delta R.T. -0.000 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 84 Resp: 10156
Ion Ratio Lower Upper
84 100
49 146.6 93.5 140.3#
51 36.1 29.4 44.2
86 62.8 53.0 79.4


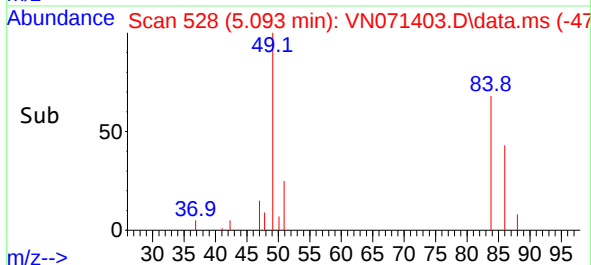
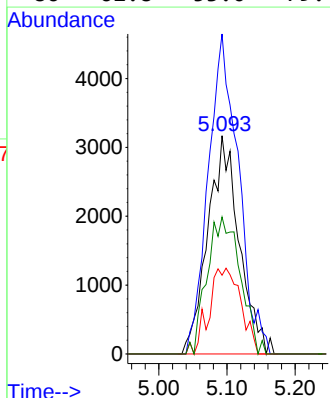
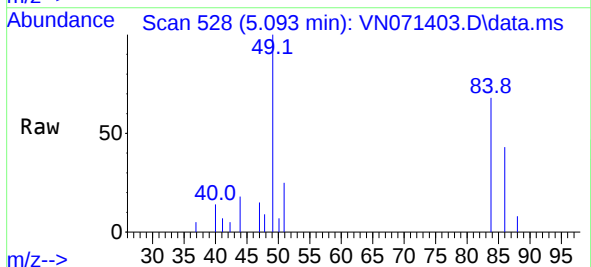




#25
2-Butanone
Concen: 1.227 ug/l
RT: 7.340 min Scan# 910
Delta R.T. 0.006 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion: 43 Resp: 9579
Ion Ratio Lower Upper
43 100
72 24.4 21.7 32.5

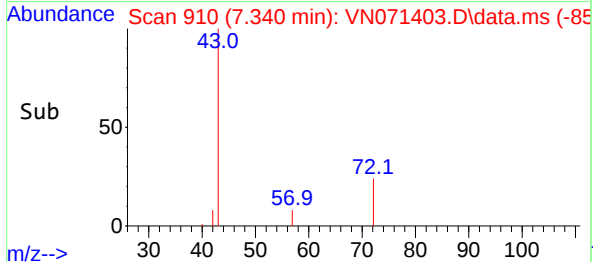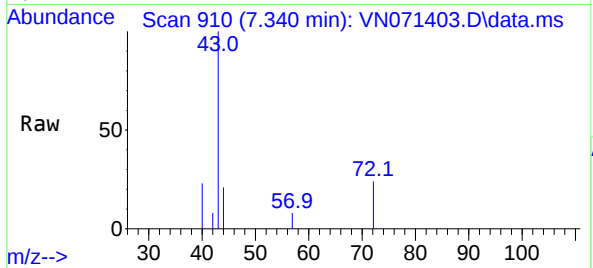

#29
Tetrahydrofuran
Concen: 0.327 ug/l
RT: 7.698 min Scan# 971
Delta R.T. 0.018 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 42 Resp: 1767
Ion Ratio Lower Upper
42 100
72 22.5 36.3 54.5#
71 22.2 34.7 52.1#

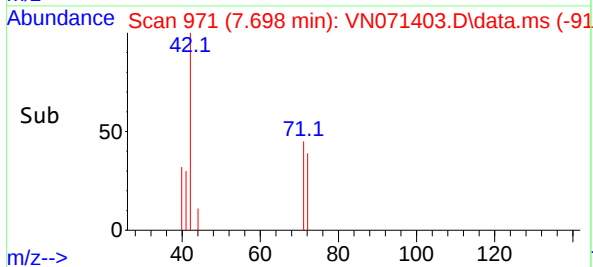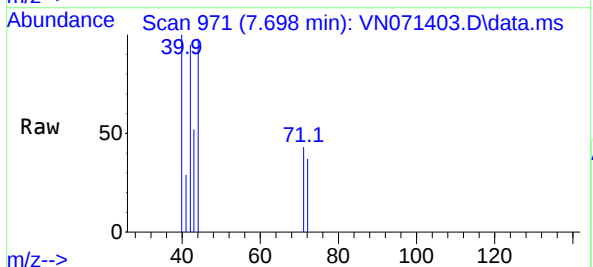



#31

Cyclohexane

Concen: 0.983 ug/l

RT: 8.081 min Scan# 1

Delta R.T. -0.012 min

Lab File: VN071403.D

Acq: 19 Mar 2022 17:19

Instrument :

MSVOA_N

ClientSampleId :

C-10-9-10





Tgt Ion: 56 Resp: 15640

Ion Ratio Lower Upper

56 100

69 187.6 27.1 40.7#

84 170.5 73.4 110.0#

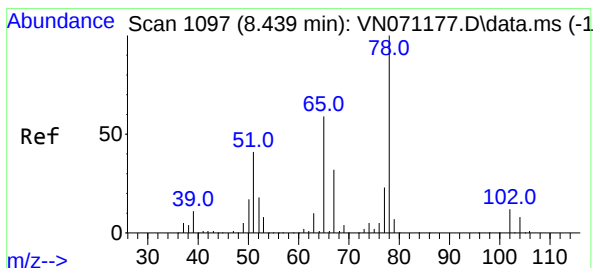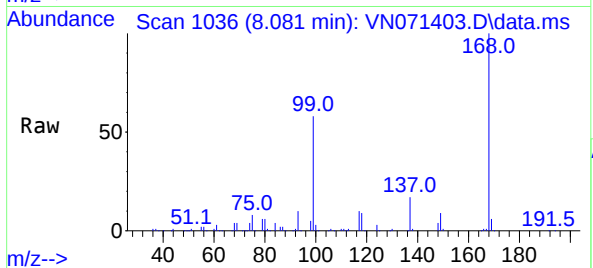

#33

1,2-Dichloroethane-d4

Concen: 48.944 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. -0.006 min

Lab File: VN071403.D




Acq: 19 Mar 2022 17:19


Tgt Ion: 65 Resp: 487630

Ion Ratio Lower Upper

65 100

67 51.9 0.0 103.0


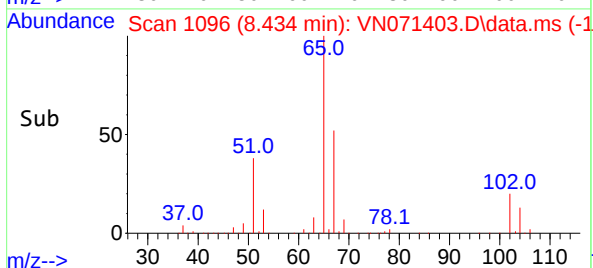

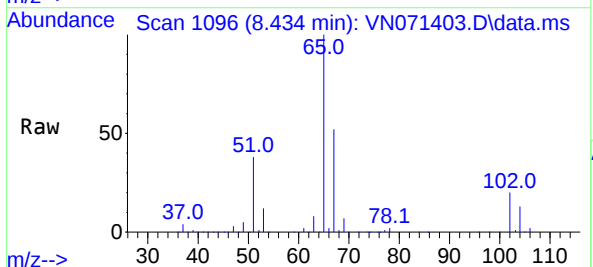


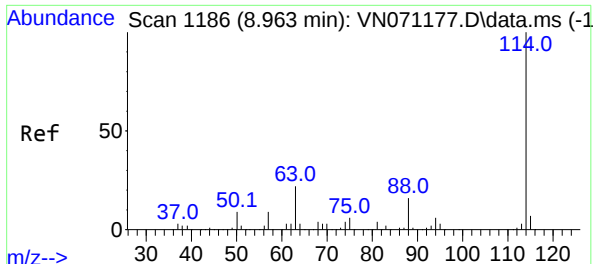

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion:114 Resp: 1234605
Ion Ratio Lower Upper
114 100
63 22.5 0.0 37.8
88 16.2 0.0 27.4

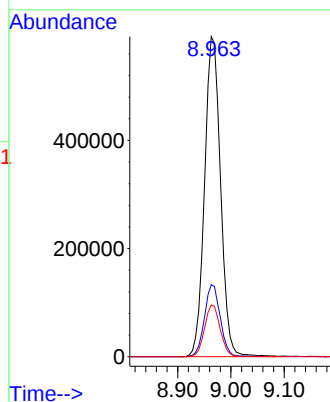

#35
Dibromofluoromethane
Concen: 46.515 ug/l
RT: 8.016 min Scan# 1025
Delta R.T. -0.006 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion:113 Resp: 362386
Ion Ratio Lower Upper
113 100
111 102.7 82.2 123.2
192 20.0 16.9 25.3


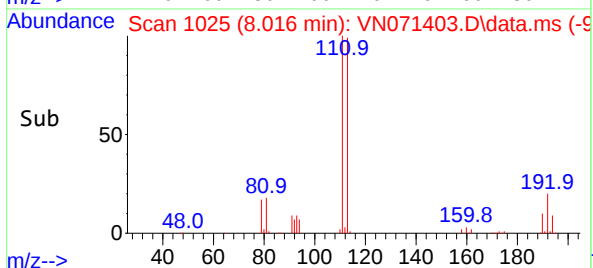
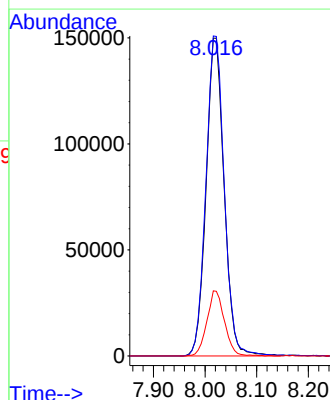
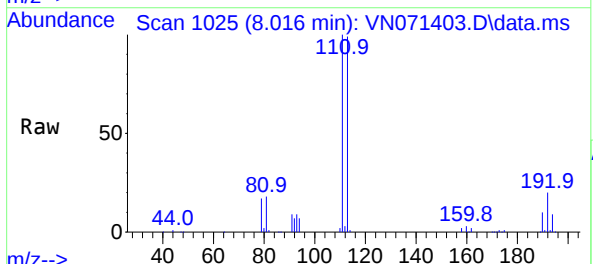




#36
1,1-Dichloropropene
Concen: 4.636 ug/l
RT: 8.087 min Scan# 1037
Delta R.T. -0.129 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion: 75 Resp: 57870
Ion Ratio Lower Upper
75 100
110 7.9 18.4 55.2#
77 0.0 24.4 36.6#

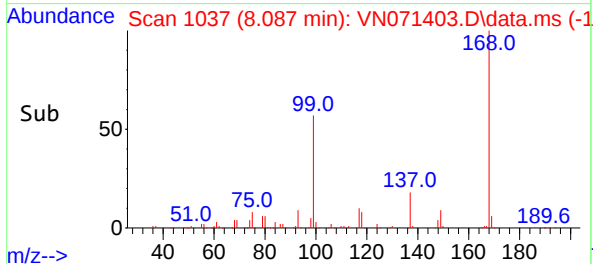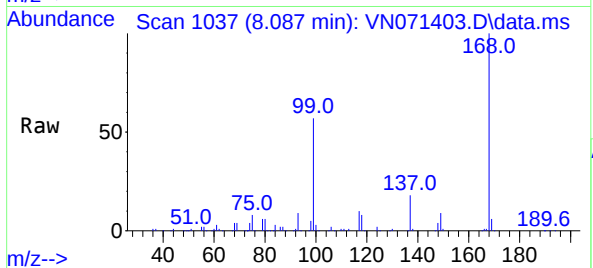

#38
Carbon Tetrachloride
Concen: 5.991 ug/l
RT: 8.087 min Scan# 1037
Delta R.T. -0.118 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 117 Resp: 72336
Ion Ratio Lower Upper
117 100
119 4.9 76.1 114.1#
121 0.0 24.2 36.2#


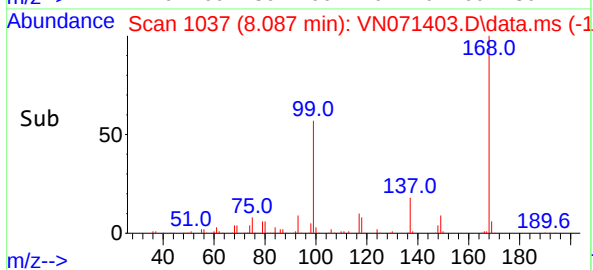

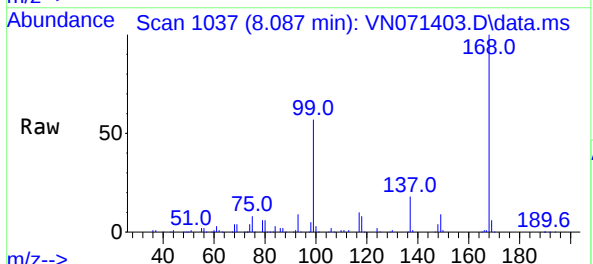




#40
Benzene
Concen: 0.971 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. 0.000 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion: 78 Resp: 36528
Ion Ratio Lower Upper
78 100
77 23.7 18.6 27.8

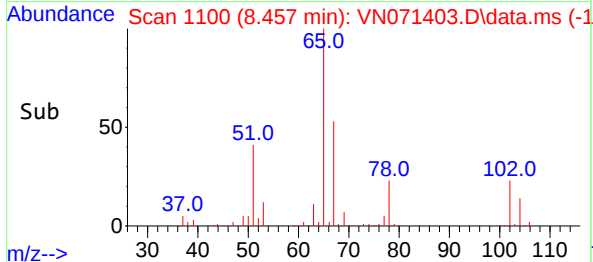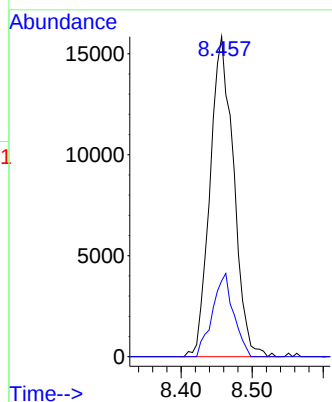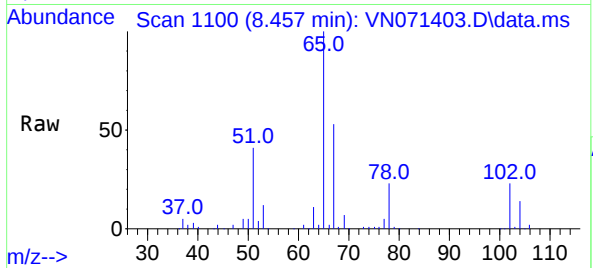

#43
Isopropyl Acetate
Concen: 2.362 ug/l
RT: 8.557 min Scan# 1117
Delta R.T. 0.000 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 43 Resp: 60682
Ion Ratio Lower Upper
43 100
61 14.1 20.4 30.6#
87 7.5 11.2 16.8#

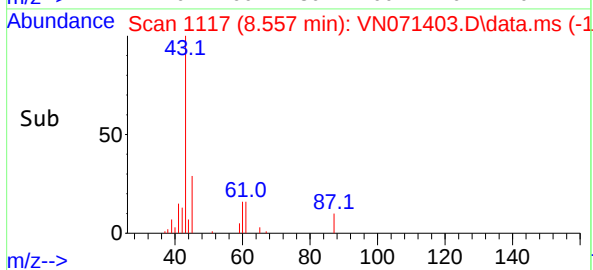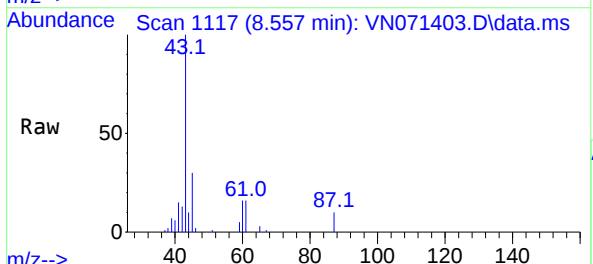



#48

Methyl methacrylate

Concen: 0.528 ug/l

RT: 9.551 min Scan# 11

Delta R.T. -0.006 min

Lab File: VN071403.D

Acq: 19 Mar 2022 17:19

Instrument :

MSVOA_N

ClientSampleId :

C-10-9-10





Tgt Ion: 41 Resp: 6286

Ion Ratio Lower Upper

41 100

69 0.0 72.4 108.6#

39 34.5 58.4 87.6#

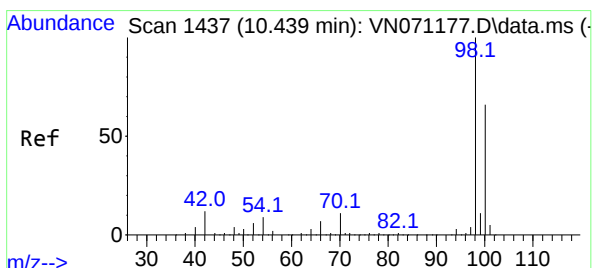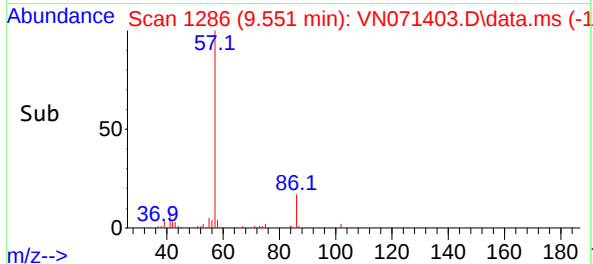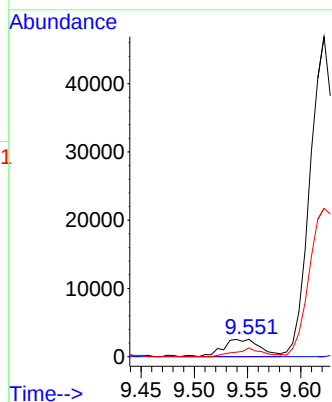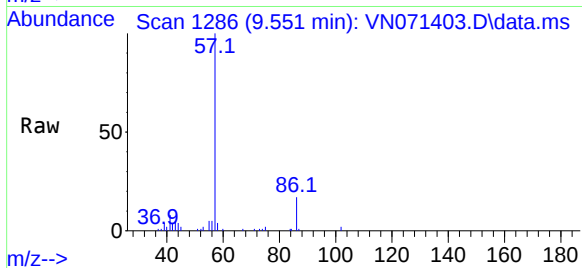

#50

Toluene-d8

Concen: 49.303 ug/l

RT: 10.439 min Scan# 1437

Delta R.T. 0.000 min

Lab File: VN071403.D




Acq: 19 Mar 2022 17:19


Tgt Ion: 98 Resp: 1546543

Ion Ratio Lower Upper

98 100

100 65.4 50.4 75.6


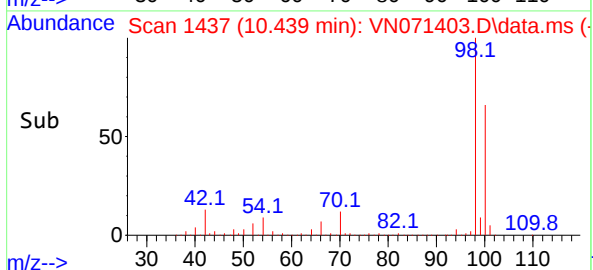

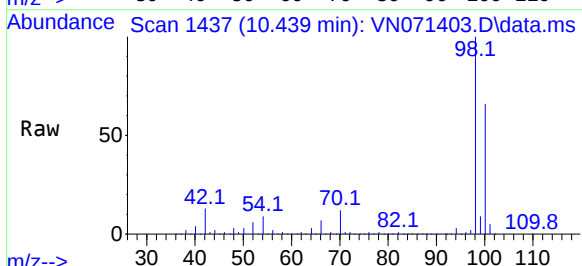




#51
4-Methyl-2-Pentanone
Concen: 0.669 ug/l
RT: 10.328 min Scan# 1418
Delta R.T. 0.001 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion: 43 Resp: 10663
Ion Ratio Lower Upper
43 100
58 48.0 30.4 45.6#

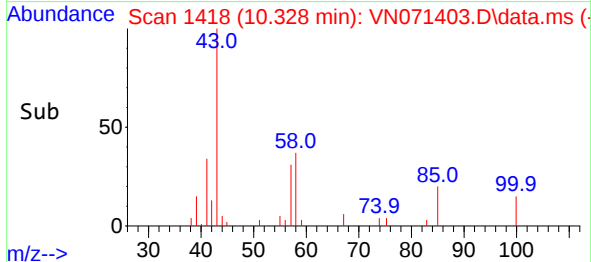

#54
cis-1,3-Dichloropropene
Concen: 4.656 ug/l
RT: 10.239 min Scan# 1403
Delta R.T. 0.053 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 75 Resp: 70421
Ion Ratio Lower Upper
75 100
77 0.8 26.4 39.6#
39 37.2 42.5 63.7#

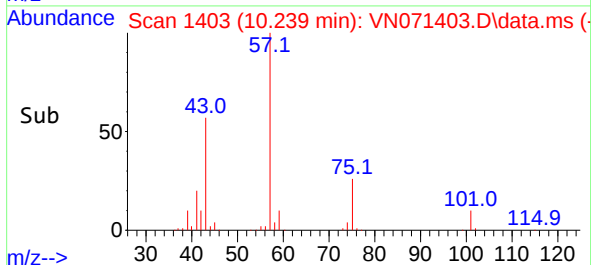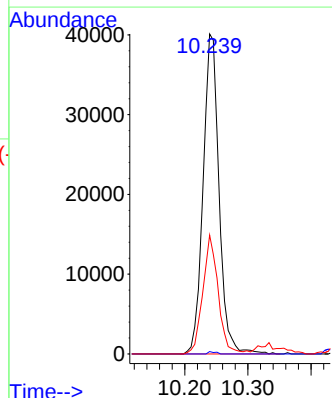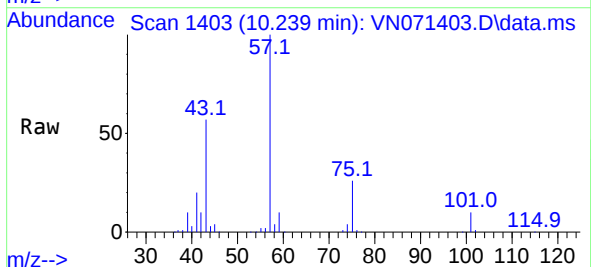



#57

1,3-Dichloropropane

Concen: 0.872 ug/l

RT: 11.086 min Scan# 1547

Delta R.T. 0.047 min

Lab File: VN071403.D

Acq: 19 Mar 2022 17:19

Instrument :

MSVOA_N

ClientSampleId :





C-10-9-10

Tgt Ion: 76 Resp: 14527

Ion Ratio Lower Upper

76 100

78 0.0 25.7 38.5#

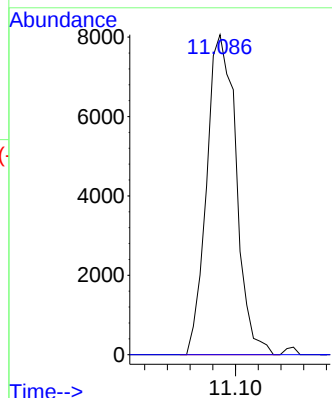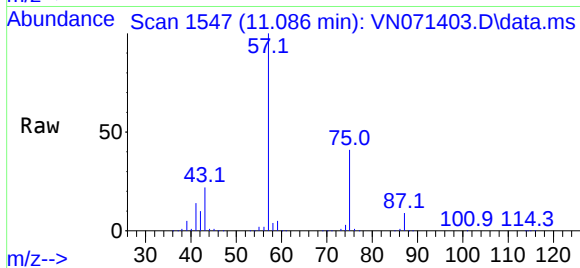

#59

2-Hexanone

Concen: 24.653 ug/l

RT: 11.086 min Scan# 1547

Delta R.T. 0.006 min

Lab File: VN071403.D




Acq: 19 Mar 2022 17:19


Tgt Ion: 43 Resp: 268182

Ion Ratio Lower Upper

43 100

58 16.2 26.9 80.7#


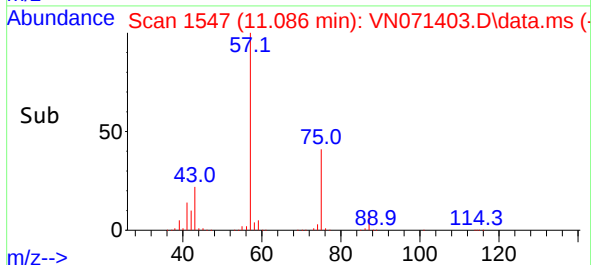

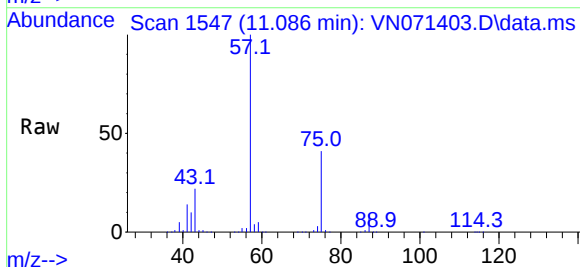




#62
4-Bromofluorobenzene
Concen: 52.867 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion: 95 Resp: 561549
Ion Ratio Lower Upper
95 100
174 79.2 0.0 187.2
176 75.2 0.0 181.4

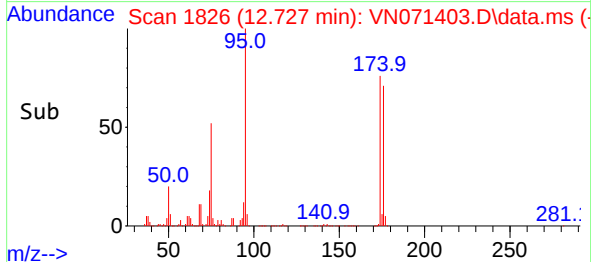

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 117 Resp: 1188735
Ion Ratio Lower Upper
117 100
82 56.3 42.4 63.6
119 32.2 25.4 38.2


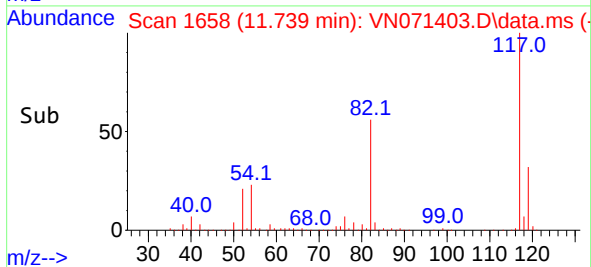

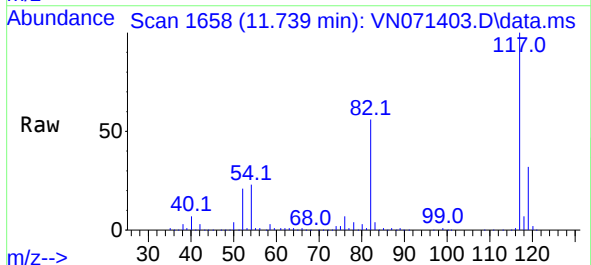




#67
Ethyl Benzene
Concen: 1.287 ug/l
RT: 11.845 min Scan# 1675
Delta R.T. 0.006 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion: 91 Resp: 58073
Ion Ratio Lower Upper
91 100
106 26.6 25.7 38.5

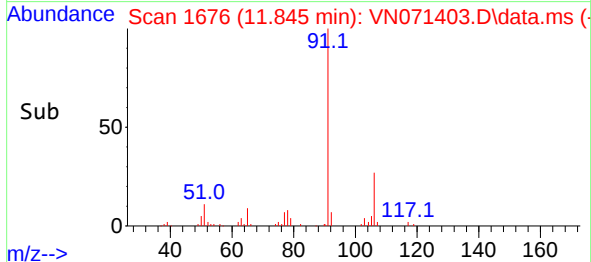

#68
m/p-Xylenes
Concen: 1.254 ug/l
RT: 11.951 min Scan# 1694
Delta R.T. -0.000 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 106 Resp: 20709
Ion Ratio Lower Upper
106 100
91 198.9 160.6 240.8


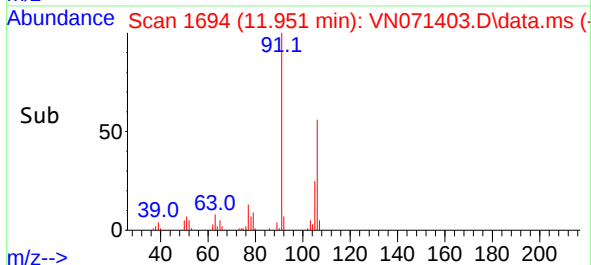

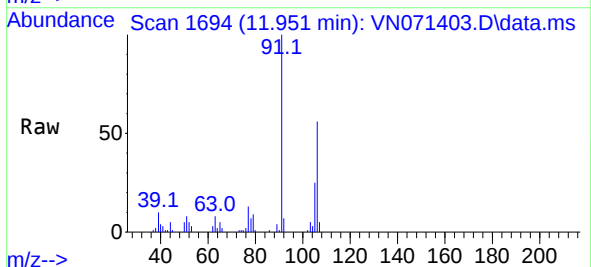




#69
o-Xylene
Concen: 0.387 ug/l
RT: 12.280 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion:106 Resp: 6399
Ion Ratio Lower Upper
106 100
91 210.5 105.8 317.3

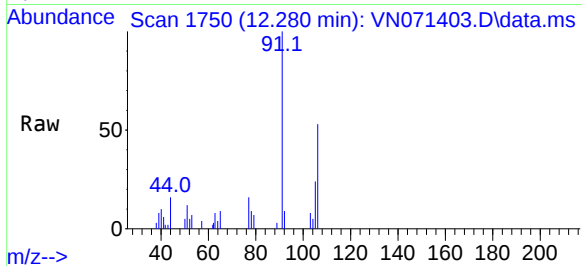

#71
Bromoform
Concen: 0.491 ug/l
RT: 12.722 min Scan# 1825
Delta R.T. 0.265 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion:173 Resp: 3489
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0


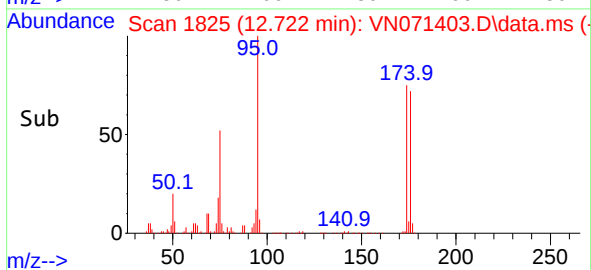

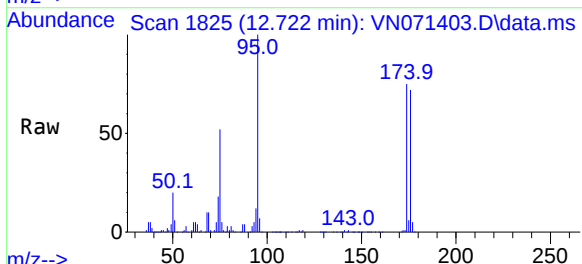




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1986
Delta R.T. 0.006 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion:152 Resp: 421932
Ion Ratio Lower Upper
152 100
115 59.0 27.5 82.5
150 156.1 0.0 344.4

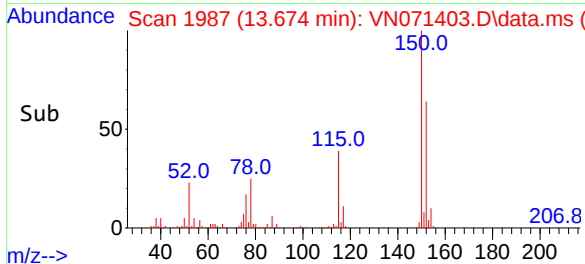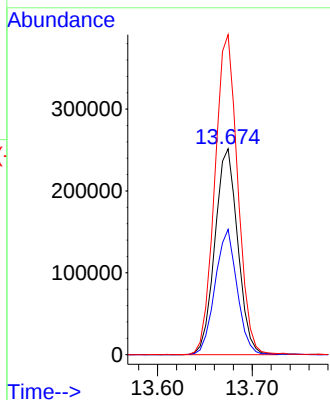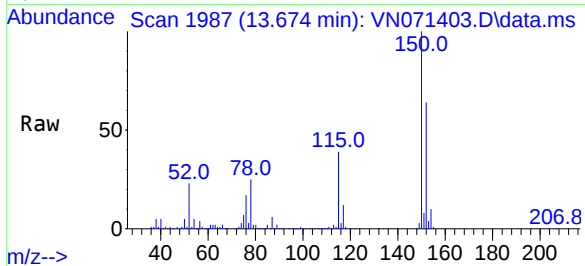

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.733 min Scan# 1827
Delta R.T. -0.088 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 83 Resp: 572
Ion Ratio Lower Upper
83 100
131 130.8 5.5 16.5#
85 0.0 32.4 97.2#


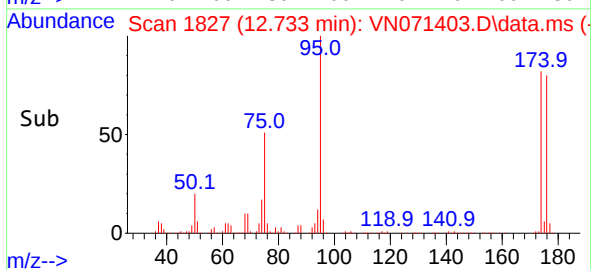
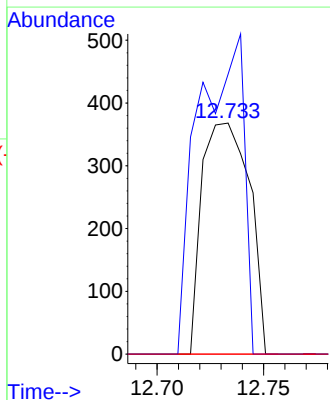
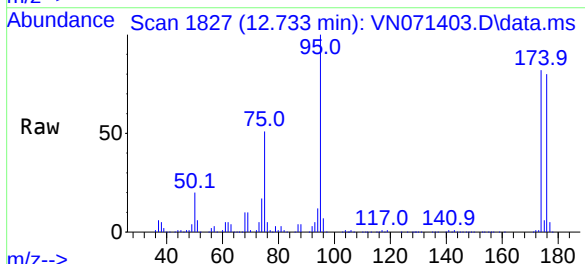




#76
1,2,3-Trichloropropane
Concen: 27.204 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion: 75 Resp: 291356
Ion Ratio Lower Upper
75 100
77 1.2 82.6 247.8#

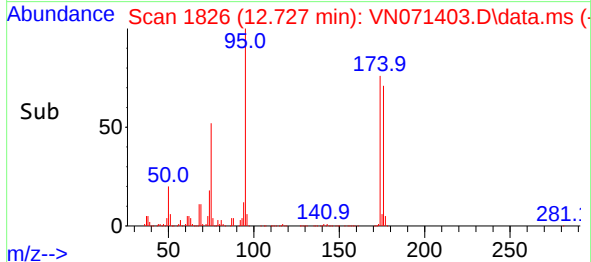

#80
1,3,5-Trimethylbenzene
Concen: 0.231 ug/l
RT: 13.051 min Scan# 1881
Delta R.T. -0.006 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 105 Resp: 7319
Ion Ratio Lower Upper
105 100
120 43.5 24.6 73.6


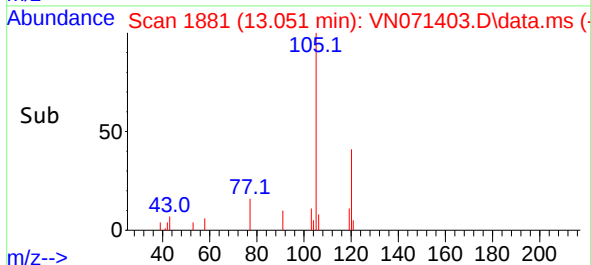
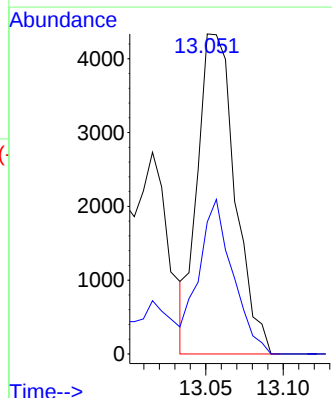
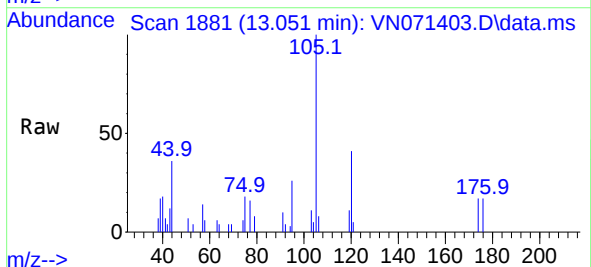




#81
trans-1,4-Dichloro-2-butene
Concen: 74.646 ug/l
RT: 12.727 min Scan# 1808
Delta R.T. 0.106 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19




Instrument :
MSVOA_N
ClientSampleId :
C-10-9-10


Tgt Ion: 75 Resp: 291356
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#



#84
1,2,4-Trimethylbenzene
Concen: 0.471 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN071403.D
Acq: 19 Mar 2022 17:19

Tgt Ion: 105 Resp: 14279
Ion Ratio Lower Upper
105 100
120 43.4 22.8 68.4


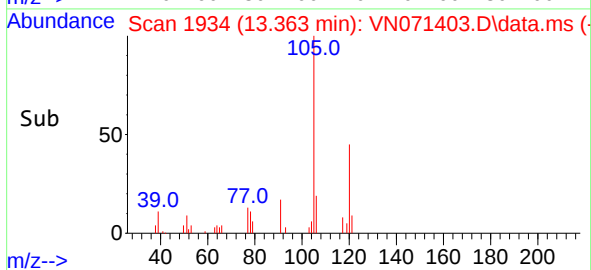






#85
 sec-Butylbenzene
 Concen: 0.380 ug/l
 RT: 13.363 min Scan# 1934
 Delta R.T. -0.135 min
 Lab File: VN071403.D
 Acq: 19 Mar 2022 17:19

Instrument :
 MSVOA_N
 ClientSampleId :
 C-10-9-10

Tgt Ion:105 Resp: 14279
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.4 31.1#

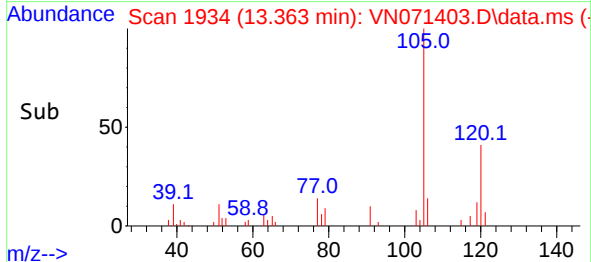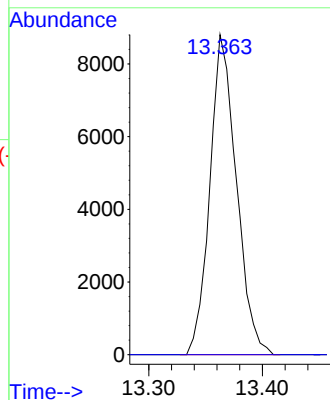

#95
 Naphthalene
 Concen: 6.372 ug/l
 RT: 15.504 min Scan# 2298
 Delta R.T. -0.000 min
 Lab File: VN071403.D
 Acq: 19 Mar 2022 17:19

Tgt Ion:128 Resp: 28067
 Ion Ratio Lower Upper
 128 100
 127 13.3 10.5 15.7
 129 9.6 8.7 13.1

