
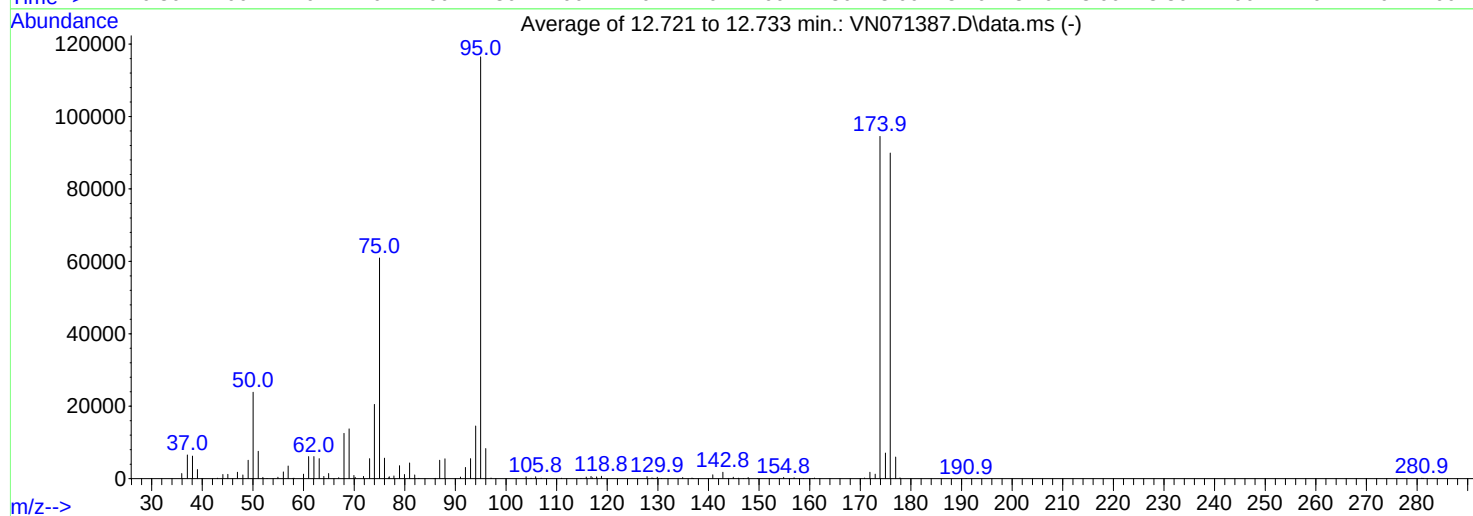


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031922\
 Data File : VN071387.D
 Acq On : 19 Mar 2022 09:59
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Title : SW846 8260
 Last Update : Tue Mar 08 06:52:46 2022

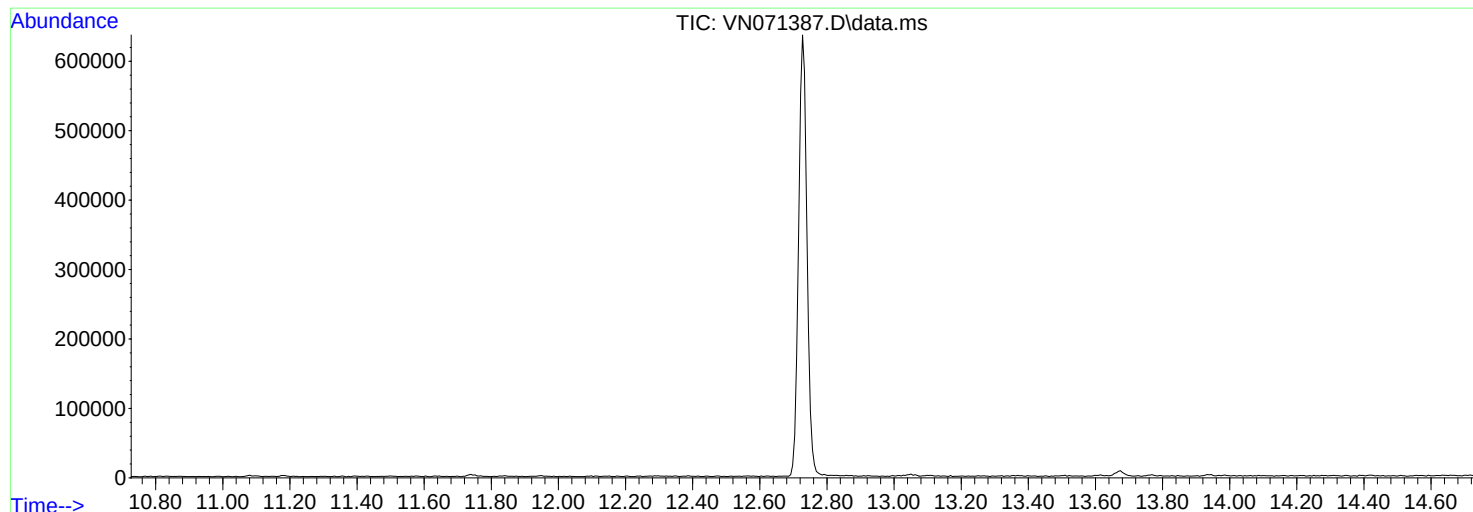

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	23869	PASS
75	95	30	60	52.3	60936	PASS
95	95	100	100	100.0	116483	PASS
96	95	5	9	7.1	8318	PASS
173	174	0.00	2	1.3	1239	PASS
174	95	50	100	81.2	94528	PASS
175	174	5	9	7.5	7059	PASS
176	174	95	101	95.1	89896	PASS
177	176	5	9	6.6	5948	PASS