
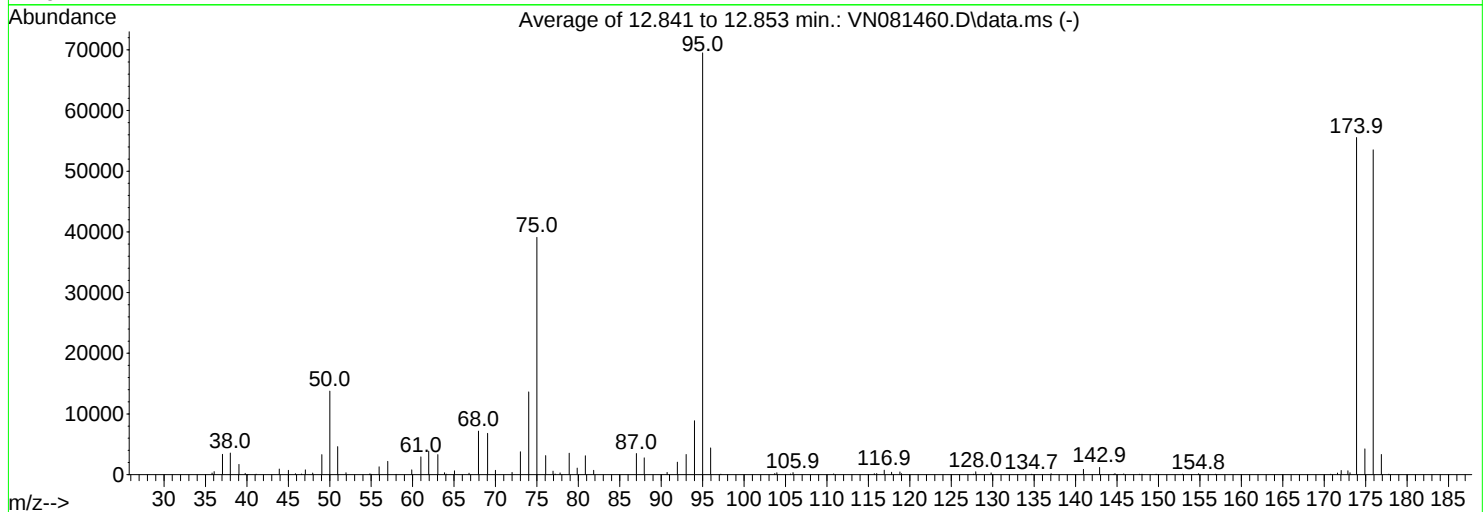


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031924\
Data File : VN081460.D
Acq On : 19 Mar 2024 08:32
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

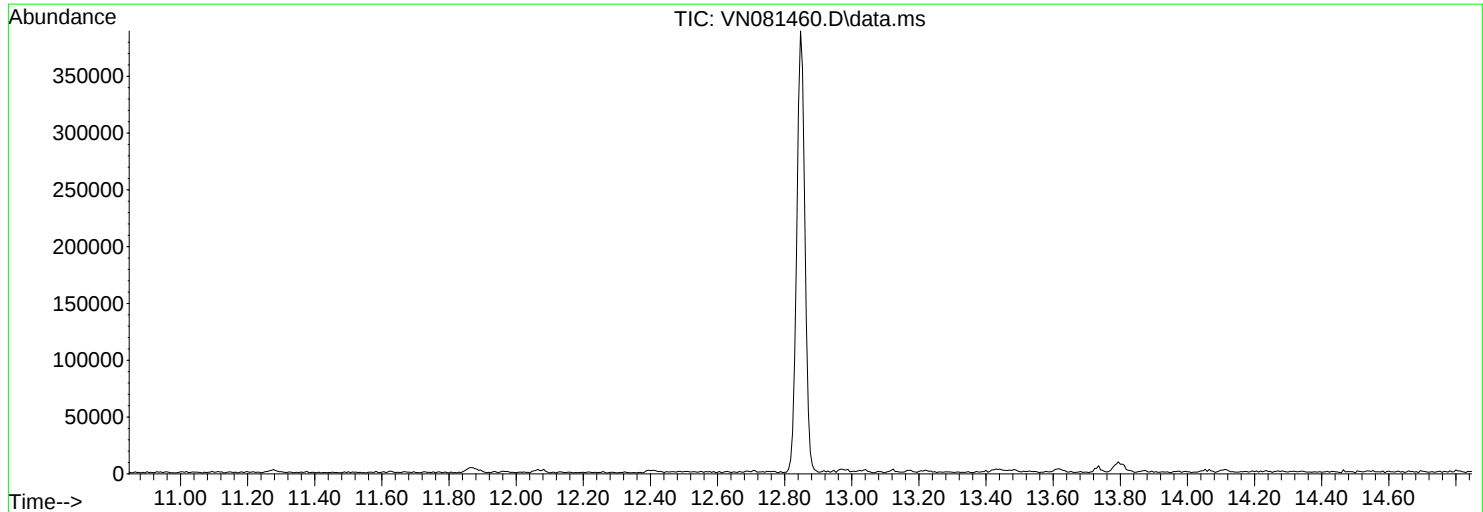

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	13770	PASS
75	95	30	60	56.3	39109	PASS
95	95	100	100	100.0	69507	PASS
96	95	5	9	6.3	4405	PASS
173	174	0.00	2	1.1	630	PASS
174	95	50	100	79.9	55552	PASS
175	174	5	9	7.6	4241	PASS
176	174	95	101	96.3	53512	PASS
177	176	5	9	6.2	3334	PASS

Average of 12.841 to 12.853 min.: VN081460.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	260	46.60	112	58.00	58	70.00	70
36.05	503	47.05	806	59.90	792	72.00	37
37.05	3346	47.95	272	61.00	2935	73.00	378
38.00	3553	49.05	3309	61.95	3869	74.00	1362
39.05	1695	50.00	13770	63.05	3298	75.00	39109
39.80	202	50.95	4606	63.85	317	76.05	3137
40.00	14	51.95	322	64.10	72	76.95	577
41.10	72	54.80	101	65.05	631	77.20	117
43.90	939	54.95	116	66.80	249	77.80	281
45.00	727	55.95	1303	67.95	7184	78.90	3542
45.85	162	57.00	2194	69.05	6810	79.85	1077

Average of 12.841 to 12.853 min.: VN081460.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.85	3118	103.70	191	119.00	153	147.70	88
81.85	707	103.95	316	127.70	80	148.00	69
87.00	3469	105.00	52	127.95	483	149.70	83
87.95	2767	105.60	98	129.80	294	152.90	78
90.70	383	105.90	355	134.70	79	154.85	156
91.95	2066	110.80	123	137.05	149	156.90	80
93.00	3335	115.70	168	140.95	887	170.80	83
94.00	8880	116.00	177	142.90	1199	171.60	277
95.00	69507	116.90	755	144.60	53	172.05	691
95.95	4405	117.80	397	144.75	196	172.85	630
97.20	76	118.80	455	145.80	128	173.10	312

Average of 12.841 to 12.853 min.: VN081460.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.90	55552						
174.90	4241						
175.90	53512						
176.90	3334						
177.80	68						