

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031925\
 Data File : VN086020.D
 Acq On : 19 Mar 2025 19:39
 Operator : JC\MD
 Sample : Q1592-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 257952

Quant Time: Mar 20 01:37:46 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 19 03:20:56 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	145847	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	274022	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	235432	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	103166	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.571	65	103141	51.644	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 103.280%	
35) Dibromofluoromethane	8.159	113	87436	45.715	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 91.420%	
50) Toluene-d8	10.565	98	313564	45.172	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 90.340%	
62) 4-Bromofluorobenzene	12.847	95	115096	46.493	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 92.980%	


Target Compounds				Qvalue		
3) Chloromethane	2.353	50	454	0.268	ug/l #	84
11) Tert butyl alcohol	5.512	59	2261	7.996	ug/l #	73
16) Acetone	4.424	43	22268	36.496	ug/l	98
18) Methyl Acetate	5.030	43	3139	2.079	ug/l #	82
25) 2-Butanone	7.477	43	14341	16.289	ug/l #	86
31) Cyclohexane	8.218	56	3204	1.288	ug/l #	1
36) 1,1-Dichloropropene	8.218	75	11397	4.525	ug/l #	51
37) Ethyl Acetate	7.565	43	6570	3.092	ug/l #	1
38) Carbon Tetrachloride	8.218	117	16395	4.951	ug/l #	16
39) Methylcyclohexane	9.600	83	1215	0.486	ug/l #	81
40) Benzene	8.600	78	41636	5.266	ug/l	96
43) Isopropyl Acetate	8.682	43	5782	1.256	ug/l #	50
51) 4-Methyl-2-Pentanone	10.441	43	673	0.331	ug/l #	30
52) Toluene	10.629	92	50286	10.363	ug/l	100
56) Ethyl methacrylate	10.900	69	706	0.490	ug/l #	1
67) Ethyl Benzene	11.959	91	20359	2.362	ug/l	93
68) m/p-Xylenes	12.065	106	35797	10.568	ug/l	98
69) o-Xylene	12.400	106	16841	5.417	ug/l	98
70) Styrene	12.406	104	5013	0.944	ug/l #	49
71) Bromoform	12.847	173	647	0.386	ug/l #	28
73) Isopropylbenzene	12.688	105	3890	0.552	ug/l	98
74) N-amyl acetate	12.453	43	1314	0.557	ug/l #	38
76) 1,2,3-Trichloropropane	12.847	75	57238	24.782	ug/l #	1
78) n-propylbenzene	13.035	91	5984	0.750	ug/l	91
79) 2-Chlorotoluene	13.100	91	3062	0.578	ug/l #	42
80) 1,3,5-Trimethylbenzene	13.170	105	13614	2.289	ug/l	95
81) trans-1,4-Dichloro-2-b...	12.847	75	57238	65.519	ug/l #	16
82) 4-Chlorotoluene	13.170	91	1766	0.324	ug/l #	43
84) 1,2,4-Trimethylbenzene	13.476	105	26556	4.427	ug/l	98
86) p-Isopropyltoluene	13.723	119	1650	0.294	ug/l	90
90) Hexachloroethane	14.323	117	390	0.301	ug/l #	10
95) Naphthalene	15.635	128	26355	5.142	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031925\
Data File : VN086020.D
Acq On : 19 Mar 2025 19:39
Operator : JC\MD
Sample : Q1592-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
257952

Quant Time: Mar 20 01:37:46 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 19 03:20:56 2025
Response via : Initial Calibration




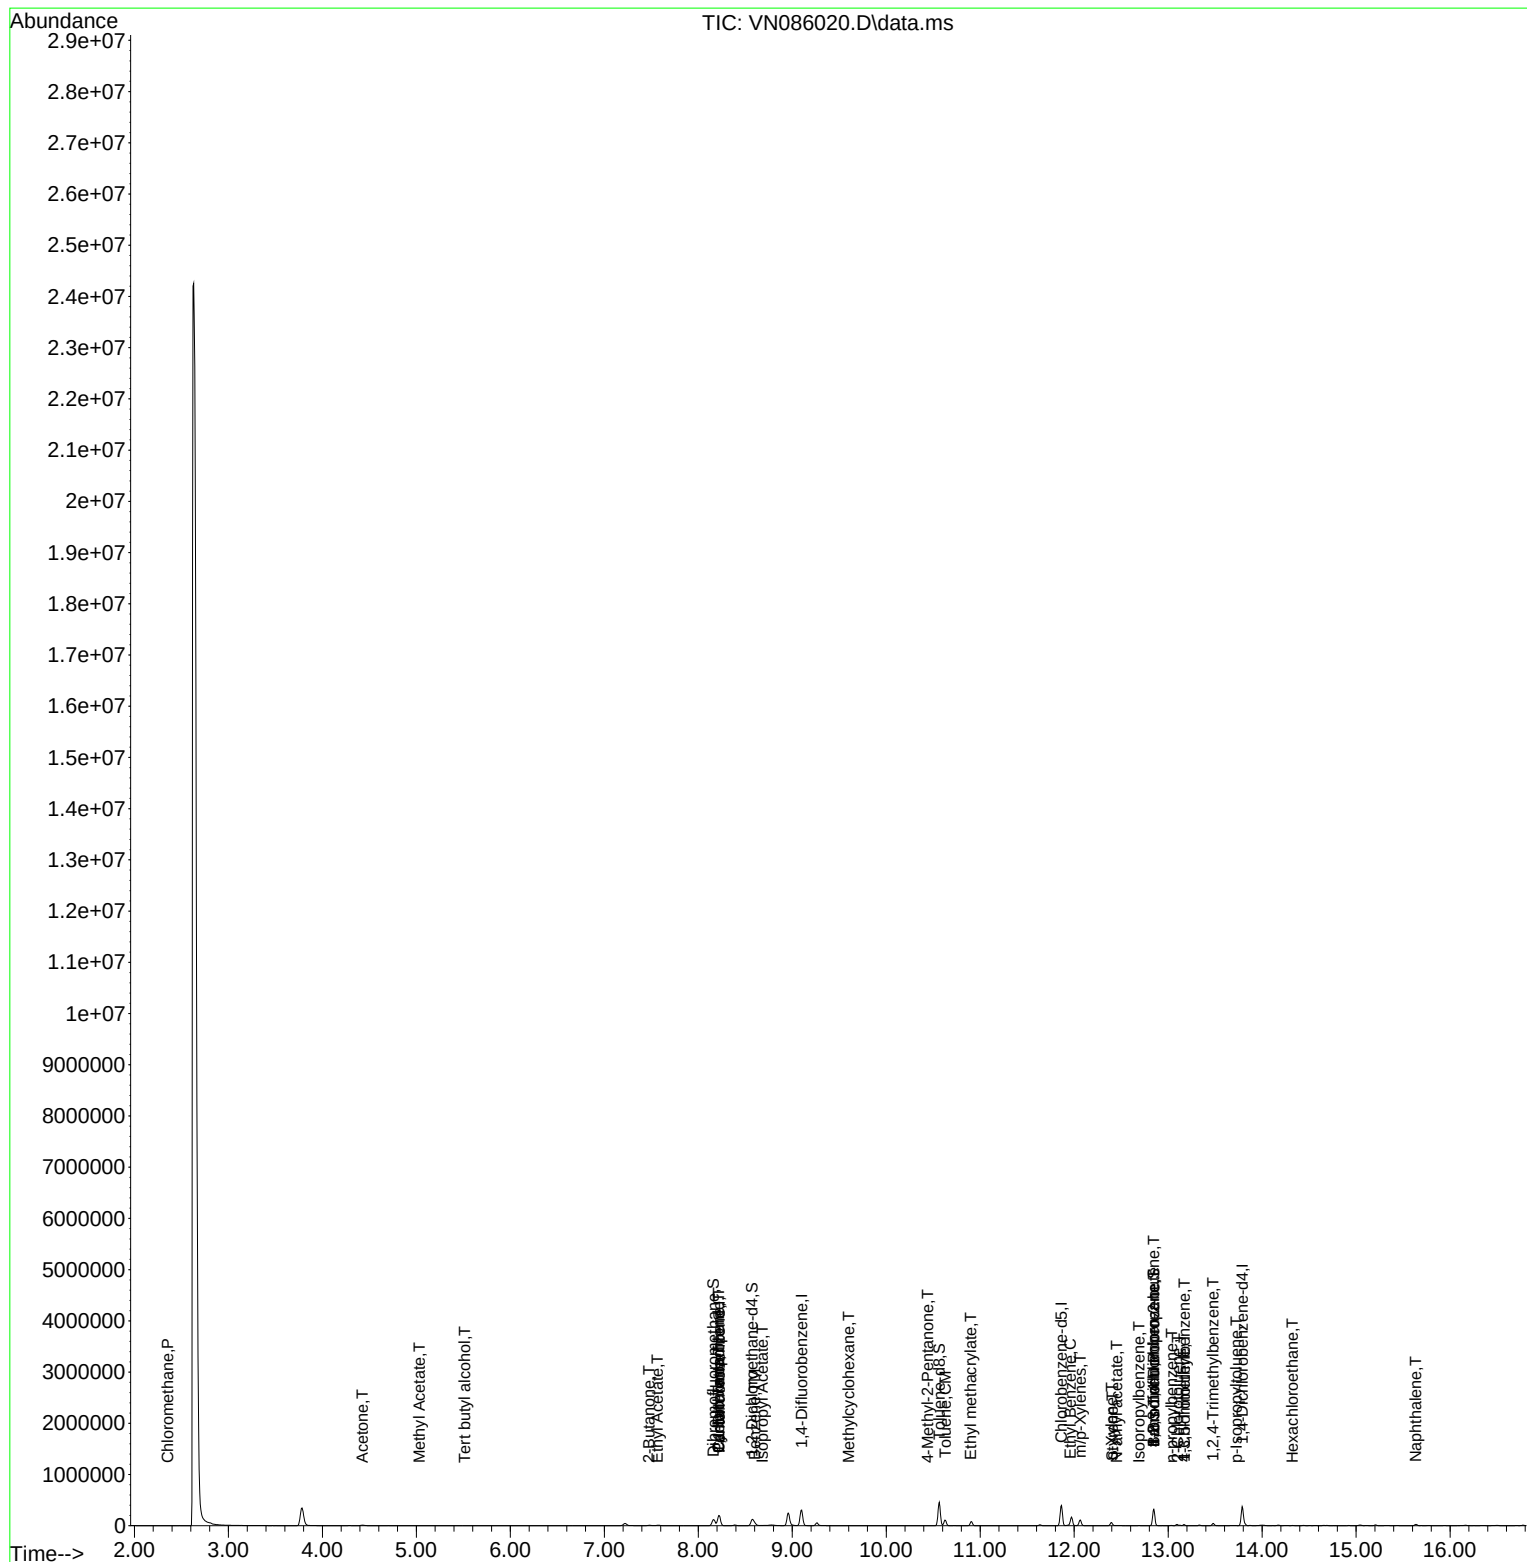




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion:168 Resp: 145847
Ion Ratio Lower Upper
168 100
99 58.8 49.4 74.2

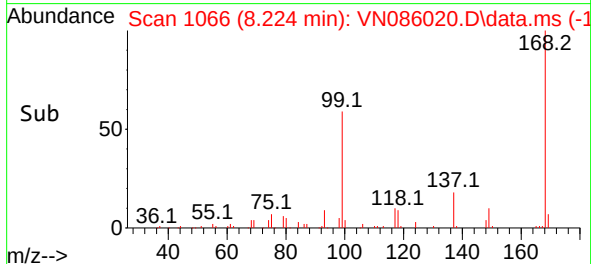

#3
Chloromethane
Concen: 0.268 ug/l
RT: 2.353 min Scan# 68
Delta R.T. -0.006 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 50 Resp: 454
Ion Ratio Lower Upper
50 100
52 41.5 26.0 39.0#









#11
Tert butyl alcohol
Concen: 7.996 ug/l
RT: 5.512 min Scan# 607
Delta R.T. -0.012 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion: 59 Resp: 2261
Ion Ratio Lower Upper
59 100
57 0.0 7.9 11.9#

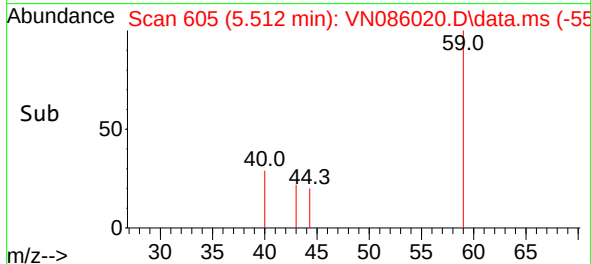

#16
Acetone
Concen: 36.496 ug/l
RT: 4.424 min Scan# 420
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 43 Resp: 22268
Ion Ratio Lower Upper
43 100
58 37.9 29.4 44.2





#18

Methyl Acetate

Concen: 2.079 ug/l

RT: 5.030 min Scan# 51

Delta R.T. 0.006 min

Lab File: VN086020.D

Acq: 19 Mar 2025 19:39

Instrument :

MSVOA_N

ClientSampleId :





257952

Tgt Ion: 43 Resp: 3139

Ion Ratio Lower Upper

43 100

74 19.9 23.9 35.9#



#25

2-Butanone

Concen: 16.289 ug/l

RT: 7.477 min Scan# 939

Delta R.T. -0.006 min

Lab File: VN086020.D




Acq: 19 Mar 2025 19:39


Tgt Ion: 43 Resp: 14341

Ion Ratio Lower Upper

43 100


72 26.3 27.4 41.0#





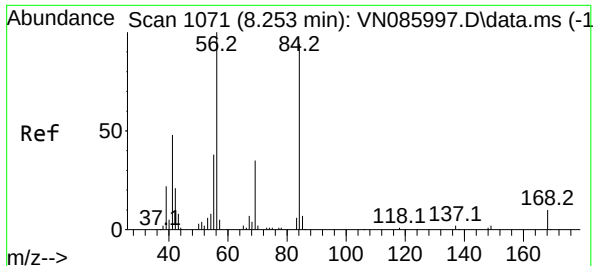


#31
Cyclohexane
Concen: 1.288 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.036 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Instrument :
MSVOA_N
ClientSampleId :
257952



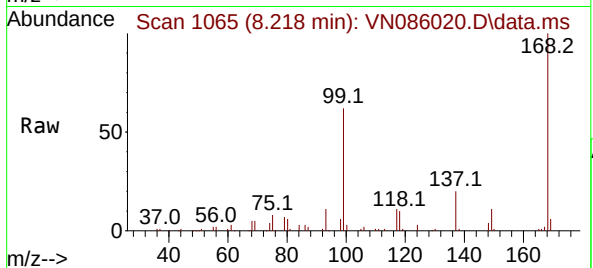



Tgt Ion: 56 Resp: 3204
Ion Ratio Lower Upper
56 100
69 200.8 28.0 42.0#
84 150.3 75.0 112.6#

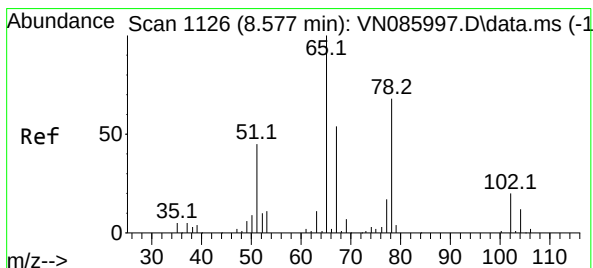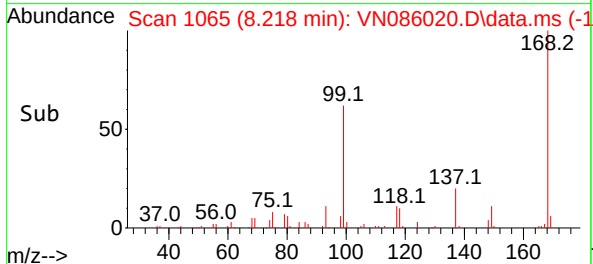

#33
1,2-Dichloroethane-d4
Concen: 51.644 ug/l
RT: 8.571 min Scan# 1125
Delta R.T. -0.006 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 65 Resp: 103141
Ion Ratio Lower Upper
65 100
67 50.9 0.0 102.2


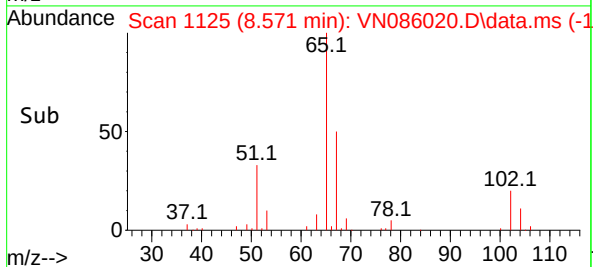

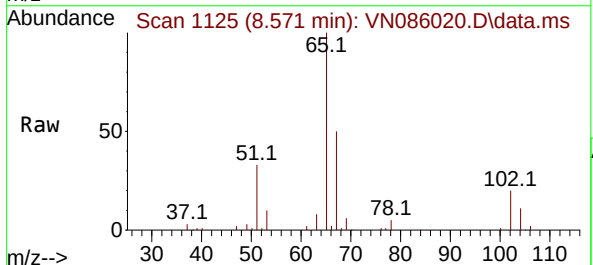


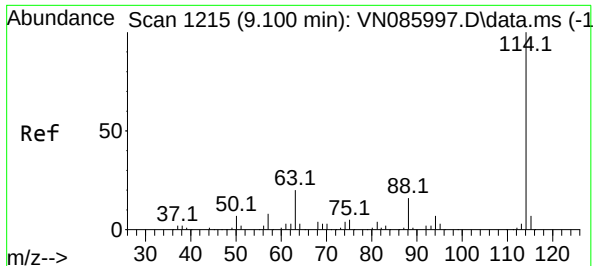

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion:114 Resp: 274022
Ion Ratio Lower Upper
114 100
63 19.6 0.0 39.6
88 15.5 0.0 32.6

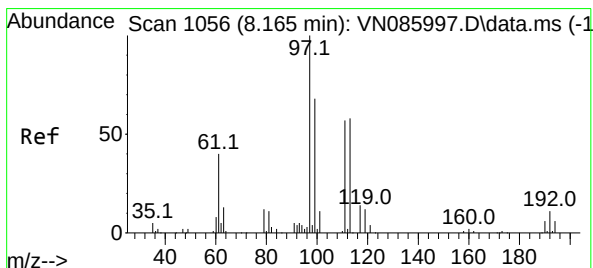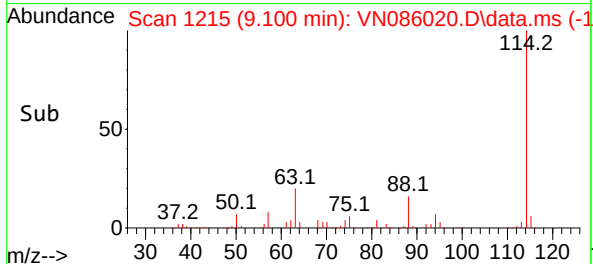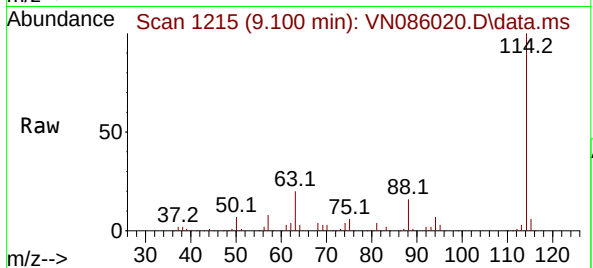

#35
Dibromofluoromethane
Concen: 45.715 ug/l
RT: 8.159 min Scan# 1055
Delta R.T. -0.006 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion:113 Resp: 87436
Ion Ratio Lower Upper
113 100
111 103.1 81.8 122.8
192 20.0 15.9 23.9


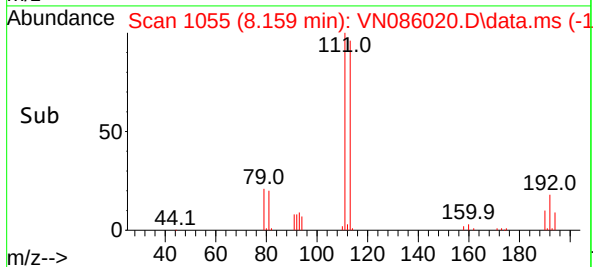

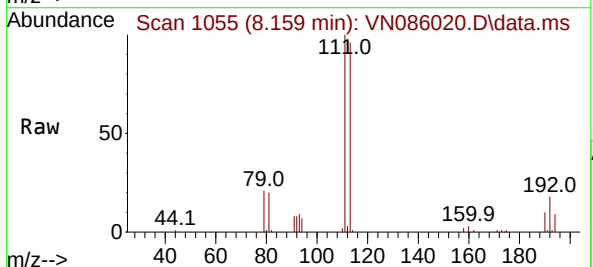


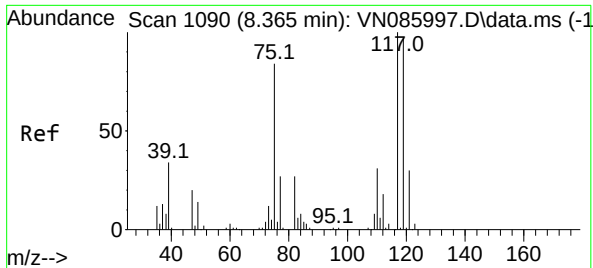

#36
1,1-Dichloropropene
Concen: 4.525 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.147 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion: 75 Resp: 11397
Ion Ratio Lower Upper
75 100
110 10.6 17.8 53.3#
77 0.0 25.0 37.4#

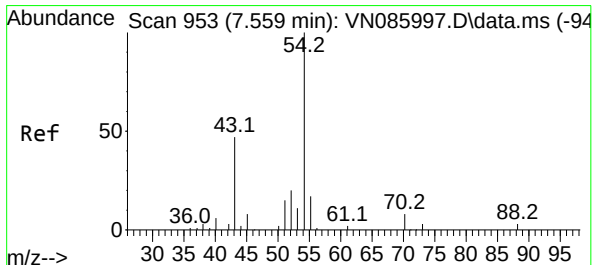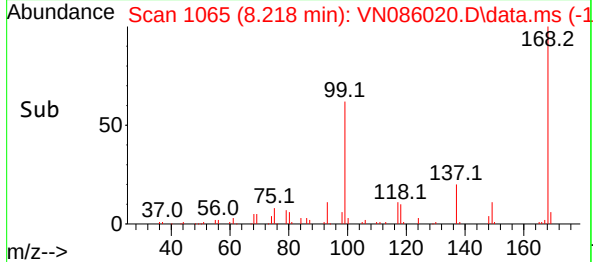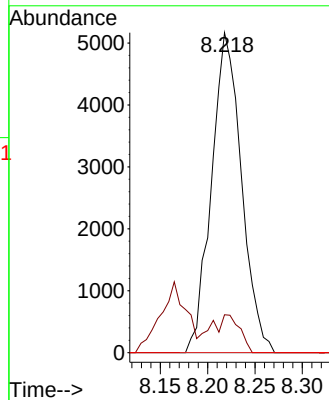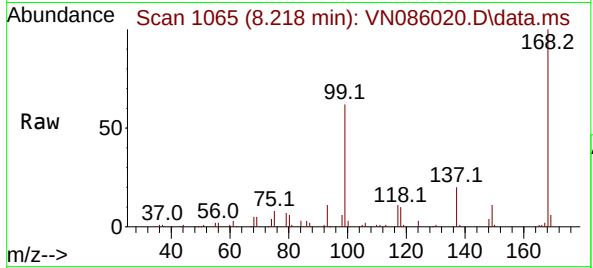

#37
Ethyl Acetate
Concen: 3.092 ug/l
RT: 7.565 min Scan# 954
Delta R.T. 0.006 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39


Tgt Ion: 43 Resp: 6570
Ion Ratio Lower Upper
43 100
61 152.9 13.0 19.4#
70 0.0 11.0 16.6#

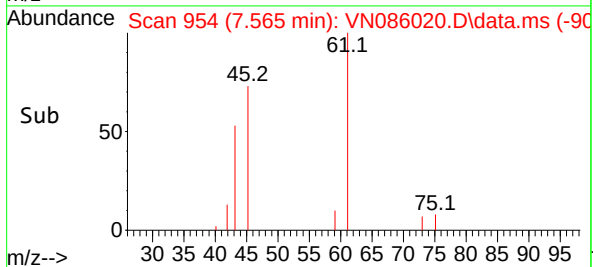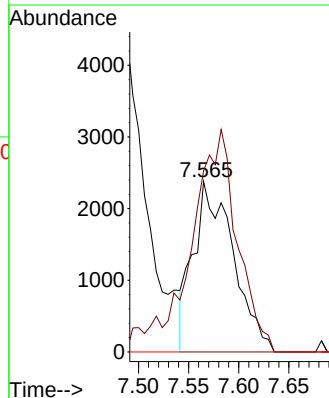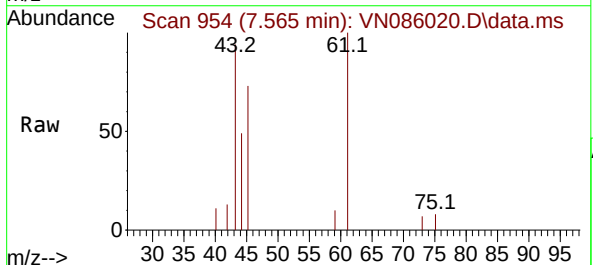



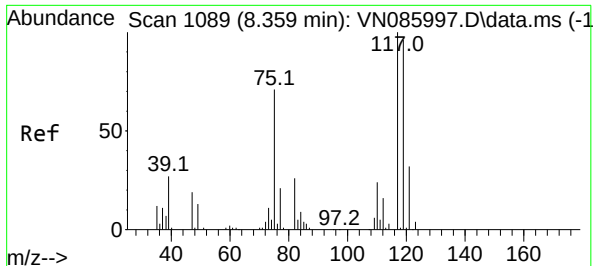


#38
Carbon Tetrachloride
Concen: 4.951 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.141 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Instrument :
MSVOA_N
ClientSampleId :
257952



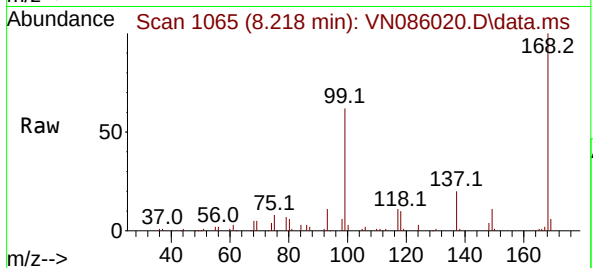



Tgt Ion:117 Resp: 16395
Ion Ratio Lower Upper
117 100
119 5.6 77.0 115.4#
121 0.0 25.6 38.4#

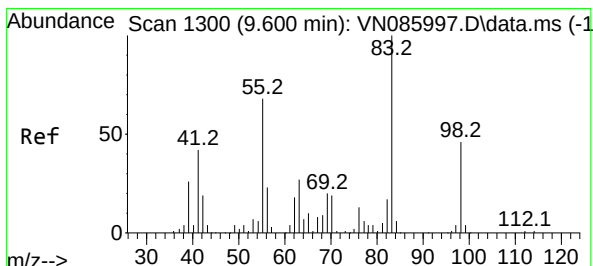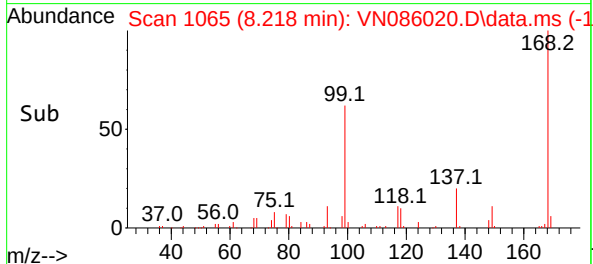

#39
Methylcyclohexane
Concen: 0.486 ug/l
RT: 9.600 min Scan# 1300
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 83 Resp: 1215
Ion Ratio Lower Upper
83 100
55 81.9 54.2 81.2#
98 60.8 37.1 55.7#


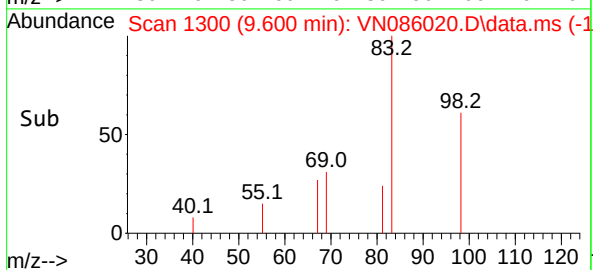

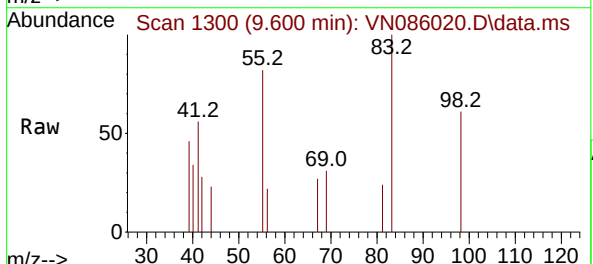


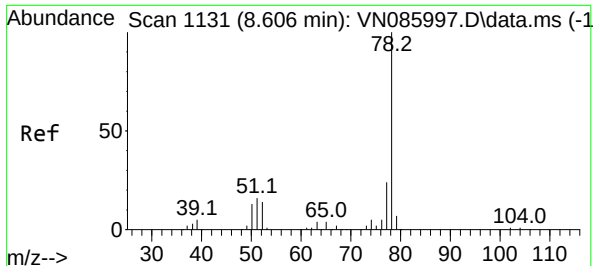

#40
Benzene
Concen: 5.266 ug/l
RT: 8.600 min Scan# 1131
Delta R.T. -0.006 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion: 78 Resp: 41636
Ion Ratio Lower Upper
78 100
77 21.9 18.9 28.3

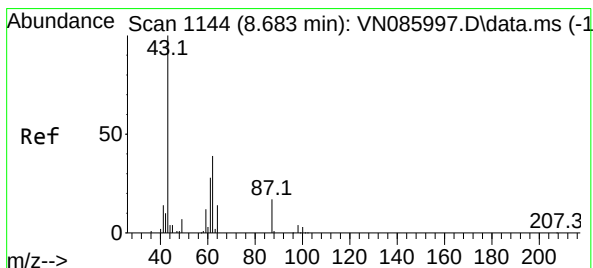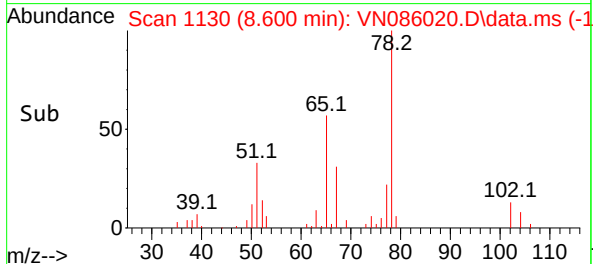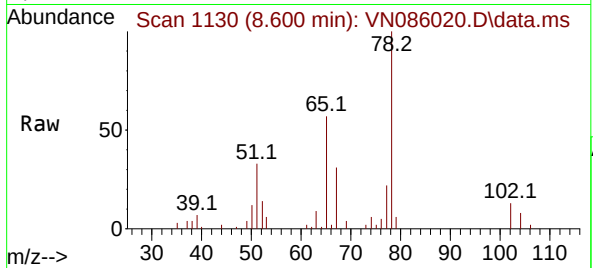

#43
Isopropyl Acetate
Concen: 1.256 ug/l
RT: 8.682 min Scan# 1144
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 43 Resp: 5782
Ion Ratio Lower Upper
43 100
61 0.0 25.0 37.6#
87 0.0 13.0 19.4#


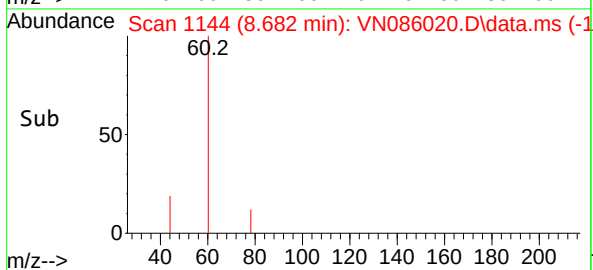

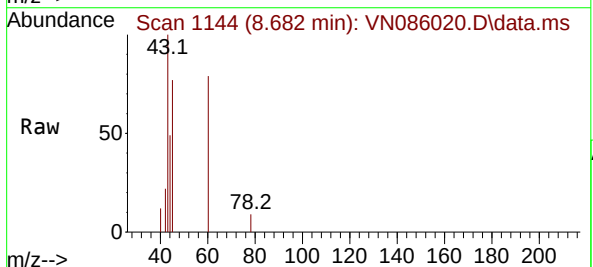




#50
Toluene-d8
Concen: 45.172 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion: 98 Resp: 313564
Ion Ratio Lower Upper
98 100
100 64.0 53.1 79.7

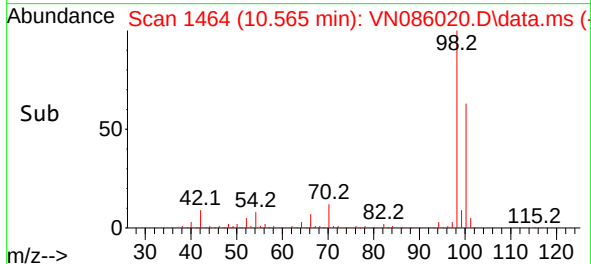

#51
4-Methyl-2-Pentanone
Concen: 0.331 ug/l
RT: 10.441 min Scan# 1443
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 43 Resp: 673
Ion Ratio Lower Upper
43 100
58 0.0 37.4 56.0#









#52
Toluene
Concen: 10.363 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion: 92 Resp: 50286
Ion Ratio Lower Upper
92 100
91 170.4 136.2 204.4

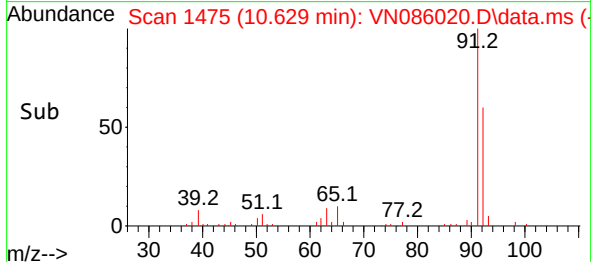

#56
Ethyl methacrylate
Concen: 0.490 ug/l
RT: 10.900 min Scan# 1521
Delta R.T. 0.029 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 69 Resp: 706
Ion Ratio Lower Upper
69 100
41 639.8 41.6 62.4#
39 564.3 21.8 32.8#


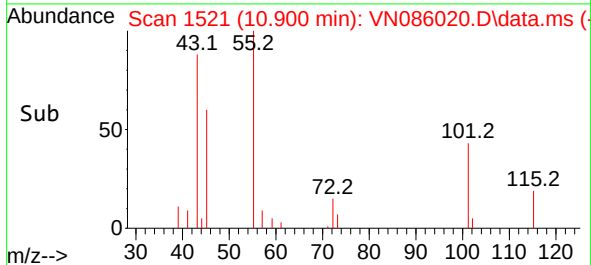






#62
4-Bromofluorobenzene
Concen: 46.493 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion: 95 Resp: 115096
Ion Ratio Lower Upper
95 100
174 79.4 0.0 156.8
176 76.4 0.0 152.2

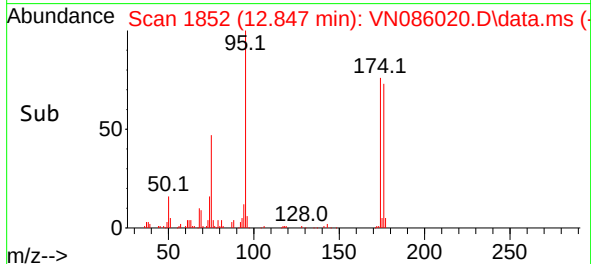

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 117 Resp: 235432
Ion Ratio Lower Upper
117 100
82 58.1 46.7 70.1
119 33.4 26.5 39.7









#67
Ethyl Benzene
Concen: 2.362 ug/l
RT: 11.959 min Scan# 1701
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion: 91 Resp: 20359
Ion Ratio Lower Upper
91 100
106 34.6 24.5 36.7

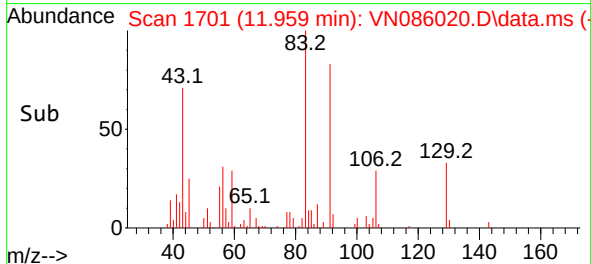

#68
m/p-Xylenes
Concen: 10.568 ug/l
RT: 12.065 min Scan# 1719
Delta R.T. -0.006 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion:106 Resp: 35797
Ion Ratio Lower Upper
106 100
91 201.2 163.9 245.9







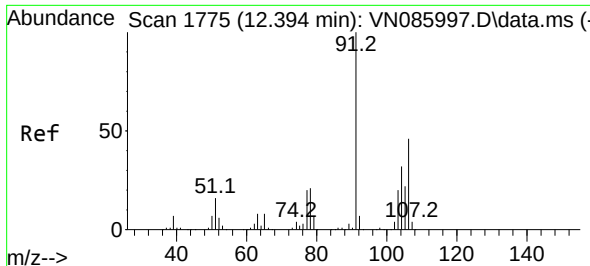

#69
o-Xylene
Concen: 5.417 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. 0.006 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion:106 Resp: 16841
Ion Ratio Lower Upper
106 100
91 222.1 109.1 327.2

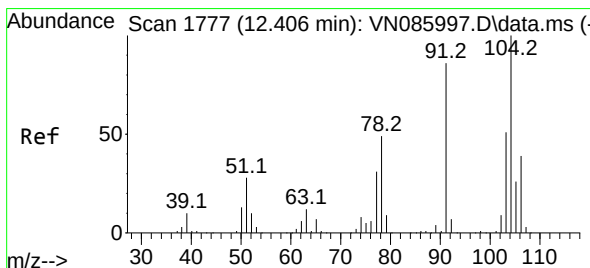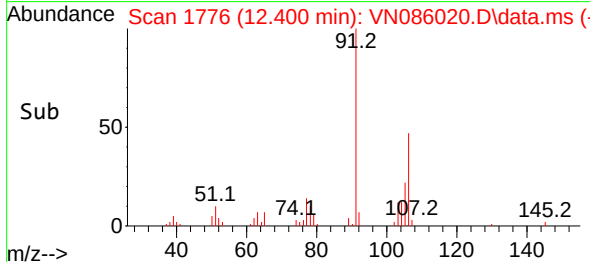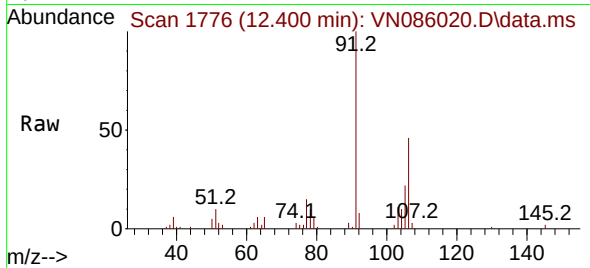

#70
Styrene
Concen: 0.944 ug/l
RT: 12.406 min Scan# 1777
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion:104 Resp: 5013
Ion Ratio Lower Upper
104 100
78 85.5 41.4 62.2#
103 92.3 42.9 64.3#

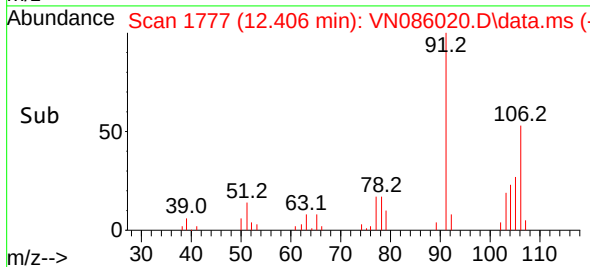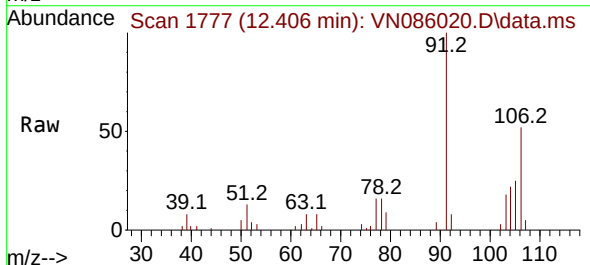



#71

Bromoform

Concen: 0.386 ug/l

RT: 12.847 min Scan# 1

Delta R.T. 0.270 min

Lab File: VN086020.D

Acq: 19 Mar 2025 19:39

Instrument :

MSVOA_N

ClientSampleId :

257952





Tgt Ion:173 Resp: 647

Ion Ratio Lower Upper

173 100

175 0.0 24.3 73.0#

254 0.0 0.0 0.0



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.788 min Scan# 2012

Delta R.T. -0.000 min

Lab File: VN086020.D

Acq: 19 Mar 2025 19:39




Tgt Ion:152 Resp: 103166


Ion Ratio Lower Upper

152 100

115 62.0 31.1 93.2

150 157.5 0.0 359.6









#73
Isopropylbenzene
Concen: 0.552 ug/l
RT: 12.688 min Scan# 1785
Delta R.T. -0.006 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion:105 Resp: 3890
Ion Ratio Lower Upper
105 100
120 27.0 13.0 39.0

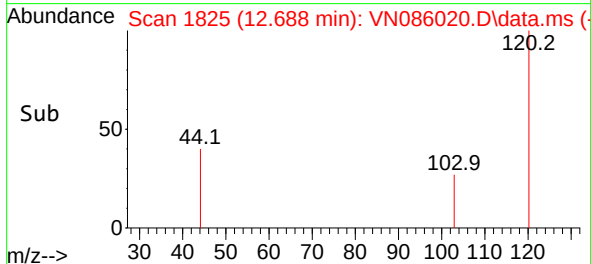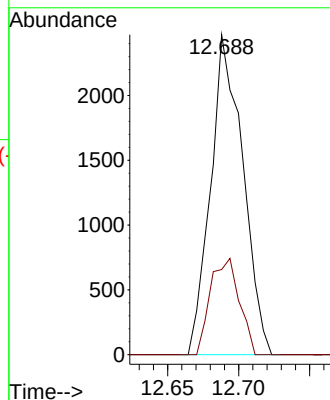

#74
N-ethyl acetate
Concen: 0.557 ug/l
RT: 12.453 min Scan# 1785
Delta R.T. -0.041 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 43 Resp: 1314
Ion Ratio Lower Upper
43 100
70 0.0 43.0 64.4#
55 4.9 23.8 35.8#
61 0.0 23.4 35.0#



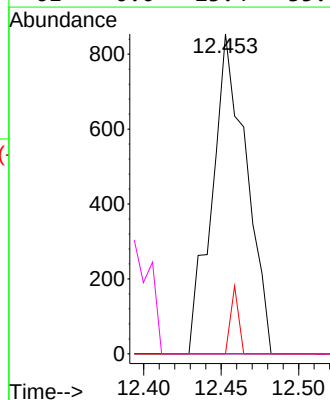





#76
1,2,3-Trichloropropane
Concen: 24.782 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.141 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion: 75 Resp: 57238
Ion Ratio Lower Upper
75 100
77 1.4 83.7 251.0#

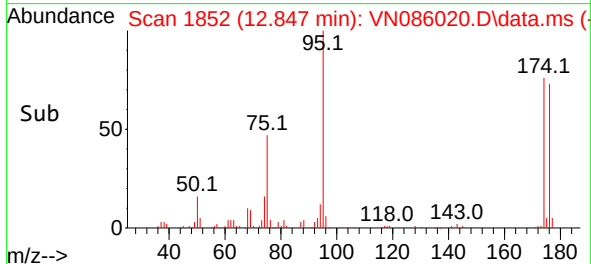

#78
n-propylbenzene
Concen: 0.750 ug/l
RT: 13.035 min Scan# 1884
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 91 Resp: 5984
Ion Ratio Lower Upper
91 100
120 27.6 11.7 35.0









#79
2-Chlorotoluene
Concen: 0.578 ug/l
RT: 13.100 min Scan# 11
Delta R.T. -0.024 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion: 91 Resp: 3062
Ion Ratio Lower Upper
91 100
126 0.0 16.4 49.2#

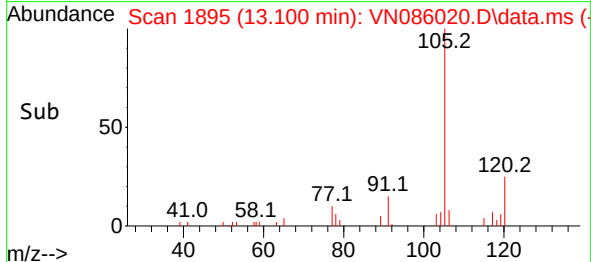

#80
1,3,5-Trimethylbenzene
Concen: 2.289 ug/l
RT: 13.170 min Scan# 1907
Delta R.T. -0.000 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 105 Resp: 13614
Ion Ratio Lower Upper
105 100
120 44.3 23.7 71.1




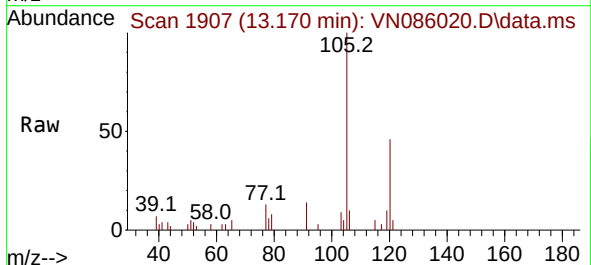


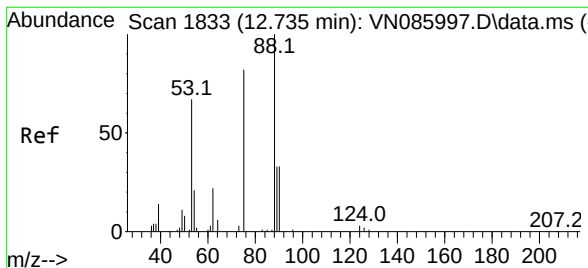

#81
trans-1,4-Dichloro-2-butene
Concen: 65.519 ug/l
RT: 12.847 min Scan# 11
Delta R.T. 0.112 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39




Instrument :
MSVOA_N
ClientSampleId :
257952


Tgt Ion: 75 Resp: 57238
Ion Ratio Lower Upper
75 100
53 0.0 66.0 99.0#
89 0.0 36.9 55.3#

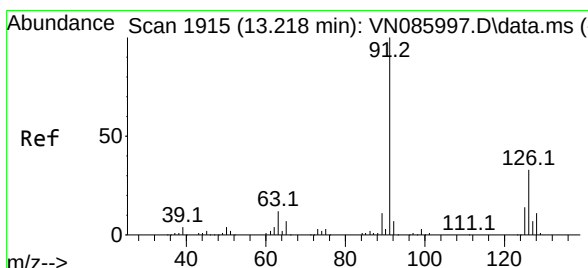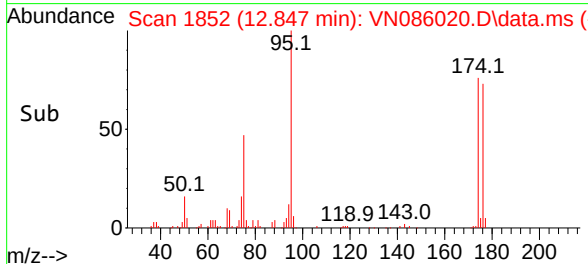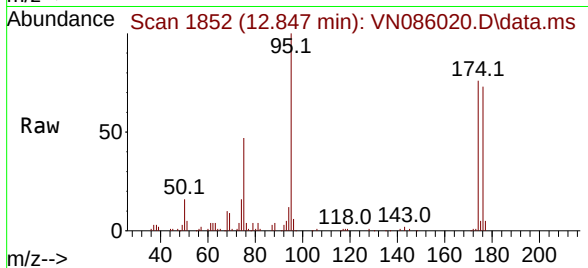

#82
4-Chlorotoluene
Concen: 0.324 ug/l
RT: 13.170 min Scan# 1907
Delta R.T. -0.047 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion: 91 Resp: 1766
Ion Ratio Lower Upper
91 100
126 0.0 16.1 48.2#


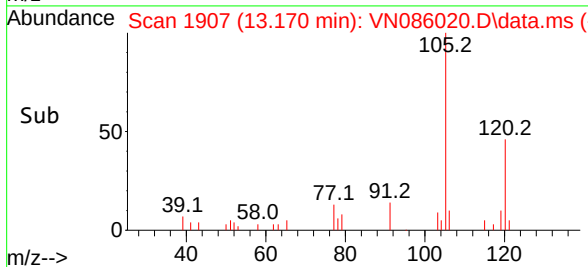

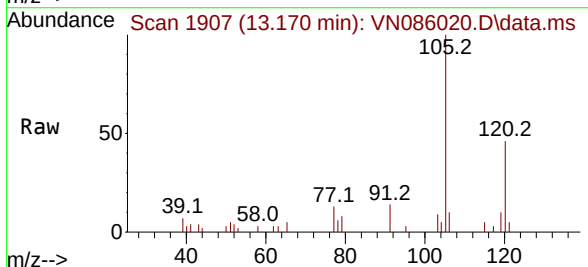




#84
 1,2,4-Trimethylbenzene
 Concen: 4.427 ug/l
 RT: 13.476 min Scan# 1959
 Delta R.T. -0.000 min
 Lab File: VN086020.D
 Acq: 19 Mar 2025 19:39




Instrument :
 MSVOA_N
 ClientSampleId :
 257952


Tgt Ion:105 Resp: 26556
 Ion Ratio Lower Upper
 105 100
 120 45.2 21.9 65.8

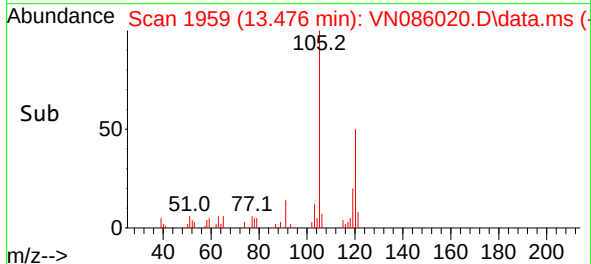

#86
 p-Isopropyltoluene
 Concen: 0.294 ug/l
 RT: 13.723 min Scan# 2001
 Delta R.T. -0.006 min
 Lab File: VN086020.D
 Acq: 19 Mar 2025 19:39

Tgt Ion:119 Resp: 1650
 Ion Ratio Lower Upper
 119 100
 134 21.8 12.6 37.8
 91 18.2 12.3 36.8




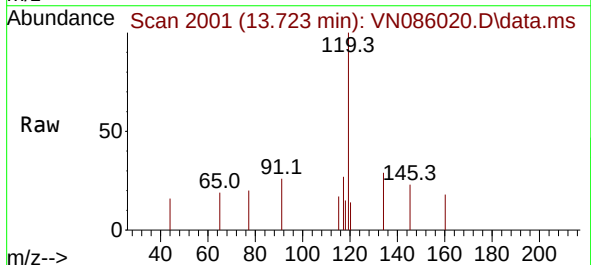




#90
Hexachloroethane
Concen: 0.301 ug/l
RT: 14.323 min Scan# 2103
Delta R.T. -0.006 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Instrument :
MSVOA_N
ClientSampleId :
257952

Tgt Ion:117 Resp: 390
Ion Ratio Lower Upper
117 100
201 0.0 39.1 117.3#

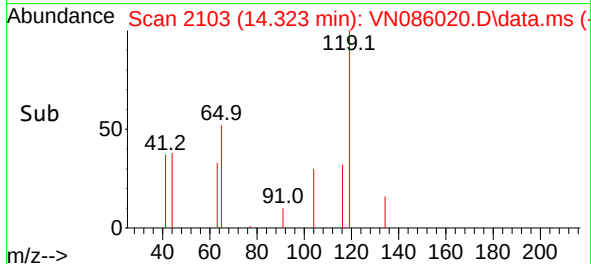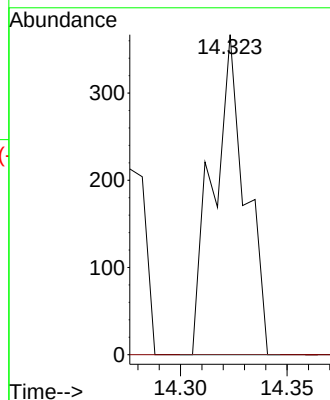

#95
Naphthalene
Concen: 5.142 ug/l
RT: 15.635 min Scan# 2326
Delta R.T. -0.006 min
Lab File: VN086020.D
Acq: 19 Mar 2025 19:39

Tgt Ion:128 Resp: 26355
Ion Ratio Lower Upper
128 100
127 13.0 10.2 15.4
129 11.1 9.0 13.6

