

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031925\
 Data File : VN086014.D
 Acq On : 19 Mar 2025 17:14
 Operator : JC\MD
 Sample : PB167194ZHE#04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB167194ZHE#04

Quant Time: Mar 20 01:34:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 19 03:20:56 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	139880	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	251910	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	243462	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	92960	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	105080	54.860	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 109.720%	
35) Dibromofluoromethane	8.165	113	88435	50.296	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.600%	
50) Toluene-d8	10.565	98	325939	51.076	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.160%	
62) 4-Bromofluorobenzene	12.847	95	100322	44.082	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 88.160%	
Target Compounds						
					Qvalue	
16) Acetone	4.436	43	17639	30.143	ug/l	95
20) Methylene Chloride	5.271	84	3616	2.112	ug/l #	78
25) 2-Butanone	7.483	43	13854	16.407	ug/l	91
43) Isopropyl Acetate	8.688	43	81448	19.243	ug/l #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031925\
Data File : VN086014.D
Acq On : 19 Mar 2025 17:14
Operator : JC\MD
Sample : PB167194ZHE#04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB167194ZHE#04

Quant Time: Mar 20 01:34:38 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 19 03:20:56 2025
Response via : Initial Calibration



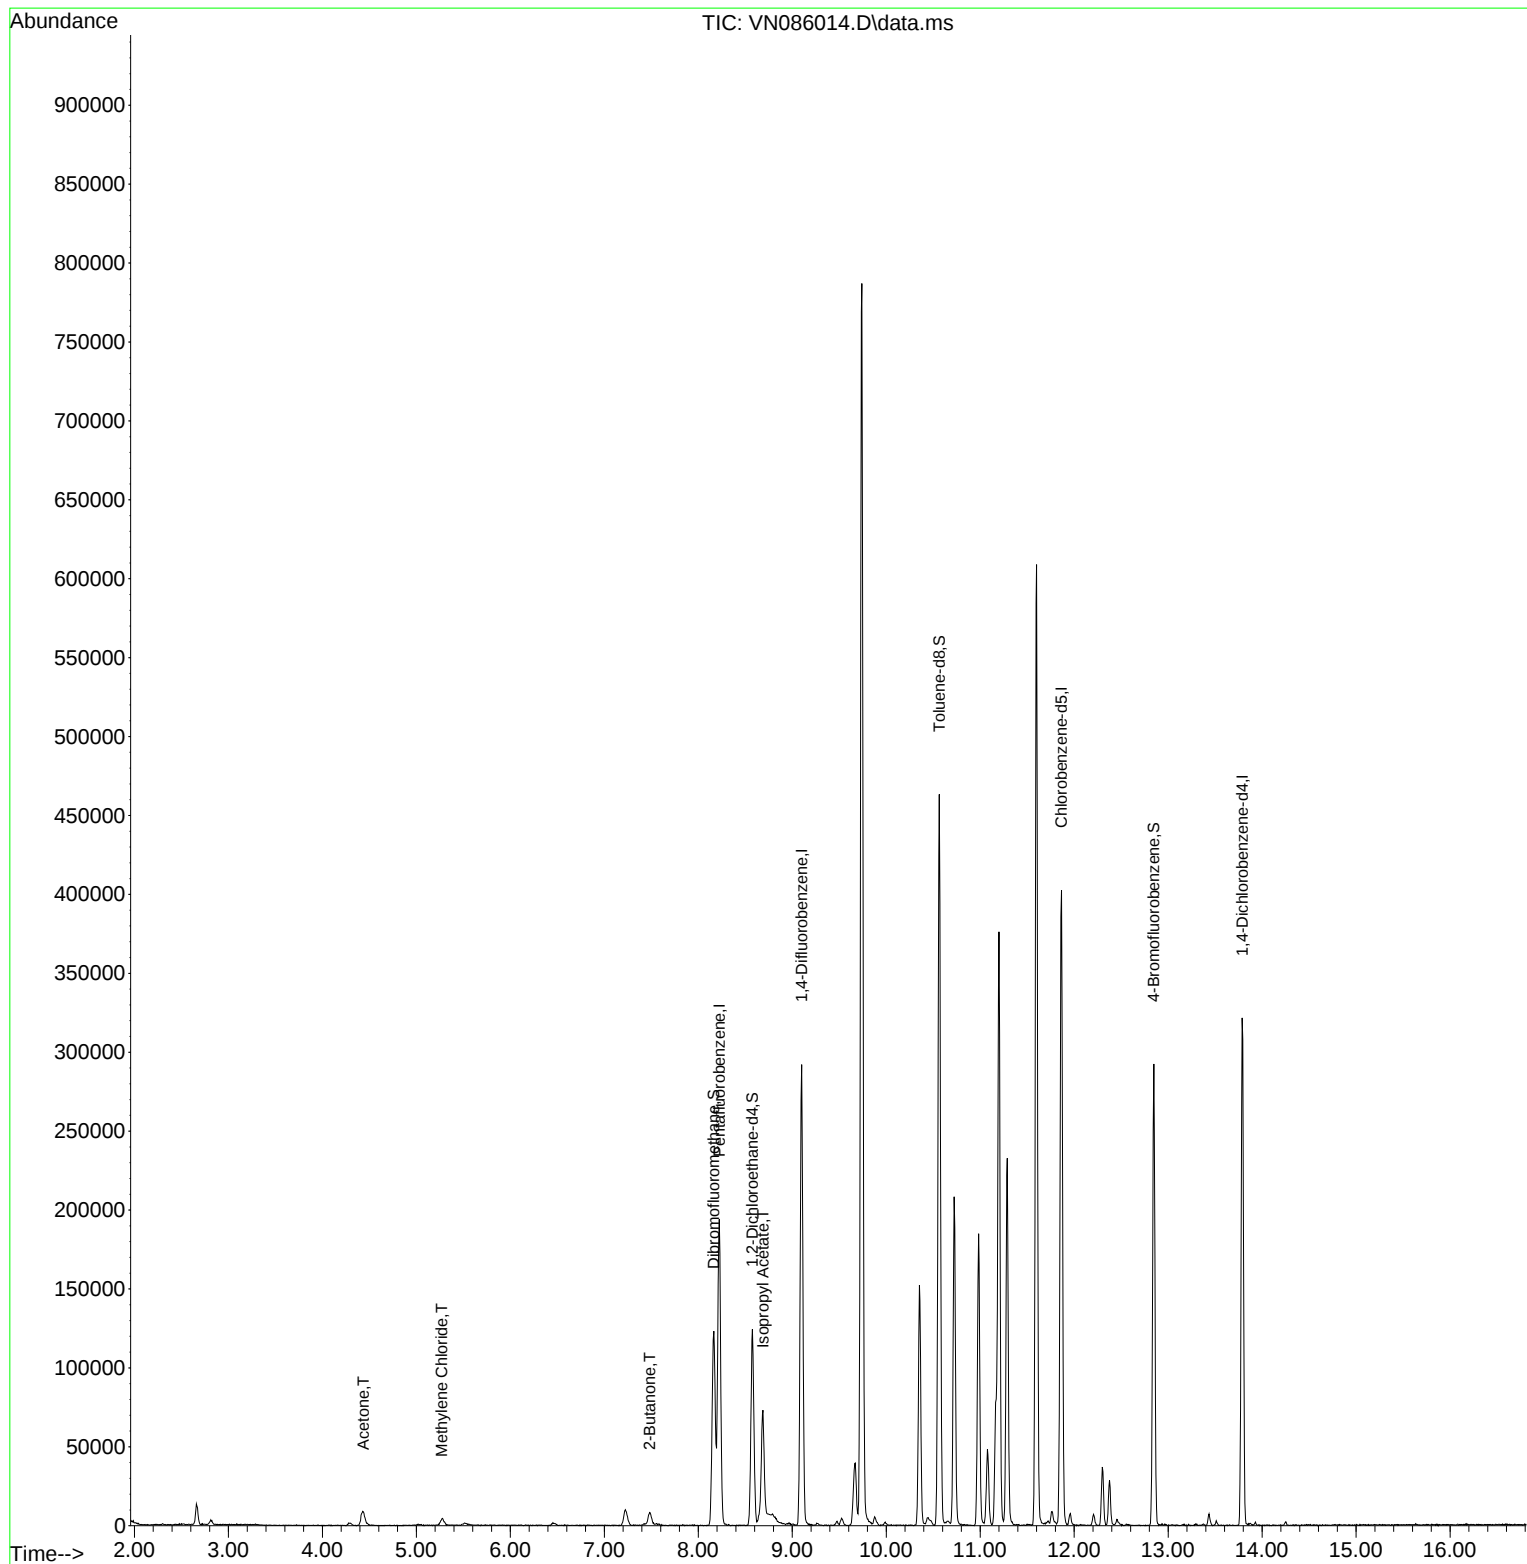


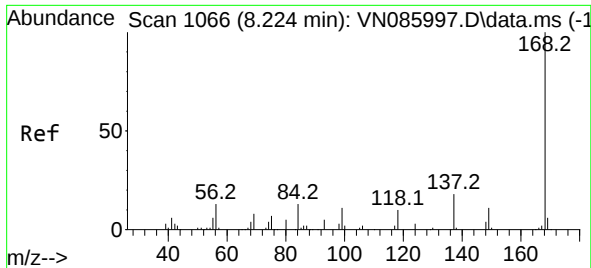

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN086014.D
Acq: 19 Mar 2025 17:14




Instrument :
MSVOA_N
ClientSampleId :
PB167194ZHE#04

Tgt Ion:168 Resp: 139880
Ion Ratio Lower Upper
168 100
99 58.6 49.4 74.2

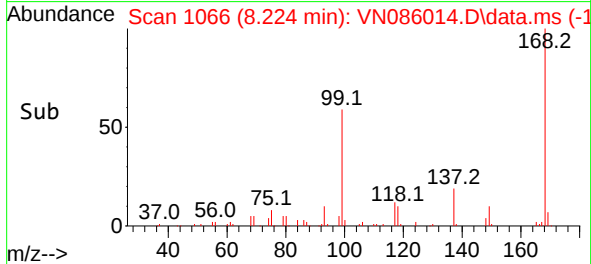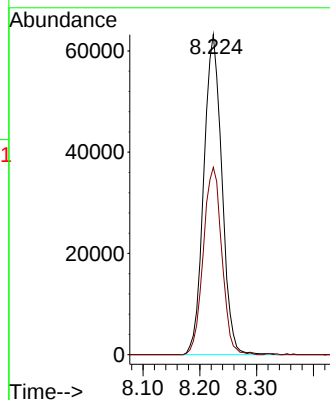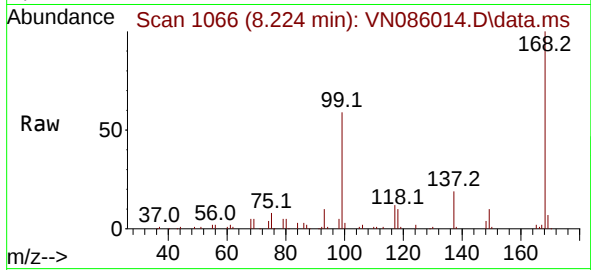

#16
Acetone
Concen: 30.143 ug/l
RT: 4.436 min Scan# 422
Delta R.T. 0.012 min
Lab File: VN086014.D
Acq: 19 Mar 2025 17:14


Tgt Ion: 43 Resp: 17639
Ion Ratio Lower Upper
43 100
58 33.9 29.4 44.2

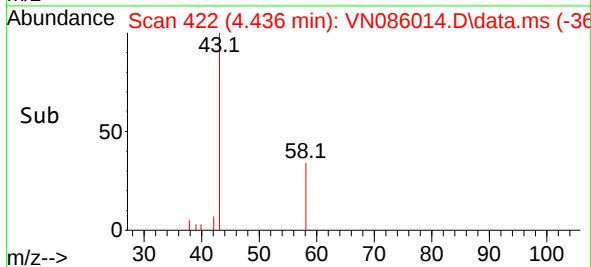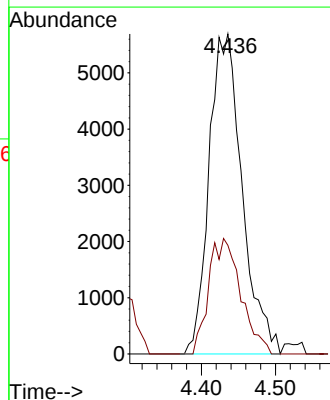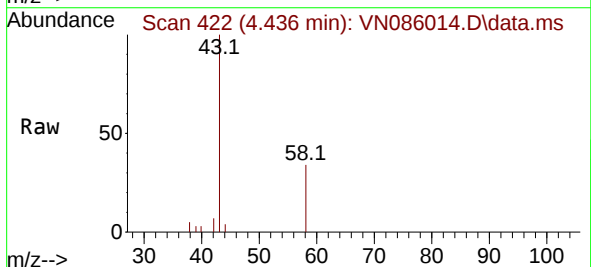






#20
Methylene Chloride
Concen: 2.112 ug/l
RT: 5.271 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN086014.D
Acq: 19 Mar 2025 17:14

Instrument :
MSVOA_N
ClientSampleId :
PB167194ZHE#04



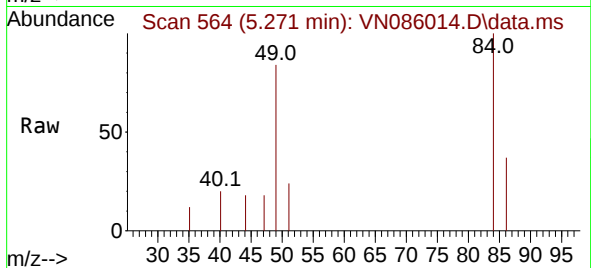



Tgt Ion: 84	Resp: 3616
Ion Ratio	Lower Upper
84 100	
49 83.7	83.3 124.9
51 24.3	24.8 37.2#
86 37.5	48.7 73.1#

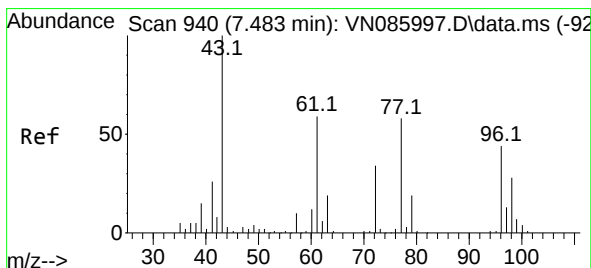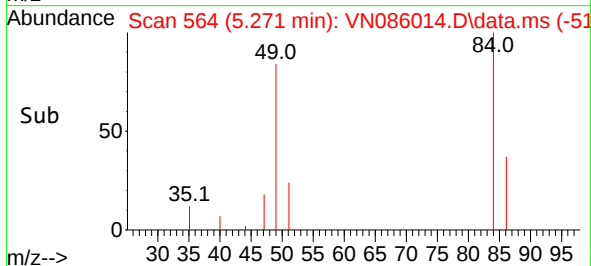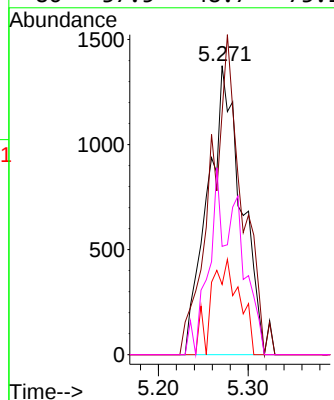

#25
2-Butanone
Concen: 16.407 ug/l
RT: 7.483 min Scan# 940
Delta R.T. -0.000 min
Lab File: VN086014.D
Acq: 19 Mar 2025 17:14

Tgt Ion: 43	Resp: 13854
Ion Ratio	Lower Upper
43 100	
72 29.3	27.4 41.0

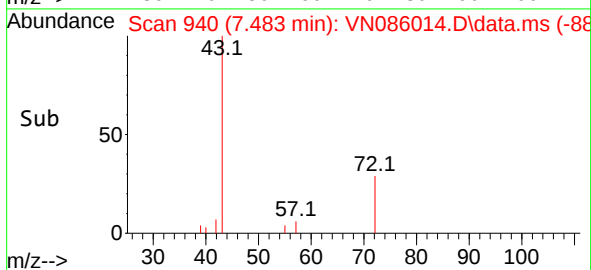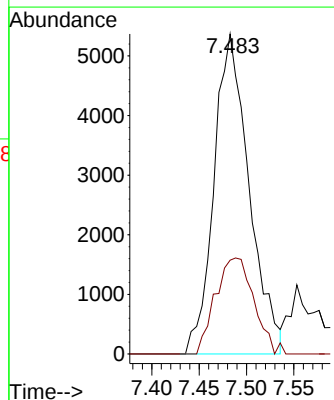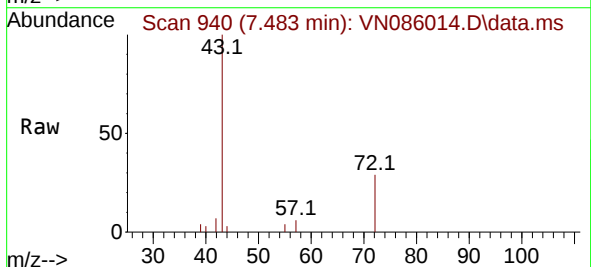

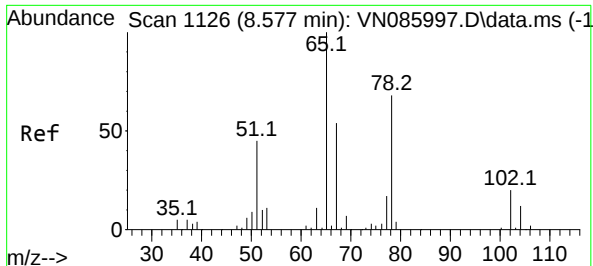

#33

1,2-Dichloroethane-d4

Concen: 54.860 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VN086014.D

Acq: 19 Mar 2025 17:14

Instrument :

MSVOA_N

ClientSampleId :





PB167194ZHE#04

Tgt Ion: 65 Resp: 105080

Ion Ratio Lower Upper

65 100

67 52.6 0.0 102.2

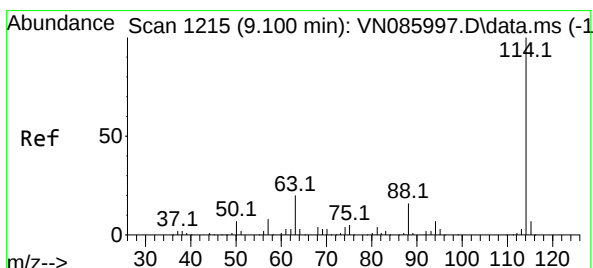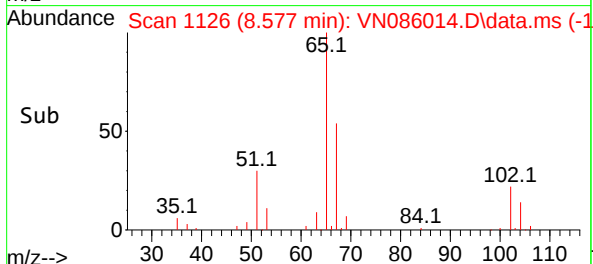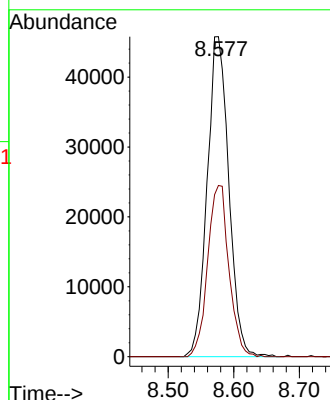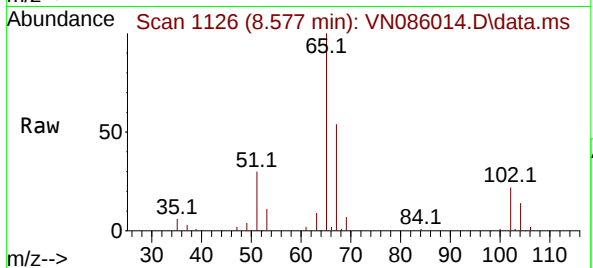

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. -0.000 min

Lab File: VN086014.D

Acq: 19 Mar 2025 17:14




Tgt Ion: 114 Resp: 251910

Ion Ratio Lower Upper

114 100

63 19.9 0.0 39.6

88 16.3 0.0 32.6


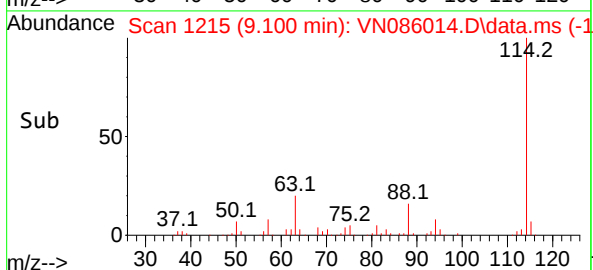
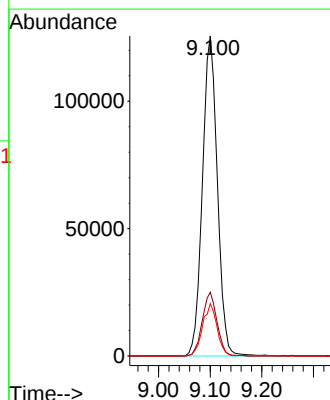
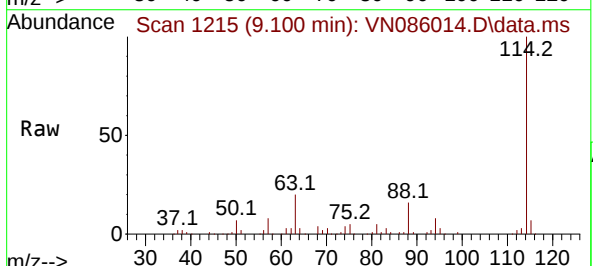




#35
Dibromofluoromethane
Concen: 50.296 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN086014.D
Acq: 19 Mar 2025 17:14




Instrument :
MSVOA_N
ClientSampleId :
PB167194ZHE#04


Tgt Ion:113 Resp: 88435
Ion Ratio Lower Upper
113 100
111 104.0 81.8 122.8
192 18.9 15.9 23.9

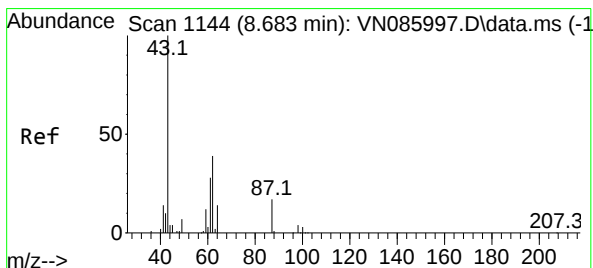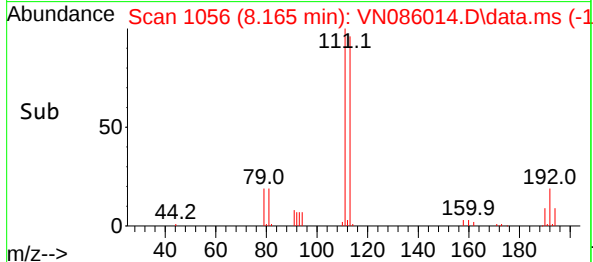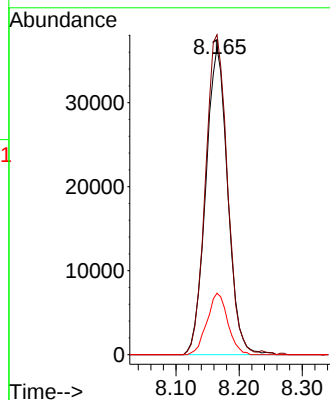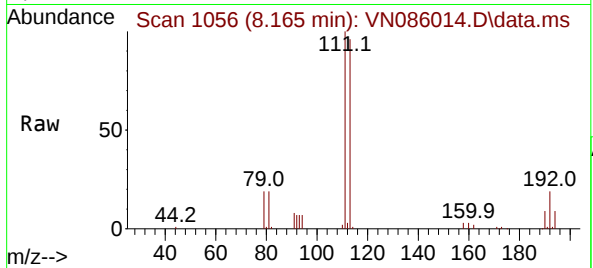

#43
Isopropyl Acetate
Concen: 19.243 ug/l
RT: 8.688 min Scan# 1145
Delta R.T. 0.006 min
Lab File: VN086014.D
Acq: 19 Mar 2025 17:14

Tgt Ion: 43 Resp: 81448
Ion Ratio Lower Upper
43 100
61 19.7 25.0 37.6#
87 14.4 13.0 19.4


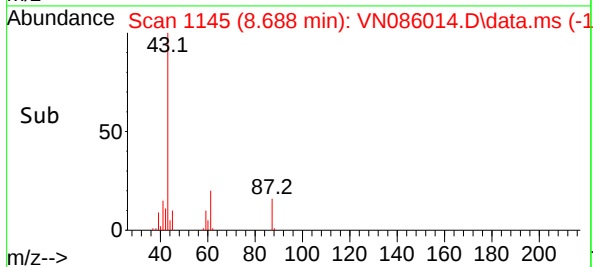
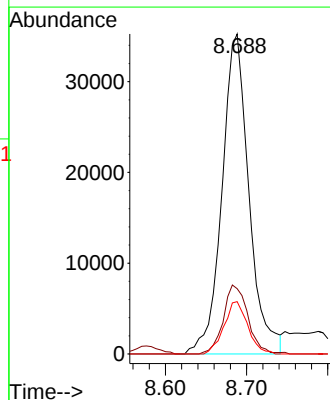
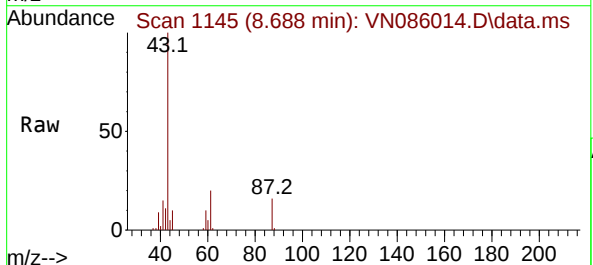


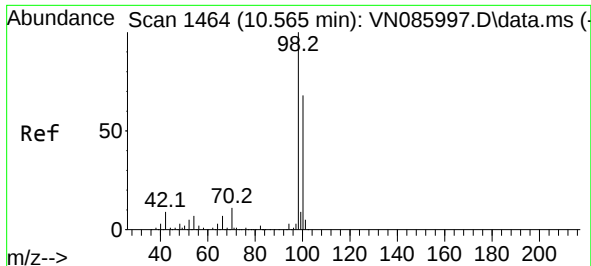

#50
Toluene-d8
Concen: 51.076 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN086014.D
Acq: 19 Mar 2025 17:14




Instrument :
MSVOA_N
ClientSampleId :
PB167194ZHE#04


Tgt Ion: 98 Resp: 325939
Ion Ratio Lower Upper
98 100
100 64.6 53.1 79.7

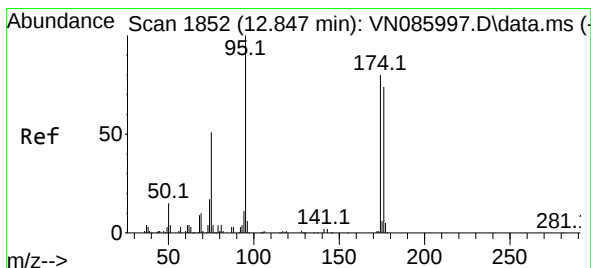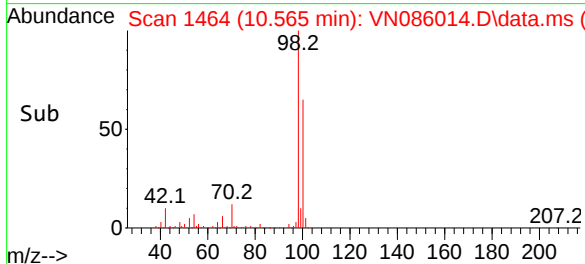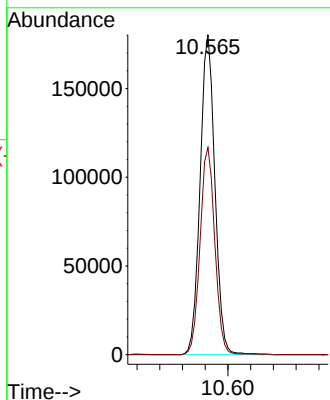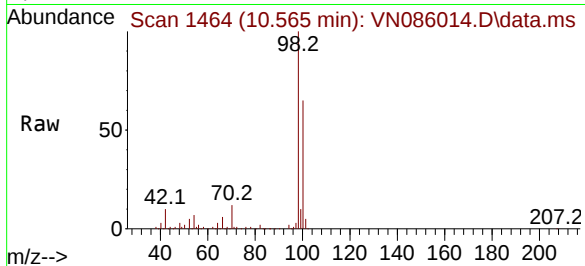

#62
4-Bromofluorobenzene
Concen: 44.082 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086014.D
Acq: 19 Mar 2025 17:14

Tgt Ion: 95 Resp: 100322
Ion Ratio Lower Upper
95 100
174 82.2 0.0 156.8
176 77.5 0.0 152.2


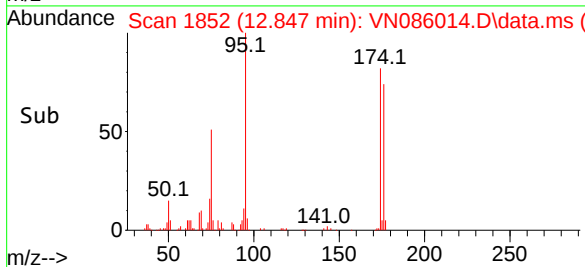
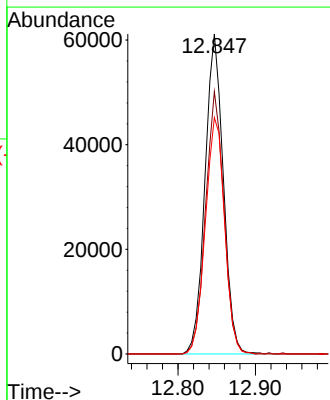
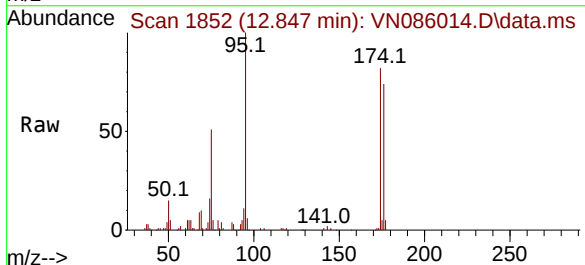


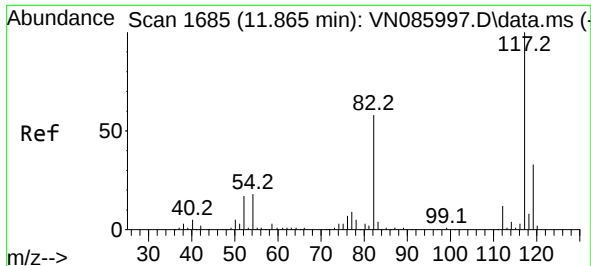

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086014.D
Acq: 19 Mar 2025 17:14

Instrument :
MSVOA_N
ClientSampleId :
PB167194ZHE#04

Tgt Ion:117 Resp: 243462
Ion Ratio Lower Upper
117 100
82 56.7 46.7 70.1
119 32.0 26.5 39.7

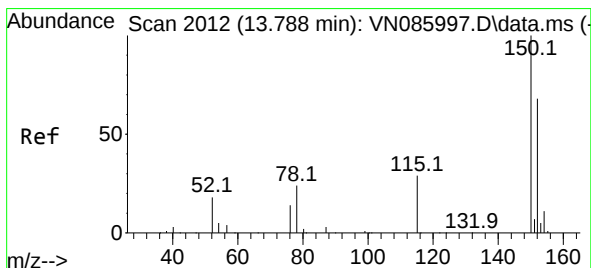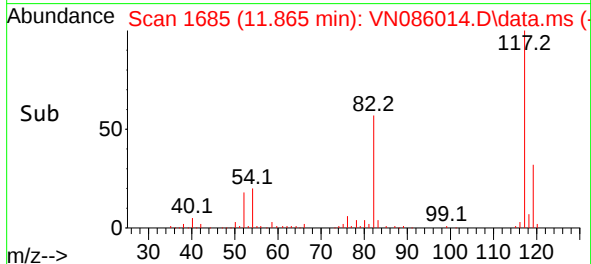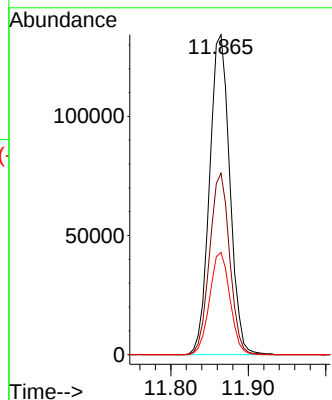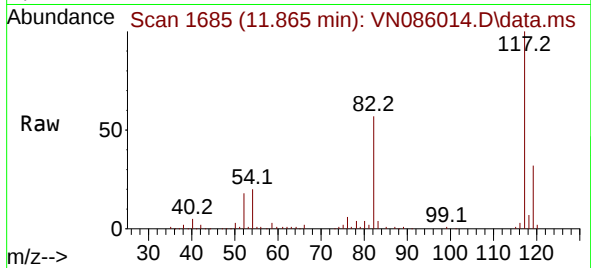

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN086014.D
Acq: 19 Mar 2025 17:14

Tgt Ion:152 Resp: 92960
Ion Ratio Lower Upper
152 100
115 62.0 31.1 93.2
150 159.4 0.0 359.6

