


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031925\
Data File : VN086004.D
Acq On : 19 Mar 2025 12:30
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Title : SW846 8260
Last Update : Wed Mar 19 03:20:56 2025

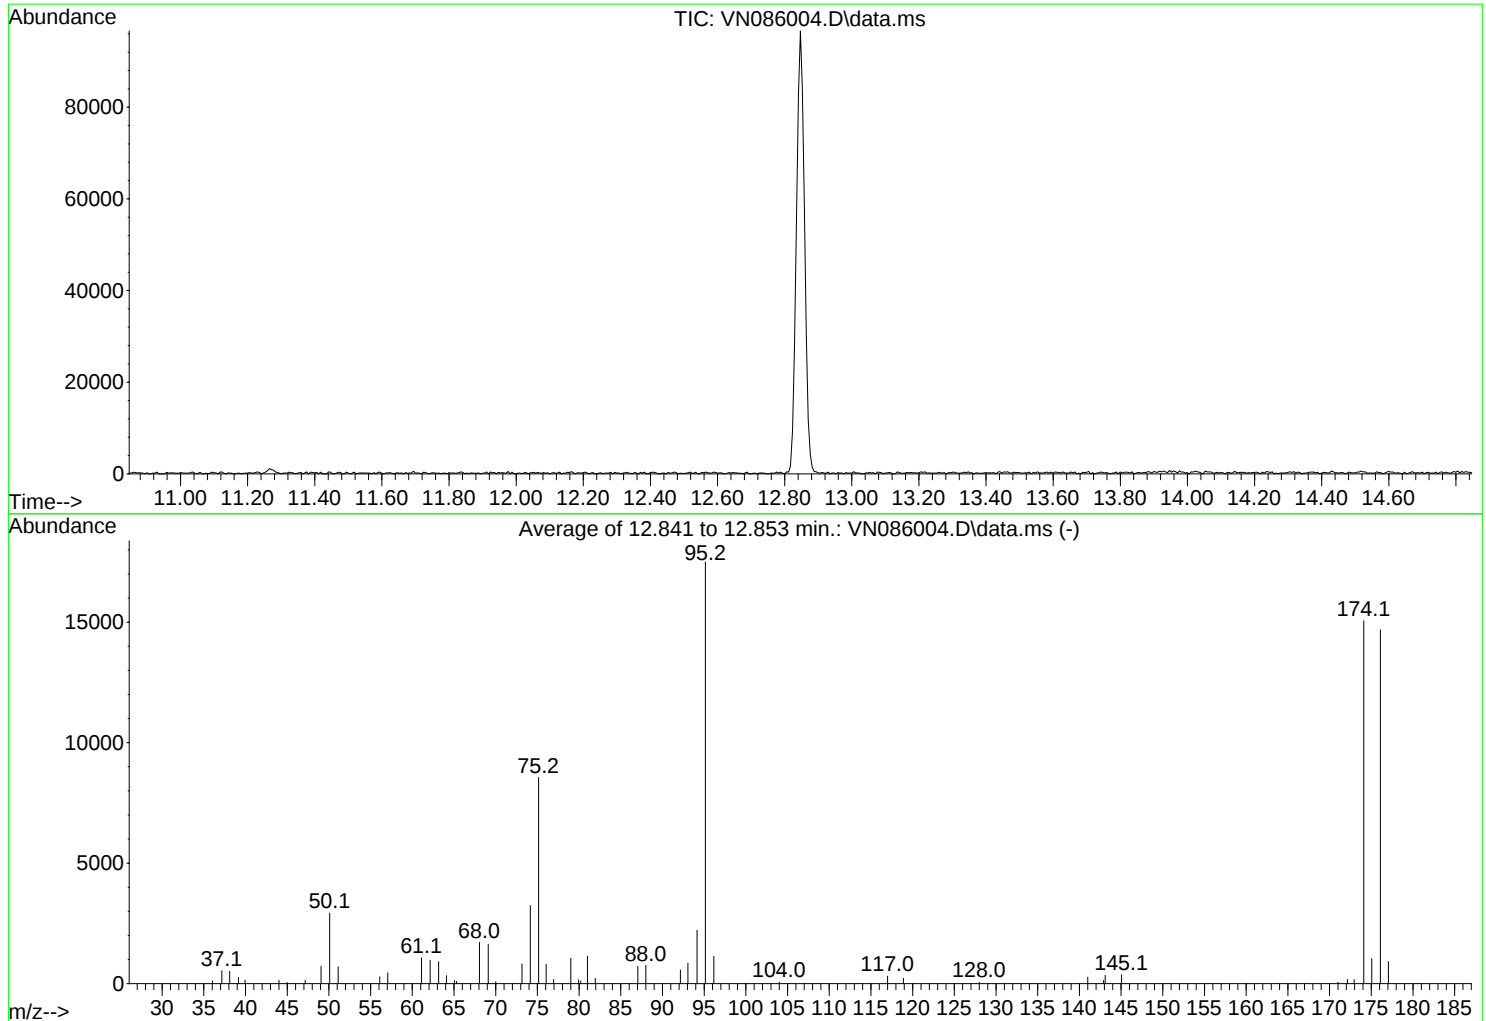

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	2929	PASS
75	95	30	60	48.9	8557	PASS
95	95	100	100	100.0	17503	PASS
96	95	5	9	6.5	1133	PASS
173	174	0.00	2	1.1	168	PASS
174	95	50	100	86.0	15056	PASS
175	174	5	9	6.9	1039	PASS
176	174	95	101	97.5	14678	PASS
177	176	5	9	6.2	915	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	121	56.10	285	73.15	818	88.00	754
37.15	538	57.05	450	74.15	3242	92.15	560
38.10	513	61.10	1068	75.15	8557	93.05	853
39.15	267	62.15	962	76.05	809	94.15	222
39.95	144	63.15	908	76.95	174	95.15	17503
44.00	138	64.10	331	79.00	1050	96.15	1133
45.00	50	65.05	126	79.95	161	104.00	58
47.15	131	65.30	92	80.20	108	117.00	313
49.05	721	68.05	1712	81.00	1145	118.90	220
50.10	2929	69.10	1636	81.95	213	128.00	55
51.10	705	70.00	78	87.05	717	141.00	269

Average of 12.841 to 12.853 min.: VN086004.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.90	138						
143.10	346						
145.05	363						
171.00	57						
172.15	172						
172.95	168						
174.10	15056						
175.05	1039						
176.10	14678						
177.05	915						

Instrument :

MSVOA_N

ClientSampleId :

BFB