


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN032019\
Data File : VN054455.D
Acq On : 20 Mar 2019 9:39
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032019W.M
Title : SW846 8260
Last Update : Fri Mar 22 02:09:07 2019

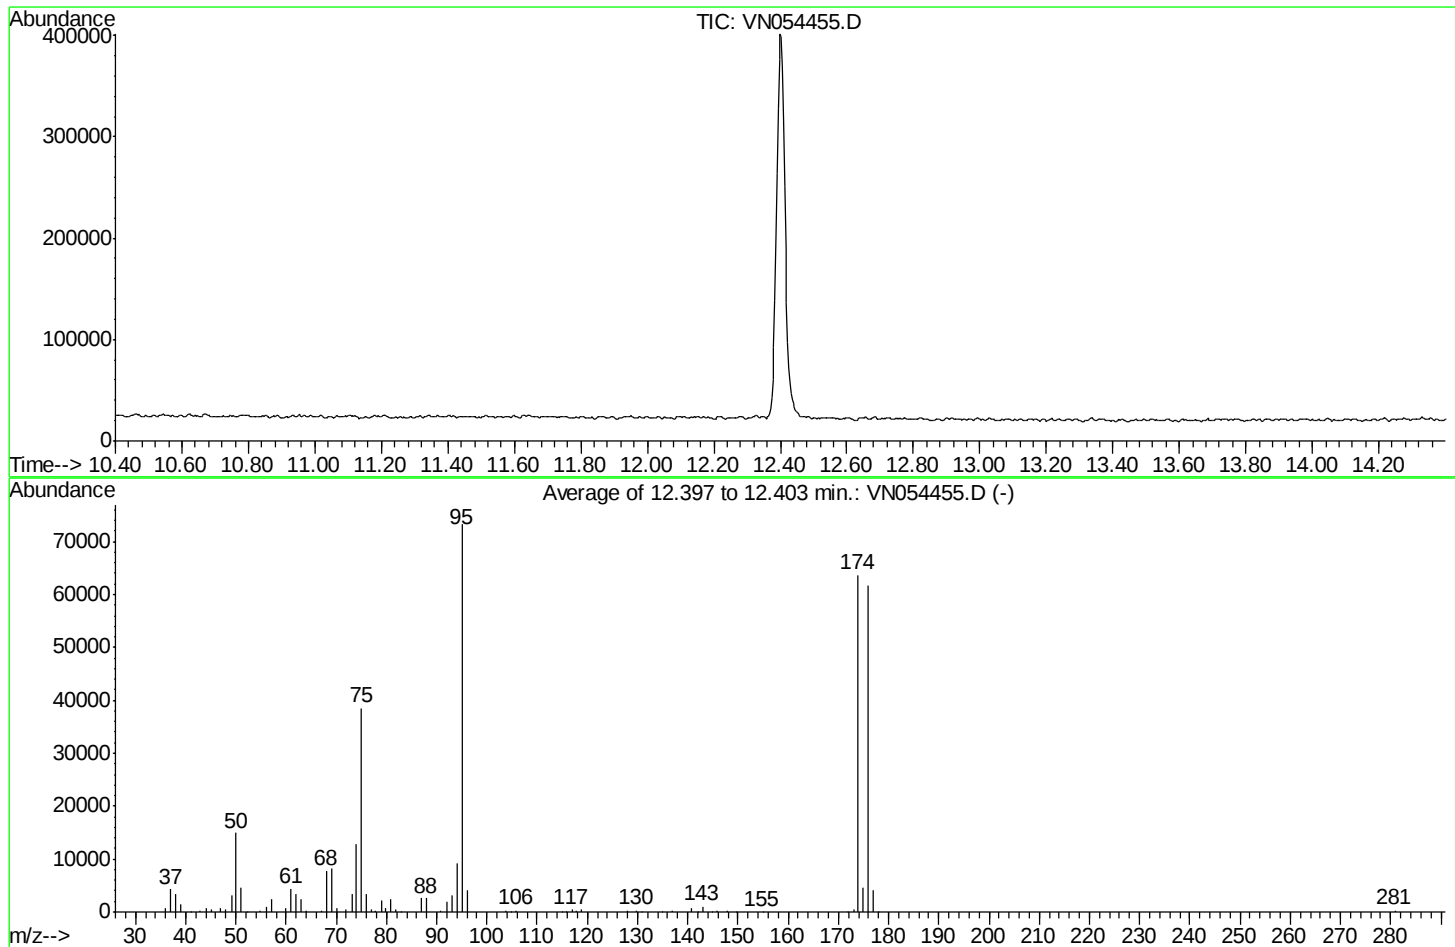

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	14967	PASS
75	95	30	60	52.6	38509	PASS
95	95	100	100	100.0	73264	PASS
96	95	5	9	5.8	4222	PASS
173	174	0.00	2	0.9	591	PASS
174	95	50	100	87.0	63725	PASS
175	174	5	9	7.3	4625	PASS
176	174	95	101	96.7	61645	PASS
177	176	5	9	6.7	4100	PASS