


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN032019\  
 Data File : VN054478.D  
 Acq On : 20 Mar 2019 22:24  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N032019W.M  
 Title : SW846 8260  
 Last Update : Fri Mar 22 02:09:07 2019

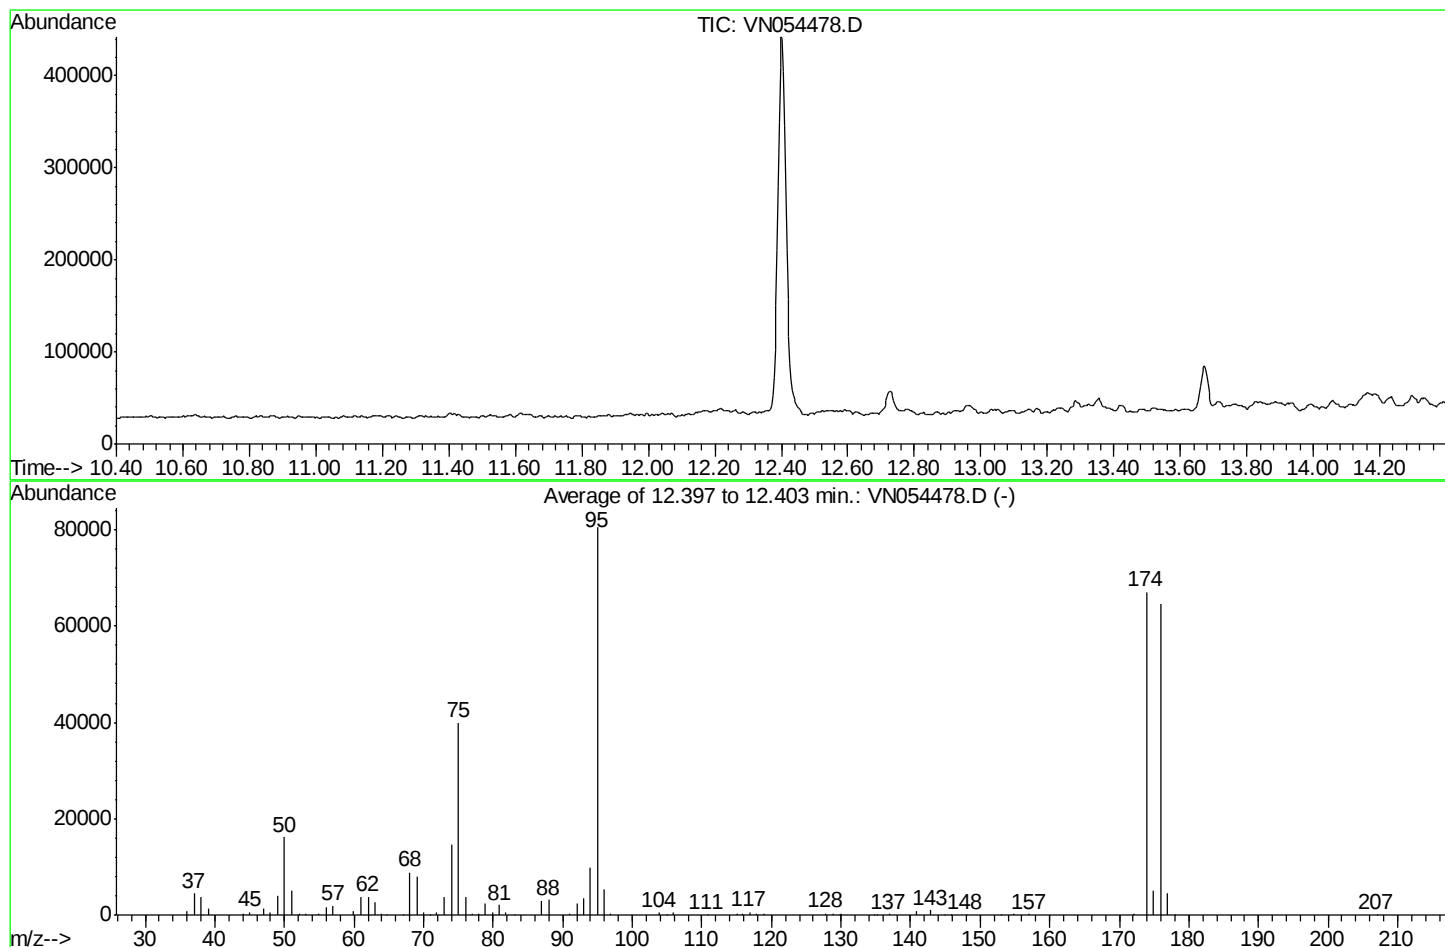

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3289

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 20.0      | 16100   | PASS             |
| 75          | 95           | 30           | 60           | 49.7      | 40002   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 80525   | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 5223    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 83.4      | 67136   | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 4935    | PASS             |
| 176         | 174          | 95           | 101          | 96.3      | 64648   | PASS             |
| 177         | 176          | 5            | 9            | 7.2       | 4652    | PASS             |