


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032020\
 Data File : VN060645.D
 Acq On : 20 Mar 2020 8:53
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
 Title : SW846 8260
 Last Update : Wed Mar 18 08:49:09 2020

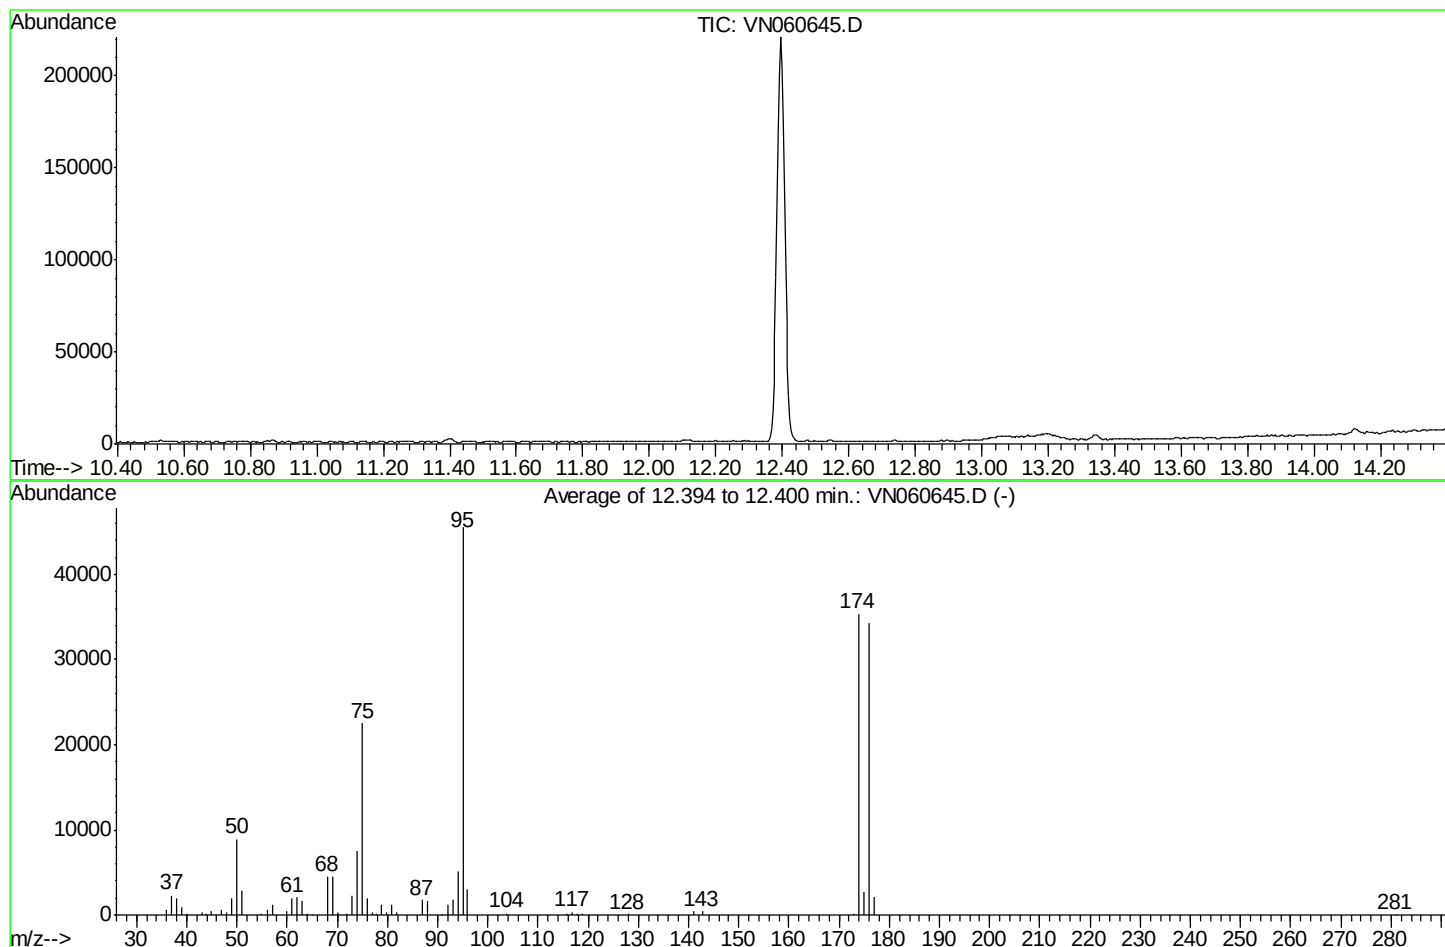

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	8928	PASS
75	95	30	60	49.5	22552	PASS
95	95	100	100	100.0	45536	PASS
96	95	5	9	6.7	3034	PASS
173	174	0.00	2	0.3	120	PASS
174	95	50	100	77.7	35402	PASS
175	174	5	9	7.6	2679	PASS
176	174	95	101	96.9	34288	PASS
177	176	5	9	6.2	2142	PASS