
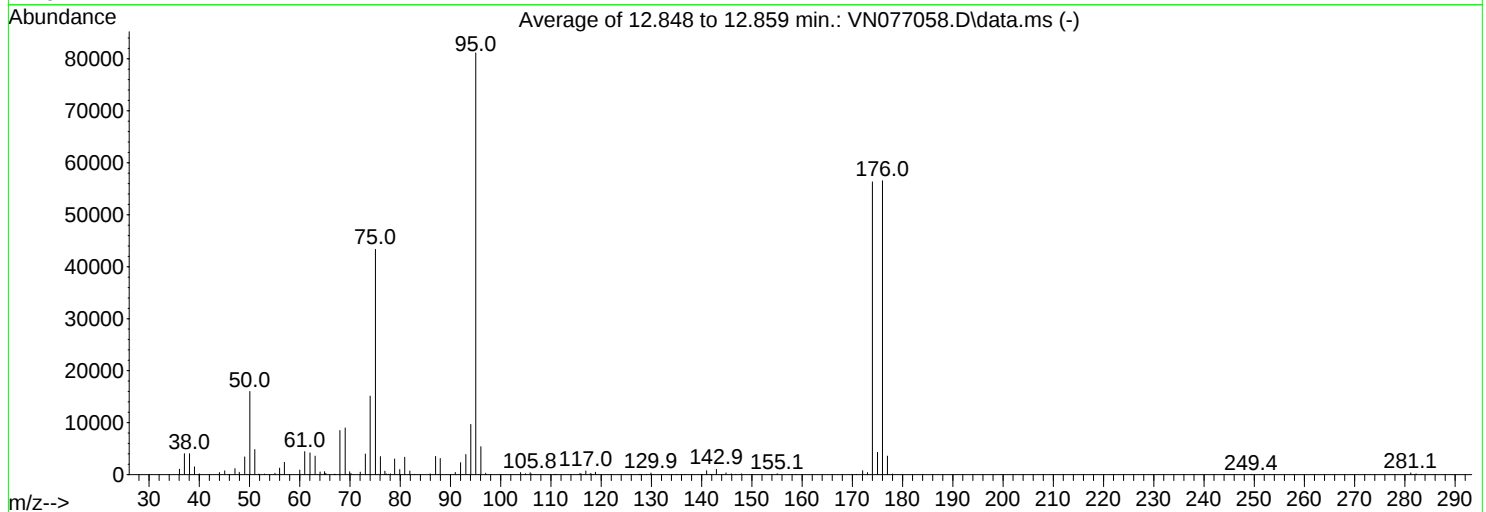


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032023\
Data File : VN077058.D
Acq On : 20 Mar 2023 09:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031723W.M
Title : SW846 8260
Last Update : Mon Mar 20 08:50:30 2023

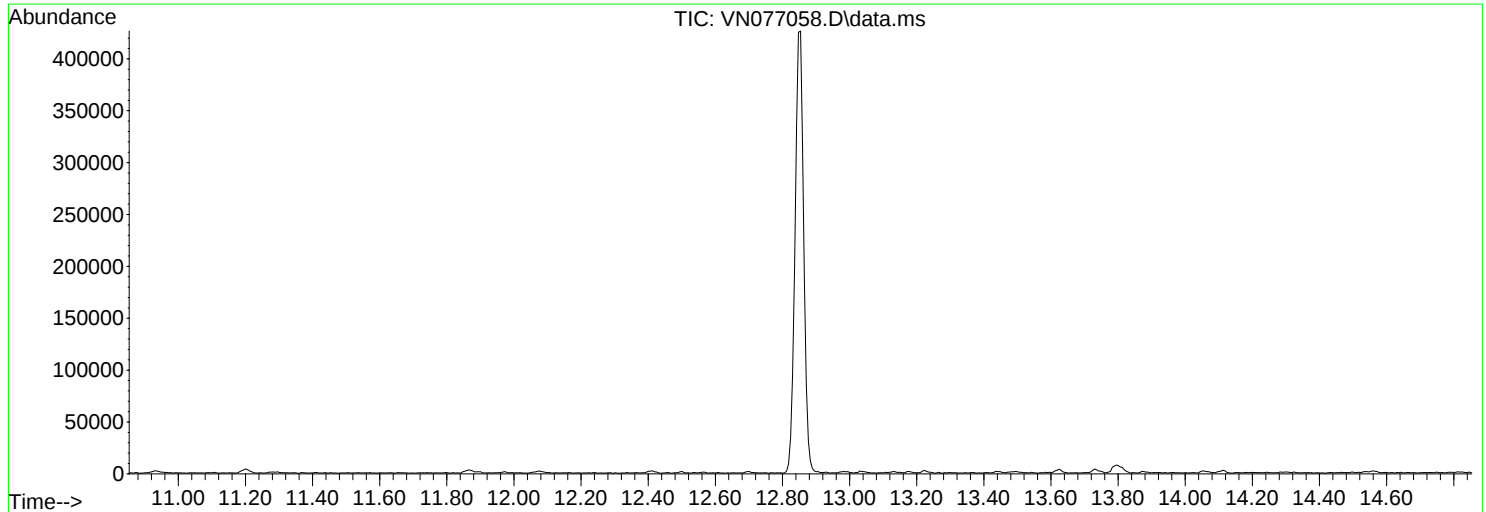

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	16007	PASS
75	95	30	60	53.4	43363	PASS
95	95	100	100	100.0	81157	PASS
96	95	5	9	6.6	5390	PASS
173	174	0.00	2	0.7	406	PASS
174	95	50	100	69.4	56333	PASS
175	174	5	9	7.6	4276	PASS
176	174	95	101	100.4	56555	PASS
177	176	5	9	6.3	3579	PASS

Average of 12.848 to 12.859 min.: VN077058.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	1038	50.05	16007	63.05	3574	73.05	398
37.05	4041	51.05	4845	64.05	533	74.00	1512
38.05	4044	51.80	105	64.95	591	75.05	4336
39.05	1518	52.00	95	65.20	253	76.05	349
40.00	153	53.00	133	66.90	83	76.95	673
44.00	419	55.05	264	67.10	62	77.20	144
45.05	729	56.00	1262	68.00	8503	77.70	98
46.00	51	56.95	2370	69.05	8994	78.05	164
47.10	1176	60.00	890	69.95	568	78.90	3027
47.95	455	61.00	4450	70.20	206	79.90	975
49.05	3408	62.05	4199	72.05	484	80.90	3355

Average of 12.848 to 12.859 min.: VN077058.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	699	97.00	289	118.10	128	144.85	334
82.80	57	103.95	406	118.85	470	145.90	162
85.95	140	104.95	180	127.60	66	146.80	53
87.05	3524	105.85	359	127.90	67	147.90	160
87.95	3123	106.10	117	129.00	53	155.05	173
90.95	438	110.80	62	129.90	302	158.80	55
92.00	2316	111.00	54	135.00	60	170.80	59
93.05	3894	115.70	141	136.70	53	172.05	760
94.05	9673	115.95	224	141.00	771	173.00	406
95.05	81157	116.95	697	141.80	67	174.00	56333
96.05	5390	117.85	222	142.95	1029	175.00	4276

Average of 12.848 to 12.859 min.: VN077058.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.00	56555						
177.00	3579						
178.00	137						
249.40	50						
281.15	328						
282.20	140						
283.30	54						