

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032024\
 Data File : VN081494.D
 Acq On : 20 Mar 2024 15:23
 Operator : JC\MD
 Sample : P1784-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TRIP-BLANK

Quant Time: Mar 21 01:20:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 19 06:00:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	523252	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	9.106	114	884284	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	775743	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	320620	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	319724	47.914	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	95.820%
35) Dibromofluoromethane	8.171	113	270746	48.514	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.020%
50) Toluene-d8	10.571	98	1037215	51.414	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.820%
62) 4-Bromofluorobenzene	12.853	95	338750	47.655	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	95.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032024\
Data File : VN081494.D
Acq On : 20 Mar 2024 15:23
Operator : JC\MD
Sample : P1784-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TRIP-BLANK

Quant Time: Mar 21 01:20:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 19 06:00:00 2024
Response via : Initial Calibration




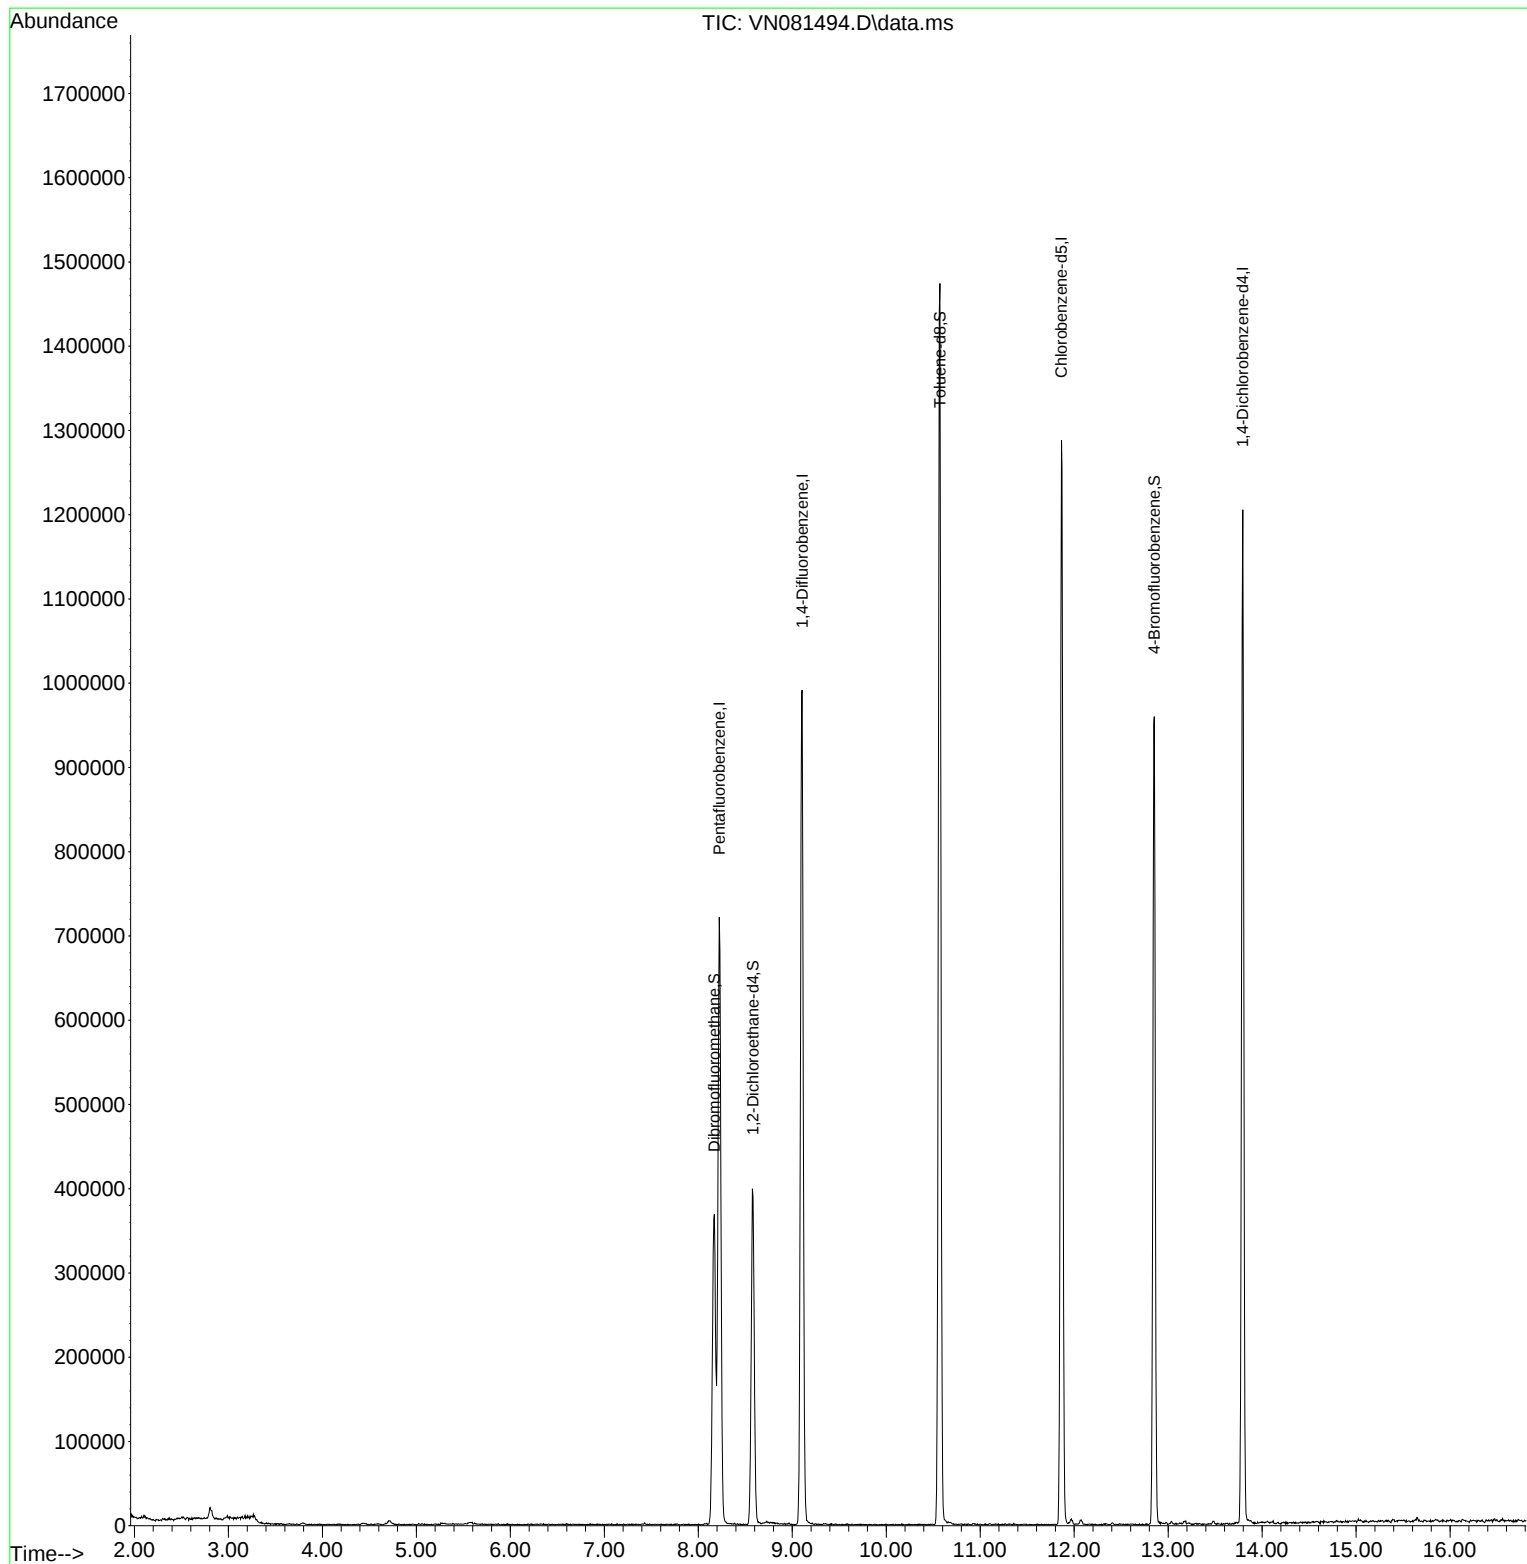


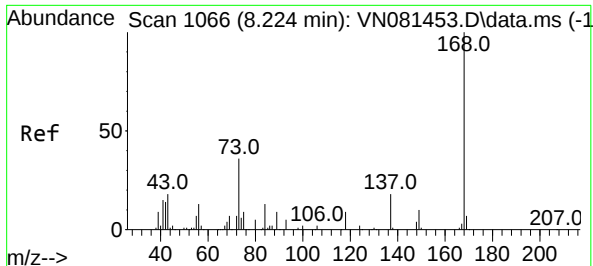

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN081494.D
Acq: 20 Mar 2024 15:23




Instrument :
MSVOA_N
ClientSampleId :
TRIP-BLANK


Tgt Ion:168 Resp: 523252
Ion Ratio Lower Upper
168 100
99 59.0 59.9 89.9#

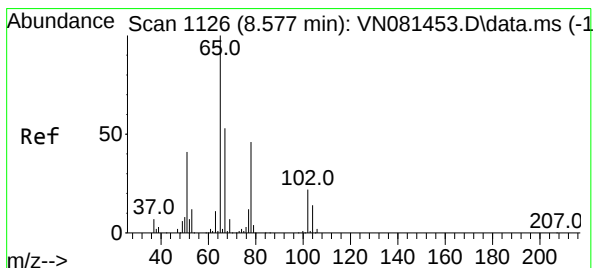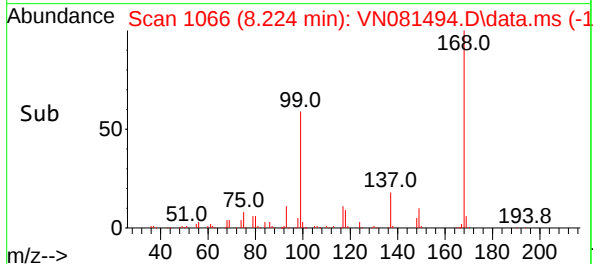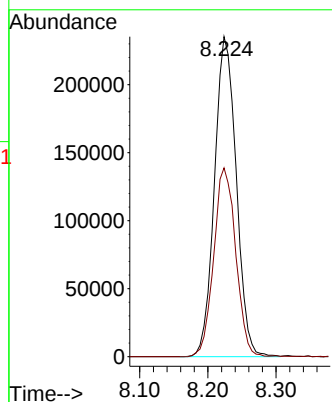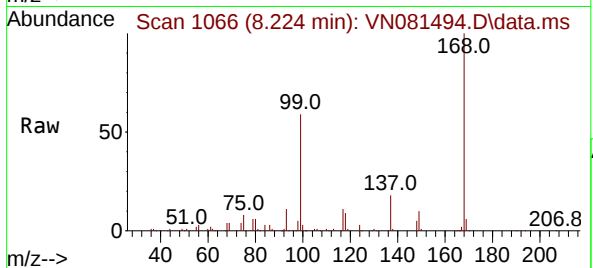

#33
1,2-Dichloroethane-d4
Concen: 47.914 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN081494.D
Acq: 20 Mar 2024 15:23

Tgt Ion: 65 Resp: 319724
Ion Ratio Lower Upper
65 100
67 52.7 0.0 102.4

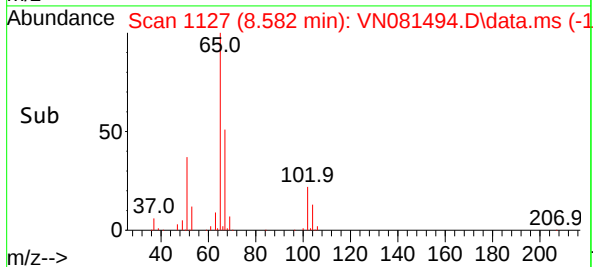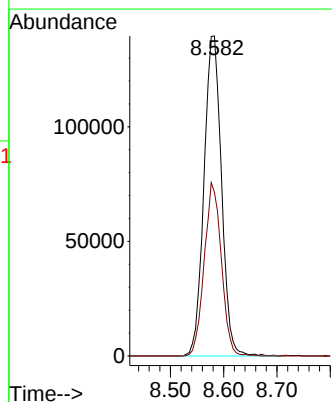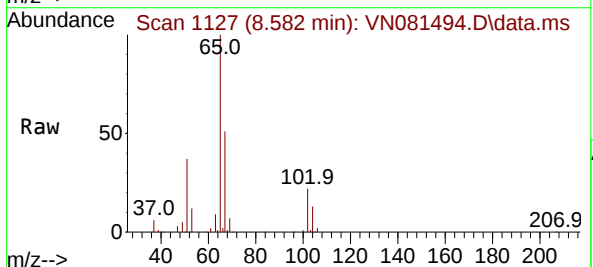

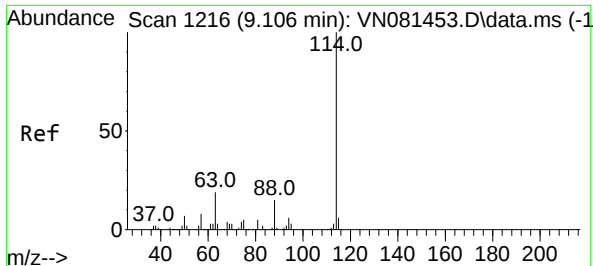

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN081494.D

Acq: 20 Mar 2024 15:23

Instrument :

MSVOA_N

ClientSampleId :

TRIP-BLANK





Tgt Ion:114 Resp: 884284

Ion Ratio Lower Upper

114 100

63 19.0 0.0 48.0

88 16.2 0.0 34.8

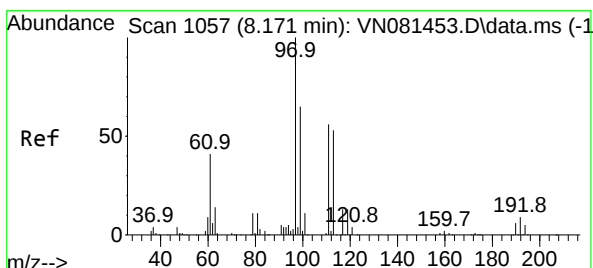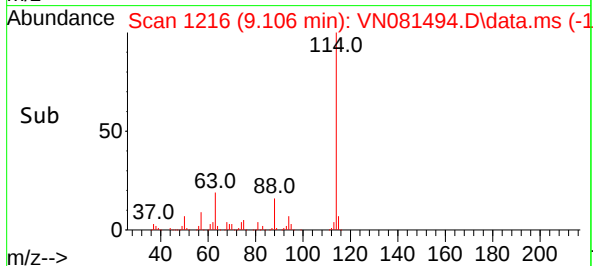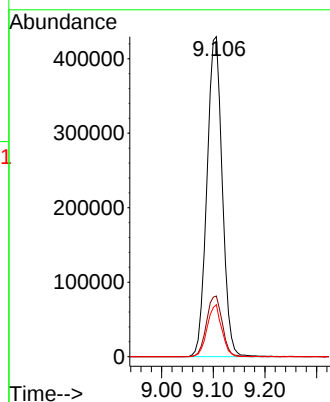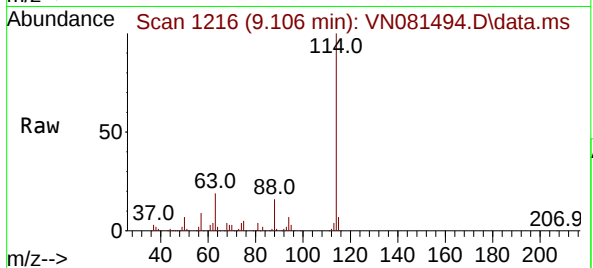

#35

Dibromofluoromethane

Concen: 48.514 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.000 min

Lab File: VN081494.D

Acq: 20 Mar 2024 15:23




Tgt Ion:113 Resp: 270746


Ion Ratio Lower Upper

113 100

111 101.5 82.2 123.4

192 17.6 12.5 18.7


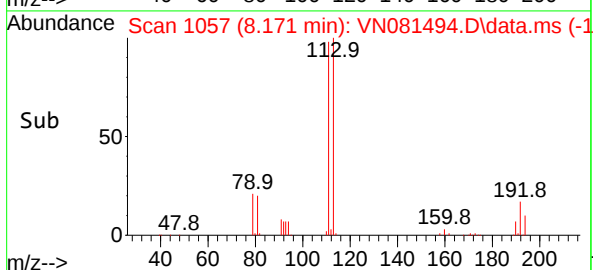
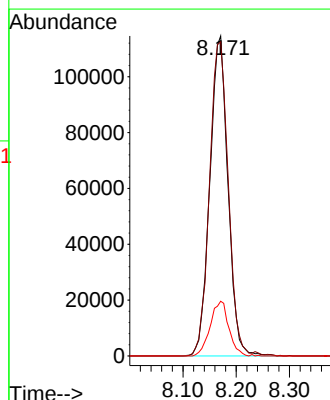
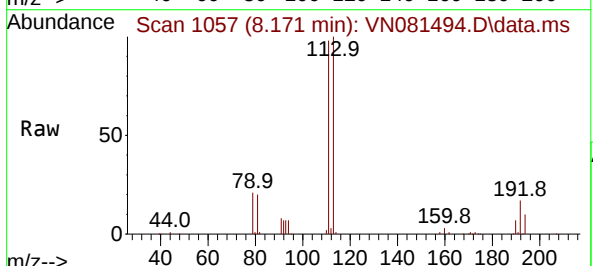


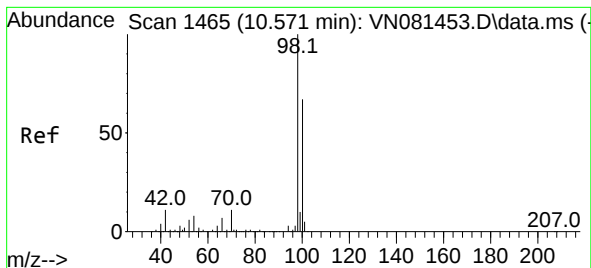

#50
Toluene-d8
Concen: 51.414 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN081494.D
Acq: 20 Mar 2024 15:23




Instrument :
MSVOA_N
ClientSampleId :
TRIP-BLANK


Tgt Ion: 98 Resp: 1037215
Ion Ratio Lower Upper
98 100
100 65.1 51.4 77.0

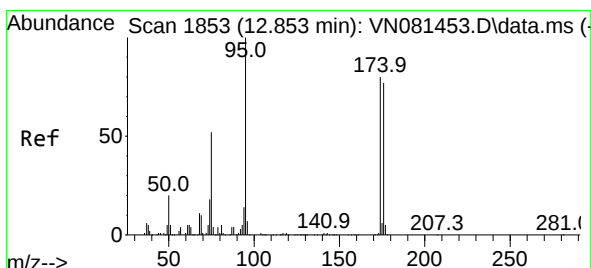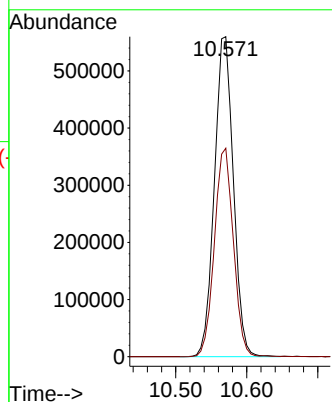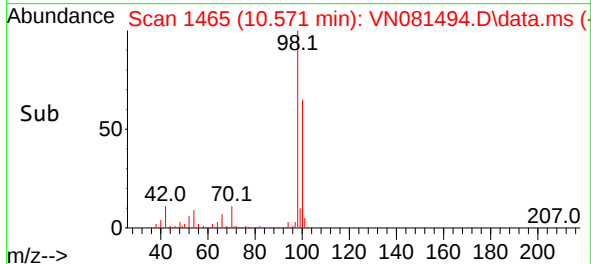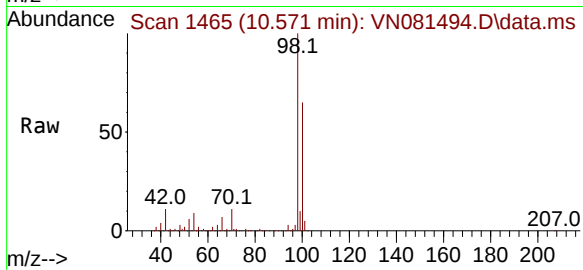

#62
4-Bromofluorobenzene
Concen: 47.655 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN081494.D
Acq: 20 Mar 2024 15:23

Tgt Ion: 95 Resp: 338750
Ion Ratio Lower Upper
95 100
174 76.1 0.0 120.4
176 73.2 0.0 121.0


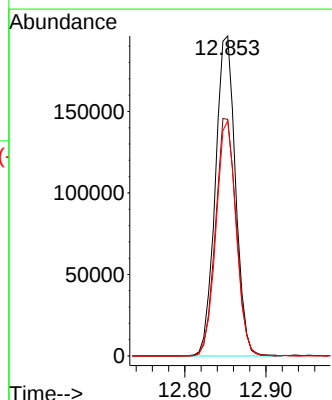
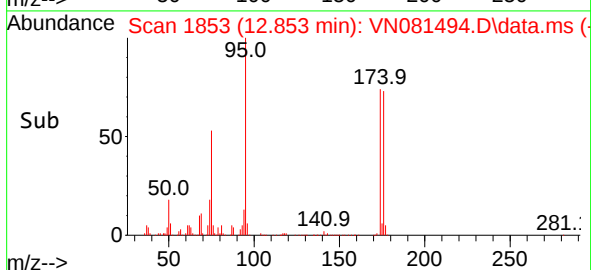
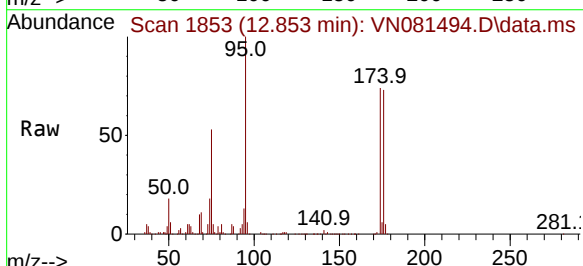


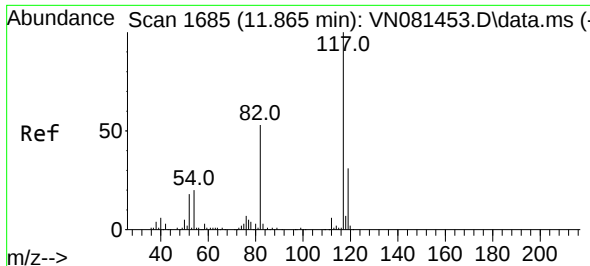

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VN081494.D
Acq: 20 Mar 2024 15:23

Instrument :
MSVOA_N
ClientSampleId :
TRIP-BLANK

Tgt Ion:117 Resp: 775743
Ion Ratio Lower Upper
117 100
82 56.5 52.7 79.1
119 31.1 25.3 37.9

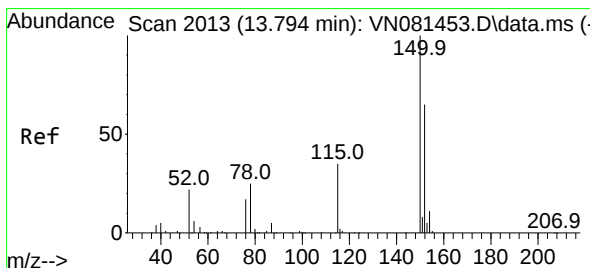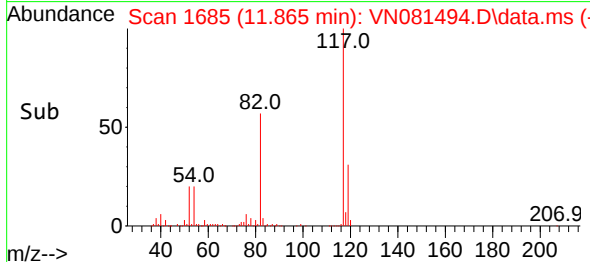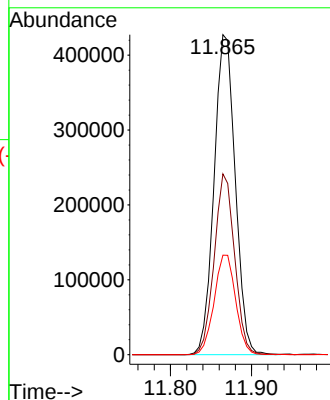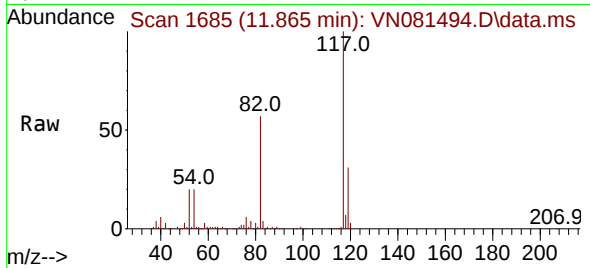

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN081494.D
Acq: 20 Mar 2024 15:23

Tgt Ion:152 Resp: 320620
Ion Ratio Lower Upper
152 100
115 62.0 32.3 96.8
150 156.5 0.0 339.8

