

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032024\
 Data File : VN081503.D
 Acq On : 20 Mar 2024 18:58
 Operator : JC\MD
 Sample : P1820-01 50X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WASTE-WATER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
 Title : SW846 8260

Signal : TIC: VN081503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.512	91	95	100	rVB	18728	27299	1.02%	0.188%
2	2.806	139	145	153	rVB4	15964	30837	1.15%	0.212%
3	8.165	1046	1056	1061	rBV	376091	898658	33.52%	6.174%
4	8.224	1061	1066	1081	rVB	720897	1584318	59.09%	10.884%
5	8.583	1116	1127	1135	rBV	388781	913092	34.06%	6.273%
6	8.665	1135	1141	1143	rBV3	28073	57783	2.16%	0.397%
7	9.100	1206	1215	1227	rBV	981676	2026685	75.59%	13.923%
8	10.571	1456	1465	1472	rBV	1422650	2681059	100.00%	18.419%
9	10.629	1472	1475	1487	rVB	53166	95305	3.55%	0.655%
10	11.865	1677	1685	1697	rBV	1279859	2287186	85.31%	15.713%
11	12.071	1713	1720	1728	rVB3	16205	33604	1.25%	0.231%
12	12.853	1844	1853	1861	rBV	963664	1679115	62.63%	11.535%
13	13.482	1955	1960	1966	rVB3	20975	33580	1.25%	0.231%
14	13.794	2005	2013	2025	rBV	1216141	2021450	75.40%	13.887%
15	13.988	2041	2046	2057	rVB5	9826	31096	1.16%	0.214%
16	15.053	2220	2227	2232	rBV5	23769	49858	1.86%	0.343%
17	15.212	2246	2254	2262	rVB3	22683	44674	1.67%	0.307%
18	16.164	2412	2416	2424	rVB9	15367	31421	1.17%	0.216%
19	16.506	2467	2474	2479	rBV9	11740	29116	1.09%	0.200%


Sum of corrected areas: 14556136

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032024\
Data File : VN081503.D
Acq On : 20 Mar 2024 18:58
Operator : JC\MD
Sample : P1820-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WASTE-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

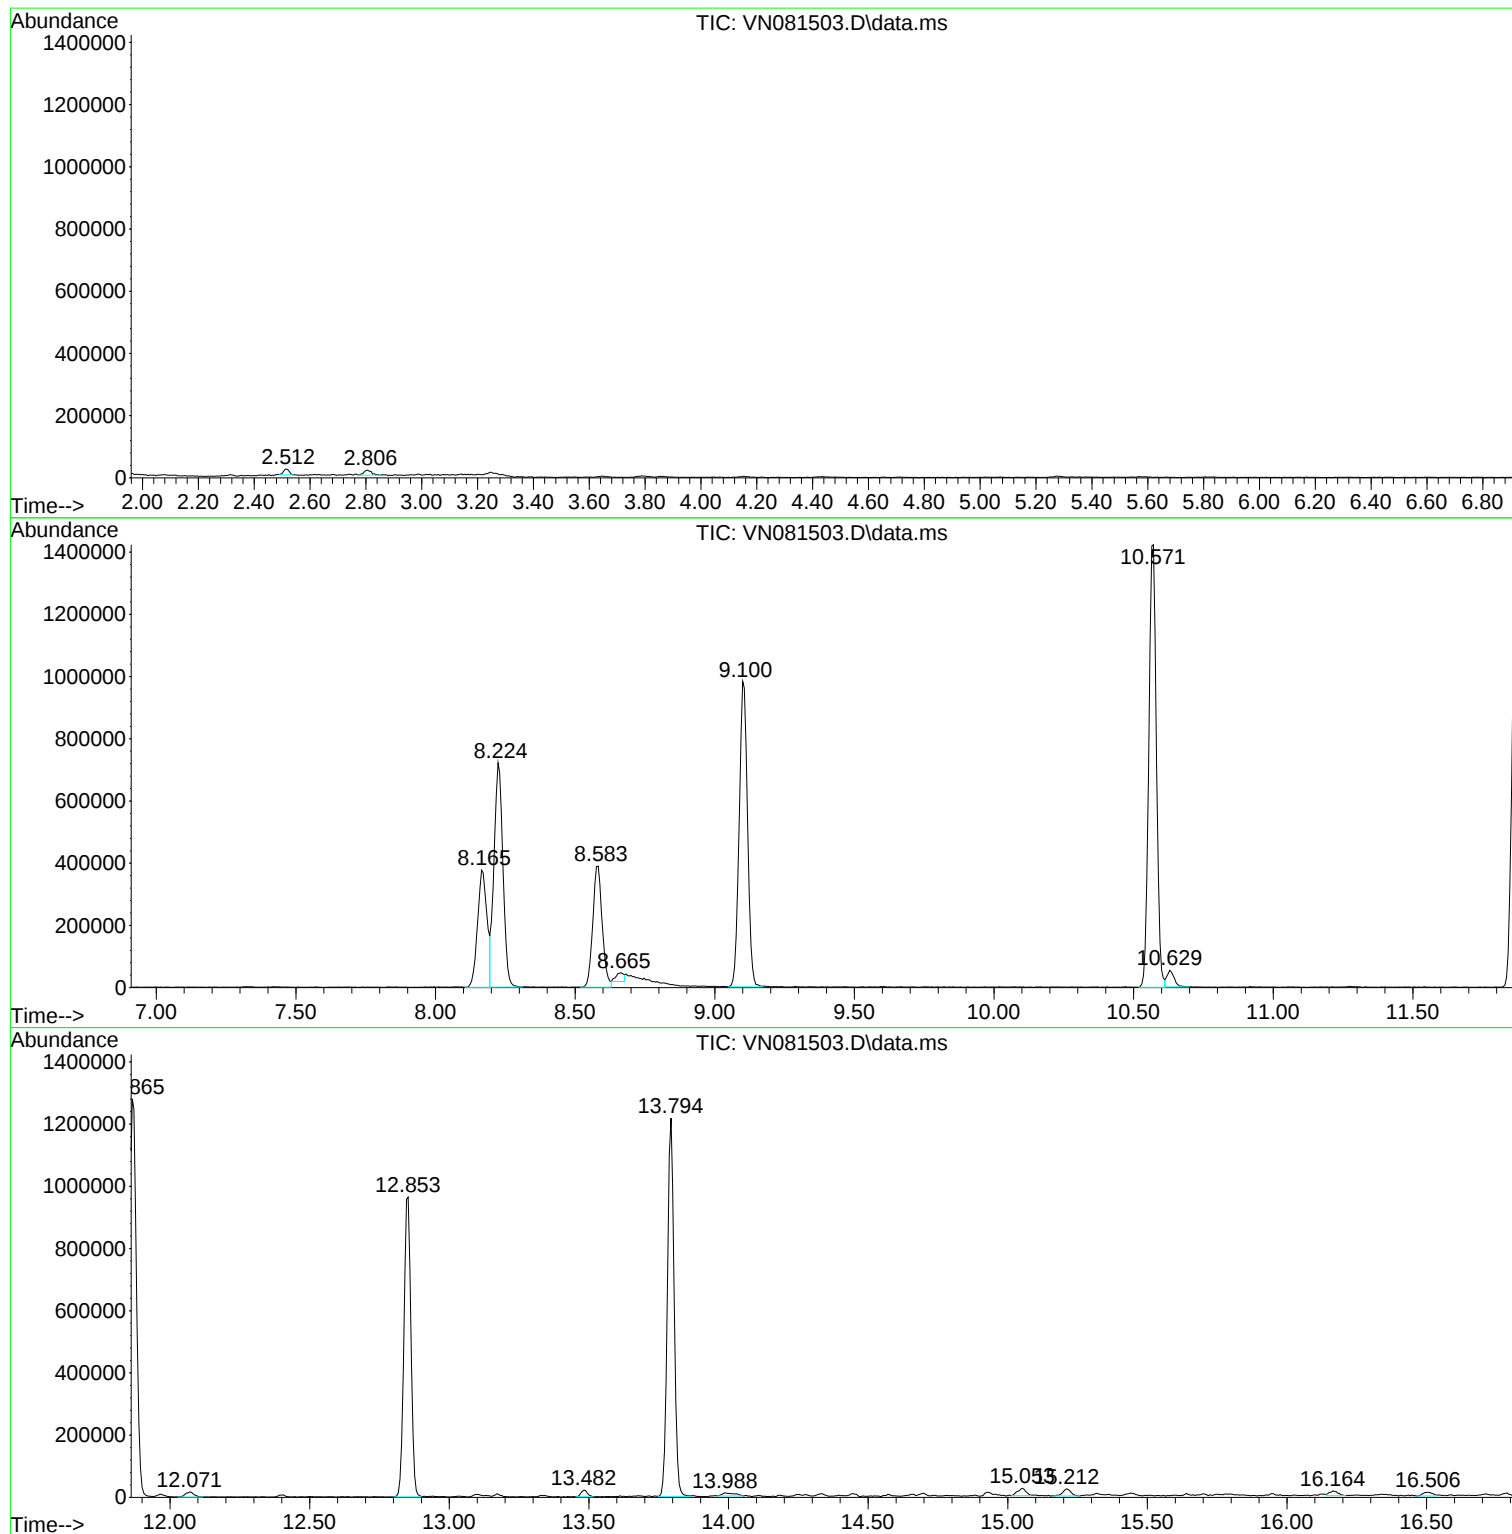

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032024\
Data File : VN081503.D
Acq On : 20 Mar 2024 18:58
Operator : JC\MD
Sample : P1820-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WASTE-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032024\
Data File : VN081503.D
Acq On : 20 Mar 2024 18:58
Operator : JC\MD
Sample : P1820-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WASTE-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc