
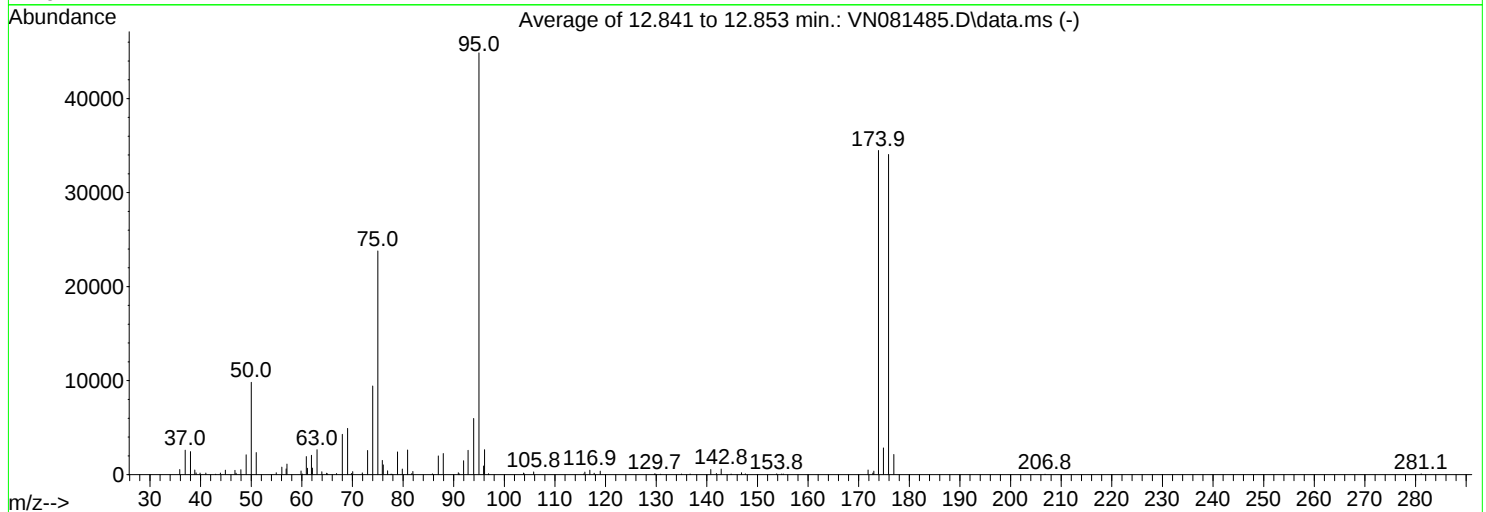


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032024\
Data File : VN081485.D
Acq On : 20 Mar 2024 08:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

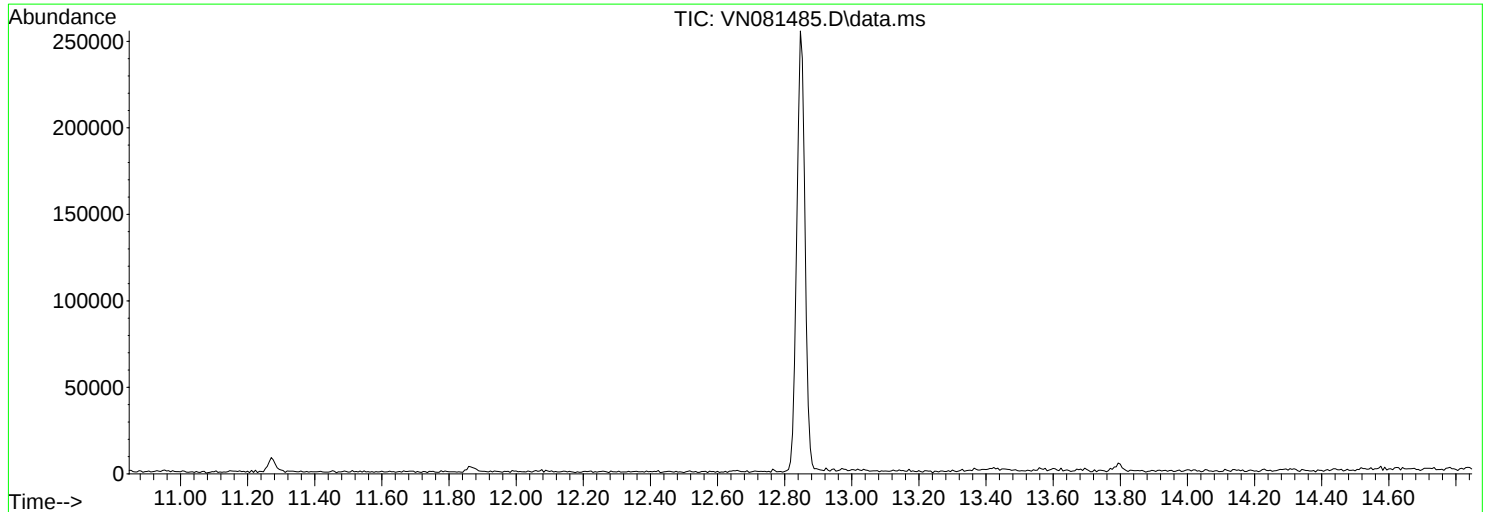

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	9822	PASS
75	95	30	60	53.0	23795	PASS
95	95	100	100	100.0	44869	PASS
96	95	5	9	5.9	2663	PASS
173	174	0.00	2	1.1	383	PASS
174	95	50	100	76.8	34477	PASS
175	174	5	9	8.2	2837	PASS
176	174	95	101	98.8	34064	PASS
177	176	5	9	6.3	2152	PASS

Average of 12.841 to 12.853 min.: VN081485.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	544	47.00	156	60.90	1924	69.80	114
36.95	2609	47.95	522	61.10	688	70.05	33
38.00	2459	49.00	2114	61.90	2066	71.95	18
38.85	489	50.00	9822	62.10	694	73.00	257
39.10	190	51.00	2357	63.00	2661	74.00	9433
39.90	171	54.95	206	63.95	310	75.00	23795
41.05	167	56.05	805	64.90	146	75.90	1513
43.00	50	56.90	618	65.10	89	76.10	1042
43.90	174	57.05	1118	66.85	112	76.95	403
44.90	474	59.85	397	68.00	4282	77.60	52
46.80	460	60.10	72	69.05	4919	77.80	53

Average of 12.841 to 12.853 min.: VN081485.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.90	2420	92.85	2595	116.90	482	144.80	76
79.85	605	93.95	5973	117.75	149	146.85	205
80.90	2629	95.00	44869	118.95	374	147.60	94
81.70	103	95.90	917	129.70	88	153.80	95
81.95	348	96.10	2663	129.90	73	154.80	66
85.80	81	96.90	109	130.90	55	155.10	74
86.95	1997	103.80	174	135.00	63	171.85	503
87.95	2247	104.00	75	136.70	71	172.80	172
90.90	212	105.80	286	140.80	541	173.00	383
91.10	82	115.70	66	141.90	113	173.90	34477
91.95	1480	115.90	280	142.85	605	174.90	2837

Average of 12.841 to 12.853 min.: VN081485.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.90	34064						
176.95	2152						
206.80	58						
281.10	84						

Instrument :

MSVOA_N

ClientSampleId :

BFB