
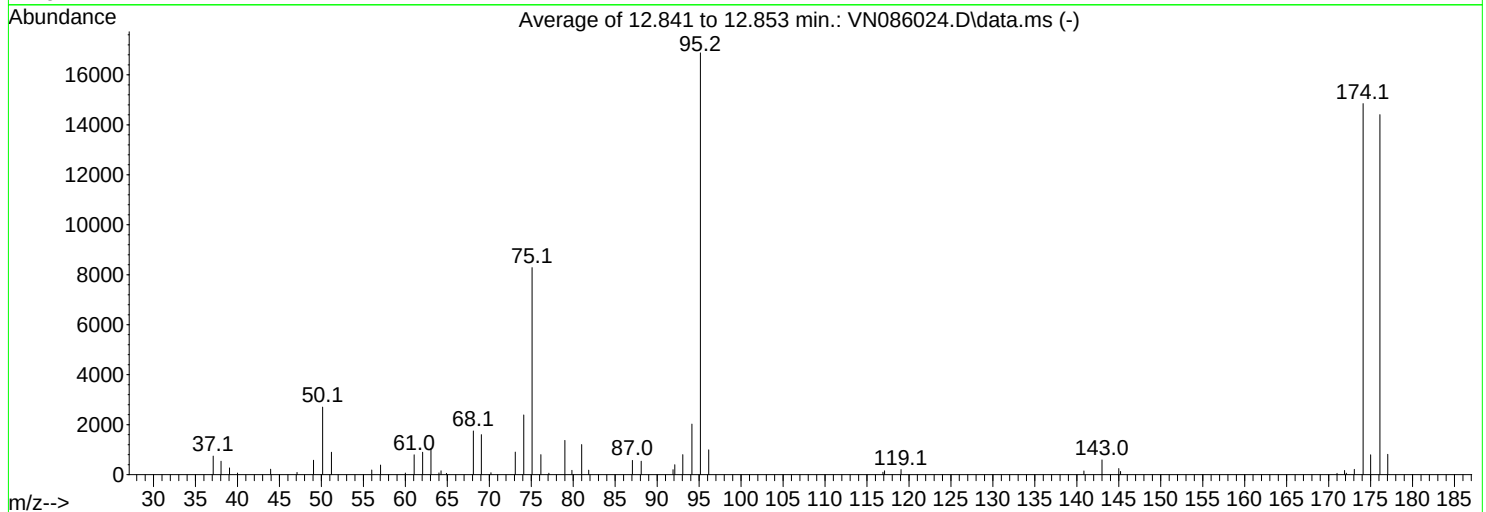


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032025\
Data File : VN086024.D
Acq On : 20 Mar 2025 14:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Title : SW846 8260
Last Update : Wed Mar 19 03:20:56 2025

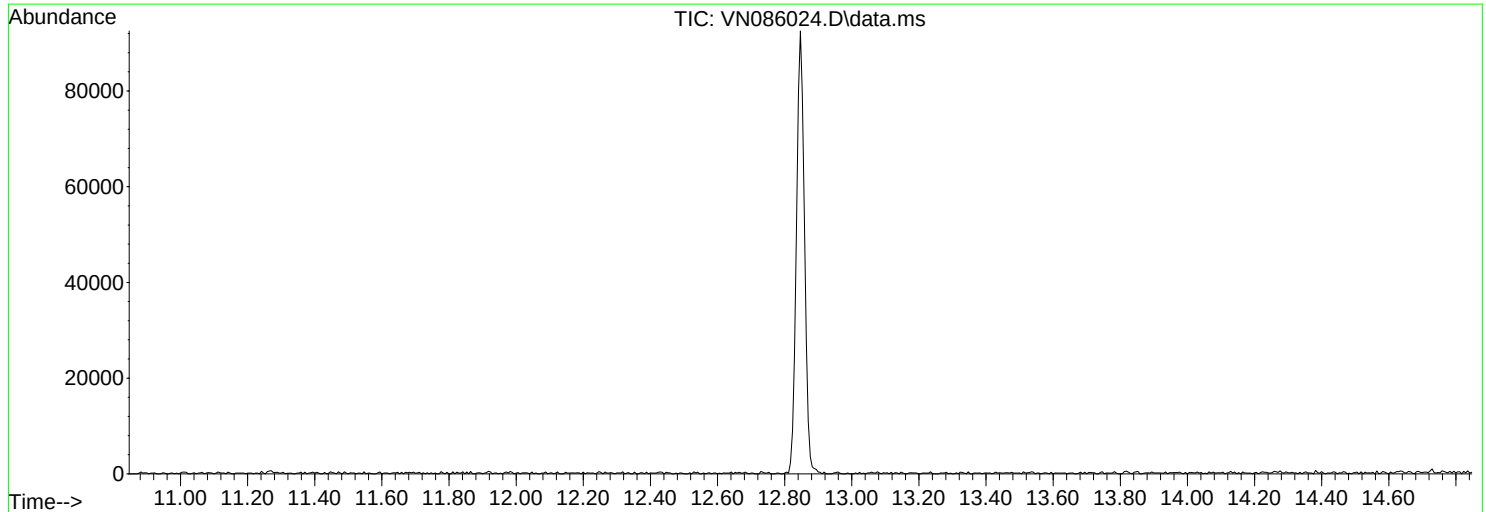

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	2705	PASS
75	95	30	60	49.1	8283	PASS
95	95	100	100	100.0	16880	PASS
96	95	5	9	5.9	993	PASS
173	174	0.00	2	1.4	210	PASS
174	95	50	100	88.0	14852	PASS
175	174	5	9	5.3	793	PASS
176	174	95	101	97.0	14405	PASS
177	176	5	9	5.6	812	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
37.10	740	60.00	62	74.10	2390	92.10	391
38.05	536	61.05	796	75.10	8283	93.05	80
39.05	272	62.05	895	76.15	803	94.15	202
40.00	63	63.05	1047	77.10	58	95.15	1688
43.95	221	64.00	72	79.00	1369	96.15	993
47.10	87	64.25	151	79.85	172	116.90	95
49.05	574	64.90	52	81.00	1207	117.10	154
50.15	2705	68.10	1747	81.85	182	119.05	202
51.20	897	69.05	1603	87.05	571	140.85	149
56.00	183	70.20	75	88.10	539	143.00	590
57.05	382	73.10	905	91.90	196	145.00	241

Average of 12.841 to 12.853 min.: VN086024.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
145.20	131						
171.00	51						
171.90	167						
172.10	55						
173.05	210						
174.10	14852						
175.00	793						
176.10	14405						
177.05	812						

Instrument :

MSVOA_N

ClientSampleId :

BFB