

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032122\
 Data File : VN071419.D
 Acq On : 21 Mar 2022 14:51
 Operator : JC\MD
 Sample : N1944-05
 Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 CHRT-26215

Quant Time: Mar 21 16:26:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.075	168	620935	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	8.957	114	1067945	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1039365	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	419829	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.428	65	412762	48.502	ug/l	-0.01
Spiked Amount 50.000	Range 61 - 141		Recovery =	97.000%		
35) Dibromofluoromethane	8.010	113	298381	44.276	ug/l	-0.01
Spiked Amount 50.000	Range 69 - 133		Recovery =	88.560%		
50) Toluene-d8	10.433	98	1345849	49.601	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	99.200%		
62) 4-Bromofluorobenzene	12.727	95	471736	51.342	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	102.680%		
Target Compounds					Qvalue	
3) Chloromethane	2.287	50	3247	0.321	ug/l	98
5) Bromomethane	2.846	94	231	Below Cal	#	3
6) Chloroethane	2.934	64	1556	0.308	ug/l #	42
13) Acrolein	4.034	56	628	0.355	ug/l #	70
16) Acetone	4.316	43	6272	1.515	ug/l	99
18) Methyl Acetate	4.846	43	22535	2.477	ug/l	98
20) Methylene Chloride	5.069	84	1862	0.626	ug/l #	71
25) 2-Butanone	7.345	43	3960	0.594	ug/l #	84
29) Tetrahydrofuran	7.687	42	5681	1.229	ug/l #	59
31) Cyclohexane	8.075	56	13635	1.003	ug/l #	1
36) 1,1-Dichloropropene	8.075	75	49541	4.588	ug/l #	49
38) Carbon Tetrachloride	8.075	117	60947	5.836	ug/l #	16
43) Isopropyl Acetate	8.563	43	23088	1.039	ug/l #	57
49) 1,4-Dioxane	9.575	88	53	0.296	ug/l #	1
51) 4-Methyl-2-Pentanone	10.333	43	5882	0.427	ug/l	88
59) 2-Hexanone	11.080	43	9857	1.048	ug/l	89
74) N-amyl acetate	12.386	43	5449	0.358	ug/l #	93
75) 1,1,2,2-Tetrachloroethane	12.822	83	1408	Below Cal		75
76) 1,2,3-Trichloropropane	12.727	75	244509	22.476	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	244509	62.957	ug/l #	5
87) 1,3-Dichlorobenzene	13.616	146	3372	0.220	ug/l	86
88) 1,4-Dichlorobenzene	13.616	146	3372	0.225	ug/l	85
89) n-Butylbenzene	13.939	91	8859	0.386	ug/l	94
91) 1,2-Dichlorobenzene	13.986	146	3412	0.231	ug/l #	68
92) 1,2-Dibromo-3-Chloropr...	14.598	75	755	0.321	ug/l	70
93) 1,2,4-Trichlorobenzene	15.257	180	6229	3.840	ug/l #	88
94) Hexachlorobutadiene	15.357	225	1033	0.250	ug/l	90
95) Naphthalene	15.504	128	26324	6.297	ug/l	98
96) 1,2,3-Trichlorobenzene	15.698	180	7229	3.769	ug/l #	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032122\
Data File : VN071419.D
Acq On : 21 Mar 2022 14:51
Operator : JC\MD
Sample : N1944-05
Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215

Quant Time: Mar 21 16:26:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration




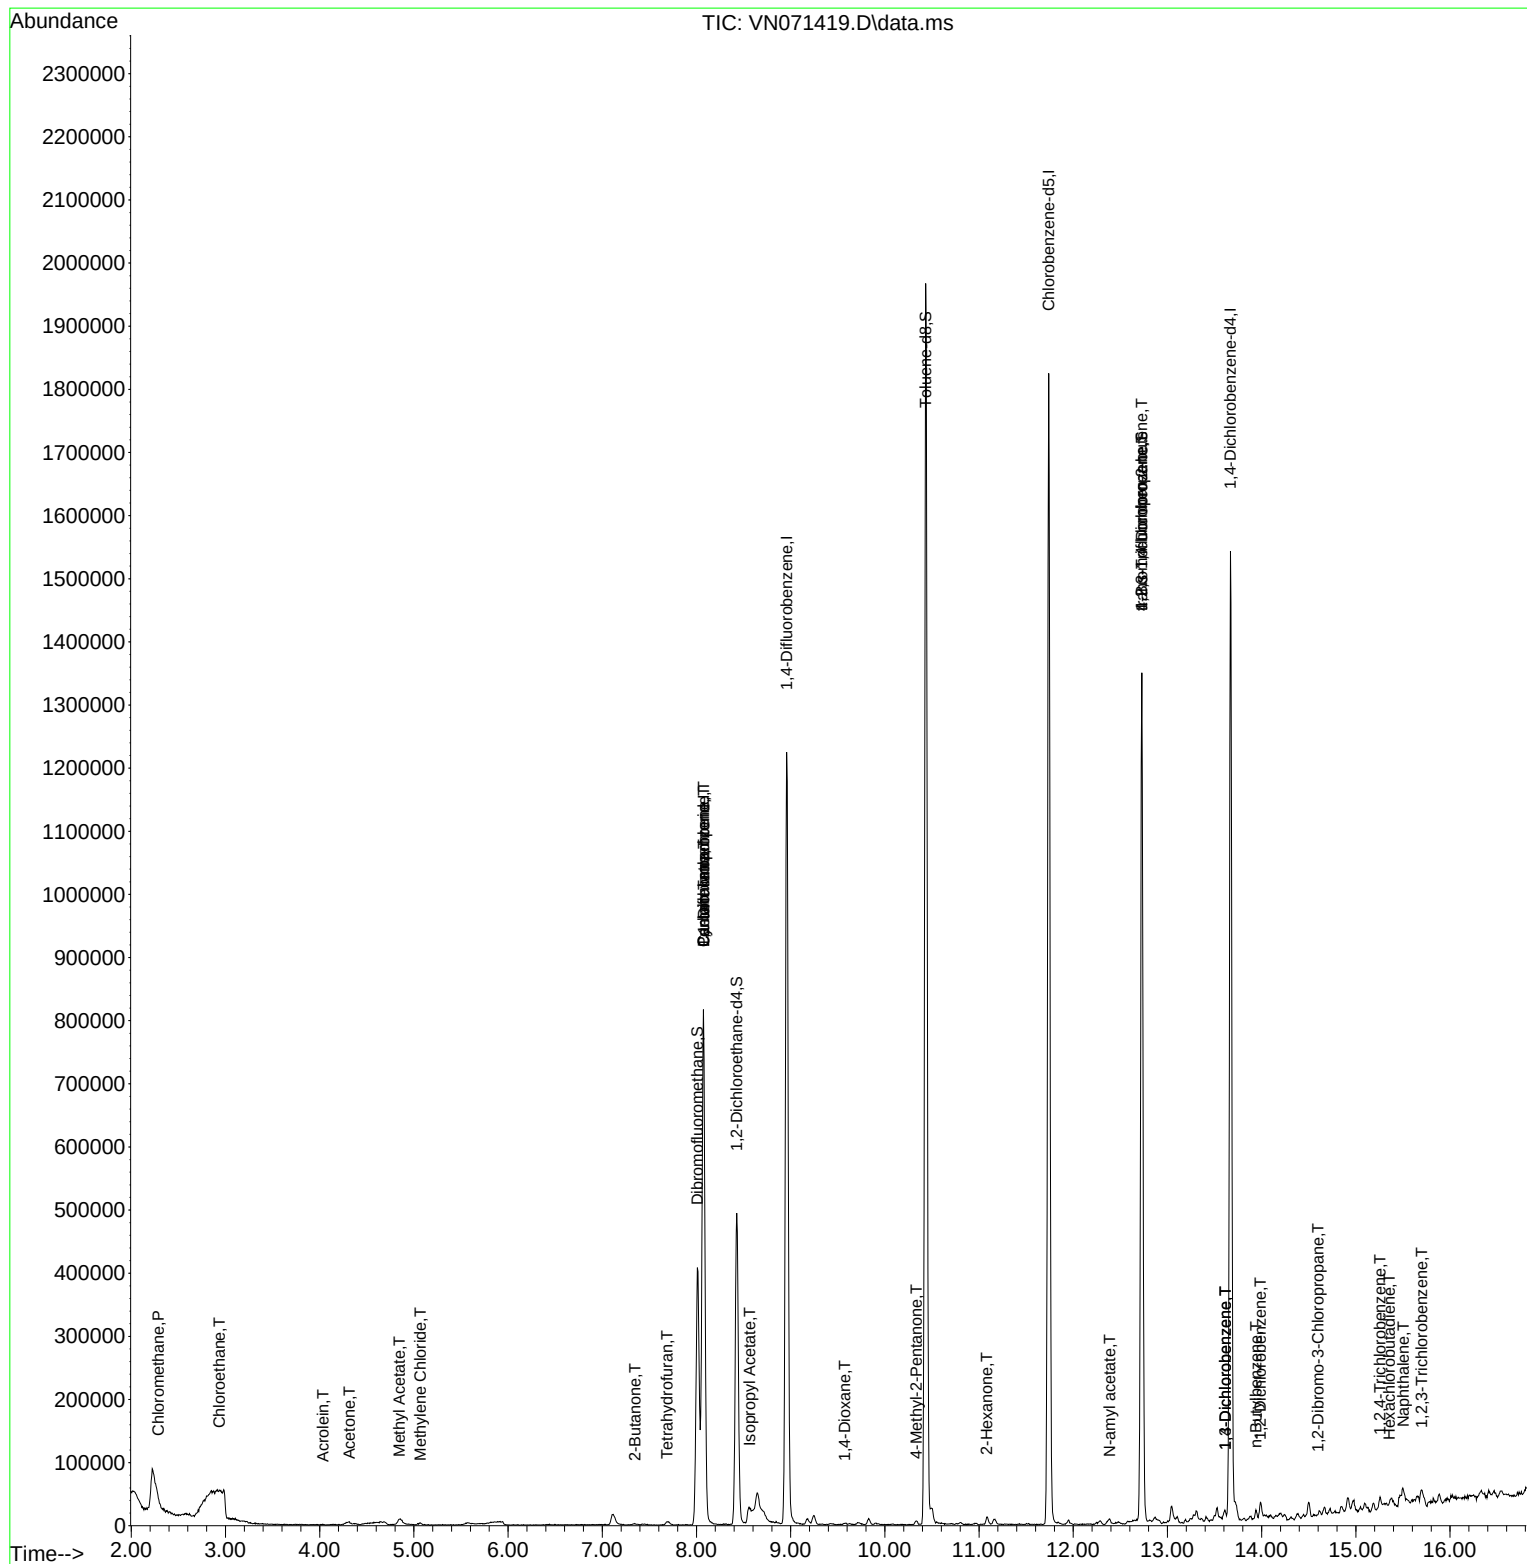




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.075 min Scan# 10
Delta R.T. -0.011 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion:168 Resp: 620935
Ion Ratio Lower Upper
168 100
99 60.9 41.3 61.9

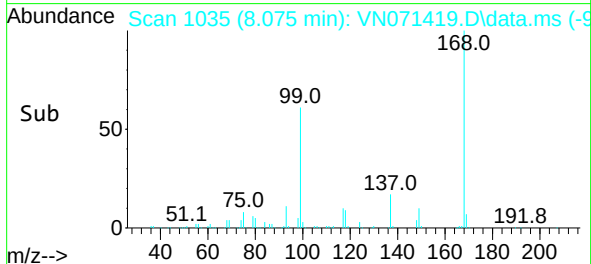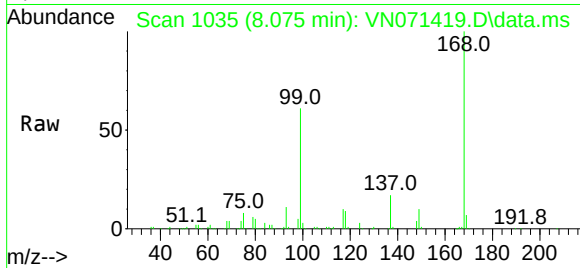

#3
Chloromethane
Concen: 0.321 ug/l
RT: 2.287 min Scan# 51
Delta R.T. -0.012 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Tgt Ion: 50 Resp: 3247
Ion Ratio Lower Upper
50 100
52 30.6 25.4 38.0




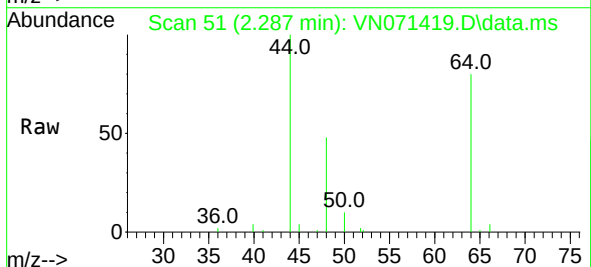


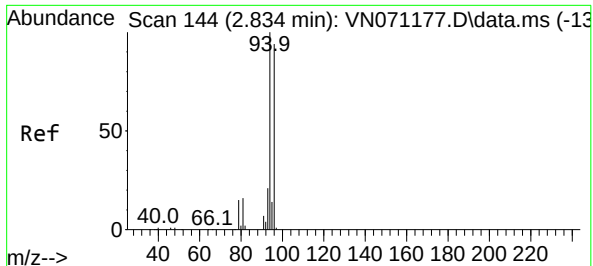

#5
Bromomethane
Concen: Below Cal
RT: 2.846 min Scan# 144
Delta R.T. 0.012 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion: 94 Resp: 231
Ion Ratio Lower Upper
94 100
96 0.0 73.8 110.8#

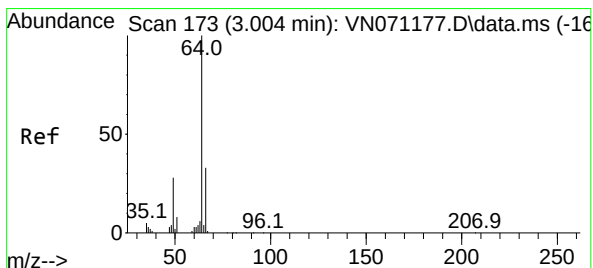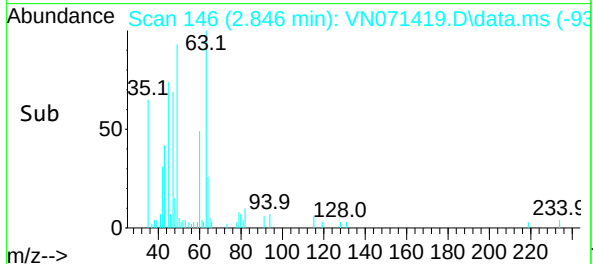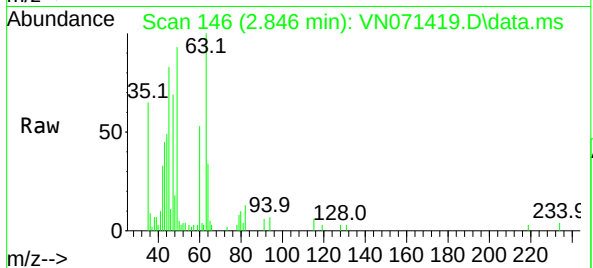

#6
Chloroethane
Concen: 0.308 ug/l
RT: 2.934 min Scan# 161
Delta R.T. -0.070 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Tgt Ion: 64 Resp: 1556
Ion Ratio Lower Upper
64 100
66 0.0 26.3 39.5#


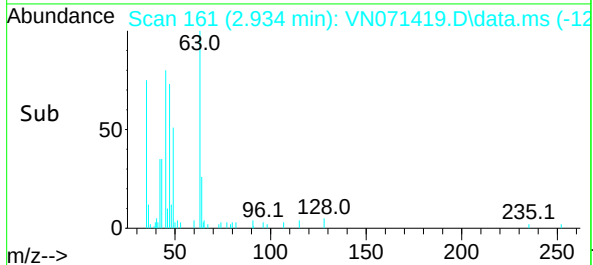

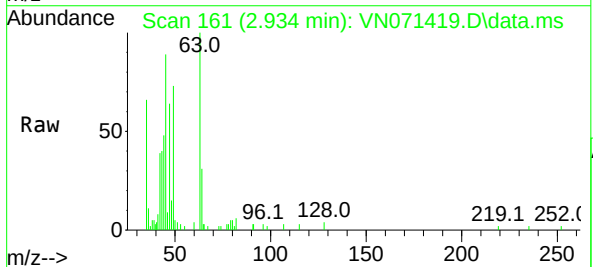




#13
Acrolein
Concen: 0.355 ug/l
RT: 4.034 min Scan# 349
Delta R.T. -0.006 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion: 56 Resp: 628
Ion Ratio Lower Upper
56 100
55 46.0 56.6 85.0#

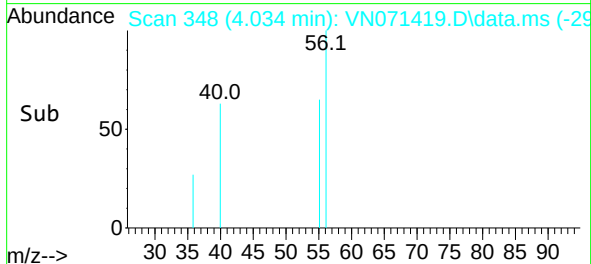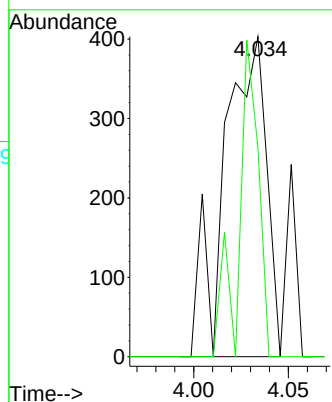

#16
Acetone
Concen: 1.515 ug/l
RT: 4.316 min Scan# 396
Delta R.T. 0.030 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Tgt Ion: 43 Resp: 6272
Ion Ratio Lower Upper
43 100
58 28.2 23.1 34.7


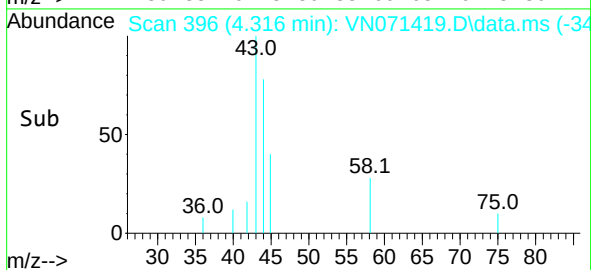
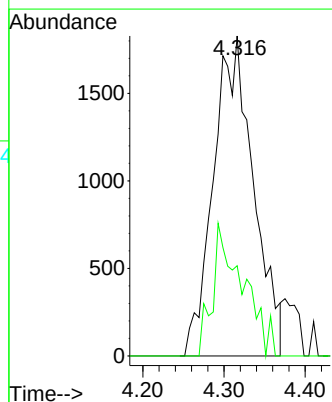
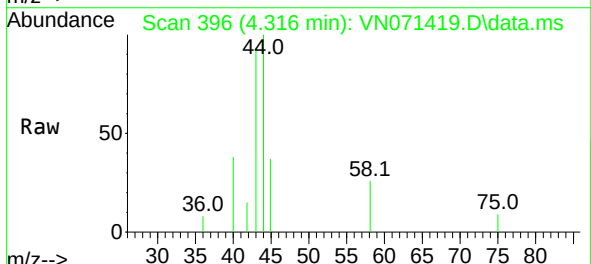




#18
Methyl Acetate
Concen: 2.477 ug/l
RT: 4.846 min Scan# 41
Delta R.T. -0.005 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion: 43 Resp: 22535
Ion Ratio Lower Upper
43 100
74 23.2 19.4 29.2

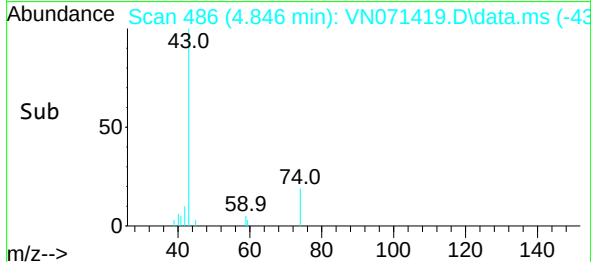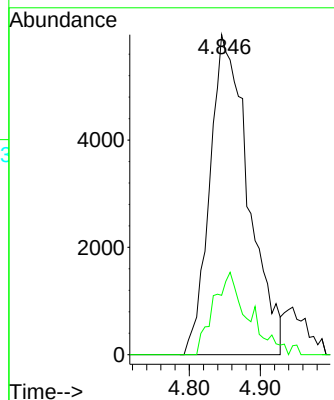

#20
Methylene Chloride
Concen: 0.626 ug/l
RT: 5.069 min Scan# 524
Delta R.T. -0.024 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Tgt Ion: 84 Resp: 1862
Ion Ratio Lower Upper
84 100
49 70.6 93.5 140.3#
51 25.1 29.4 44.2#
86 57.9 53.0 79.4


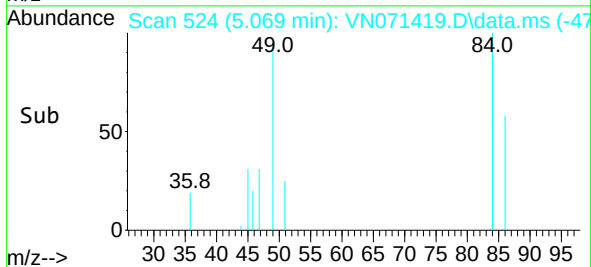
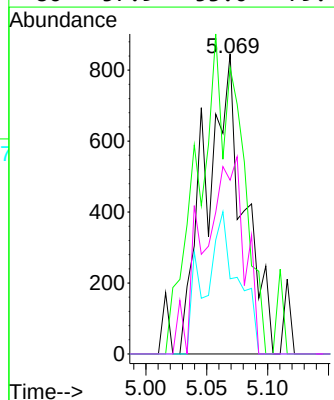
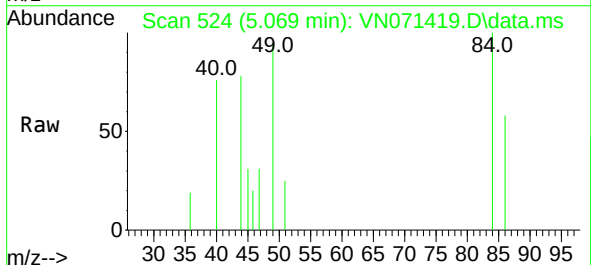


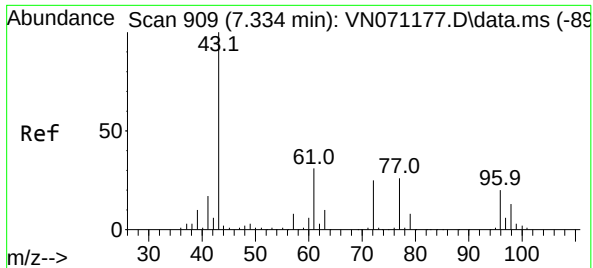

#25
2-Butanone
Concen: 0.594 ug/l
RT: 7.345 min Scan# 911
Delta R.T. 0.012 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion: 43 Resp: 3960
Ion Ratio Lower Upper
43 100
72 35.4 21.7 32.5#

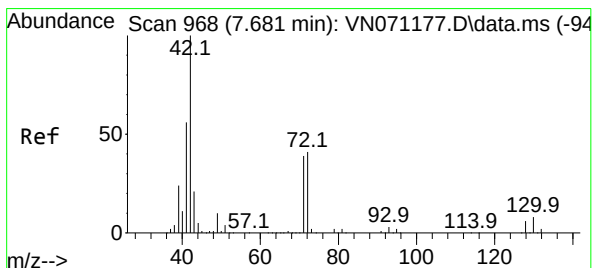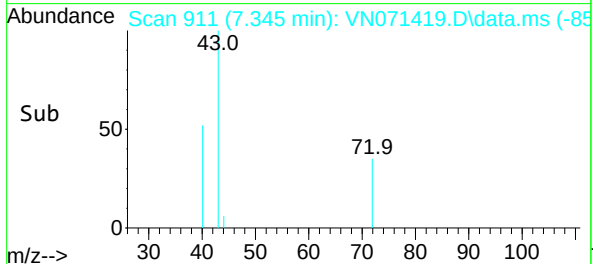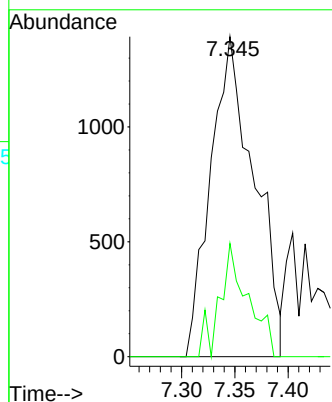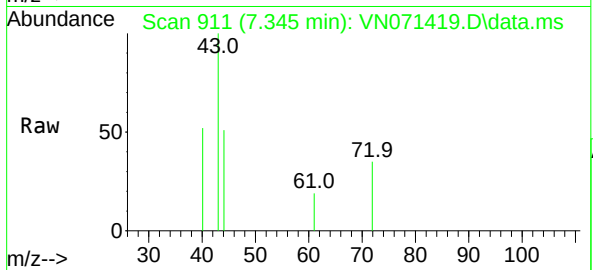

#29
Tetrahydrofuran
Concen: 1.229 ug/l
RT: 7.687 min Scan# 969
Delta R.T. 0.006 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Tgt Ion: 42 Resp: 5681
Ion Ratio Lower Upper
42 100
72 35.3 36.3 54.5#
71 0.0 34.7 52.1#

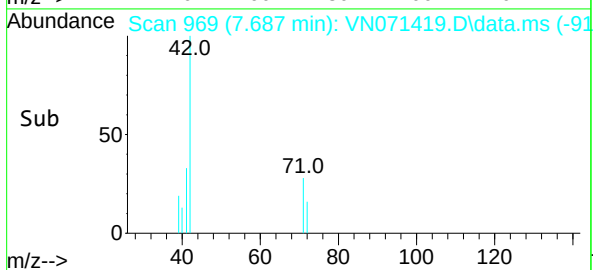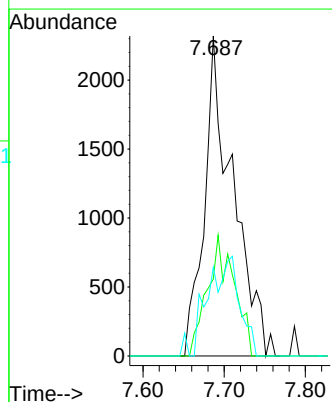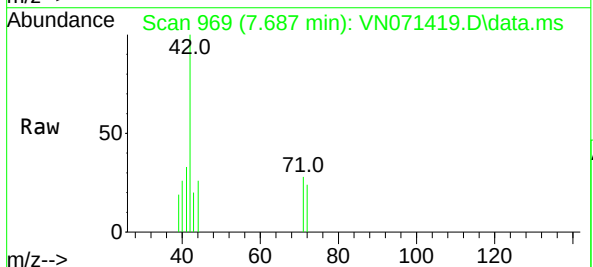

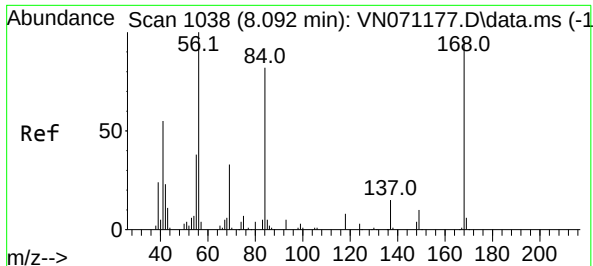

#31

Cyclohexane

Concen: 1.003 ug/l

RT: 8.075 min Scan# 1035

Delta R.T. -0.018 min

Lab File: VN071419.D

Acq: 21 Mar 2022 14:51

Instrument :

MSVOA_N

ClientSampleId :

CHRT-26215





Tgt Ion: 56 Resp: 13635

Ion Ratio Lower Upper

56 100

69 168.4 27.1 40.7#

84 145.9 73.4 110.0#

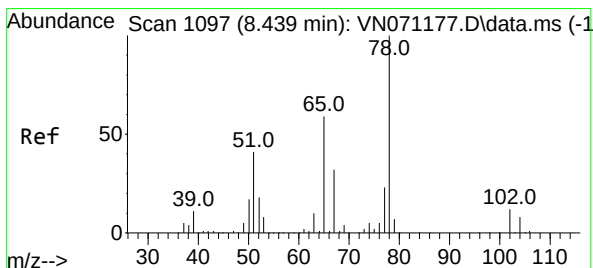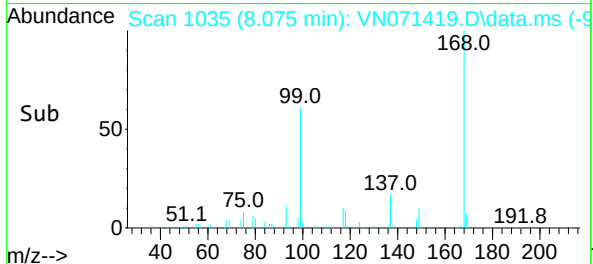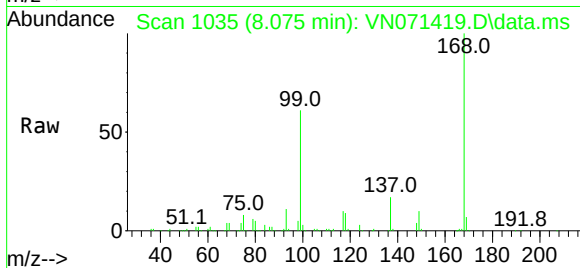

#33

1,2-Dichloroethane-d4

Concen: 48.502 ug/l

RT: 8.428 min Scan# 1095

Delta R.T. -0.012 min

Lab File: VN071419.D




Acq: 21 Mar 2022 14:51


Tgt Ion: 65 Resp: 412762

Ion Ratio Lower Upper

65 100

67 52.2 0.0 103.0

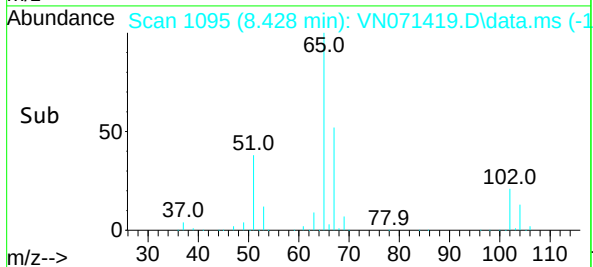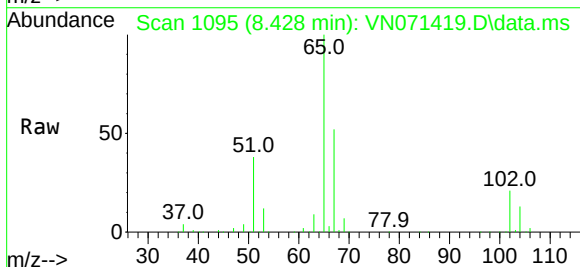

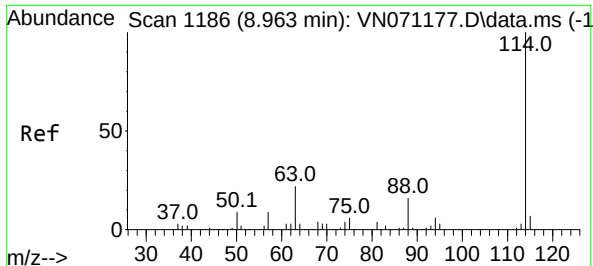

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.957 min Scan# 1185

Delta R.T. -0.006 min

Lab File: VN071419.D

Acq: 21 Mar 2022 14:51

Instrument :

MSVOA_N

ClientSampleId :

CHRT-26215





Tgt Ion:114 Resp: 1067945

Ion Ratio Lower Upper

114 100

63 22.7 0.0 37.8

88 16.5 0.0 27.4

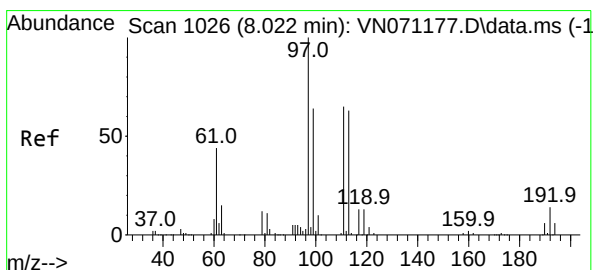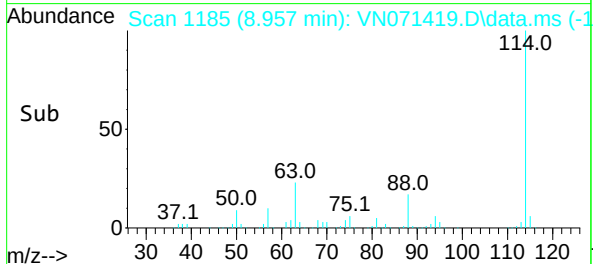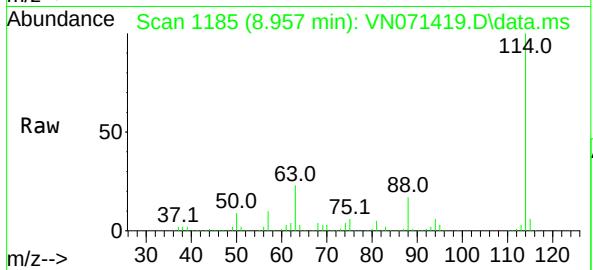

#35

Dibromofluoromethane

Concen: 44.276 ug/l

RT: 8.010 min Scan# 1024

Delta R.T. -0.012 min

Lab File: VN071419.D

Acq: 21 Mar 2022 14:51




Tgt Ion:113 Resp: 298381


Ion Ratio Lower Upper

113 100

111 103.2 82.2 123.2

192 20.6 16.9 25.3

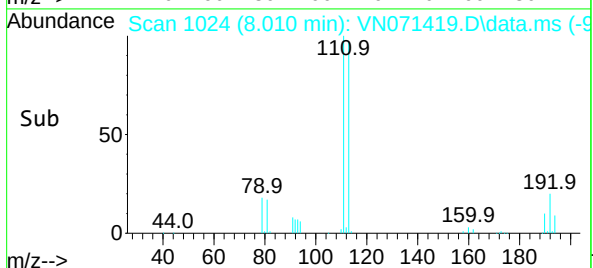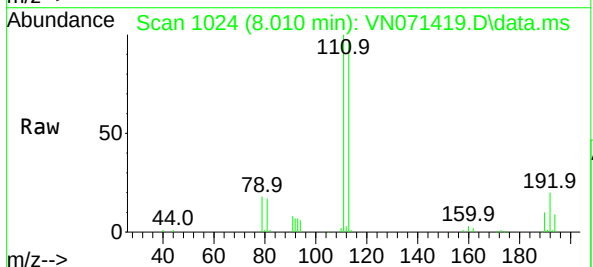

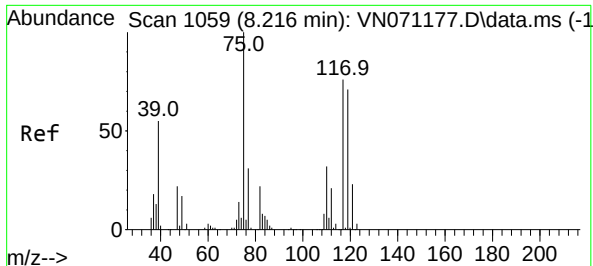

#36

1,1-Dichloropropene

Concen: 4.588 ug/l

RT: 8.075 min Scan# 1035

Delta R.T. -0.141 min

Lab File: VN071419.D

Acq: 21 Mar 2022 14:51

Instrument :

MSVOA_N

ClientSampleId :

CHRT-26215





Tgt Ion: 75 Resp: 49541

Ion Ratio Lower Upper

75 100

110 8.4 18.4 55.2#

77 0.0 24.4 36.6#

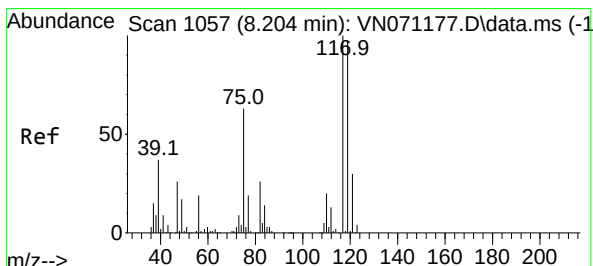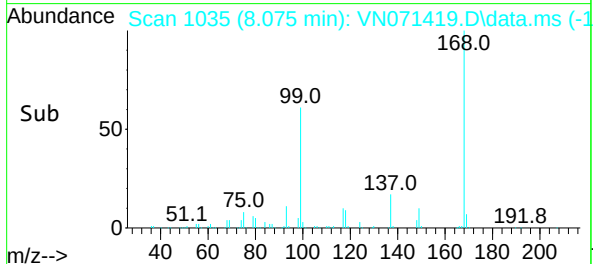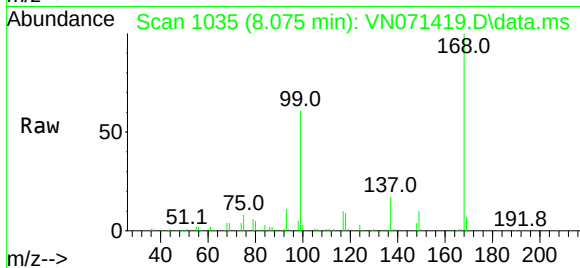

#38

Carbon Tetrachloride

Concen: 5.836 ug/l

RT: 8.075 min Scan# 1035

Delta R.T. -0.129 min

Lab File: VN071419.D

Acq: 21 Mar 2022 14:51




Tgt Ion: 117 Resp: 60947


Ion Ratio Lower Upper

117 100

119 4.9 76.1 114.1#

121 0.0 24.2 36.2#


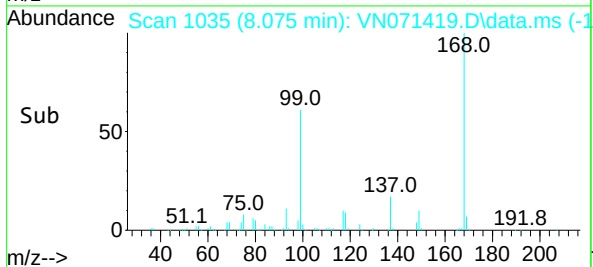

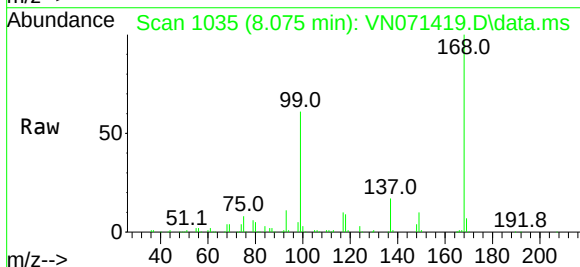


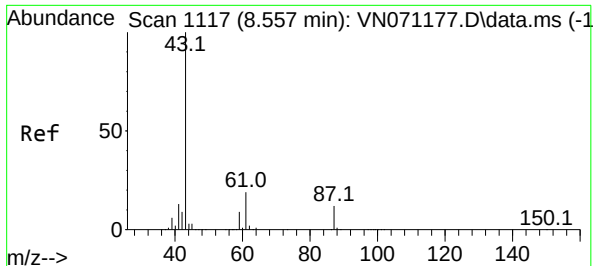

#43
Isopropyl Acetate
Concen: 1.039 ug/l
RT: 8.563 min Scan# 1117
Delta R.T. 0.006 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion: 43 Resp: 23088
Ion Ratio Lower Upper
43 100
61 1.3 20.4 30.6#
87 0.0 11.2 16.8#

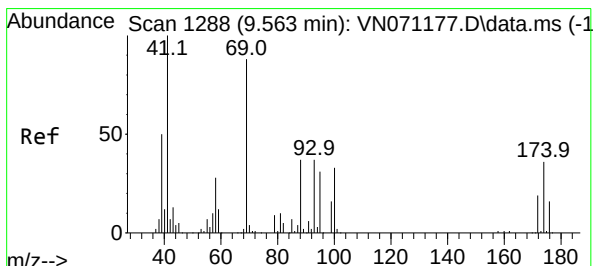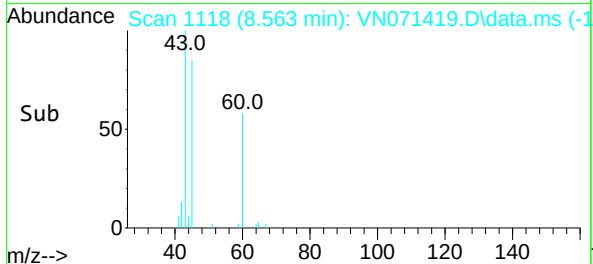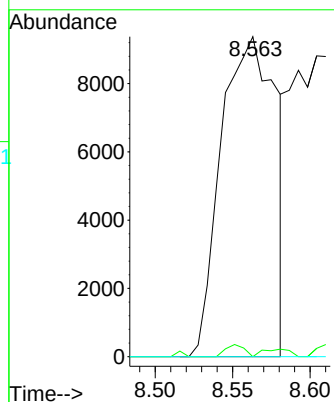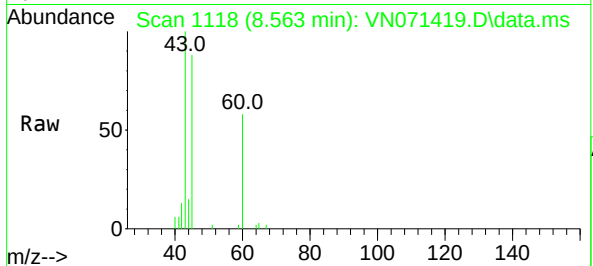

#49
1,4-Dioxane
Concen: 0.296 ug/l
RT: 9.575 min Scan# 1290
Delta R.T. 0.012 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Tgt Ion: 88 Resp: 53
Ion Ratio Lower Upper
88 100
43 447.2 23.4 35.2#
58 0.0 50.6 75.8#


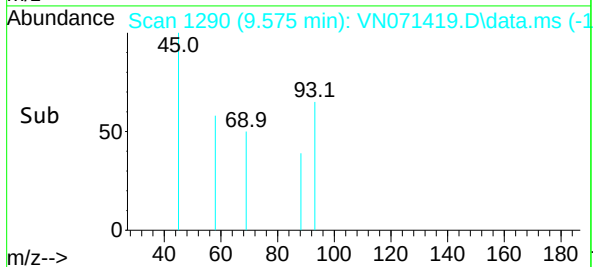
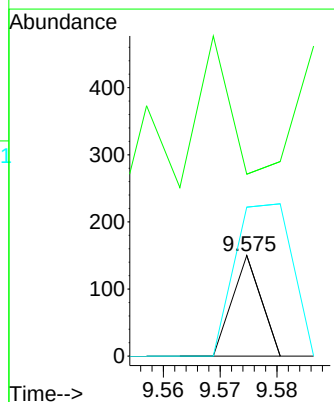
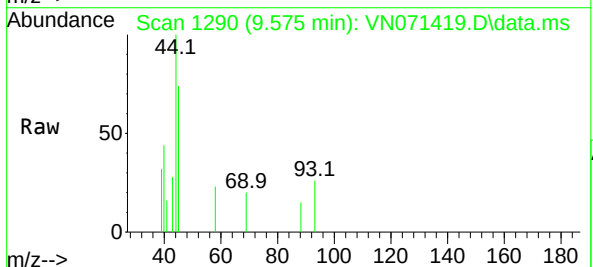




#50
Toluene-d8
Concen: 49.601 ug/l
RT: 10.433 min Scan# 1437
Delta R.T. -0.006 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion: 98 Resp: 1345849
Ion Ratio Lower Upper
98 100
100 65.8 50.4 75.6

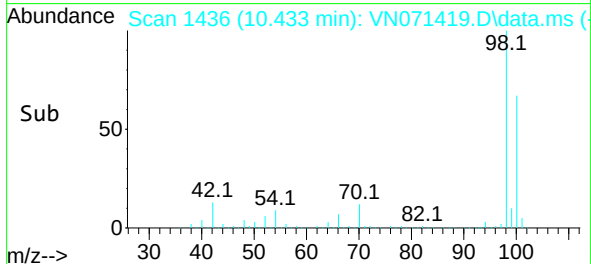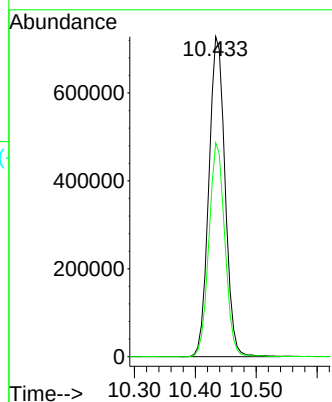

#51
4-Methyl-2-Pentanone
Concen: 0.427 ug/l
RT: 10.333 min Scan# 1419
Delta R.T. 0.006 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Tgt Ion: 43 Resp: 5882
Ion Ratio Lower Upper
43 100
58 30.8 30.4 45.6


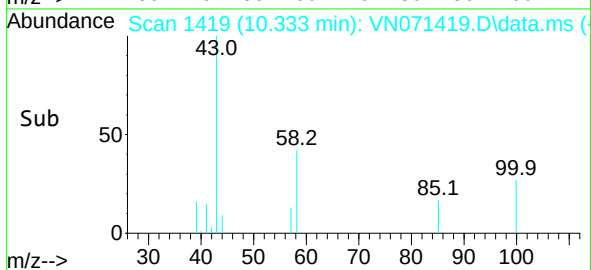
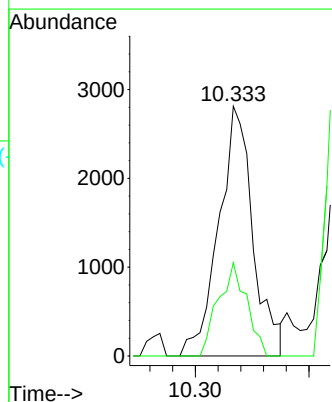
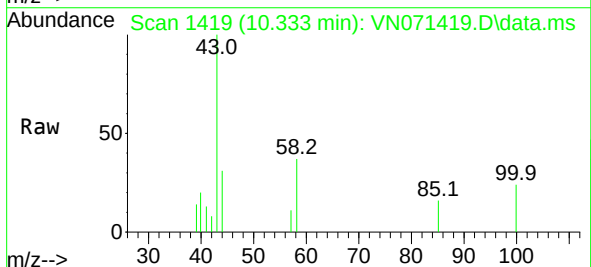




#59
2-Hexanone
Concen: 1.048 ug/l
RT: 11.080 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion: 43 Resp: 9857
Ion Ratio Lower Upper
43 100
58 46.3 26.9 80.7

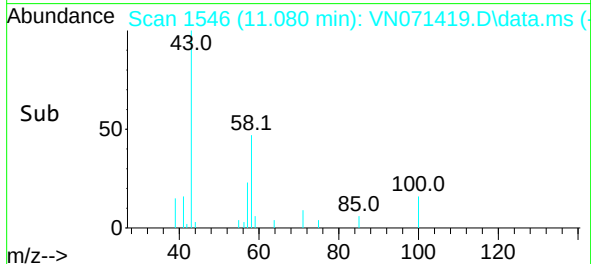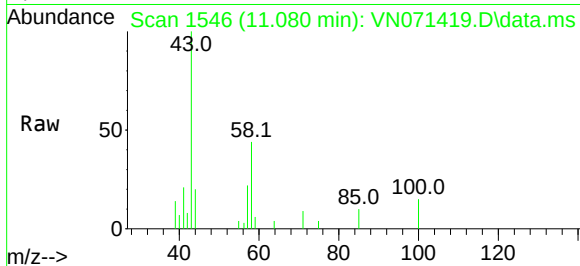

#62
4-Bromofluorobenzene
Concen: 51.342 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Tgt Ion: 95 Resp: 471736
Ion Ratio Lower Upper
95 100
174 78.3 0.0 187.2
176 75.0 0.0 181.4


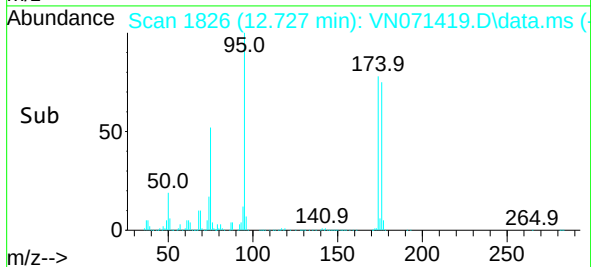

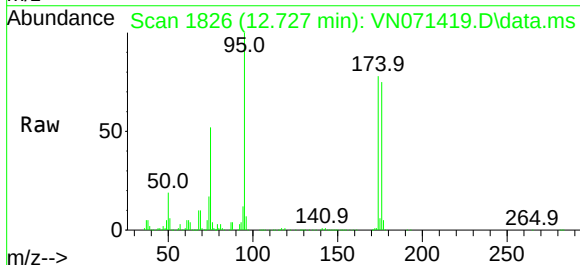




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion:117 Resp: 1039365
Ion Ratio Lower Upper
117 100
82 59.0 42.4 63.6
119 33.1 25.4 38.2

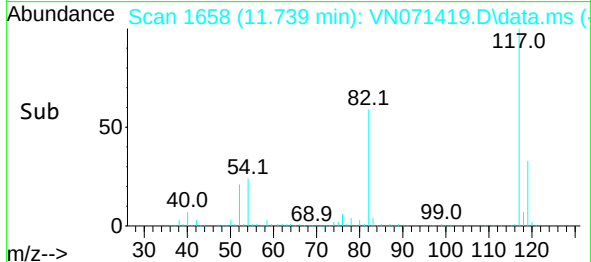

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.669 min Scan# 1986
Delta R.T. 0.001 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51


Tgt Ion:152 Resp: 419829
Ion Ratio Lower Upper
152 100
115 59.8 27.5 82.5
150 158.2 0.0 344.4

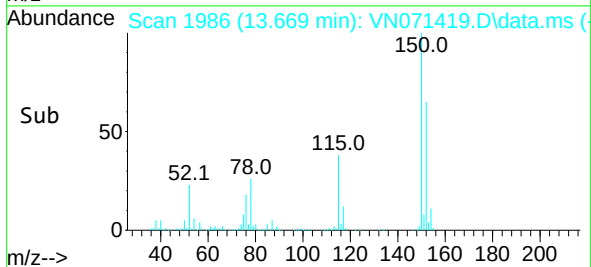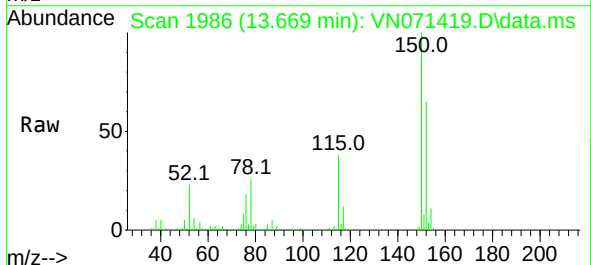






#74
N-amy1 acetate
Concen: 0.358 ug/l
RT: 12.386 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215



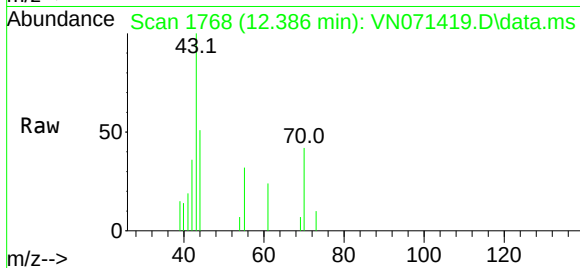



Tgt Ion:	43	Resp:	5449
Ion	Ratio	Lower	Upper
43	100		
70	46.2	33.4	50.0
55	19.0	19.3	28.9#
61	21.4	18.5	27.7



#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.822 min Scan# 1842
Delta R.T. 0.001 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Tgt Ion:	83	Resp:	1408
Ion	Ratio	Lower	Upper
83	100		
131	5.5	5.5	16.5
85	85.7	32.4	97.2


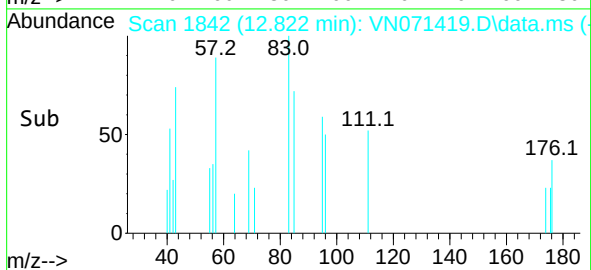

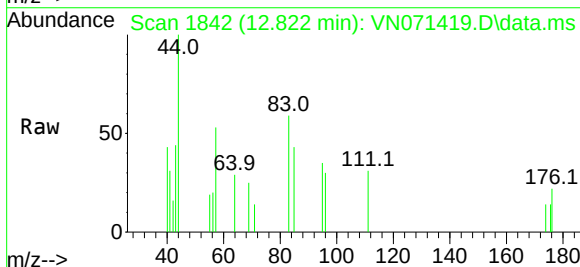




#76
1,2,3-Trichloropropane
Concen: 22.476 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion: 75 Resp: 244509
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#

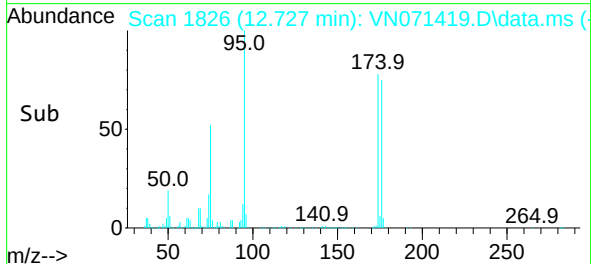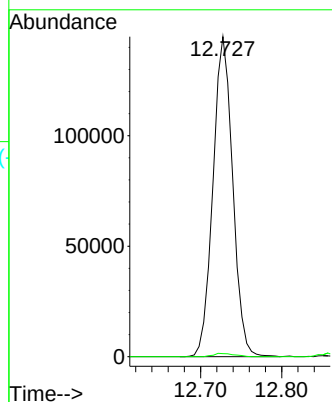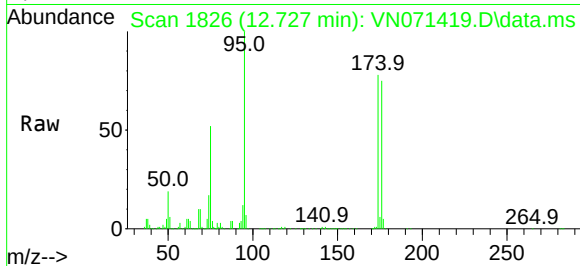

#81
trans-1,4-Dichloro-2-butene
Concen: 62.957 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Tgt Ion: 75 Resp: 244509
Ion Ratio Lower Upper
75 100
53 0.2 90.5 135.7#
89 0.0 38.2 57.4#

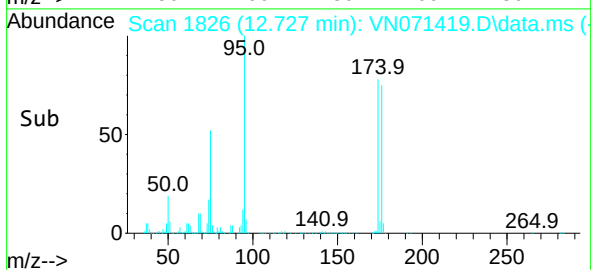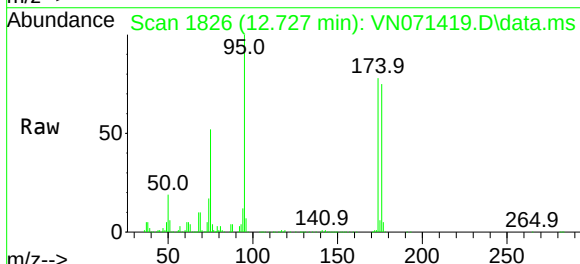



#87

1,3-Dichlorobenzene

Concen: 0.220 ug/l

RT: 13.616 min Scan# 1976

Delta R.T. 0.006 min

Lab File: VN071419.D

Acq: 21 Mar 2022 14:51

Instrument :

MSVOA_N

ClientSampleId :

CHRT-26215





Tgt Ion:146 Resp: 3372

Ion Ratio Lower Upper

146 100

111 44.1 18.6 55.6

148 51.3 31.6 95.0

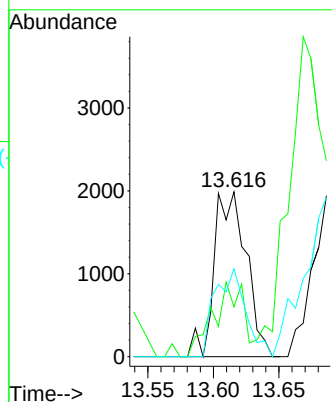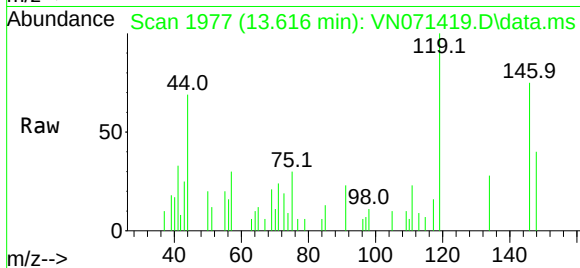

#88

1,4-Dichlorobenzene

Concen: 0.225 ug/l

RT: 13.616 min Scan# 1977

Delta R.T. -0.076 min

Lab File: VN071419.D

Acq: 21 Mar 2022 14:51




Tgt Ion:146 Resp: 3372


Ion Ratio Lower Upper

146 100

111 44.1 18.3 54.8

148 51.3 31.8 95.4


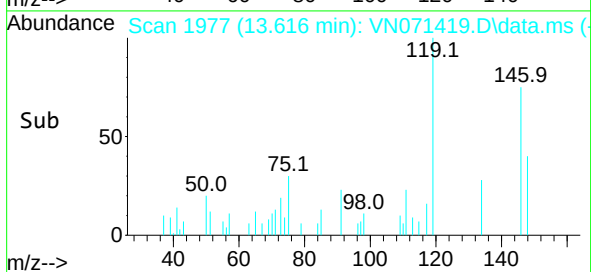
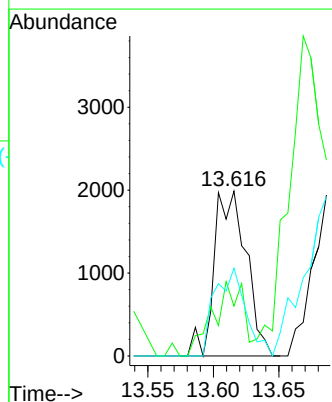
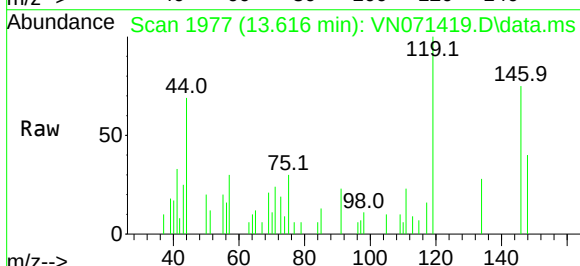


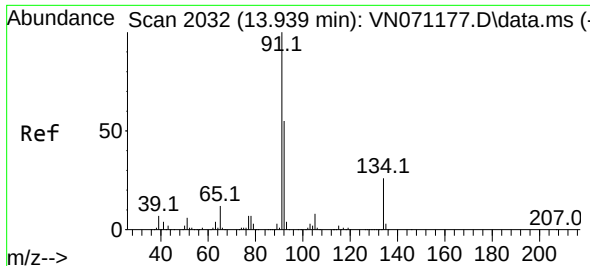

#89
n-Butylbenzene
Concen: 0.386 ug/l
RT: 13.939 min Scan# 2032
Delta R.T. 0.000 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion:	91	Resp:	8859
Ion	Ratio	Lower	Upper
91	100		
92	48.2	25.4	76.0
134	21.8	13.6	40.8

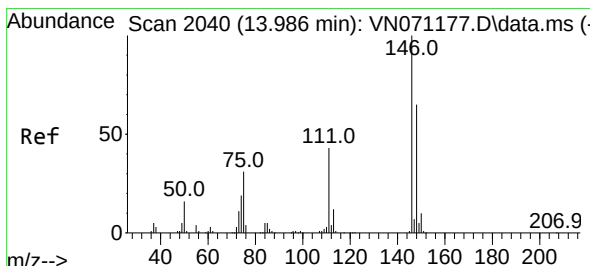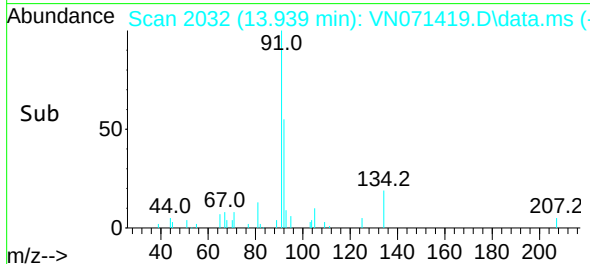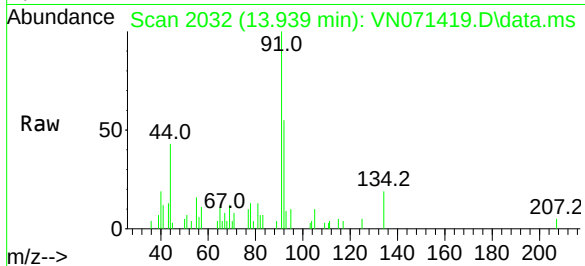

#91
1,2-Dichlorobenzene
Concen: 0.231 ug/l
RT: 13.986 min Scan# 2040
Delta R.T. 0.000 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51

Tgt Ion:	146	Resp:	3412
Ion	Ratio	Lower	Upper
146	100		
111	89.2	19.1	57.3
148	65.1	32.1	96.3


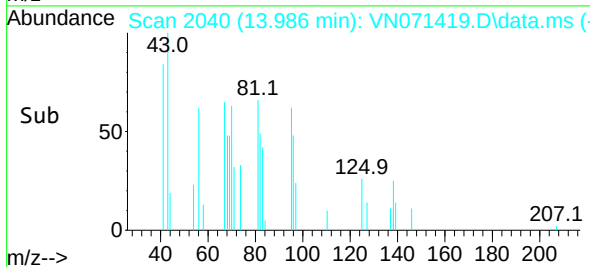

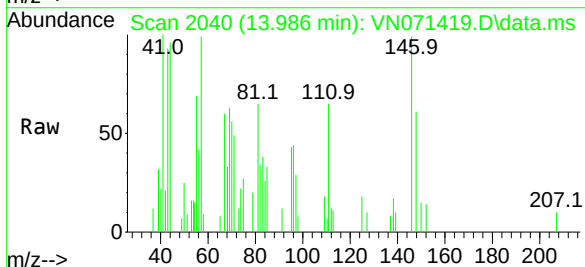


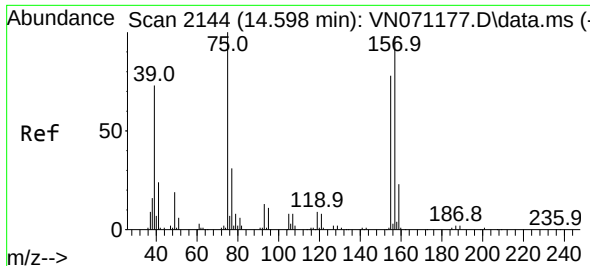

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.321 ug/l
 RT: 14.598 min Scan# 2144
 Delta R.T. 0.000 min
 Lab File: VN071419.D
 Acq: 21 Mar 2022 14:51




Instrument :
 MSVOA_N
 ClientSampleId :
 CHRT-26215


Tgt Ion: 75 Resp: 755
 Ion Ratio Lower Upper
 75 100
 155 67.9 46.9 140.7
 157 85.7 60.6 181.7

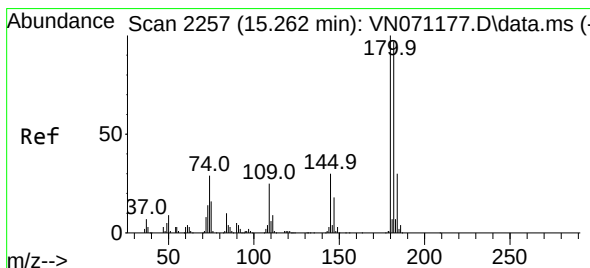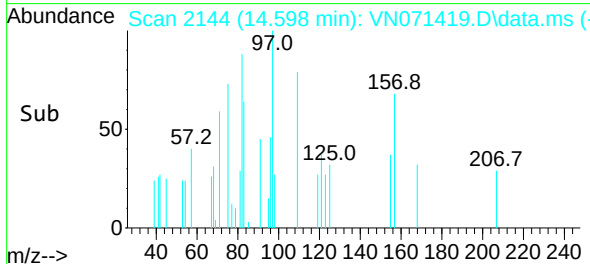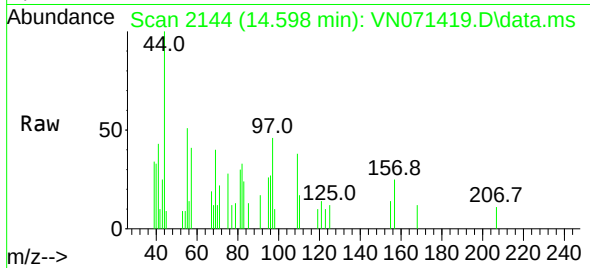

#93
 1,2,4-Trichlorobenzene
 Concen: 3.840 ug/l
 RT: 15.257 min Scan# 2256
 Delta R.T. -0.005 min
 Lab File: VN071419.D
 Acq: 21 Mar 2022 14:51

Tgt Ion: 180 Resp: 6229
 Ion Ratio Lower Upper
 180 100
 182 90.2 48.3 144.9
 145 44.2 14.5 43.5#


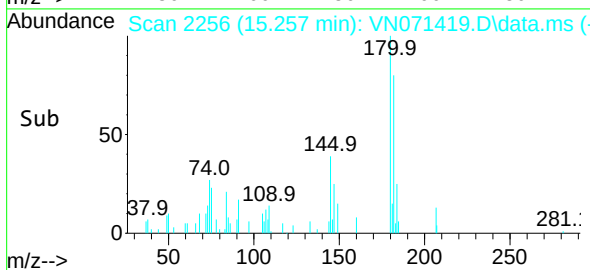

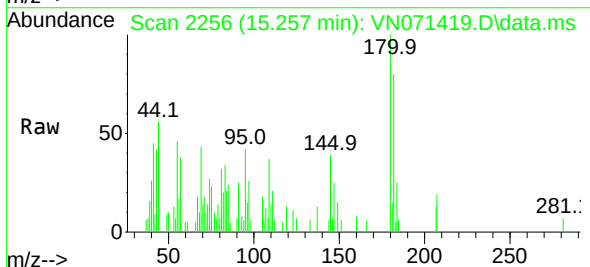




#94
Hexachlorobutadiene
Concen: 0.250 ug/l
RT: 15.357 min Scan# 21
Delta R.T. -0.005 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51




Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215


Tgt Ion:225 Resp: 1033
Ion Ratio Lower Upper
225 100
223 55.1 31.9 95.7
227 57.8 32.1 96.3

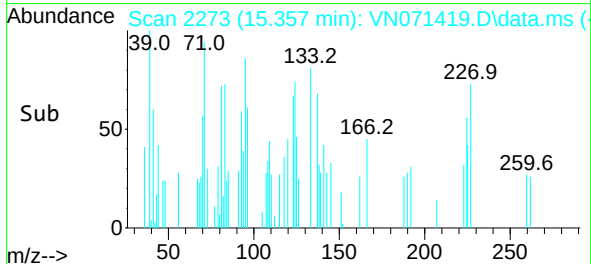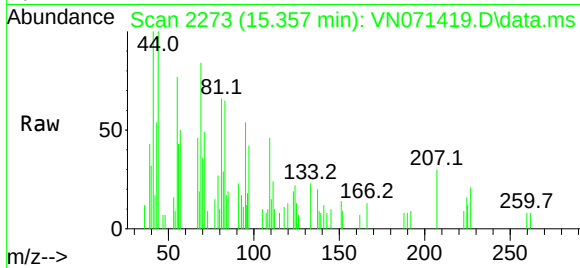

#95
Naphthalene
Concen: 6.297 ug/l
RT: 15.504 min Scan# 2298
Delta R.T. -0.000 min
Lab File: VN071419.D
Acq: 21 Mar 2022 14:51


Tgt Ion:128 Resp: 26324
Ion Ratio Lower Upper
128 100
127 14.2 10.5 15.7
129 11.5 8.7 13.1

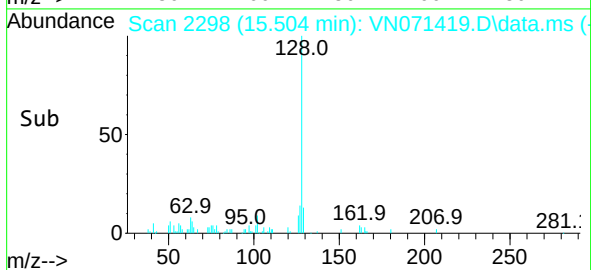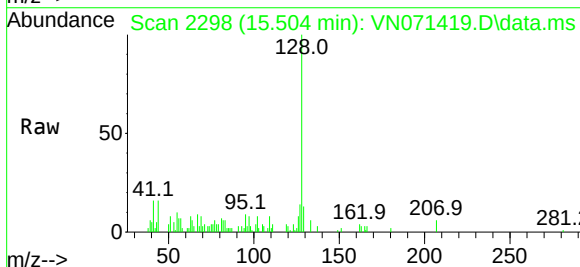



#96
 1,2,3-Trichlorobenzene
 Concen: 3.769 ug/l
 RT: 15.698 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN071419.D
 Acq: 21 Mar 2022 14:51

Instrument :
 MSVOA_N
 ClientSampleId :
 CHRT-26215

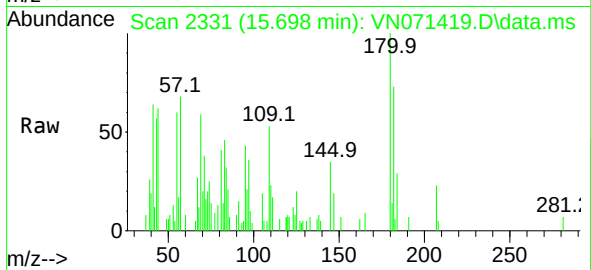

Tgt Ion:180 Resp: 7229
 Ion Ratio Lower Upper
 180 100
 182 80.5 47.4 142.2
 145 62.6 15.0 45.1#

