

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032122\
 Data File : VN071421.D
 Acq On : 21 Mar 2022 15:39
 Operator : JC\MD
 Sample : N1951-06
 Misc : 6.59g/5mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DB-14-(20-25)-3-12-22

Quant Time: Mar 21 16:27:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.075	168	627358	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	8.957	114	1056572	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	998095	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	394866	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.428	65	411089	47.811	ug/l	-0.01
Spiked Amount 50.000	Range 61 - 141		Recovery =	95.620%		
35) Dibromofluoromethane	8.010	113	296418	44.458	ug/l	-0.01
Spiked Amount 50.000	Range 69 - 133		Recovery =	88.920%		
50) Toluene-d8	10.433	98	1345277	50.113	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	100.220%		
62) 4-Bromofluorobenzene	12.727	95	455396	50.097	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	100.200%		
Target Compounds						Qvalue
3) Chloromethane	2.293	50	3751	0.372	ug/l	89
5) Bromomethane	2.799	94	2085	Below Cal		82
13) Acrolein	4.028	56	663	0.371	ug/l #	57
16) Acetone	4.304	43	6057	1.448	ug/l #	86
18) Methyl Acetate	4.851	43	26411	2.799	ug/l #	84
20) Methylene Chloride	5.093	84	137	0.400	ug/l #	59
25) 2-Butanone	7.345	43	9405	1.396	ug/l #	79
31) Cyclohexane	8.081	56	13713	0.999	ug/l #	24
36) 1,1-Dichloropropene	8.075	75	49365	4.621	ug/l #	49
37) Ethyl Acetate	7.345	43	9405	0.640	ug/l #	68
38) Carbon Tetrachloride	8.075	117	61386	5.941	ug/l #	15
43) Isopropyl Acetate	8.557	43	31737	1.444	ug/l #	58
49) 1,4-Dioxane	9.575	88	240	1.355	ug/l #	9
51) 4-Methyl-2-Pentanone	10.333	43	5315	0.390	ug/l #	86
58) 2-Chloroethyl Vinyl ether	10.045	63	116	27.903	ug/l #	45
59) 2-Hexanone	11.086	43	9538	1.025	ug/l	94
74) N-amyl acetate	12.386	43	4883	0.341	ug/l #	83
75) 1,1,2,2-Tetrachloroethane	12.822	83	1802	Below Cal	#	74
76) 1,2,3-Trichloropropane	12.727	75	235400	23.077	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	235400	64.444	ug/l #	5
87) 1,3-Dichlorobenzene	13.610	146	3513	0.244	ug/l	87
88) 1,4-Dichlorobenzene	13.610	146	3513	0.249	ug/l	86
89) n-Butylbenzene	13.939	91	6577	0.304	ug/l	87
91) 1,2-Dichlorobenzene	13.980	146	2935	0.212	ug/l	88
92) 1,2-Dibromo-3-Chloropr...	14.598	75	648	0.293	ug/l	68
93) 1,2,4-Trichlorobenzene	15.257	180	4114	3.587	ug/l #	82
95) Naphthalene	15.504	128	20672	6.094	ug/l	96
96) 1,2,3-Trichlorobenzene	15.698	180	5203	3.525	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032122\
Data File : VN071421.D
Acq On : 21 Mar 2022 15:39
Operator : JC\MD
Sample : N1951-06
Misc : 6.59g/5mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22

Quant Time: Mar 21 16:27:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration

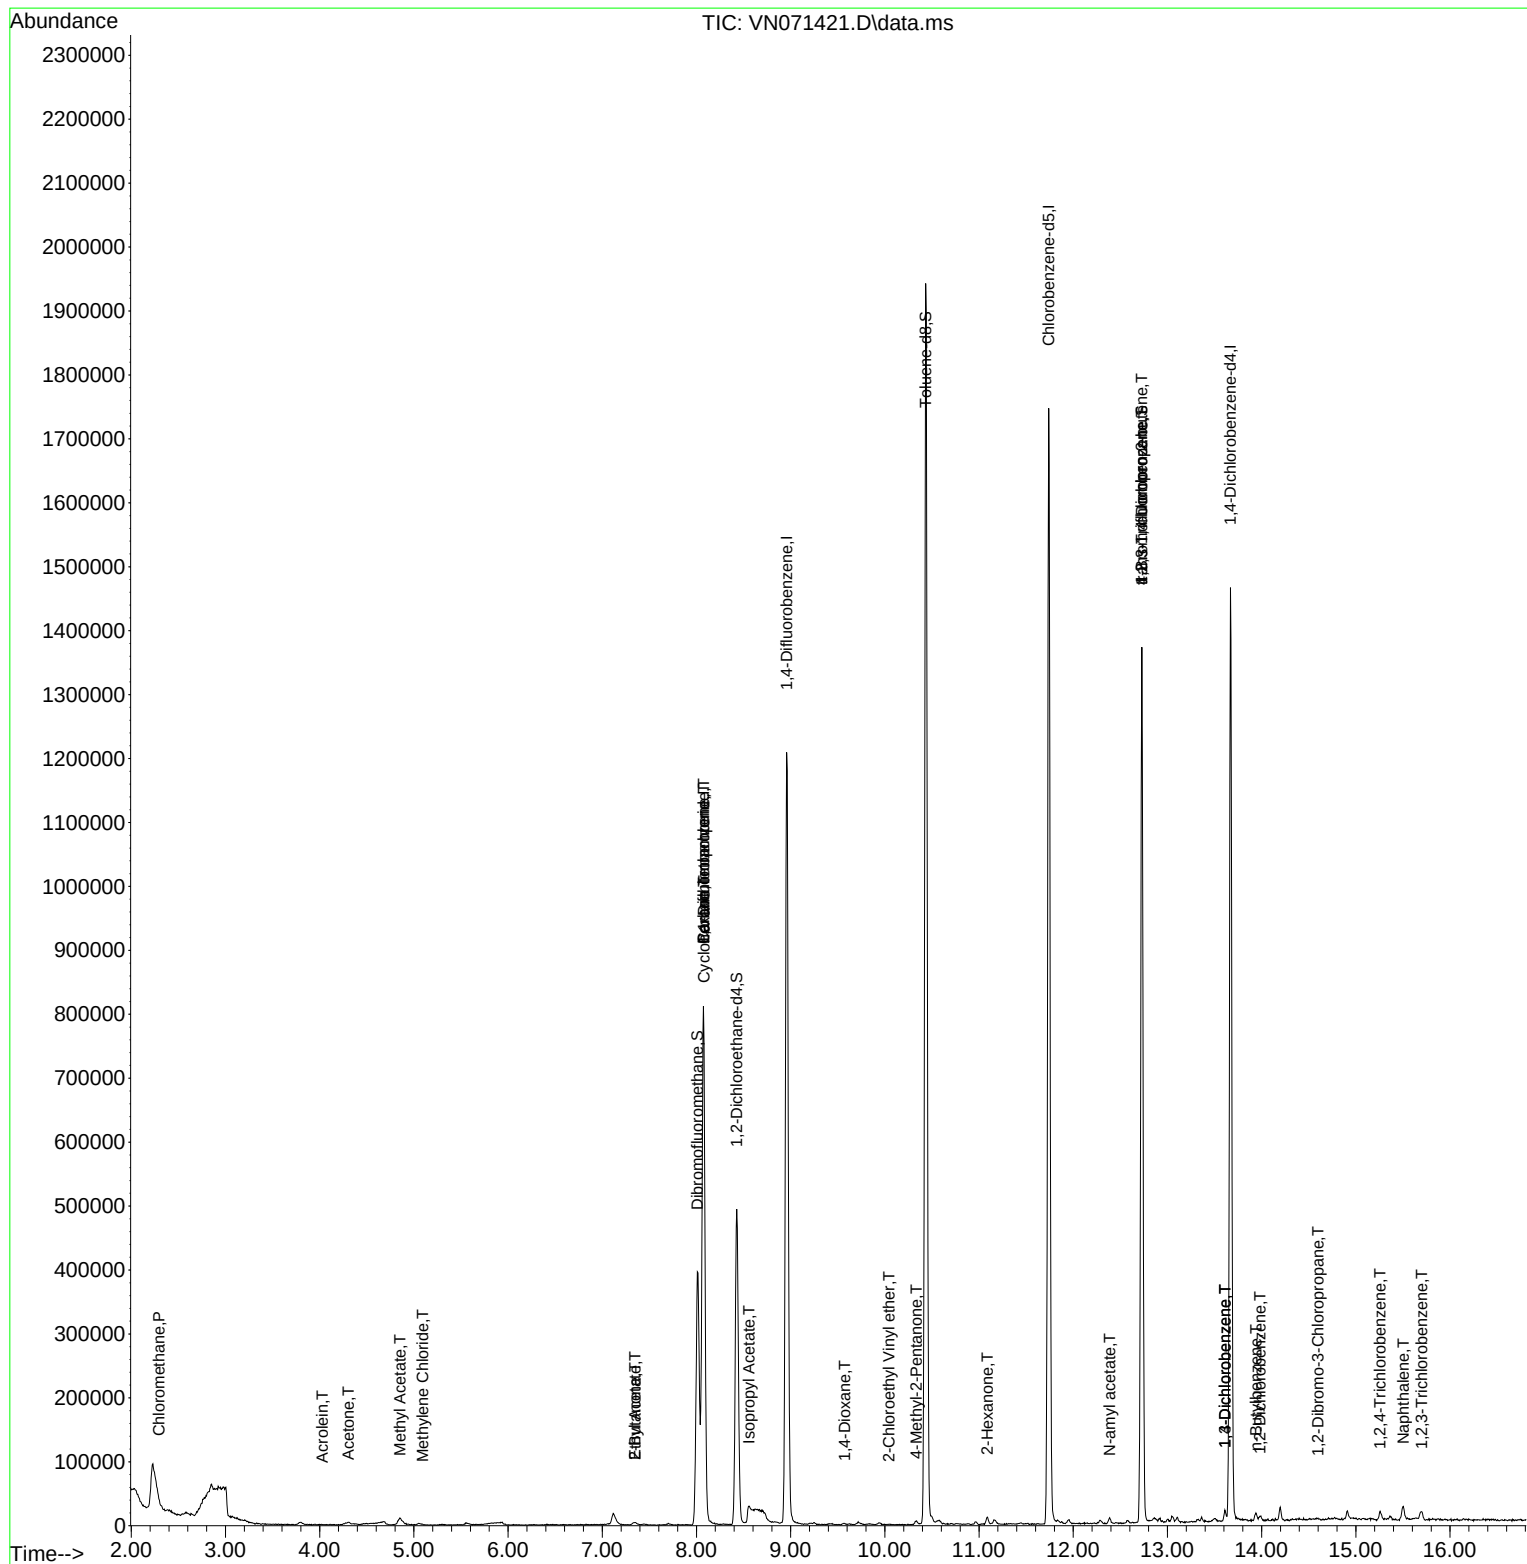



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.075 min Scan# 1

Delta R.T. -0.011 min

Lab File: VN071421.D

Acq: 21 Mar 2022 15:39

Instrument :

MSVOA_N

ClientSampleId :





DB-14-(20-25)-3-12-22

Tgt Ion:168 Resp: 627358

Ion Ratio Lower Upper

168 100

99 59.1 41.3 61.9

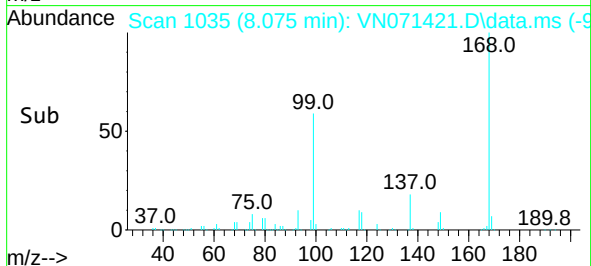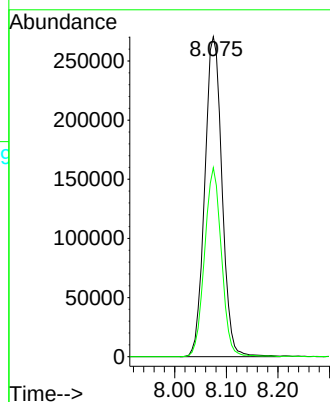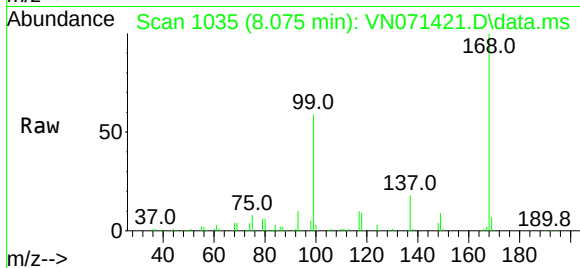

#3

Chloromethane

Concen: 0.372 ug/l

RT: 2.293 min Scan# 52

Delta R.T. -0.006 min

Lab File: VN071421.D




Acq: 21 Mar 2022 15:39


Tgt Ion: 50 Resp: 3751

Ion Ratio Lower Upper

50 100

52 25.4 25.4 38.0


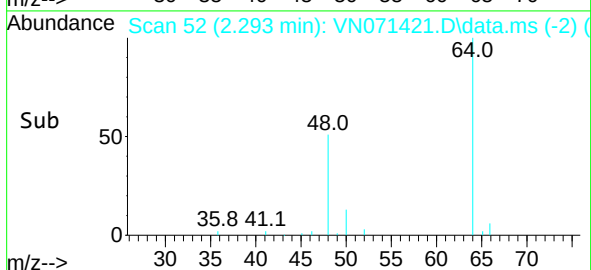
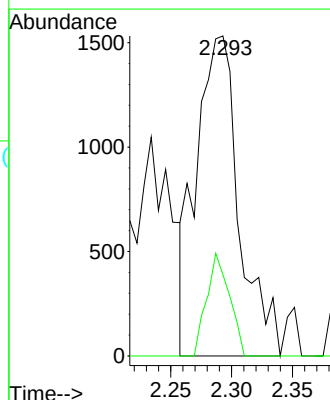
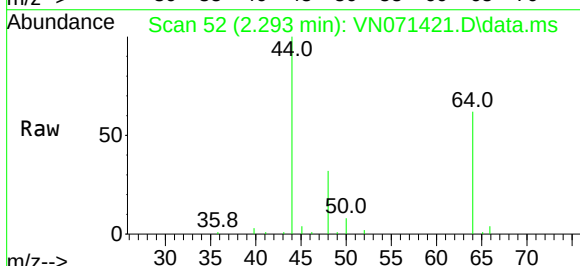


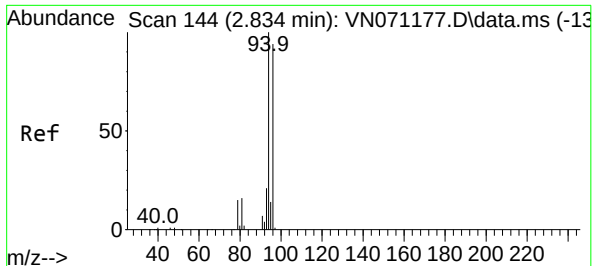

#5
Bromomethane
Concen: Below Cal
RT: 2.799 min Scan# 11
Delta R.T. -0.035 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39




Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22


Tgt Ion: 94 Resp: 2085
Ion Ratio Lower Upper
94 100
96 74.9 73.8 110.8

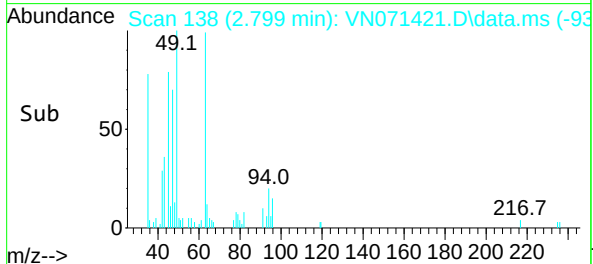

#13
Acrolein
Concen: 0.371 ug/l
RT: 4.028 min Scan# 347
Delta R.T. -0.012 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

Tgt Ion: 56 Resp: 663
Ion Ratio Lower Upper
56 100
55 35.4 56.6 85.0#

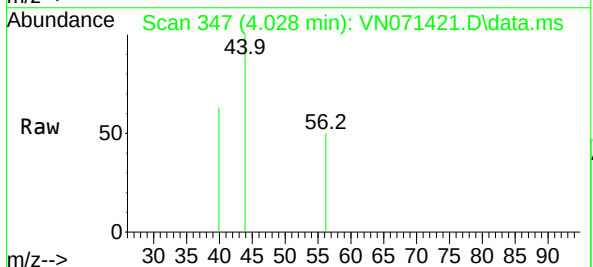

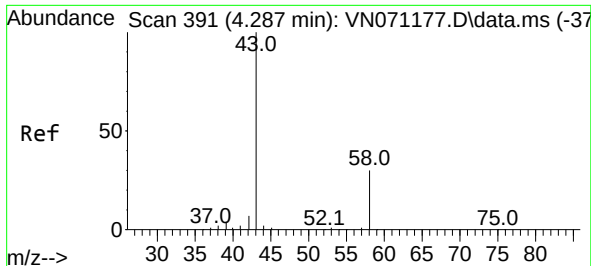

#16

Acetone

Concen: 1.448 ug/l

RT: 4.304 min Scan# 391

Delta R.T. 0.018 min

Lab File: VN071421.D

Acq: 21 Mar 2022 15:39

Instrument :

MSVOA_N

ClientSampleId :





DB-14-(20-25)-3-12-22

Tgt Ion: 43 Resp: 6057

Ion Ratio Lower Upper

43 100

58 21.4 23.1 34.7#

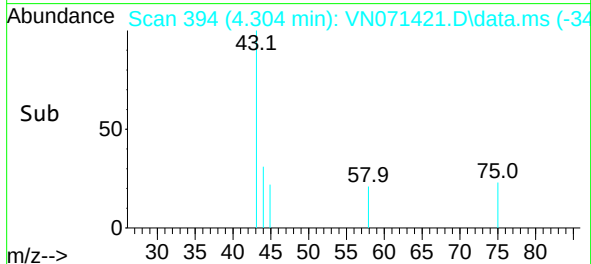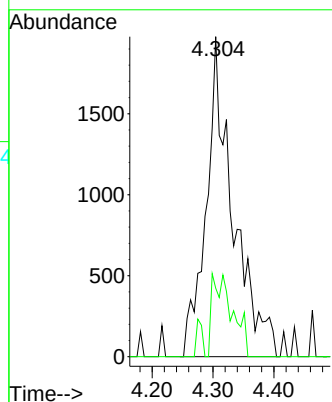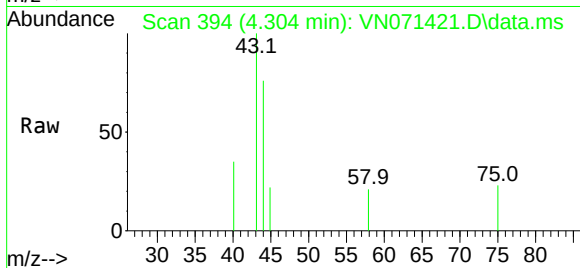

#18

Methyl Acetate

Concen: 2.799 ug/l

RT: 4.851 min Scan# 487

Delta R.T. 0.000 min

Lab File: VN071421.D




Acq: 21 Mar 2022 15:39


Tgt Ion: 43 Resp: 26411

Ion Ratio Lower Upper

43 100


74 16.5 19.4 29.2#

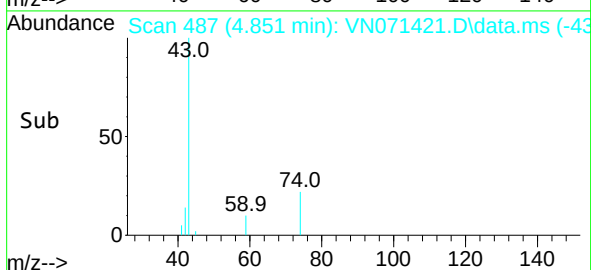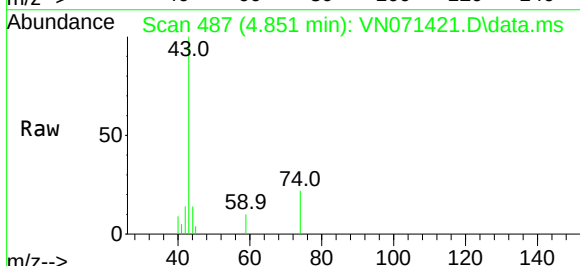



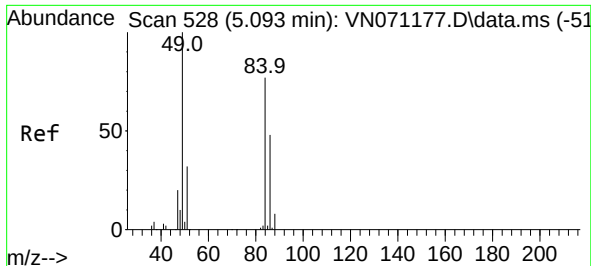


#20
Methylene Chloride
Concen: 0.400 ug/l
RT: 5.093 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39


Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22





Tgt Ion: 84 Resp: 137
Ion Ratio Lower Upper
84 100
49 177.5 93.5 140.3#
51 0.0 29.4 44.2#
86 68.8 53.0 79.4

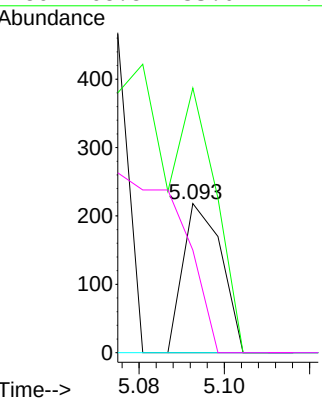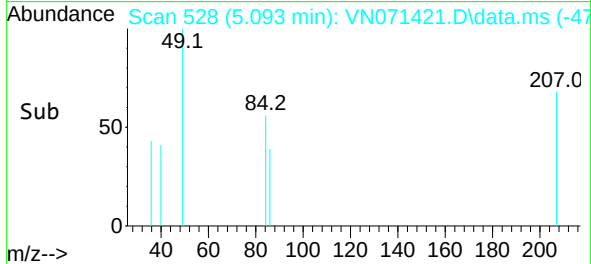


#25
2-Butanone
Concen: 1.396 ug/l
RT: 7.345 min Scan# 911
Delta R.T. 0.012 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

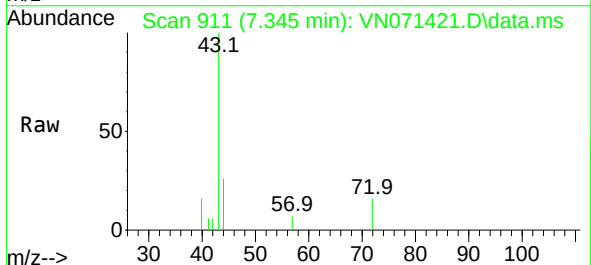


Tgt Ion: 43 Resp: 9405
Ion Ratio Lower Upper
43 100
72 16.1 21.7 32.5#

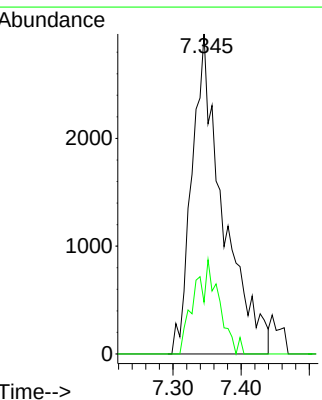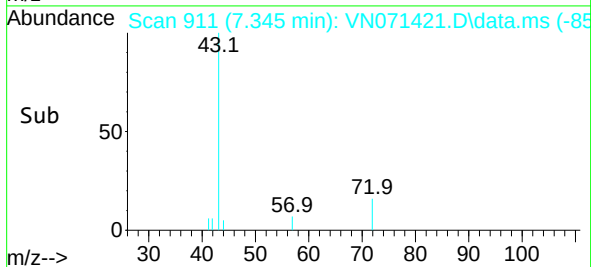






#31
Cyclohexane
Concen: 0.999 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.012 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22







Tgt Ion: 56 Resp: 13713
Ion Ratio Lower Upper
56 100
69 143.5 27.1 40.7#
84 123.0 73.4 110.0#

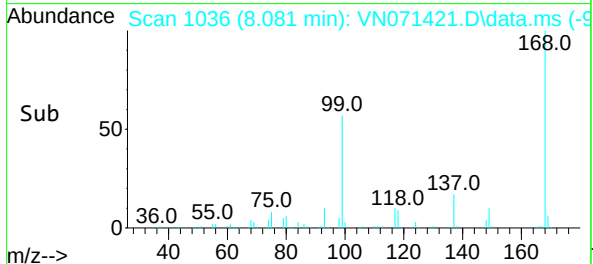

#33
1,2-Dichloroethane-d4
Concen: 47.811 ug/l
RT: 8.428 min Scan# 1095
Delta R.T. -0.012 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

Tgt Ion: 65 Resp: 411089
Ion Ratio Lower Upper
65 100
67 53.6 0.0 103.0

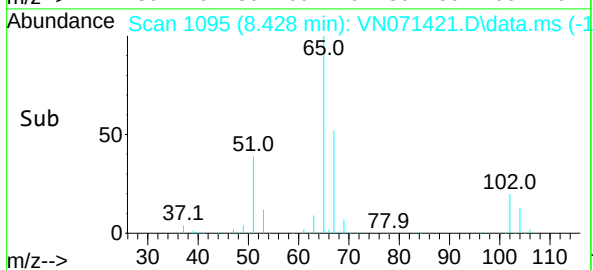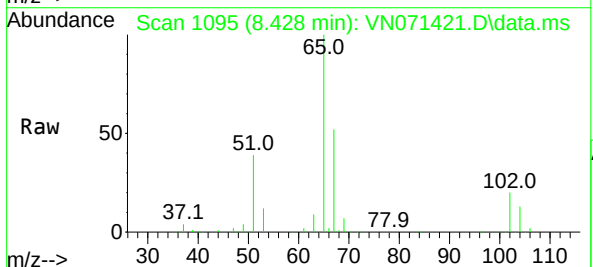

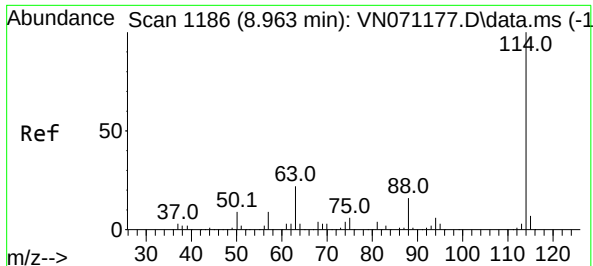

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.957 min Scan# 1185

Delta R.T. -0.006 min

Lab File: VN071421.D

Acq: 21 Mar 2022 15:39

Instrument :

MSVOA_N

ClientSampleId :

DB-14-(20-25)-3-12-22





Tgt Ion:114 Resp: 1056572

Ion Ratio Lower Upper

114 100

63 22.6 0.0 37.8

88 16.2 0.0 27.4

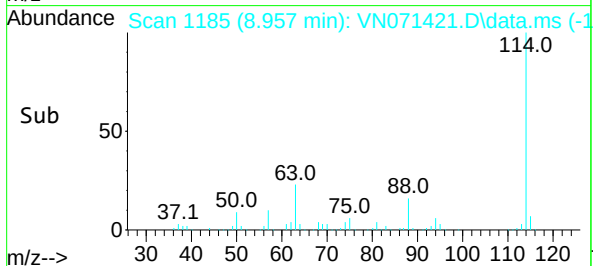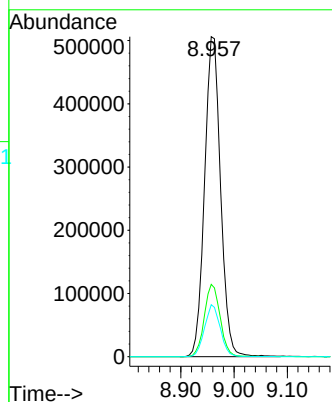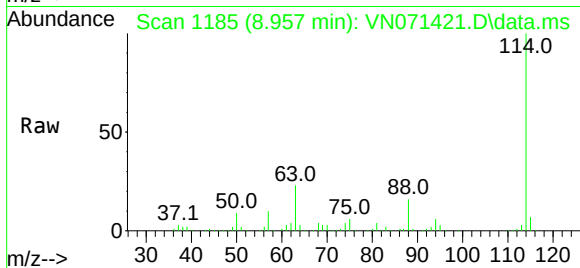

#35

Dibromofluoromethane

Concen: 44.458 ug/l

RT: 8.010 min Scan# 1024

Delta R.T. -0.012 min

Lab File: VN071421.D

Acq: 21 Mar 2022 15:39




Tgt Ion:113 Resp: 296418


Ion Ratio Lower Upper

113 100

111 103.4 82.2 123.2

192 20.4 16.9 25.3

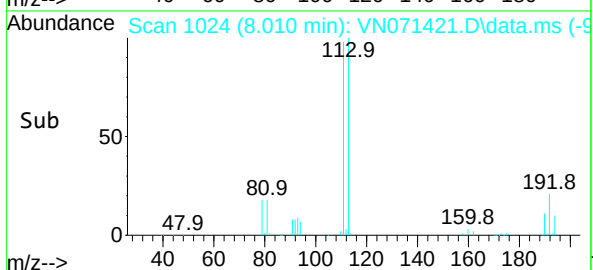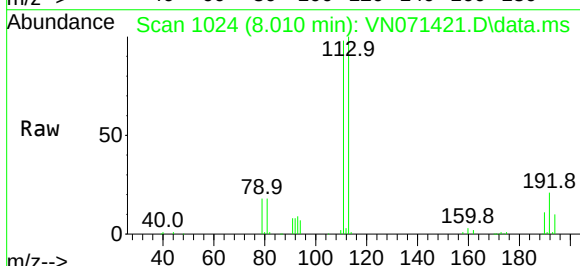

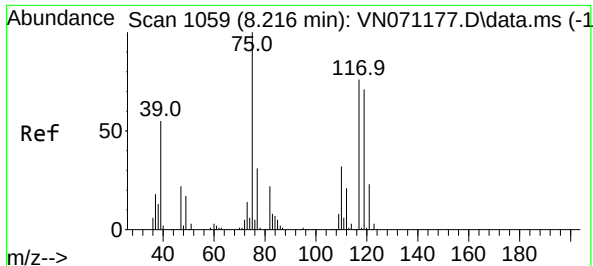

#36

1,1-Dichloropropene

Concen: 4.621 ug/l

RT: 8.075 min Scan# 1

Delta R.T. -0.141 min

Lab File: VN071421.D

Acq: 21 Mar 2022 15:39

Instrument :

MSVOA_N

ClientSampleId :

DB-14-(20-25)-3-12-22





Tgt Ion: 75 Resp: 49365

Ion Ratio Lower Upper

75 100

110 8.4 18.4 55.2#

77 0.0 24.4 36.6#

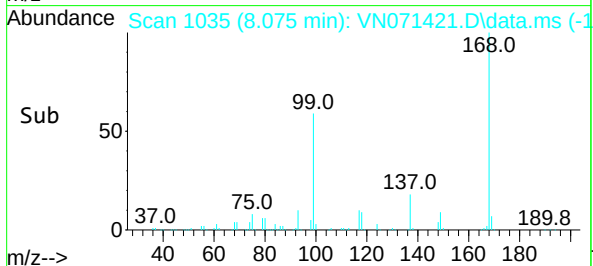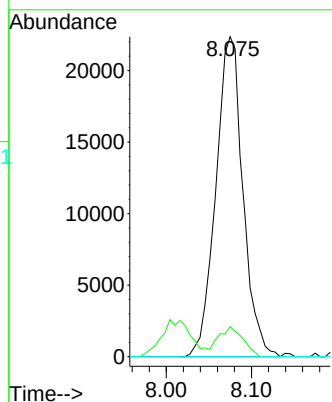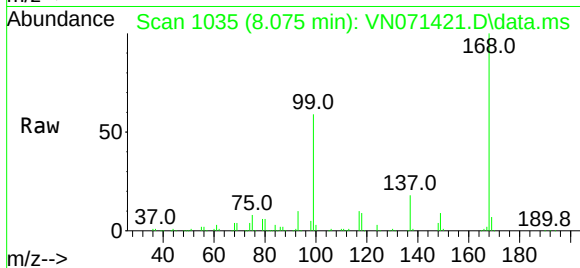

#37

Ethyl Acetate

Concen: 0.640 ug/l

RT: 7.345 min Scan# 911

Delta R.T. -0.065 min

Lab File: VN071421.D

Acq: 21 Mar 2022 15:39




Tgt Ion: 43 Resp: 9405


Ion Ratio Lower Upper

43 100

61 0.0 11.5 17.3#


70 0.0 7.9 11.9#

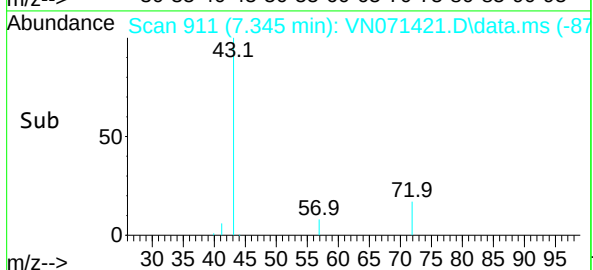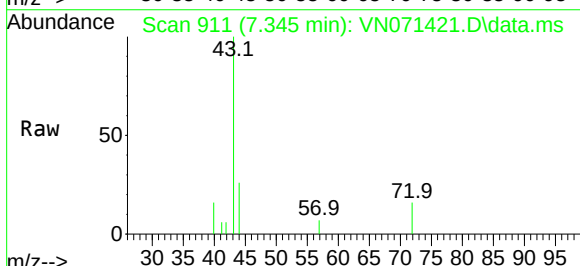






#38
Carbon Tetrachloride
Concen: 5.941 ug/l
RT: 8.075 min Scan# 1105
Delta R.T. -0.129 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39


Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22





Tgt Ion:117 Resp: 61386
Ion Ratio Lower Upper
117 100
119 3.8 76.1 114.1#
121 0.0 24.2 36.2#

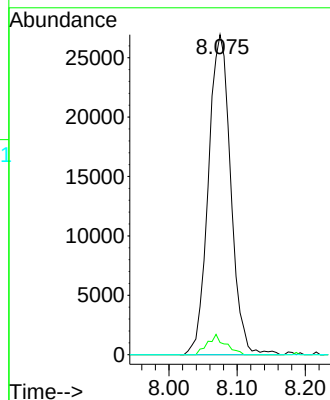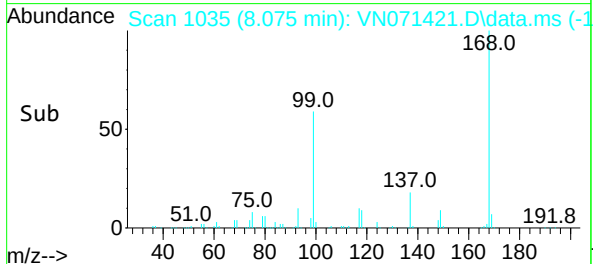


#43
Isopropyl Acetate
Concen: 1.444 ug/l
RT: 8.557 min Scan# 1117
Delta R.T. 0.000 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

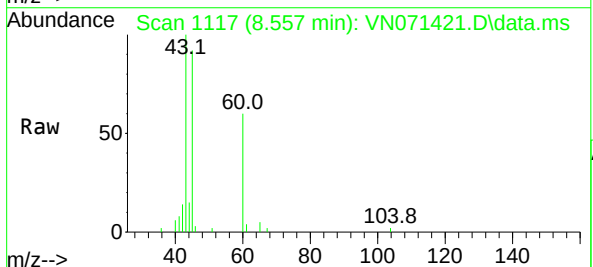

Tgt Ion: 43 Resp: 31737
Ion Ratio Lower Upper
43 100
61 1.9 20.4 30.6#
87 0.0 11.2 16.8#



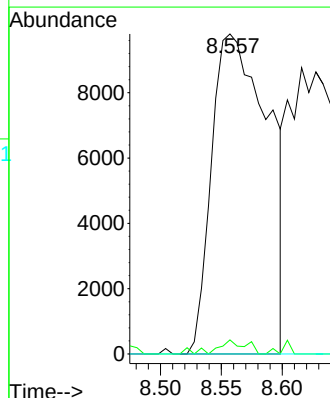



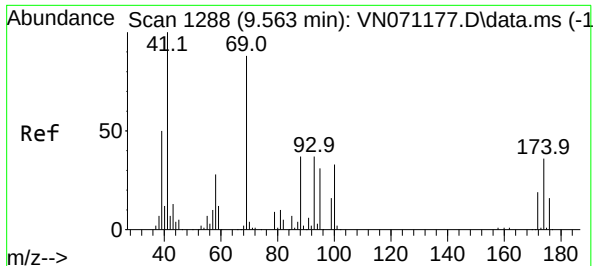

#49
1,4-Dioxane
Concen: 1.355 ug/l
RT: 9.575 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39




Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22


Tgt Ion: 88 Resp: 240
Ion Ratio Lower Upper
88 100
43 89.6 23.4 35.2#
58 0.0 50.6 75.8#

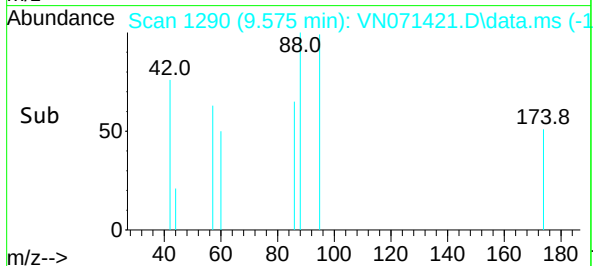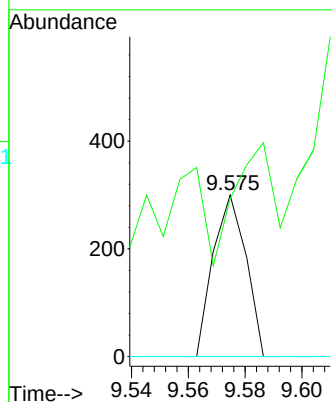

#50
Toluene-d8
Concen: 50.113 ug/l
RT: 10.433 min Scan# 1436
Delta R.T. -0.006 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

Tgt Ion: 98 Resp: 1345277
Ion Ratio Lower Upper
98 100
100 65.2 50.4 75.6


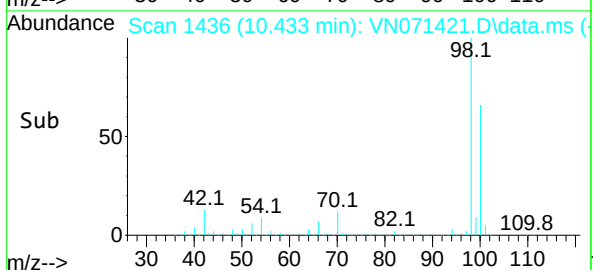

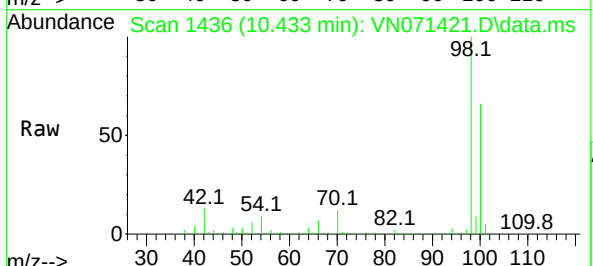




#51
4-Methyl-2-Pentanone
Concen: 0.390 ug/l
RT: 10.333 min Scan# 1418
Delta R.T. 0.006 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39




Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22


Tgt Ion: 43 Resp: 5315
Ion Ratio Lower Upper
43 100
58 29.6 30.4 45.6#

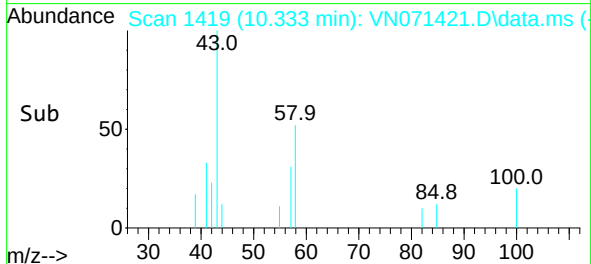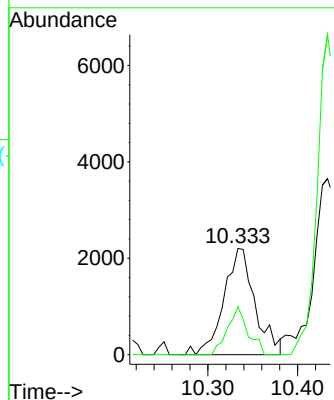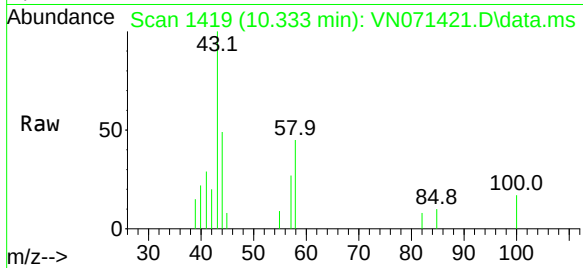

#58
2-Chloroethyl Vinyl ether
Concen: 27.903 ug/l
RT: 10.045 min Scan# 1370
Delta R.T. 0.006 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

Tgt Ion: 63 Resp: 116
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#


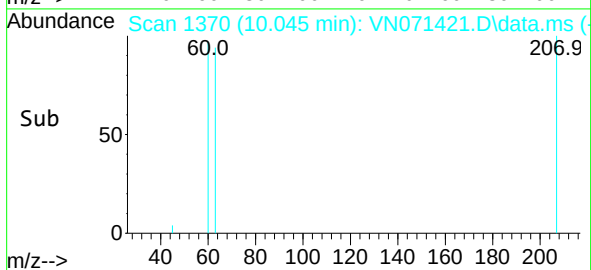
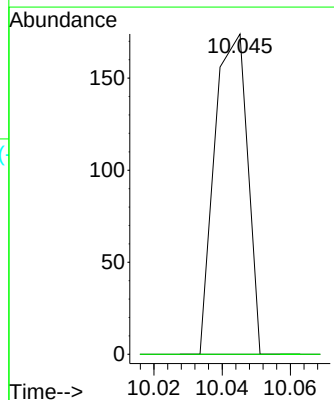
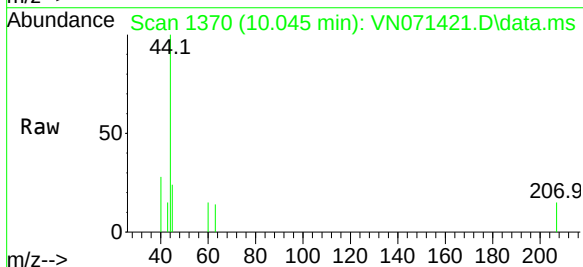


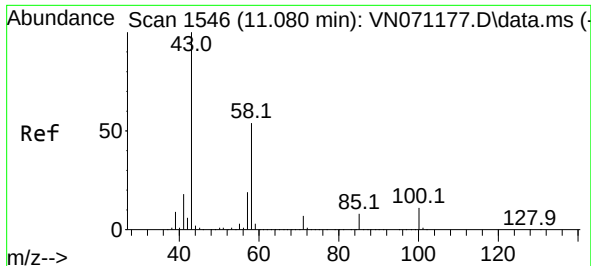

#59
2-Hexanone
Concen: 1.025 ug/l
RT: 11.086 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39




Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22


Tgt Ion: 43 Resp: 9538
Ion Ratio Lower Upper
43 100
58 49.2 26.9 80.7

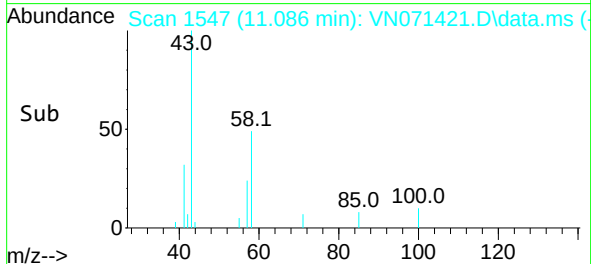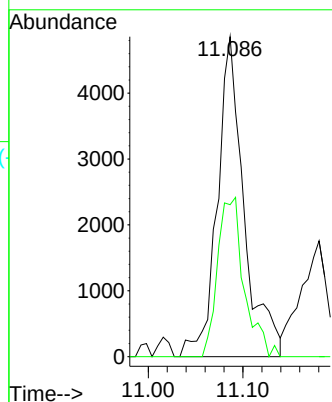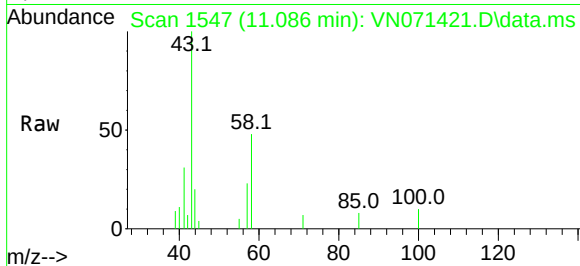

#62
4-Bromofluorobenzene
Concen: 50.097 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

Tgt Ion: 95 Resp: 455396
Ion Ratio Lower Upper
95 100
174 78.1 0.0 187.2
176 75.6 0.0 181.4


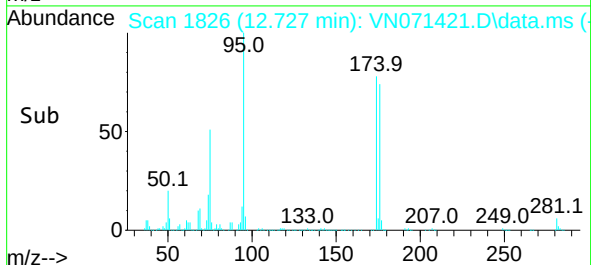

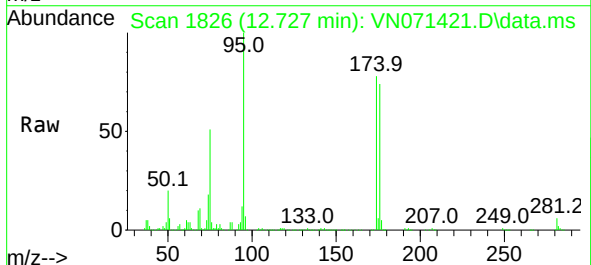


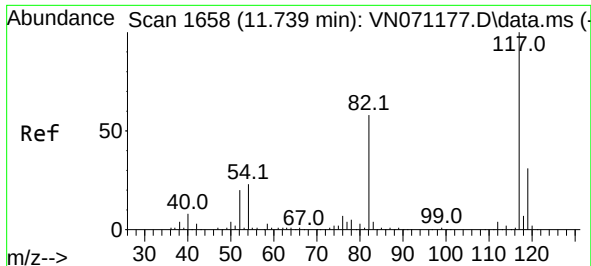

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39




Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22


Tgt Ion:117 Resp: 998095
Ion Ratio Lower Upper
117 100
82 57.7 42.4 63.6
119 31.7 25.4 38.2

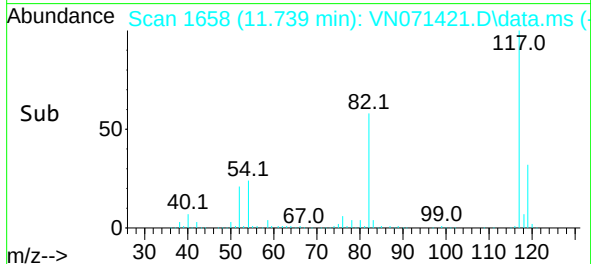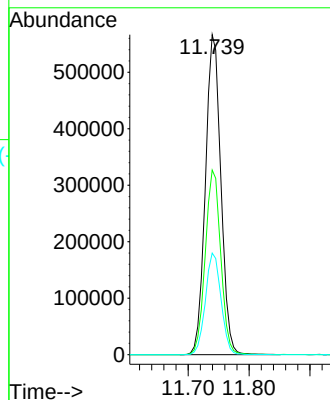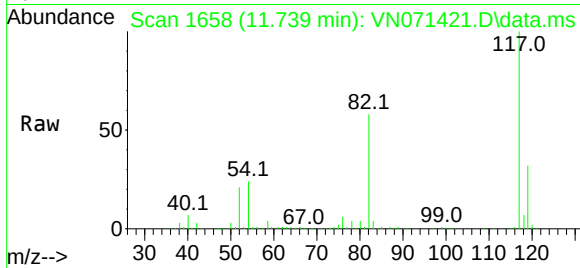

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.669 min Scan# 1986
Delta R.T. 0.001 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

Tgt Ion:152 Resp: 394866
Ion Ratio Lower Upper
152 100
115 58.5 27.5 82.5
150 157.7 0.0 344.4



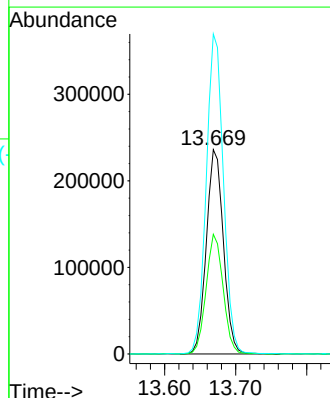
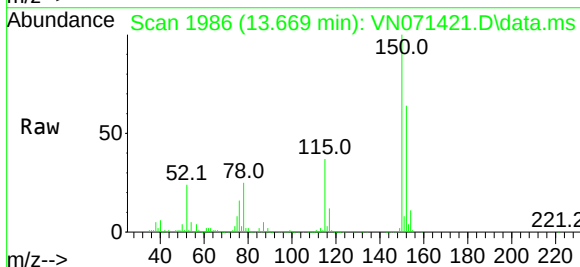




#74
N-amy1 acetate
Concen: 0.341 ug/l
RT: 12.386 min Scan# 1768
Delta R.T. 0.000 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39




Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22


Tgt Ion: 43	Resp: 4883
Ion Ratio	Lower Upper
43 100	
70 34.8	33.4 50.0
55 44.1	19.3 28.9#
61 21.0	18.5 27.7

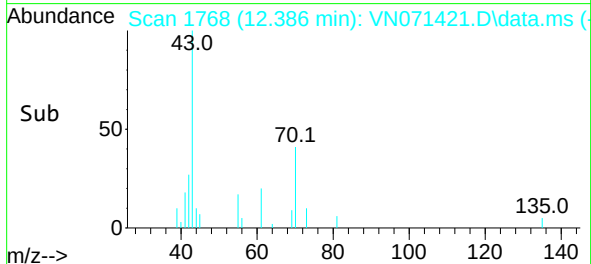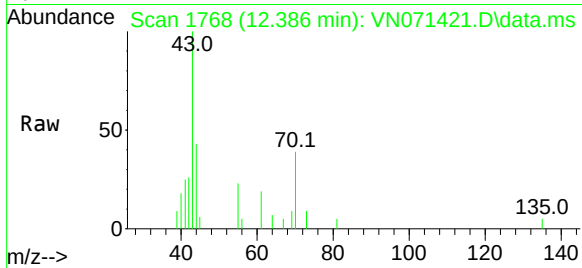

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.822 min Scan# 1842
Delta R.T. 0.001 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

Tgt Ion: 83	Resp: 1802
Ion Ratio	Lower Upper
83 100	
131 0.0	5.5 16.5#
85 44.3	32.4 97.2



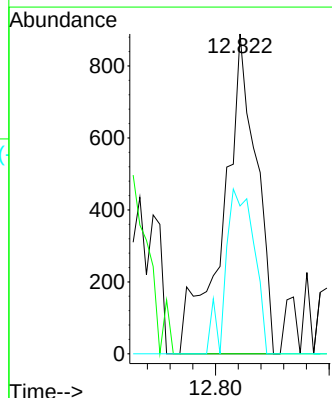
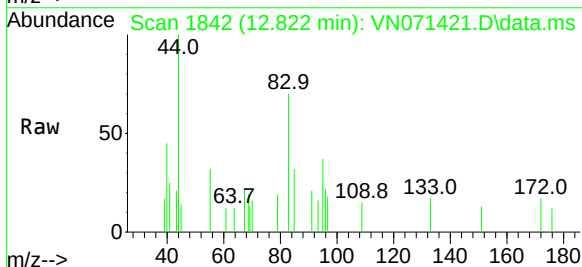


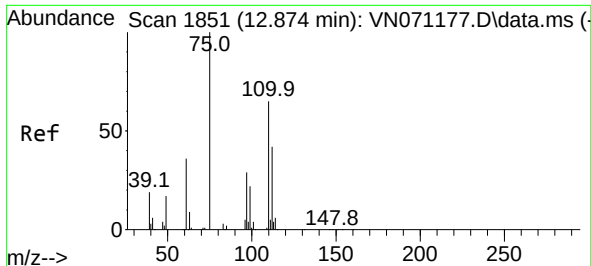

#76
1,2,3-Trichloropropane
Concen: 23.077 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39




Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22


Tgt Ion: 75 Resp: 235400
Ion Ratio Lower Upper
75 100
77 1.4 82.6 247.8#

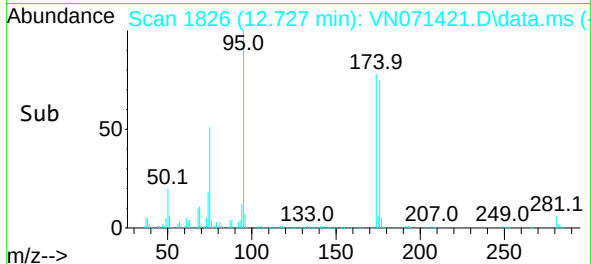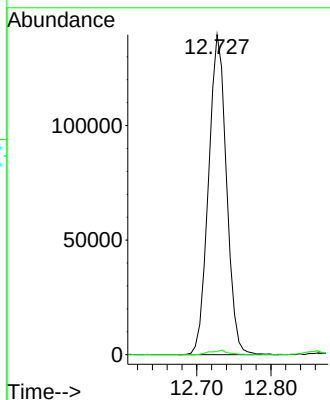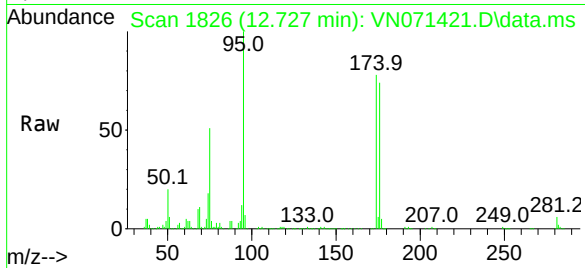

#81
trans-1,4-Dichloro-2-butene
Concen: 64.444 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

Tgt Ion: 75 Resp: 235400
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#



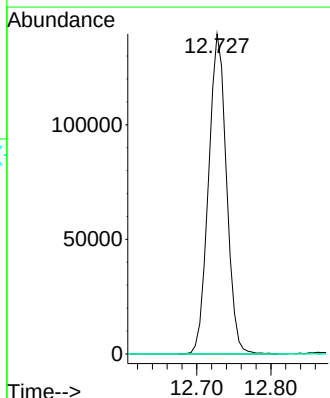
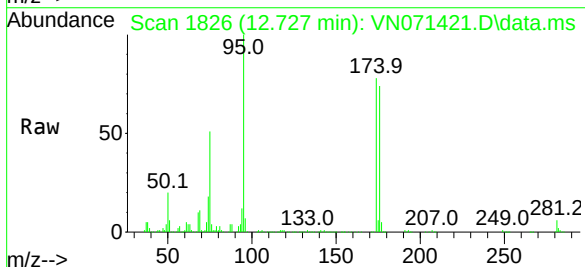


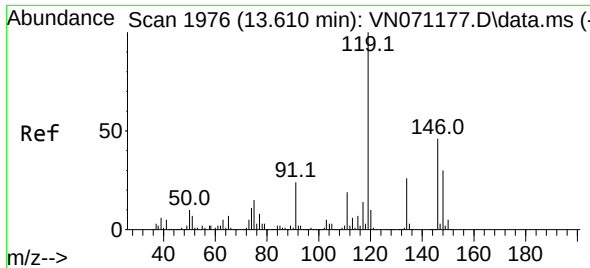

#87
1,3-Dichlorobenzene
Concen: 0.244 ug/l
RT: 13.610 min Scan# 1976
Delta R.T. 0.000 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39




Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22


Tgt Ion:146	Resp:	3513
Ion	Ratio	Lower Upper
146	100	
111	43.6	18.6 55.6
148	52.4	31.6 95.0

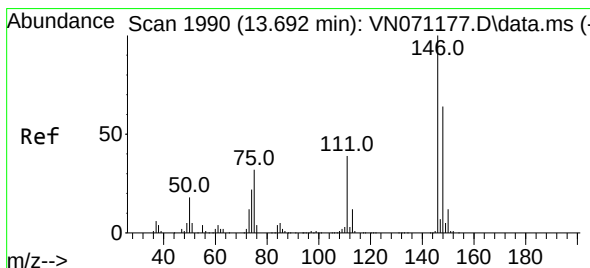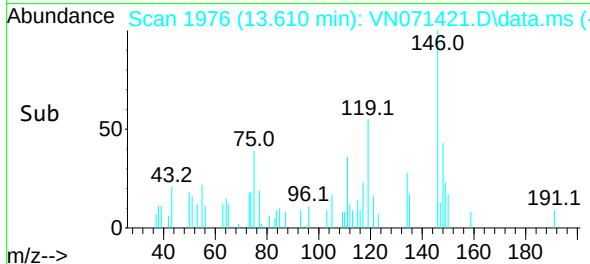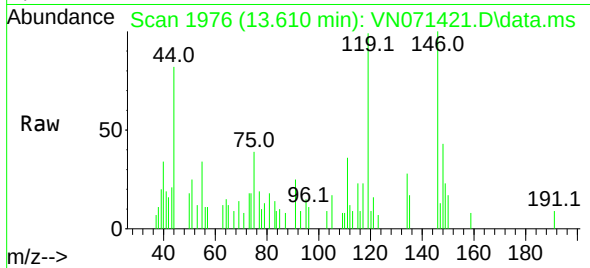

#88
1,4-Dichlorobenzene
Concen: 0.249 ug/l
RT: 13.610 min Scan# 1976
Delta R.T. -0.082 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

Tgt Ion:146	Resp:	3513
Ion	Ratio	Lower Upper
146	100	
111	43.6	18.3 54.8
148	52.4	31.8 95.4


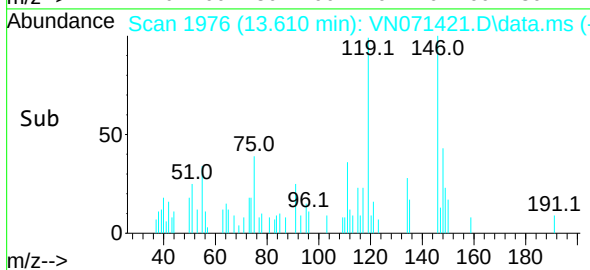

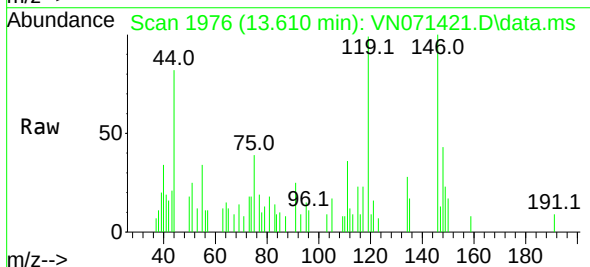


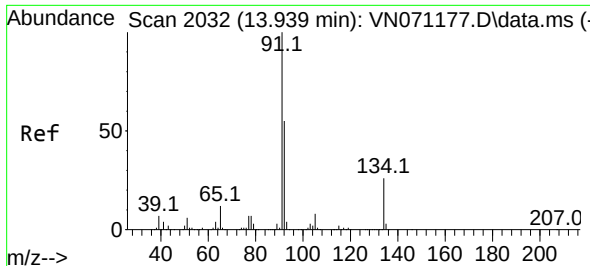

#89
n-Butylbenzene
Concen: 0.304 ug/l
RT: 13.939 min Scan# 2032
Delta R.T. 0.000 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39




Instrument :
MSVOA_N
ClientSampleId :
DB-14-(20-25)-3-12-22


Tgt Ion: 91	Resp:	6577	
Ion	Ratio	Lower	Upper
91	100		
92	60.3	25.4	76.0
134	20.8	13.6	40.8

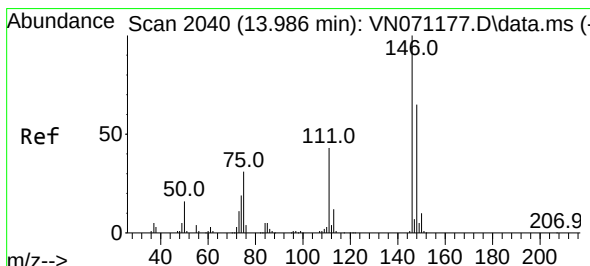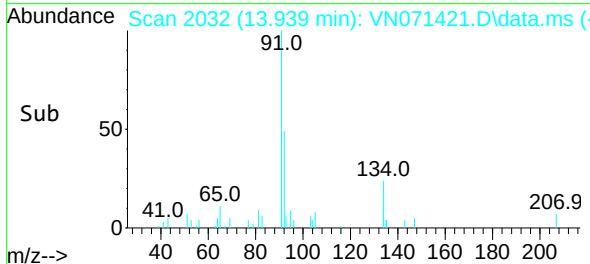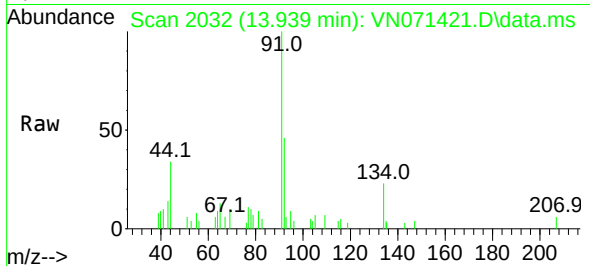

#91
1,2-Dichlorobenzene
Concen: 0.212 ug/l
RT: 13.980 min Scan# 2039
Delta R.T. -0.006 min
Lab File: VN071421.D
Acq: 21 Mar 2022 15:39

Tgt Ion:146	Resp:	2935	
Ion	Ratio	Lower	Upper
146	100		
111	53.8	19.1	57.3
148	61.4	32.1	96.3


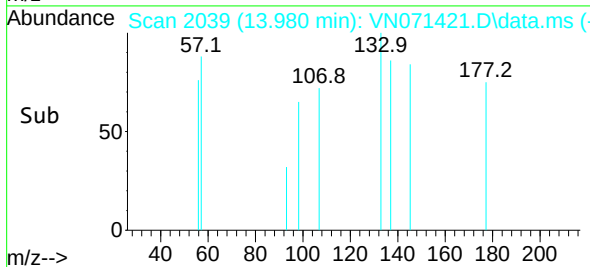

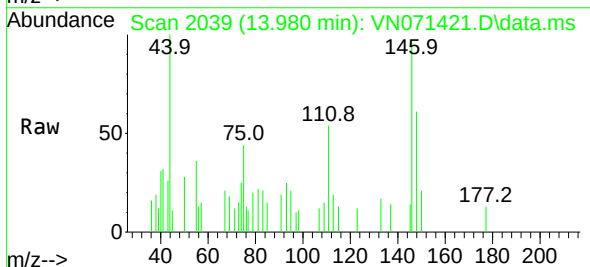


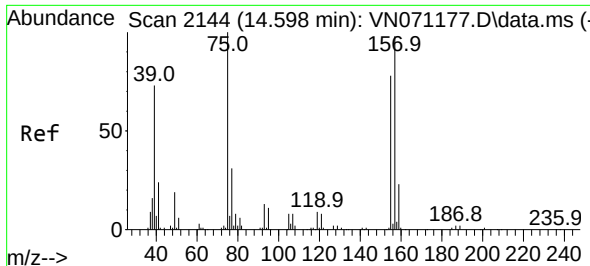

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.293 ug/l
 RT: 14.598 min Scan# 2144
 Delta R.T. 0.000 min
 Lab File: VN071421.D
 Acq: 21 Mar 2022 15:39




Instrument :
 MSVOA_N
 ClientSampleId :
 DB-14-(20-25)-3-12-22


Tgt Ion: 75 Resp: 648
 Ion Ratio Lower Upper
 75 100
 155 76.2 46.9 140.7
 157 169.0 60.6 181.7

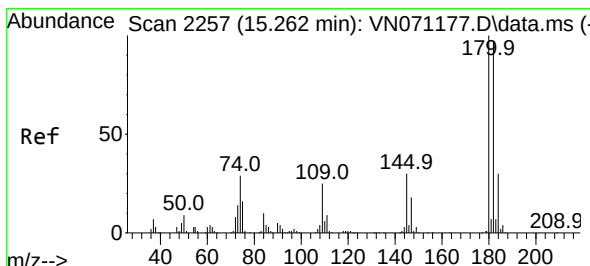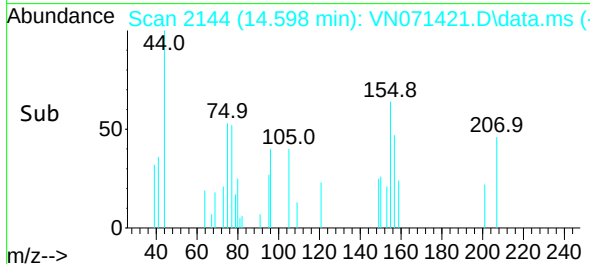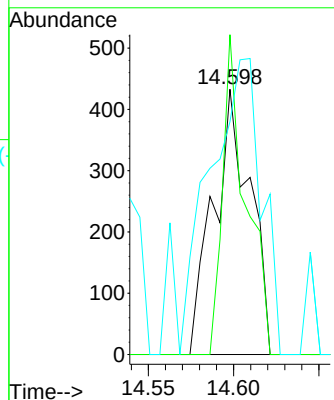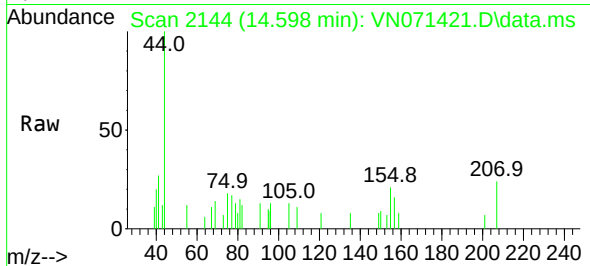

#93
 1,2,4-Trichlorobenzene
 Concen: 3.587 ug/l
 RT: 15.257 min Scan# 2256
 Delta R.T. -0.005 min
 Lab File: VN071421.D
 Acq: 21 Mar 2022 15:39

Tgt Ion: 180 Resp: 4114
 Ion Ratio Lower Upper
 180 100
 182 109.1 48.3 144.9
 145 48.7 14.5 43.5#

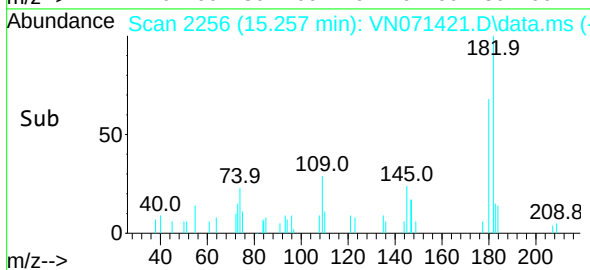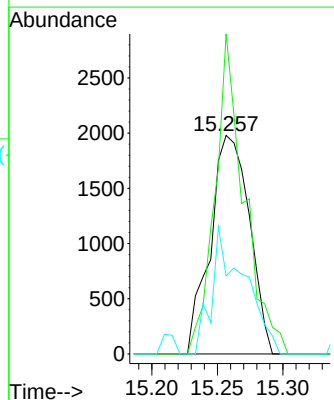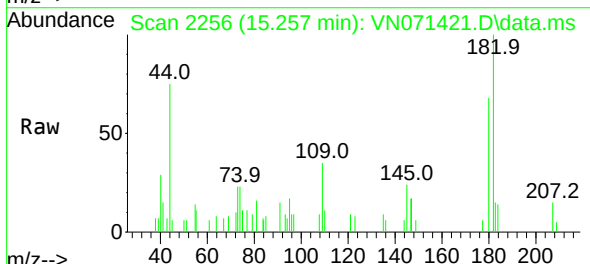

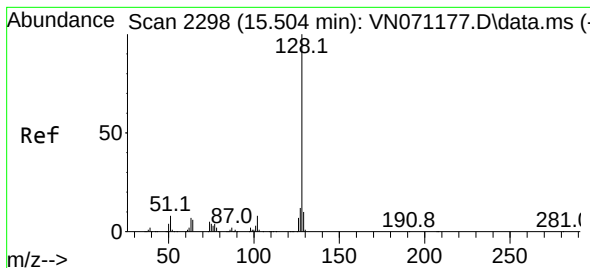

#95

Naphthalene

Concen: 6.094 ug/l

RT: 15.504 min Scan# 2298

Delta R.T. -0.000 min

Lab File: VN071421.D

Acq: 21 Mar 2022 15:39

Instrument :

MSVOA_N

ClientSampleId :

DB-14-(20-25)-3-12-22





Tgt Ion:128 Resp: 20672

Ion Ratio Lower Upper

128 100

127 11.7 10.5 15.7

129 12.8 8.7 13.1

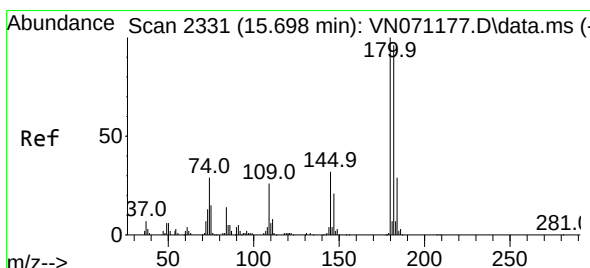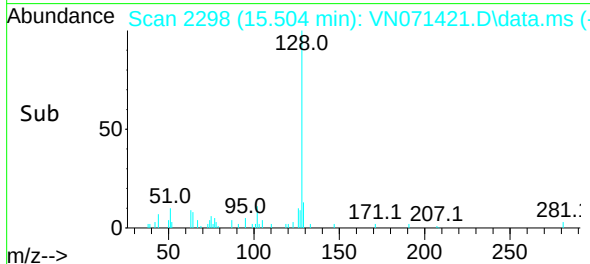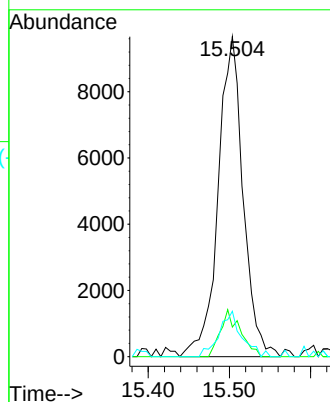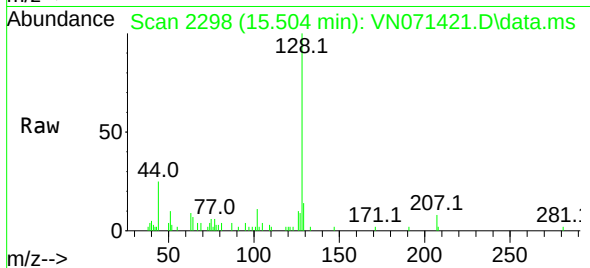

#96

1,2,3-Trichlorobenzene

Concen: 3.525 ug/l

RT: 15.698 min Scan# 2331

Delta R.T. -0.000 min

Lab File: VN071421.D

Acq: 21 Mar 2022 15:39

Tgt Ion:180 Resp: 5203

Ion Ratio Lower Upper

180 100

182 97.0 47.4 142.2

145 27.5 15.0 45.1

