

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032122\
 Data File : VN071432.D
 Acq On : 21 Mar 2022 20:53
 Operator : JC\MD
 Sample : N1966-13
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 G-1-13-26-27

Quant Time: Mar 22 06:23:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 06:52:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	832240	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1419435	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1368095	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	502707	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	540274	47.367	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	94.740%
35) Dibromofluoromethane	8.016	113	410165	45.792	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	91.580%
50) Toluene-d8	10.439	98	1785145	49.499	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.000%
62) 4-Bromofluorobenzene	12.727	95	656396	53.749	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	107.500%
Target Compounds						
					Qvalue	
3) Chloromethane	2.305	50	3987	0.291	ug/l	98
5) Bromomethane	2.857	94	662	Below Cal		81
6) Chloroethane	3.122	64	7736	1.143	ug/l #	52
11) Tert butyl alcohol	5.328	59	525	0.234	ug/l #	71
13) Acrolein	4.034	56	2221	0.936	ug/l	97
16) Acetone	4.287	43	119206	21.479	ug/l	94
18) Methyl Acetate	4.851	43	18184	1.679	ug/l #	90
20) Methylene Chloride	5.087	84	12187	1.574	ug/l	98
25) 2-Butanone	7.340	43	44330	4.959	ug/l	91
29) Tetrahydrofuran	7.692	42	2134	0.345	ug/l #	53
31) Cyclohexane	8.087	56	18050	0.991	ug/l #	1
36) 1,1-Dichloropropene	8.081	75	66136	4.608	ug/l #	48
37) Ethyl Acetate	7.340	43	44330	2.244	ug/l #	68
38) Carbon Tetrachloride	8.081	117	83238	5.996	ug/l #	16
40) Benzene	8.457	78	182039	4.210	ug/l	98
43) Isopropyl Acetate	8.557	43	102633	3.475	ug/l #	83
45) 1,2-Dichloropropane	9.622	63	5560	0.479	ug/l #	44
48) Methyl methacrylate	9.539	41	24168	1.766	ug/l #	8
49) 1,4-Dioxane	9.610	88	647	2.719	ug/l #	1
51) 4-Methyl-2-Pentanone	10.333	43	16731	0.913	ug/l	90
54) cis-1,3-Dichloropropene	10.239	75	112376	6.462	ug/l #	62
57) 1,3-Dichloropropane	11.086	76	59873	3.126	ug/l #	43
59) 2-Hexanone	11.086	43	942656	75.372	ug/l #	49
71) Bromoform	12.727	173	3957	0.484	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	12.733	83	477	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.727	75	338213	26.428	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	338213	72.728	ug/l #	5
95) Naphthalene	15.504	128	8848	5.413	ug/l #	95
96) 1,2,3-Trichlorobenzene	15.704	180	73	2.741	ug/l #	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032122\
Data File : VN071432.D
Acq On : 21 Mar 2022 20:53
Operator : JC\MD
Sample : N1966-13
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
G-1-13-26-27

Quant Time: Mar 22 06:23:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 06:52:46 2022
Response via : Initial Calibration




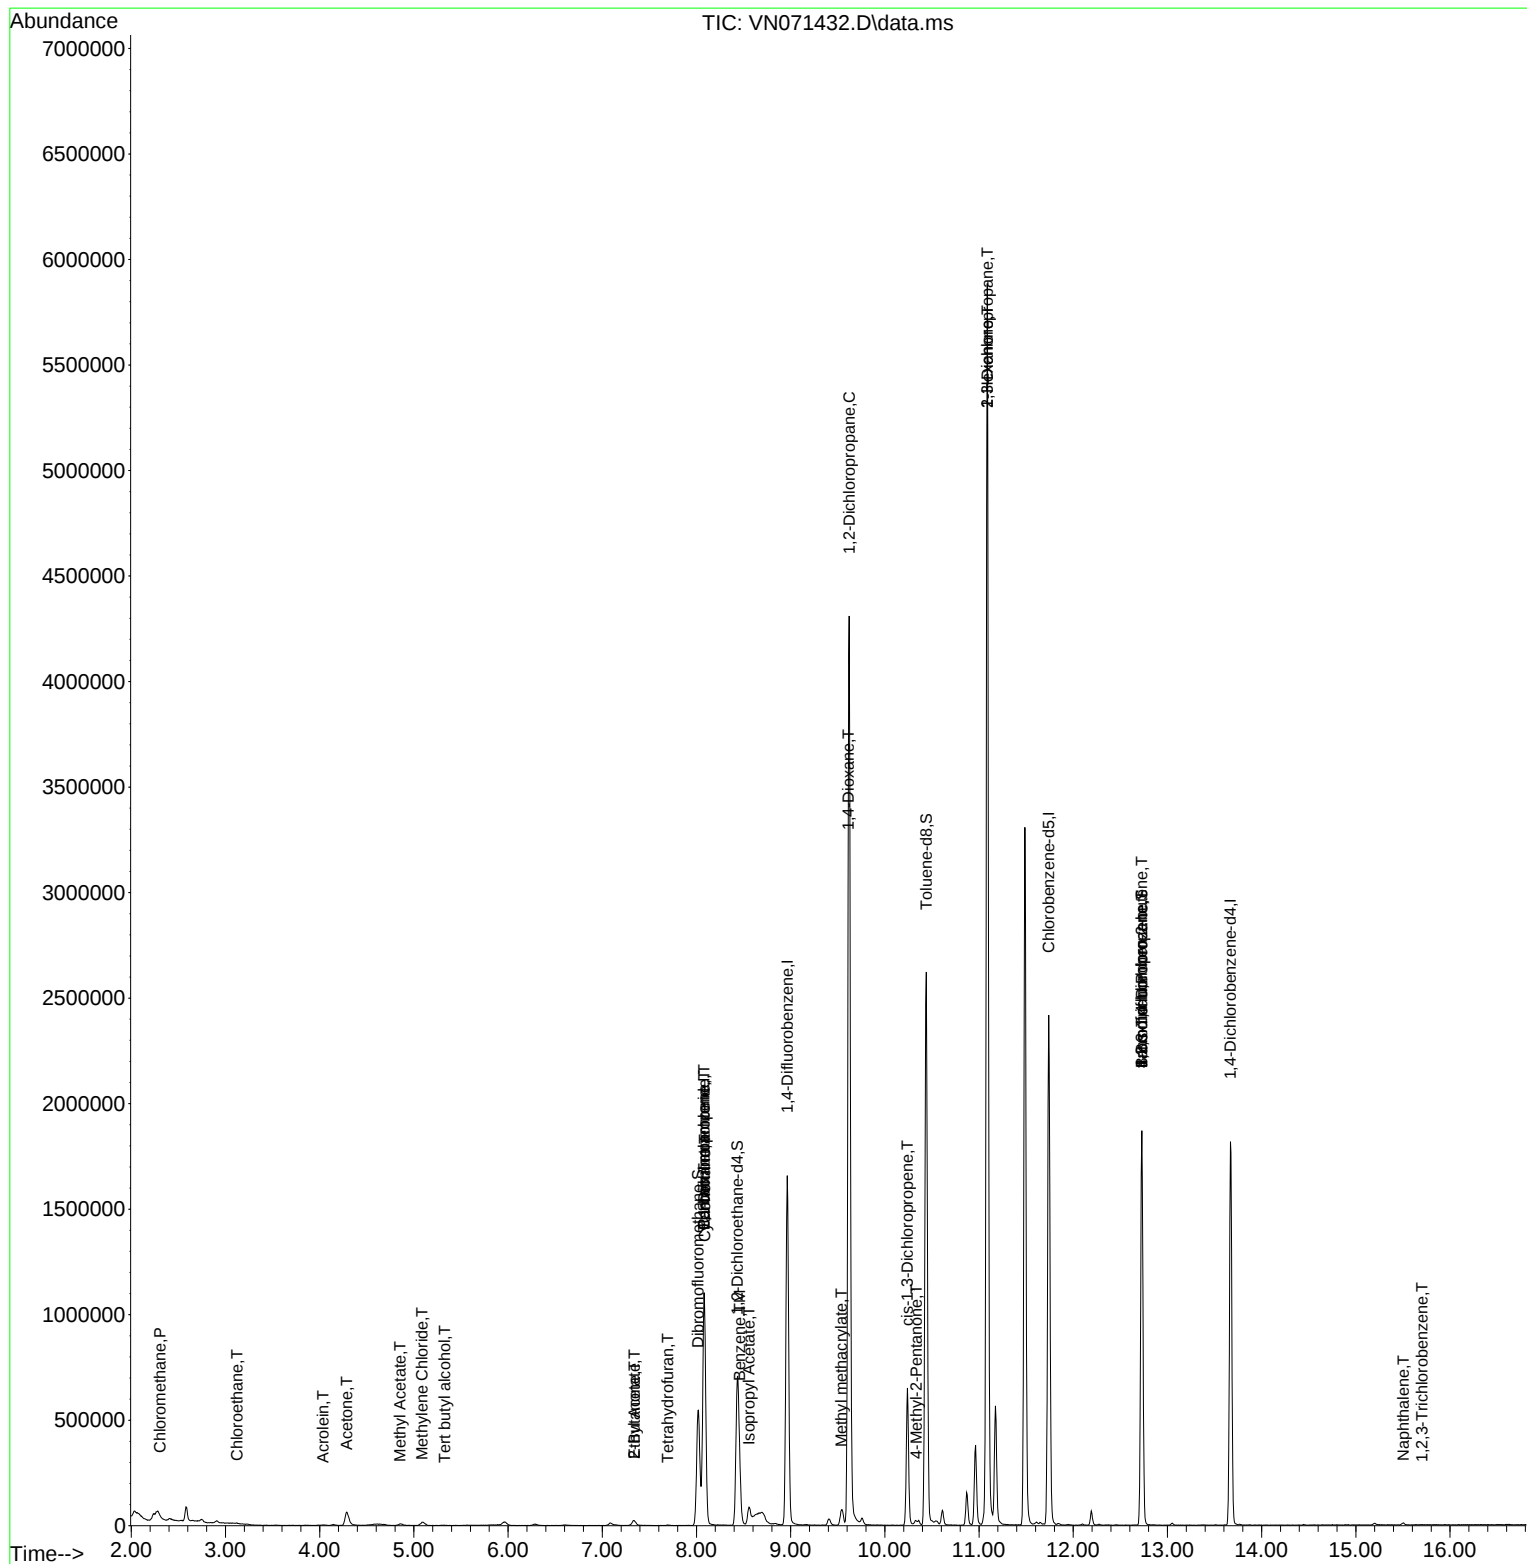




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.005 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53




Instrument :
MSVOA_N
ClientSampleId :
G-1-13-26-27


Tgt Ion:168 Resp: 832240
Ion Ratio Lower Upper
168 100
99 59.8 41.3 61.9

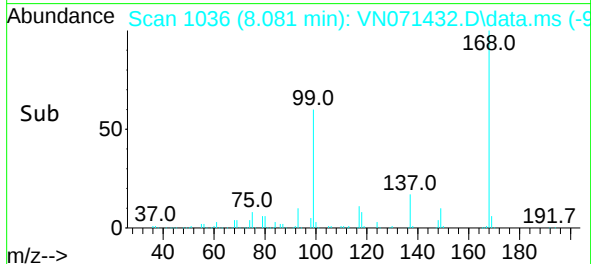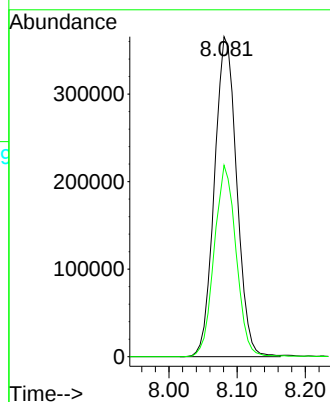

#3
Chloromethane
Concen: 0.291 ug/l
RT: 2.305 min Scan# 54
Delta R.T. 0.006 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53

Tgt Ion: 50 Resp: 3987
Ion Ratio Lower Upper
50 100
52 32.9 25.4 38.0




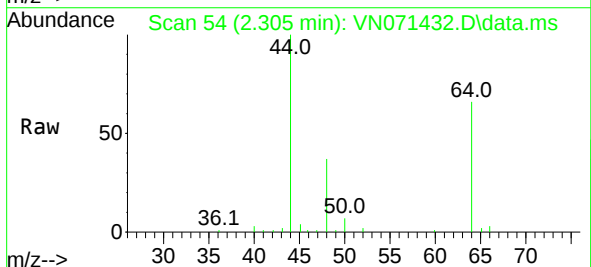


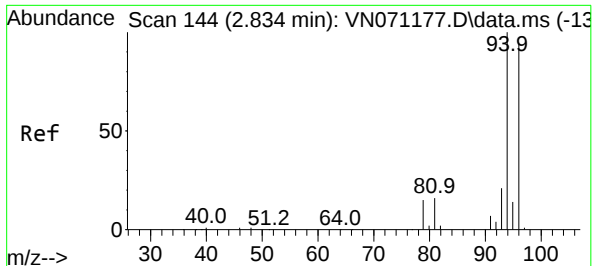

#5
Bromomethane
Concen: Below Cal
RT: 2.857 min Scan# 14
Delta R.T. 0.023 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53




Instrument :
MSVOA_N
ClientSampleId :
G-1-13-26-27


Tgt Ion: 94 Resp: 662
Ion Ratio Lower Upper
94 100
96 74.5 73.8 110.8

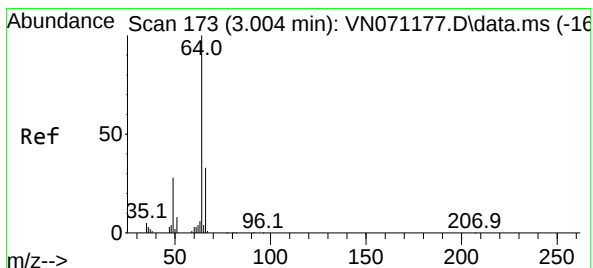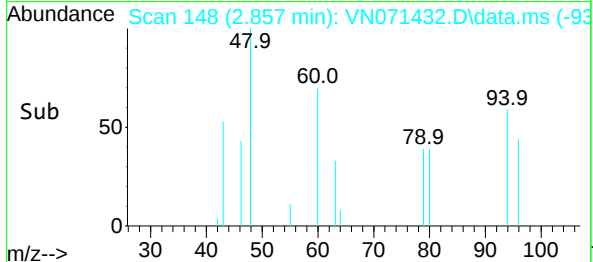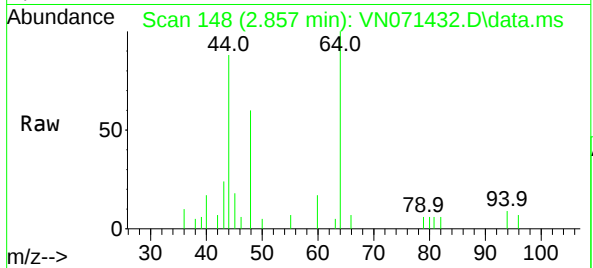

#6
Chloroethane
Concen: 1.143 ug/l
RT: 3.122 min Scan# 193
Delta R.T. 0.118 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53

Tgt Ion: 64 Resp: 7736
Ion Ratio Lower Upper
64 100
66 5.9 26.3 39.5#

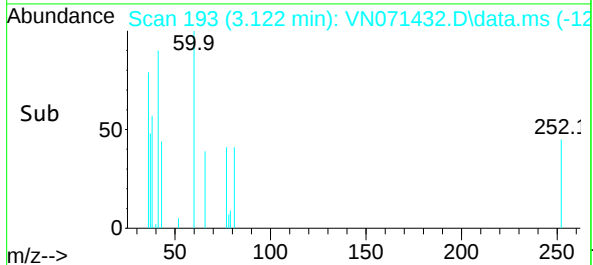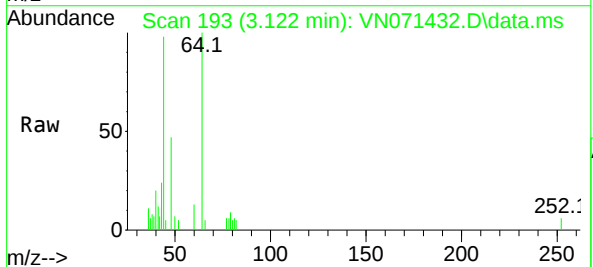



#11

Tert butyl alcohol

Concen: 0.234 ug/l

RT: 5.328 min Scan# 5

Delta R.T. -0.041 min

Lab File: VN071432.D


Acq: 21 Mar 2022 20:53

Instrument :

MSVOA_N

ClientSampleId :

G-1-13-26-27






Tgt Ion: 59 Resp: 525

Ion Ratio Lower Upper

59 100

57 0.0 8.7 13.1#

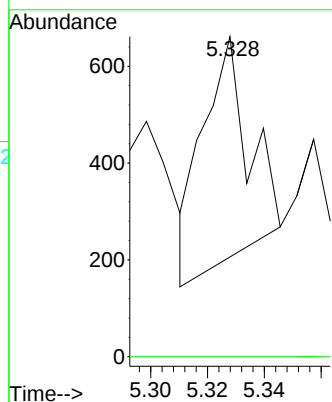

#13

Acrolein

Concen: 0.936 ug/l

RT: 4.034 min Scan# 348

Delta R.T. -0.006 min

Lab File: VN071432.D




Acq: 21 Mar 2022 20:53


Tgt Ion: 56 Resp: 2221

Ion Ratio Lower Upper

56 100

55 68.6 56.6 85.0









#16
Acetone
Concen: 21.479 ug/l
RT: 4.287 min Scan# 391
Delta R.T. 0.000 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53




Instrument :
MSVOA_N
ClientSampleId :
G-1-13-26-27


Tgt Ion: 43 Resp: 119206
Ion Ratio Lower Upper
43 100
58 32.0 23.1 34.7

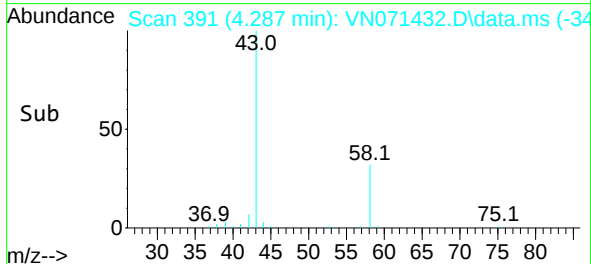

#18
Methyl Acetate
Concen: 1.679 ug/l
RT: 4.851 min Scan# 487
Delta R.T. 0.000 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53


Tgt Ion: 43 Resp: 18184
Ion Ratio Lower Upper
43 100
74 19.2 19.4 29.2#

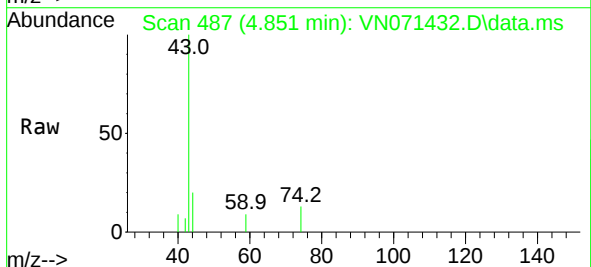






#20
Methylene Chloride
Concen: 1.574 ug/l
RT: 5.087 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53

Instrument :
MSVOA_N
ClientSampleId :
G-1-13-26-27







Tgt Ion:	84	Resp:	12187
Ion	Ratio	Lower	Upper
84	100		
49	116.4	93.5	140.3
51	36.0	29.4	44.2
86	63.2	53.0	79.4



#25
2-Butanone
Concen: 4.959 ug/l
RT: 7.340 min Scan# 910
Delta R.T. 0.006 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53

Tgt Ion:	43	Resp:	44330
Ion	Ratio	Lower	Upper
43	100		
72	22.7	21.7	32.5

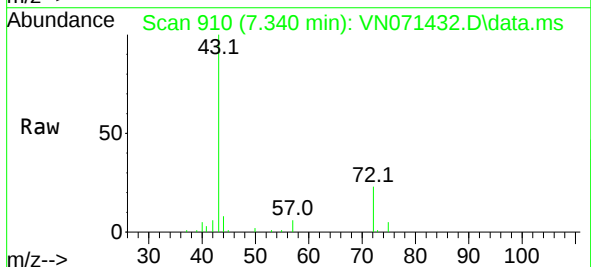



#29

Tetrahydrofuran

Concen: 0.345 ug/l

RT: 7.692 min Scan# 91

Delta R.T. 0.012 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53

Instrument :

MSVOA_N

ClientSampleId :

G-1-13-26-27





Tgt Ion: 42 Resp: 2134

Ion Ratio Lower Upper

42 100

72 10.8 36.3 54.5#

71 16.9 34.7 52.1#

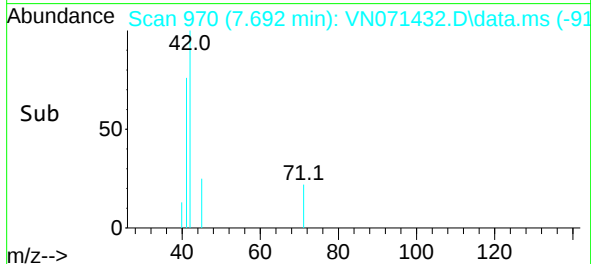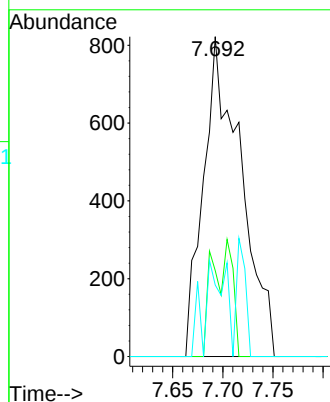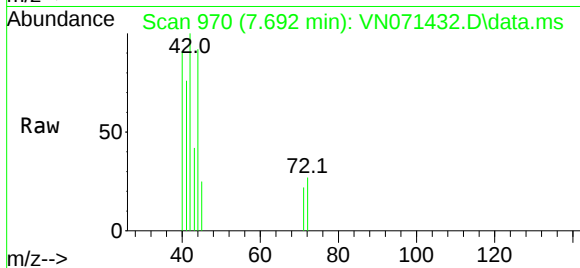

#31

Cyclohexane

Concen: 0.991 ug/l

RT: 8.087 min Scan# 1037

Delta R.T. -0.006 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53




Tgt Ion: 56 Resp: 18050


Ion Ratio Lower Upper

56 100

69 176.7 27.1 40.7#

84 137.9 73.4 110.0#

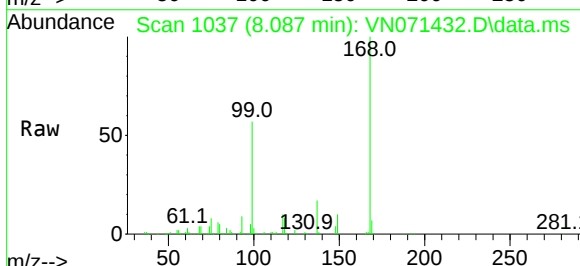

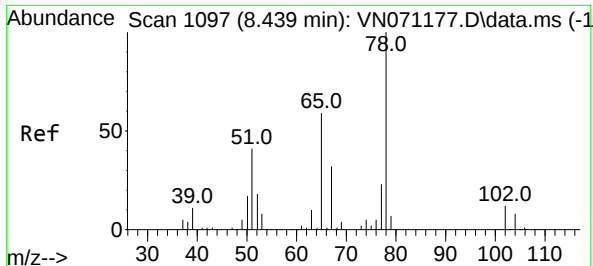

#33

1,2-Dichloroethane-d4

Concen: 47.367 ug/l

RT: 8.434 min Scan# 1109

Delta R.T. -0.006 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53

Instrument :

MSVOA_N

ClientSampleId :





G-1-13-26-27

Tgt Ion: 65 Resp: 540274

Ion Ratio Lower Upper

65 100

67 52.6 0.0 103.0

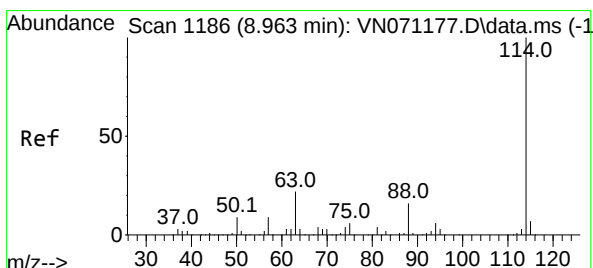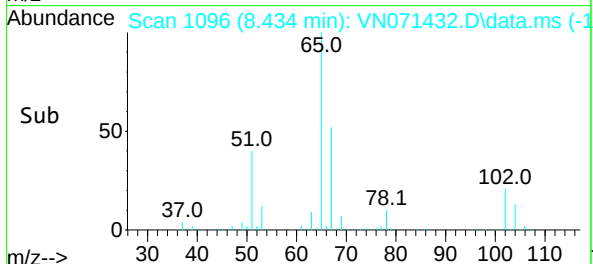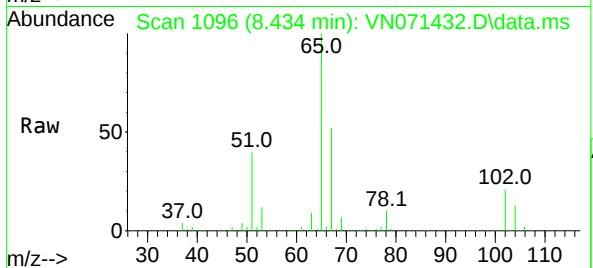

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53




Tgt Ion: 114 Resp: 1419435


Ion Ratio Lower Upper

114 100

63 22.3 0.0 37.8

88 16.6 0.0 27.4

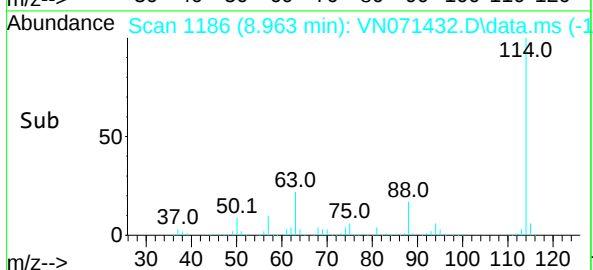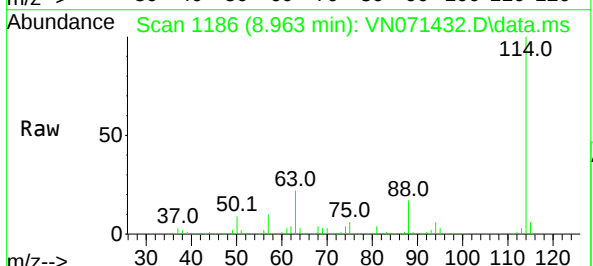

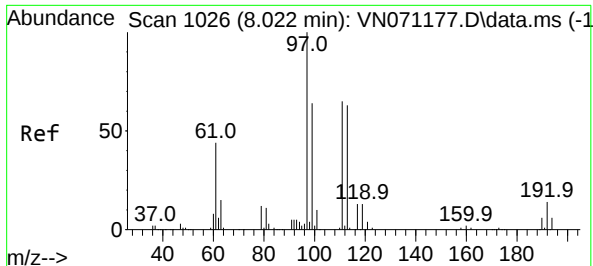

#35

Dibromofluoromethane

Concen: 45.792 ug/l

RT: 8.016 min Scan# 1025

Delta R.T. -0.006 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53

Instrument :

MSVOA_N

ClientSampleId :

G-1-13-26-27





Tgt Ion:113 Resp: 410165

Ion Ratio Lower Upper

113 100

111 102.4 82.2 123.2

192 20.0 16.9 25.3

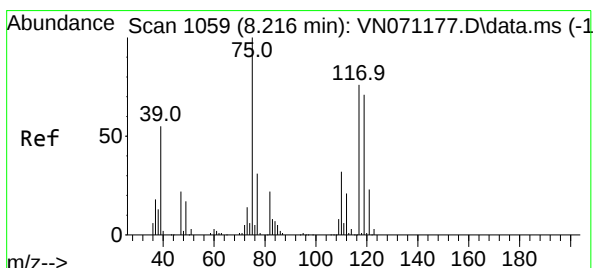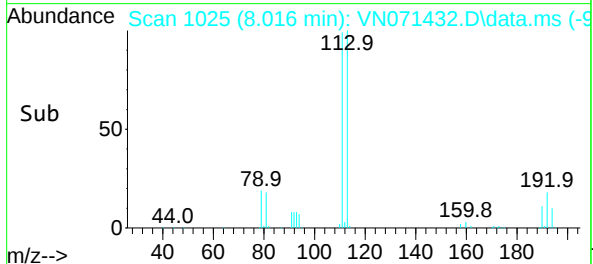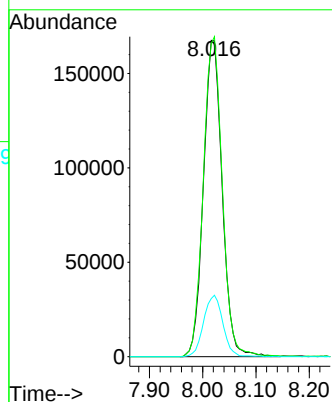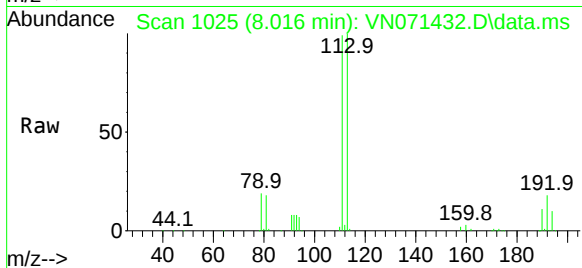

#36

1,1-Dichloropropene

Concen: 4.608 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.135 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53




Tgt Ion: 75 Resp: 66136


Ion Ratio Lower Upper

75 100

110 7.6 18.4 55.2#

77 0.0 24.4 36.6#

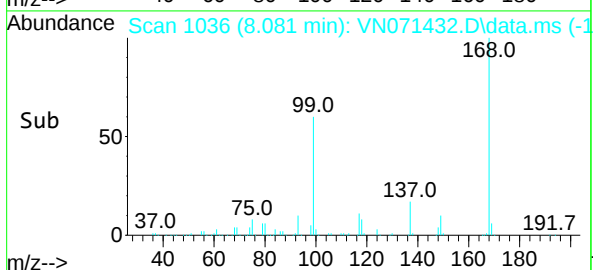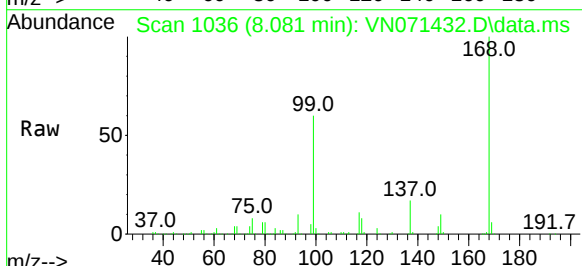



#37

Ethyl Acetate

Concen: 2.244 ug/l

RT: 7.340 min Scan# 91

Delta R.T. -0.070 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53





Instrument :

MSVOA_N

ClientSampleId :

G-1-13-26-27

Tgt Ion: 43	Resp: 44330
Ion Ratio	Lower Upper
43 100	
61 0.0	11.5 17.3#
70 0.0	7.9 11.9#

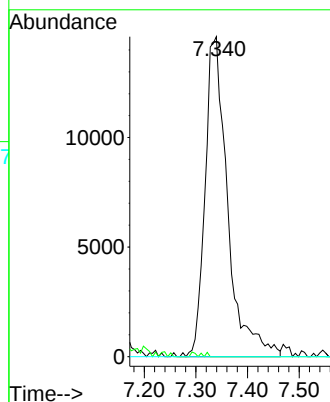

#38

Carbon Tetrachloride

Concen: 5.996 ug/l




RT: 8.081 min Scan# 1036


Delta R.T. -0.123 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53

Tgt Ion: 117	Resp: 83238
Ion Ratio	Lower Upper
117 100	
119 5.1	76.1 114.1#
121 0.0	24.2 36.2#







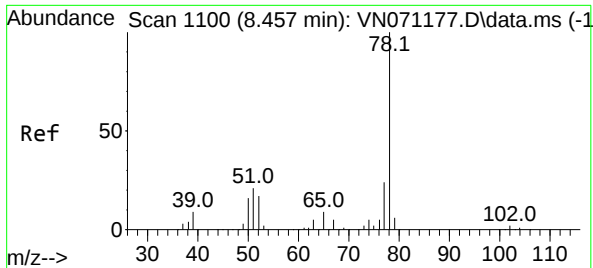

#40
Benzene
Concen: 4.210 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. 0.000 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53




Instrument :
MSVOA_N
ClientSampleId :
G-1-13-26-27


Tgt Ion: 78 Resp: 182039
Ion Ratio Lower Upper
78 100
77 22.2 18.6 27.8

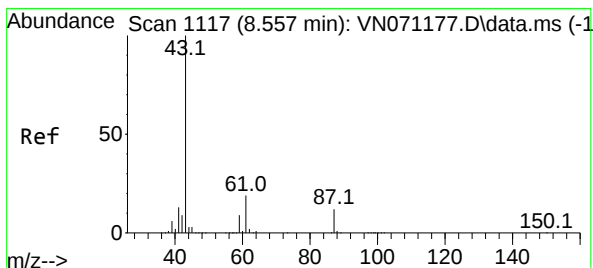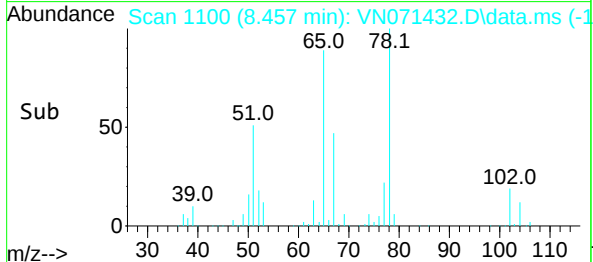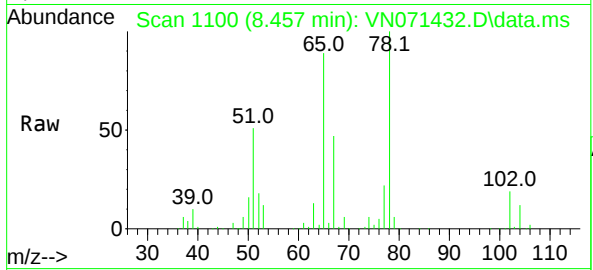

#43
Isopropyl Acetate
Concen: 3.475 ug/l
RT: 8.557 min Scan# 1117
Delta R.T. 0.000 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53

Tgt Ion: 43 Resp: 102633
Ion Ratio Lower Upper
43 100
61 15.7 20.4 30.6#
87 9.3 11.2 16.8#

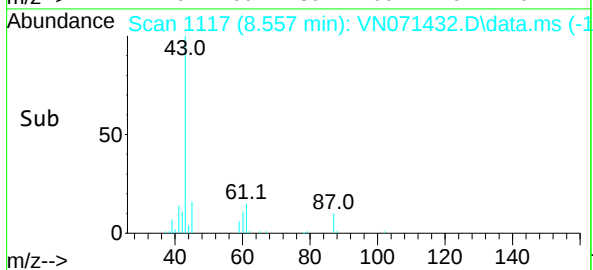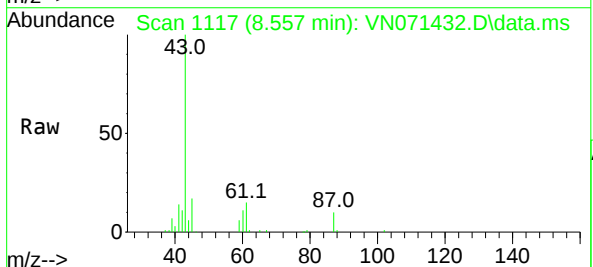

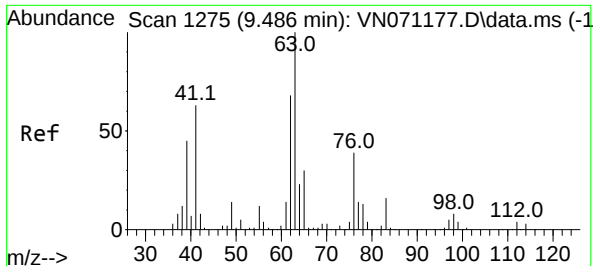

#45

1,2-Dichloropropane

Concen: 0.479 ug/l

RT: 9.622 min Scan# 11

Delta R.T. 0.136 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53

Instrument :

MSVOA_N

ClientSampleId :





G-1-13-26-27

Tgt Ion: 63 Resp: 5560

Ion Ratio Lower Upper

63 100

65 0.0 24.7 37.1#

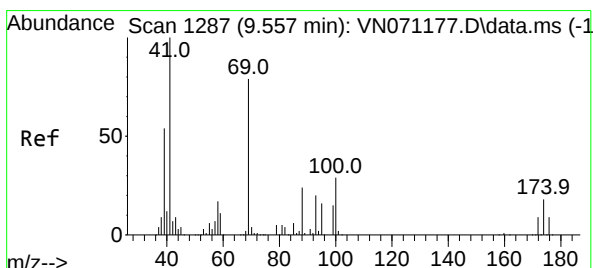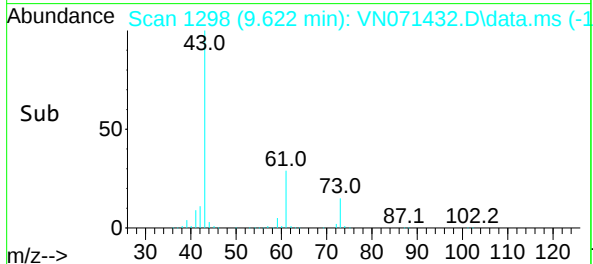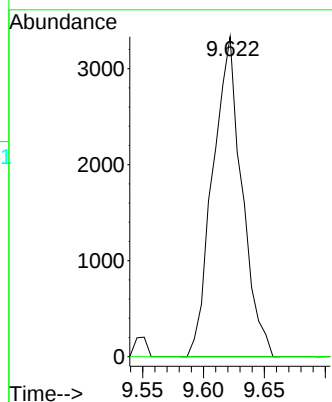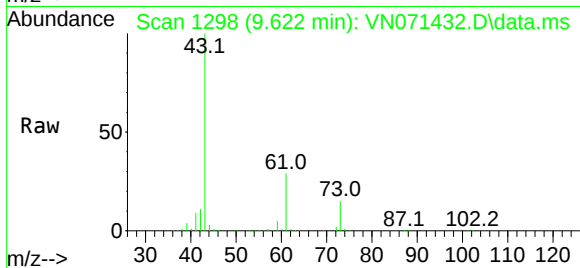

#48

Methyl methacrylate

Concen: 1.766 ug/l

RT: 9.539 min Scan# 1284

Delta R.T. -0.018 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53




Tgt Ion: 41 Resp: 24168


Ion Ratio Lower Upper

41 100

69 0.0 72.4 108.6#

39 0.0 58.4 87.6#

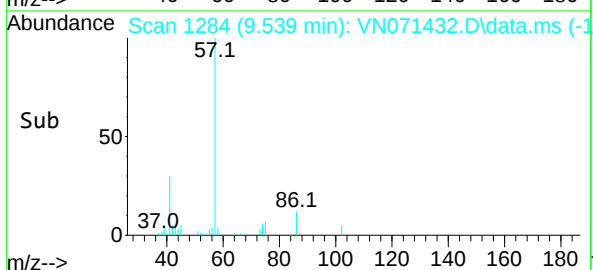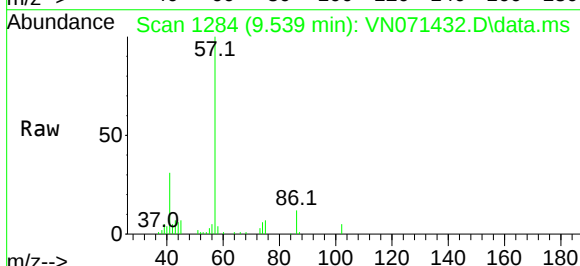



#49

1,4-Dioxane

Concen: 2.719 ug/l

RT: 9.610 min Scan# 11

Delta R.T. 0.047 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53

Instrument :

MSVOA_N

ClientSampleId :

G-1-13-26-27





Tgt Ion: 88 Resp: 647

Ion Ratio Lower Upper

88 100

43 664794.4 23.4 35.2#

58 2759.8 50.6 75.8#

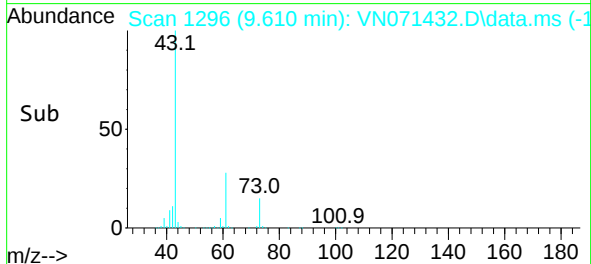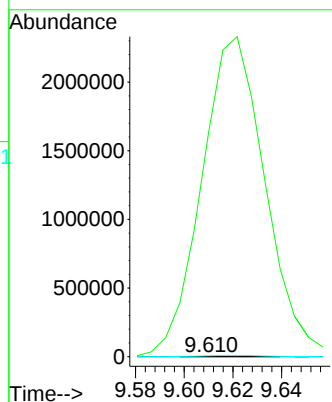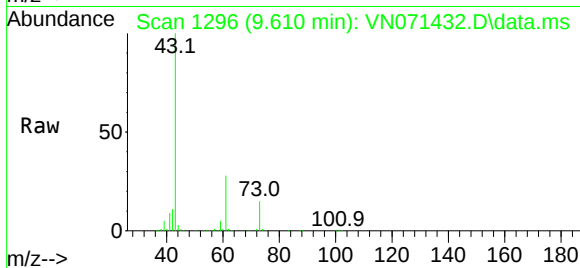

#50

Toluene-d8

Concen: 49.499 ug/l

RT: 10.439 min Scan# 1437

Delta R.T. 0.000 min

Lab File: VN071432.D




Acq: 21 Mar 2022 20:53


Tgt Ion: 98 Resp: 1785145

Ion Ratio Lower Upper

98 100

100 65.1 50.4 75.6

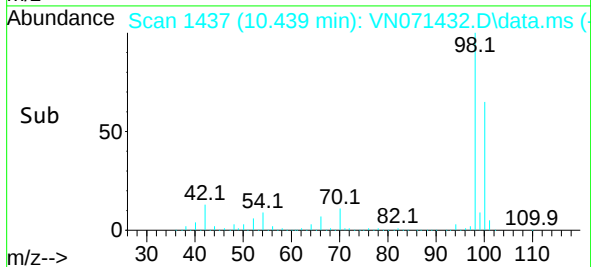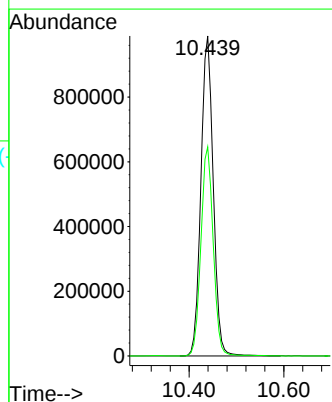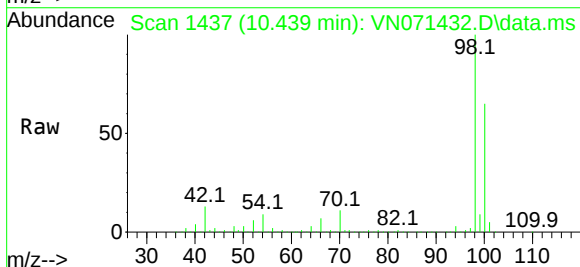



#51

4-Methyl-2-Pentanone

Concen: 0.913 ug/l

RT: 10.333 min Scan# 1418

Delta R.T. 0.006 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53

Instrument :

MSVOA_N

ClientSampleId :





G-1-13-26-27

Tgt Ion: 43 Resp: 16731

Ion Ratio Lower Upper

43 100

58 31.8 30.4 45.6



#54

cis-1,3-Dichloropropene

Concen: 6.462 ug/l

RT: 10.239 min Scan# 1403

Delta R.T. 0.053 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53




Tgt Ion: 75 Resp: 112376


Ion Ratio Lower Upper

75 100

77 0.3 26.4 39.6#

39 34.5 42.5 63.7#

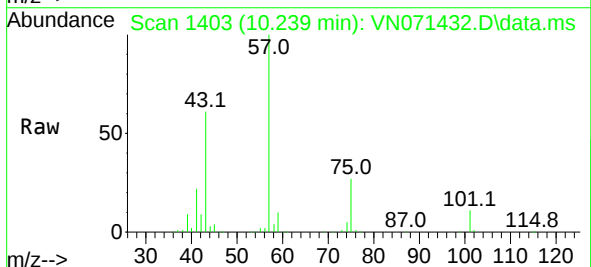



#57

1,3-Dichloropropane

Concen: 3.126 ug/l

RT: 11.086 min Scan# 1547

Delta R.T. 0.047 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53

Instrument :

MSVOA_N

ClientSampleId :





G-1-13-26-27

Tgt Ion: 76 Resp: 59873

Ion Ratio Lower Upper

76 100

78 0.4 25.7 38.5#

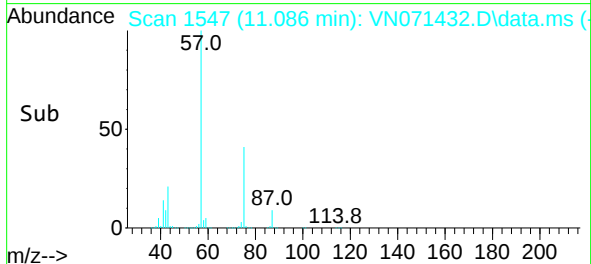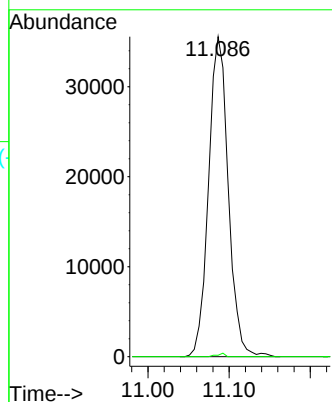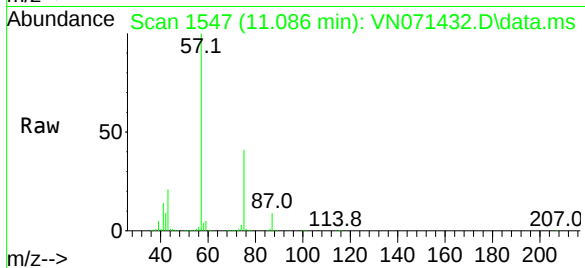

#59

2-Hexanone

Concen: 75.372 ug/l

RT: 11.086 min Scan# 1547

Delta R.T. 0.006 min

Lab File: VN071432.D




Acq: 21 Mar 2022 20:53


Tgt Ion: 43 Resp: 942656

Ion Ratio Lower Upper

43 100

58 17.1 26.9 80.7#




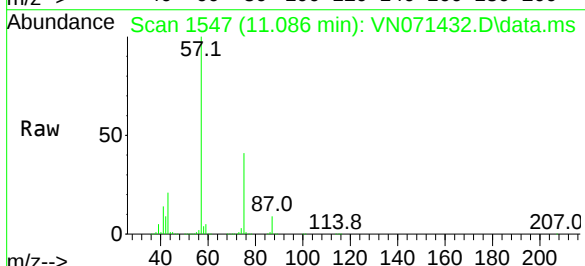


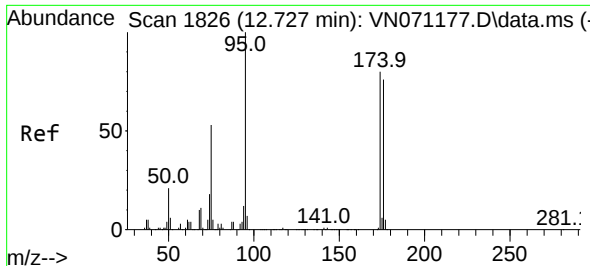

#62
4-Bromofluorobenzene
Concen: 53.749 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53




Instrument :
MSVOA_N
ClientSampleId :
G-1-13-26-27


Tgt Ion: 95 Resp: 656396
Ion Ratio Lower Upper
95 100
174 78.5 0.0 187.2
176 75.2 0.0 181.4

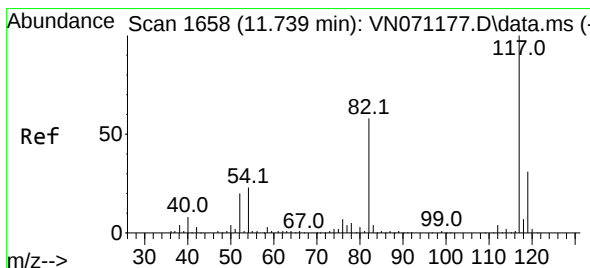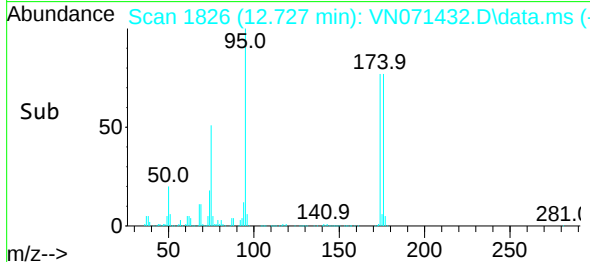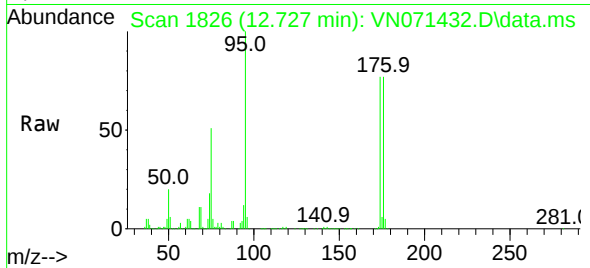

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53

Tgt Ion: 117 Resp: 1368095
Ion Ratio Lower Upper
117 100
82 58.4 42.4 63.6
119 31.8 25.4 38.2

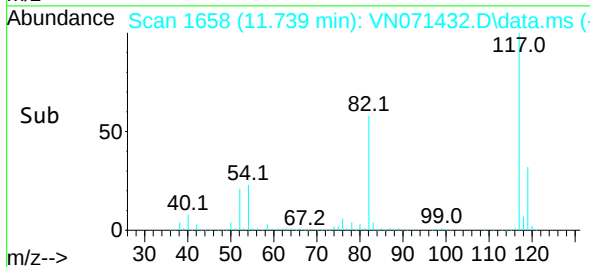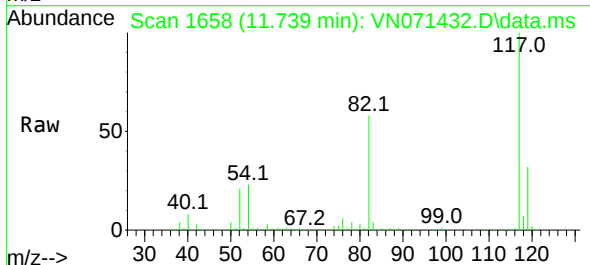



#71

Bromoform

Concen: 0.484 ug/l

RT: 12.727 min Scan# 11

Delta R.T. 0.270 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53

Instrument :

MSVOA_N

ClientSampleId :

G-1-13-26-27





Tgt Ion:173 Resp: 3957

Ion Ratio Lower Upper

173 100

175 718.8 24.2 72.6#

254 0.0 0.0 0.0

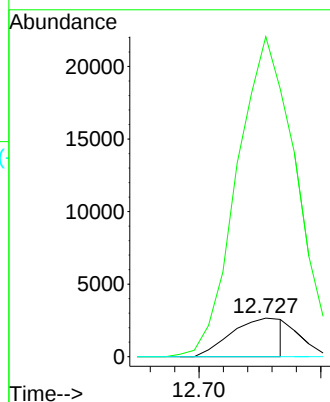

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.669 min Scan# 1986

Delta R.T. 0.001 min

Lab File: VN071432.D

Acq: 21 Mar 2022 20:53




Tgt Ion:152 Resp: 502707


Ion Ratio Lower Upper

152 100

115 58.4 27.5 82.5

150 156.9 0.0 344.4









#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.733 min Scan# 1827
Delta R.T. -0.088 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53




Instrument :
MSVOA_N
ClientSampleId :
G-1-13-26-27


Tgt Ion: 83 Resp: 477
Ion Ratio Lower Upper
83 100
131 177.8 5.5 16.5#
85 0.0 32.4 97.2#

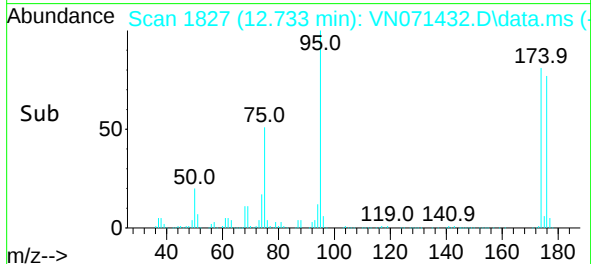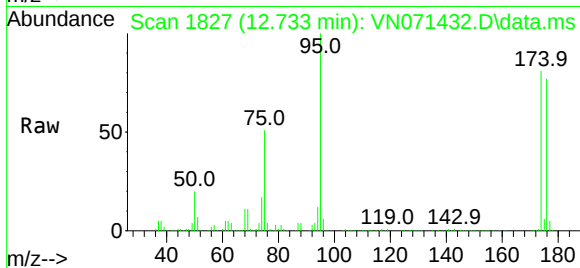

#76
1,2,3-Trichloropropane
Concen: 26.428 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53

Tgt Ion: 75 Resp: 338213
Ion Ratio Lower Upper
75 100
77 1.2 82.6 247.8#


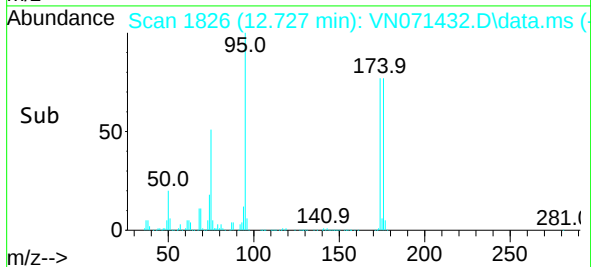

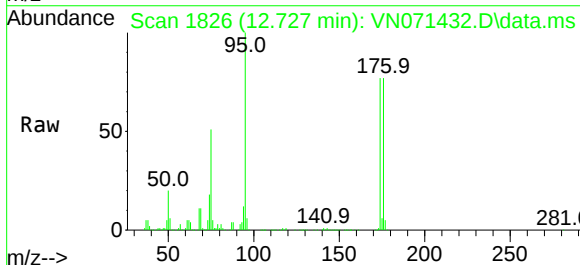


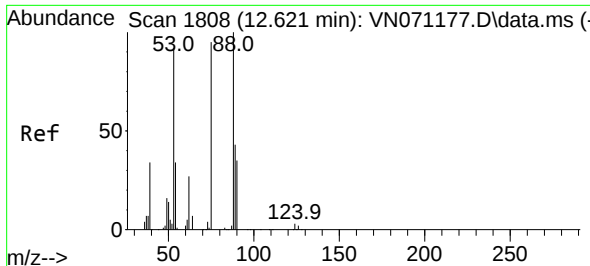

#81
trans-1,4-Dichloro-2-butene
Concen: 72.728 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53




Instrument :
MSVOA_N
ClientSampleId :
G-1-13-26-27


Tgt Ion: 75 Resp: 338213
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#

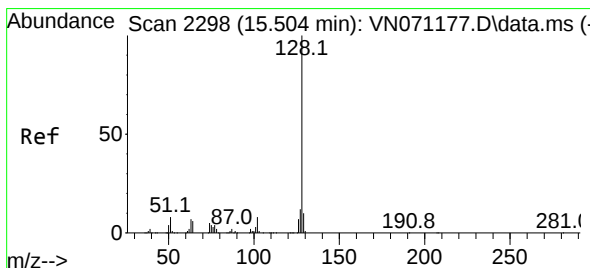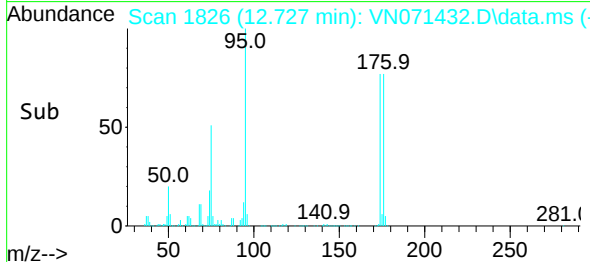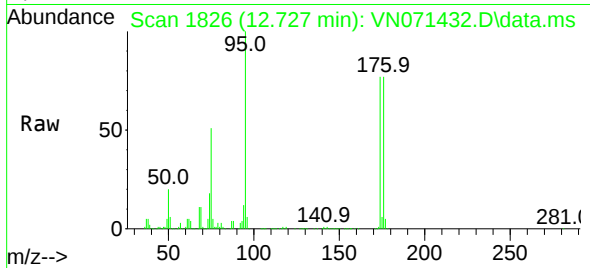

#95
Naphthalene
Concen: 5.413 ug/l
RT: 15.504 min Scan# 2298
Delta R.T. -0.000 min
Lab File: VN071432.D
Acq: 21 Mar 2022 20:53


Tgt Ion: 128 Resp: 8848
Ion Ratio Lower Upper
128 100
127 11.4 10.5 15.7
129 8.5 8.7 13.1#

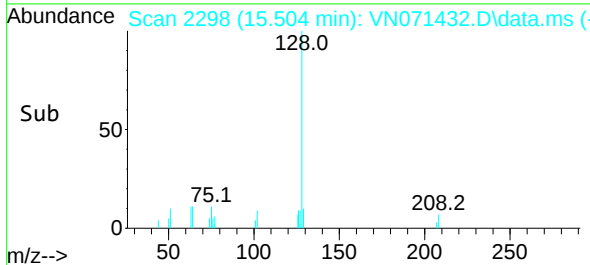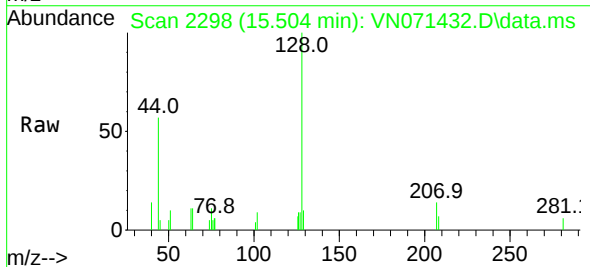



#96
 1,2,3-Trichlorobenzene
 Concen: 2.741 ug/l
 RT: 15.704 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VN071432.D
 Acq: 21 Mar 2022 20:53

Instrument :
 MSVOA_N
 ClientSampleId :
 G-1-13-26-27



Tgt Ion	Ratio	Lower	Upper
180	100		
182	106.8	47.4	142.2
145	0.0	15.0	45.1#

