

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032122\
 Data File : VN071419.D
 Acq On : 21 Mar 2022 14:51
 Operator : JC\MD
 Sample : N1944-05
 Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 CHRT-26215

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Title : SW846 8260

Signal : TIC: VN071419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.222	34	40	58	rVB4	63721	245259	6.82%	1.286%
2	2.775	121	134	135	rBV7	20915	60527	1.68%	0.317%
3	7.116	861	872	885	rBV2	16480	52444	1.46%	0.275%
4	8.010	1014	1024	1029	rBV	407527	967838	26.90%	5.075%
5	8.075	1029	1035	1053	rVB	815330	1848826	51.39%	9.694%
6	8.428	1086	1095	1108	rBV	492856	1131763	31.46%	5.934%
7	8.557	1111	1117	1119	rBV2	24908	45675	1.27%	0.239%
8	8.645	1126	1132	1154	rVB4	45272	196349	5.46%	1.030%
9	8.957	1174	1185	1198	rBV	1222488	2527915	70.27%	13.255%
10	10.433	1428	1436	1444	rBV	1965185	3597332	100.00%	18.863%
11	11.739	1647	1658	1673	rBV	1823401	3206696	89.14%	16.814%
12	12.727	1815	1826	1836	rVB	1343917	2310327	64.22%	12.114%
13	13.045	1875	1880	1887	rBV3	23300	44817	1.25%	0.235%
14	13.669	1979	1986	1994	rBV	1528196	2600945	72.30%	13.638%
15	13.986	2036	2040	2046	rBV5	24225	41974	1.17%	0.220%
16	14.498	2120	2127	2133	rBV7	22902	40542	1.13%	0.213%
17	14.916	2193	2198	2203	rVV5	22052	44705	1.24%	0.234%
18	15.468	2288	2292	2295	rBV5	18129	37214	1.03%	0.195%
19	15.698	2327	2331	2341	rVB10	26367	69922	1.94%	0.367%


Sum of corrected areas: 19071070

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032122\
Data File : VN071419.D
Acq On : 21 Mar 2022 14:51
Operator : JC\MD
Sample : N1944-05
Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

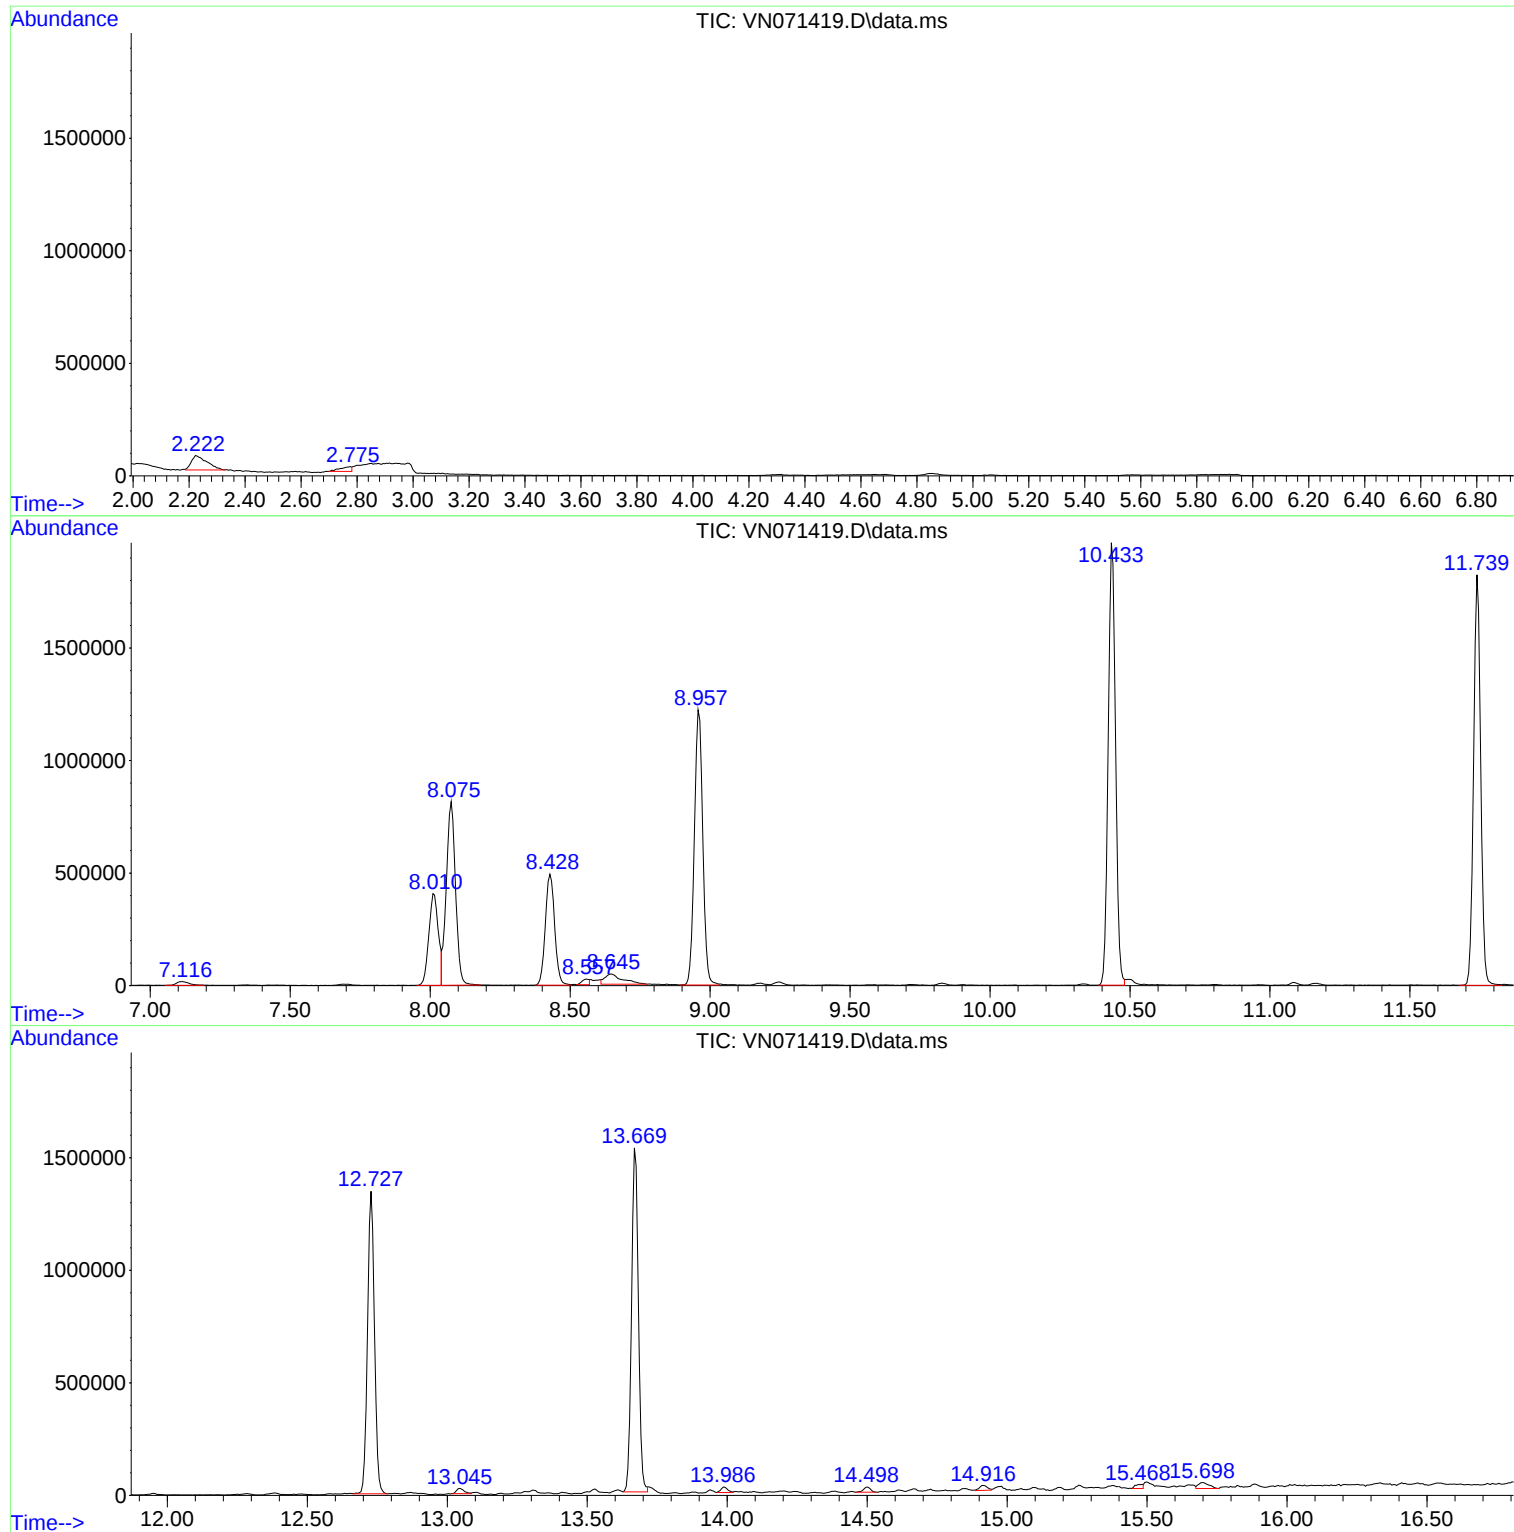

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032122\
Data File : VN071419.D
Acq On : 21 Mar 2022 14:51
Operator : JC\MD
Sample : N1944-05
Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.222 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.222	6.63 ug/l	245259	Pentafluorobenzene	8.075

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	43
2			Sulfur dioxide	64	O2S	007446-09-5	9
3			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	9
4			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
5			Ethanol, 2-fluoro-	64	C2H5FO	000371-62-0	5

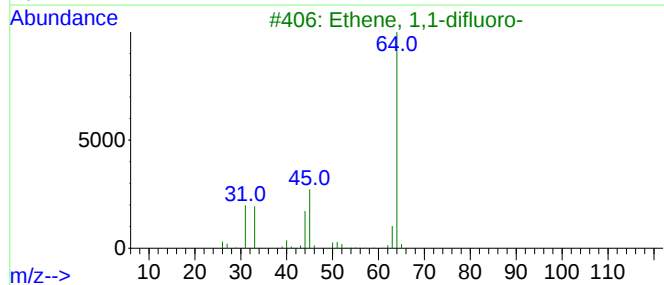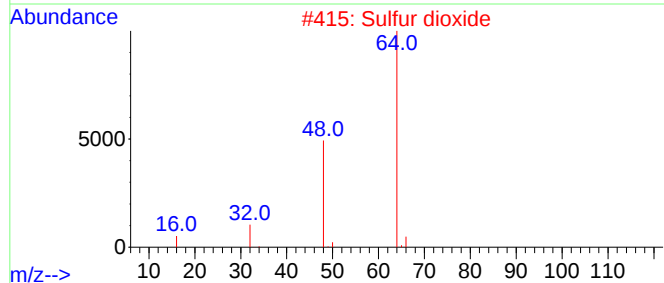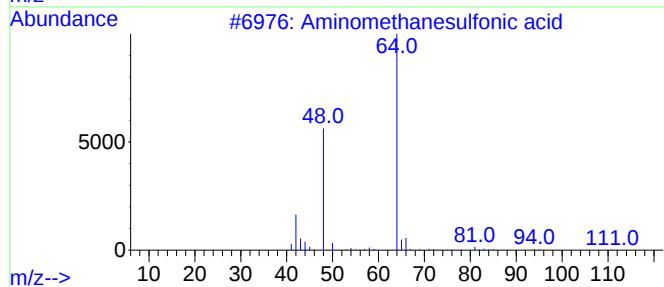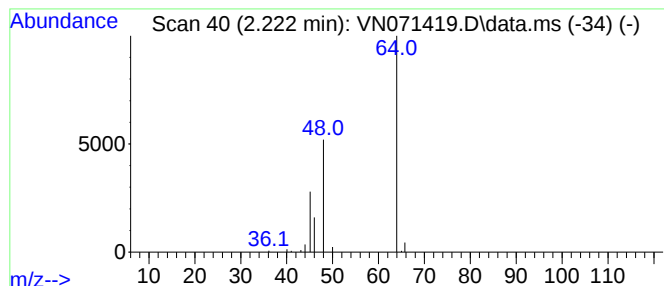

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032122\
Data File : VN071419.D
Acq On : 21 Mar 2022 14:51
Operator : JC\MD
Sample : N1944-05
Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CHRT-26215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.222	2.222	6.6	ug/l	245259	1	8.075	1848830	50.0