


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032122\
 Data File : VN071436.D
 Acq On : 21 Mar 2022 22:54
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030722W.M
 Title : SW846 8260
 Last Update : Tue Mar 08 06:52:46 2022

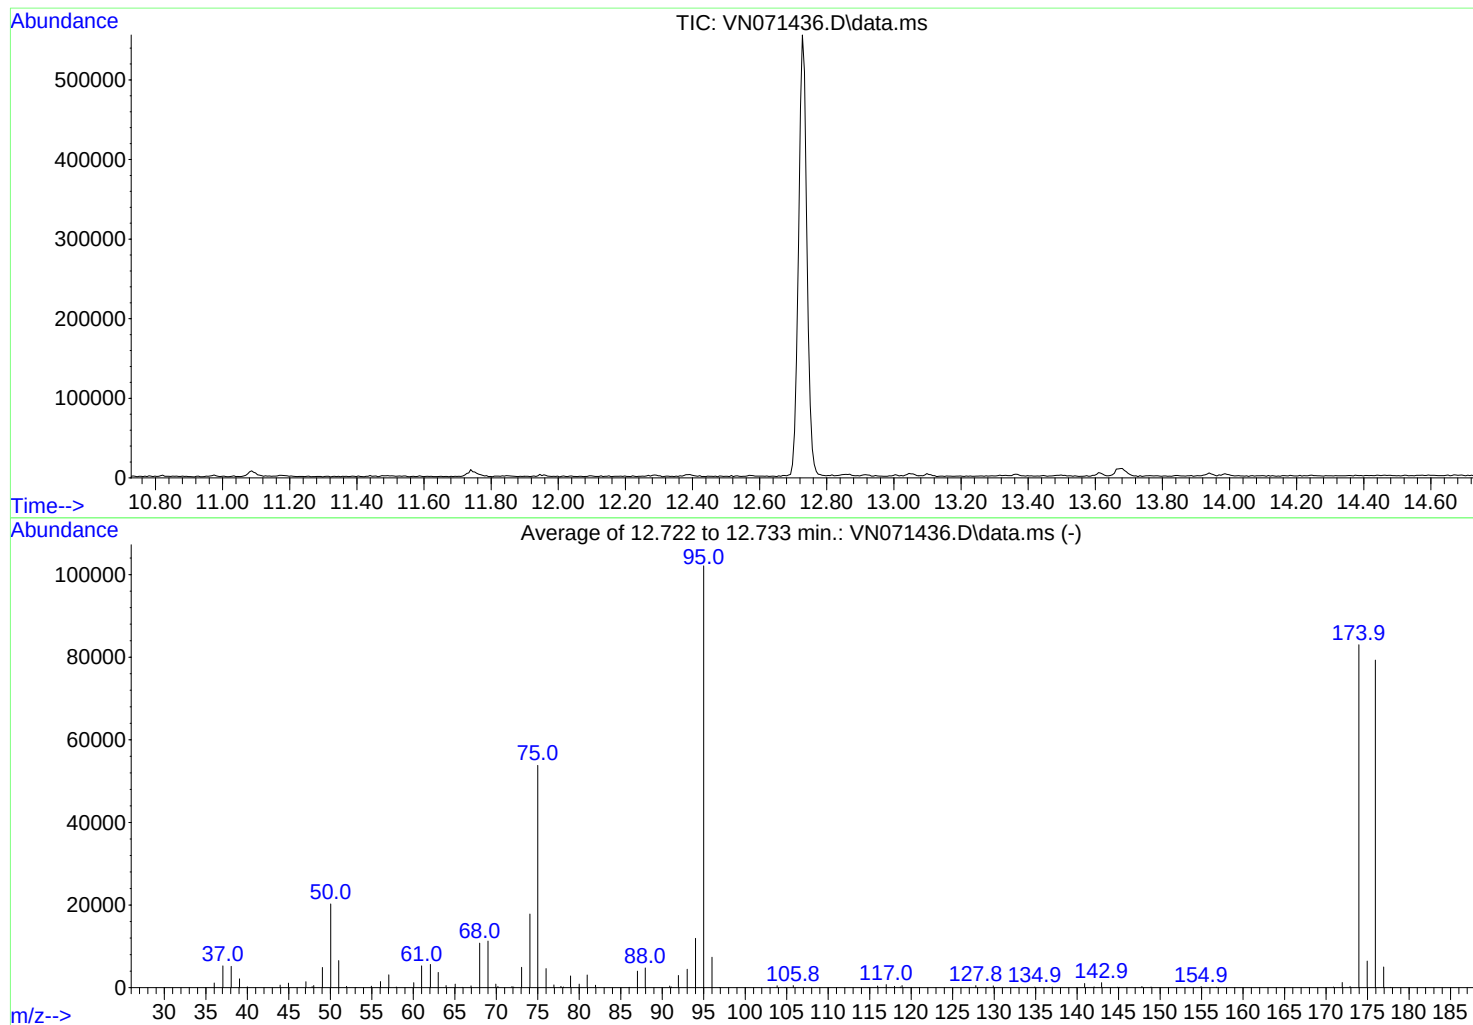

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	20259	PASS
75	95	30	60	52.7	53821	PASS
95	95	100	100	100.0	102128	PASS
96	95	5	9	7.2	7368	PASS
173	174	0.00	2	0.3	271	PASS
174	95	50	100	81.3	83016	PASS
175	174	5	9	7.7	6418	PASS
176	174	95	101	95.5	79296	PASS
177	176	5	9	6.3	5006	PASS