

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN032123\  
Data File : VN077093.D  
Acq On : 21 Mar 2023 16:20  
Operator : JC\MD  
Sample : VIBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
VIBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N031723W.M

Title : SW846 8260

Signal : TIC: VN077093.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.825       | 142           | 151         | 152          | rBV3     | 12584          | 23566         | 1.03%           | 0.204%        |
| 2         | 8.172       | 1051          | 1060        | 1065         | rBV      | 300295         | 734808        | 32.16%          | 6.351%        |
| 3         | 8.231       | 1065          | 1070        | 1083         | rVB      | 536645         | 1192419       | 52.19%          | 10.307%       |
| 4         | 8.584       | 1120          | 1130        | 1142         | rBV      | 359575         | 818723        | 35.84%          | 7.077%        |
| 5         | 8.719       | 1144          | 1153        | 1154         | rBV4     | 14117          | 29399         | 1.29%           | 0.254%        |
| 6         | 9.107       | 1208          | 1219        | 1231         | rBV      | 849529         | 1719964       | 75.29%          | 14.867%       |
| 7         | 10.572      | 1459          | 1468        | 1477         | rBV      | 1248746        | 2284585       | 100.00%         | 19.747%       |
| 8         | 11.872      | 1678          | 1689        | 1702         | rBV      | 1070576        | 1944237       | 85.10%          | 16.805%       |
| 9         | 12.854      | 1848          | 1856        | 1868         | rBV      | 797312         | 1312069       | 57.43%          | 11.341%       |
| 10        | 13.795      | 2006          | 2016        | 2027         | rBV      | 907195         | 1509433       | 66.07%          | 13.047%       |




Sum of corrected areas: 11569203

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN032123\  
Data File : VN077093.D  
Acq On : 21 Mar 2023 16:20  
Operator : JC\MD  
Sample : VIBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N031723W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

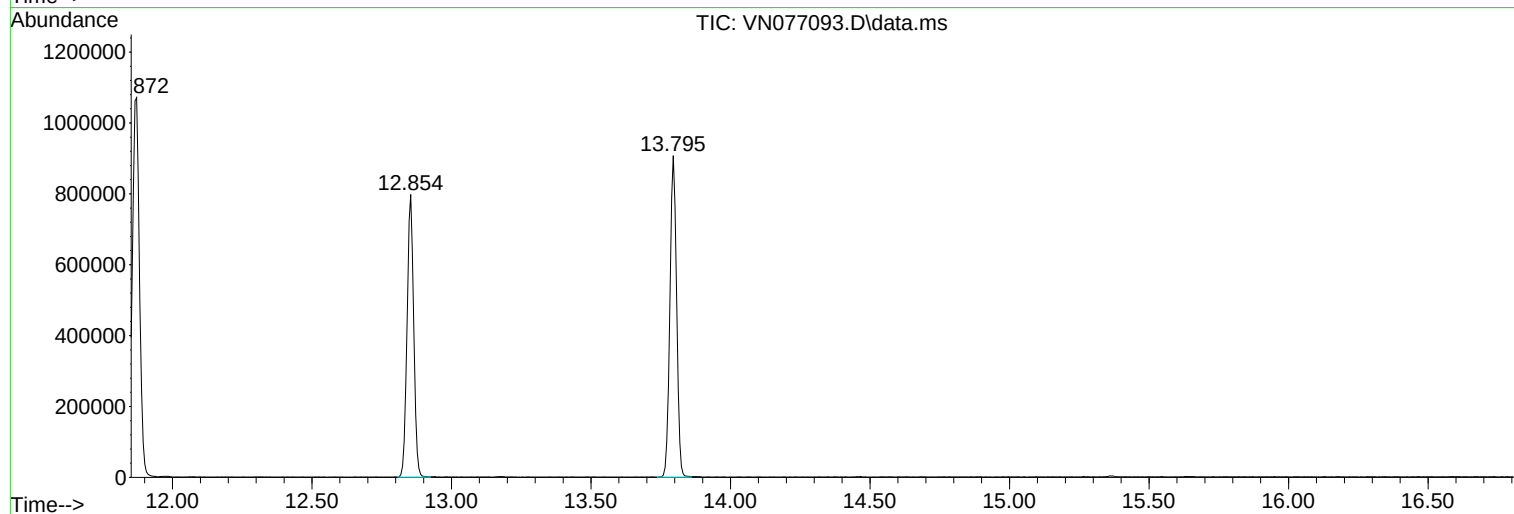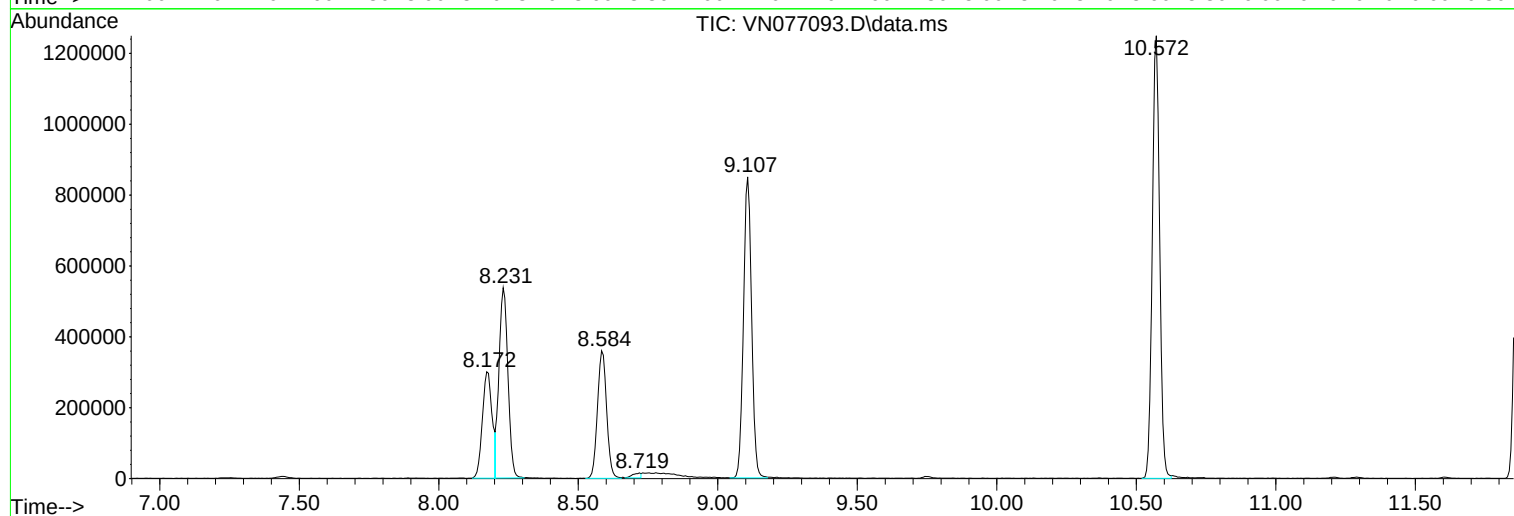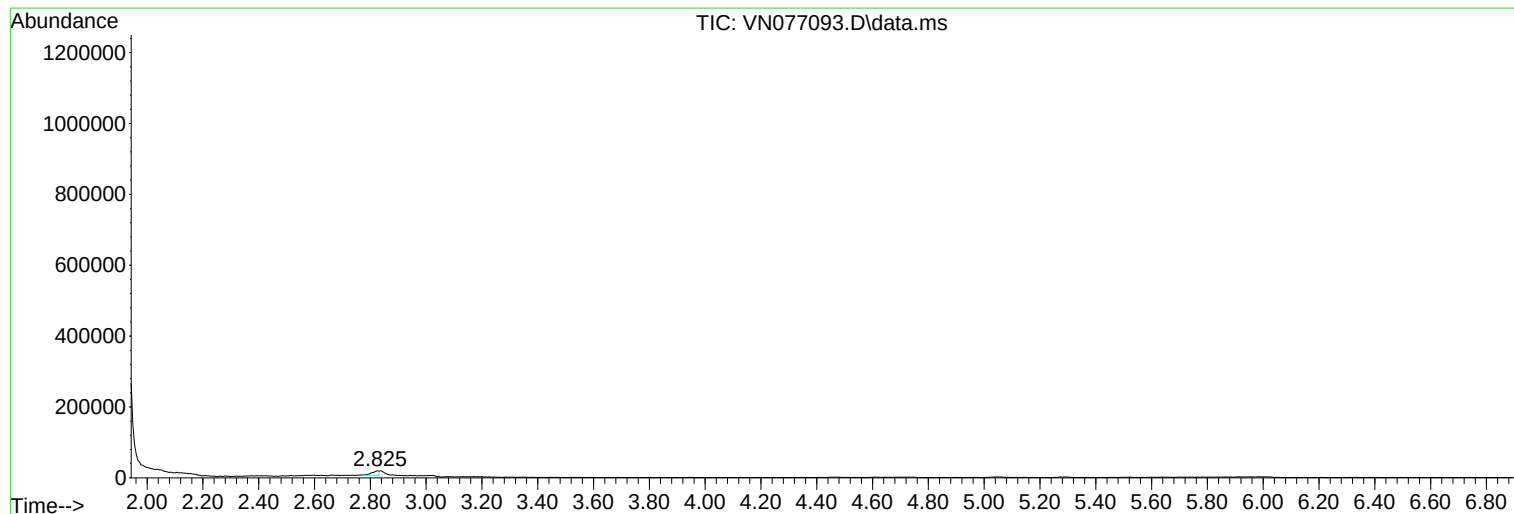

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN032123\  
Data File : VN077093.D  
Acq On : 21 Mar 2023 16:20  
Operator : JC\MD  
Sample : VIBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N031723W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN032123\  
Data File : VN077093.D  
Acq On : 21 Mar 2023 16:20  
Operator : JC\MD  
Sample : VIBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N031723W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|