


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032123\
Data File : VN077081.D
Acq On : 21 Mar 2023 09:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031723W.M
Title : SW846 8260
Last Update : Mon Mar 20 08:50:30 2023

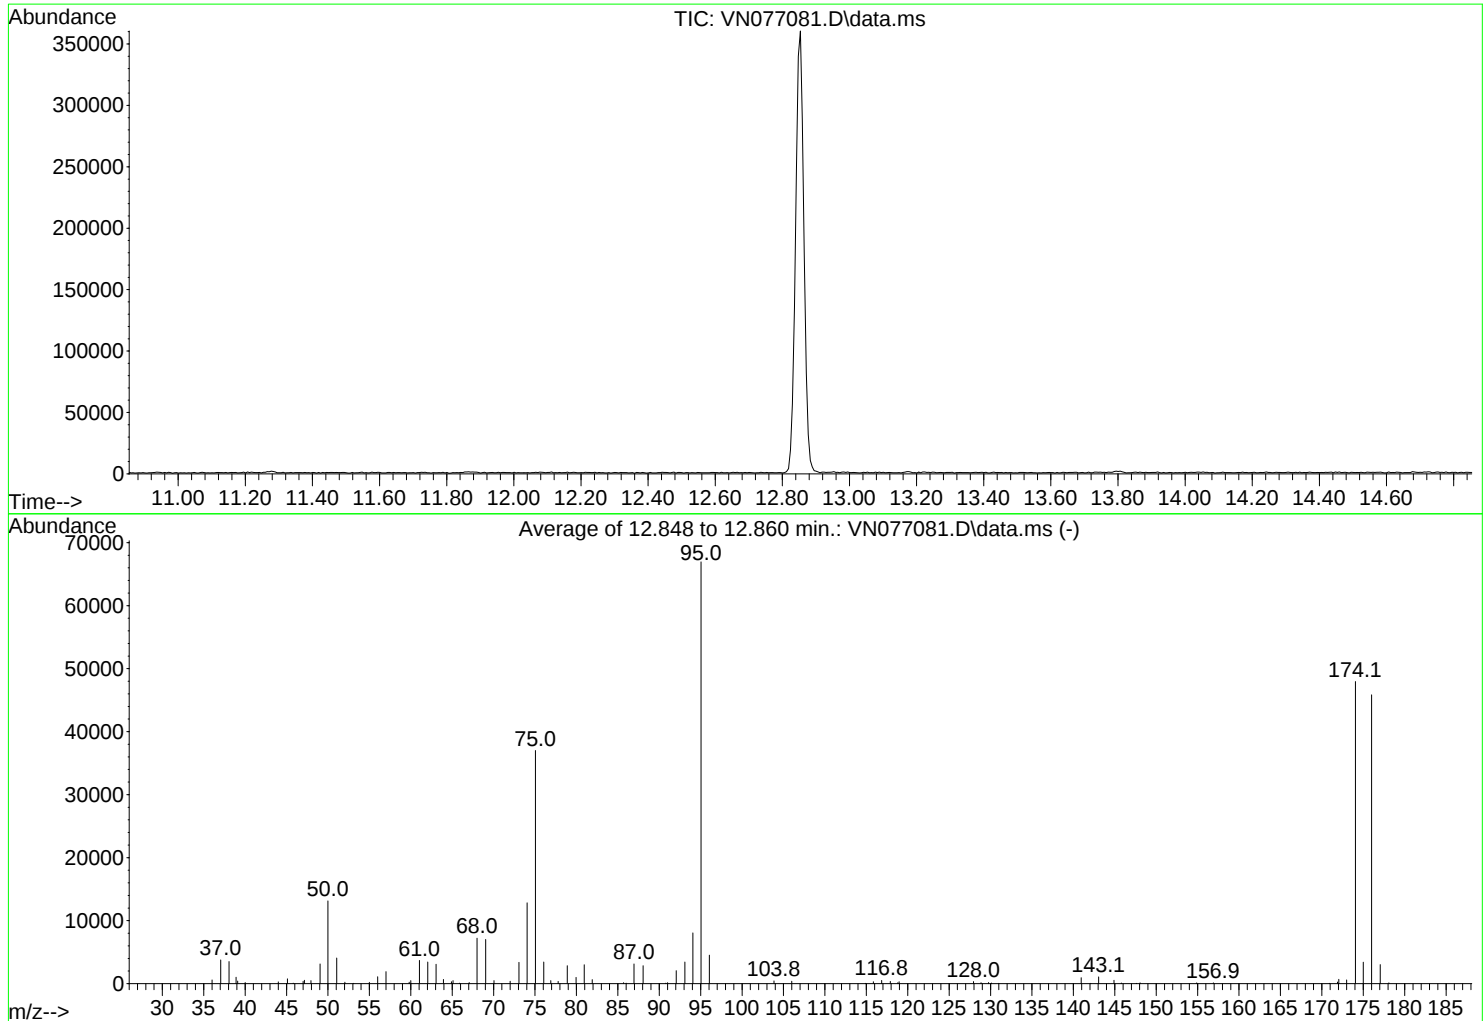

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	13123	PASS
75	95	30	60	55.3	37019	PASS
95	95	100	100	100.0	66952	PASS
96	95	5	9	6.8	4532	PASS
173	174	0.00	2	1.2	585	PASS
174	95	50	100	71.6	47957	PASS
175	174	5	9	7.1	3415	PASS
176	174	95	101	95.6	45845	PASS
177	176	5	9	6.6	3033	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	588	47.95	493	61.05	3682	72.00	381
37.05	3752	49.05	3133	62.05	3426	73.05	338
38.05	3511	50.00	13123	63.05	3082	74.05	1281
38.90	1020	51.05	4066	63.95	673	75.05	3701
39.10	419	52.05	225	64.90	314	76.05	3420
40.00	188	53.10	65	65.10	488	76.90	483
44.00	282	55.00	213	65.90	85	77.80	354
45.10	761	56.00	1091	67.05	184	78.90	2837
45.80	69	57.00	1917	68.00	7209	79.95	1000
47.00	353	59.80	234	69.05	7017	80.95	3007
47.15	530	60.00	491	70.05	480	81.90	629

Average of 12.848 to 12.860 min.: VN077081.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.70	148	103.85	420	130.10	108	170.90	58
86.00	71	106.00	376	131.00	52	171.90	262
86.95	3138	114.90	51	140.95	950	172.05	697
88.05	2842	115.85	304	142.10	52	173.00	585
90.80	85	116.85	511	143.05	1066	174.05	47957
91.00	153	117.90	366	144.90	526	175.00	3415
92.05	2068	118.80	158	145.80	95	176.00	45845
93.10	3440	118.95	319	147.60	62	177.05	3033
94.05	8059	127.95	325	148.05	124	178.10	135
95.05	66952	128.85	156	154.90	133		
96.05	4532	129.75	182	156.90	137		

Instrument :

MSVOA_N

ClientSampleId :

BFB