

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032124\
 Data File : VN081524.D
 Acq On : 21 Mar 2024 17:00
 Operator : JC\MD
 Sample : P1798-07 20X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 S-7

Quant Time: Mar 22 05:09:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 19 06:00:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	495186	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	870935	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	752181	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	325693	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.576	65	313119	49.584	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	99.160%		
35) Dibromofluoromethane	8.165	113	260240	47.347	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.700%		
50) Toluene-d8	10.565	98	1009812	50.823	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	101.640%		
62) 4-Bromofluorobenzene	12.847	95	331153	47.300	ug/l	0.00
Spiked Amount 50.000	Range 64 - 133		Recovery =	94.600%		
Target Compounds						Qvalue
5) Bromomethane	2.965	94	1398	0.265	ug/l #	69
11) Tert butyl alcohol	5.518	59	275	0.250	ug/l #	72
13) Acrolein	4.165	56	292	0.296	ug/l #	15
16) Acetone	4.441	43	9020	4.420	ug/l #	79
18) Methyl Acetate	5.024	43	1753	0.279	ug/l #	81
20) Methylene Chloride	5.277	84	2656	0.397	ug/l #	57
25) 2-Butanone	7.482	43	4667	1.333	ug/l #	82
31) Cyclohexane	8.224	56	13823	1.345	ug/l #	1
36) 1,1-Dichloropropene	8.224	75	41196	4.454	ug/l #	52
38) Carbon Tetrachloride	8.229	117	51950	5.127	ug/l #	19
39) Methylcyclohexane	9.606	83	2633	0.255	ug/l #	64
40) Benzene	8.606	78	2206479	81.592	ug/l	98
42) 1,2-Dichloroethane	8.612	62	18890	1.985	ug/l #	75
43) Isopropyl Acetate	8.682	43	17101	1.302	ug/l #	77
51) 4-Methyl-2-Pentanone	10.441	43	1758	0.219	ug/l #	38
52) Toluene	10.629	92	722097	42.011	ug/l	100
53) t-1,3-Dichloropropene	10.635	75	8936	0.850	ug/l #	1
55) 1,1,2-Trichloroethane	10.876	97	5739	0.830	ug/l #	16
56) Ethyl methacrylate	10.882	69	293	0.602	ug/l #	20
59) 2-Hexanone	11.176	43	8763	1.479	ug/l #	44
67) Ethyl Benzene	11.964	91	67409	2.182	ug/l	97
68) m/p-Xylenes	12.065	106	132495	11.442	ug/l	98
69) o-Xylene	12.394	106	82448	7.253	ug/l	97
70) Styrene	12.412	104	13570	0.740	ug/l #	13
71) Bromoform	12.847	173	2463	0.497	ug/l #	1
76) 1,2,3-Trichloropropane	12.847	75	171875	22.061	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.170	105	25409	1.108	ug/l	88
81) trans-1,4-Dichloro-2-b...	12.847	75	171875	59.617	ug/l #	14
84) 1,2,4-Trimethylbenzene	13.482	105	72988	3.167	ug/l	99
85) sec-Butylbenzene	13.482	105	72988	2.582	ug/l #	60
95) Naphthalene	15.641	128	938149	41.288	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032124\
Data File : VN081524.D
Acq On : 21 Mar 2024 17:00
Operator : JC\MD
Sample : P1798-07 20X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
S-7

Quant Time: Mar 22 05:09:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 19 06:00:00 2024
Response via : Initial Calibration

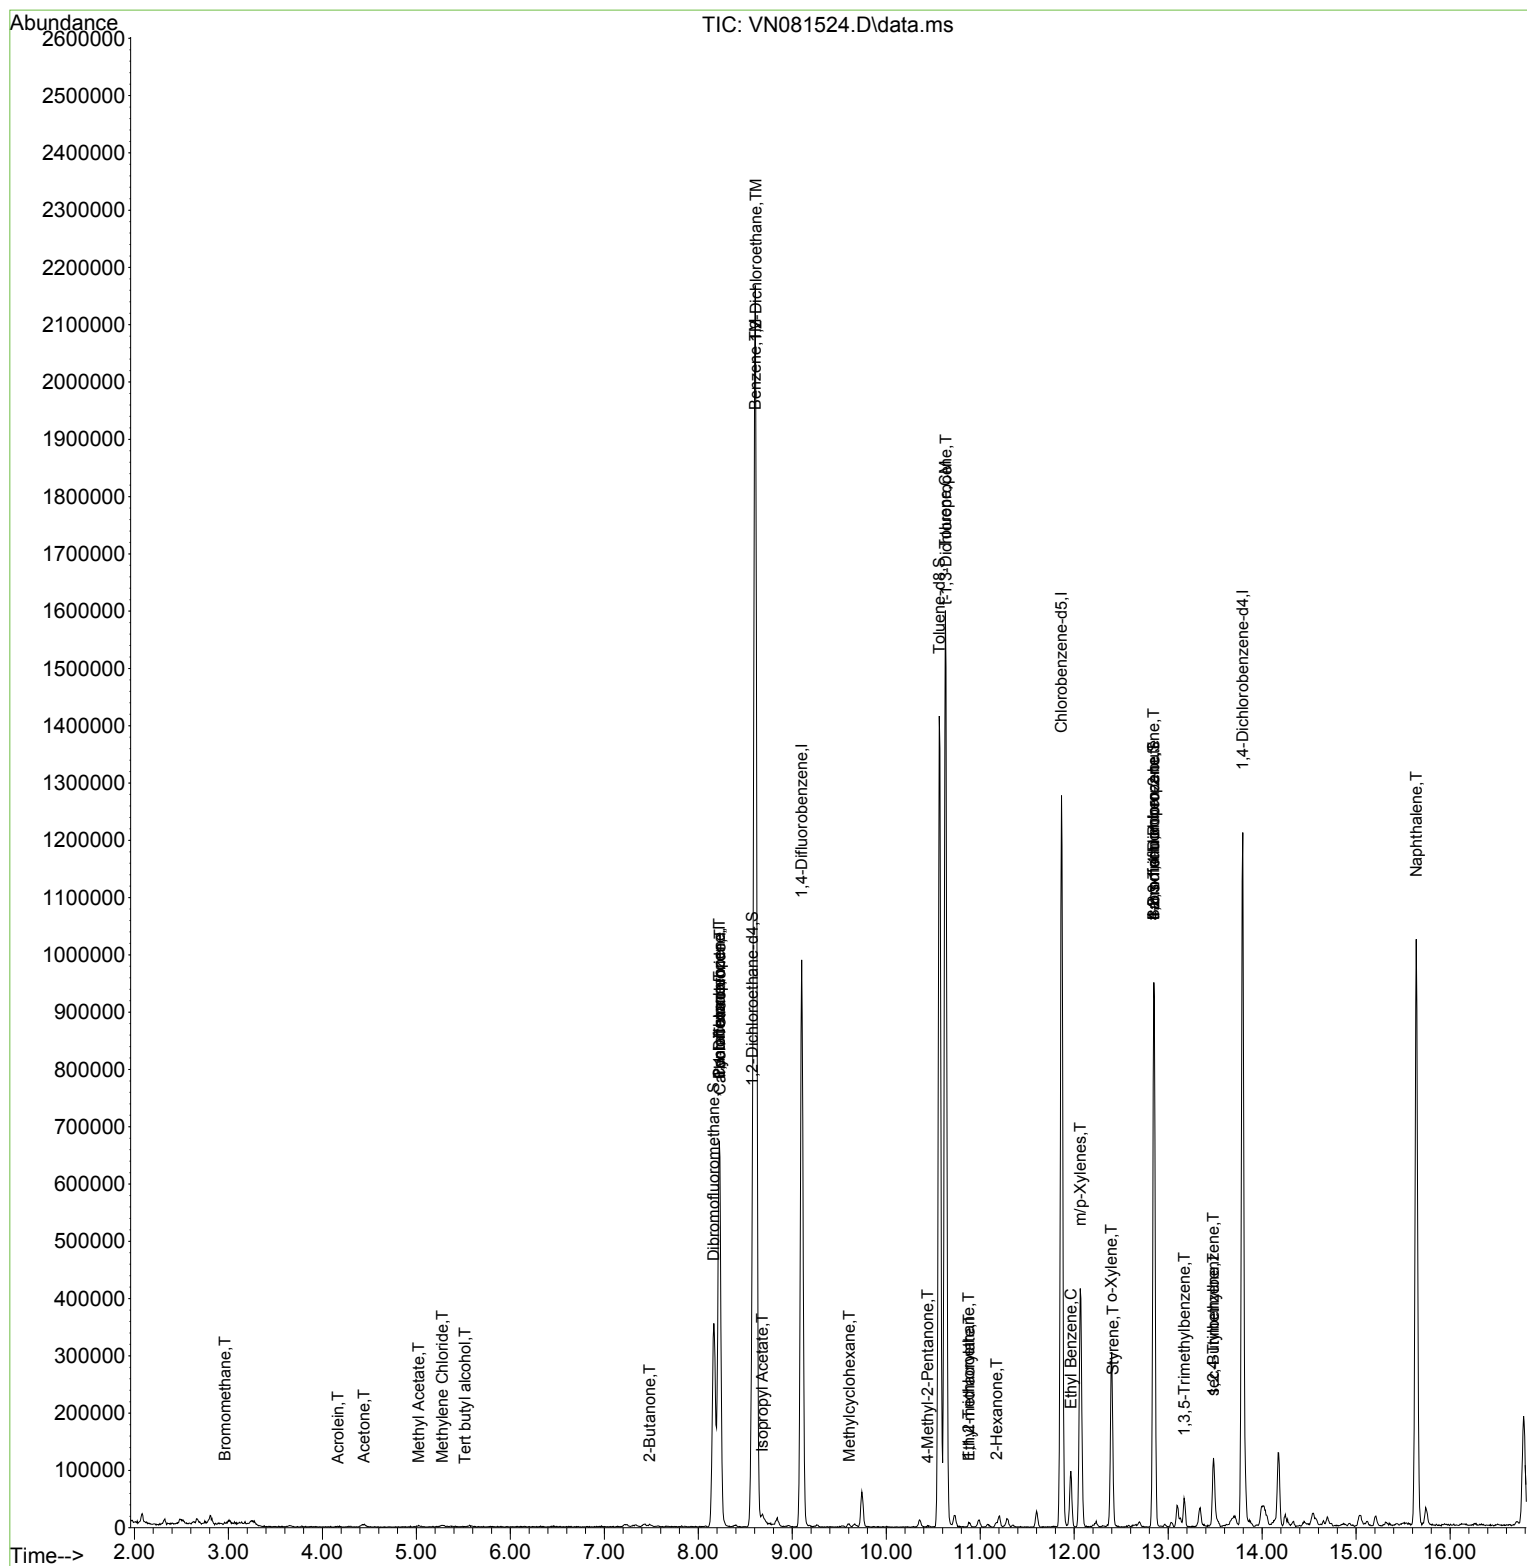



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.224 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN081524.D

Acq: 21 Mar 2024 17:00

Instrument :

MSVOA_N

ClientSampleId :





S-7

Tgt Ion:168 Resp: 495186

Ion Ratio Lower Upper

168 100

99 61.1 59.9 89.9

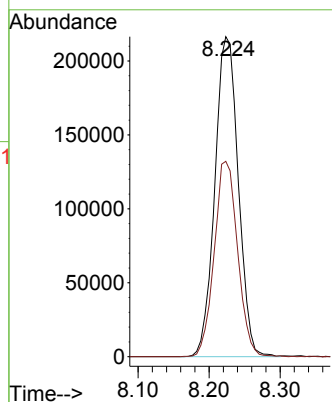

#5

Bromomethane

Concen: 0.265 ug/l

RT: 2.965 min Scan# 172

Delta R.T. 0.018 min

Lab File: VN081524.D




Acq: 21 Mar 2024 17:00


Tgt Ion: 94 Resp: 1398

Ion Ratio Lower Upper

94 100

96 114.8 69.2 103.8#


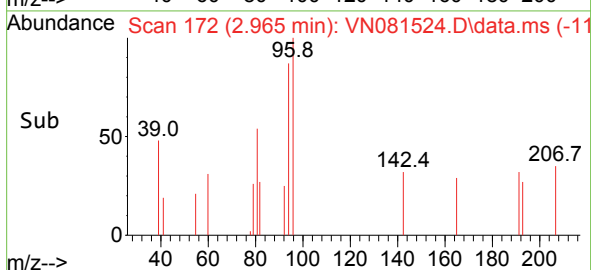






#11
Tert butyl alcohol
Concen: 0.250 ug/l
RT: 5.518 min Scan# 606
Delta R.T. -0.000 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00




Instrument :
MSVOA_N
ClientSampleId :
S-7


Tgt Ion: 59 Resp: 275
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#

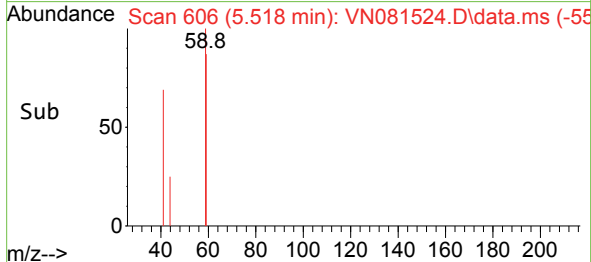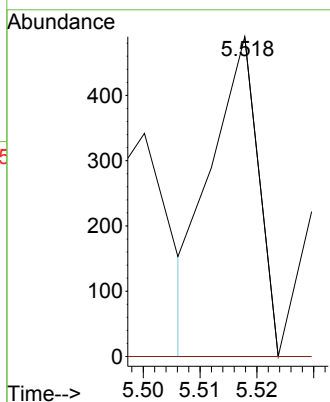

#13
Acrolein
Concen: 0.296 ug/l
RT: 4.165 min Scan# 376
Delta R.T. -0.012 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00

Tgt Ion: 56 Resp: 292
Ion Ratio Lower Upper
56 100
55 0.0 55.3 82.9#


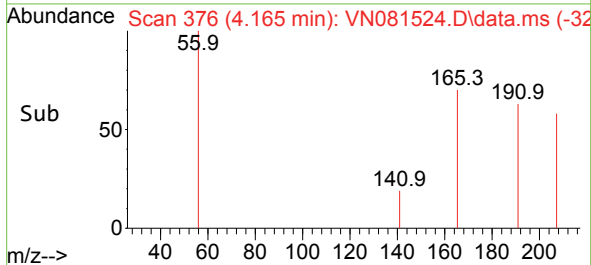

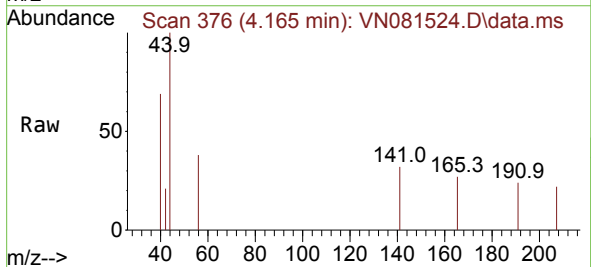




#16
Acetone
Concen: 4.420 ug/l
RT: 4.441 min Scan# 43
Delta R.T. 0.018 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00




Instrument :
MSVOA_N
ClientSampleId :
S-7


Tgt Ion: 43 Resp: 9020
Ion Ratio Lower Upper
43 100
58 42.8 24.8 37.2#

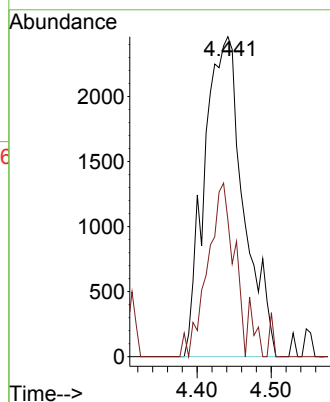

#18
Methyl Acetate
Concen: 0.279 ug/l
RT: 5.024 min Scan# 522
Delta R.T. 0.006 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00

Tgt Ion: 43 Resp: 1753
Ion Ratio Lower Upper
43 100
74 30.6 17.3 25.9#


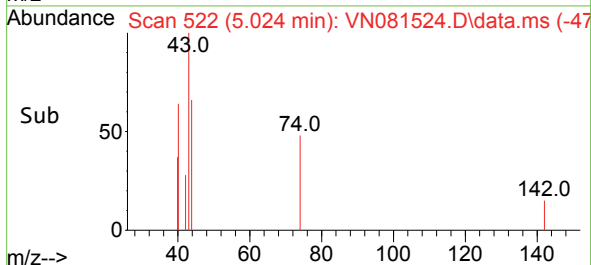

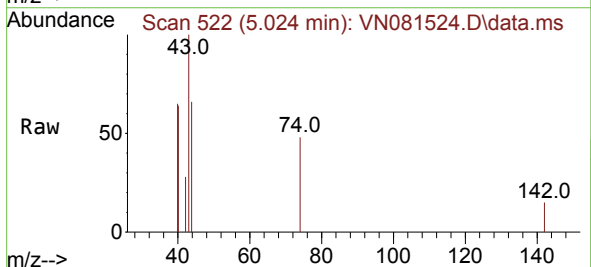




#20
Methylene Chloride
Concen: 0.397 ug/l
RT: 5.277 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00




Instrument :
MSVOA_N
ClientSampleId :
S-7


Tgt Ion:	84	Resp:	2656
Ion	Ratio	Lower	Upper
84	100		
49	59.2	108.1	162.1#
51	37.3	32.9	49.3
86	43.8	48.6	73.0#



#25
2-Butanone
Concen: 1.333 ug/l
RT: 7.482 min Scan# 940
Delta R.T. -0.000 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00

Tgt Ion:	43	Resp:	4667
Ion	Ratio	Lower	Upper
43	100		
72	33.4	19.5	29.3#

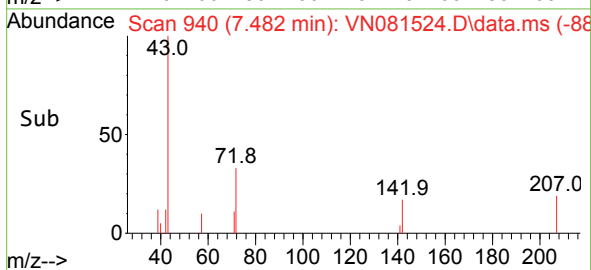



#31

Cyclohexane

Concen: 1.345 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.035 min

Lab File: VN081524.D

Acq: 21 Mar 2024 17:00

Instrument :

MSVOA_N

ClientSampleId :

S-7





Tgt Ion: 56 Resp: 13823

Ion Ratio Lower Upper

56 100

69 173.9 20.1 30.1#

84 168.3 56.9 85.3#

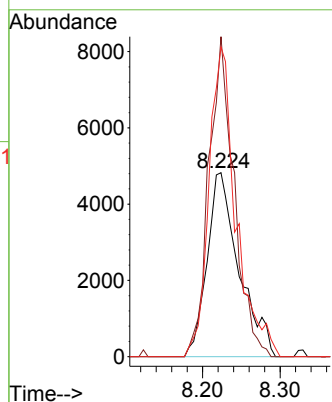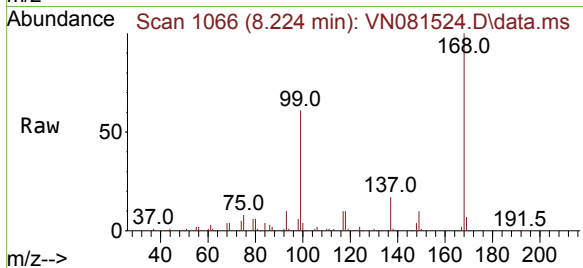

#33

1,2-Dichloroethane-d4

Concen: 49.584 ug/l

RT: 8.576 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VN081524.D




Acq: 21 Mar 2024 17:00


Tgt Ion: 65 Resp: 313119

Ion Ratio Lower Upper

65 100

67 52.2 0.0 102.4


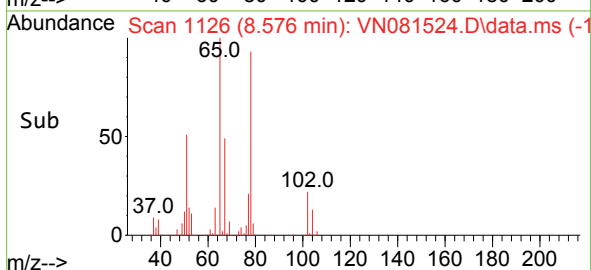

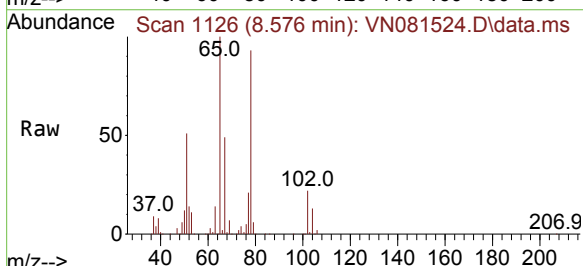




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00




Instrument :
MSVOA_N
ClientSampleId :
S-7


Tgt Ion:114 Resp: 870935
Ion Ratio Lower Upper
114 100
63 19.0 0.0 48.0
88 14.8 0.0 34.8

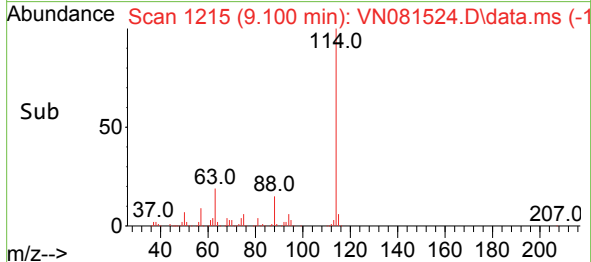

#35
Dibromofluoromethane
Concen: 47.347 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.006 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00

Tgt Ion:113 Resp: 260240
Ion Ratio Lower Upper
113 100
111 104.3 82.2 123.4
192 17.7 12.5 18.7

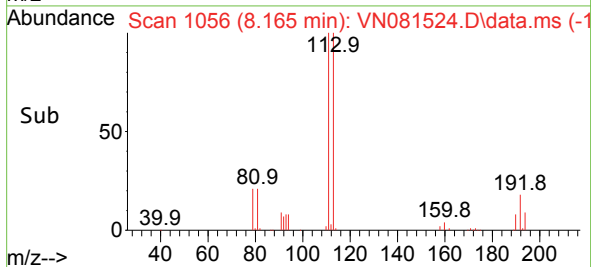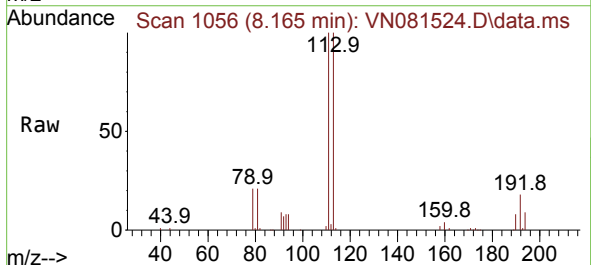



#36

1,1-Dichloropropene

Concen: 4.454 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.147 min

Lab File: VN081524.D

Acq: 21 Mar 2024 17:00

Instrument :

MSVOA_N

ClientSampleId :

S-7





Tgt Ion: 75 Resp: 41196

Ion Ratio Lower Upper

75 100

110 10.2 16.0 48.0#

77 0.0 25.8 38.6#



#38

Carbon Tetrachloride

Concen: 5.127 ug/l

RT: 8.229 min Scan# 1067

Delta R.T. -0.135 min

Lab File: VN081524.D

Acq: 21 Mar 2024 17:00




Tgt Ion: 117 Resp: 51950


Ion Ratio Lower Upper

117 100

119 6.1 73.4 110.2#

121 0.0 24.4 36.6#

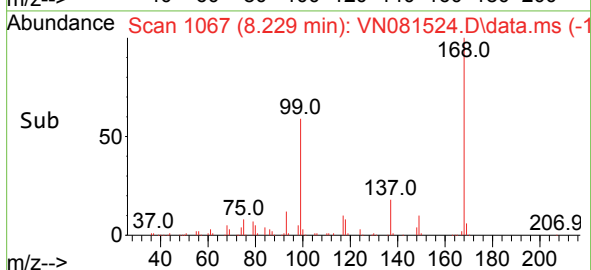



#39

Methylcyclohexane

Concen: 0.255 ug/l

RT: 9.606 min Scan# 1130

Delta R.T. 0.006 min

Lab File: VN081524.D

Acq: 21 Mar 2024 17:00

Instrument :

MSVOA_N

ClientSampleId :

S-7





Tgt Ion: 83 Resp: 2633

Ion Ratio Lower Upper

83 100

55 39.1 65.7 98.5#

98 49.7 33.8 50.6

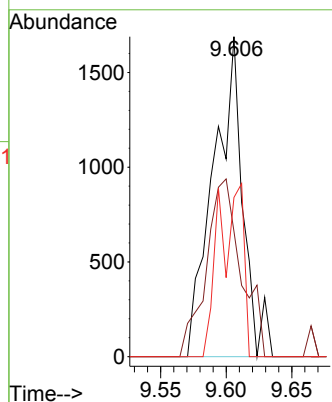

#40

Benzene

Concen: 81.592 ug/l

RT: 8.606 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VN081524.D




Acq: 21 Mar 2024 17:00


Tgt Ion: 78 Resp: 2206479

Ion Ratio Lower Upper

78 100

77 24.3 20.4 30.6





#42

1,2-Dichloroethane

Concen: 1.985 ug/l

RT: 8.612 min Scan# 1142

Delta R.T. -0.059 min

Lab File: VN081524.D

Acq: 21 Mar 2024 17:00

Instrument :

MSVOA_N

ClientSampleId :





S-7

Tgt Ion: 62 Resp: 18890

Ion Ratio Lower Upper

62 100

98 0.0 0.0 18.0

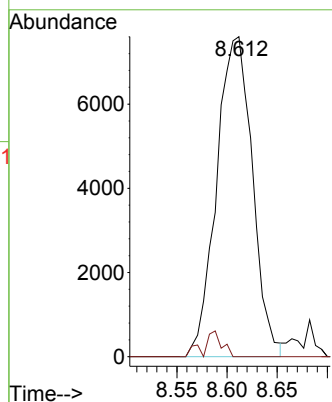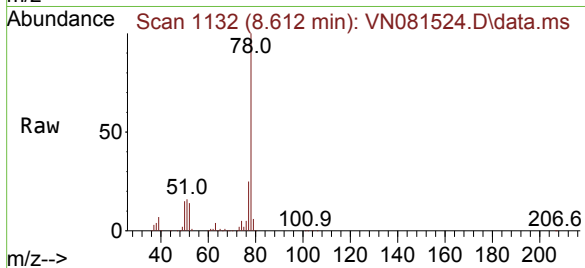

#43

Isopropyl Acetate

Concen: 1.302 ug/l

RT: 8.682 min Scan# 1144

Delta R.T. -0.006 min

Lab File: VN081524.D

Acq: 21 Mar 2024 17:00




Tgt Ion: 43 Resp: 17101


Ion Ratio Lower Upper

43 100

61 10.5 19.9 29.9#

87 7.3 9.0 13.6#


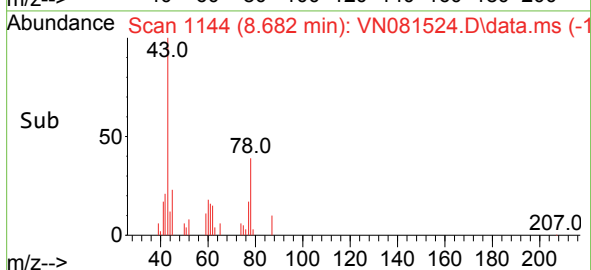

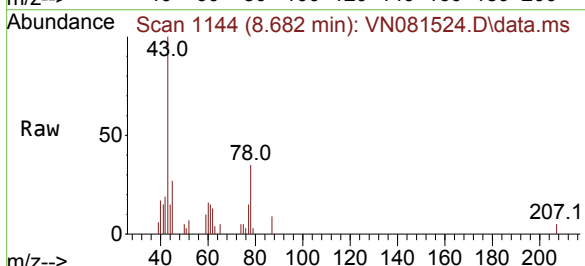




#50
Toluene-d8
Concen: 50.823 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.006 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00




Instrument :
MSVOA_N
ClientSampleId :
S-7


Tgt Ion: 98 Resp: 1009812
Ion Ratio Lower Upper
98 100
100 65.4 51.4 77.0

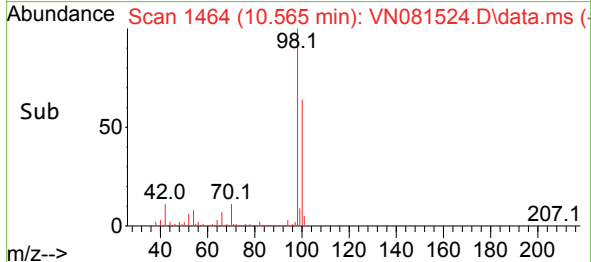

#51
4-Methyl-2-Pentanone
Concen: 0.219 ug/l
RT: 10.441 min Scan# 1443
Delta R.T. -0.006 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00

Tgt Ion: 43 Resp: 1758
Ion Ratio Lower Upper
43 100
58 0.0 29.4 44.0#

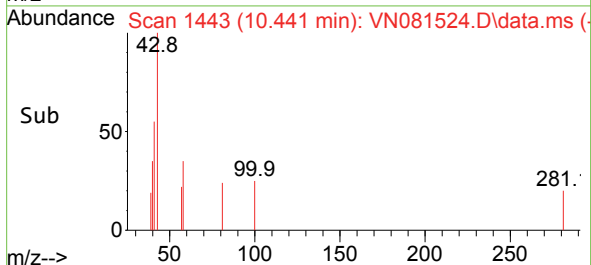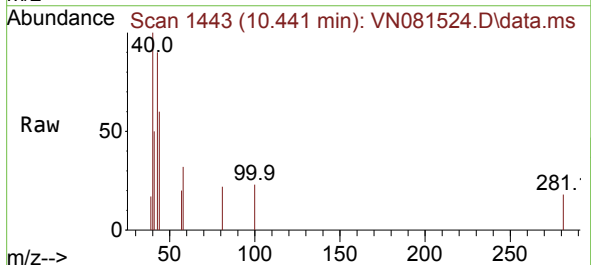

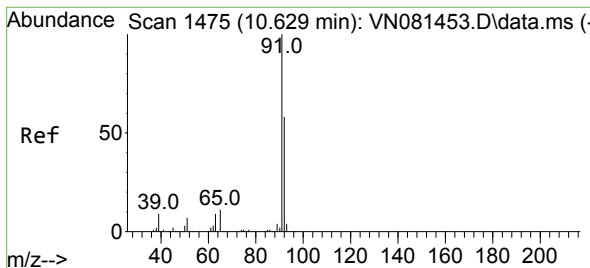

#52

Toluene

Concen: 42.011 ug/l

RT: 10.629 min Scan# 1475

Delta R.T. -0.000 min

Lab File: VN081524.D

Acq: 21 Mar 2024 17:00

Instrument :

MSVOA_N

ClientSampleId :





S-7

Tgt Ion: 92 Resp: 722097

Ion Ratio Lower Upper

92 100

91 173.6 139.4 209.0

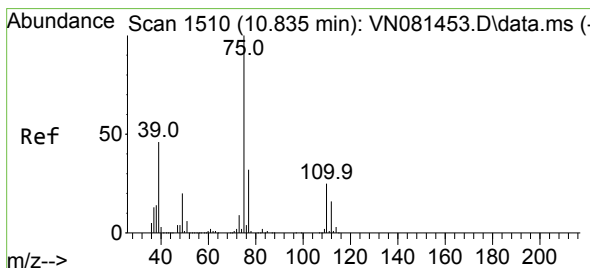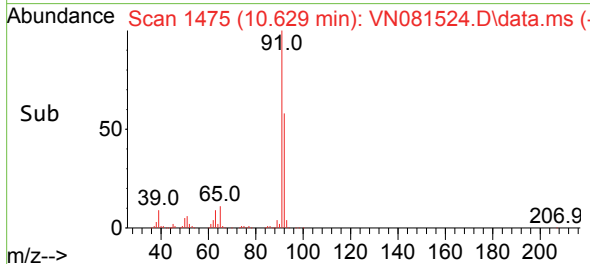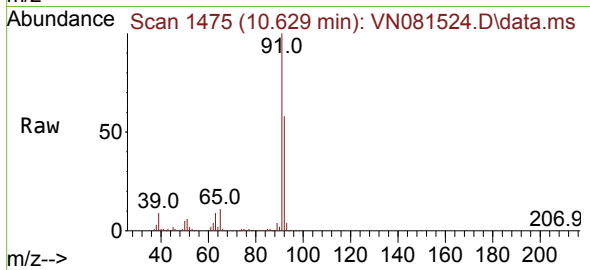

#53

t-1,3-Dichloropropene

Concen: 0.850 ug/l

RT: 10.635 min Scan# 1476

Delta R.T. -0.200 min

Lab File: VN081524.D




Acq: 21 Mar 2024 17:00


Tgt Ion: 75 Resp: 8936

Ion Ratio Lower Upper

75 100

77 139.0 25.5 38.3#


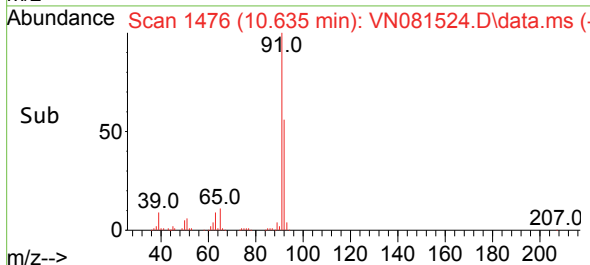
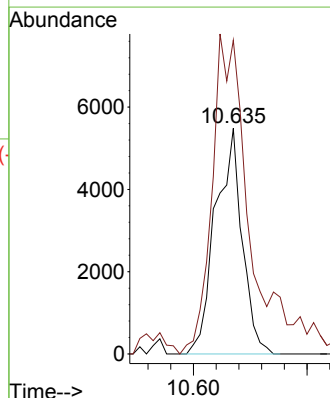
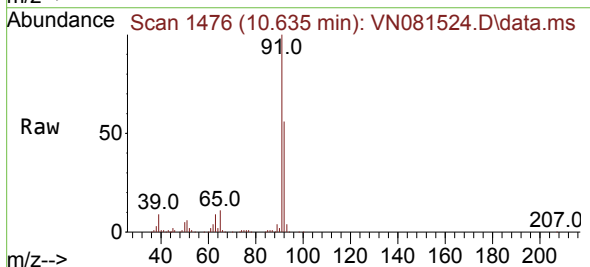




#55
1,1,2-Trichloroethane
Concen: 0.830 ug/l
RT: 10.876 min Scan# 1517
Delta R.T. -0.141 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00




Instrument :
MSVOA_N
ClientSampleId :
S-7


Tgt Ion:	97	Resp:	5739
Ion	Ratio	Lower	Upper
97	100		
83	0.0	72.9	109.3#
85	0.0	50.2	75.2#
99	8.4	49.6	74.4#

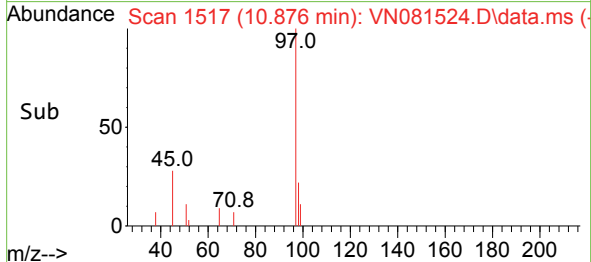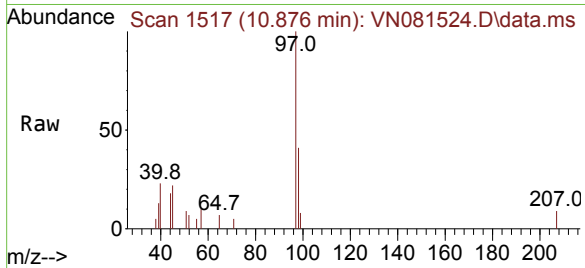

#56
Ethyl methacrylate
Concen: 0.602 ug/l
RT: 10.882 min Scan# 1518
Delta R.T. 0.006 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00

Tgt Ion:	69	Resp:	293
Ion	Ratio	Lower	Upper
69	100		
41	0.0	61.0	91.6#
39	0.0	31.8	47.6#


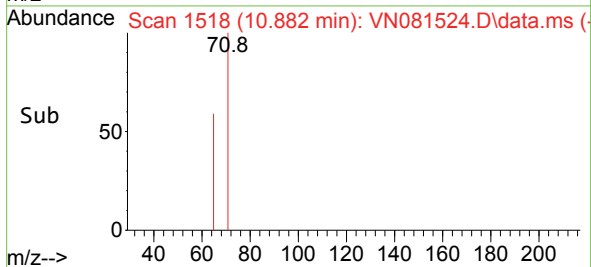

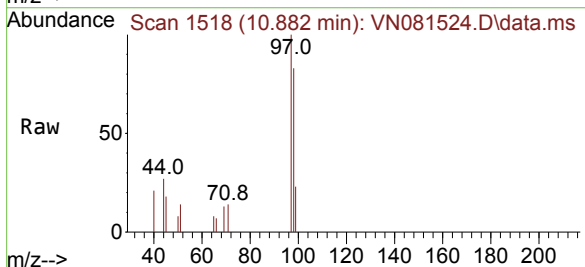




#59
2-Hexanone
Concen: 1.479 ug/l
RT: 11.176 min Scan# 1568
Delta R.T. -0.018 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00




Instrument :
MSVOA_N
ClientSampleId :
S-7


Tgt Ion: 43 Resp: 8763
Ion Ratio Lower Upper
43 100
58 12.8 25.9 77.8#

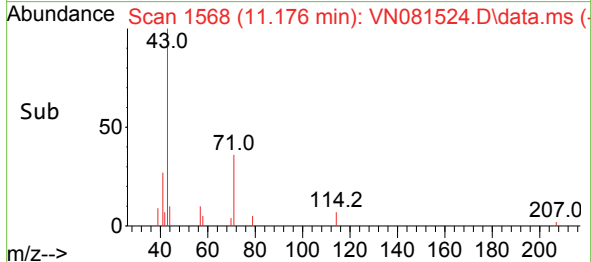

#62
4-Bromofluorobenzene
Concen: 47.300 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.006 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00

Tgt Ion: 95 Resp: 331153
Ion Ratio Lower Upper
95 100
174 77.8 0.0 120.4
176 74.9 0.0 121.0


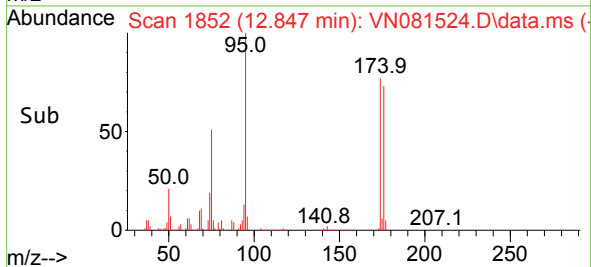

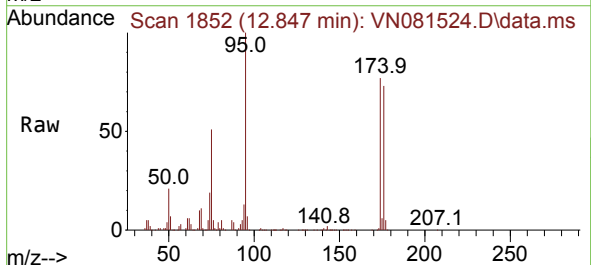


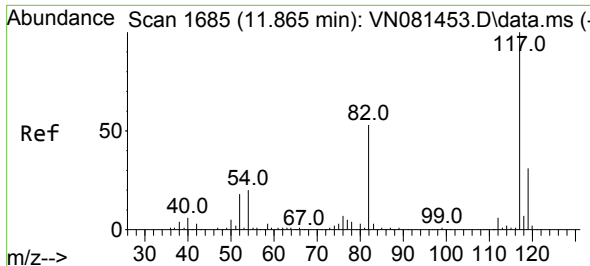

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00




Instrument :
MSVOA_N
ClientSampleId :
S-7


Tgt Ion:117 Resp: 752181
Ion Ratio Lower Upper
117 100
82 54.5 52.7 79.1
119 31.9 25.3 37.9

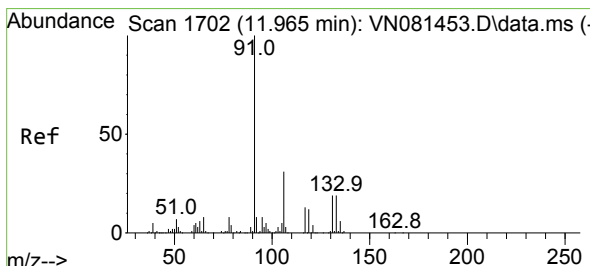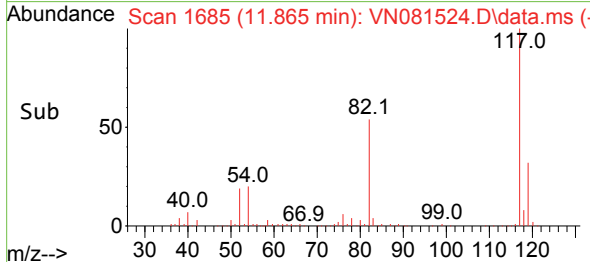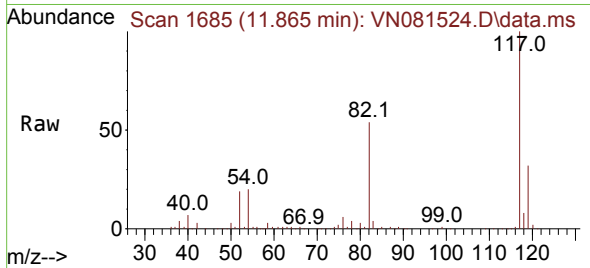

#67
Ethyl Benzene
Concen: 2.182 ug/l
RT: 11.964 min Scan# 1702
Delta R.T. -0.000 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00

Tgt Ion: 91 Resp: 67409
Ion Ratio Lower Upper
91 100
106 28.0 23.8 35.6


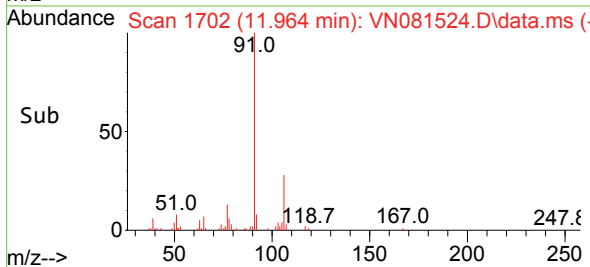

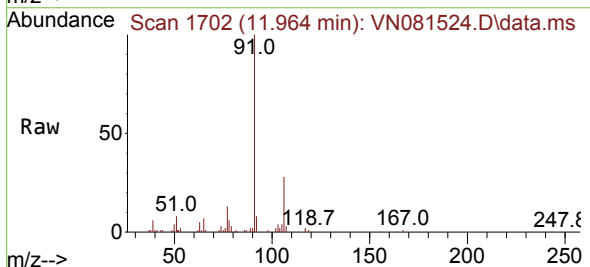


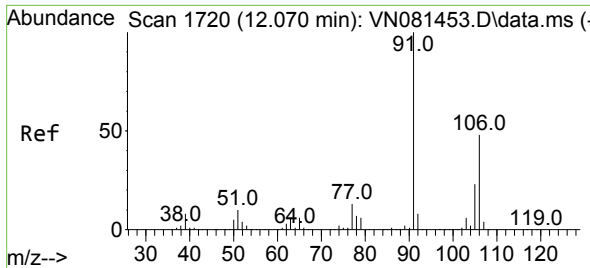

#68
m/p-Xylenes
Concen: 11.442 ug/l
RT: 12.065 min Scan# 1719
Delta R.T. -0.006 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00




Instrument :
MSVOA_N
ClientSampleId :
S-7


Tgt Ion:106 Resp: 132495
Ion Ratio Lower Upper
106 100
91 207.4 169.0 253.6

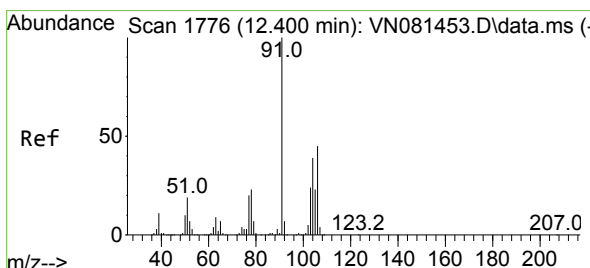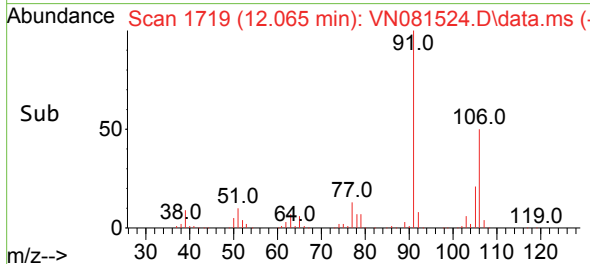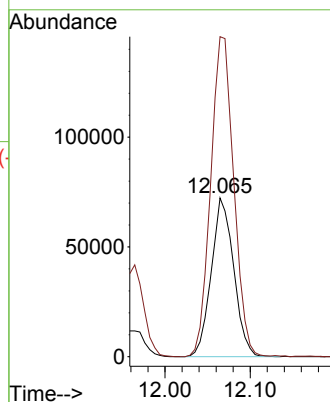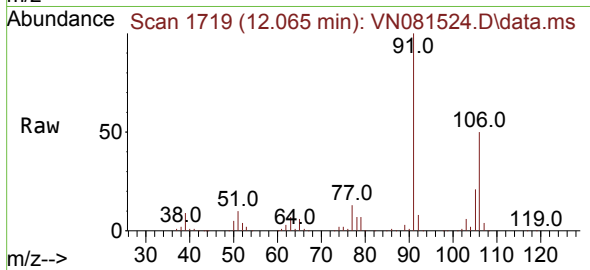

#69
o-Xylene
Concen: 7.253 ug/l
RT: 12.394 min Scan# 1775
Delta R.T. -0.006 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00

Tgt Ion:106 Resp: 82448
Ion Ratio Lower Upper
106 100
91 220.0 112.1 336.3

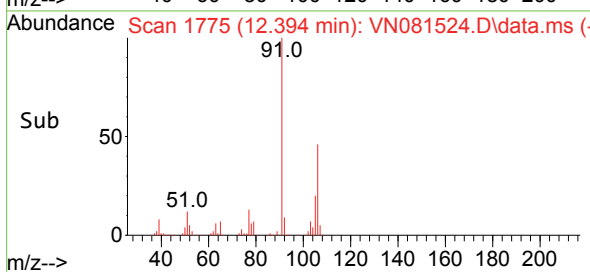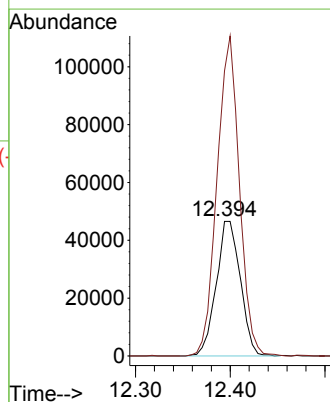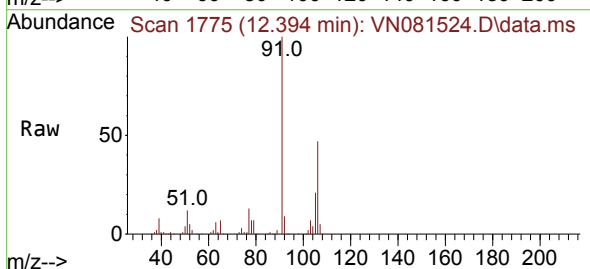



#70

Styrene

Concen: 0.740 ug/l

RT: 12.412 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN081524.D

Acq: 21 Mar 2024 17:00

Instrument :

MSVOA_N

ClientSampleId :

S-7





Tgt Ion:104 Resp: 13570

Ion Ratio Lower Upper

104 100

78 119.3 43.8 65.8#

103 116.8 44.2 66.2#



#71

Bromoform

Concen: 0.497 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.265 min

Lab File: VN081524.D

Acq: 21 Mar 2024 17:00




Tgt Ion:173 Resp: 2463


Ion Ratio Lower Upper

173 100

175 725.8 23.1 69.2#

254 0.0 0.0 0.0


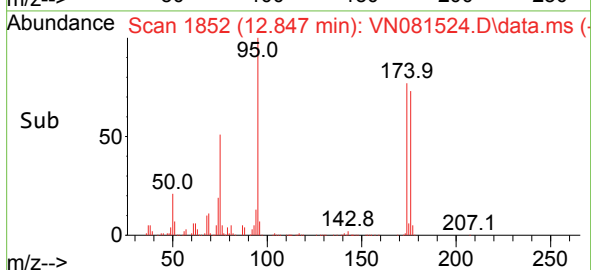




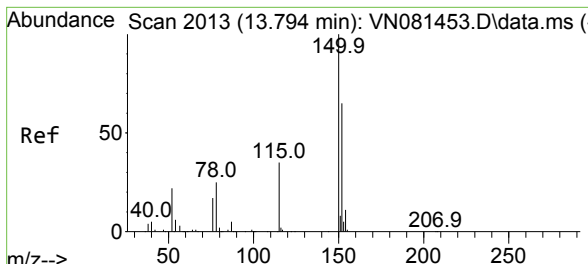

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VN081524.D
 Acq: 21 Mar 2024 17:00




Instrument :
 MSVOA_N
 ClientSampleId :
 S-7


Tgt Ion:	152	Resp:	325693
Ion	Ratio	Lower	Upper
152	100		
115	61.1	32.3	96.8
150	157.7	0.0	339.8

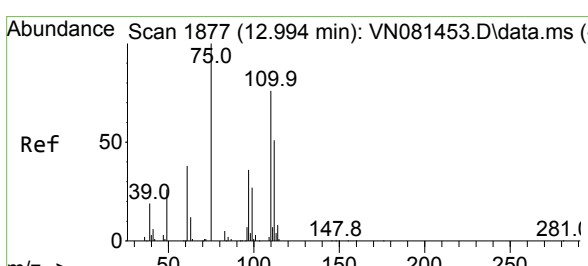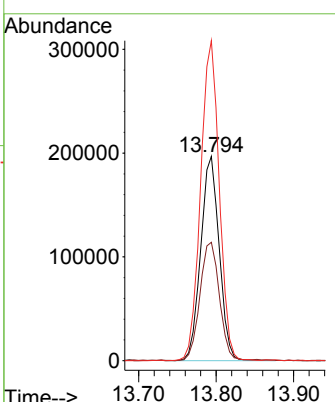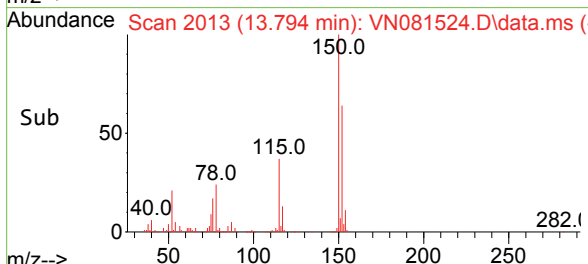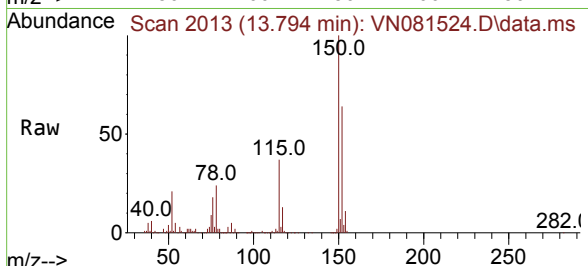

#76
 1,2,3-Trichloropropane
 Concen: 22.061 ug/l
 RT: 12.847 min Scan# 1852
 Delta R.T. -0.147 min
 Lab File: VN081524.D
 Acq: 21 Mar 2024 17:00

Tgt Ion:	75	Resp:	171875
Ion	Ratio	Lower	Upper
75	100		
77	1.7	91.0	272.8#


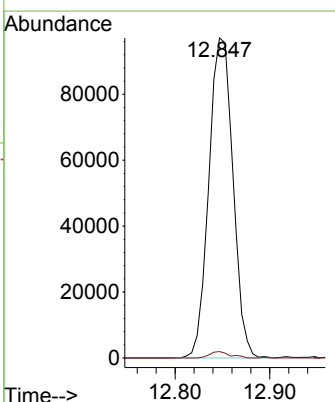
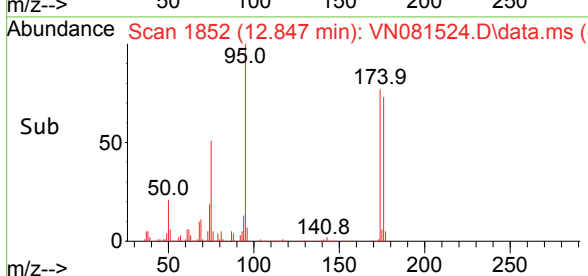
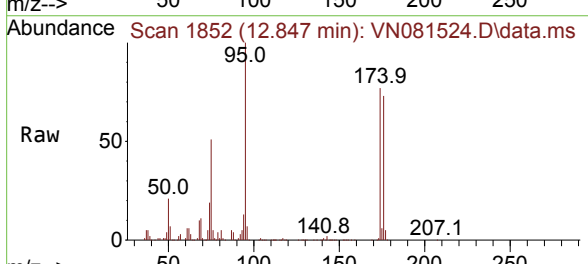


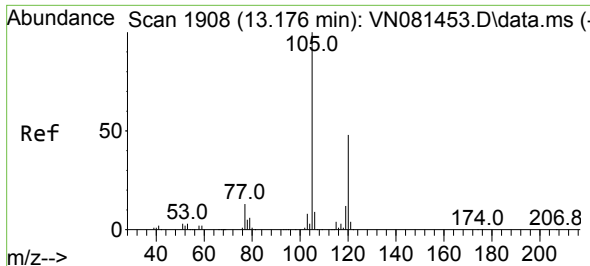

#80
1,3,5-Trimethylbenzene
Concen: 1.108 ug/l
RT: 13.170 min Scan# 1908
Delta R.T. -0.006 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00




Instrument :
MSVOA_N
ClientSampleId :
S-7


Tgt Ion:105 Resp: 25409
Ion Ratio Lower Upper
105 100
120 54.1 23.0 69.0

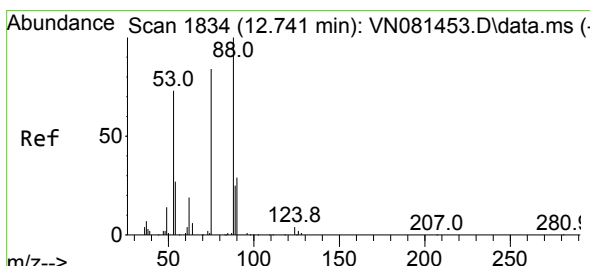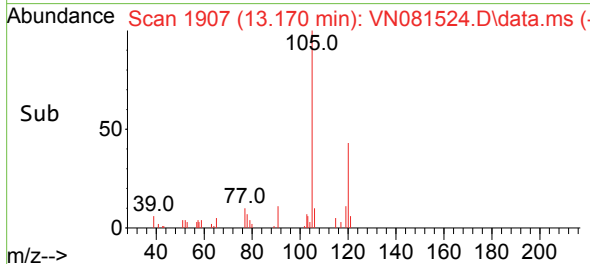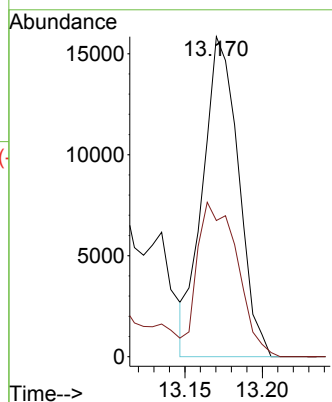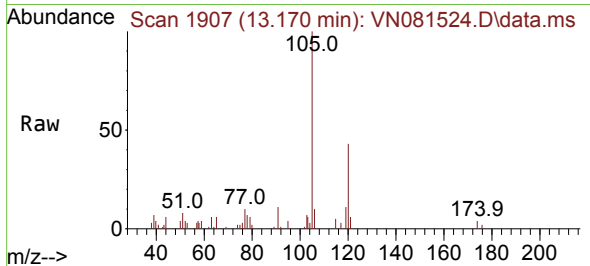

#81
trans-1,4-Dichloro-2-butene
Concen: 59.617 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.106 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00

Tgt Ion: 75 Resp: 171875
Ion Ratio Lower Upper
75 100
53 0.2 71.4 107.2#
89 0.1 33.4 50.0#


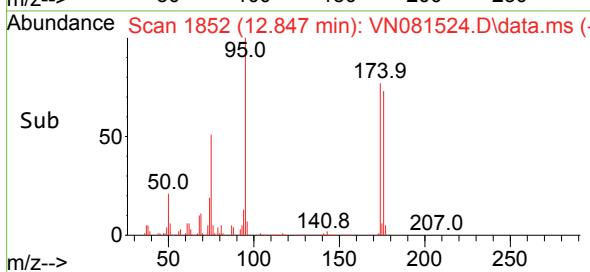
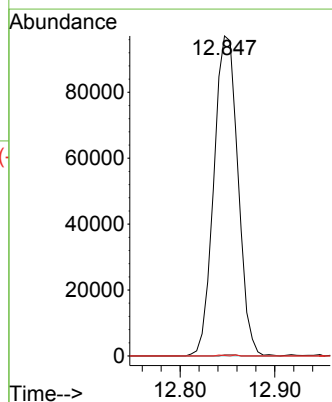
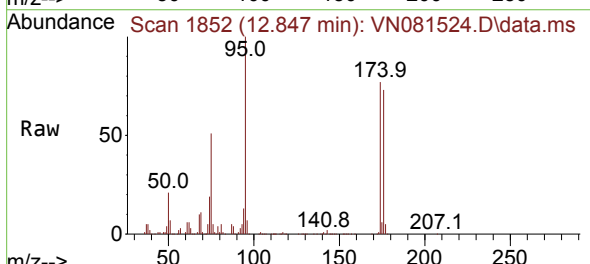




#84
1,2,4-Trimethylbenzene
Concen: 3.167 ug/l
RT: 13.482 min Scan# 1960
Delta R.T. -0.000 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00




Instrument :
MSVOA_N
ClientSampleId :
S-7


Tgt Ion:105 Resp: 72988
Ion Ratio Lower Upper
105 100
120 41.4 20.9 62.7

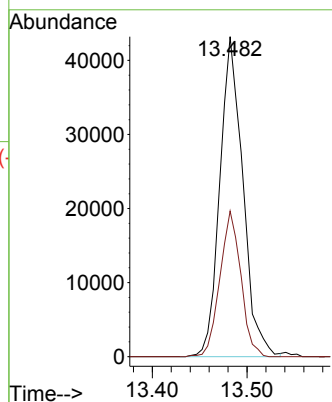

#85
sec-Butylbenzene
Concen: 2.582 ug/l
RT: 13.482 min Scan# 1960
Delta R.T. -0.135 min
Lab File: VN081524.D
Acq: 21 Mar 2024 17:00


Tgt Ion:105 Resp: 72988
Ion Ratio Lower Upper
105 100
134 0.0 8.6 25.8#

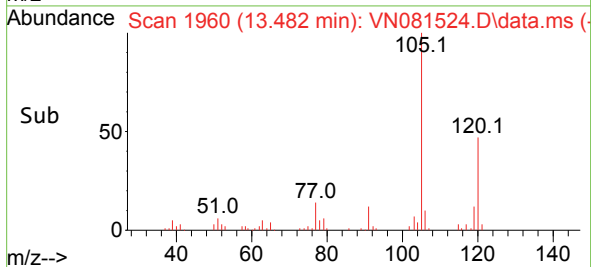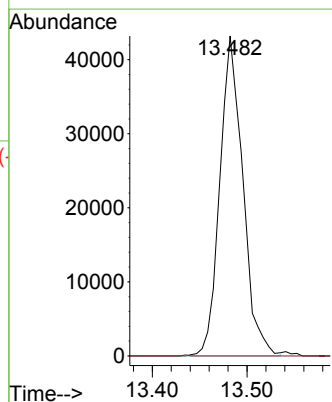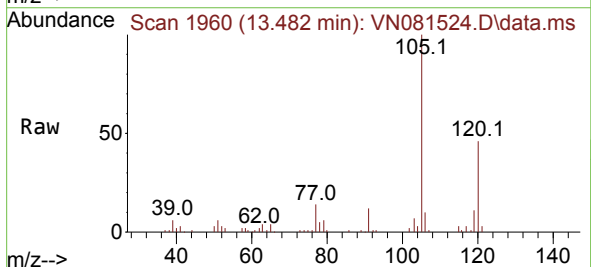

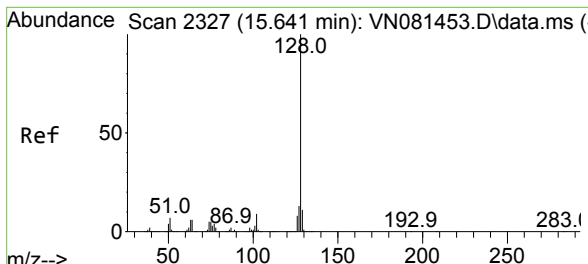

#95
 Naphthalene
 Concen: 41.288 ug/l
 RT: 15.641 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN081524.D
 Acq: 21 Mar 2024 17:00

Instrument :
 MSVOA_N
 ClientSampleId :
 S-7

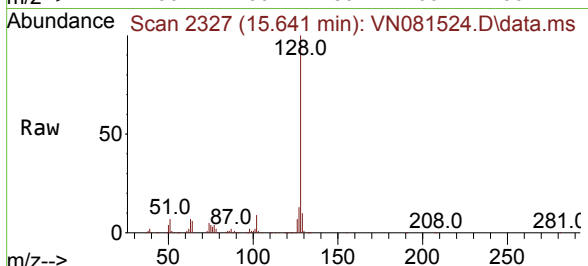

Tgt Ion:128 Resp: 938149

Ion	Ratio	Lower	Upper
128	100		
127	13.2	10.0	15.0
129	11.1	8.7	13.1

