

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032124\
 Data File : VN081530.D
 Acq On : 21 Mar 2024 19:23
 Operator : JC\MD
 Sample : P1798-13 20X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 S-13

Quant Time: Mar 22 05:12:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 19 06:00:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	433571	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	768212	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	723289	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	305161	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	274528	49.651	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	99.300%		
35) Dibromofluoromethane	8.165	113	238678	49.230	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	98.460%		
50) Toluene-d8	10.571	98	930516	53.095	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	106.180%		
62) 4-Bromofluorobenzene	12.847	95	310221	50.235	ug/l	0.00
Spiked Amount 50.000	Range 64 - 133		Recovery =	100.480%		
Target Compounds						Qvalue
11) Tert butyl alcohol	5.506	59	324	0.336	ug/l #	72
13) Acrolein	4.171	56	457	0.529	ug/l #	15
16) Acetone	4.442	43	11521	6.447	ug/l #	86
18) Methyl Acetate	5.030	43	1441	0.262	ug/l #	64
20) Methylene Chloride	5.265	84	1556	0.266	ug/l #	32
25) 2-Butanone	7.483	43	3202	1.045	ug/l #	86
31) Cyclohexane	8.230	56	14093	1.566	ug/l #	3
36) 1,1-Dichloropropene	8.224	75	35108	4.303	ug/l #	51
38) Carbon Tetrachloride	8.224	117	45700	5.113	ug/l #	18
39) Methylcyclohexane	9.594	83	2847	0.312	ug/l #	83
40) Benzene	8.606	78	2911114	122.043	ug/l	96
43) Isopropyl Acetate	8.688	43	15868	1.370	ug/l #	89
51) 4-Methyl-2-Pentanone	10.447	43	1442	0.204	ug/l #	83
52) Toluene	10.630	92	1069876	70.568	ug/l	100
53) t-1,3-Dichloropropene	10.635	75	13026	1.405	ug/l #	1
54) cis-1,3-Dichloropropene	10.359	75	3635	0.366	ug/l #	54
55) 1,1,2-Trichloroethane	10.888	97	11124	1.823	ug/l #	17
56) Ethyl methacrylate	10.882	69	689	0.654	ug/l #	20
59) 2-Hexanone	11.171	43	8319	1.592	ug/l #	26
67) Ethyl Benzene	11.965	91	93823	3.159	ug/l	96
68) m/p-Xylenes	12.071	106	194635	17.480	ug/l	94
69) o-Xylene	12.400	106	123296	11.279	ug/l	91
70) Styrene	12.412	104	20472	1.161	ug/l #	12
76) 1,2,3-Trichloropropane	12.853	75	163280	22.368	ug/l #	1
78) n-propylbenzene	13.035	91	8410	0.274	ug/l	99
80) 1,3,5-Trimethylbenzene	13.176	105	35882	1.670	ug/l	93
81) trans-1,4-Dichloro-2-b...	12.853	75	163280	60.447	ug/l #	15
82) 4-Chlorotoluene	13.171	91	4171	0.230	ug/l #	44
84) 1,2,4-Trimethylbenzene	13.482	105	101433	4.697	ug/l	98
85) sec-Butylbenzene	13.482	105	101433	3.830	ug/l #	60
95) Naphthalene	15.641	128	1694522	79.593	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032124\
Data File : VN081530.D
Acq On : 21 Mar 2024 19:23
Operator : JC\MD
Sample : P1798-13 20X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
S-13

Quant Time: Mar 22 05:12:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 19 06:00:00 2024
Response via : Initial Calibration




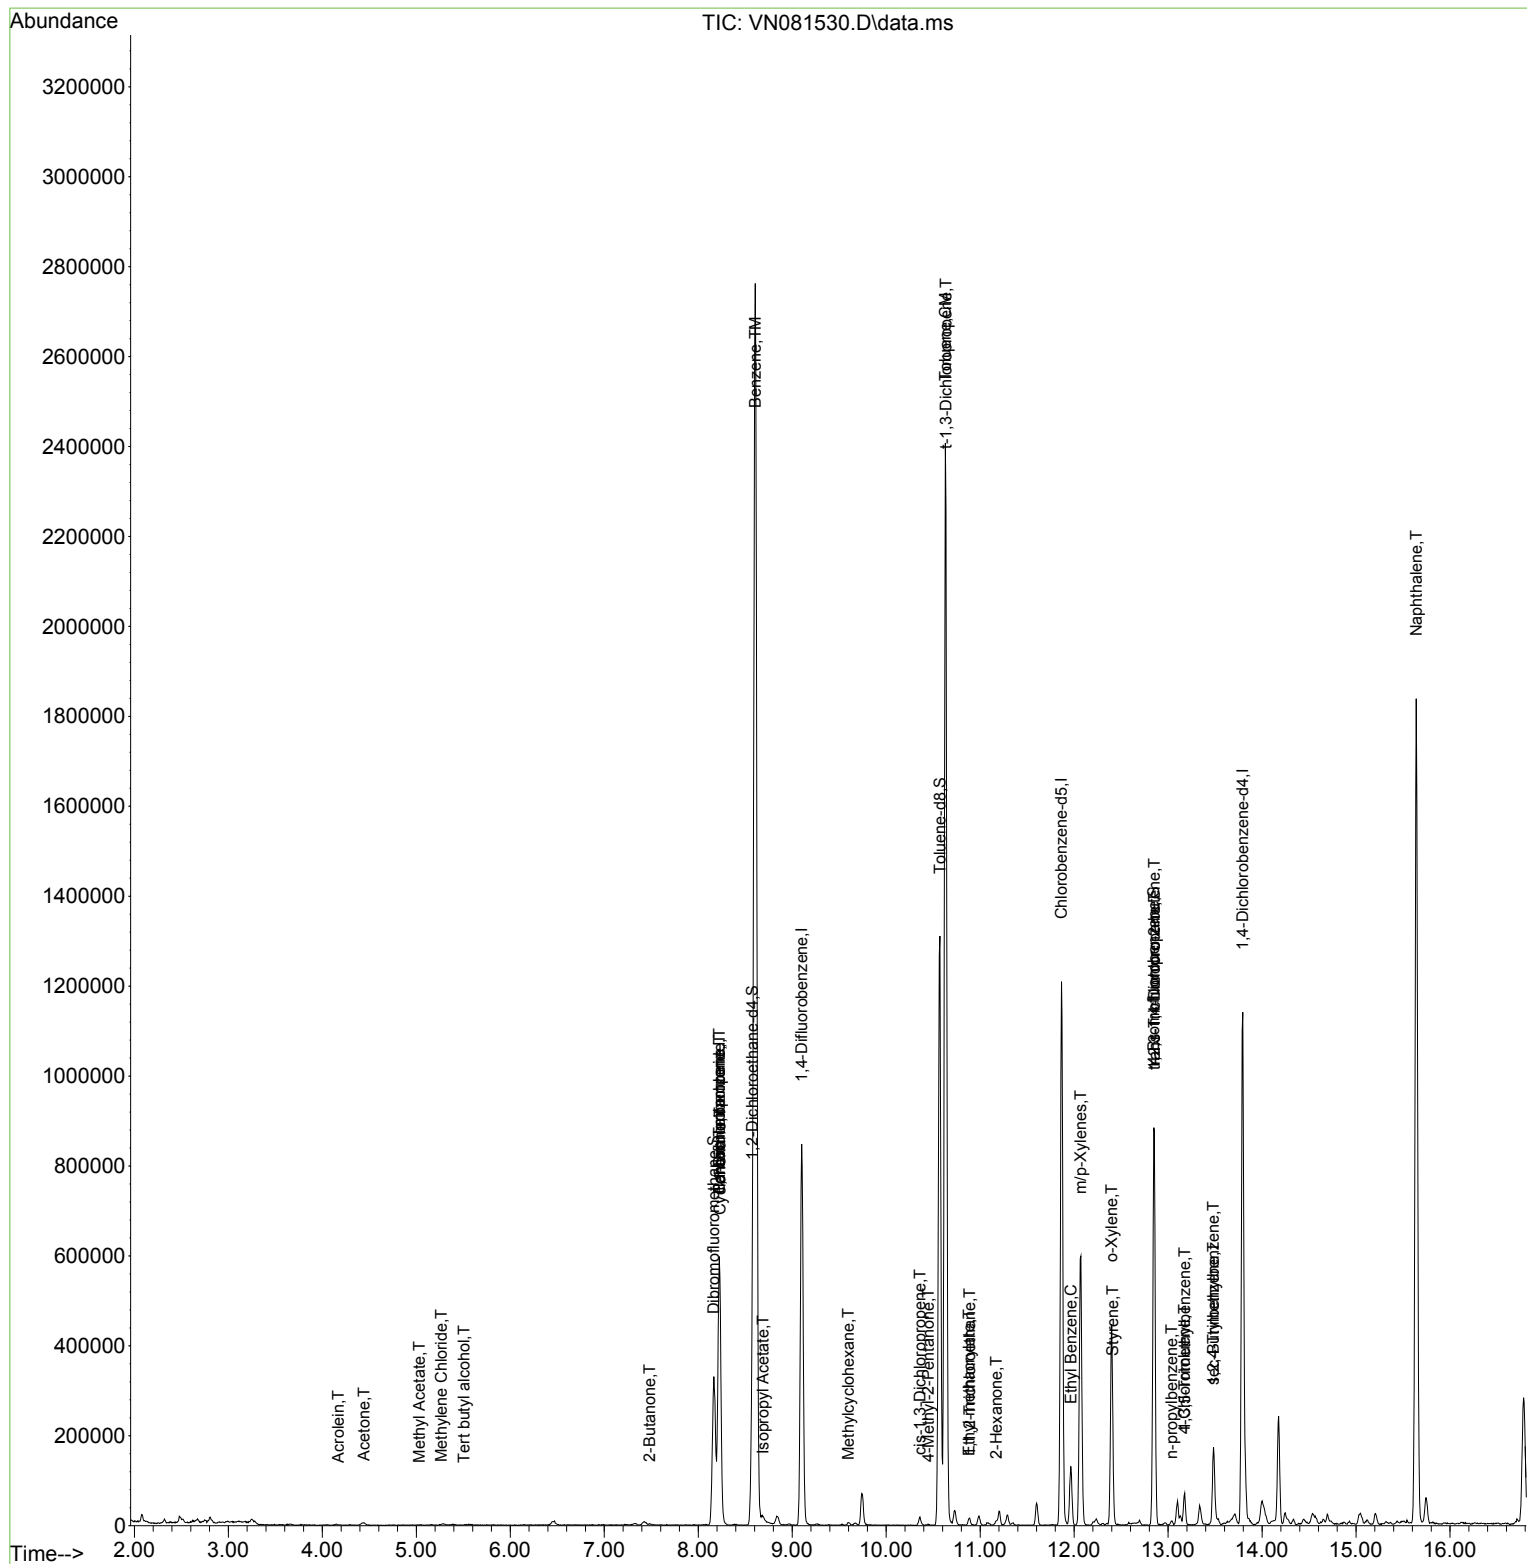


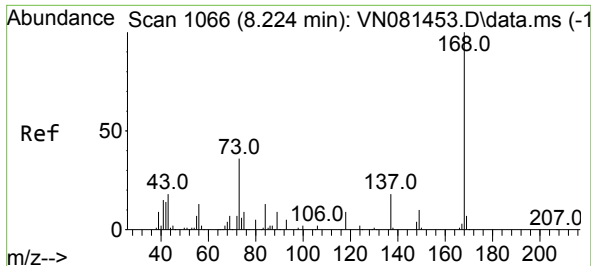

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23




Instrument :
MSVOA_N
ClientSampleId :
S-13


Tgt Ion:168 Resp: 433571
Ion Ratio Lower Upper
168 100
99 62.4 59.9 89.9

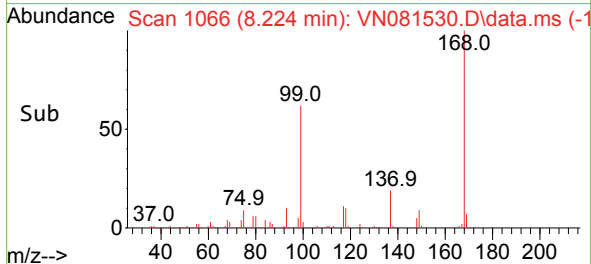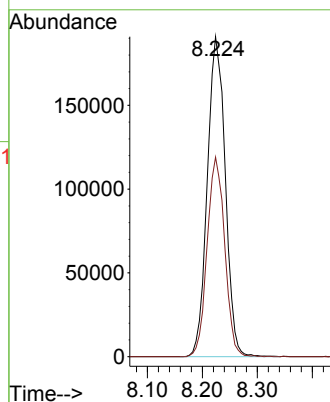

#11
Tert butyl alcohol
Concen: 0.336 ug/l
RT: 5.506 min Scan# 604
Delta R.T. -0.012 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23

Tgt Ion: 59 Resp: 324
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#

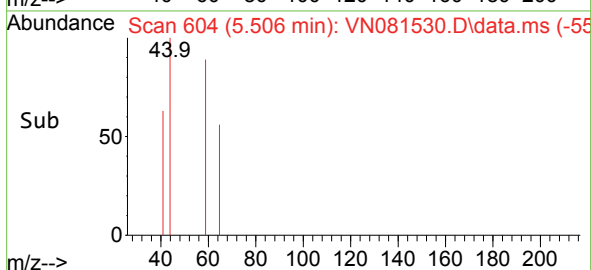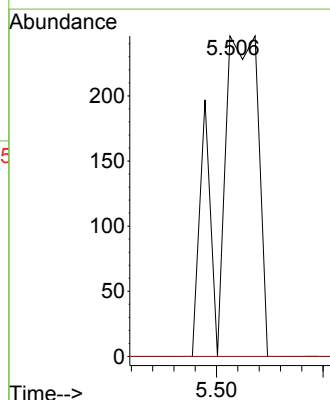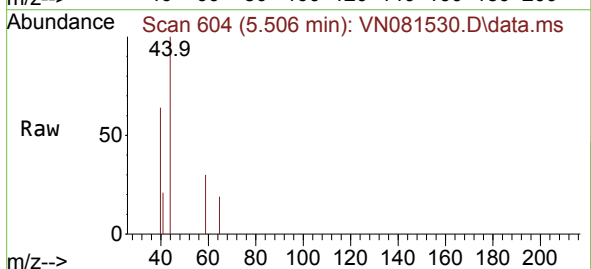

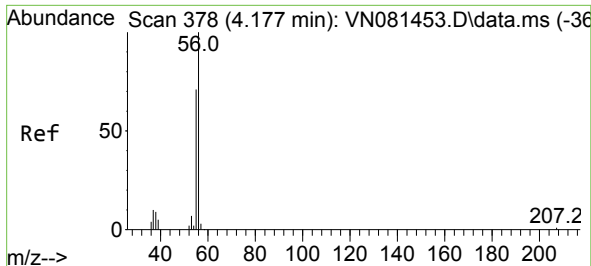

#13

Acrolein

Concen: 0.529 ug/l

RT: 4.171 min Scan# 31

Delta R.T. -0.006 min

Lab File: VN081530.D

Acq: 21 Mar 2024 19:23

Instrument :

MSVOA_N

ClientSampleId :





S-13

Tgt Ion: 56 Resp: 457

Ion Ratio Lower Upper

56 100

55 0.0 55.3 82.9#

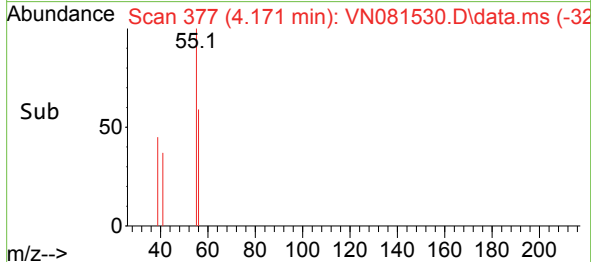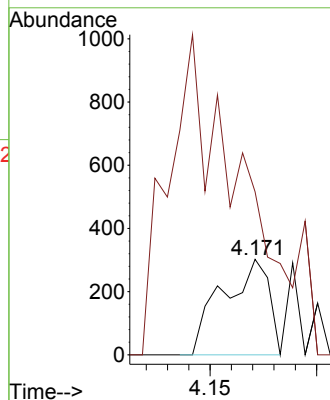

#16

Acetone

Concen: 6.447 ug/l

RT: 4.442 min Scan# 423

Delta R.T. 0.018 min

Lab File: VN081530.D




Acq: 21 Mar 2024 19:23


Tgt Ion: 43 Resp: 11521

Ion Ratio Lower Upper

43 100

58 38.5 24.8 37.2#


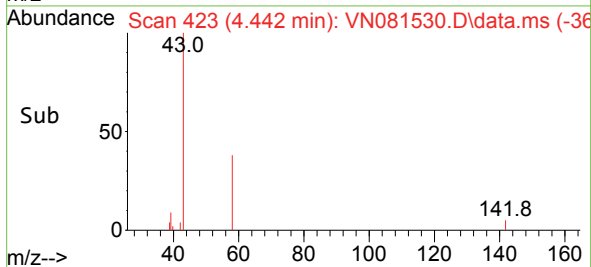
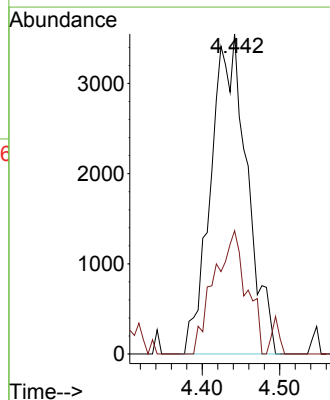
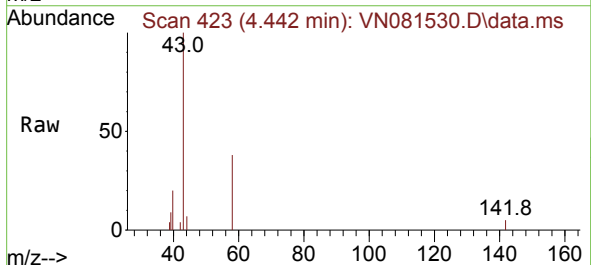




#18
Methyl Acetate
Concen: 0.262 ug/l
RT: 5.030 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23




Instrument :
MSVOA_N
ClientSampleId :
S-13


Tgt Ion: 43 Resp: 1441
Ion Ratio Lower Upper
43 100
74 4.6 17.3 25.9#

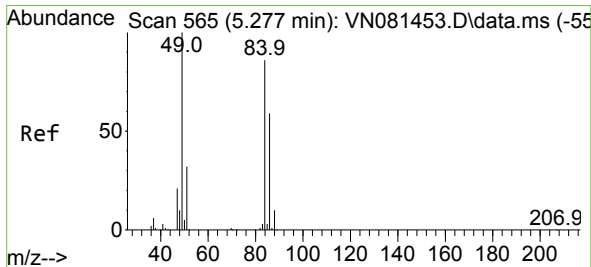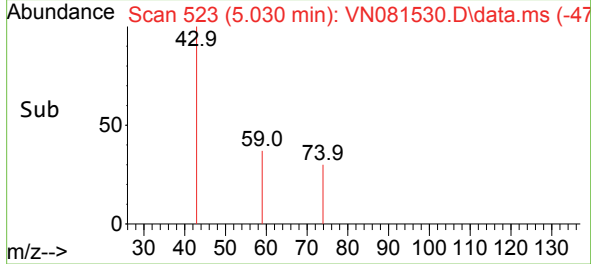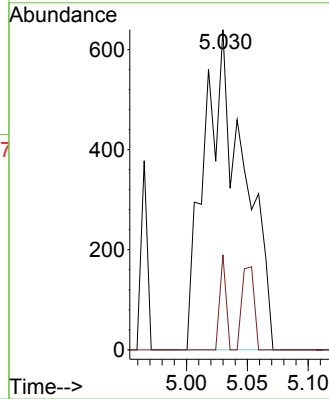

#20
Methylene Chloride
Concen: 0.266 ug/l
RT: 5.265 min Scan# 563
Delta R.T. -0.012 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23

Tgt Ion: 84 Resp: 1556
Ion Ratio Lower Upper
84 100
49 46.3 108.1 162.1#
51 0.0 32.9 49.3#
86 20.1 48.6 73.0#


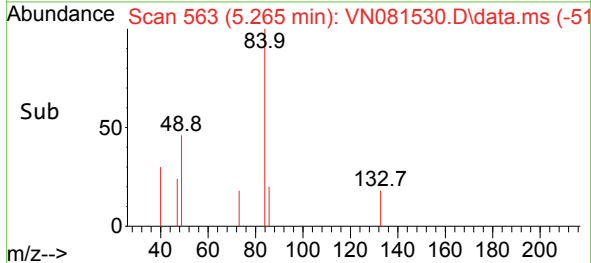
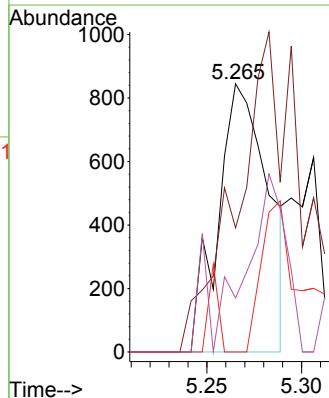
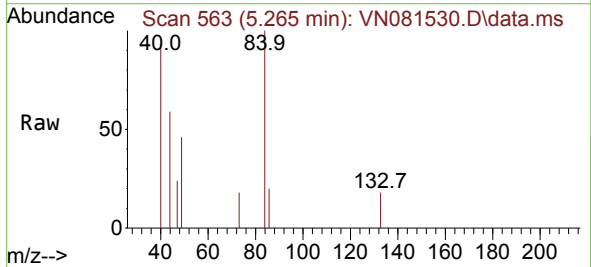


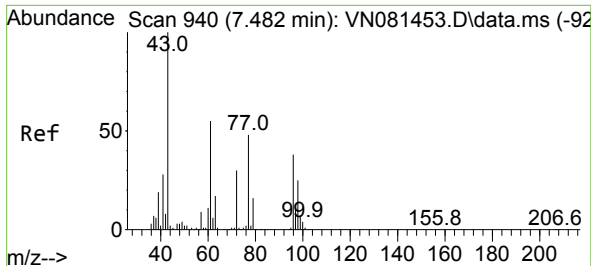

#25
2-Butanone
Concen: 1.045 ug/l
RT: 7.483 min Scan# 940
Delta R.T. 0.000 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23




Instrument :
MSVOA_N
ClientSampleId :
S-13


Tgt Ion: 43 Resp: 3202
Ion Ratio Lower Upper
43 100
72 31.3 19.5 29.3#

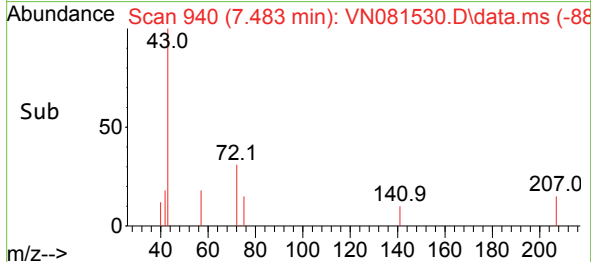

#31
Cyclohexane
Concen: 1.566 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.029 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23

Tgt Ion: 56 Resp: 14093
Ion Ratio Lower Upper
56 100
69 140.5 20.1 30.1#
84 112.7 56.9 85.3#

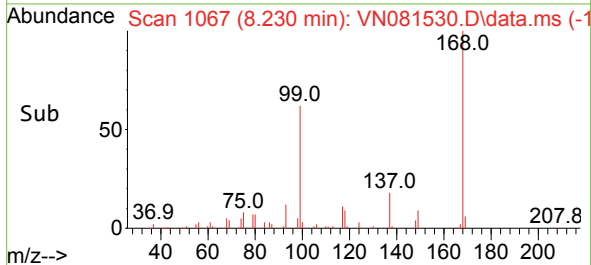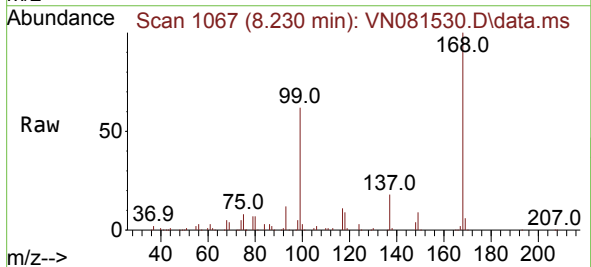

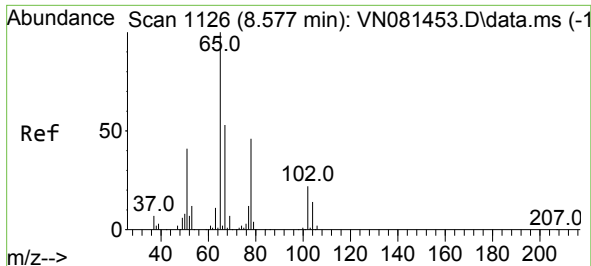

#33

1,2-Dichloroethane-d4

Concen: 49.651 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VN081530.D

Acq: 21 Mar 2024 19:23

Instrument :

MSVOA_N

ClientSampleId :





S-13

Tgt Ion: 65 Resp: 274528

Ion Ratio Lower Upper

65 100

67 53.0 0.0 102.4

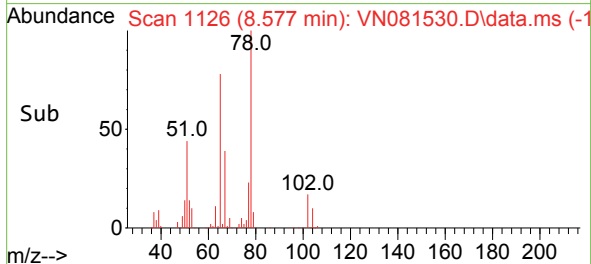

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. -0.006 min

Lab File: VN081530.D

Acq: 21 Mar 2024 19:23




Tgt Ion: 114 Resp: 768212


Ion Ratio Lower Upper

114 100

63 20.3 0.0 48.0

88 15.2 0.0 34.8


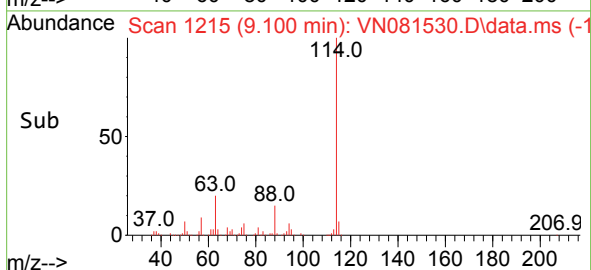

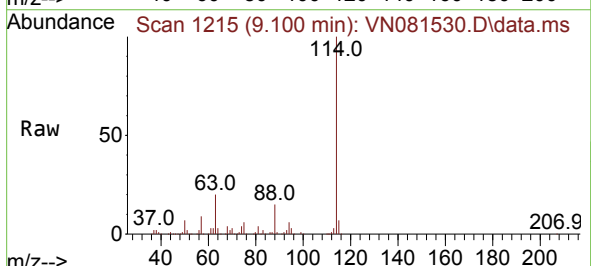


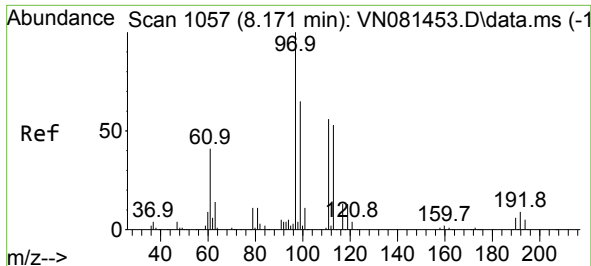

#35
 Dibromofluoromethane
 Concen: 49.230 ug/l
 RT: 8.165 min Scan# 1056
 Delta R.T. -0.006 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23




Instrument :
 MSVOA_N
 ClientSampleId :
 S-13


Tgt Ion:113 Resp: 238678
 Ion Ratio Lower Upper
 113 100
 111 102.3 82.2 123.4
 192 16.4 12.5 18.7

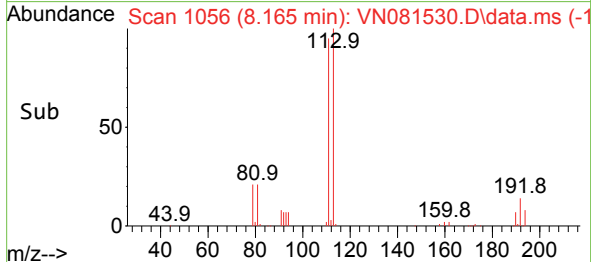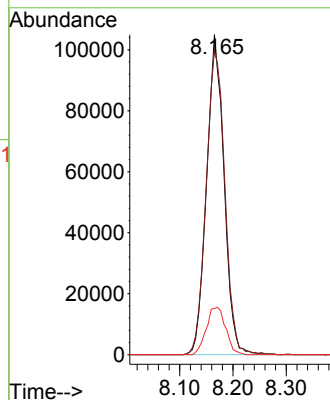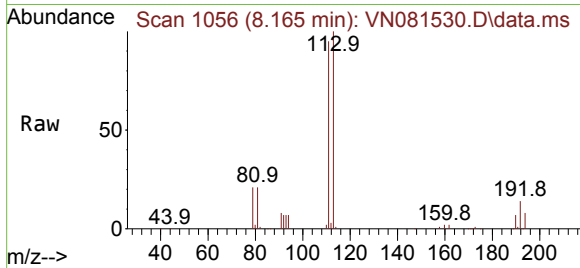

#36
 1,1-Dichloropropene
 Concen: 4.303 ug/l
 RT: 8.224 min Scan# 1066
 Delta R.T. -0.147 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23

Tgt Ion: 75 Resp: 35108
 Ion Ratio Lower Upper
 75 100
 110 9.7 16.0 48.0#
 77 0.0 25.8 38.6#

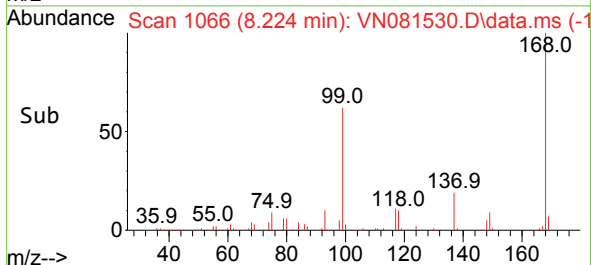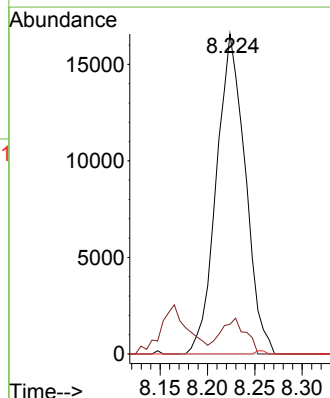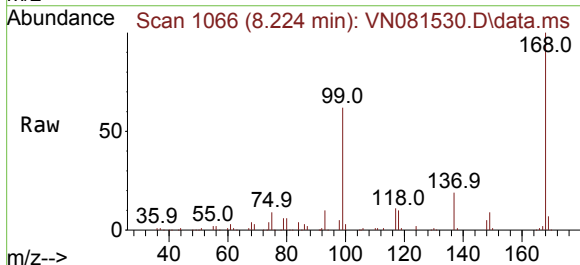



#38

Carbon Tetrachloride

Concen: 5.113 ug/l

RT: 8.224 min Scan# 1

Delta R.T. -0.141 min

Lab File: VN081530.D

Acq: 21 Mar 2024 19:23

Instrument :

MSVOA_N

ClientSampleId :

S-13





Tgt Ion:117 Resp: 45700

Ion Ratio Lower Upper

117 100

119 5.0 73.4 110.2#

121 0.0 24.4 36.6#

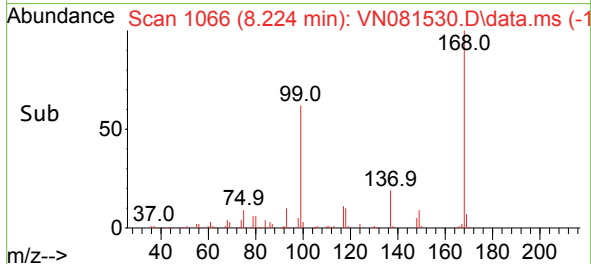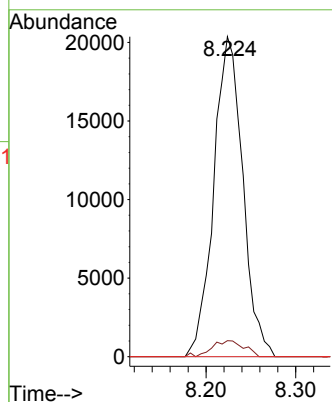

#39

Methylcyclohexane

Concen: 0.312 ug/l

RT: 9.594 min Scan# 1299

Delta R.T. -0.006 min

Lab File: VN081530.D

Acq: 21 Mar 2024 19:23




Tgt Ion: 83 Resp: 2847


Ion Ratio Lower Upper

83 100

55 62.9 65.7 98.5#

98 37.2 33.8 50.6


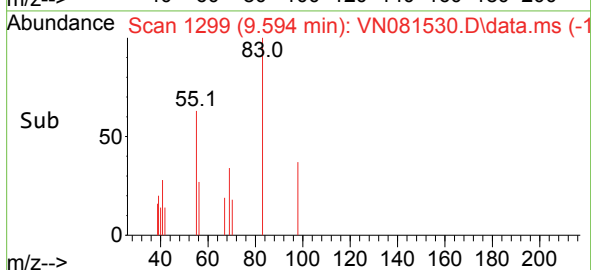

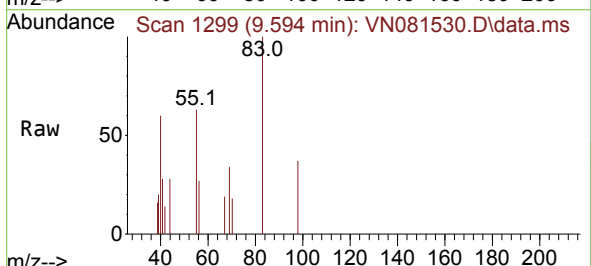


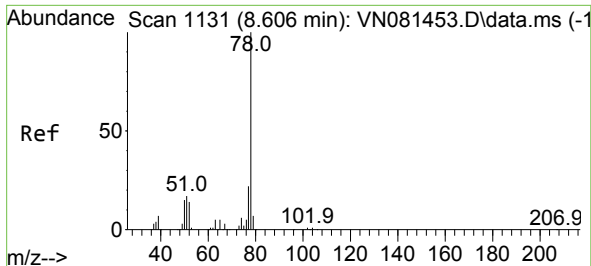

#40
Benzene
Concen: 122.043 ug/l
RT: 8.606 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23




Instrument :
MSVOA_N
ClientSampleId :
S-13


Tgt Ion: 78 Resp: 2911114
Ion Ratio Lower Upper
78 100
77 23.4 20.4 30.6

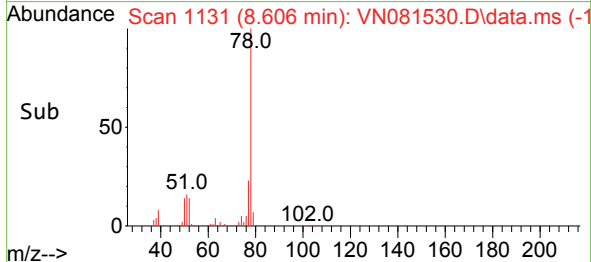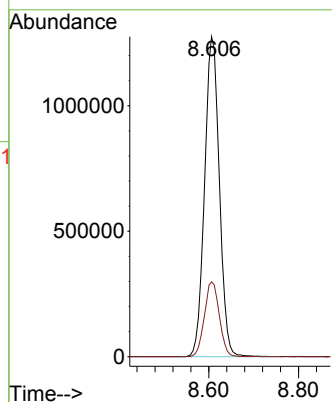

#43
Isopropyl Acetate
Concen: 1.370 ug/l
RT: 8.688 min Scan# 1145
Delta R.T. 0.000 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23

Tgt Ion: 43 Resp: 15868
Ion Ratio Lower Upper
43 100
61 18.0 19.9 29.9#
87 9.0 9.0 13.6#


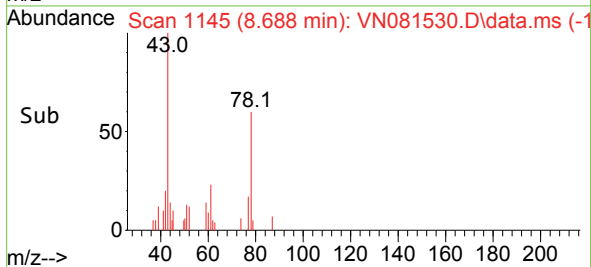

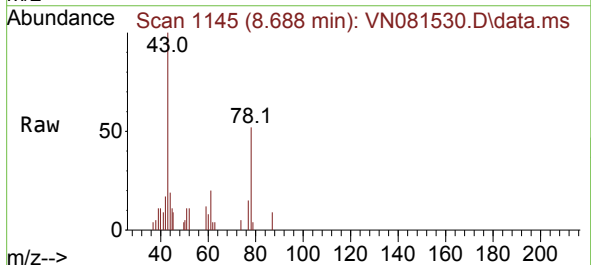




#50
Toluene-d8
Concen: 53.095 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23




Instrument :
MSVOA_N
ClientSampleId :
S-13


Tgt Ion: 98 Resp: 930516
Ion Ratio Lower Upper
98 100
100 64.9 51.4 77.0

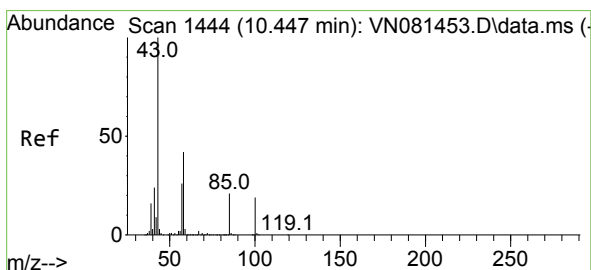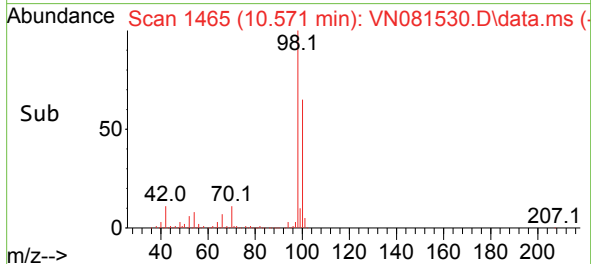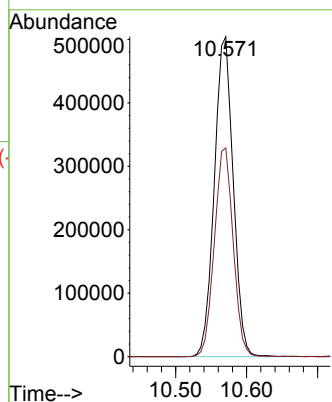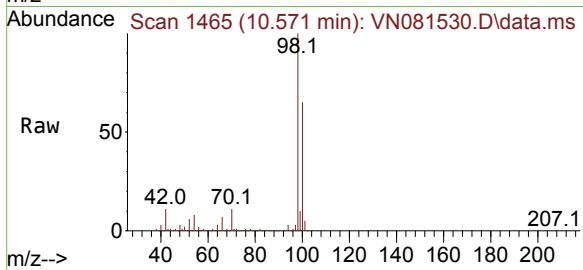

#51
4-Methyl-2-Pentanone
Concen: 0.204 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23

Tgt Ion: 43 Resp: 1442
Ion Ratio Lower Upper
43 100
58 26.8 29.4 44.0#

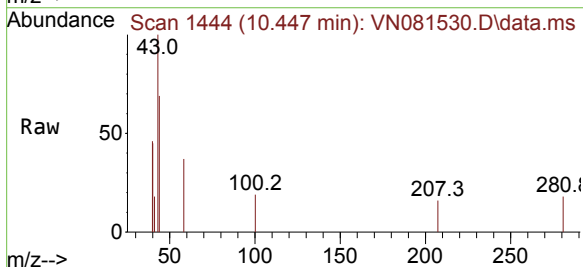

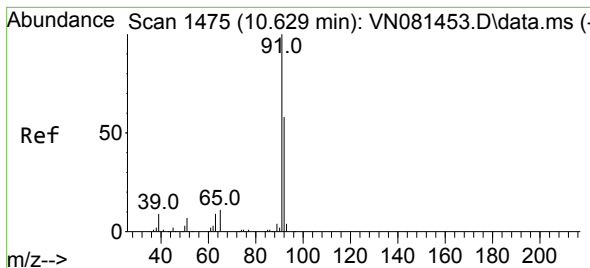

#52

Toluene

Concen: 70.568 ug/l

RT: 10.630 min Scan# 1475

Delta R.T. 0.000 min

Lab File: VN081530.D

Acq: 21 Mar 2024 19:23

Instrument :

MSVOA_N

ClientSampleId :





S-13

Tgt Ion: 92 Resp: 1069876

Ion Ratio Lower Upper

92 100

91 174.8 139.4 209.0

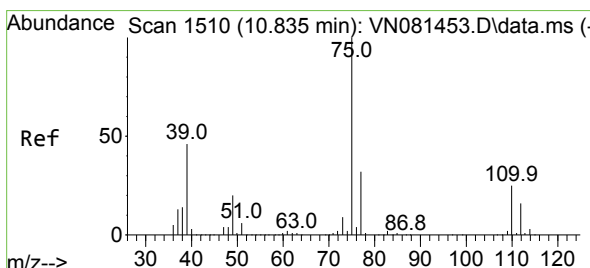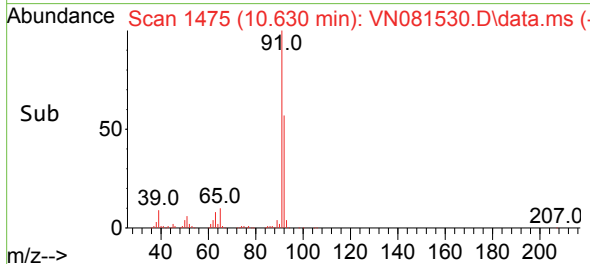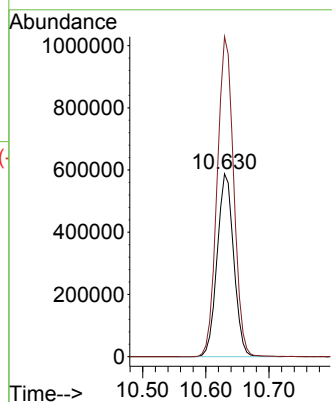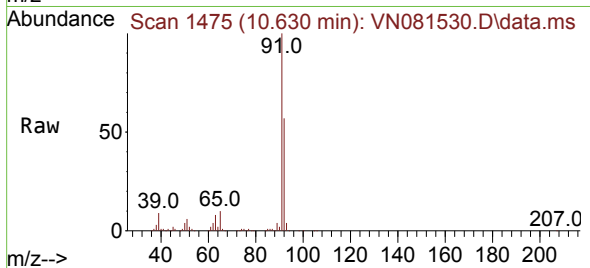

#53

t-1,3-Dichloropropene

Concen: 1.405 ug/l

RT: 10.635 min Scan# 1476

Delta R.T. -0.200 min

Lab File: VN081530.D




Acq: 21 Mar 2024 19:23


Tgt Ion: 75 Resp: 13026

Ion Ratio Lower Upper

75 100

77 134.0 25.5 38.3#


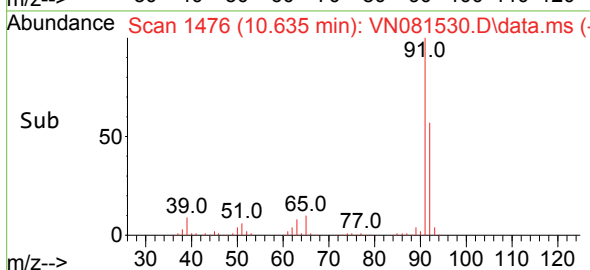

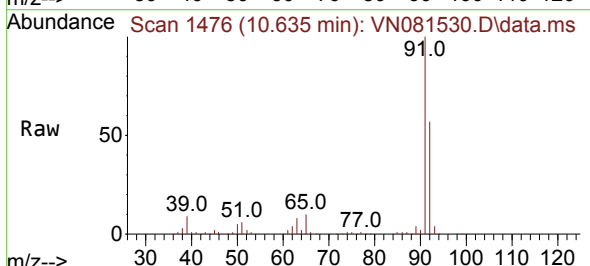


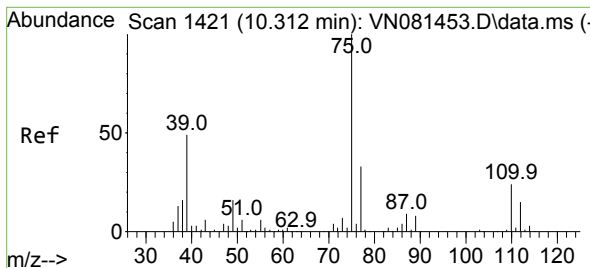

#54
cis-1,3-Dichloropropene
Concen: 0.366 ug/l
RT: 10.359 min Scan# 1429
Delta R.T. 0.047 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23




Instrument :
MSVOA_N
ClientSampleId :
S-13


Tgt Ion: 75 Resp: 3635
Ion Ratio Lower Upper
75 100
77 0.0 23.3 34.9#
39 86.1 44.6 66.8#

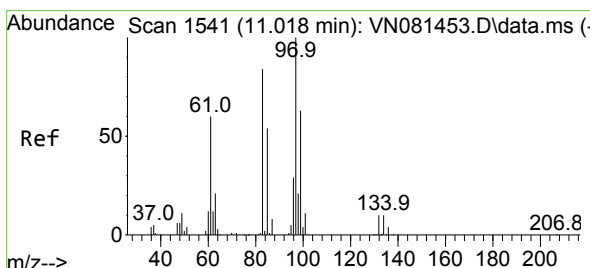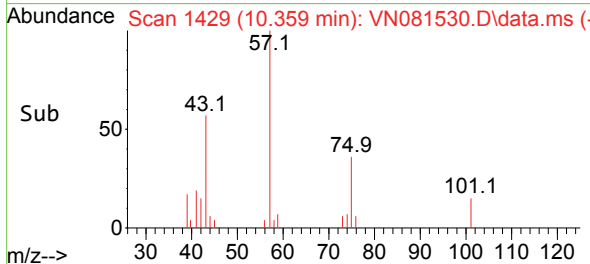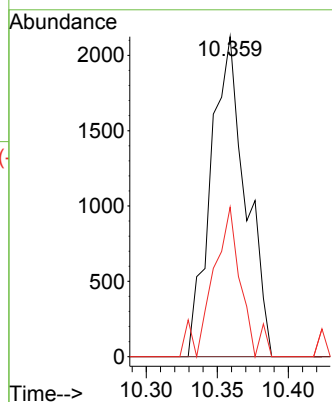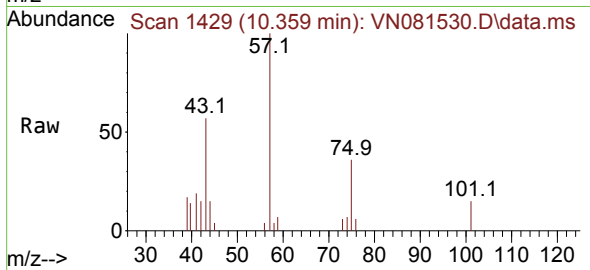

#55
1,1,2-Trichloroethane
Concen: 1.823 ug/l
RT: 10.888 min Scan# 1519
Delta R.T. -0.129 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23

Tgt Ion: 97 Resp: 11124
Ion Ratio Lower Upper
97 100
83 0.0 72.9 109.3#
85 0.0 50.2 75.2#
99 11.9 49.6 74.4#


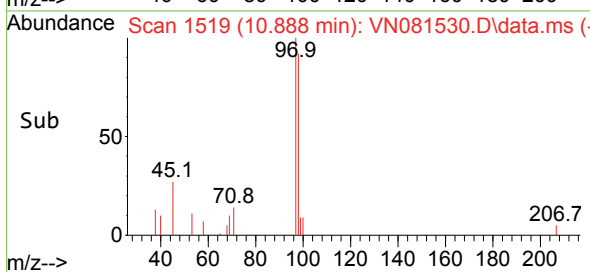

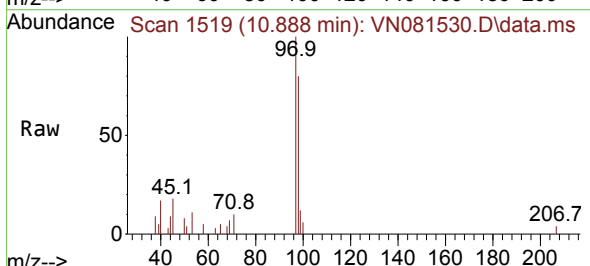


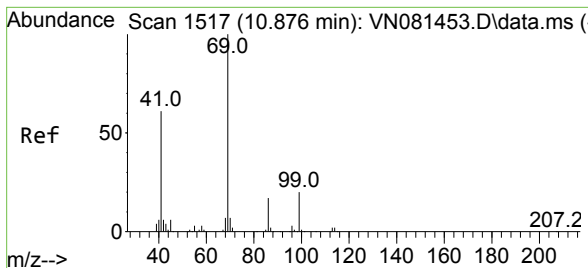

#56
Ethyl methacrylate
Concen: 0.654 ug/l
RT: 10.882 min Scan# 1518
Delta R.T. 0.006 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23




Instrument :
MSVOA_N
ClientSampleId :
S-13


Tgt Ion: 69 Resp: 689
Ion Ratio Lower Upper
69 100
41 0.0 61.0 91.6#
39 0.0 31.8 47.6#

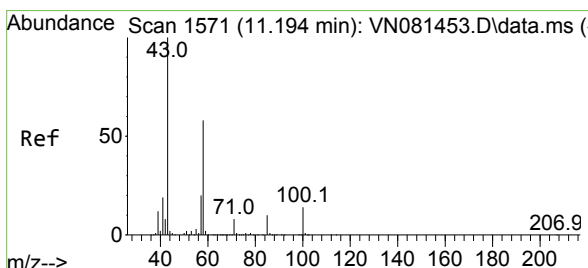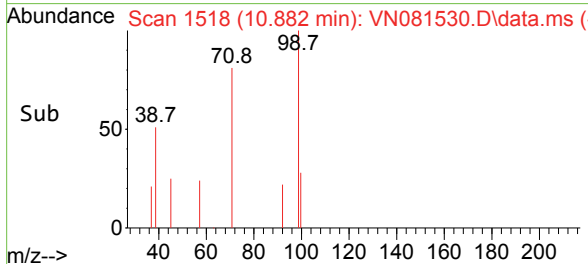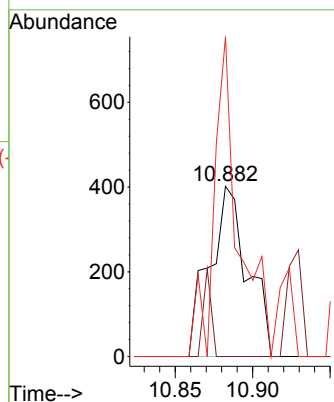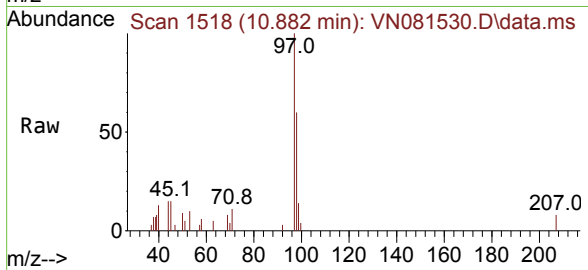

#59
2-Hexanone
Concen: 1.592 ug/l
RT: 11.171 min Scan# 1567
Delta R.T. -0.023 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23

Tgt Ion: 43 Resp: 8319
Ion Ratio Lower Upper
43 100
58 0.0 25.9 77.8#


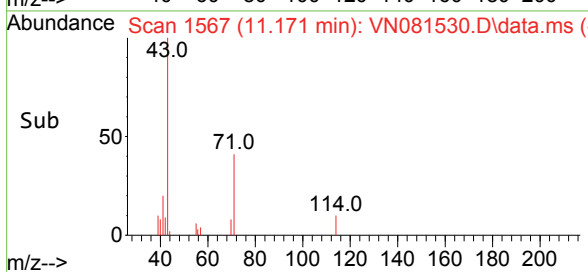
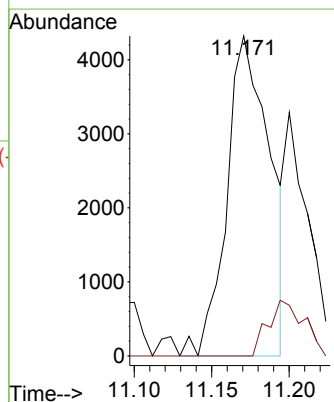
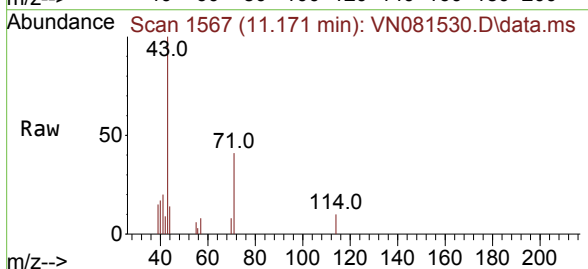


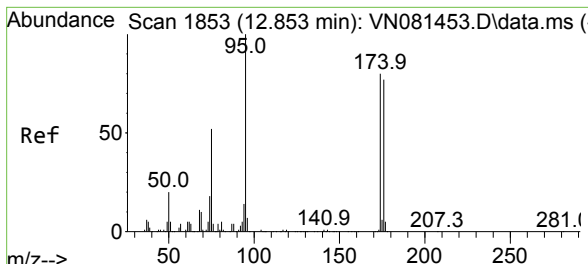

#62
 4-Bromofluorobenzene
 Concen: 50.235 ug/l
 RT: 12.847 min Scan# 1852
 Delta R.T. -0.006 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23




Instrument :
 MSVOA_N
 ClientSampleId :
 S-13


Tgt Ion:	95	Resp:	310221
Ion	Ratio	Lower	Upper
95	100		
174	76.9	0.0	120.4
176	72.5	0.0	121.0

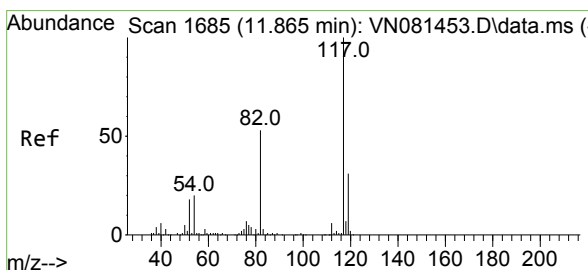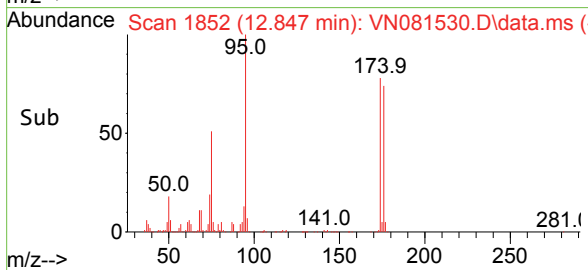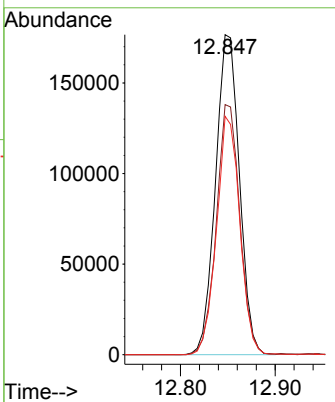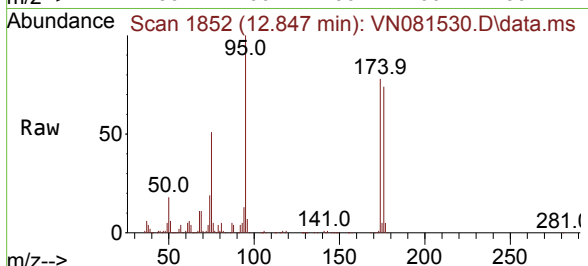

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 11.865 min Scan# 1685
 Delta R.T. 0.000 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23

Tgt Ion:	117	Resp:	723289
Ion	Ratio	Lower	Upper
117	100		
82	53.8	52.7	79.1
119	32.2	25.3	37.9


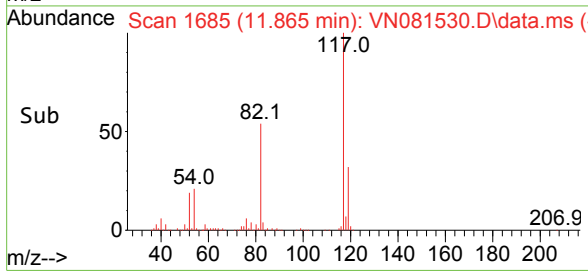
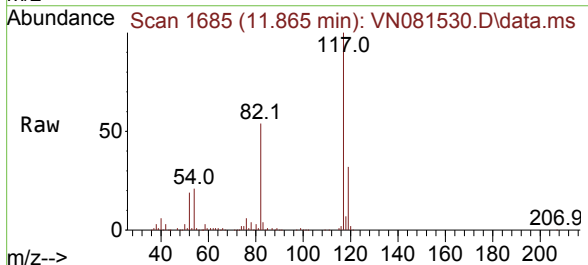
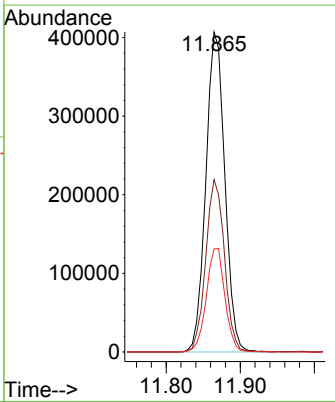


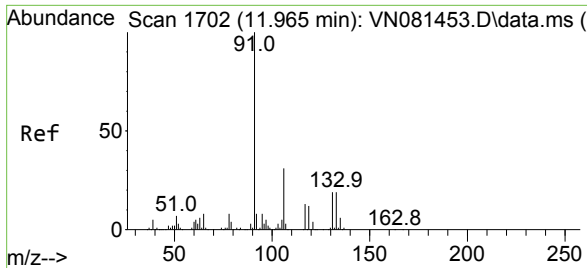

#67
Ethyl Benzene
Concen: 3.159 ug/l
RT: 11.965 min Scan# 1702
Delta R.T. 0.000 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23




Instrument :
MSVOA_N
ClientSampleId :
S-13


Tgt Ion: 91 Resp: 93823
Ion Ratio Lower Upper
91 100
106 32.1 23.8 35.6

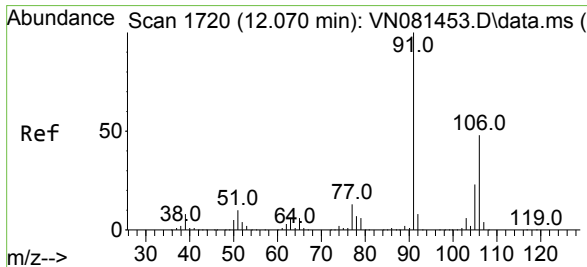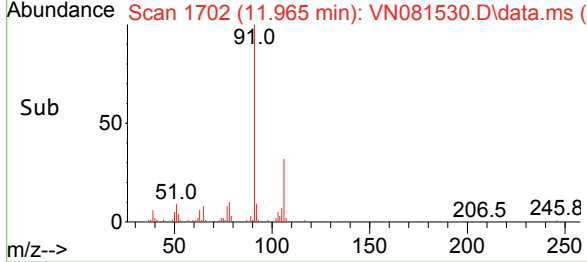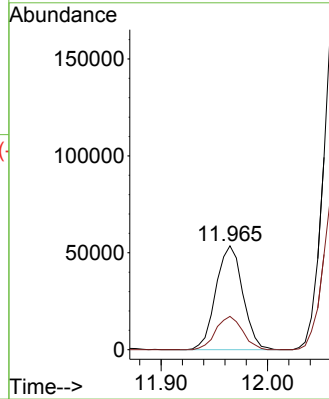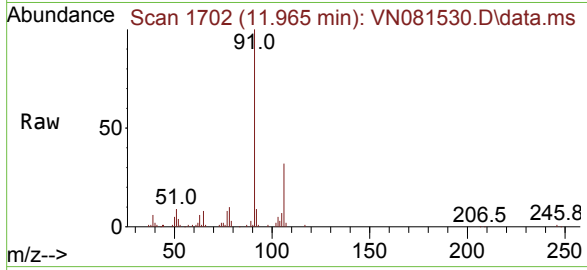

#68
m/p-Xylenes
Concen: 17.480 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. 0.000 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23

Tgt Ion:106 Resp: 194635
Ion Ratio Lower Upper
106 100
91 201.5 169.0 253.6


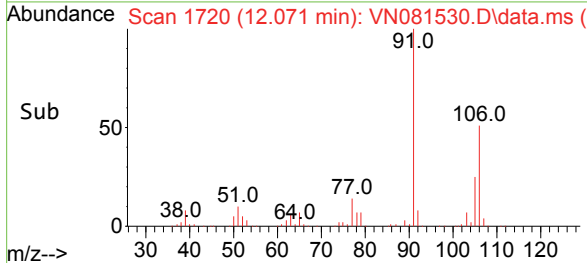
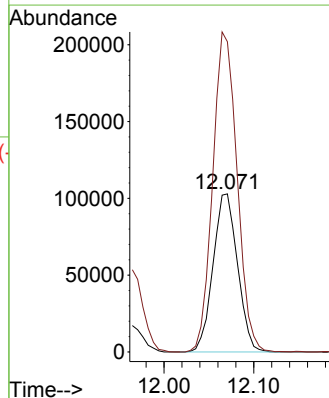
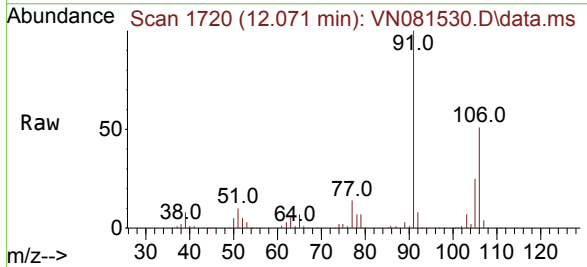


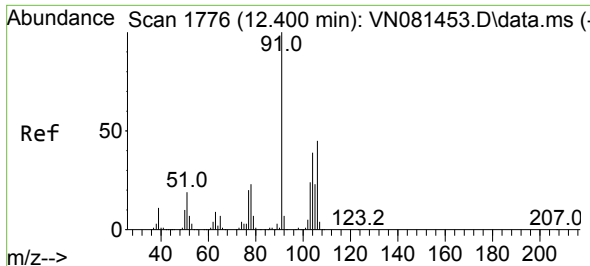

#69
o-Xylene
Concen: 11.279 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. 0.000 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23




Instrument :
MSVOA_N
ClientSampleId :
S-13


Tgt Ion:106 Resp: 123296
Ion Ratio Lower Upper
106 100
91 210.2 112.1 336.3

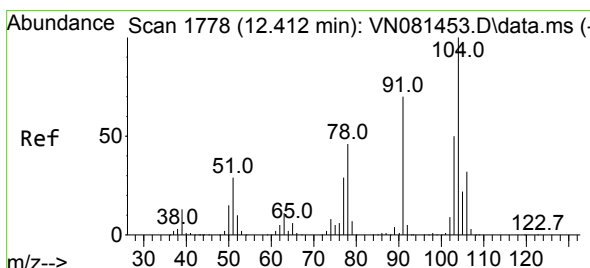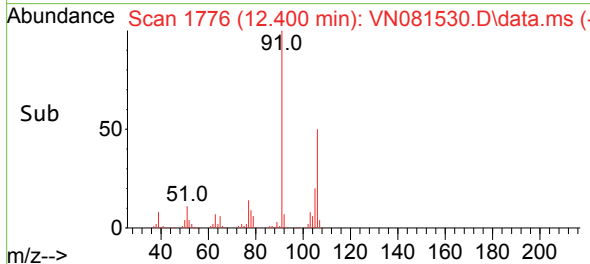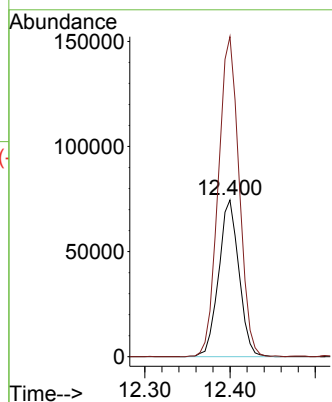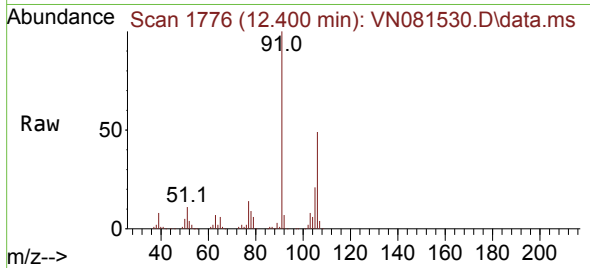

#70
Styrene
Concen: 1.161 ug/l
RT: 12.412 min Scan# 1778
Delta R.T. 0.000 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23

Tgt Ion:104 Resp: 20472
Ion Ratio Lower Upper
104 100
78 122.8 43.8 65.8#
103 113.9 44.2 66.2#


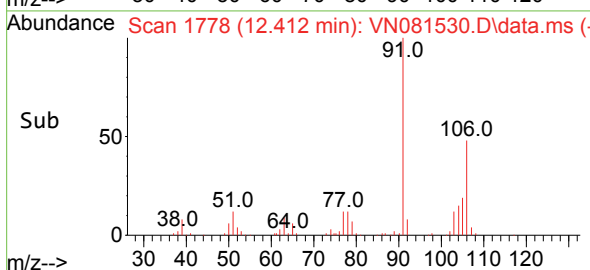

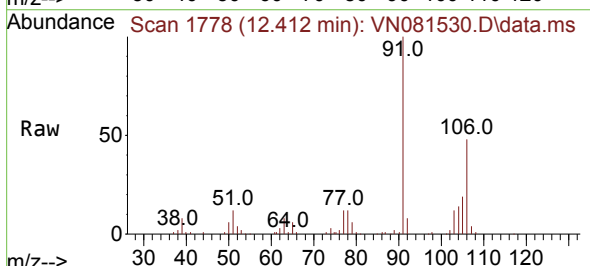


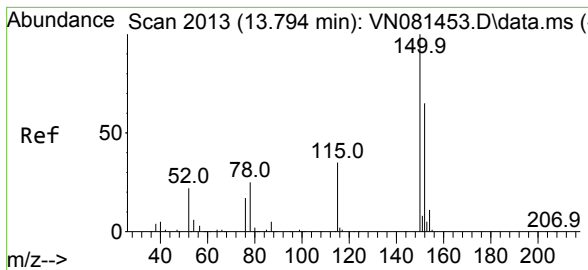

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 2013
 Delta R.T. 0.000 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23




Instrument :
 MSVOA_N
 ClientSampleId :
 S-13


Tgt Ion:152 Resp: 305161
 Ion Ratio Lower Upper
 152 100
 115 63.3 32.3 96.8
 150 162.2 0.0 339.8

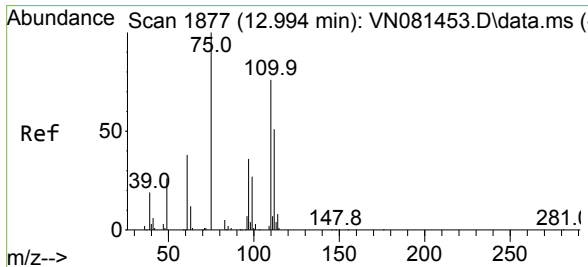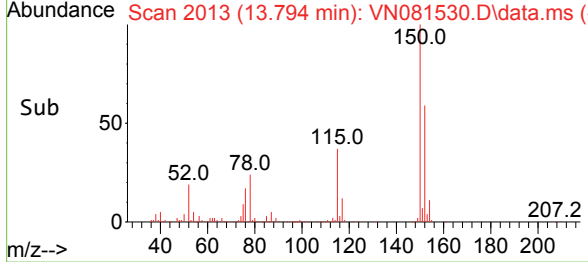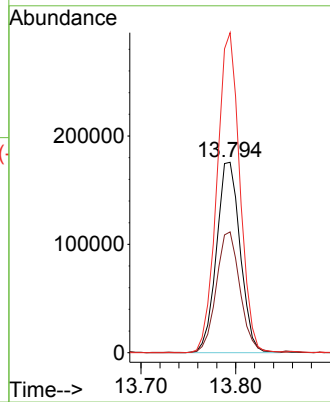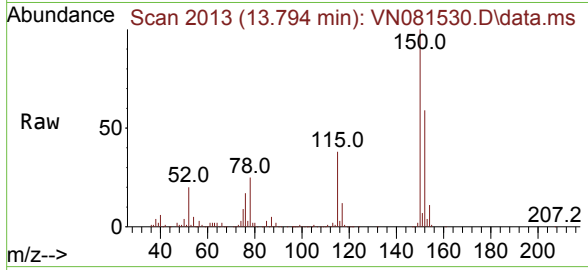

#76
 1,2,3-Trichloropropane
 Concen: 22.368 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.141 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23

Tgt Ion: 75 Resp: 163280
 Ion Ratio Lower Upper
 75 100
 77 1.5 91.0 272.8#


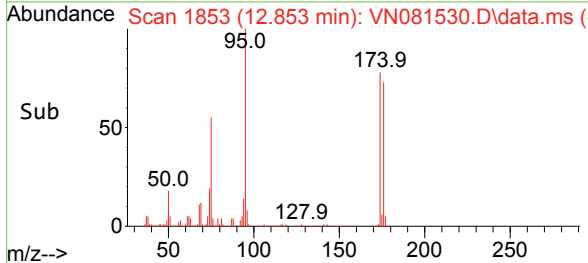
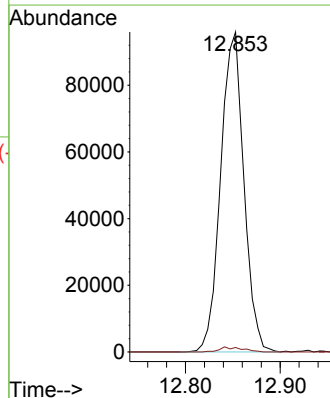
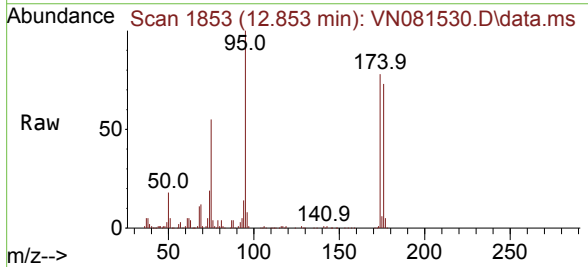


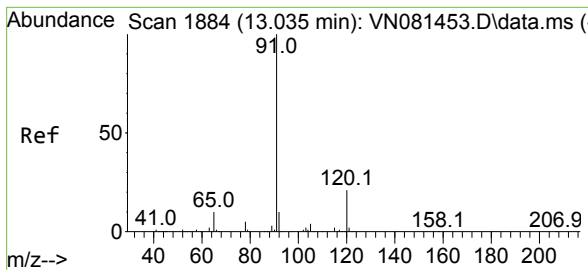

#78
 n-propylbenzene
 Concen: 0.274 ug/l
 RT: 13.035 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23




Instrument :
 MSVOA_N
 ClientSampleId :
 S-13


Tgt Ion: 91 Resp: 8410
 Ion Ratio Lower Upper
 91 100
 120 20.2 10.3 30.9

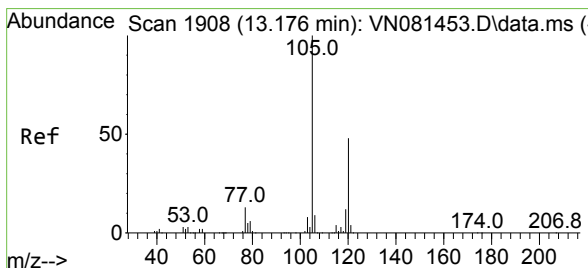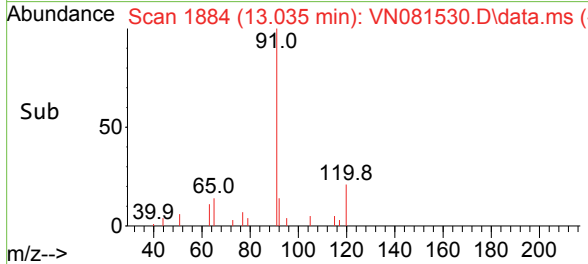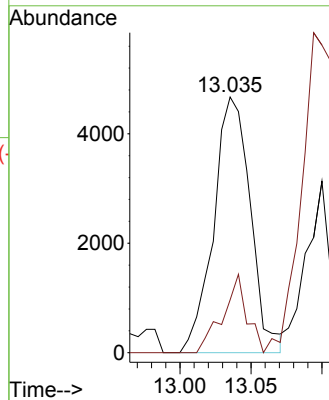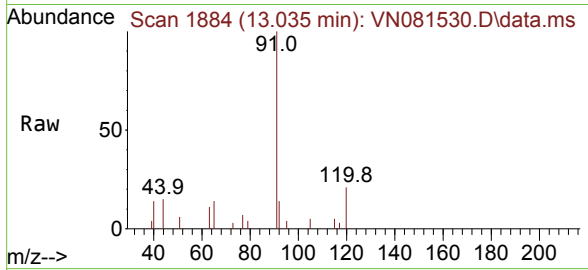

#80
 1,3,5-Trimethylbenzene
 Concen: 1.670 ug/l
 RT: 13.176 min Scan# 1908
 Delta R.T. 0.000 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23

Tgt Ion: 105 Resp: 35882
 Ion Ratio Lower Upper
 105 100
 120 50.6 23.0 69.0


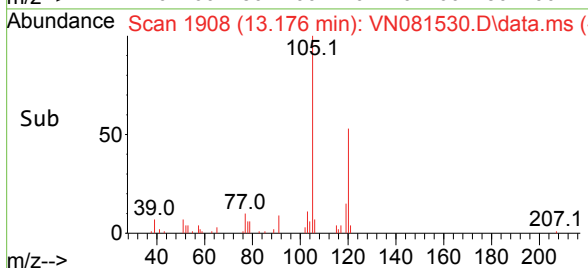
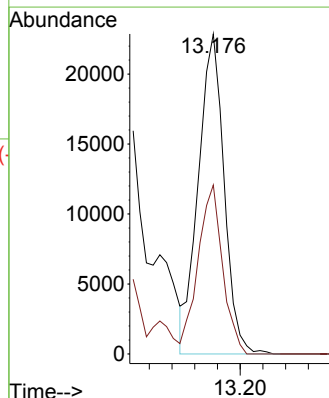
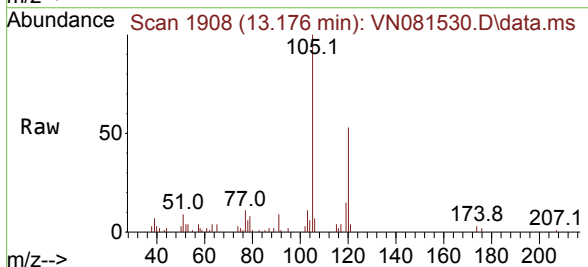


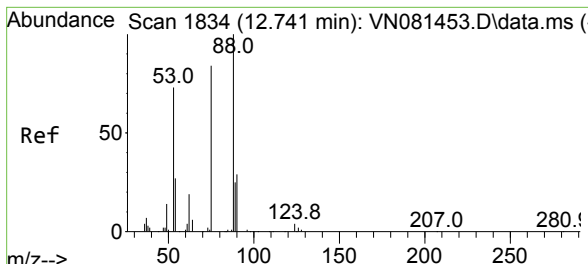

#81
 trans-1,4-Dichloro-2-butene
 Concen: 60.447 ug/l
 RT: 12.853 min Scan# 11
 Delta R.T. 0.112 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23




Instrument :
 MSVOA_N
 ClientSampleId :
 S-13


Tgt Ion:	75	Resp:	163280
Ion Ratio	Lower	Upper	
75	100		
53	0.6	71.4	107.2#
89	0.1	33.4	50.0#

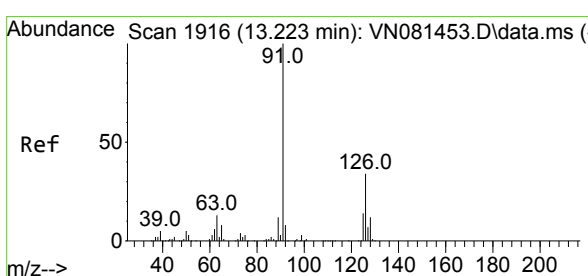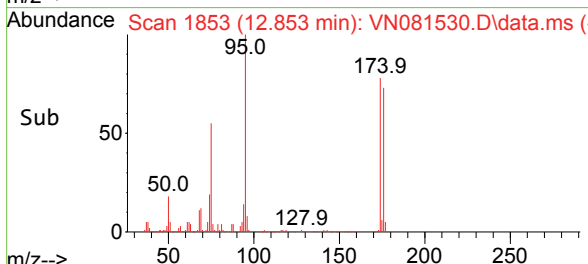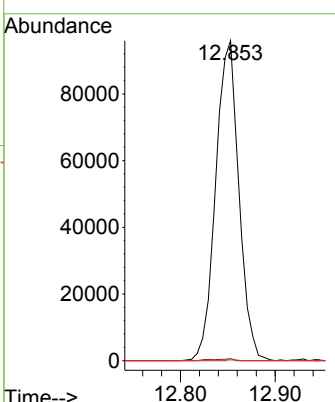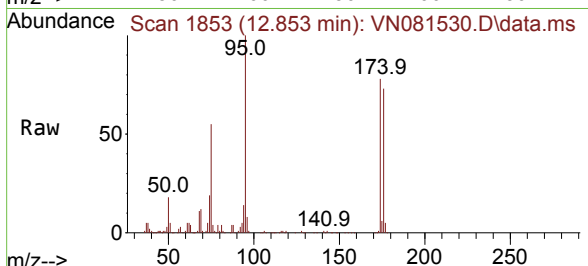

#82
 4-Chlorotoluene
 Concen: 0.230 ug/l
 RT: 13.171 min Scan# 1907
 Delta R.T. -0.053 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23

Tgt Ion:	91	Resp:	4171
Ion Ratio	Lower	Upper	
91	100		
126	0.0	15.3	45.9#


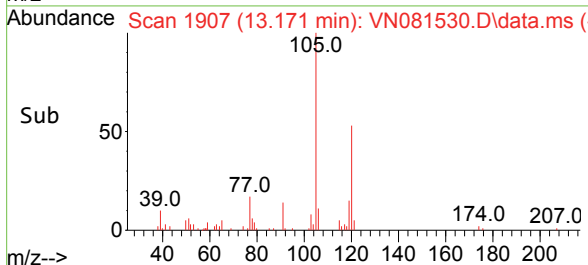
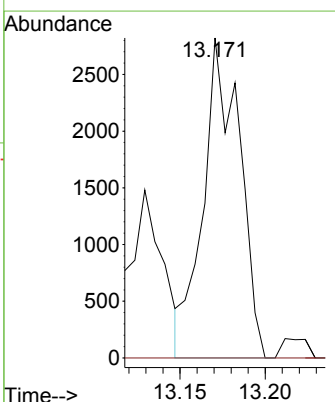
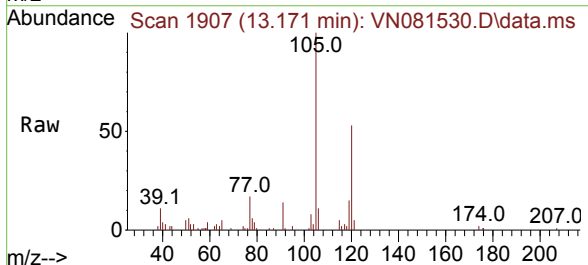


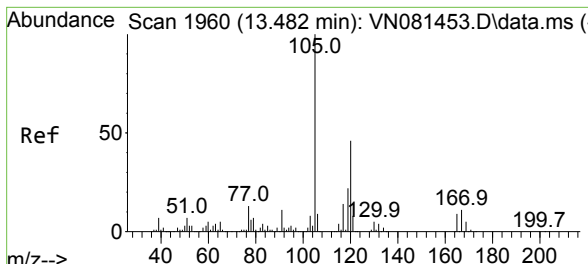

#84
 1,2,4-Trimethylbenzene
 Concen: 4.697 ug/l
 RT: 13.482 min Scan# 1960
 Delta R.T. 0.000 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23




Instrument :
 MSVOA_N
 ClientSampleId :
 S-13


Tgt Ion:105 Resp: 101433
 Ion Ratio Lower Upper
 105 100
 120 40.8 20.9 62.7

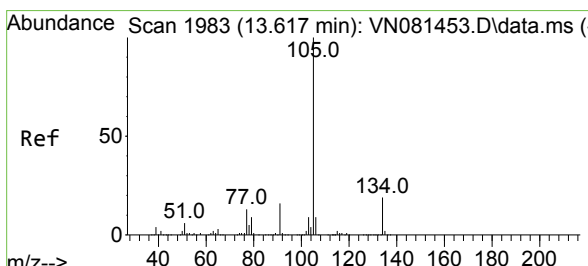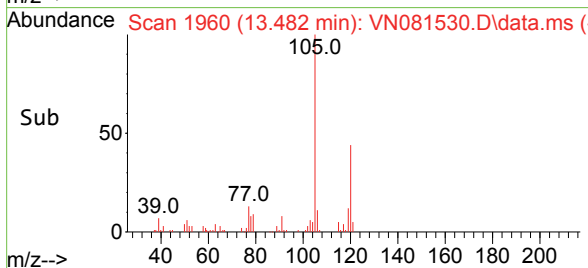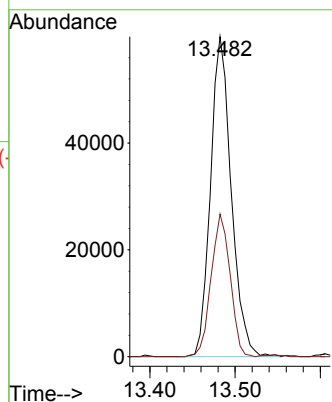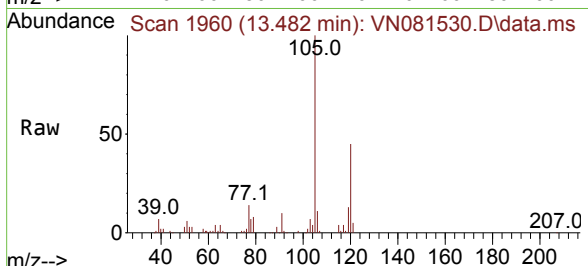

#85
 sec-Butylbenzene
 Concen: 3.830 ug/l
 RT: 13.482 min Scan# 1960
 Delta R.T. -0.135 min
 Lab File: VN081530.D
 Acq: 21 Mar 2024 19:23


Tgt Ion:105 Resp: 101433
 Ion Ratio Lower Upper
 105 100
 134 0.0 8.6 25.8#

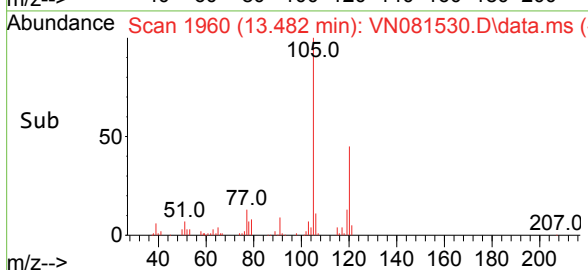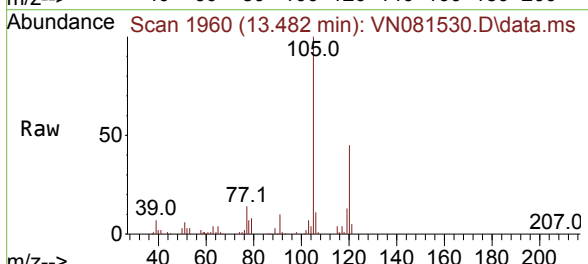

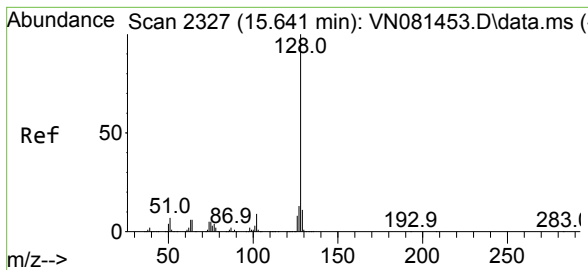

#95
Naphthalene
Concen: 79.593 ug/l
RT: 15.641 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN081530.D
Acq: 21 Mar 2024 19:23

Instrument :
MSVOA_N
ClientSampleId :
S-13

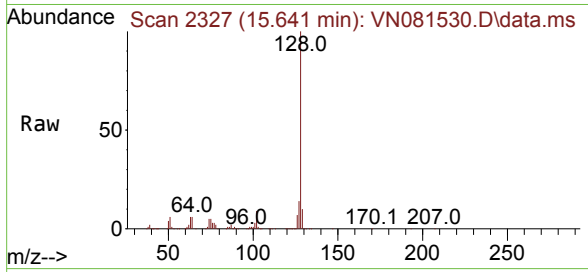

Tgt Ion:128 Resp: 1694522
Ion Ratio Lower Upper
128 100
127 13.2 10.0 15.0
129 10.7 8.7 13.1

