
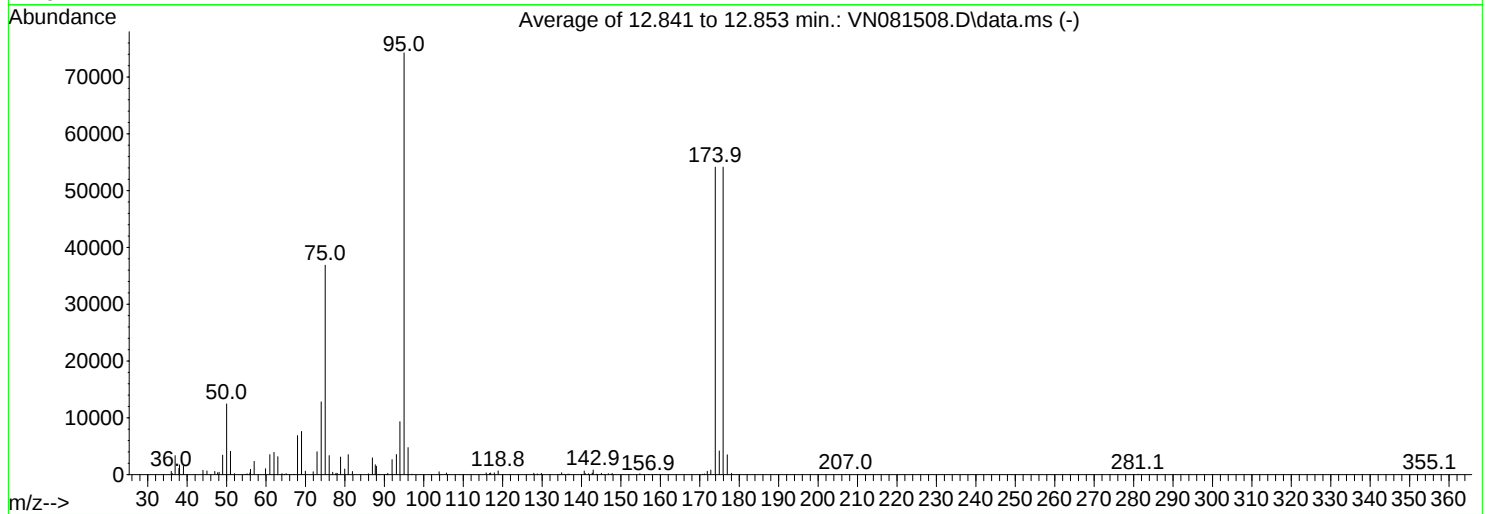


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032124\
Data File : VN081508.D
Acq On : 21 Mar 2024 08:29
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

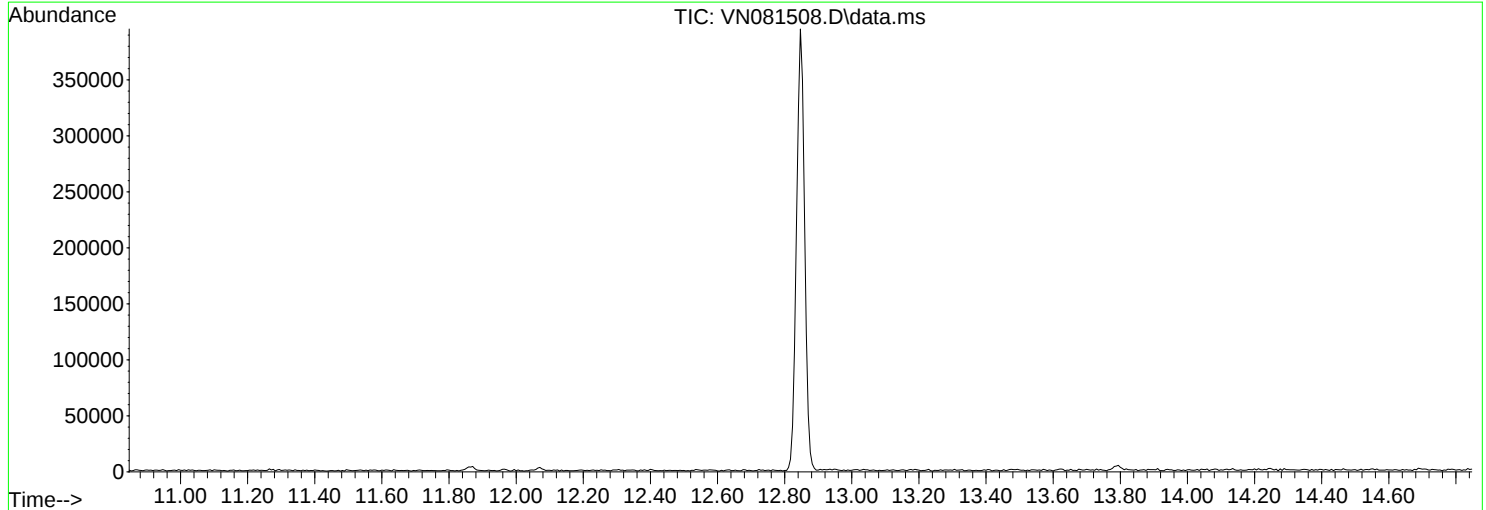

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	12466	PASS
75	95	30	60	49.6	36869	PASS
95	95	100	100	100.0	74259	PASS
96	95	5	9	6.4	4768	PASS
173	174	0.00	2	1.5	819	PASS
174	95	50	100	72.9	54141	PASS
175	174	5	9	7.7	4178	PASS
176	174	95	101	100.0	54133	PASS
177	176	5	9	6.5	3504	PASS

Average of 12.841 to 12.853 min.: VN081508.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	602	48.10	431	60.95	3522	72.95	403
36.20	212	49.00	3443	62.00	3906	74.00	1282
36.95	3364	50.00	12466	63.00	3154	75.00	3686
37.90	1093	51.00	4107	64.05	161	76.00	335
38.05	1709	52.00	156	64.70	63	76.90	419
39.05	1497	54.70	58	65.10	183	77.60	97
39.95	53	55.20	149	67.10	52	77.75	258
44.00	750	55.90	295	68.00	6877	78.10	196
45.00	636	56.05	928	69.00	7601	78.90	3106
47.00	563	57.00	2340	69.95	613	79.95	995
47.75	343	59.85	1050	71.95	503	80.85	3539

Average of 12.841 to 12.853 min.: VN081508.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	565	95.00	74259	128.80	139	142.70	291
85.95	140	96.00	4768	129.80	219	142.95	821
86.95	2957	97.00	98	134.50	57	143.80	72
87.70	1761	103.90	513	134.95	332	145.05	236
88.00	1482	105.75	287	135.60	56	145.90	55
88.70	63	115.80	301	136.60	125	146.80	176
90.70	54	116.70	237	137.00	57	147.60	75
90.85	227	116.95	288	139.90	51	147.80	187
91.95	2656	117.90	323	140.70	656	154.80	167
93.05	3544	118.85	662	141.00	170	156.90	54
93.95	9330	127.90	268	141.80	158	158.90	51

Average of 12.841 to 12.853 min.: VN081508.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.70	57	355.10	68				
171.20	116						
171.90	597						
172.80	819						
173.90	54141						
174.95	4178						
175.90	54133						
176.95	3504						
178.05	217						
207.00	68						
281.10	88						

Instrument :

MSVOA_N

ClientSampleId :

BFB