

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032125\
 Data File : VN086056.D
 Acq On : 21 Mar 2025 21:42
 Operator : JC\MD
 Sample : Q1606-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 CHRT24743

Quant Time: Mar 21 23:06:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 19 03:20:56 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	141153	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	272815	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	264858	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	97851	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	113088	58.508	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 117.020%	
35) Dibromofluoromethane	8.165	113	95919	50.372	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.740%	
50) Toluene-d8	10.565	98	354788	51.337	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.680%	
62) 4-Bromofluorobenzene	12.847	95	102182	41.459	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 82.920%	
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	5.530	59	224	0.819	ug/l #	73
16) Acetone	4.430	43	26979	45.688	ug/l	95
18) Methyl Acetate	5.030	43	2376	1.626	ug/l #	53
20) Methylene Chloride	5.277	84	9403	5.443	ug/l #	84
25) 2-Butanone	7.489	43	4491	5.271	ug/l	91
30) Chloroform	7.959	83	722	0.231	ug/l	94
31) Cyclohexane	8.218	56	3097	1.286	ug/l #	1
36) 1,1-Dichloropropene	8.224	75	11225	4.477	ug/l #	51
37) Ethyl Acetate	7.565	43	1745	0.825	ug/l #	64
38) Carbon Tetrachloride	8.224	117	15139	4.592	ug/l #	15
40) Benzene	8.606	78	171756	21.821	ug/l	98
43) Isopropyl Acetate	8.683	43	106792	23.298	ug/l #	78
45) 1,2-Dichloropropane	9.741	63	969	0.541	ug/l #	44
48) Methyl methacrylate	9.671	41	2059	1.361	ug/l #	7
51) 4-Methyl-2-Pentanone	10.441	43	6721	3.325	ug/l #	64
52) Toluene	10.630	92	12147	2.514	ug/l	94
53) t-1,3-Dichloropropene	10.724	75	598	0.209	ug/l #	43
54) cis-1,3-Dichloropropene	10.353	75	27112	8.992	ug/l #	70
56) Ethyl methacrylate	10.982	69	1516	0.839	ug/l #	1
57) 1,3-Dichloropropane	11.200	76	3546	1.132	ug/l #	42
59) 2-Hexanone	11.200	43	35111	23.841	ug/l #	53
67) Ethyl Benzene	11.959	91	6194	0.639	ug/l	98
68) m/p-Xylenes	12.065	106	2273	0.597	ug/l	100
69) o-Xylene	12.400	106	1116	0.319	ug/l	93
71) Bromoform	12.841	173	382	0.203	ug/l #	1
76) 1,2,3-Trichloropropane	12.847	75	51818	23.654	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	51818	62.536	ug/l #	16
89) n-Butylbenzene	13.988	91	1339	0.309	ug/l #	33
90) Hexachloroethane	14.441	117	974	0.792	ug/l #	10
95) Naphthalene	15.641	128	6777	1.394	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032125\
Data File : VN086056.D
Acq On : 21 Mar 2025 21:42
Operator : JC\MD
Sample : Q1606-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CHRT24743


Quant Time: Mar 21 23:06:24 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 19 03:20:56 2025
Response via : Initial Calibration

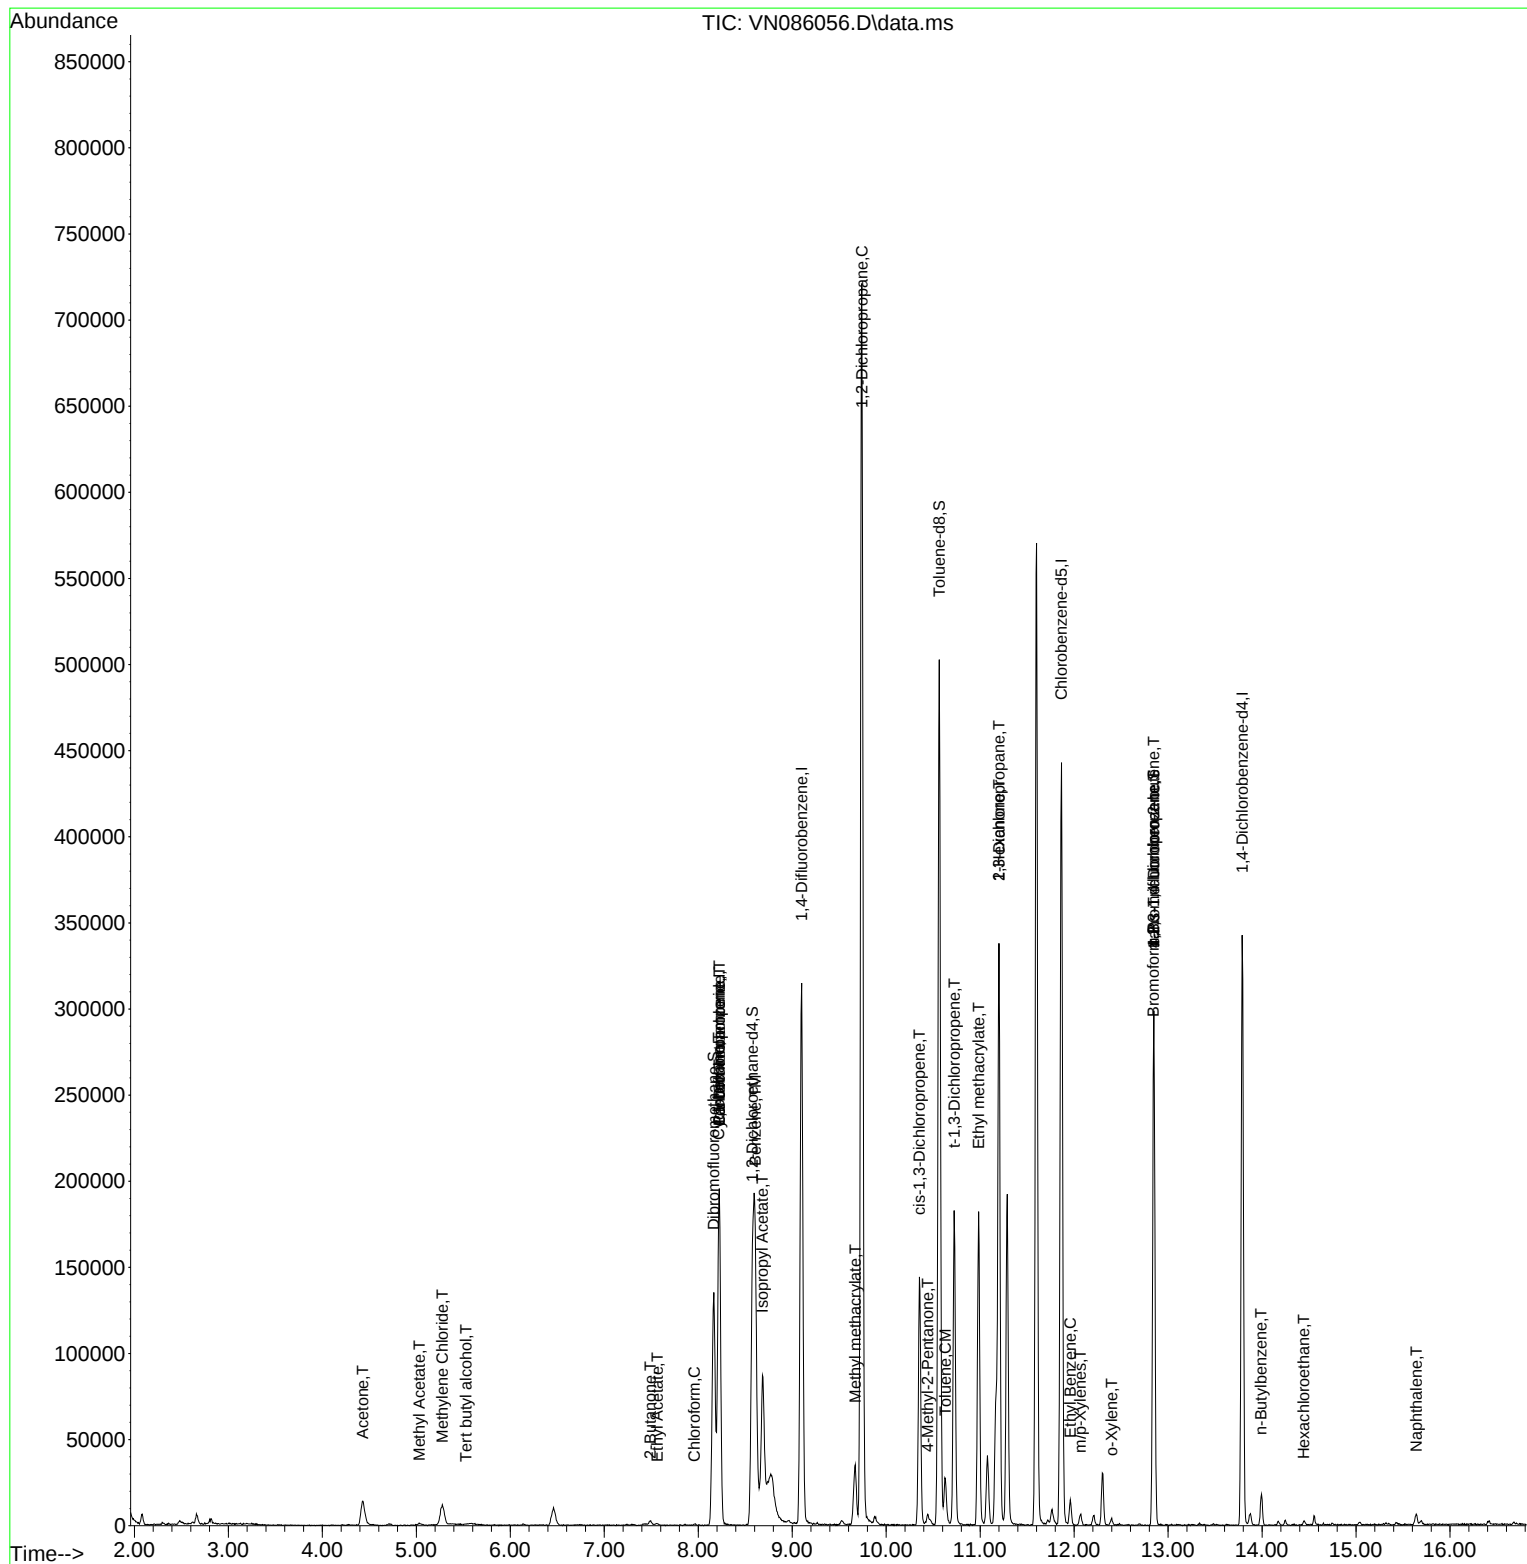






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Instrument :
MSVOA_N
ClientSampleId :
CHRT24743



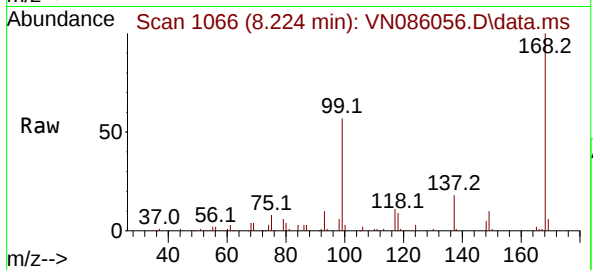



Tgt Ion:168 Resp: 141153
Ion Ratio Lower Upper
168 100
99 56.9 49.4 74.2

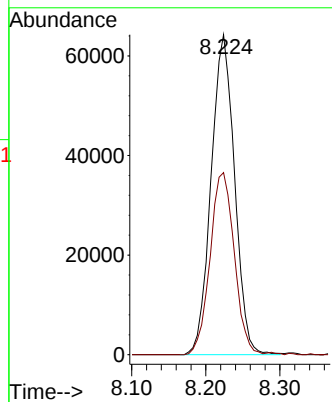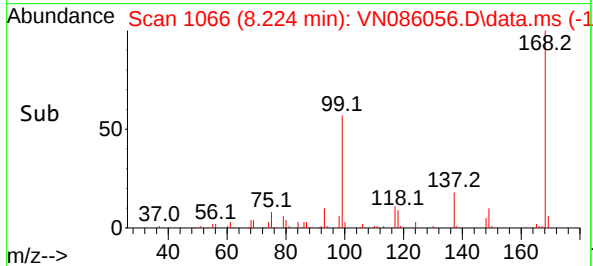

#11
Tert butyl alcohol
Concen: 0.819 ug/l
RT: 5.530 min Scan# 608
Delta R.T. 0.006 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Tgt Ion: 59 Resp: 224
Ion Ratio Lower Upper
59 100
57 0.0 7.9 11.9#



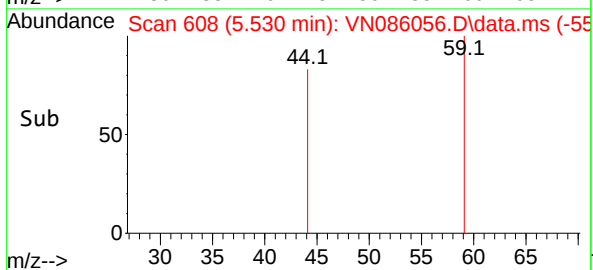
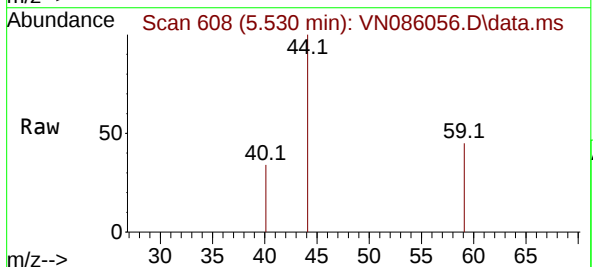




#16
Acetone
Concen: 45.688 ug/l
RT: 4.430 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42




Instrument :
MSVOA_N
ClientSampleId :
CHRT24743


Tgt Ion: 43 Resp: 26979
Ion Ratio Lower Upper
43 100
58 33.7 29.4 44.2

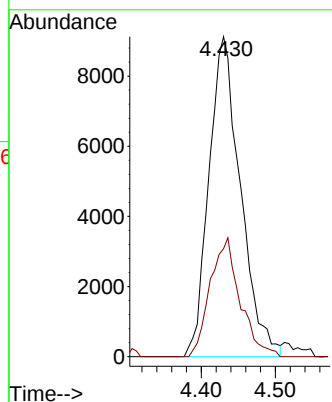

#18
Methyl Acetate
Concen: 1.626 ug/l
RT: 5.030 min Scan# 523
Delta R.T. 0.006 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Tgt Ion: 43 Resp: 2376
Ion Ratio Lower Upper
43 100
74 4.3 23.9 35.9#

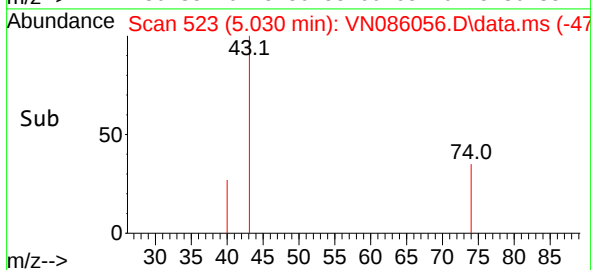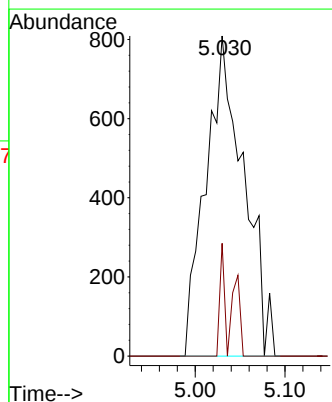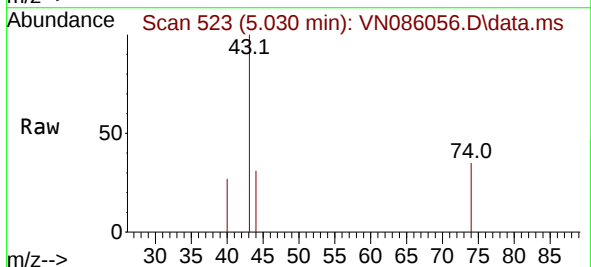

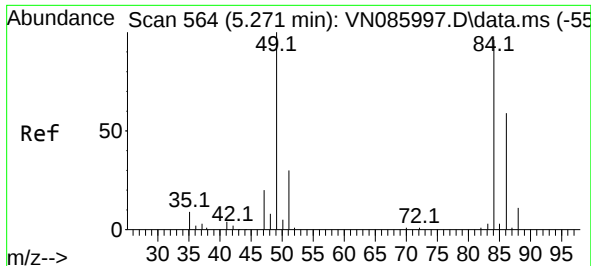

#20

Methylene Chloride

Concen: 5.443 ug/l

RT: 5.277 min Scan# 5

Delta R.T. 0.006 min

Lab File: VN086056.D

Acq: 21 Mar 2025 21:42

Instrument :

MSVOA_N

ClientSampleId :

CHRT24743

Tgt Ion: 84 Resp: 9403





Ion Ratio Lower Upper

84 100

49 131.3 83.3 124.9#

51 36.0 24.8 37.2

86 63.0 48.7 73.1



#25

2-Butanone

Concen: 5.271 ug/l

RT: 7.489 min Scan# 941

Delta R.T. 0.006 min

Lab File: VN086056.D




Acq: 21 Mar 2025 21:42


Tgt Ion: 43 Resp: 4491

Ion Ratio Lower Upper

43 100

72 29.2 27.4 41.0

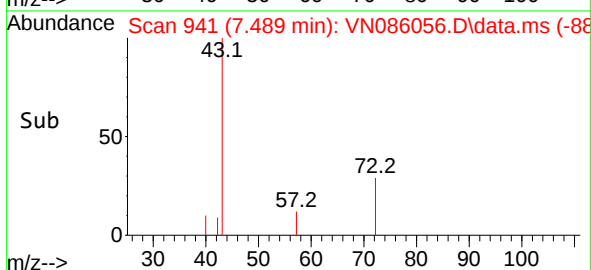

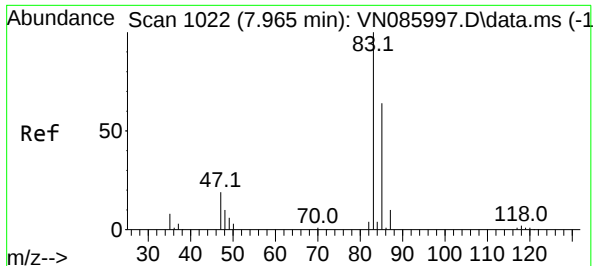

#30

Chloroform

Concen: 0.231 ug/l

RT: 7.959 min Scan# 1021

Delta R.T. -0.006 min

Lab File: VN086056.D

Acq: 21 Mar 2025 21:42

Instrument :

MSVOA_N

ClientSampleId :





CHRT24743

Tgt Ion: 83 Resp: 722

Ion Ratio Lower Upper

83 100

85 69.3 51.5 77.3

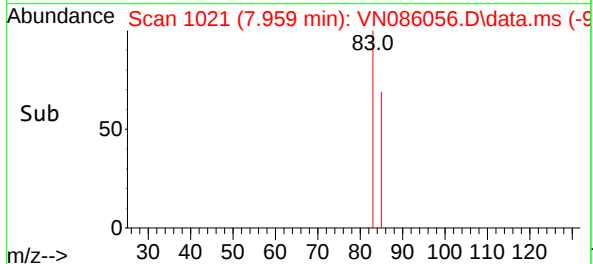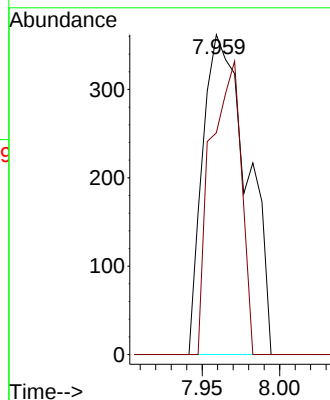

#31

Cyclohexane

Concen: 1.286 ug/l

RT: 8.218 min Scan# 1065

Delta R.T. -0.035 min

Lab File: VN086056.D

Acq: 21 Mar 2025 21:42




Tgt Ion: 56 Resp: 3097


Ion Ratio Lower Upper

56 100

69 204.6 28.0 42.0#

84 143.2 75.0 112.6#

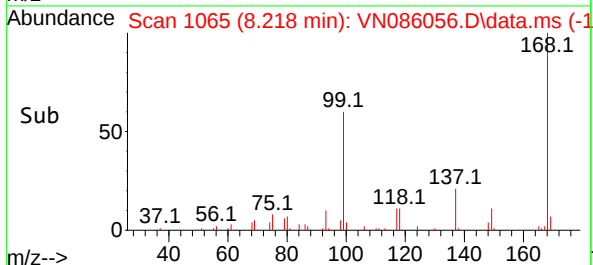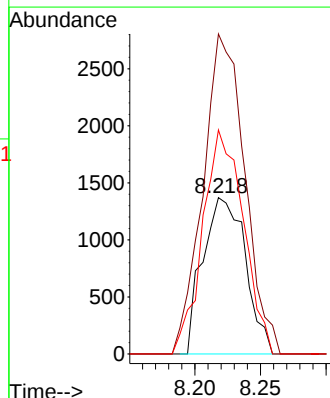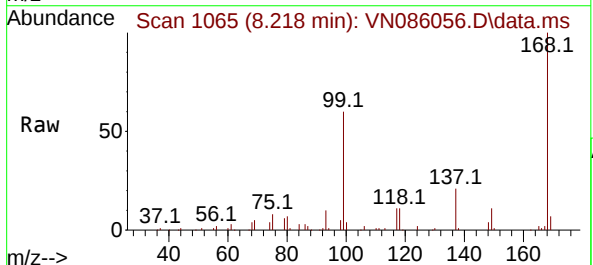

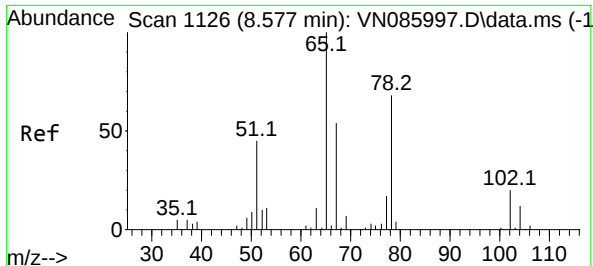

#33

1,2-Dichloroethane-d4

Concen: 58.508 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VN086056.D

Acq: 21 Mar 2025 21:42

Instrument :

MSVOA_N

ClientSampleId :





CHRT24743

Tgt Ion: 65 Resp: 113088

Ion Ratio Lower Upper

65 100

67 52.3 0.0 102.2

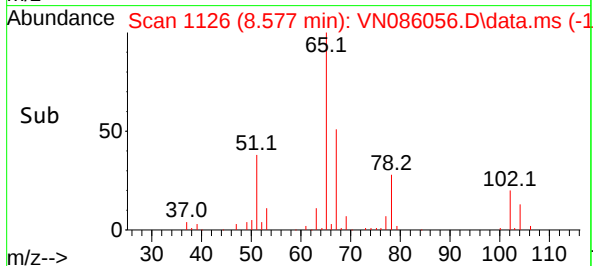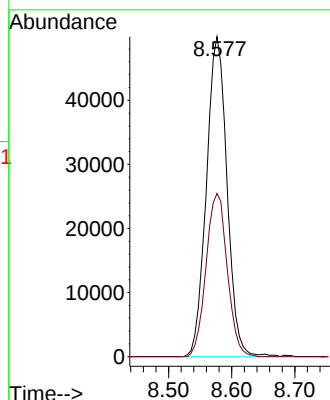

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. -0.000 min

Lab File: VN086056.D

Acq: 21 Mar 2025 21:42




Tgt Ion: 114 Resp: 272815


Ion Ratio Lower Upper

114 100

63 19.8 0.0 39.6


88 16.1 0.0 32.6

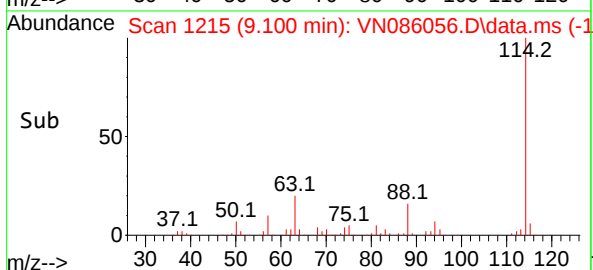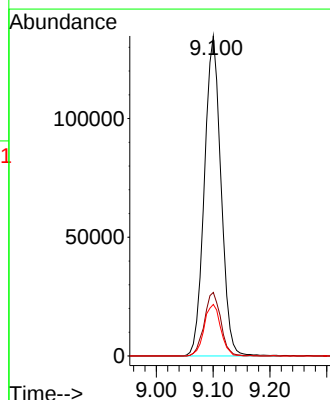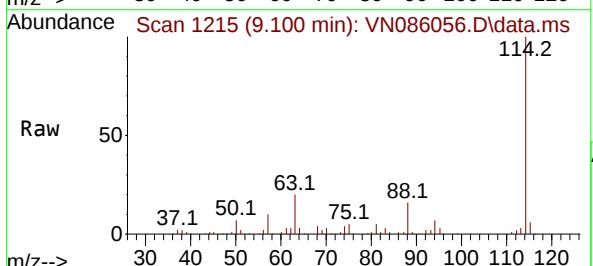



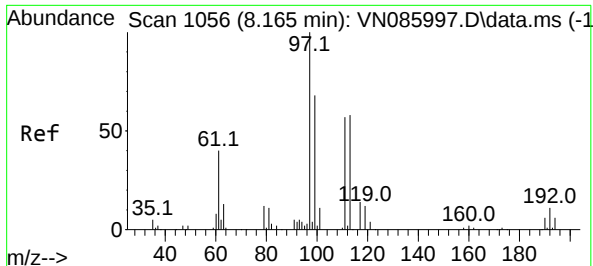


#35
Dibromofluoromethane
Concen: 50.372 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Instrument :
MSVOA_N
ClientSampleId :
CHRT24743



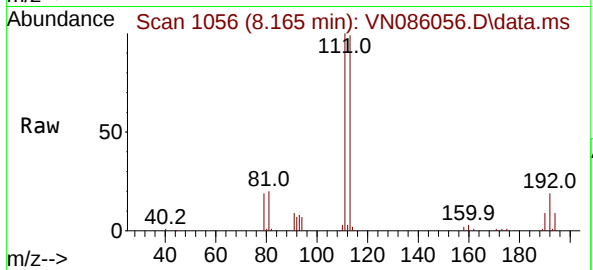



Tgt Ion:113 Resp: 95919
Ion Ratio Lower Upper
113 100
111 102.6 81.8 122.8
192 20.0 15.9 23.9

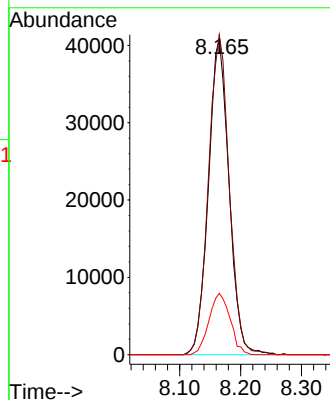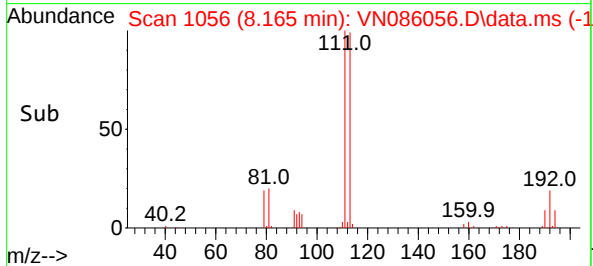

#36
1,1-Dichloropropene
Concen: 4.477 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.141 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Tgt Ion: 75 Resp: 11225
Ion Ratio Lower Upper
75 100
110 10.8 17.8 53.3#
77 0.0 25.0 37.4#

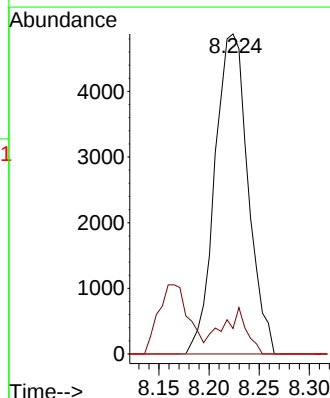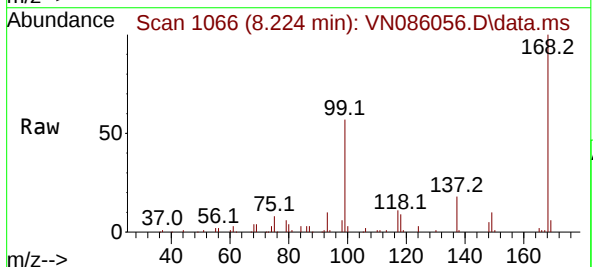



#37

Ethyl Acetate

Concen: 0.825 ug/l

RT: 7.565 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN086056.D

Acq: 21 Mar 2025 21:42

Instrument :

MSVOA_N

ClientSampleId :

CHRT24743





Tgt Ion: 43 Resp: 1745

Ion Ratio Lower Upper

43 100

61 0.0 13.0 19.4#

70 0.0 11.0 16.6#

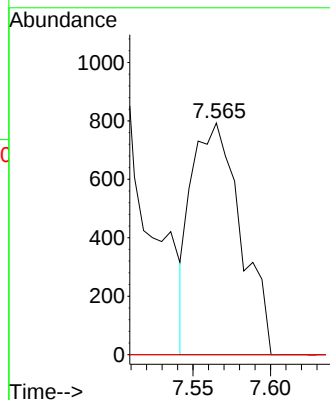

#38

Carbon Tetrachloride

Concen: 4.592 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.135 min

Lab File: VN086056.D

Acq: 21 Mar 2025 21:42




Tgt Ion: 117 Resp: 15139


Ion Ratio Lower Upper

117 100

119 4.5 77.0 115.4#

121 0.0 25.6 38.4#


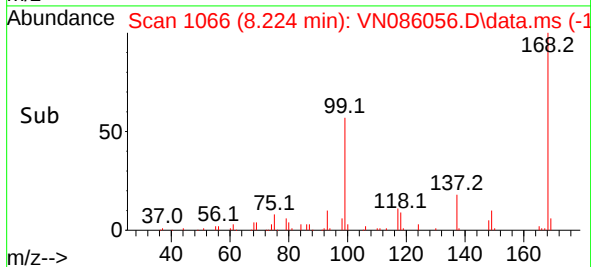
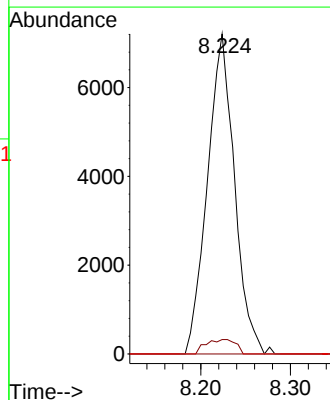
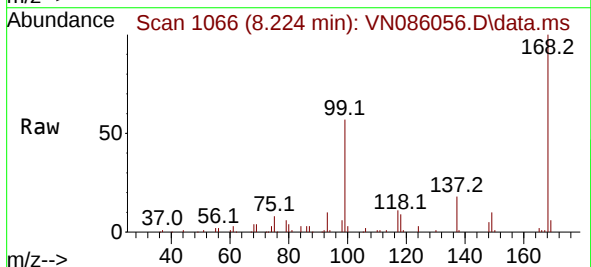




#40
Benzene
Concen: 21.821 ug/l
RT: 8.606 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42




Instrument :
MSVOA_N
ClientSampleId :
CHRT24743


Tgt Ion: 78 Resp: 171756
Ion Ratio Lower Upper
78 100
77 24.8 18.9 28.3

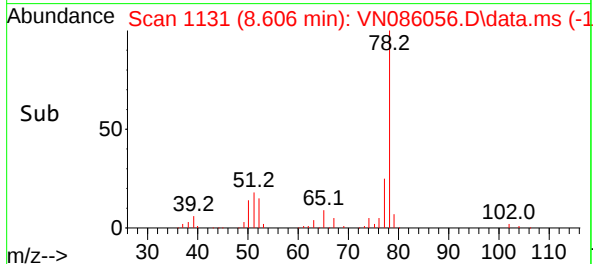

#43
Isopropyl Acetate
Concen: 23.298 ug/l
RT: 8.683 min Scan# 1144
Delta R.T. -0.000 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Tgt Ion: 43 Resp: 106792
Ion Ratio Lower Upper
43 100
61 16.3 25.0 37.6#
87 11.3 13.0 19.4#

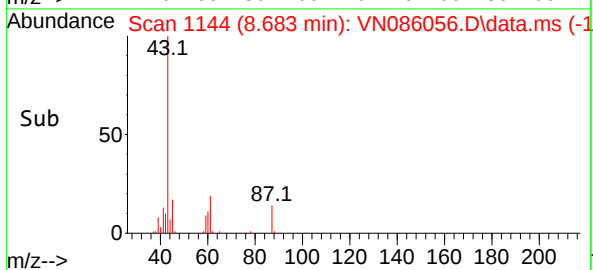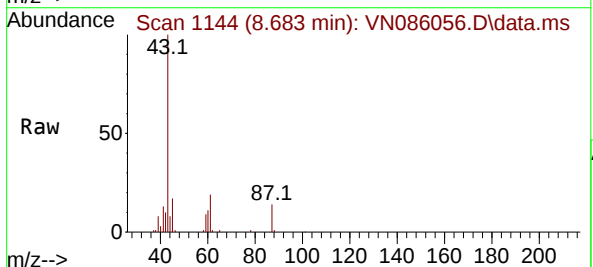

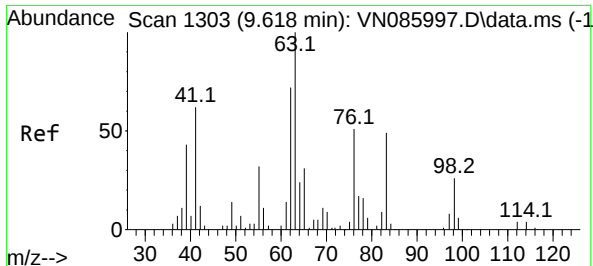

#45

1,2-Dichloropropane

Concen: 0.541 ug/l

RT: 9.741 min Scan# 1

Delta R.T. 0.123 min

Lab File: VN086056.D

Acq: 21 Mar 2025 21:42

Instrument :

MSVOA_N

ClientSampleId :





CHRT24743

Tgt Ion: 63 Resp: 969

Ion Ratio Lower Upper

63 100

65 0.0 24.7 37.1#

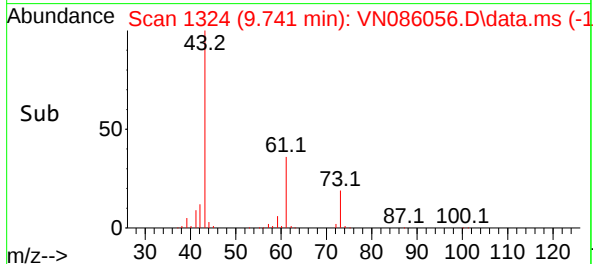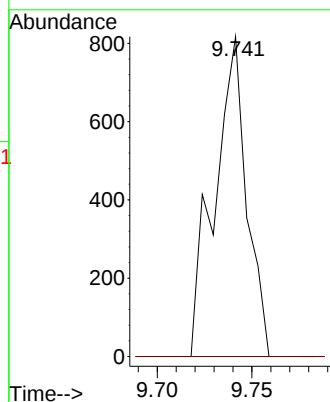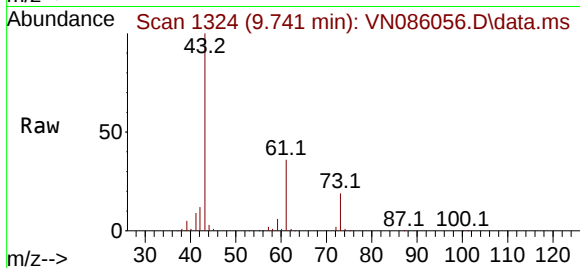

#48

Methyl methacrylate

Concen: 1.361 ug/l

RT: 9.671 min Scan# 1312

Delta R.T. -0.006 min

Lab File: VN086056.D

Acq: 21 Mar 2025 21:42




Tgt Ion: 41 Resp: 2059


Ion Ratio Lower Upper

41 100

69 0.0 83.1 124.7#

39 0.0 45.6 68.4#


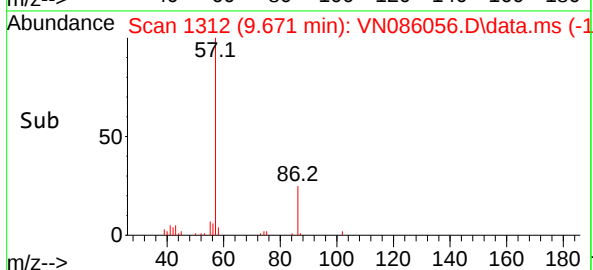
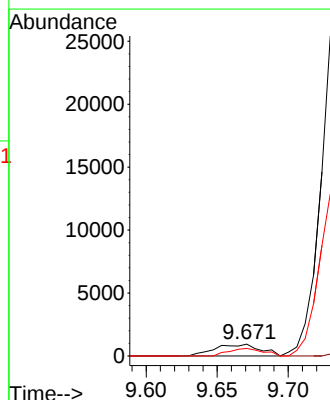
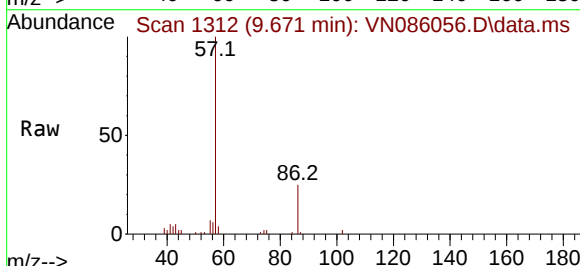




#50
Toluene-d8
Concen: 51.337 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42




Instrument :
MSVOA_N
ClientSampleId :
CHRT24743


Tgt Ion: 98 Resp: 354788
Ion Ratio Lower Upper
98 100
100 63.7 53.1 79.7



#51
4-Methyl-2-Pentanone
Concen: 3.325 ug/l
RT: 10.441 min Scan# 1443
Delta R.T. -0.000 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Tgt Ion: 43 Resp: 6721
Ion Ratio Lower Upper
43 100
58 22.9 37.4 56.0#

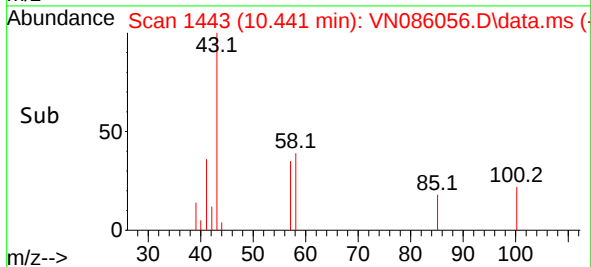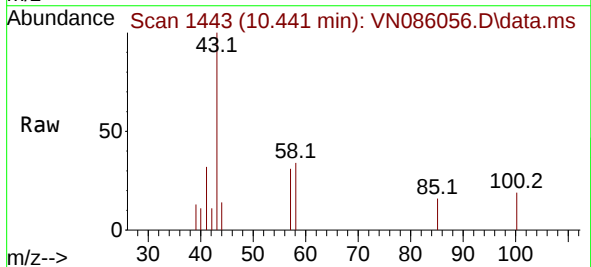



#52

Toluene

Concen: 2.514 ug/l

RT: 10.630 min Scan# 1491

Delta R.T. -0.000 min

Lab File: VN086056.D

Acq: 21 Mar 2025 21:42

Instrument :

MSVOA_N

ClientSampleId :





CHRT24743

Tgt Ion: 92 Resp: 12147

Ion Ratio Lower Upper

92 100

91 162.1 136.2 204.4

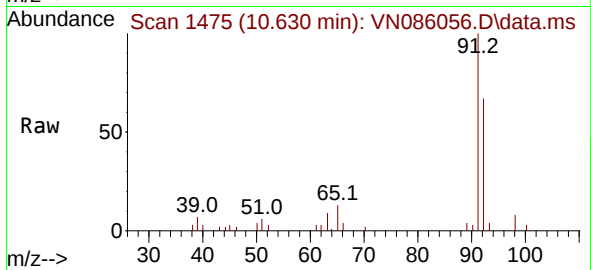

#53

t-1,3-Dichloropropene

Concen: 0.209 ug/l

RT: 10.724 min Scan# 1491

Delta R.T. -0.112 min

Lab File: VN086056.D




Acq: 21 Mar 2025 21:42


Tgt Ion: 75 Resp: 598

Ion Ratio Lower Upper

75 100

77 0.0 25.3 37.9#


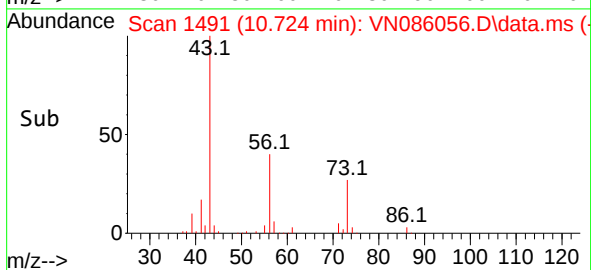

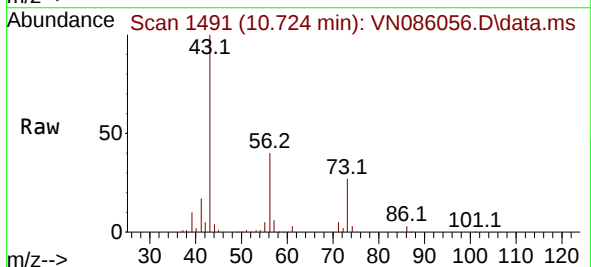




#54
 cis-1,3-Dichloropropene
 Concen: 8.992 ug/l
 RT: 10.353 min Scan# 1428
 Delta R.T. 0.041 min
 Lab File: VN086056.D
 Acq: 21 Mar 2025 21:42




Instrument :
 MSVOA_N
 ClientSampleId :
 CHRT24743


Tgt Ion: 75 Resp: 27112
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.3 37.9#
 39 32.3 29.6 44.4



#56
 Ethyl methacrylate
 Concen: 0.839 ug/l
 RT: 10.982 min Scan# 1535
 Delta R.T. 0.111 min
 Lab File: VN086056.D
 Acq: 21 Mar 2025 21:42

Tgt Ion: 69 Resp: 1516
 Ion Ratio Lower Upper
 69 100
 41 2117.1 41.6 62.4#
 39 964.3 21.8 32.8#

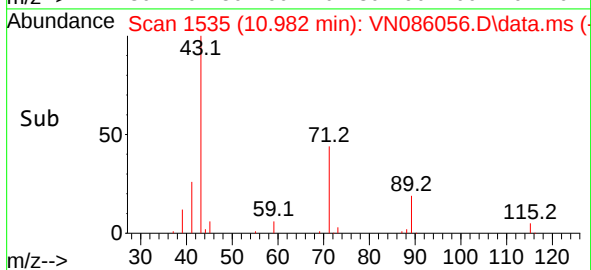



#57

1,3-Dichloropropane

Concen: 1.132 ug/l

RT: 11.200 min Scan# 1572

Delta R.T. 0.041 min

Lab File: VN086056.D

Acq: 21 Mar 2025 21:42

Instrument :

MSVOA_N

ClientSampleId :





CHRT24743

Tgt Ion: 76 Resp: 3546

Ion Ratio Lower Upper

76 100

78 0.0 25.8 38.6#

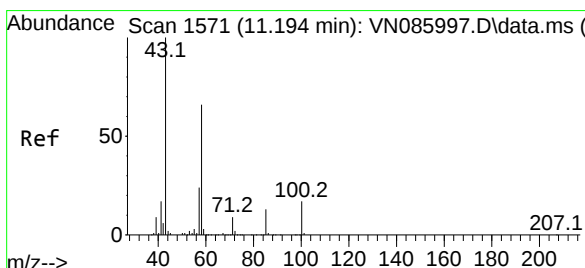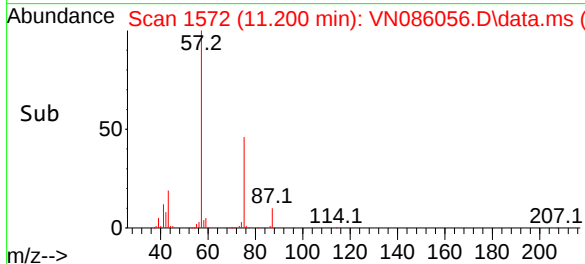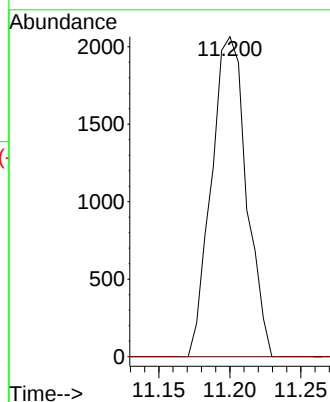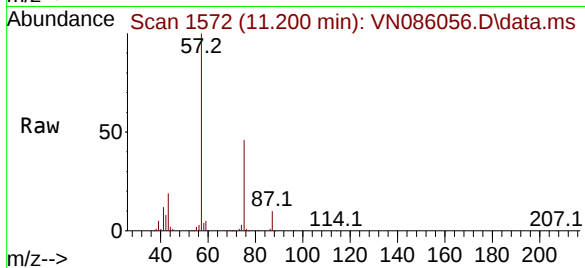

#59

2-Hexanone

Concen: 23.841 ug/l

RT: 11.200 min Scan# 1572

Delta R.T. 0.006 min

Lab File: VN086056.D




Acq: 21 Mar 2025 21:42


Tgt Ion: 43 Resp: 35111

Ion Ratio Lower Upper

43 100

58 27.8 32.4 97.2#


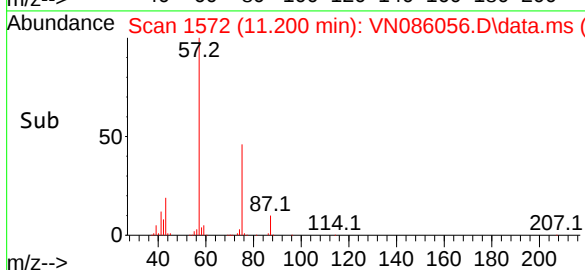
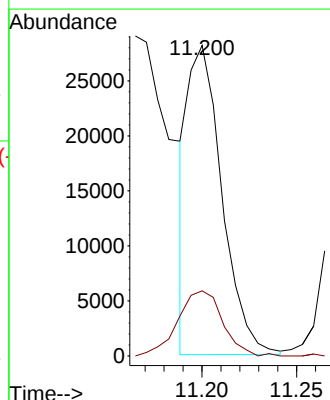
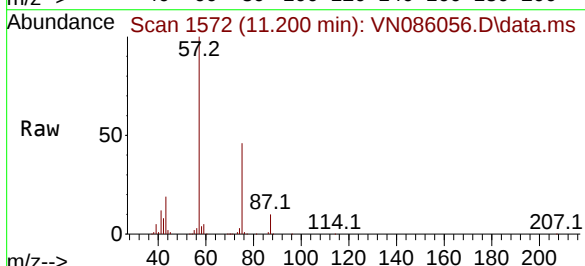




#62
4-Bromofluorobenzene
Concen: 41.459 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42




Instrument :
MSVOA_N
ClientSampleId :
CHRT24743


Tgt Ion: 95 Resp: 102182
Ion Ratio Lower Upper
95 100
174 82.0 0.0 156.8
176 78.5 0.0 152.2

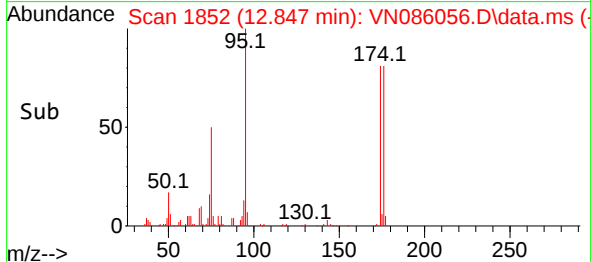

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Tgt Ion: 117 Resp: 264858
Ion Ratio Lower Upper
117 100
82 55.4 46.7 70.1
119 32.2 26.5 39.7


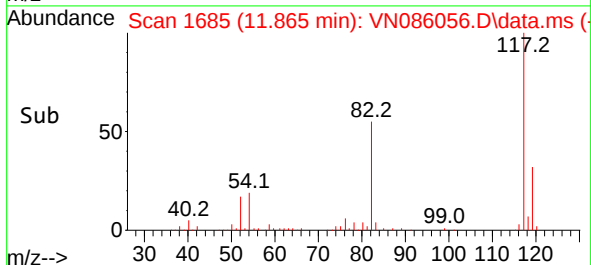
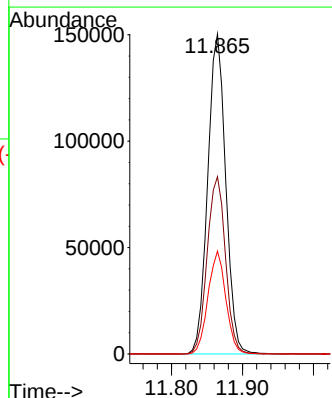
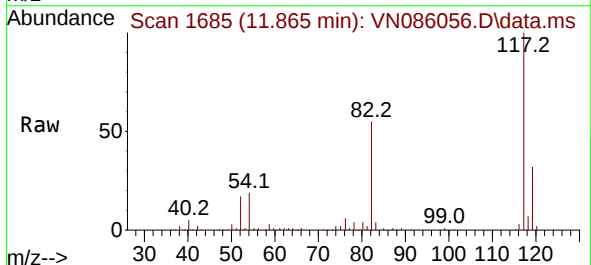




#67
Ethyl Benzene
Concen: 0.639 ug/l
RT: 11.959 min Scan# 1701
Delta R.T. -0.000 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42




Instrument :
MSVOA_N
ClientSampleId :
CHRT24743


Tgt Ion: 91 Resp: 6194
Ion Ratio Lower Upper
91 100
106 29.3 24.5 36.7

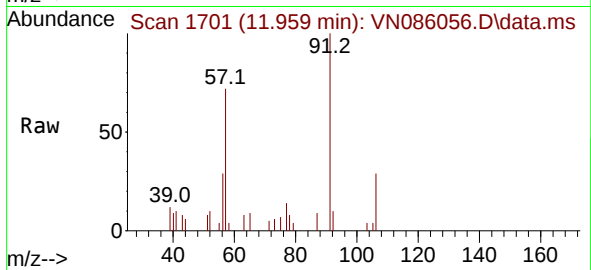

#68
m/p-Xylenes
Concen: 0.597 ug/l
RT: 12.065 min Scan# 1719
Delta R.T. -0.006 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Tgt Ion: 106 Resp: 2273
Ion Ratio Lower Upper
106 100
91 205.4 163.9 245.9


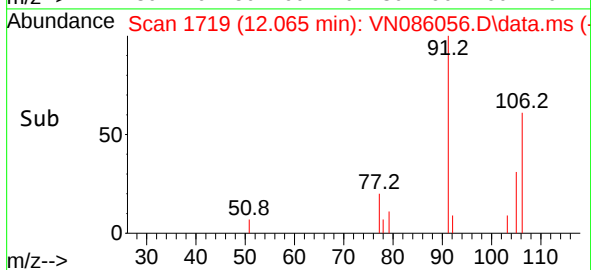

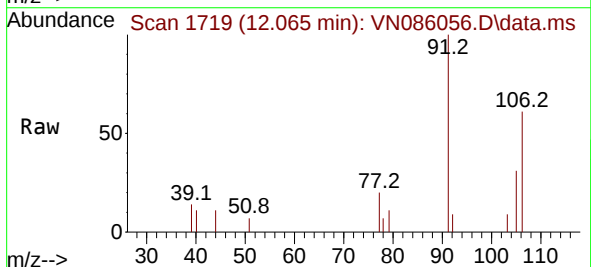




#69
o-Xylene
Concen: 0.319 ug/l
RT: 12.400 min Scan# 1116
Delta R.T. 0.006 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42




Instrument :
MSVOA_N
ClientSampleId :
CHRT24743


Tgt Ion:106 Resp: 1116
Ion Ratio Lower Upper
106 100
91 207.2 109.1 327.2



#71
Bromoform
Concen: 0.203 ug/l
RT: 12.841 min Scan# 1851
Delta R.T. 0.265 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Tgt Ion:173 Resp: 382
Ion Ratio Lower Upper
173 100
175 1205.5 24.3 73.0#
254 0.0 0.0 0.0


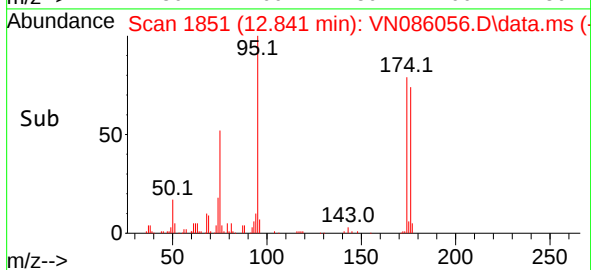

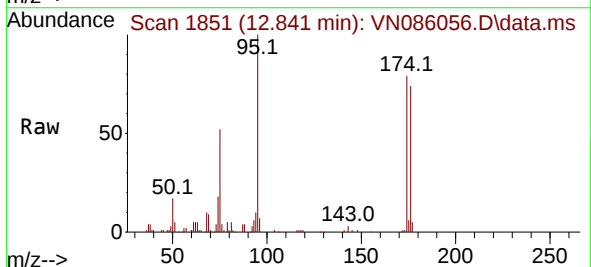




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 20
Delta R.T. -0.000 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42




Instrument :
MSVOA_N
ClientSampleId :
CHRT24743


Tgt Ion:152 Resp: 97851
Ion Ratio Lower Upper
152 100
115 61.0 31.1 93.2
150 157.3 0.0 359.6

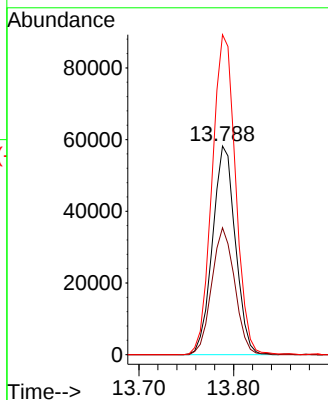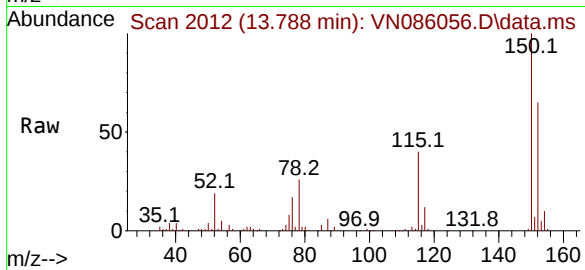

#76
1,2,3-Trichloropropane
Concen: 23.654 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.141 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Tgt Ion: 75 Resp: 51818
Ion Ratio Lower Upper
75 100
77 1.3 83.7 251.0#



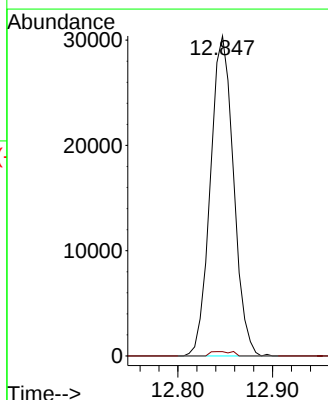
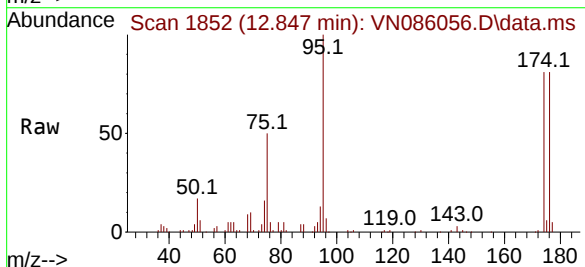


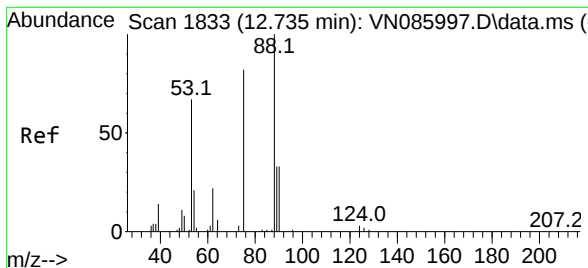

#81
trans-1,4-Dichloro-2-butene
Concen: 62.536 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.112 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42




Instrument :
MSVOA_N
ClientSampleId :
CHRT24743


Tgt Ion: 75 Resp: 51818
Ion Ratio Lower Upper
75 100
53 0.2 66.0 99.0#
89 0.0 36.9 55.3#

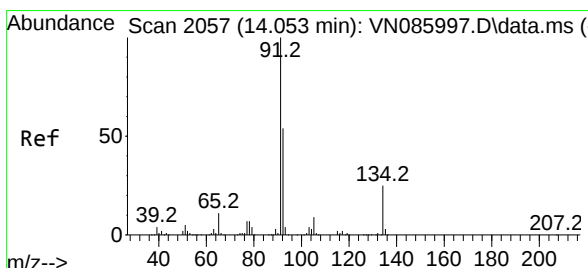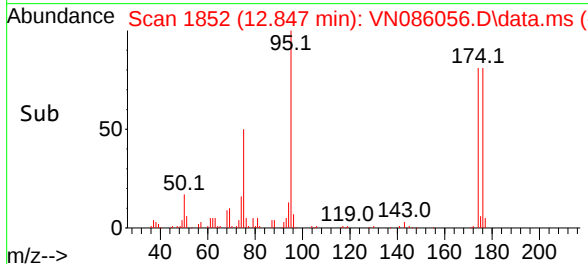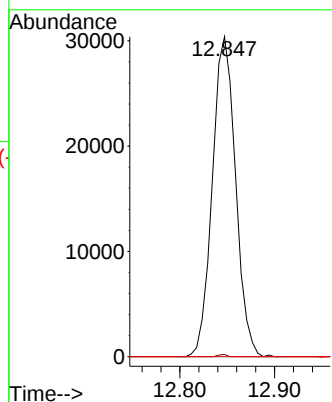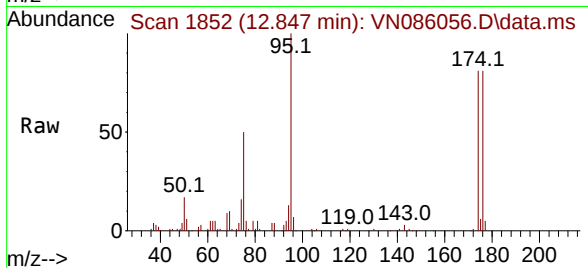

#89
n-Butylbenzene
Concen: 0.309 ug/l
RT: 13.988 min Scan# 2046
Delta R.T. -0.065 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Tgt Ion: 91 Resp: 1339
Ion Ratio Lower Upper
91 100
92 0.0 26.9 80.6#
134 0.0 13.0 39.0#


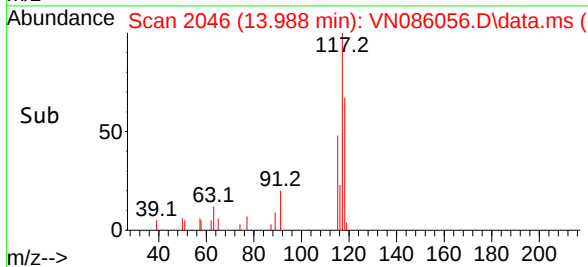

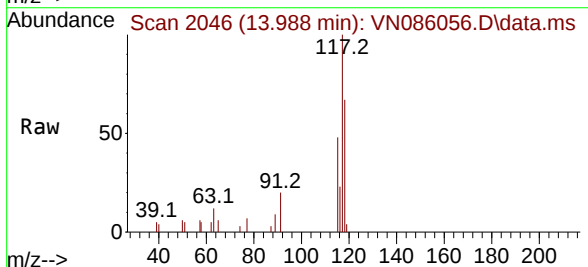




#90
Hexachloroethane
Concen: 0.792 ug/l
RT: 14.441 min Scan# 2104
Delta R.T. 0.112 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Instrument :
MSVOA_N
ClientSampleId :
CHRT24743

Tgt Ion:117 Resp: 974
Ion Ratio Lower Upper
117 100
201 0.0 39.1 117.3#

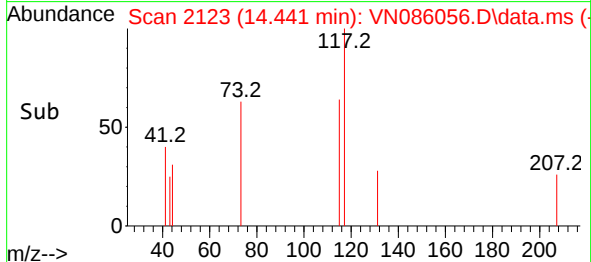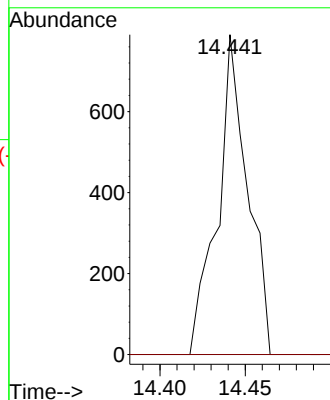

#95
Naphthalene
Concen: 1.394 ug/l
RT: 15.641 min Scan# 2327
Delta R.T. -0.000 min
Lab File: VN086056.D
Acq: 21 Mar 2025 21:42

Tgt Ion:128 Resp: 6777
Ion Ratio Lower Upper
128 100
127 14.7 10.2 15.4
129 9.8 9.0 13.6

