

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032125\
 Data File : VN086057.D
 Acq On : 21 Mar 2025 22:07
 Operator : JC\MD
 Sample : Q1606-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RBR251346

Quant Time: Mar 21 23:06:55 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 19 03:20:56 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	139512	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	266795	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	257663	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	95635	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	112974	59.137	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 118.280%	
35) Dibromofluoromethane	8.165	113	94141	50.554	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 101.100%	
50) Toluene-d8	10.565	98	344230	50.933	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 101.860%	
62) 4-Bromofluorobenzene	12.847	95	101527	42.123	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 84.240%	


Target Compounds					Qvalue	
16) Acetone	4.424	43	27813	47.654	ug/l	92
17) Carbon Disulfide	4.718	76	1518	0.323	ug/l #	74
18) Methyl Acetate	5.041	43	1771	1.226	ug/l #	84
20) Methylene Chloride	5.277	84	10215	5.983	ug/l	89
25) 2-Butanone	7.494	43	3997	4.746	ug/l #	88
29) Tetrahydrofuran	7.847	42	185	0.356	ug/l #	24
30) Chloroform	7.971	83	816	0.264	ug/l #	76
31) Cyclohexane	8.218	56	3074	1.291	ug/l #	1
36) 1,1-Dichloropropene	8.224	75	11581	4.723	ug/l #	48
37) Ethyl Acetate	7.553	43	1920	0.928	ug/l #	73
38) Carbon Tetrachloride	8.224	117	15182	4.709	ug/l #	16
40) Benzene	8.606	78	63758	8.283	ug/l	99
42) 1,2-Dichloroethane	8.682	62	568	0.212	ug/l #	74
43) Isopropyl Acetate	8.688	43	108487	24.201	ug/l #	78
45) 1,2-Dichloropropane	9.723	63	981	0.560	ug/l #	44
48) Methyl methacrylate	9.659	41	2031	1.373	ug/l #	7
49) 1,4-Dioxane	9.729	88	69	1.973	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	3546	1.794	ug/l	99
52) Toluene	10.629	92	10832	2.293	ug/l	95
54) cis-1,3-Dichloropropene	10.353	75	26027	8.827	ug/l #	68
56) Ethyl methacrylate	10.982	69	1371	0.790	ug/l #	1
57) 1,3-Dichloropropane	11.200	76	3767	1.230	ug/l #	42
59) 2-Hexanone	11.200	43	35069	24.350	ug/l #	56
67) Ethyl Benzene	11.959	91	6050	0.641	ug/l	90
68) m/p-Xylenes	12.070	106	2508	0.677	ug/l	98
69) o-Xylene	12.400	106	1000	0.294	ug/l	92
71) Bromoform	12.841	173	1047	0.571	ug/l #	1
74) N-amyl acetate	12.470	43	685	0.314	ug/l #	35
76) 1,2,3-Trichloropropane	12.847	75	51185	23.906	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	51185	63.204	ug/l #	16
89) n-Butylbenzene	13.994	91	905	0.213	ug/l #	33
95) Naphthalene	15.641	128	2739	0.577	ug/l #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032125\
Data File : VN086057.D
Acq On : 21 Mar 2025 22:07
Operator : JC\MD
Sample : Q1606-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RBR251346

Quant Time: Mar 21 23:06:55 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 19 03:20:56 2025
Response via : Initial Calibration



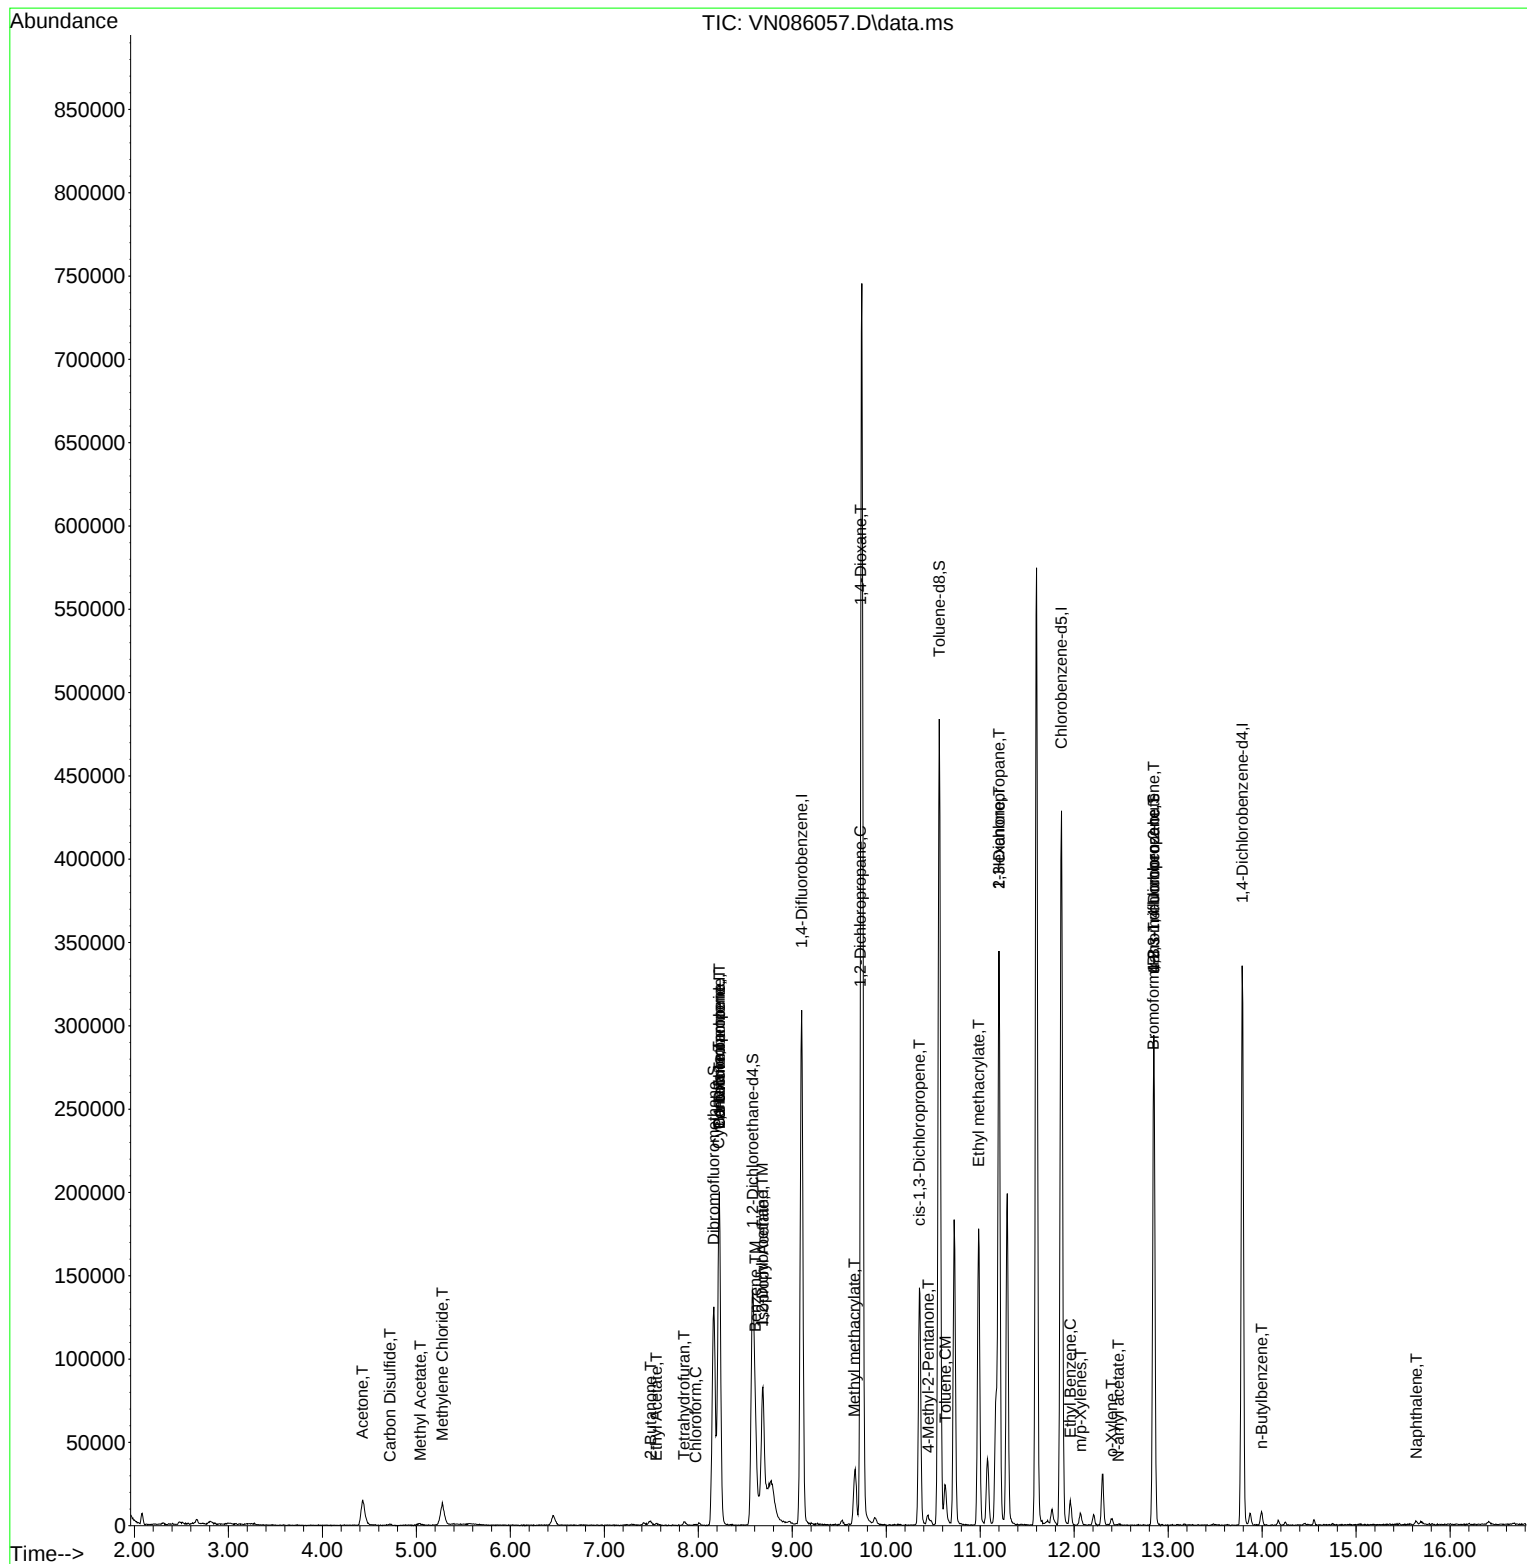




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07




Instrument :
MSVOA_N
ClientSampleId :
RBR251346


Tgt Ion:168 Resp: 139512
Ion Ratio Lower Upper
168 100
99 60.1 49.4 74.2

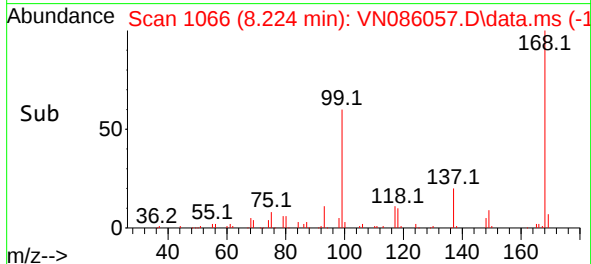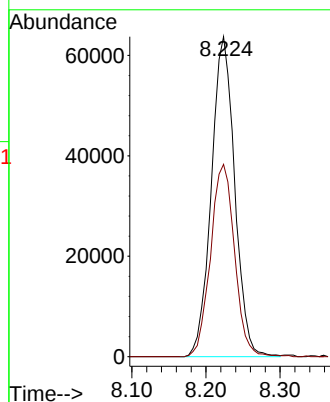

#16
Acetone
Concen: 47.654 ug/l
RT: 4.424 min Scan# 420
Delta R.T. -0.000 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07

Tgt Ion: 43 Resp: 27813
Ion Ratio Lower Upper
43 100
58 41.4 29.4 44.2


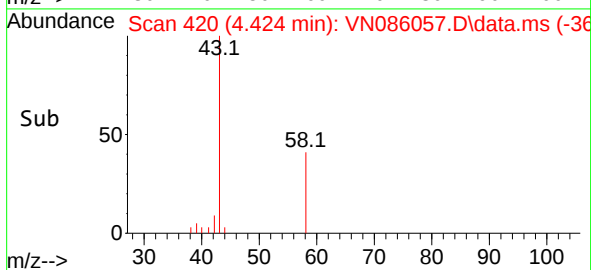
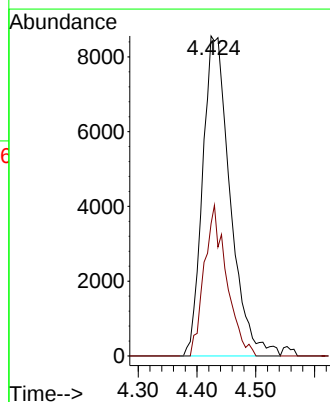
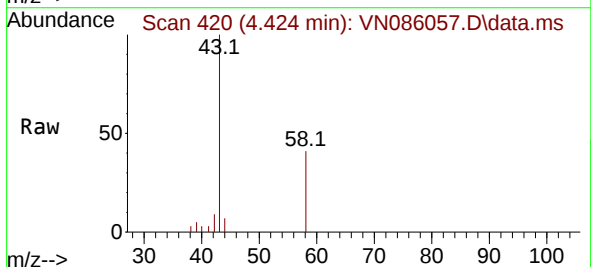




#17
Carbon Disulfide
Concen: 0.323 ug/l
RT: 4.718 min Scan# 41
Delta R.T. 0.012 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07




Instrument :
MSVOA_N
ClientSampleId :
RBR251346


Tgt Ion: 76 Resp: 1518
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.2#

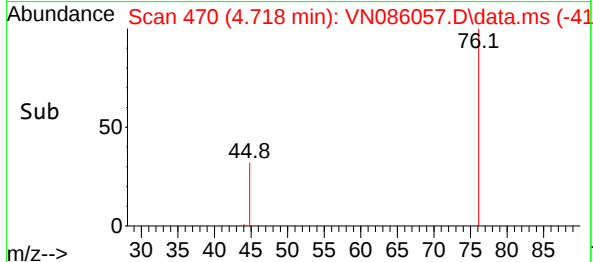

#18
Methyl Acetate
Concen: 1.226 ug/l
RT: 5.041 min Scan# 525
Delta R.T. 0.017 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07


Tgt Ion: 43 Resp: 1771
Ion Ratio Lower Upper
43 100
74 21.5 23.9 35.9#

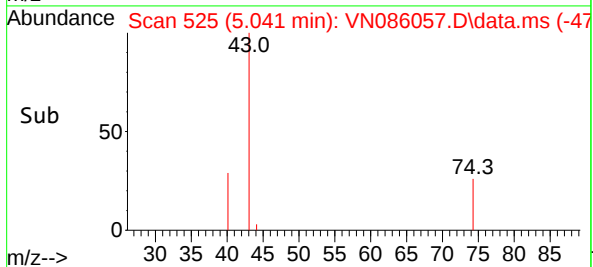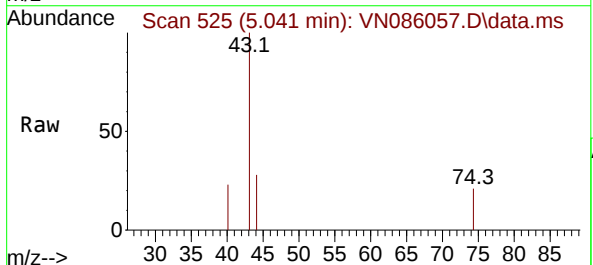



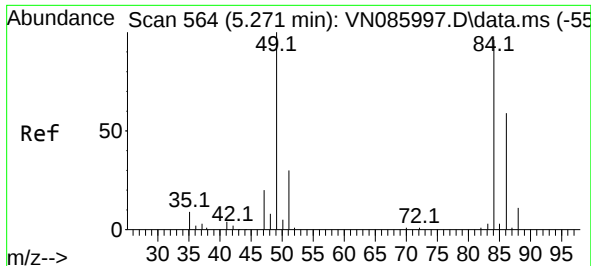


#20
Methylene Chloride
Concen: 5.983 ug/l
RT: 5.277 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07

Instrument :
MSVOA_N
ClientSampleId :
RBR251346







Tgt Ion:	84	Resp:	10215
Ion	Ratio	Lower	Upper
84	100		
49	120.5	83.3	124.9
51	37.1	24.8	37.2
86	62.0	48.7	73.1

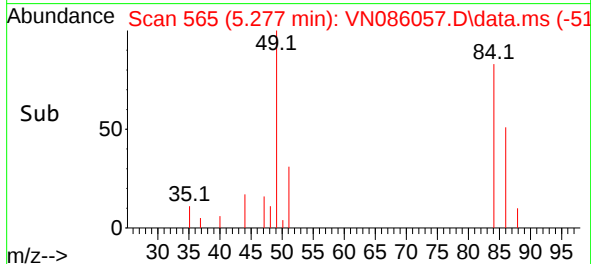

#25
2-Butanone
Concen: 4.746 ug/l
RT: 7.494 min Scan# 942
Delta R.T. 0.012 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07

Tgt Ion:	43	Resp:	3997
Ion	Ratio	Lower	Upper
43	100		
72	27.2	27.4	41.0#

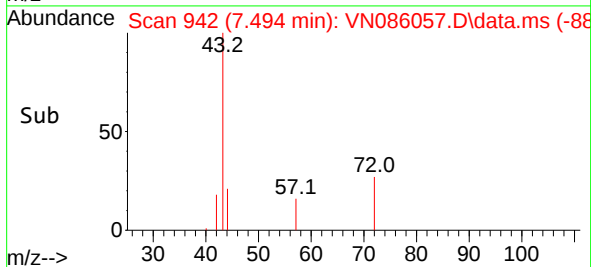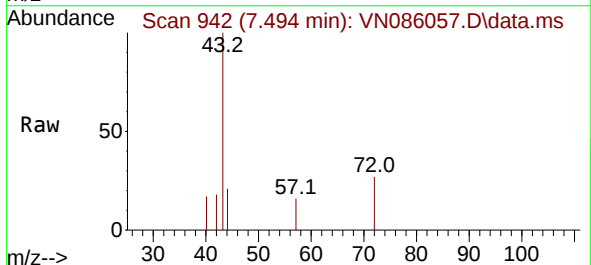



#29

Tetrahydrofuran

Concen: 0.356 ug/l

RT: 7.847 min Scan# 1000

Delta R.T. 0.011 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Instrument :

MSVOA_N

ClientSampleId :

RBR251346





Tgt Ion: 42 Resp: 185

Ion Ratio Lower Upper

42 100

72 0.0 45.0 67.4#

71 0.0 41.9 62.9#

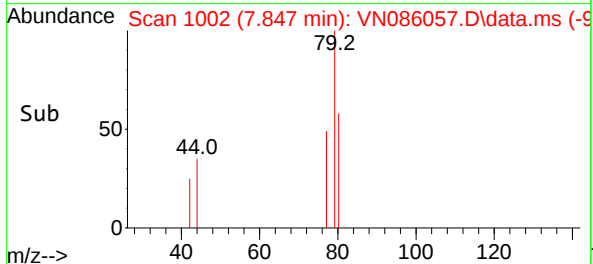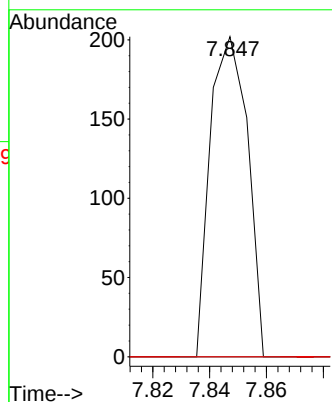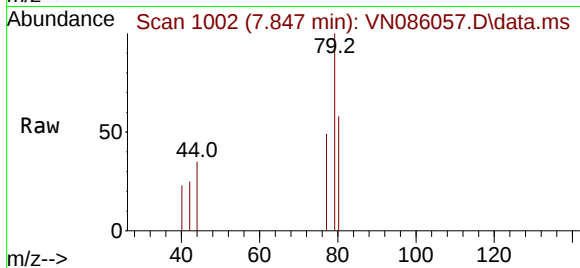

#30

Chloroform

Concen: 0.264 ug/l

RT: 7.971 min Scan# 1023

Delta R.T. 0.006 min

Lab File: VN086057.D




Acq: 21 Mar 2025 22:07


Tgt Ion: 83 Resp: 816

Ion Ratio Lower Upper

83 100

85 45.4 51.5 77.3#

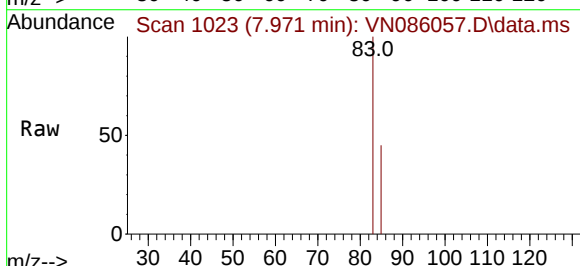



#31

Cyclohexane

Concen: 1.291 ug/l

RT: 8.218 min Scan# 1

Delta R.T. -0.036 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Instrument :

MSVOA_N

ClientSampleId :

RBR251346





Tgt Ion: 56 Resp: 3074

Ion Ratio Lower Upper

56 100

69 195.3 28.0 42.0#

84 136.6 75.0 112.6#

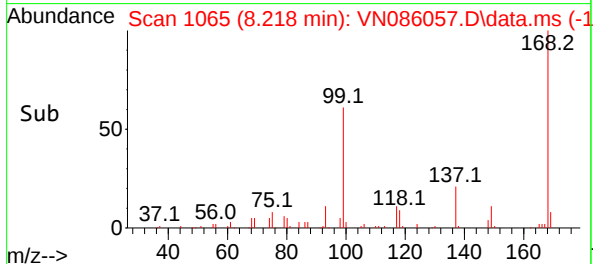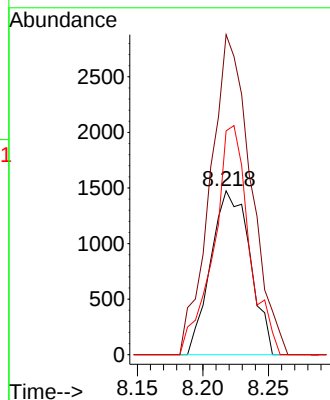

#33

1,2-Dichloroethane-d4

Concen: 59.137 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VN086057.D




Acq: 21 Mar 2025 22:07


Tgt Ion: 65 Resp: 112974

Ion Ratio Lower Upper

65 100

67 50.2 0.0 102.2

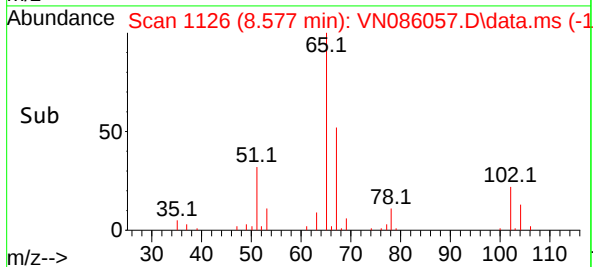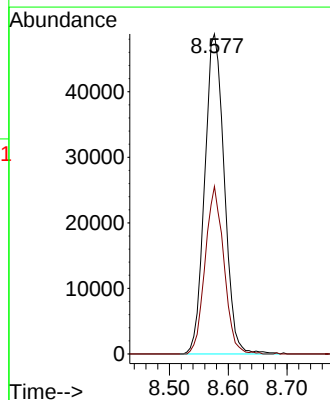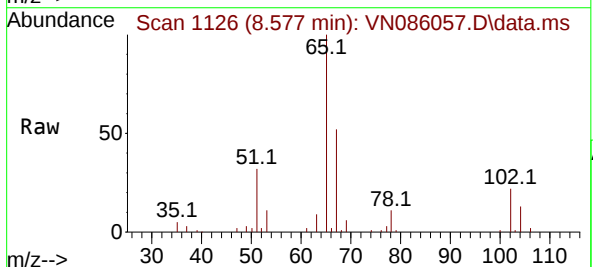



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Instrument :

MSVOA_N

ClientSampleId :

RBR251346





Tgt Ion:114 Resp: 266795

Ion Ratio Lower Upper

114 100

63 18.4 0.0 39.6

88 15.2 0.0 32.6

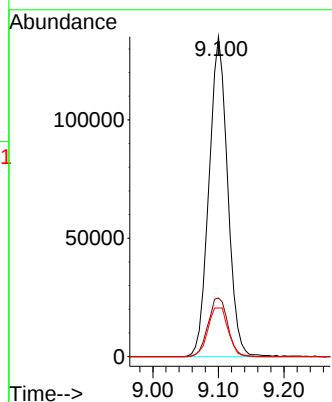

#35

Dibromofluoromethane

Concen: 50.554 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07




Tgt Ion:113 Resp: 94141


Ion Ratio Lower Upper

113 100

111 103.3 81.8 122.8

192 20.3 15.9 23.9

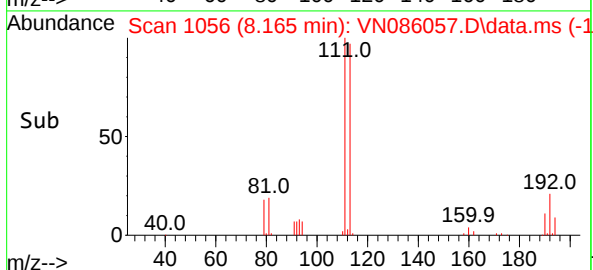



#36

1,1-Dichloropropene

Concen: 4.723 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.141 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Instrument :

MSVOA_N

ClientSampleId :

RBR251346





Tgt Ion: 75 Resp: 11581

Ion Ratio Lower Upper

75 100

110 7.6 17.8 53.3#

77 0.0 25.0 37.4#

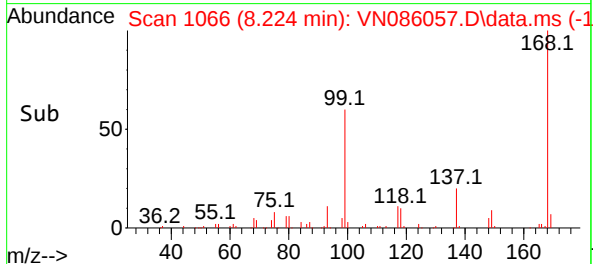

#37

Ethyl Acetate

Concen: 0.928 ug/l

RT: 7.553 min Scan# 952

Delta R.T. -0.006 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07




Tgt Ion: 43 Resp: 1920


Ion Ratio Lower Upper

43 100

61 3.9 13.0 19.4#

70 3.5 11.0 16.6#

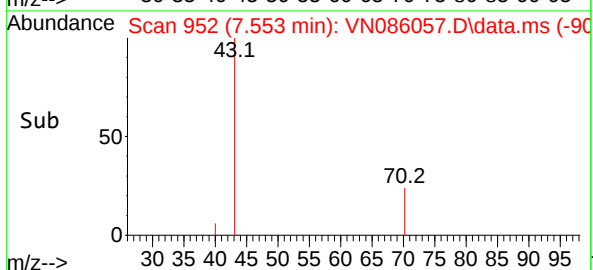



#38

Carbon Tetrachloride

Concen: 4.709 ug/l

RT: 8.224 min Scan# 1

Delta R.T. -0.136 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Instrument :

MSVOA_N

ClientSampleId :

RBR251346





Tgt Ion:117 Resp: 15182

Ion Ratio Lower Upper

117 100

119 5.9 77.0 115.4#

121 0.0 25.6 38.4#

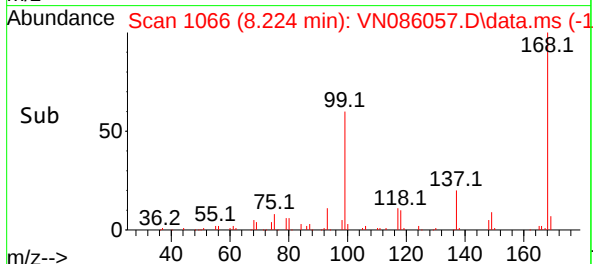

#40

Benzene

Concen: 8.283 ug/l

RT: 8.606 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VN086057.D




Acq: 21 Mar 2025 22:07


Tgt Ion: 78 Resp: 63758

Ion Ratio Lower Upper

78 100

77 23.1 18.9 28.3

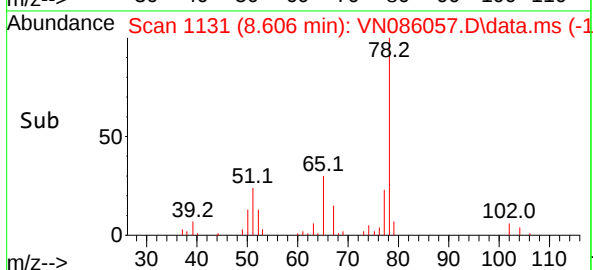



#42

1,2-Dichloroethane

Concen: 0.212 ug/l

RT: 8.682 min Scan# 1144

Delta R.T. 0.012 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Instrument :

MSVOA_N

ClientSampleId :





RBR251346

Tgt Ion: 62 Resp: 568

Ion Ratio Lower Upper

62 100

98 0.0 0.0 18.6

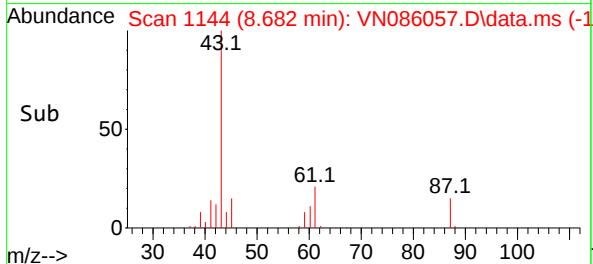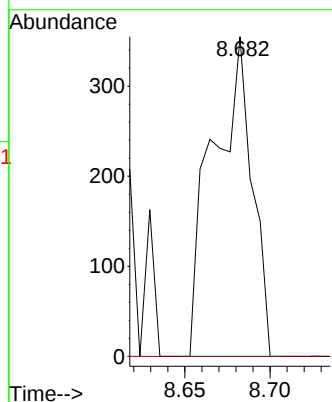

#43

Isopropyl Acetate

Concen: 24.201 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. 0.006 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07




Tgt Ion: 43 Resp: 108487


Ion Ratio Lower Upper

43 100

61 16.1 25.0 37.6#

87 10.9 13.0 19.4#

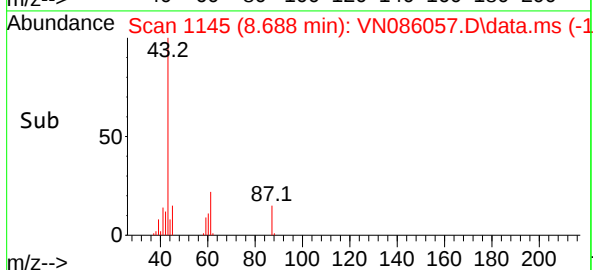



#45

1,2-Dichloropropane

Concen: 0.560 ug/l

RT: 9.723 min Scan# 11

Delta R.T. 0.106 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Instrument :

MSVOA_N

ClientSampleId :





RBR251346

Tgt Ion: 63 Resp: 981

Ion Ratio Lower Upper

63 100

65 0.0 24.7 37.1#

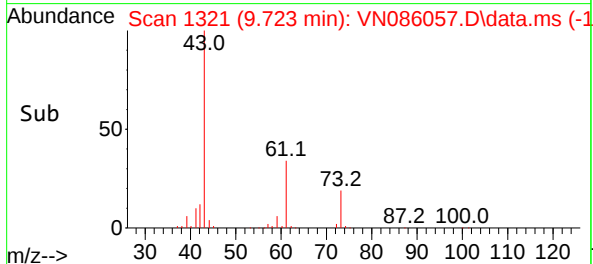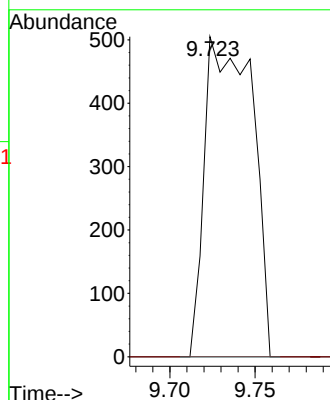

#48

Methyl methacrylate

Concen: 1.373 ug/l

RT: 9.659 min Scan# 1310

Delta R.T. -0.018 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07




Tgt Ion: 41 Resp: 2031


Ion Ratio Lower Upper

41 100

69 0.0 83.1 124.7#

39 0.0 45.6 68.4#

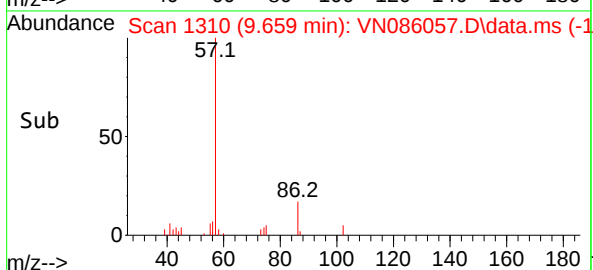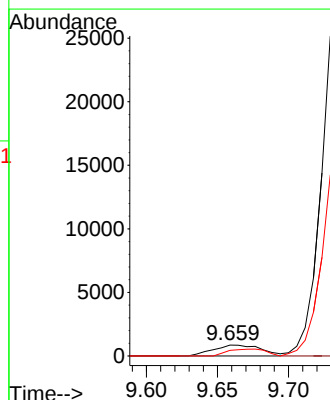



#49

1,4-Dioxane

Concen: 1.973 ug/l

RT: 9.729 min Scan# 1322

Delta R.T. 0.035 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Instrument :

MSVOA_N

ClientSampleId :

RBR251346





Tgt Ion: 88 Resp: 69

Ion Ratio Lower Upper

88 100

43 955695.7 21.7 32.5#

58 6882.6 50.4 75.6#

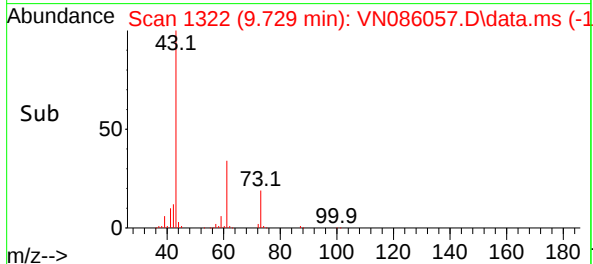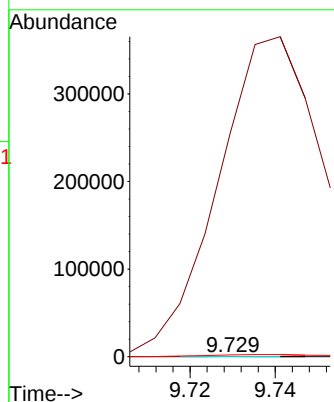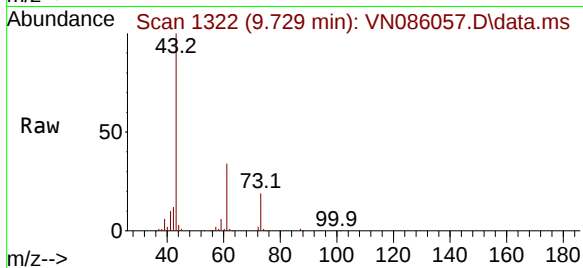

#50

Toluene-d8

Concen: 50.933 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. -0.000 min

Lab File: VN086057.D




Acq: 21 Mar 2025 22:07


Tgt Ion: 98 Resp: 344230

Ion Ratio Lower Upper

98 100

100 65.0 53.1 79.7

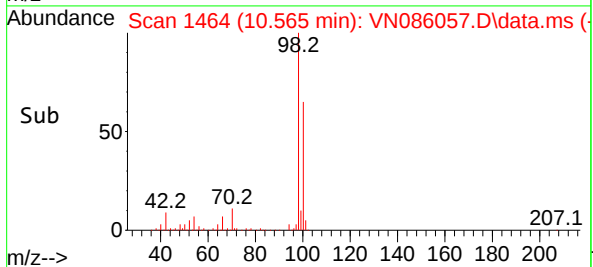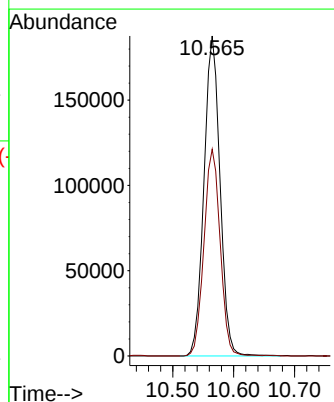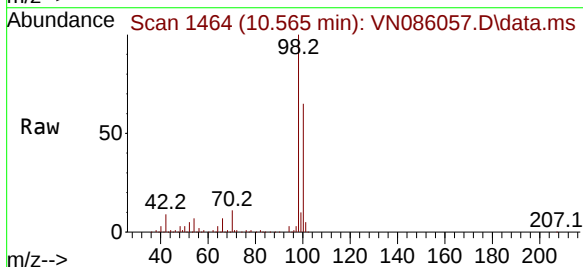

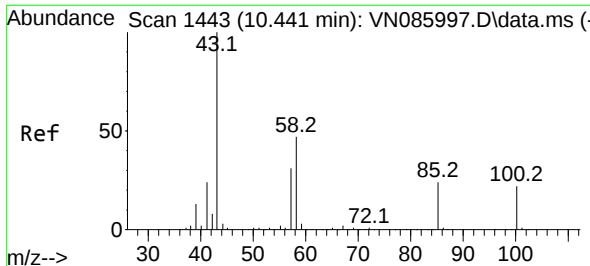

#51

4-Methyl-2-Pentanone

Concen: 1.794 ug/l

RT: 10.447 min Scan# 1443

Delta R.T. 0.006 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Instrument :

MSVOA_N

ClientSampleId :





RBR251346

Tgt Ion: 43 Resp: 3546

Ion Ratio Lower Upper

43 100

58 47.2 37.4 56.0

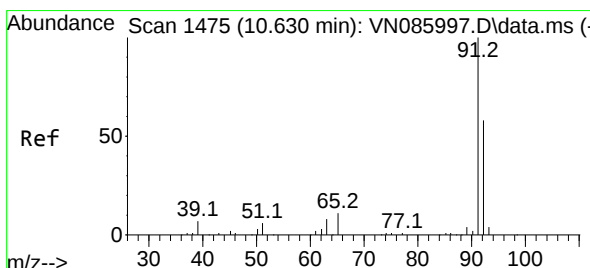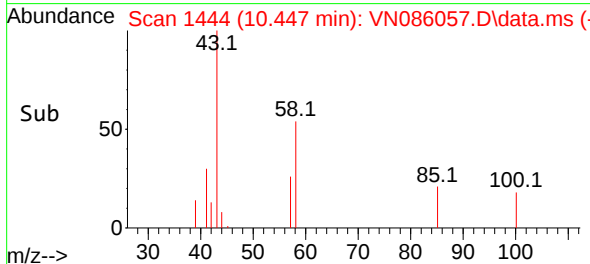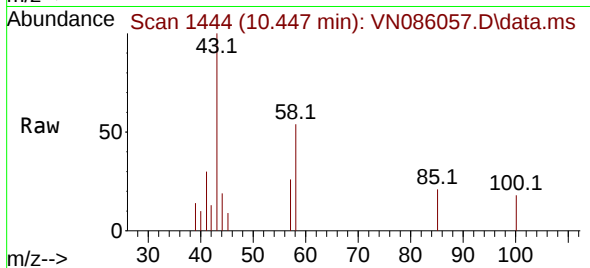

#52

Toluene

Concen: 2.293 ug/l

RT: 10.629 min Scan# 1475

Delta R.T. -0.000 min

Lab File: VN086057.D




Acq: 21 Mar 2025 22:07


Tgt Ion: 92 Resp: 10832

Ion Ratio Lower Upper

92 100

91 163.2 136.2 204.4


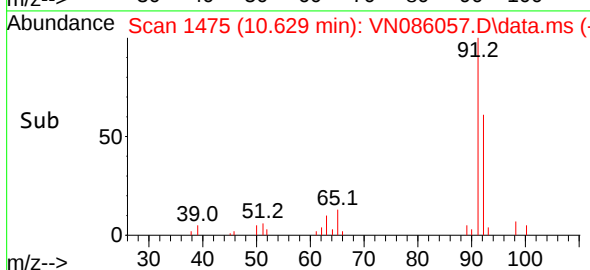

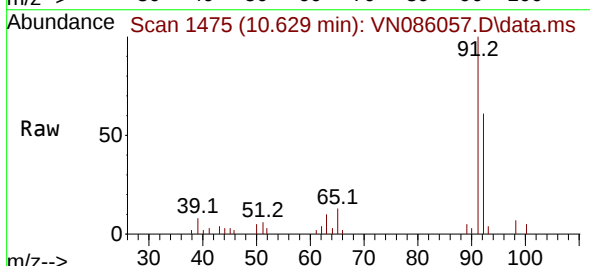




#54
 cis-1,3-Dichloropropene
 Concen: 8.827 ug/l
 RT: 10.353 min Scan# 1428
 Delta R.T. 0.041 min
 Lab File: VN086057.D
 Acq: 21 Mar 2025 22:07




Instrument :
 MSVOA_N
 ClientSampleId :
 RBR251346


Tgt Ion: 75 Resp: 26027
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.3 37.9#
 39 30.1 29.6 44.4

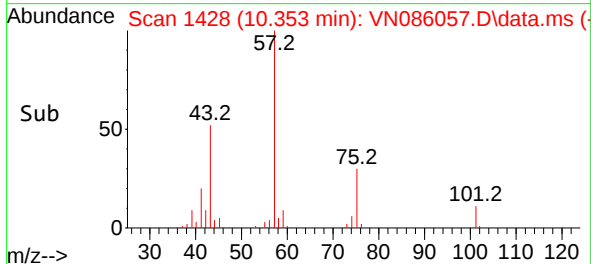

#56
 Ethyl methacrylate
 Concen: 0.790 ug/l
 RT: 10.982 min Scan# 1535
 Delta R.T. 0.111 min
 Lab File: VN086057.D
 Acq: 21 Mar 2025 22:07

Tgt Ion: 69 Resp: 1371
 Ion Ratio Lower Upper
 69 100
 41 2320.0 41.6 62.4#
 39 1051.9 21.8 32.8#

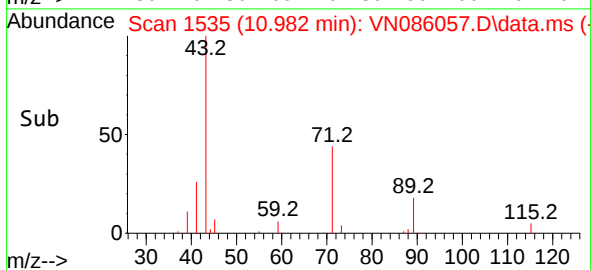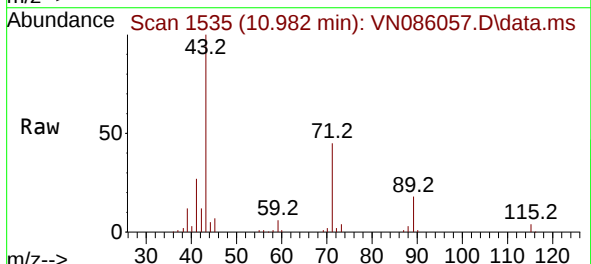



#57

1,3-Dichloropropane

Concen: 1.230 ug/l

RT: 11.200 min Scan# 1572

Delta R.T. 0.041 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Instrument :

MSVOA_N

ClientSampleId :





RBR251346

Tgt Ion: 76 Resp: 3767

Ion Ratio Lower Upper

76 100

78 0.0 25.8 38.6#

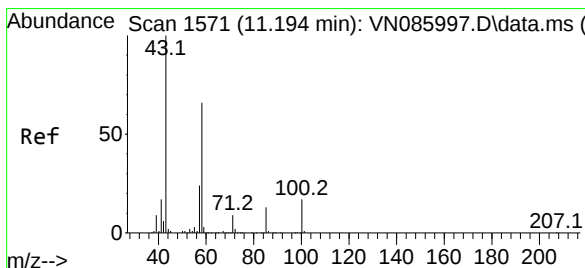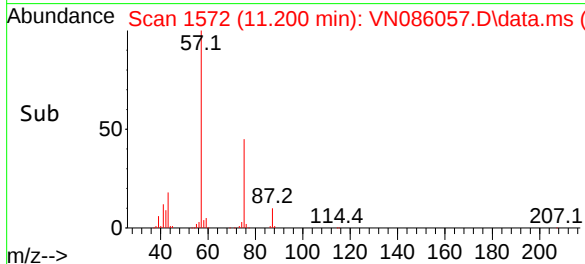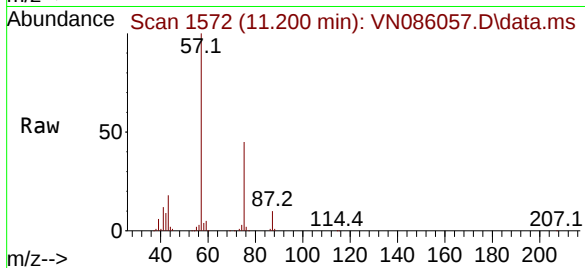

#59

2-Hexanone

Concen: 24.350 ug/l

RT: 11.200 min Scan# 1572

Delta R.T. 0.006 min

Lab File: VN086057.D




Acq: 21 Mar 2025 22:07


Tgt Ion: 43 Resp: 35069

Ion Ratio Lower Upper

43 100

58 29.9 32.4 97.2#


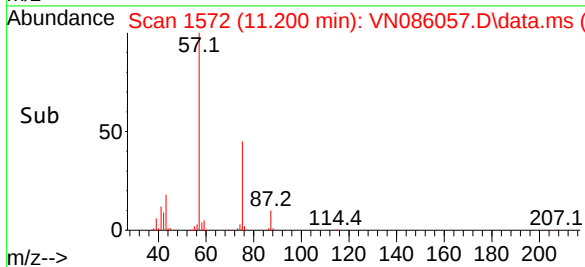

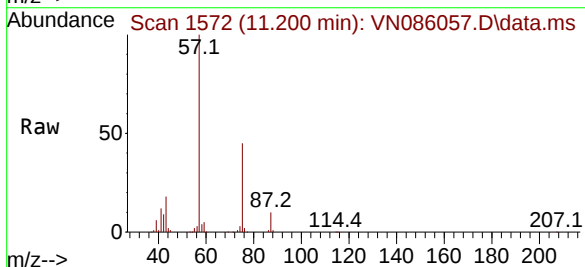




#62
4-Bromofluorobenzene
Concen: 42.123 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07




Instrument :
MSVOA_N
ClientSampleId :
RBR251346


Tgt Ion: 95 Resp: 101527
Ion Ratio Lower Upper
95 100
174 79.6 0.0 156.8
176 78.2 0.0 152.2

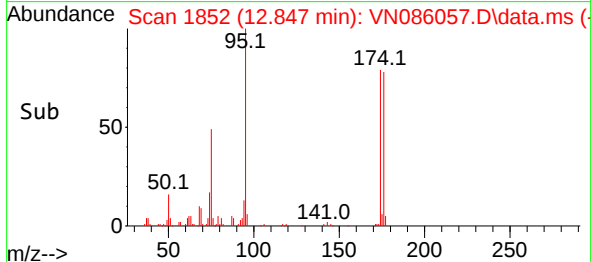

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07

Tgt Ion: 117 Resp: 257663
Ion Ratio Lower Upper
117 100
82 56.2 46.7 70.1
119 31.7 26.5 39.7


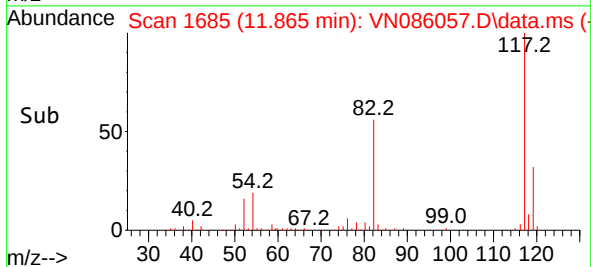

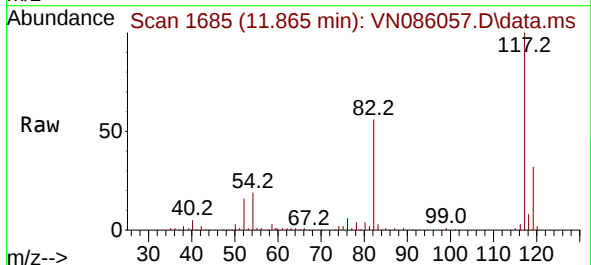




#67
Ethyl Benzene
Concen: 0.641 ug/l
RT: 11.959 min Scan# 1701
Delta R.T. -0.000 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07




Instrument :
MSVOA_N
ClientSampleId :
RBR251346


Tgt Ion: 91 Resp: 6050
Ion Ratio Lower Upper
91 100
106 35.8 24.5 36.7

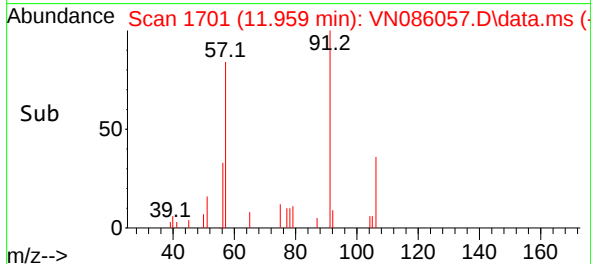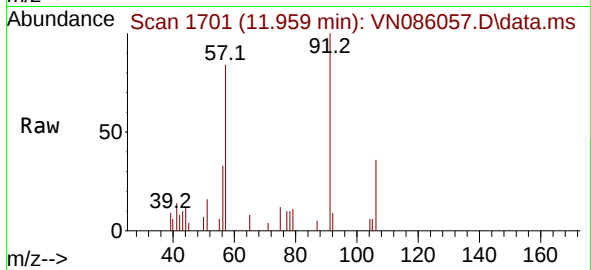

#68
m/p-Xylenes
Concen: 0.677 ug/l
RT: 12.070 min Scan# 1720
Delta R.T. -0.000 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07

Tgt Ion: 106 Resp: 2508
Ion Ratio Lower Upper
106 100
91 202.2 163.9 245.9




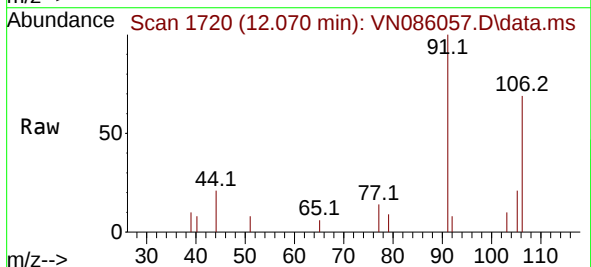




#69
o-Xylene
Concen: 0.294 ug/l
RT: 12.400 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07




Instrument :
MSVOA_N
ClientSampleId :
RBR251346


Tgt Ion:106 Resp: 1000
Ion Ratio Lower Upper
106 100
91 230.9 109.1 327.2

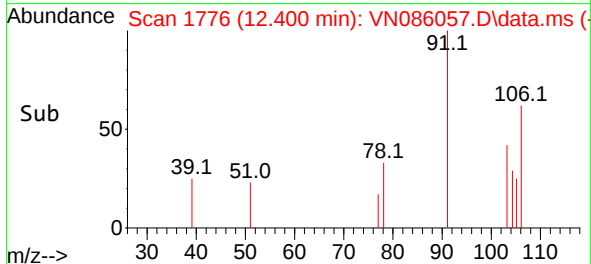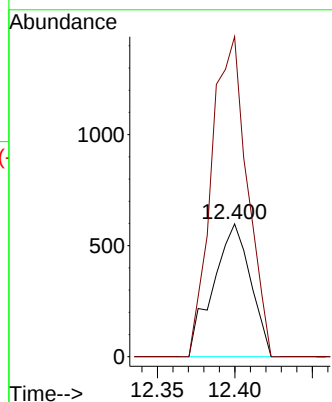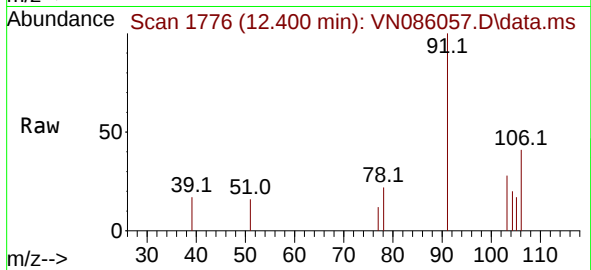

#71
Bromoform
Concen: 0.571 ug/l
RT: 12.841 min Scan# 1851
Delta R.T. 0.264 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07

Tgt Ion:173 Resp: 1047
Ion Ratio Lower Upper
173 100
175 441.5 24.3 73.0#
254 0.0 0.0 0.0

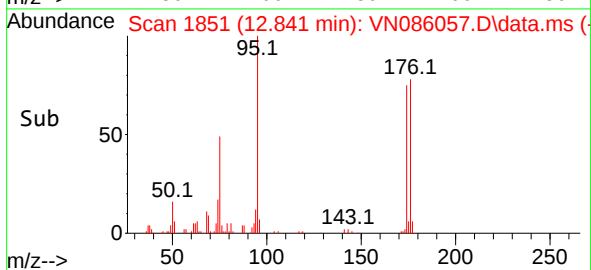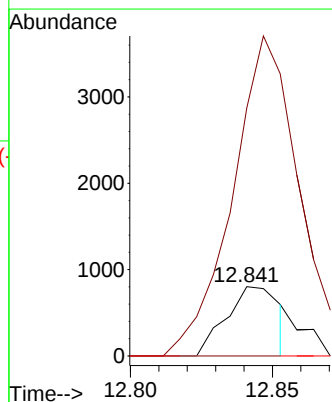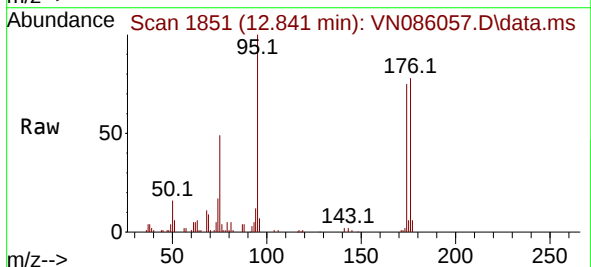



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.788 min Scan# 20

Delta R.T. -0.000 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Instrument :

MSVOA_N

ClientSampleId :

RBR251346





Tgt Ion:152 Resp: 95635

Ion Ratio Lower Upper

152 100

115 61.4 31.1 93.2

150 156.0 0.0 359.6

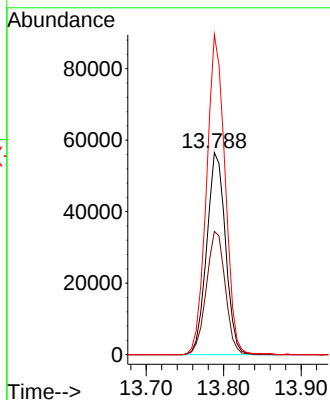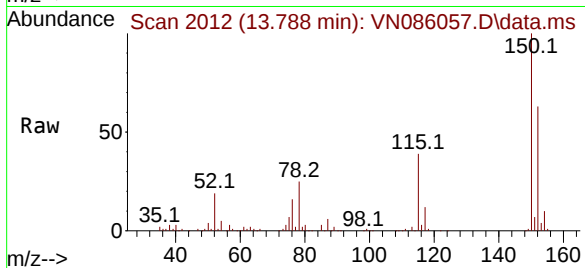

#74

N-ethyl acetate

Concen: 0.314 ug/l

RT: 12.470 min Scan# 1788

Delta R.T. -0.024 min

Lab File: VN086057.D

Acq: 21 Mar 2025 22:07

Tgt Ion: 43 Resp: 685




Ion Ratio Lower Upper


43 100

70 0.0 43.0 64.4#

55 0.0 23.8 35.8#

61 0.0 23.4 35.0#



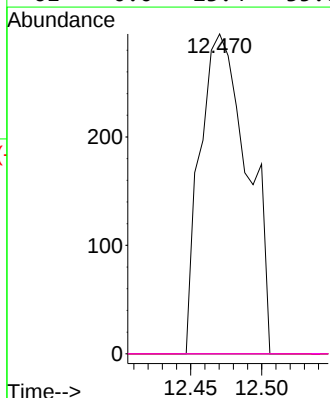
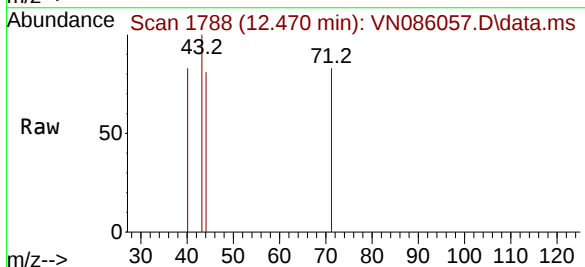




#76
1,2,3-Trichloropropane
Concen: 23.906 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.141 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07




Instrument :
MSVOA_N
ClientSampleId :
RBR251346


Tgt Ion: 75 Resp: 51185
Ion Ratio Lower Upper
75 100
77 1.5 83.7 251.0#

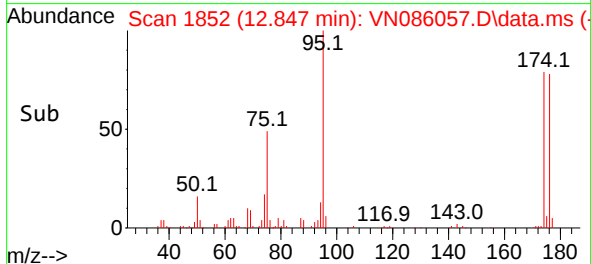

#81
trans-1,4-Dichloro-2-butene
Concen: 63.204 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.112 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07

Tgt Ion: 75 Resp: 51185
Ion Ratio Lower Upper
75 100
53 0.0 66.0 99.0#
89 0.0 36.9 55.3#


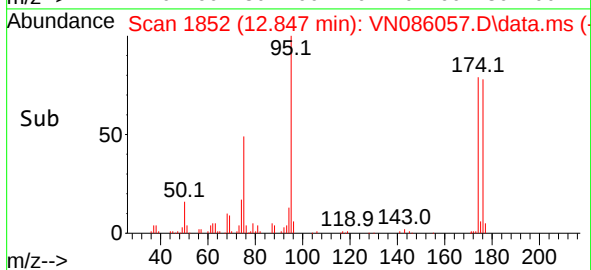

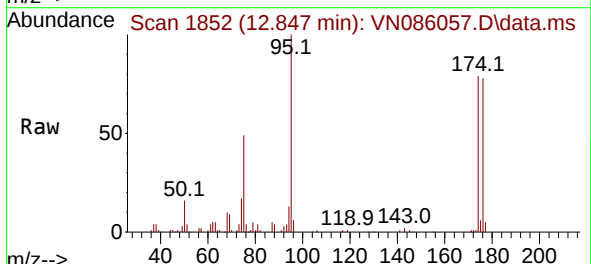


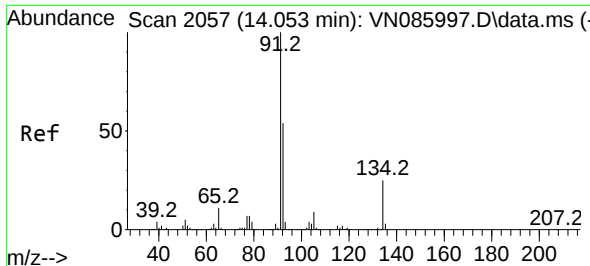

#89
n-Butylbenzene
Concen: 0.213 ug/l
RT: 13.994 min Scan# 2057
Delta R.T. -0.059 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07

Instrument :
MSVOA_N
ClientSampleId :
RBR251346

Tgt Ion: 91 Resp: 905
Ion Ratio Lower Upper
91 100
92 0.0 26.9 80.6#
134 0.0 13.0 39.0#

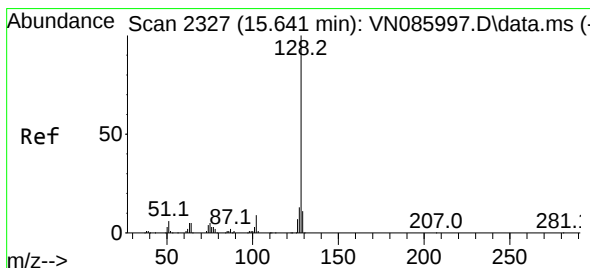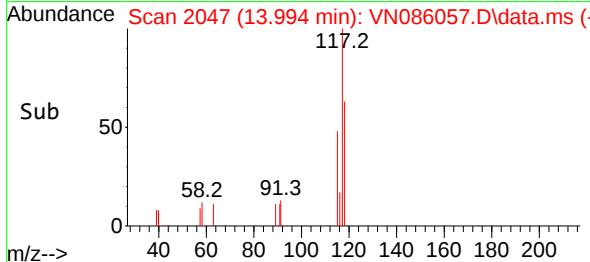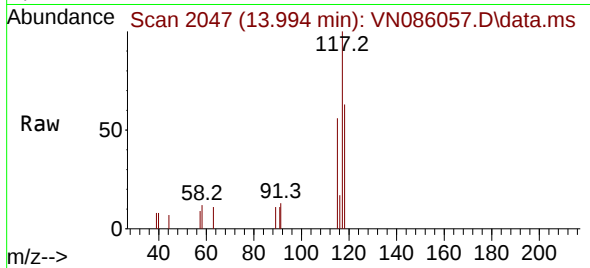

#95
Naphthalene
Concen: 0.577 ug/l
RT: 15.641 min Scan# 2327
Delta R.T. -0.000 min
Lab File: VN086057.D
Acq: 21 Mar 2025 22:07

Tgt Ion: 128 Resp: 2739
Ion Ratio Lower Upper
128 100
127 5.8 10.2 15.4#
129 7.5 9.0 13.6#

